

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011823\
Data File : VX033776.D
Acq On : 18 Jan 2023 15:56
Operator : JC/MD
Sample : 01137-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Integration Parameters: RTEINT3.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX033776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.392	206	214	230	rBV	473764	988474	2.68%	2.607%
2	2.642	232	255	299	rBV	4743381	36924312	100.00%	97.393%




Sum of corrected areas: 37912786

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011823\
Data File : VX033776.D
Acq On : 18 Jan 2023 15:56
Operator : JC/MD
Sample : 01137-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011823W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

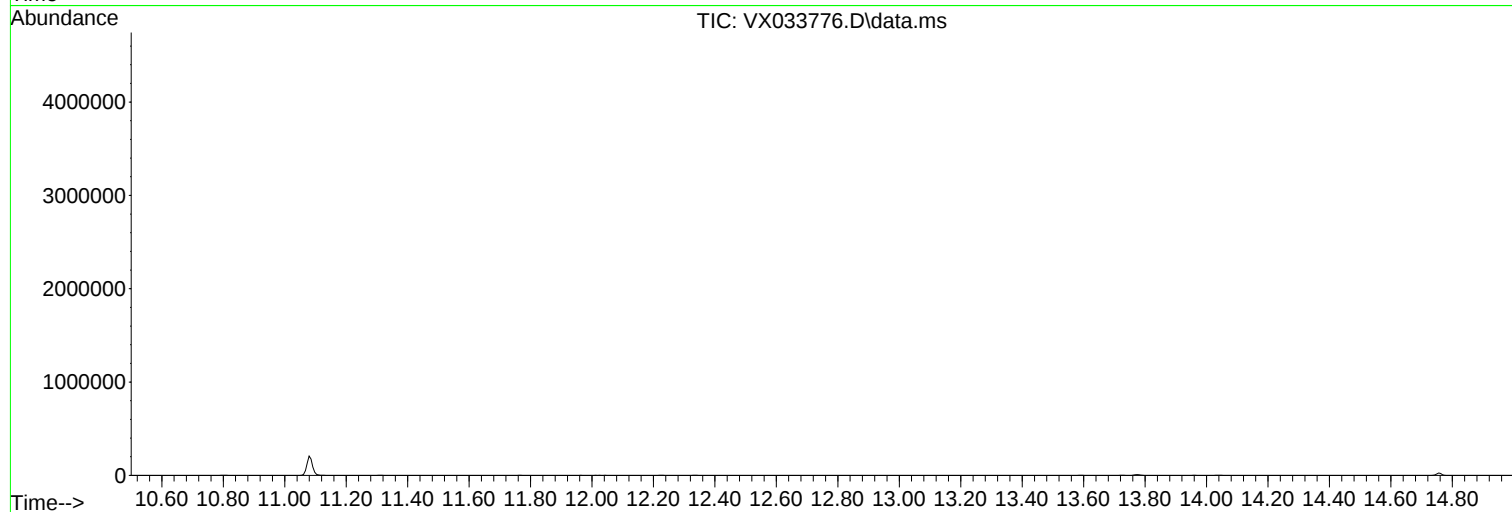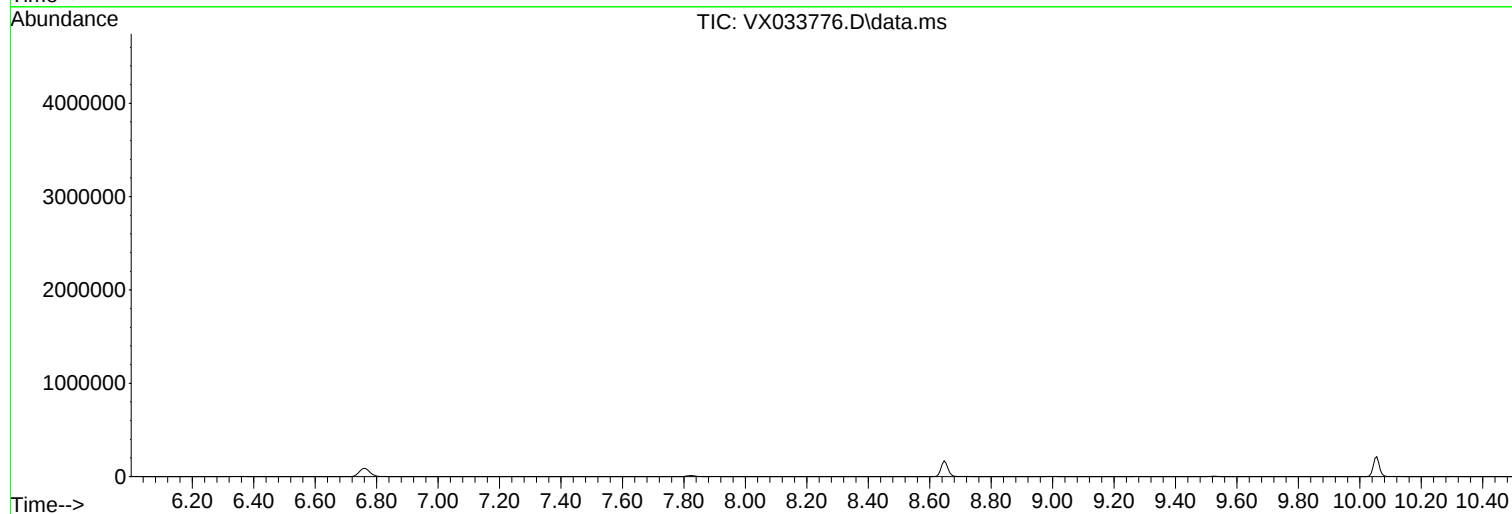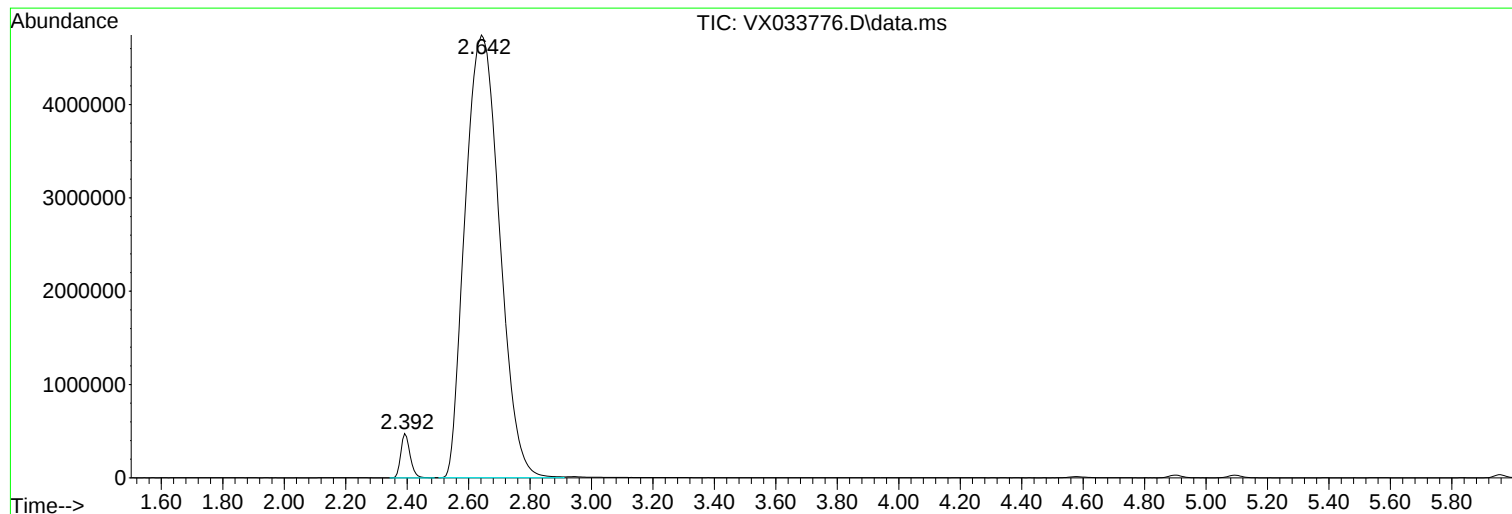

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011823\
Data File : VX033776.D
Acq On : 18 Jan 2023 15:56
Operator : JC/MD
Sample : 01137-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011823W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.642	30.00 ug/l	36924300	Bromochloromethane	4.898

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	83
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	64

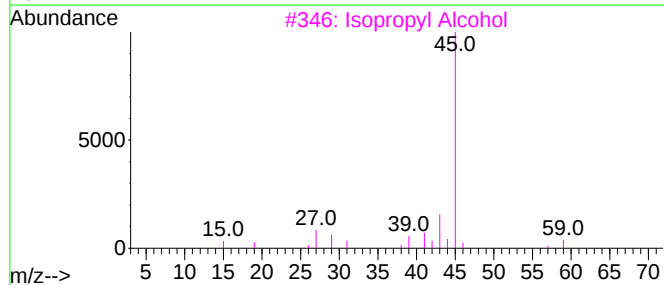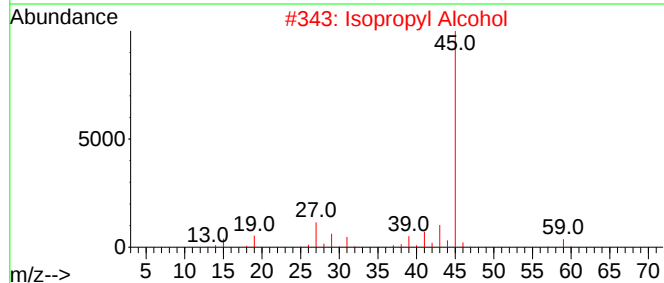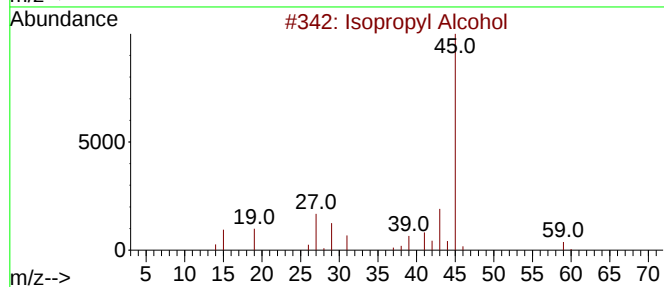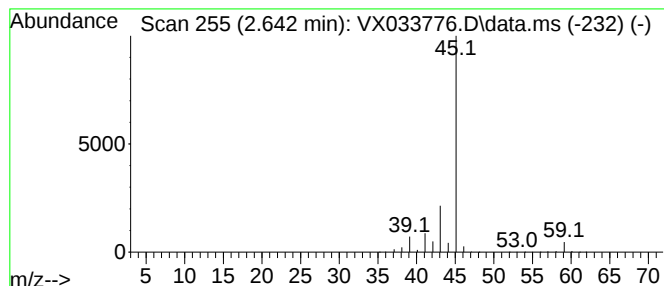

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011823\
Data File : VX033776.D
Acq On : 18 Jan 2023 15:56
Operator : JC/MD
Sample : 01137-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011823W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.642	30.0	ug/l	36924300	1	4.898	36924300	30.0