
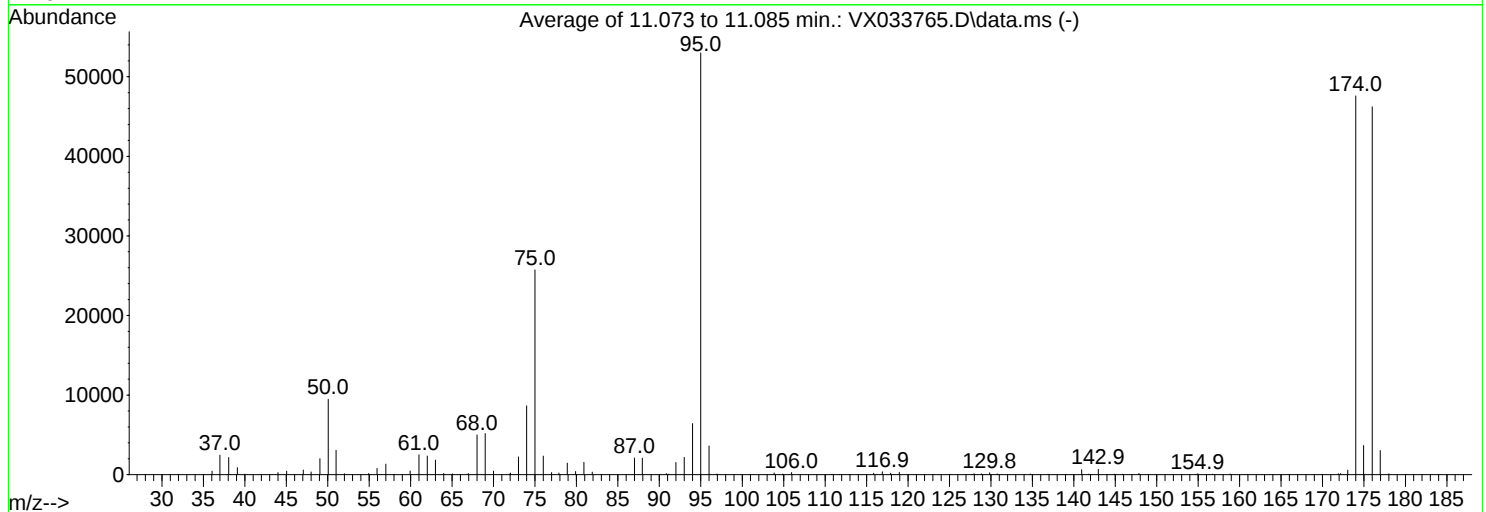


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011823\
Data File : VX033765.D
Acq On : 18 Jan 2023 08:32
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Jan 18 14:40:07 2023

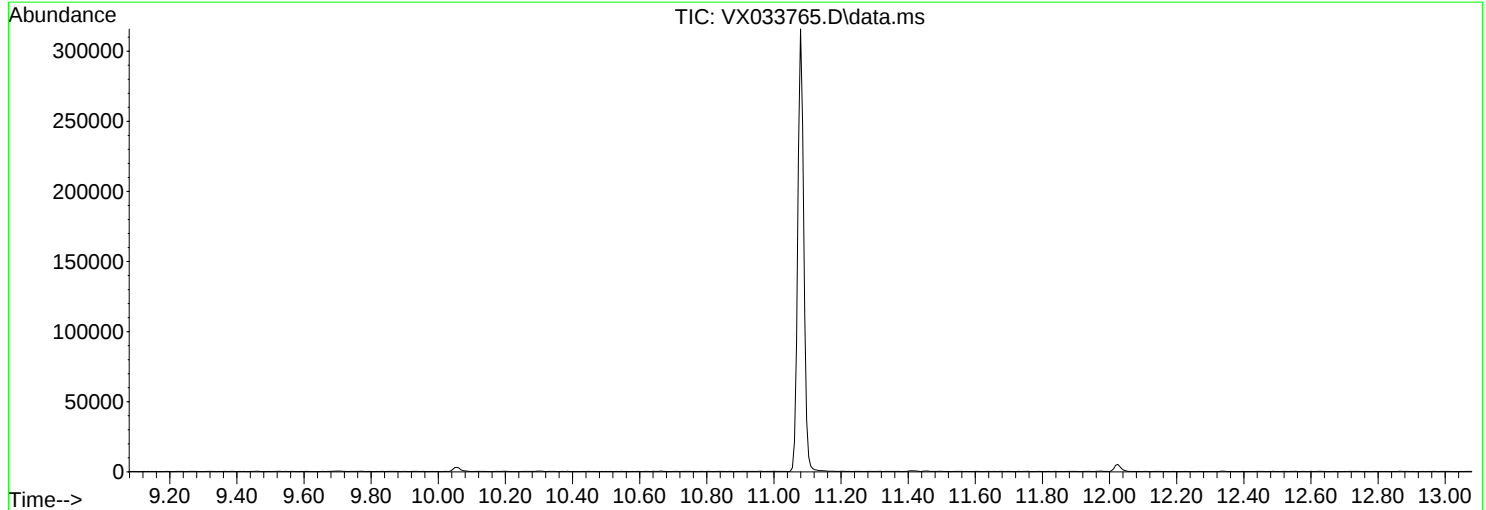

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	9472	PASS
75	95	30	60	48.6	25741	PASS
95	95	100	100	100.0	53005	PASS
96	95	5	9	6.8	3599	PASS
173	174	0.00	2	1.2	573	PASS
174	95	50	100	89.8	47603	PASS
175	174	5	9	7.7	3667	PASS
176	174	95	101	97.1	46219	PASS
177	176	5	9	6.6	3033	PASS