

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011921\
 Data File : VX020664.D
 Acq On : 19 Jan 2021 17:17
 Operator : JC/SP
 Sample : M1125-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1693-94

Quant Time: Jan 20 03:21:15 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 19 14:09:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	239841	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	404747	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.092	117	386587	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	183694	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.025	65	162047	49.42	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	98.84%		
35) Dibromofluoromethane	5.464	113	132150	47.39	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	94.78%		
50) Toluene-d8	8.696	98	503887	50.11	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	100.22%		
62) 4-Bromofluorobenzene	11.116	95	191155	50.30	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	100.60%		
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.179	85	51	0.76	ug/l #	42
6) Chloroethane	1.715	64	285	Below Cal	#	25
11) Tert butyl alcohol	2.995	59	4166	7.16	ug/l #	73
13) Acrolein	2.276	56	1525	34.09	ug/l	91
14) Allyl chloride	2.684	41	12819	3.31	ug/l #	40
15) Acrylonitrile	3.117	53	1631	1.13	ug/l	91
16) Acetone	2.416	43	65288	51.27	ug/l	99
18) Methyl Acetate	2.745	43	930	0.32	ug/l	91
20) Methylene Chloride	2.831	84	752	0.24	ug/l #	93
22) Diisopropyl ether	3.965	45	166709	21.56	ug/l #	1
23) Vinyl Acetate	3.965	43	391620	59.35	ug/l #	68
25) 2-Butanone	4.635	43	12822	6.89	ug/l	95
29) Tetrahydrofuran	5.111	42	1387	1.20	ug/l #	28
30) Chloroform	5.172	83	3239	0.60	ug/l	87
31) Cyclohexane	5.623	56	5041	1.17	ug/l #	1
36) 1,1-Dichloropropene	5.629	75	18643	4.57	ug/l #	49
37) Ethyl Acetate	4.800	43	1811	0.48	ug/l #	80
38) Carbon Tetrachloride	5.623	117	24688	5.67	ug/l #	16
40) Benzene	6.111	78	4403	0.37	ug/l	92
51) 4-Methyl-2-Pentanone	8.622	43	2296	0.63	ug/l	92
52) Toluene	8.763	92	3960	0.54	ug/l	98
56) Ethyl methacrylate	9.122	69	53	2.10	ug/l #	1
59) 2-Hexanone	9.476	43	798	0.29	ug/l	98
68) m/p-Xylenes	10.342	106	2132	0.40	ug/l	90
69) o-Xylene	10.683	106	1281	0.25	ug/l	83
70) Styrene	10.695	104	859	1.51	ug/l #	85
74) N-amyl acetate	10.903	43	595	2.05	ug/l #	59
76) 1,2,3-Trichloropropane	11.116	75	94423	21.42	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.116	75	94423	61.96	ug/l #	12
84) 1,2,4-Trimethylbenzene	11.793	105	4156	0.75	ug/l	88
86) p-Isopropyltoluene	12.049	119	6746	1.42	ug/l	89
89) n-Butylbenzene	12.372	91	962	1.51	ug/l #	78
93) 1,2,4-Trichlorobenzene	13.634	180	226	2.29	ug/l #	42
95) Naphthalene	13.817	128	13801	2.92	ug/l #	92

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011921\
Data File : VX020664.D
Acq On : 19 Jan 2021 17:17
Operator : JC/SP
Sample : M1125-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1693-94

Quant Time: Jan 20 03:21:15 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 19 14:09:08 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011921\
 Data File : VX020664.D
 Acq On : 19 Jan 2021 17:17
 Operator : JC/SP
 Sample : M1125-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1693-94

Quant Time: Jan 20 03:21:15 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 19 14:09:08 2021
 Response via : Initial Calibration




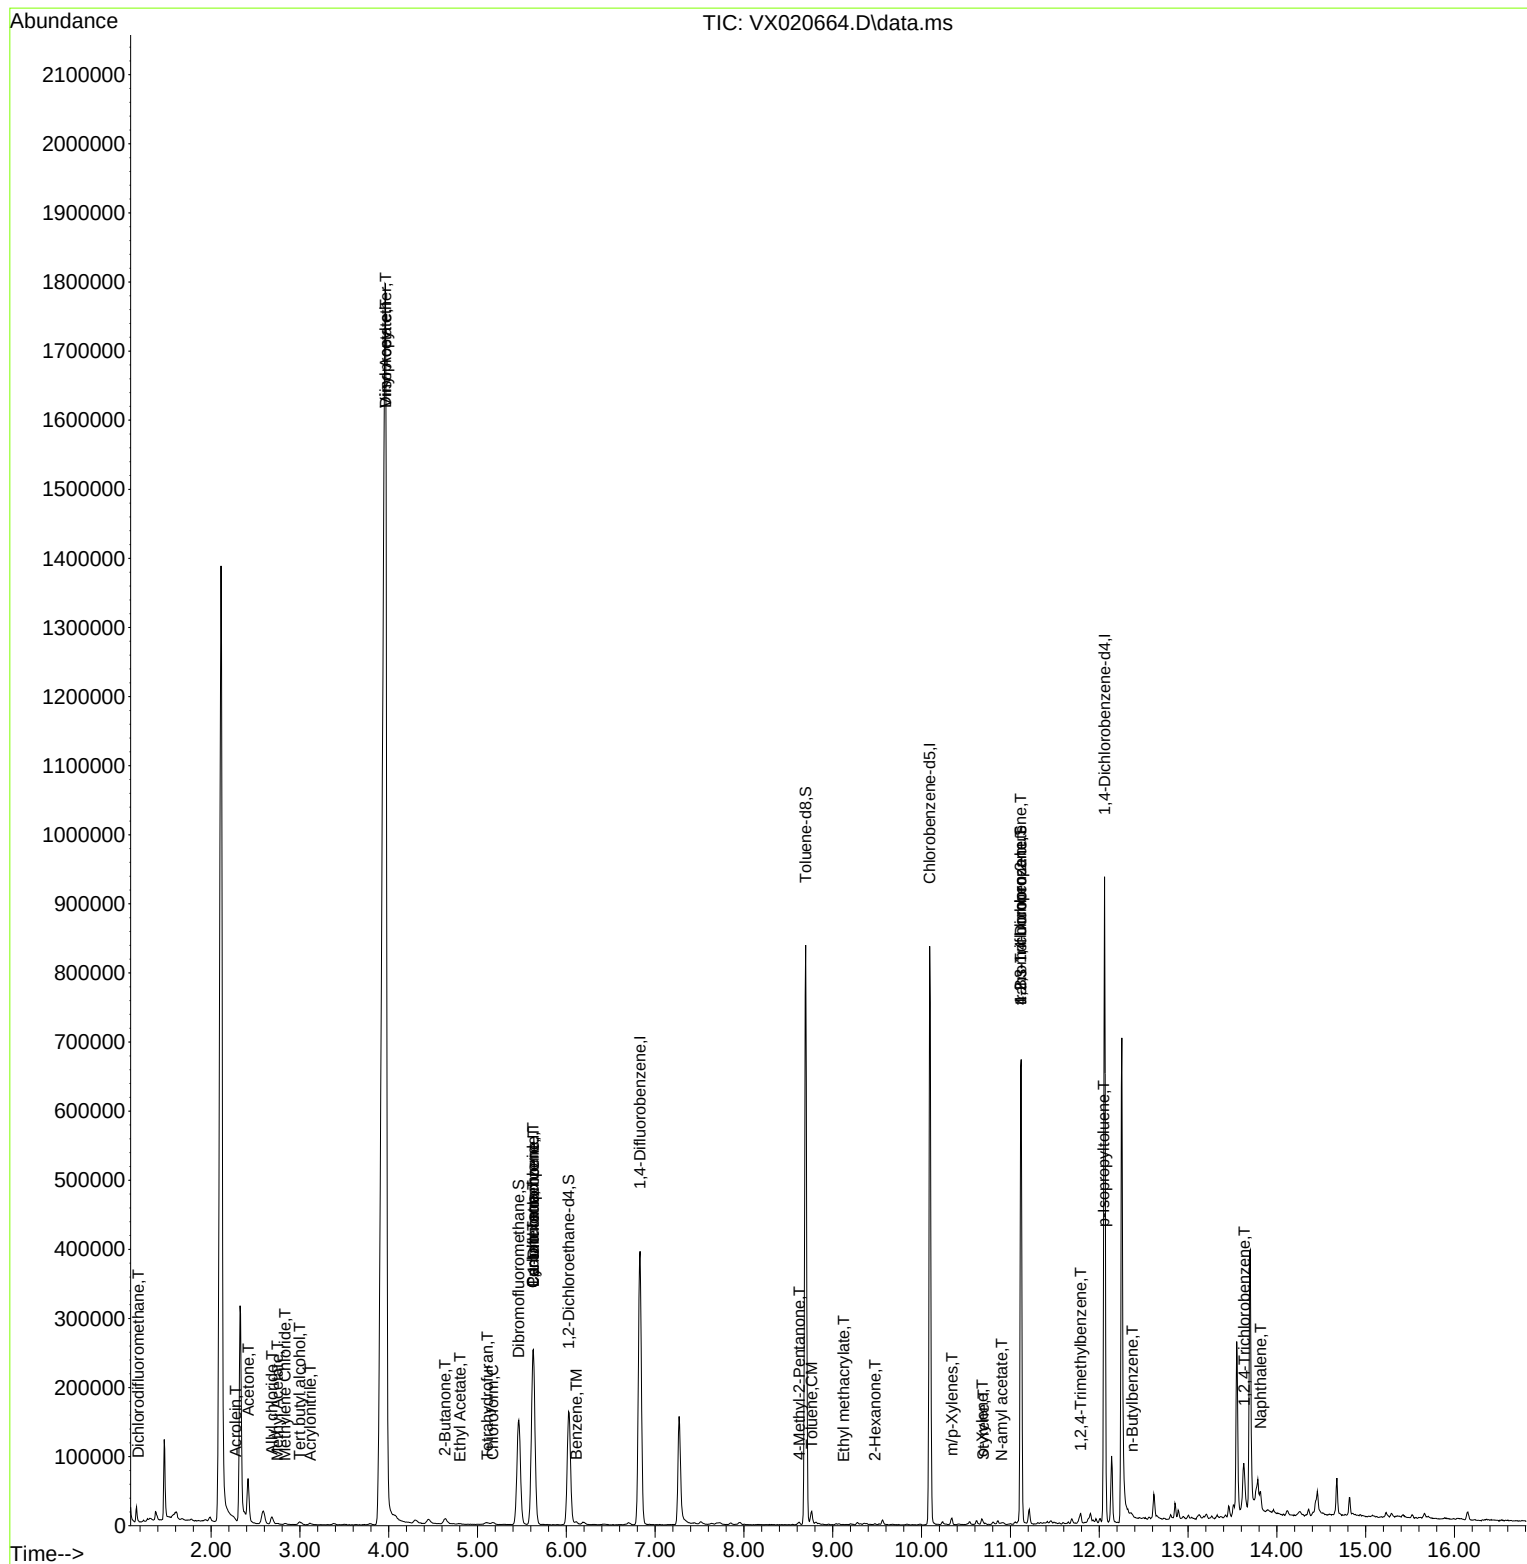




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampleId :
1693-94


Tgt Ion:168 Resp: 239841
Ion Ratio Lower Upper
168 100
99 61.4 45.8 68.6

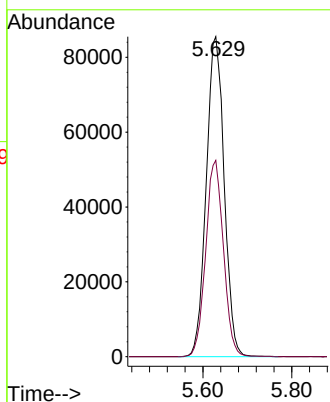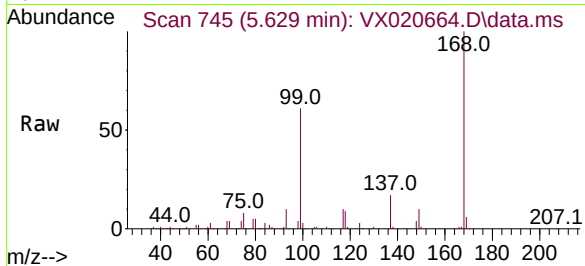

#2
Dichlorodifluoromethane
Concen: 0.76 ug/l
RT: 1.179 min Scan# 15
Delta R.T. -0.006 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 85 Resp: 51
Ion Ratio Lower Upper
85 100
87 0.0 16.4 49.2#




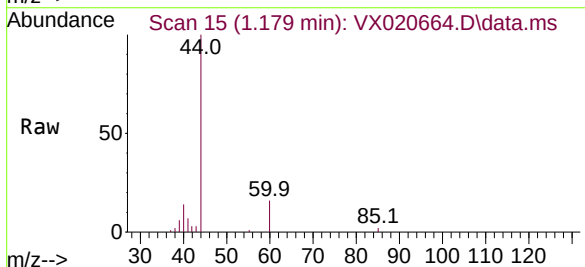




#6
Chloroethane
Concen: Below Cal
RT: 1.715 min Scan# 103
Delta R.T. 0.006 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampled :
1693-94


Tgt Ion: 64 Resp: 285
Ion Ratio Lower Upper
64 100
66 73.4 25.4 38.0#

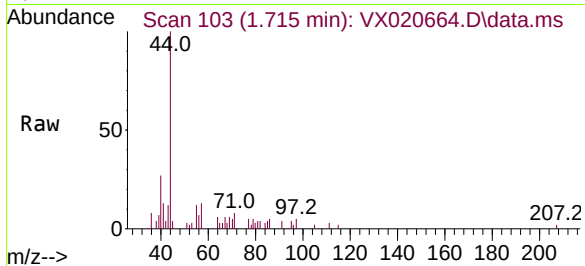

#11
Tert butyl alcohol
Concen: 7.16 ug/l
RT: 2.995 min Scan# 313
Delta R.T. -0.043 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 59 Resp: 4166
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#


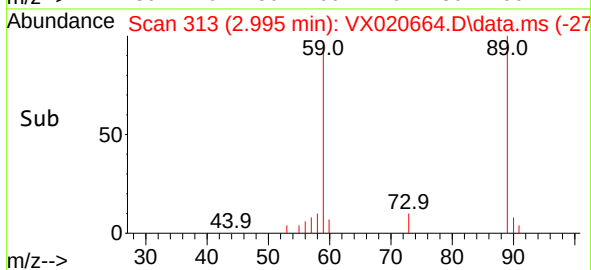

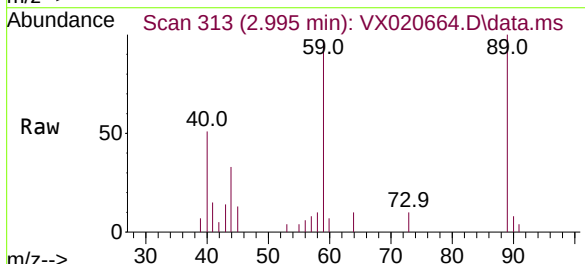


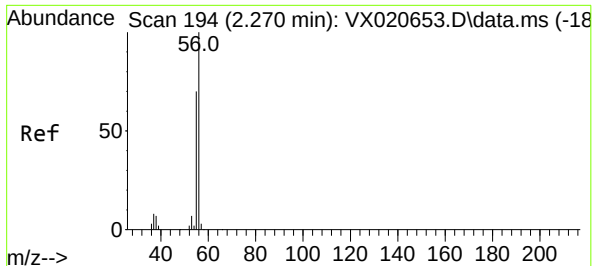

#13
Acrolein
Concen: 34.09 ug/l
RT: 2.276 min Scan# 195
Delta R.T. 0.006 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampled :
1693-94


Tgt Ion: 56 Resp: 1525
Ion Ratio Lower Upper
56 100
55 77.7 56.4 84.6

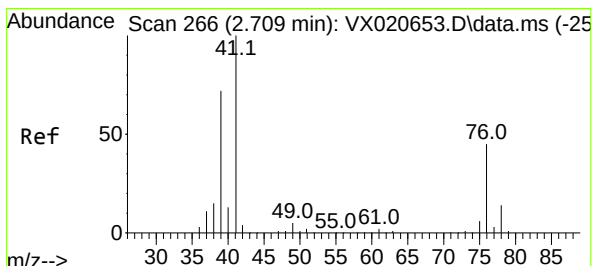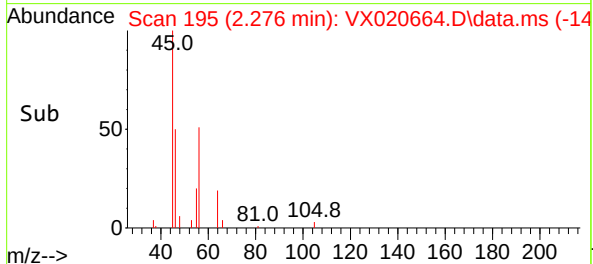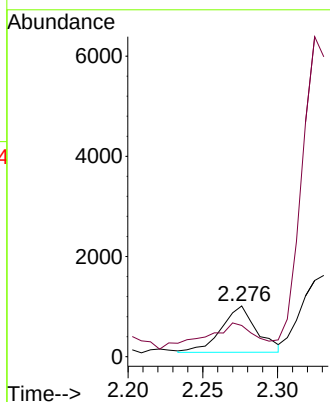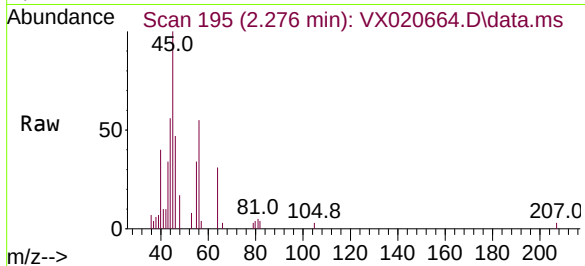

#14
Allyl chloride
Concen: 3.31 ug/l
RT: 2.684 min Scan# 262
Delta R.T. -0.025 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 41 Resp: 12819
Ion Ratio Lower Upper
41 100
39 18.5 51.6 77.4#
76 0.0 30.5 45.7#


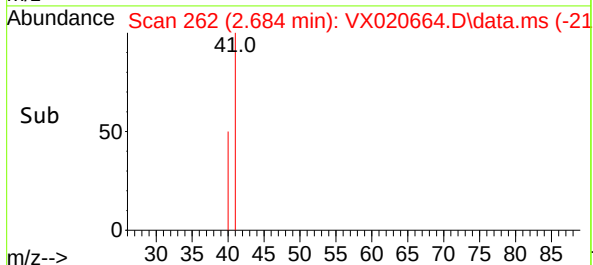

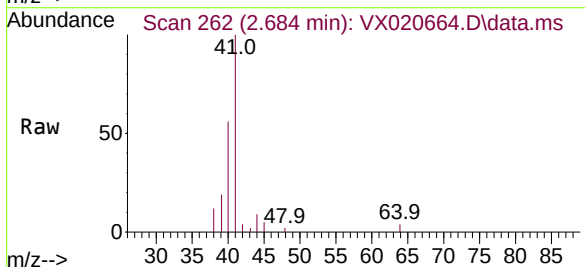




#15
Acrylonitrile
Concen: 1.13 ug/l
RT: 3.117 min Scan# 333
Delta R.T. 0.006 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampleId :
1693-94


Tgt Ion: 53	Resp: 1631
Ion Ratio	Lower Upper
53 100	
52 91.8	65.3 97.9
51 36.8	28.2 42.2

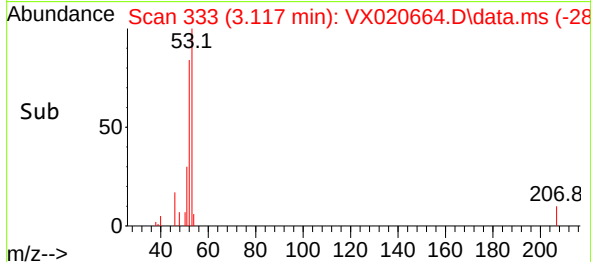

#16
Acetone
Concen: 51.27 ug/l
RT: 2.416 min Scan# 218
Delta R.T. 0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 43	Resp: 65288
Ion Ratio	Lower Upper
43 100	
58 35.6	27.8 41.8

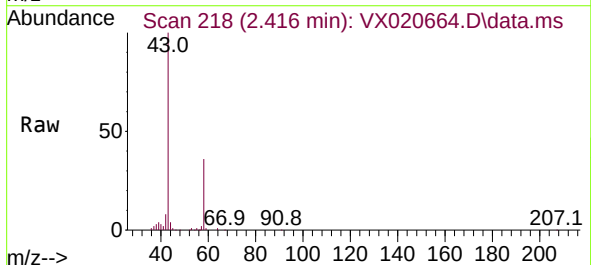



#18

Methyl Acetate

Concen: 0.32 ug/l

RT: 2.745 min Scan# 272

Delta R.T. 0.000 min

Lab File: VX020664.D

Acq: 19 Jan 2021 17:17

Instrument :

MSVOA_X

ClientSampled :





1693-94

Tgt Ion: 43 Resp: 930

Ion Ratio Lower Upper

43 100

74 22.6 21.9 32.9

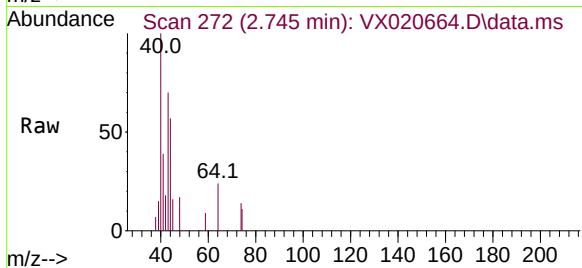

#20

Methylene Chloride

Concen: 0.24 ug/l

RT: 2.831 min Scan# 286

Delta R.T. -0.000 min

Lab File: VX020664.D

Acq: 19 Jan 2021 17:17

Tgt Ion: 84 Resp: 752




Ion Ratio Lower Upper


84 100

49 108.2 88.6 132.8

51 40.8 27.0 40.6#


86 54.1 50.3 75.5

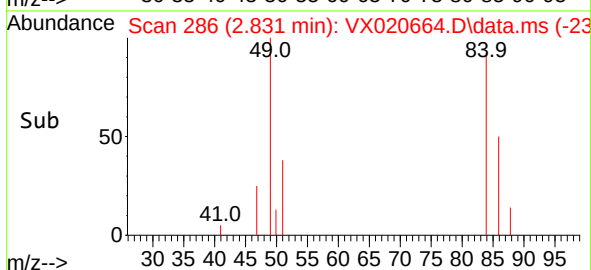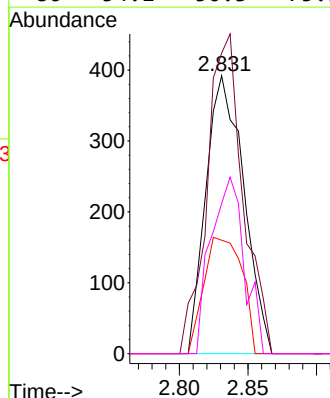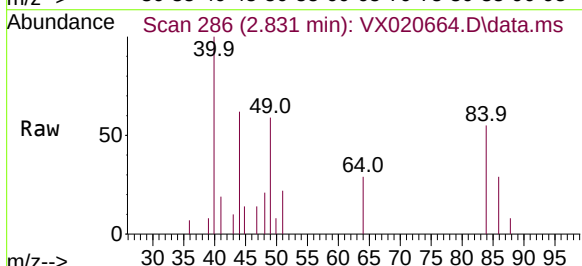






#22
Diisopropyl ether
Concen: 21.56 ug/l
RT: 3.965 min Scan# 472
Delta R.T. 0.140 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17


Instrument :
MSVOA_X
ClientSampleId :
1693-94





Tgt Ion: 45 Resp: 166709
Ion Ratio Lower Upper
45 100
43 238.2 58.0 87.0#
87 0.0 25.4 38.0#
59 970.4 10.2 15.2#




#23
Vinyl Acetate
Concen: 59.35 ug/l
RT: 3.965 min Scan# 472
Delta R.T. 0.183 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17



Tgt Ion: 43 Resp: 391620
Ion Ratio Lower Upper
43 100
86 0.0 9.9 14.9#



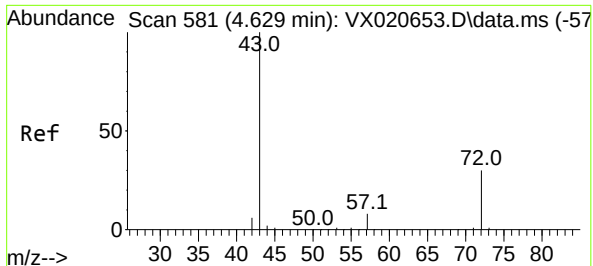

#25

2-Butanone

Concen: 6.89 ug/l

RT: 4.635 min Scan# 582

Delta R.T. 0.006 min

Lab File: VX020664.D





Acq: 19 Jan 2021 17:17

Tgt Ion: 43 Resp: 12822

Ion Ratio Lower Upper

43 100

72 26.9 23.7 35.5

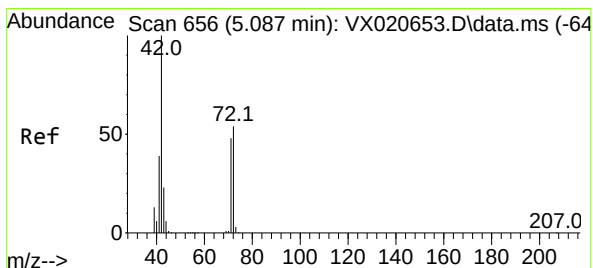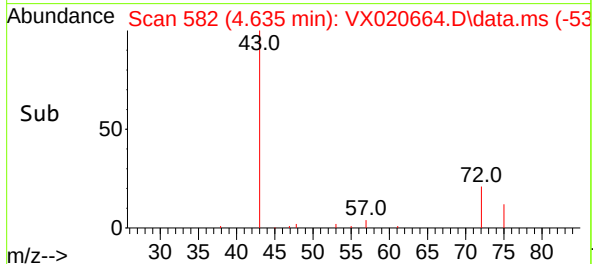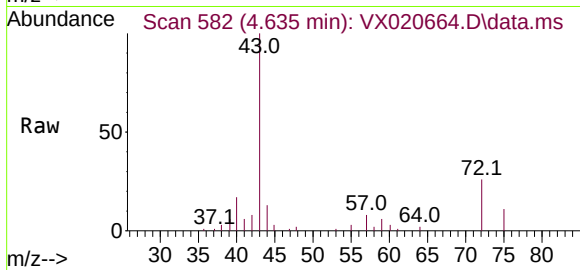

#29

Tetrahydrofuran

Concen: 1.20 ug/l

RT: 5.111 min Scan# 660

Delta R.T. 0.024 min

Lab File: VX020664.D

Acq: 19 Jan 2021 17:17




Tgt Ion: 42 Resp: 1387


Ion Ratio Lower Upper

42 100

72 1.5 41.7 62.5#

71 0.0 38.4 57.6#


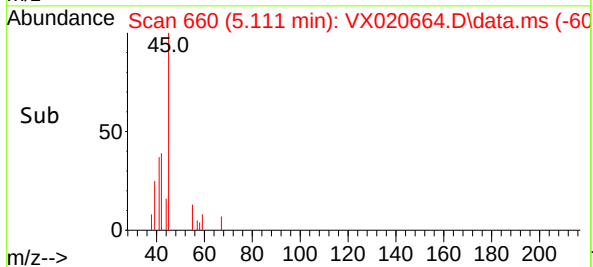

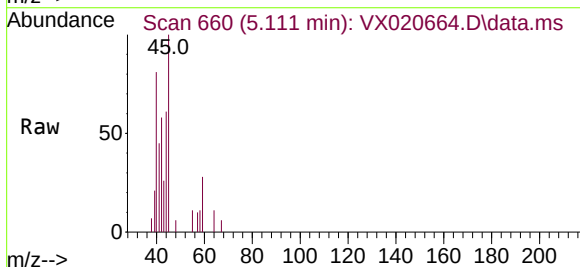




#30
Chloroform
Concen: 0.60 ug/l
RT: 5.172 min Scan# 670
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampled :
1693-94


Tgt Ion: 83 Resp: 3239
Ion Ratio Lower Upper
83 100
85 54.9 52.0 78.0

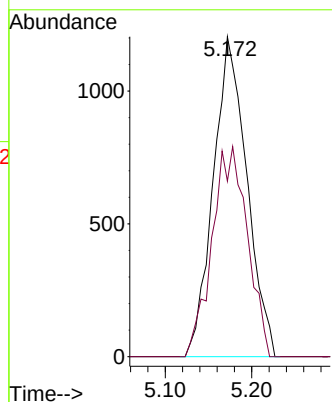

#31
Cyclohexane
Concen: 1.17 ug/l
RT: 5.623 min Scan# 744
Delta R.T. 0.079 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 56 Resp: 5041
Ion Ratio Lower Upper
56 100
69 175.4 25.3 37.9#
84 142.1 71.4 107.0#

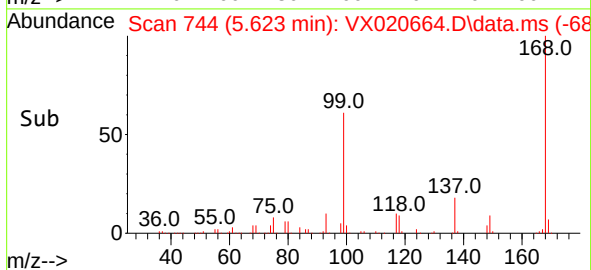

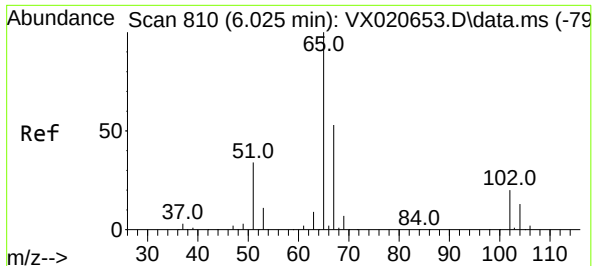

#33

1,2-Dichloroethane-d4

Concen: 49.42 ug/l

RT: 6.025 min Scan# 810

Delta R.T. 0.000 min

Lab File: VX020664.D

Acq: 19 Jan 2021 17:17

Tgt Ion: 65 Resp: 162047

Ion Ratio Lower Upper

65 100





67 51.9 0.0 105.4

Instrument :

MSVOA_X

ClientSampleId :

1693-94

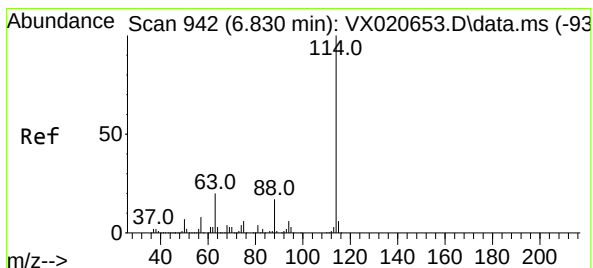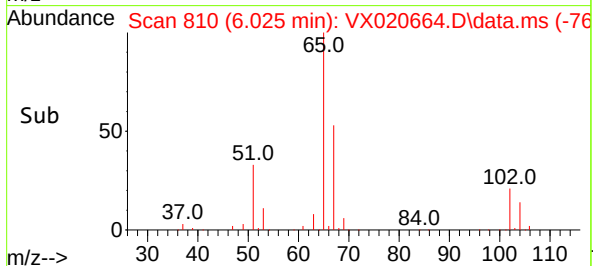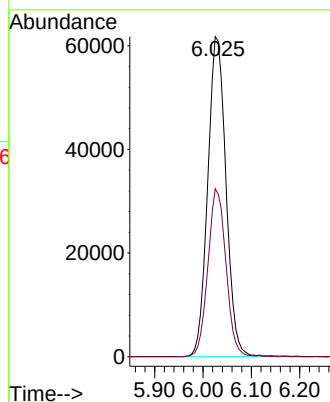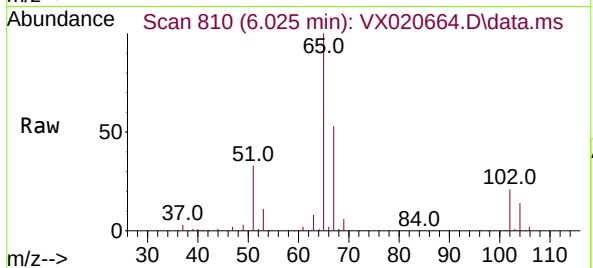

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.830 min Scan# 942

Delta R.T. 0.000 min

Lab File: VX020664.D

Acq: 19 Jan 2021 17:17




Tgt Ion: 114 Resp: 404747


Ion Ratio Lower Upper

114 100

63 20.7 0.0 40.8

88 17.3 0.0 32.8


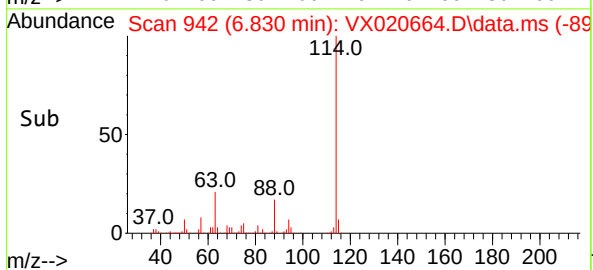

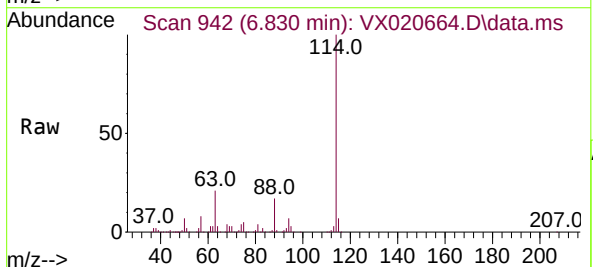


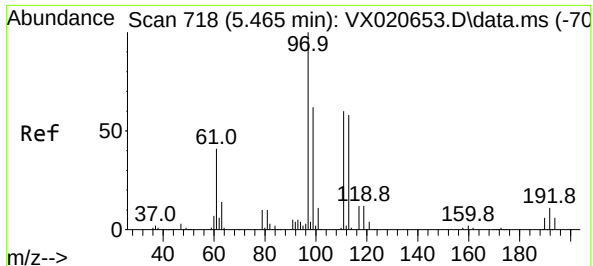

#35
Dibromofluoromethane
Concen: 47.39 ug/l
RT: 5.464 min Scan# 718
Delta R.T. -0.001 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampled :
1693-94


Tgt Ion:113 Resp: 132150
Ion Ratio Lower Upper
113 100
111 103.9 81.9 122.9
192 19.6 16.7 25.1

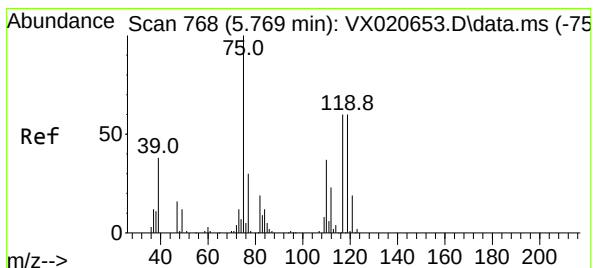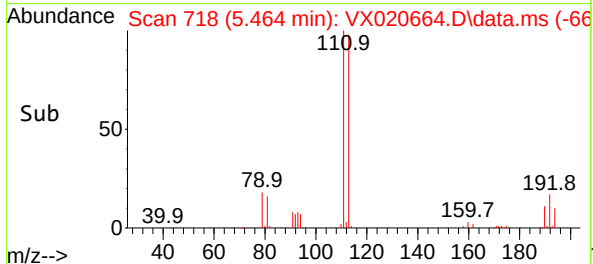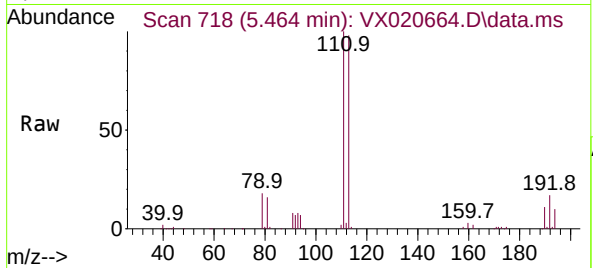

#36
1,1-Dichloropropene
Concen: 4.57 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.140 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 75 Resp: 18643
Ion Ratio Lower Upper
75 100
110 8.9 18.1 54.4#
77 0.0 25.3 37.9#

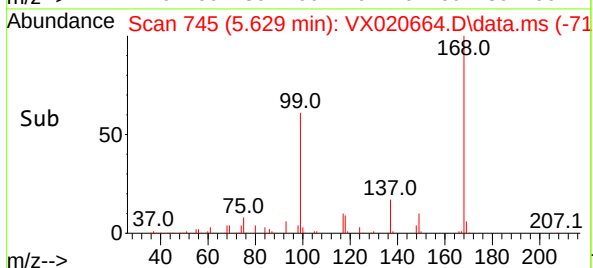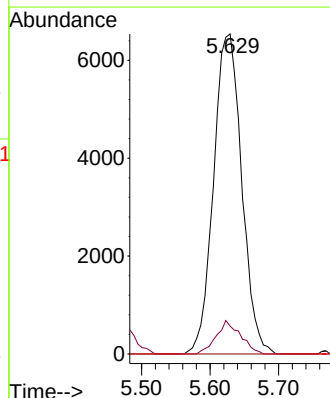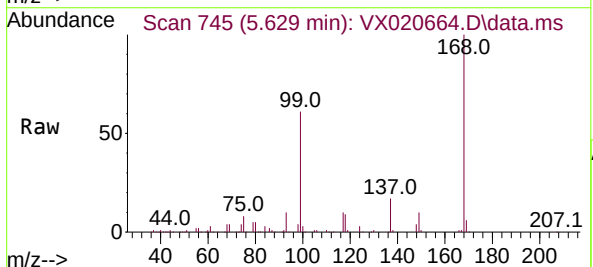



#37

Ethyl Acetate

Concen: 0.48 ug/l

RT: 4.800 min Scan# 609





Delta R.T. 0.012 min

Lab File: VX020664.D

Acq: 19 Jan 2021 17:17

Tgt Ion:	43	Resp:	1811
Ion	Ratio	Lower	Upper
43	100		
61	6.5	12.8	19.2#
70	6.4	10.5	15.7#

Instrument :
MSVOA_X
ClientSampled :
1693-94

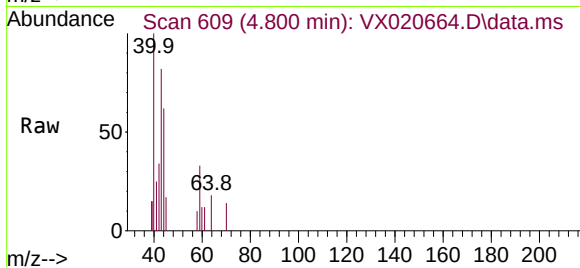

#38

Carbon Tetrachloride

Concen: 5.67 ug/l




RT: 5.623 min Scan# 744


Delta R.T. -0.134 min

Lab File: VX020664.D

Acq: 19 Jan 2021 17:17

Tgt Ion:	117	Resp:	24688
Ion	Ratio	Lower	Upper
117	100		
119	5.2	76.2	114.2#
121	0.0	24.8	37.2#


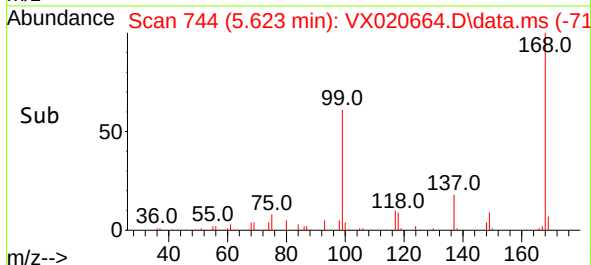
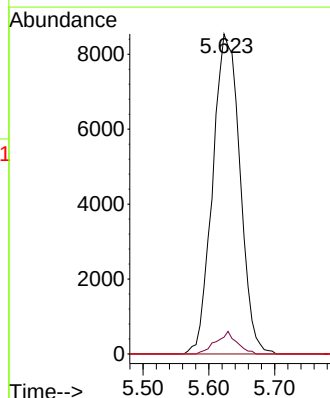
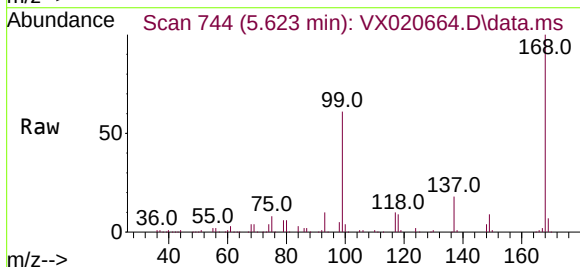




#40
Benzene
Concen: 0.37 ug/l
RT: 6.111 min Scan# 824
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampled :
1693-94


Tgt Ion: 78 Resp: 4403
Ion Ratio Lower Upper
78 100
77 27.6 18.9 28.3



#50
Toluene-d8
Concen: 50.11 ug/l
RT: 8.696 min Scan# 1248
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 98 Resp: 503887
Ion Ratio Lower Upper
98 100
100 65.4 51.9 77.9


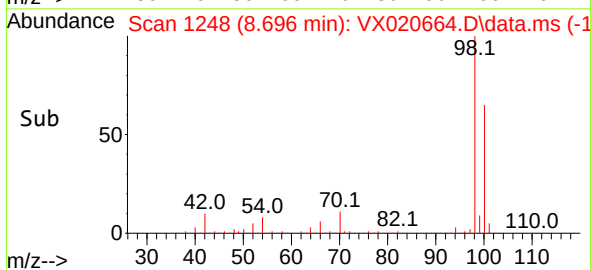






#51
4-Methyl-2-Pentanone
Concen: 0.63 ug/l
RT: 8.622 min Scan# 1236
Delta R.T. 0.006 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampled :
1693-94


Tgt Ion: 43 Resp: 2296
Ion Ratio Lower Upper
43 100
58 39.0 35.4 53.0

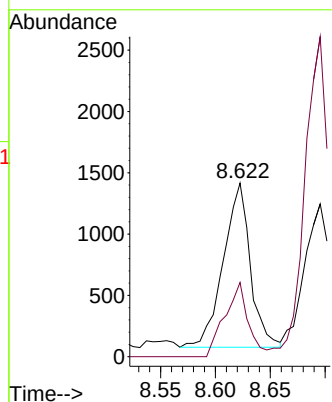

#52
Toluene
Concen: 0.54 ug/l
RT: 8.763 min Scan# 1259
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17


Tgt Ion: 92 Resp: 3960
Ion Ratio Lower Upper
92 100
91 173.7 137.1 205.7

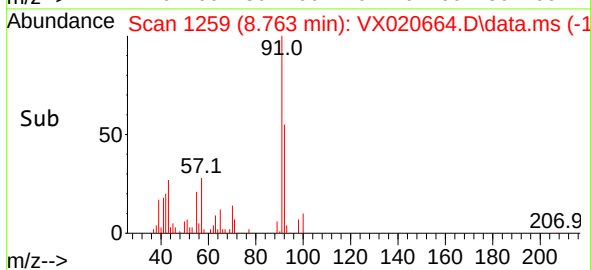






#56
Ethyl methacrylate
Concen: 2.10 ug/l
RT: 9.122 min Scan# 1318
Delta R.T. -0.037 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Instrument :
MSVOA_X
ClientSampleId :
1693-94







Tgt Ion: 69 Resp: 53
Ion Ratio Lower Upper
69 100
41 103.8 46.8 70.2#
39 571.7 24.7 37.1#



#59
2-Hexanone
Concen: 0.29 ug/l
RT: 9.476 min Scan# 1376
Delta R.T. 0.006 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 43 Resp: 798
Ion Ratio Lower Upper
43 100
58 63.4 30.9 92.8


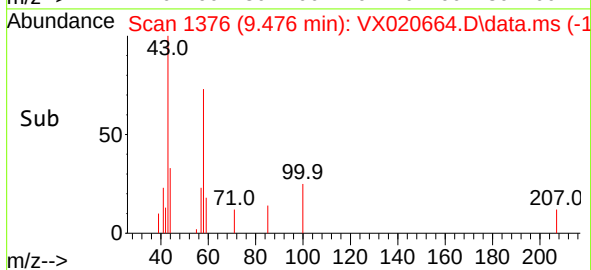






#62
4-Bromofluorobenzene
Concen: 50.30 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. -0.006 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampleId :
1693-94


Tgt Ion: 95 Resp: 191155
Ion Ratio Lower Upper
95 100
174 74.3 0.0 154.6
176 71.2 0.0 155.8

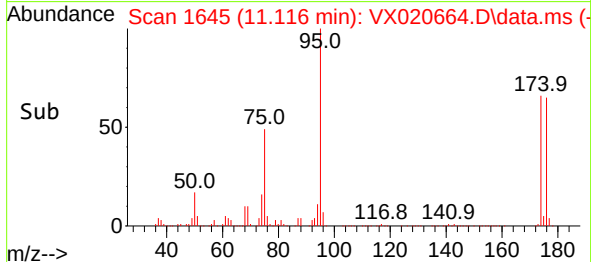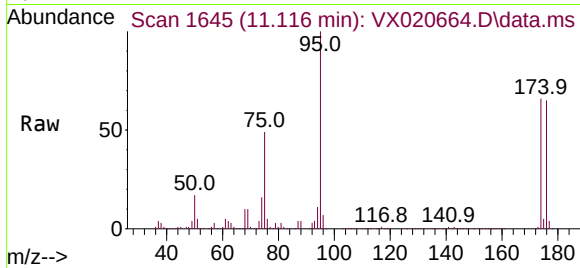

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.092 min Scan# 1477
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 117 Resp: 386587
Ion Ratio Lower Upper
117 100
82 57.5 47.4 71.2
119 30.4 26.6 39.8




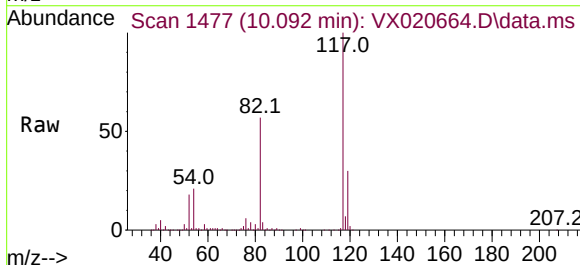




#68
m/p-Xylenes
Concen: 0.40 ug/l
RT: 10.342 min Scan# 1518
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampleId :
1693-94


Tgt Ion:106 Resp: 2132
Ion Ratio Lower Upper
106 100
91 219.6 162.8 244.2



#69
o-Xylene
Concen: 0.25 ug/l
RT: 10.683 min Scan# 1574
Delta R.T. 0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion:106 Resp: 1281
Ion Ratio Lower Upper
106 100
91 242.9 108.1 324.2


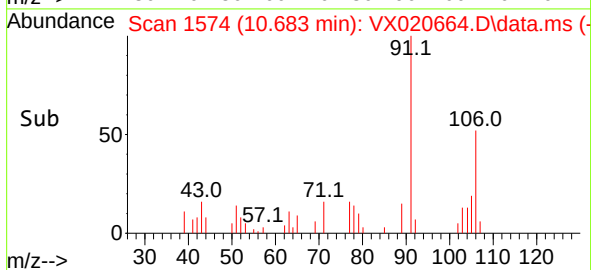






#70
Styrene
Concen: 1.51 ug/l
RT: 10.695 min Scan# 1576
Delta R.T. 0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampled :
1693-94


Tgt Ion:104 Resp: 859
Ion Ratio Lower Upper
104 100
78 69.2 40.0 60.0#
103 57.0 43.4 65.0

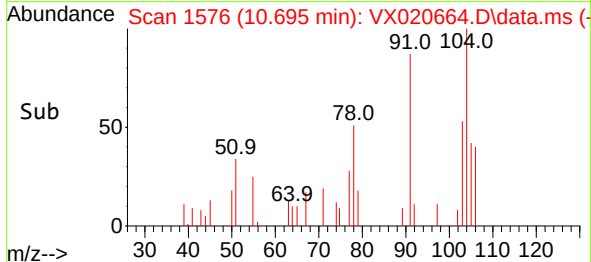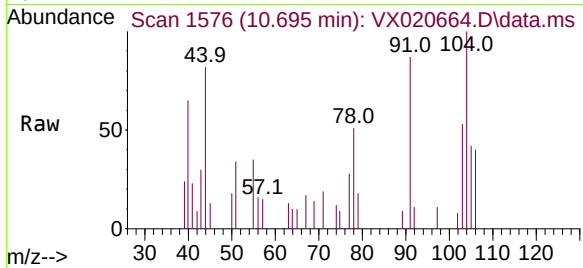

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion:152 Resp: 183694
Ion Ratio Lower Upper
152 100
115 62.9 41.1 123.3
150 158.8 0.0 349.0




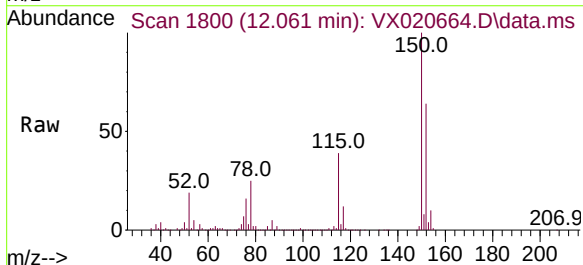




#74
N-amy1 acetate
Concen: 2.05 ug/l
RT: 10.903 min Scan# 1610
Delta R.T. 0.025 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampled :
1693-94


Tgt Ion: 43	Resp: 595
Ion Ratio	Lower Upper
43	100
70	81.3 39.0 58.6#
55	36.3 21.5 32.3#
61	0.0 22.1 33.1#

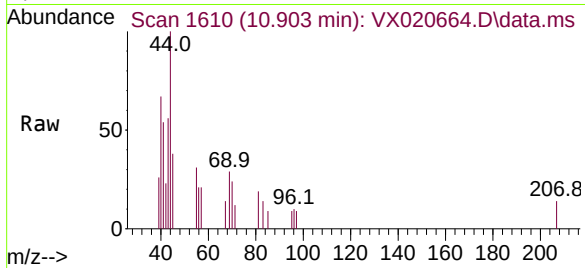

#76
1,2,3-Trichloropropane
Concen: 21.42 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. -0.165 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 75	Resp: 94423
Ion Ratio	Lower Upper
75	100
77	1.2 19.1 57.5#




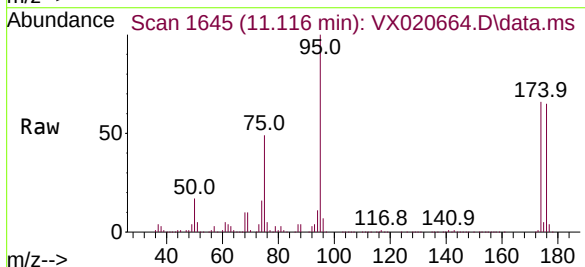




#81
trans-1,4-Dichloro-2-butene
Concen: 61.96 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. 0.061 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampleId :
1693-94


Tgt Ion: 75 Resp: 94423
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

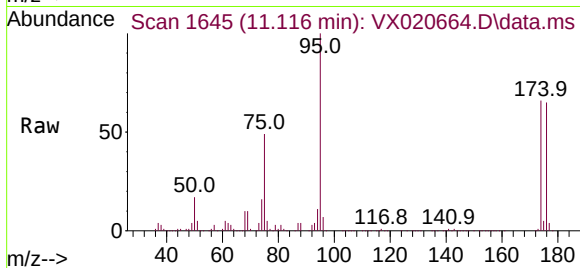

#84
1,2,4-Trimethylbenzene
Concen: 0.75 ug/l
RT: 11.793 min Scan# 1756
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 105 Resp: 4156
Ion Ratio Lower Upper
105 100
120 36.8 22.4 67.3


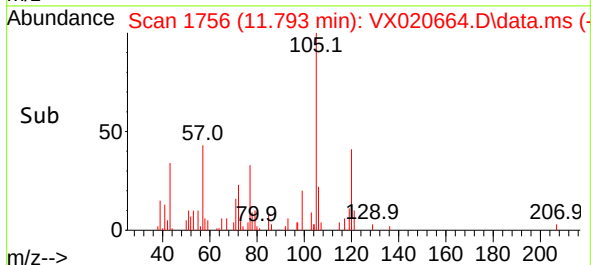

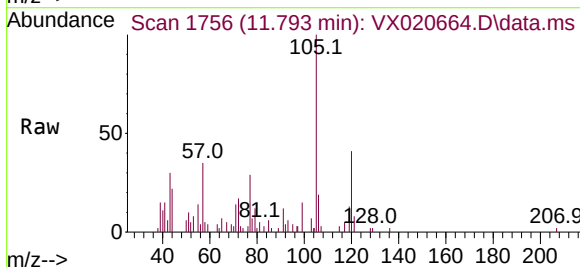




#86
p-Isopropyltoluene
Concen: 1.42 ug/l
RT: 12.049 min Scan# 1798
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17




Instrument :
MSVOA_X
ClientSampleId :
1693-94


Tgt Ion:119 Resp: 6746
Ion Ratio Lower Upper
119 100
134 29.6 12.9 38.7
91 30.9 11.7 35.0

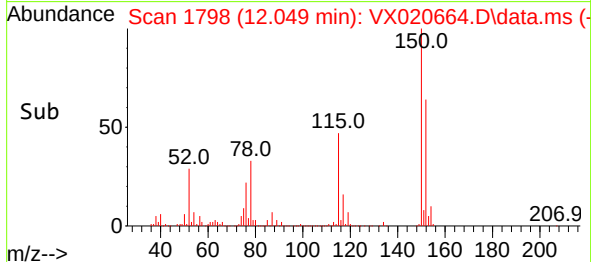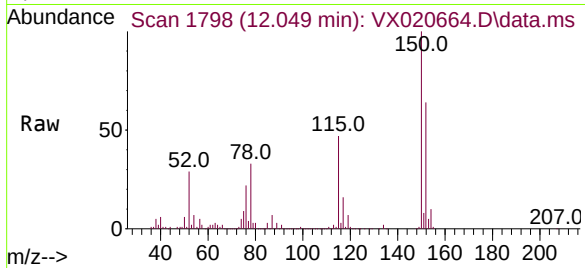

#89
n-Butylbenzene
Concen: 1.51 ug/l
RT: 12.372 min Scan# 1851
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion: 91 Resp: 962
Ion Ratio Lower Upper
91 100
92 53.0 27.4 82.0
134 57.9 13.2 39.5#




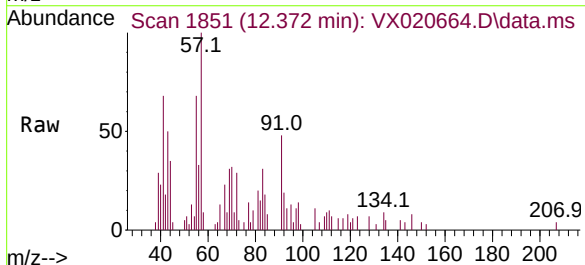




#93
1,2,4-Trichlorobenzene
Concen: 2.29 ug/l
RT: 13.634 min Scan# 2058
Delta R.T. 0.006 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Instrument :
MSVOA_X
ClientSampled :
1693-94

Tgt Ion:180 Resp: 226
Ion Ratio Lower Upper
180 100
182 152.2 47.7 143.1#
145 61.1 15.0 45.0#

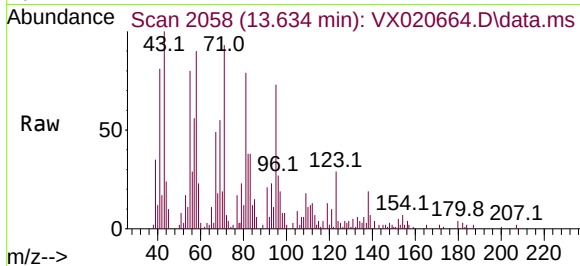

#95
Naphthalene
Concen: 2.92 ug/l
RT: 13.817 min Scan# 2088
Delta R.T. -0.000 min
Lab File: VX020664.D
Acq: 19 Jan 2021 17:17

Tgt Ion:128 Resp: 13801
Ion Ratio Lower Upper
128 100
127 16.8 10.3 15.5#
129 13.2 8.8 13.2#

