

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011921\
 Data File : VX020671.D
 Acq On : 19 Jan 2021 19:59
 Operator : JC/SP
 Sample : M1125-09 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1714-1715

Quant Time: Jan 20 03:22:27 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 19 14:09:08 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	240005	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	422856	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.098	117	389668	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	185834	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	166293	50.68	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	101.36%
35) Dibromofluoromethane	5.458	113	140936	48.38	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.76%
50) Toluene-d8	8.696	98	517675	49.28	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.56%
62) 4-Bromofluorobenzene	11.122	95	194494	48.98	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	97.96%

Target Compounds						Qvalue
6) Chloroethane	1.721	64	181	Below Cal	#	43
11) Tert butyl alcohol	3.002	59	12220	21.00	ug/l	100
13) Acrolein	2.239	56	113	30.59	ug/l #	1
16) Acetone	2.410	43	357308	280.38	ug/l	98
25) 2-Butanone	4.641	43	1140	0.61	ug/l	94
31) Cyclohexane	5.629	56	6556	1.53	ug/l #	1
36) 1,1-Dichloropropene	5.629	75	19417	4.56	ug/l #	49
37) Ethyl Acetate	4.641	43	1140	0.29	ug/l #	64
38) Carbon Tetrachloride	5.629	117	24756	5.44	ug/l #	16
39) Methylcyclohexane	7.440	83	3615	0.75	ug/l #	92
40) Benzene	6.111	78	4548	0.36	ug/l	95
52) Toluene	8.763	92	186520	24.30	ug/l	99
53) t-1,3-Dichloropropene	8.763	75	2408	0.52	ug/l #	1
56) Ethyl methacrylate	9.141	69	96	2.11	ug/l #	1
67) Ethyl Benzene	10.232	91	15598	1.09	ug/l	100
68) m/p-Xylenes	10.342	106	19266	3.63	ug/l	97
69) o-Xylene	10.683	106	8398	1.65	ug/l	96
70) Styrene	10.683	104	1006	1.52	ug/l #	1
74) N-amyl acetate	10.890	43	150	1.97	ug/l #	1
76) 1,2,3-Trichloropropane	11.122	75	93242	20.91	ug/l #	39
78) n-propylbenzene	11.341	91	6580	0.44	ug/l	97
79) 2-Chlorotoluene	11.415	91	3119	0.34	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.488	105	6394	0.58	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.122	75	93242	60.48	ug/l #	12
83) tert-Butylbenzene	12.012	119	2171	0.20	ug/l	68
84) 1,2,4-Trimethylbenzene	11.787	105	24570	2.43	ug/l	98
86) p-Isopropyltoluene	12.012	119	2171	1.05	ug/l	88
89) n-Butylbenzene	12.372	91	4006	1.78	ug/l #	53
90) Hexachloroethane	12.567	117	532	0.26	ug/l #	9
93) 1,2,4-Trichlorobenzene	13.628	180	114	2.27	ug/l #	1
95) Naphthalene	13.817	128	572197	41.75	ug/l	100





(#) = qualifier out of range (m) = manual integration (+) = signals summed

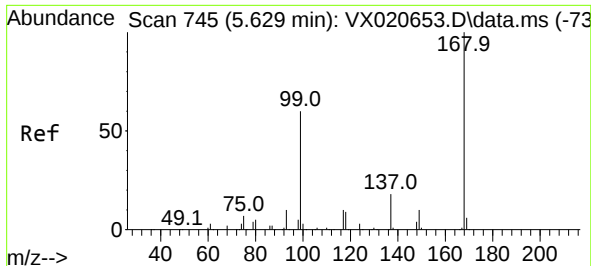

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59



Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion:168 Resp: 240005
Ion Ratio Lower Upper
168 100
99 62.7 45.8 68.6

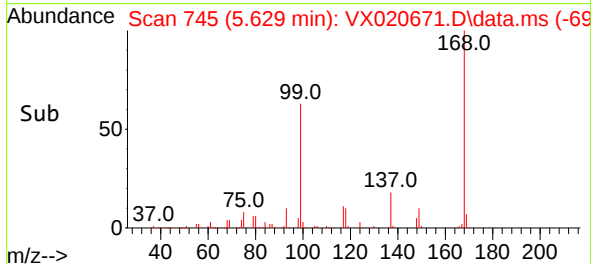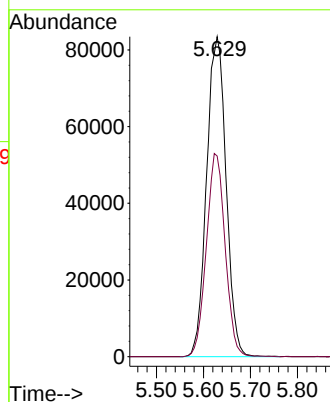

#6
Chloroethane
Concen: Below Cal
RT: 1.721 min Scan# 104
Delta R.T. 0.012 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion: 64 Resp: 181
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

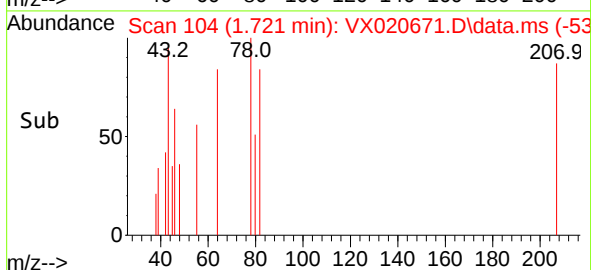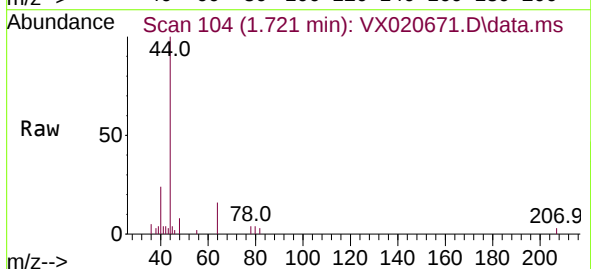




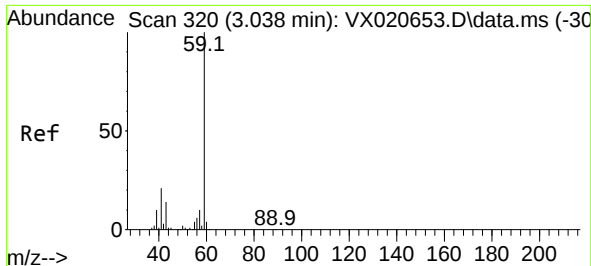


#11

Tert butyl alcohol
Concen: 21.00 ug/l
RT: 3.002 min Scan# 314
Delta R.T. -0.036 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Instrument :
MSVOA_X
ClientSampleId :
1714-1715




Tgt Ion: 59 Resp: 12220
Ion Ratio Lower Upper
59 100
57 10.0 7.8 11.8

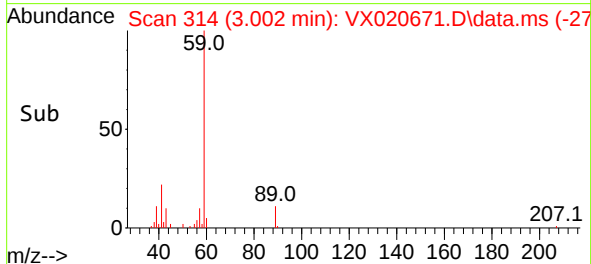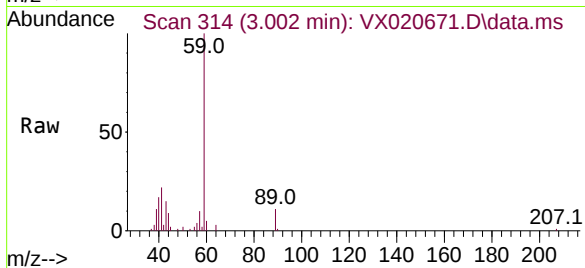


#13

Acrolein
Concen: 30.59 ug/l
RT: 2.239 min Scan# 189
Delta R.T. -0.031 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion: 56 Resp: 113
Ion Ratio Lower Upper
56 100
55 999.1 56.4 84.6#


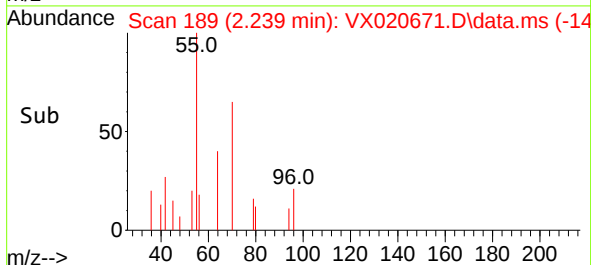

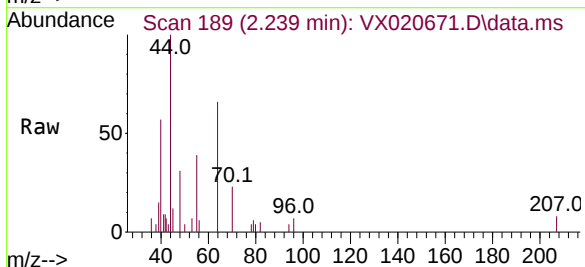


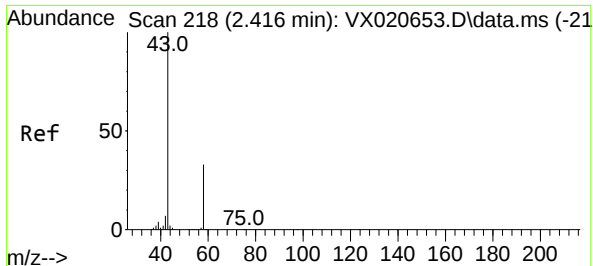

#16
Acetone
Concen: 280.38 ug/l
RT: 2.410 min Scan# 217
Delta R.T. -0.006 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion: 43 Resp: 357308
Ion Ratio Lower Upper
43 100
58 33.4 27.8 41.8

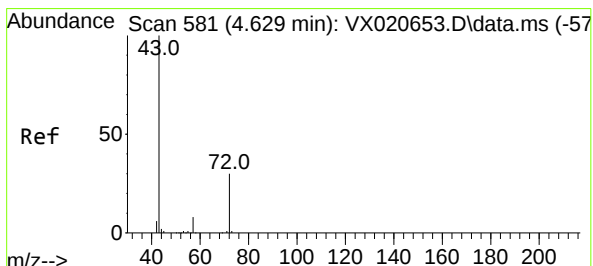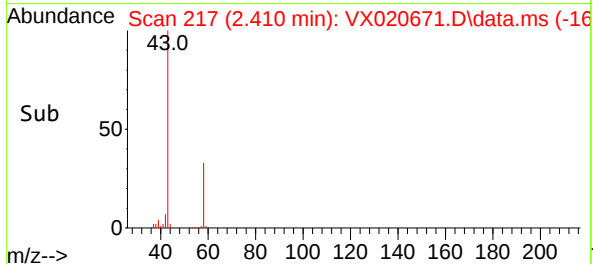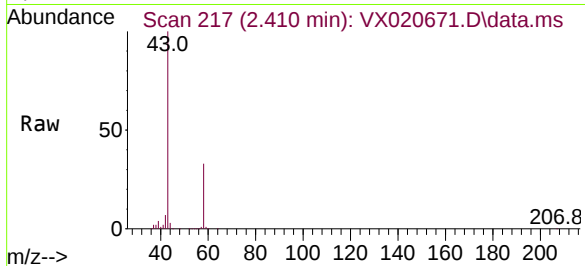

#25
2-Butanone
Concen: 0.61 ug/l
RT: 4.641 min Scan# 583
Delta R.T. 0.012 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59


Tgt Ion: 43 Resp: 1140
Ion Ratio Lower Upper
43 100
72 26.3 23.7 35.5

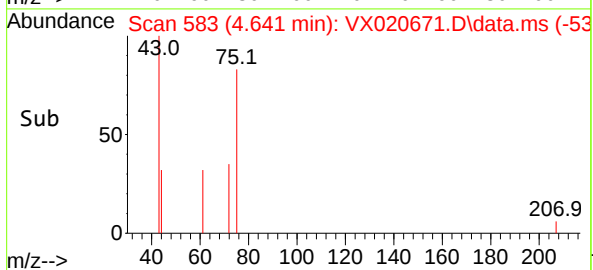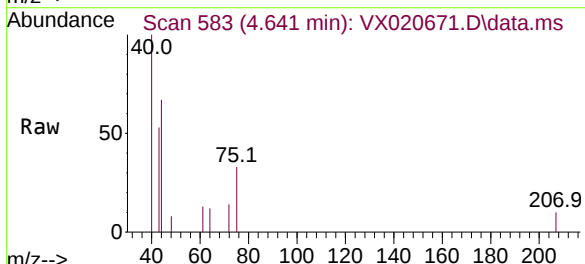



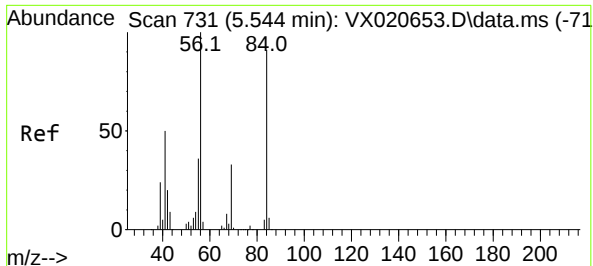


#31
Cyclohexane
Concen: 1.53 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.085 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59


Instrument :
MSVOA_X
ClientSampleId :
1714-1715

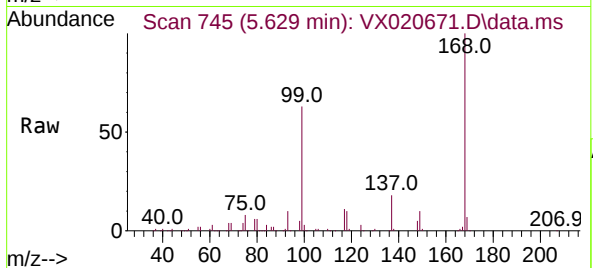



Tgt Ion: 56 Resp: 6556
Ion Ratio Lower Upper
56 100
69 176.2 25.3 37.9#
84 138.9 71.4 107.0#

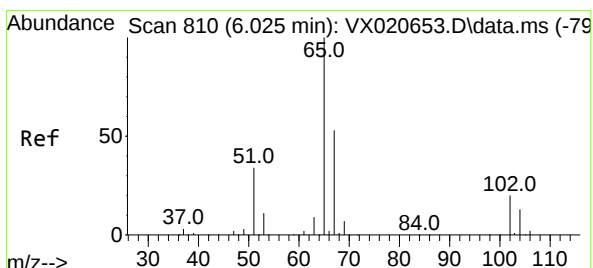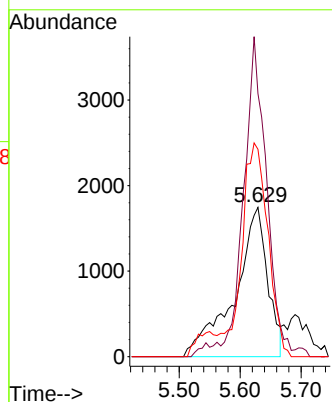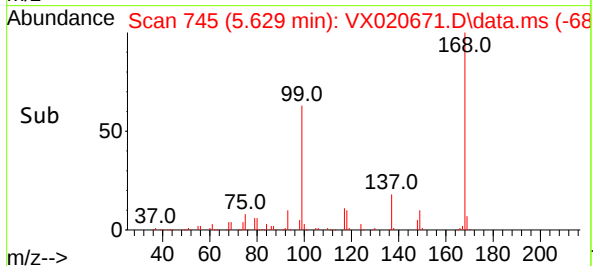


#33
1,2-Dichloroethane-d4
Concen: 50.68 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.006 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

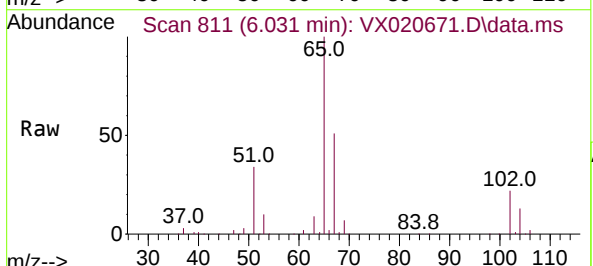

Tgt Ion: 65 Resp: 166293
Ion Ratio Lower Upper
65 100
67 52.6 0.0 105.4

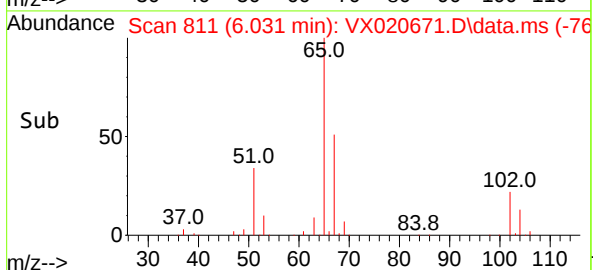

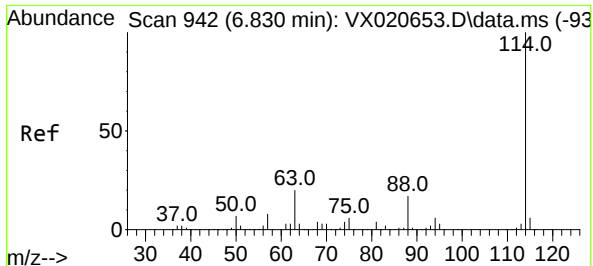

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.830 min Scan# 942

Delta R.T. 0.000 min

Lab File: VX020671.D

Acq: 19 Jan 2021 19:59

Tgt Ion:114 Resp: 422856

Ion Ratio Lower Upper

114 100

63 20.6 0.0 40.8





88 16.6 0.0 32.8

Instrument :

MSVOA_X

ClientSampleId :

1714-1715

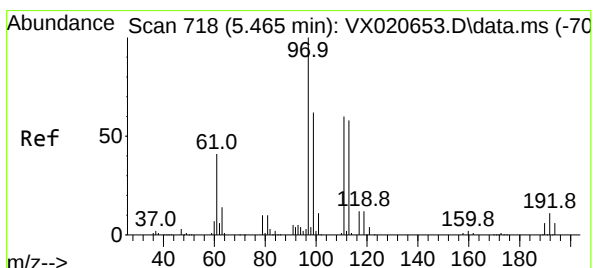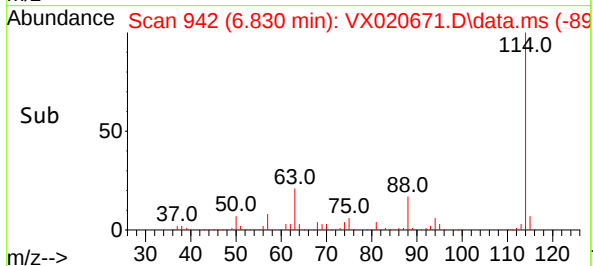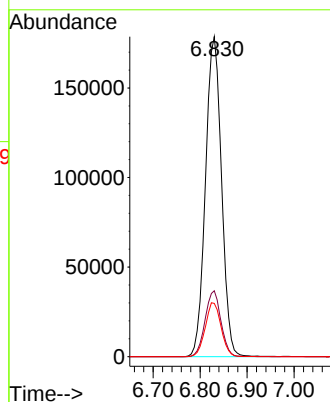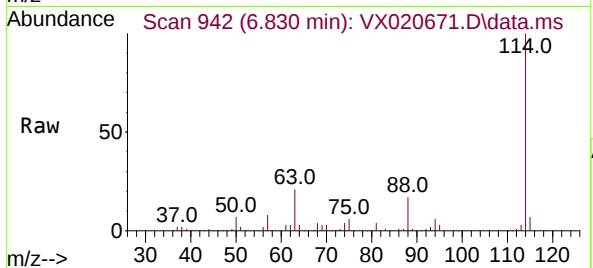

#35

Dibromofluoromethane

Concen: 48.38 ug/l

RT: 5.458 min Scan# 717

Delta R.T. -0.007 min

Lab File: VX020671.D

Acq: 19 Jan 2021 19:59




Tgt Ion:113 Resp: 140936


Ion Ratio Lower Upper

113 100

111 102.8 81.9 122.9

192 19.4 16.7 25.1


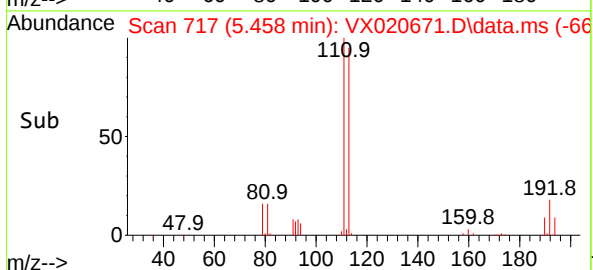

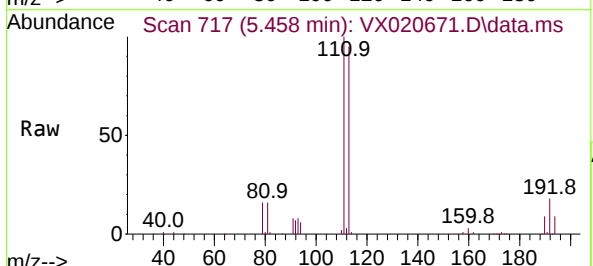


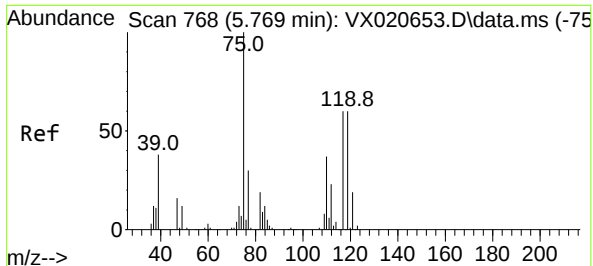

#36
1,1-Dichloropropene
Concen: 4.56 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.140 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion: 75 Resp: 19417
Ion Ratio Lower Upper
75 100
110 9.0 18.1 54.4#
77 0.0 25.3 37.9#

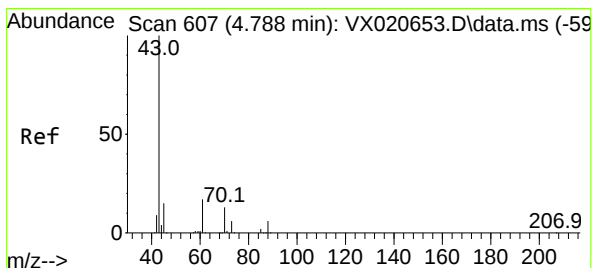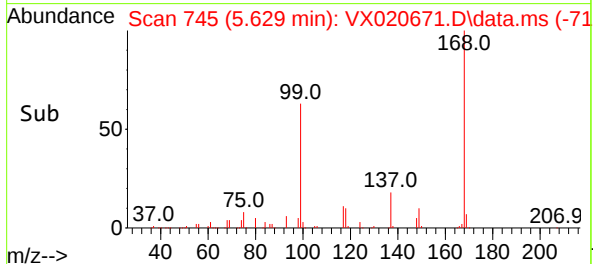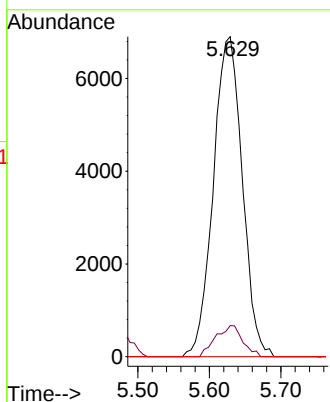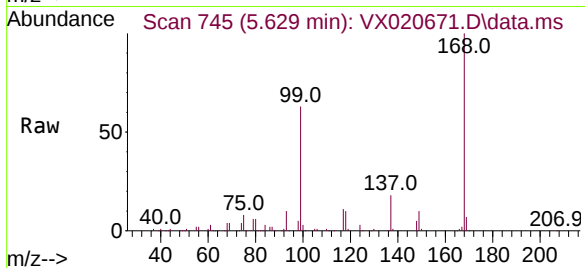

#37
Ethyl Acetate
Concen: 0.29 ug/l
RT: 4.641 min Scan# 583
Delta R.T. -0.147 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59


Tgt Ion: 43 Resp: 1140
Ion Ratio Lower Upper
43 100
61 0.0 12.8 19.2#
70 0.0 10.5 15.7#

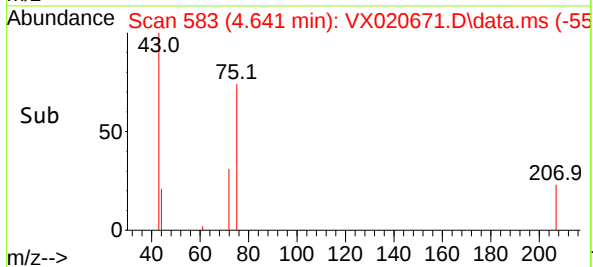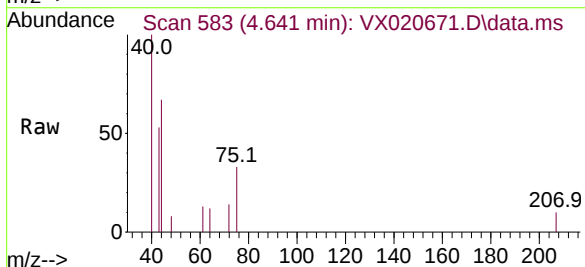



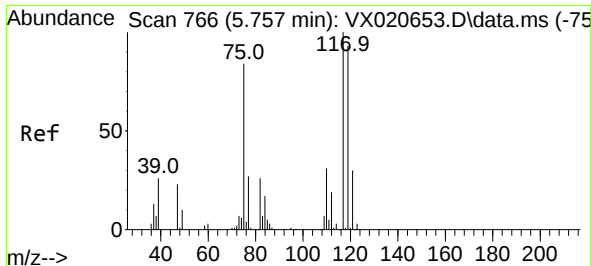


#38
Carbon Tetrachloride
Concen: 5.44 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.128 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59


Instrument :
MSVOA_X
ClientSampleId :
1714-1715





Tgt Ion:117 Resp: 24756
Ion Ratio Lower Upper
117 100
119 5.1 76.2 114.2#
121 0.0 24.8 37.2#

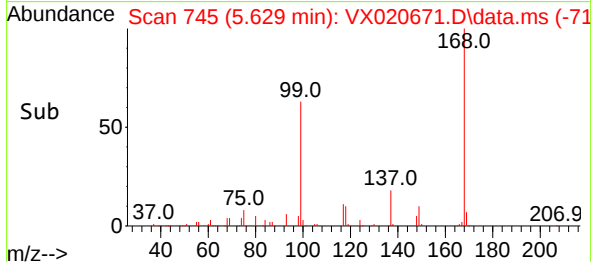


#39
Methylcyclohexane
Concen: 0.75 ug/l
RT: 7.440 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

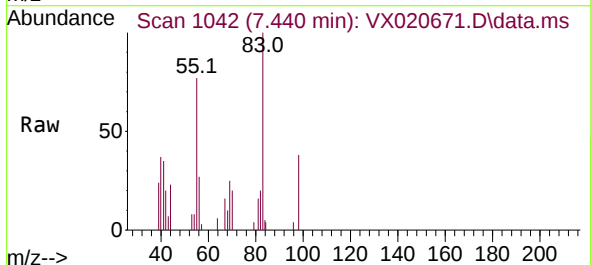

Tgt Ion: 83 Resp: 3615
Ion Ratio Lower Upper
83 100
55 77.0 58.9 88.3
98 37.9 38.1 57.1#



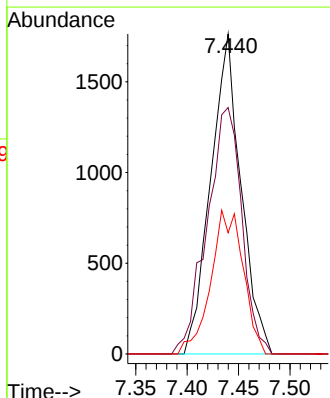
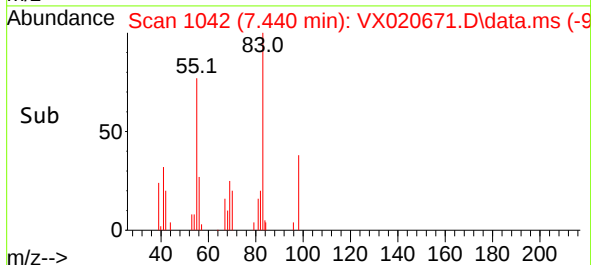


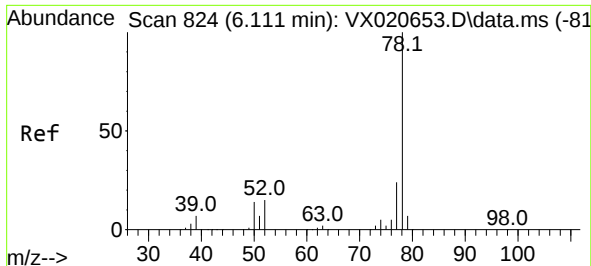

#40
Benzene
Concen: 0.36 ug/l
RT: 6.111 min Scan# 824
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion: 78 Resp: 4548
Ion Ratio Lower Upper
78 100
77 26.3 18.9 28.3

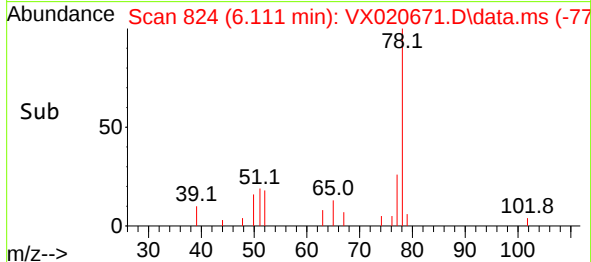

#50
Toluene-d8
Concen: 49.28 ug/l
RT: 8.696 min Scan# 1248
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion: 98 Resp: 517675
Ion Ratio Lower Upper
98 100
100 64.4 51.9 77.9


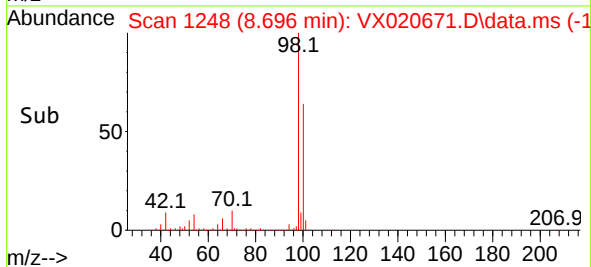

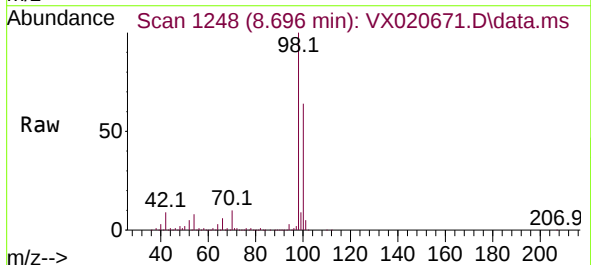


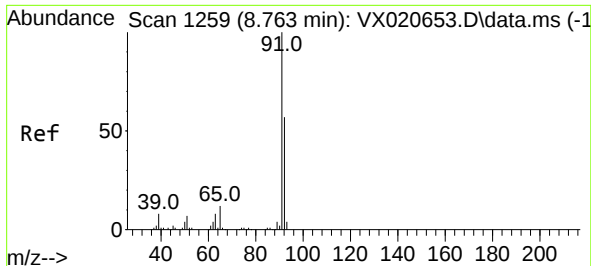

#52
Toluene
Concen: 24.30 ug/l
RT: 8.763 min Scan# 1259
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion: 92 Resp: 186520
Ion Ratio Lower Upper
92 100
91 172.6 137.1 205.7

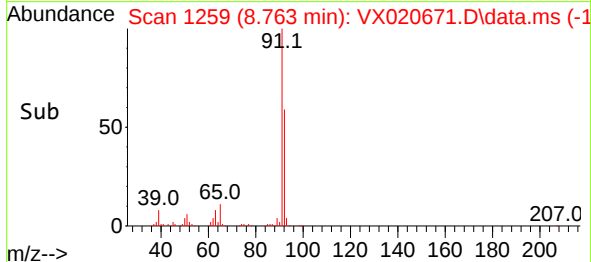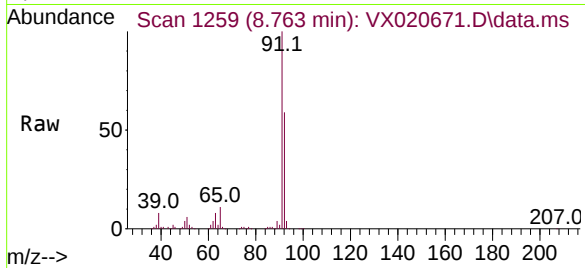

#53
t-1,3-Dichloropropene
Concen: 0.52 ug/l
RT: 8.763 min Scan# 1259
Delta R.T. -0.256 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion: 75 Resp: 2408
Ion Ratio Lower Upper
75 100
77 158.2 24.9 37.3#


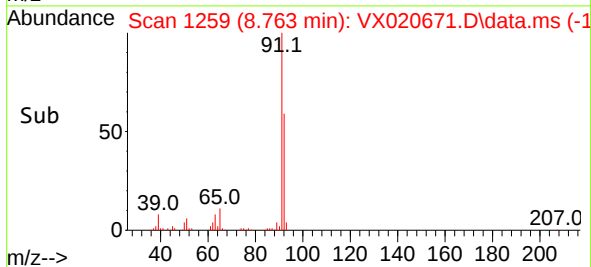

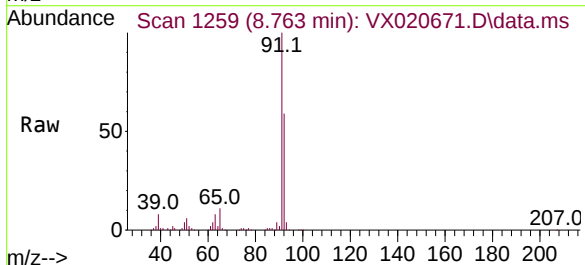


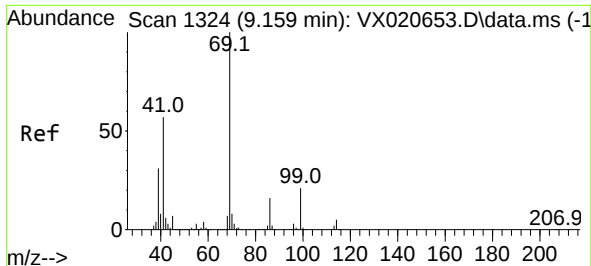

#56
Ethyl methacrylate
Concen: 2.11 ug/l
RT: 9.141 min Scan# 1321
Delta R.T. -0.018 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampled :
1714-1715


Tgt Ion: 69	Resp: 96
Ion Ratio	Lower Upper
69 100	
41 203.1	46.8 70.2#
39 109.4	24.7 37.1#

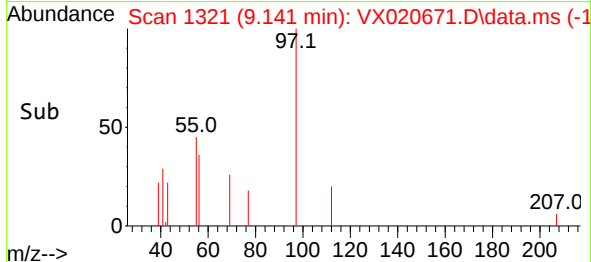

#62
4-Bromofluorobenzene
Concen: 48.98 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion: 95	Resp: 194494
Ion Ratio	Lower Upper
95 100	
174 75.3	0.0 154.6
176 71.6	0.0 155.8


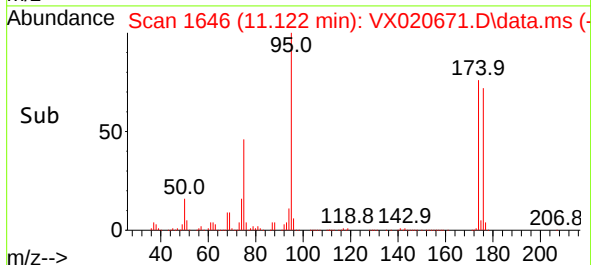
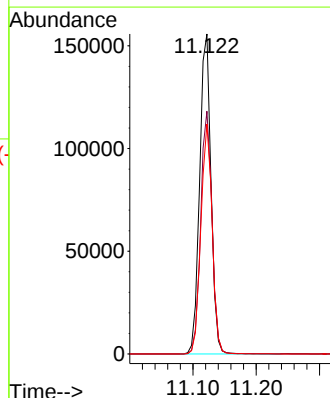
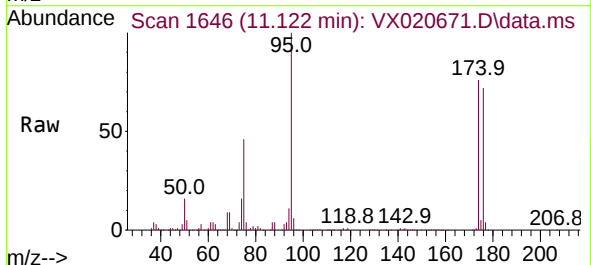




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.098 min Scan# 1478
Delta R.T. 0.006 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion:117 Resp: 389668
Ion Ratio Lower Upper
117 100
82 55.9 47.4 71.2
119 31.8 26.6 39.8

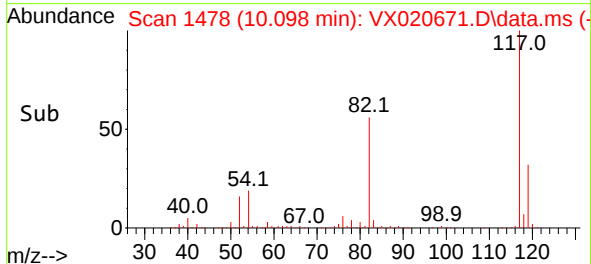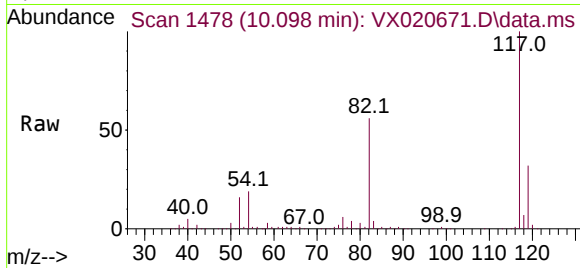

#67
Ethyl Benzene
Concen: 1.09 ug/l
RT: 10.232 min Scan# 1500
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion: 91 Resp: 15598
Ion Ratio Lower Upper
91 100
106 31.0 24.6 37.0


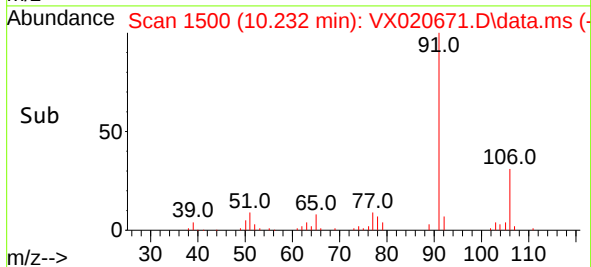

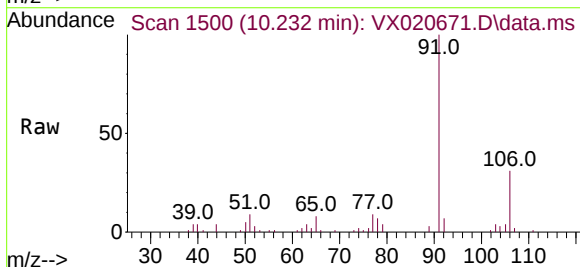




#68
m/p-Xylenes
Concen: 3.63 ug/l
RT: 10.342 min Scan# 1518
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion:106 Resp: 19266
Ion Ratio Lower Upper
106 100
91 207.6 162.8 244.2

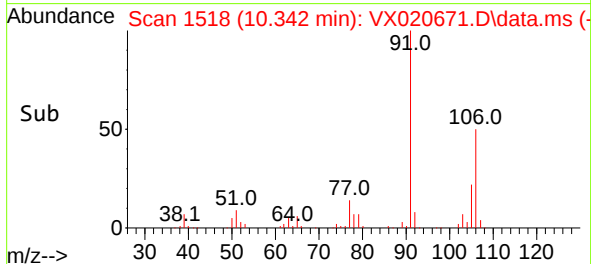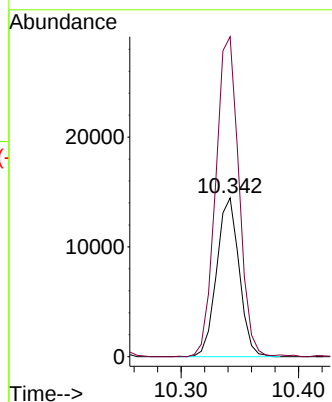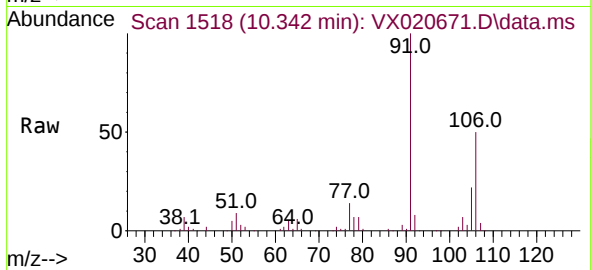

#69
o-Xylene
Concen: 1.65 ug/l
RT: 10.683 min Scan# 1574
Delta R.T. 0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion:106 Resp: 8398
Ion Ratio Lower Upper
106 100
91 222.4 108.1 324.2

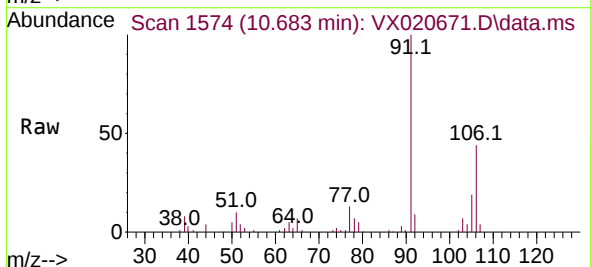



#70

Styrene

Concen: 1.52 ug/l

RT: 10.683 min Scan# 1574





Delta R.T. -0.012 min

Lab File: VX020671.D

Acq: 19 Jan 2021 19:59

Tgt Ion:104	Resp:	1006
Ion Ratio	Lower	Upper
104	100	
78	149.5	40.0 60.0#
103	149.1	43.4 65.0#

Instrument :
MSVOA_X
ClientSampleId :
1714-1715

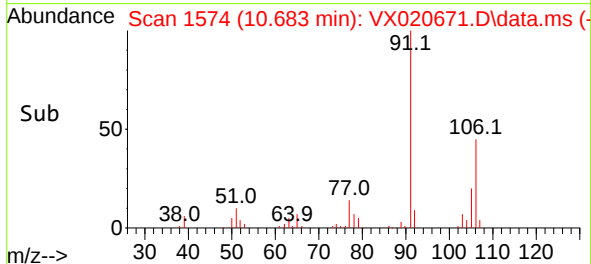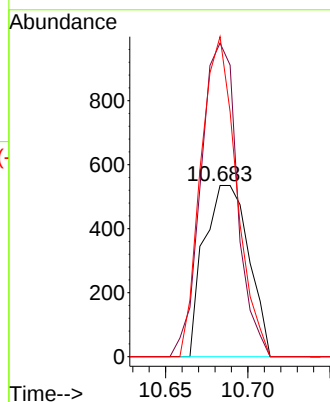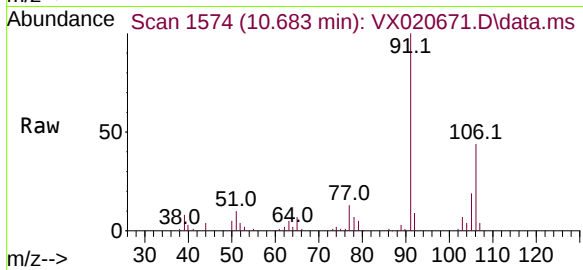

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l




RT: 12.061 min Scan# 1800


Delta R.T. -0.000 min

Lab File: VX020671.D

Acq: 19 Jan 2021 19:59

Tgt Ion:152	Resp:	185834
Ion Ratio	Lower	Upper
152	100	
115	61.4	41.1 123.3
150	157.2	0.0 349.0




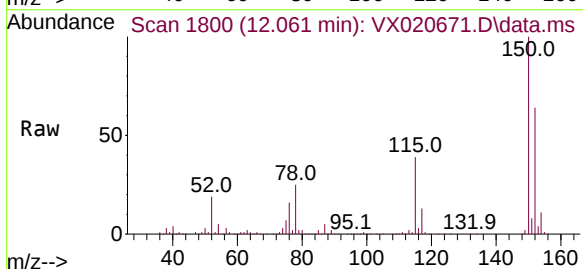


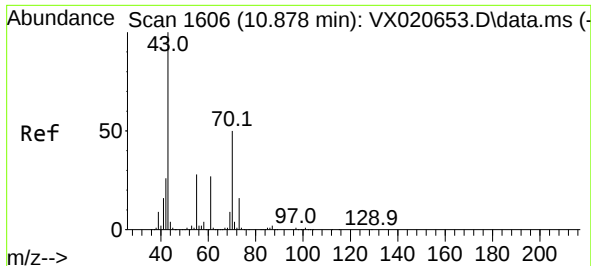

#74
N-amy1 acetate
Concen: 1.97 ug/l
RT: 10.890 min Scan# 1608
Delta R.T. 0.012 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion: 43	Resp:	150
Ion	Ratio	Lower Upper
43	100	
70	100.7	39.0 58.6#
55	568.0	21.5 32.3#
61	0.0	22.1 33.1#

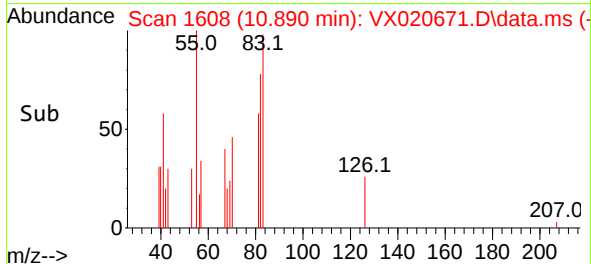

#76
1,2,3-Trichloropropane
Concen: 20.91 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.159 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion: 75	Resp:	93242
Ion	Ratio	Lower Upper
75	100	
77	1.2	19.1 57.5#


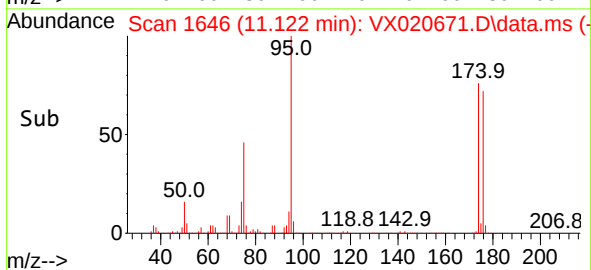

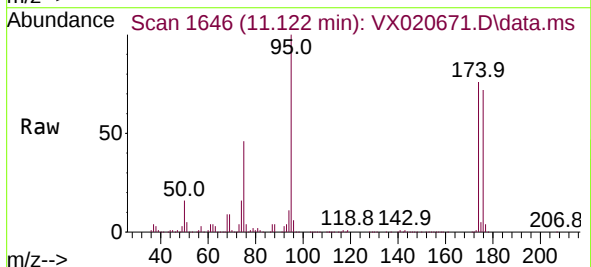


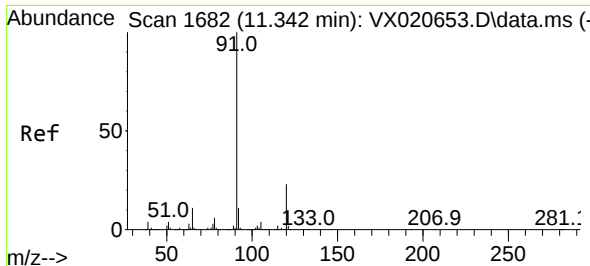

#78
n-propylbenzene
Concen: 0.44 ug/l
RT: 11.341 min Scan# 1682
Delta R.T. -0.001 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion: 91 Resp: 6580
Ion Ratio Lower Upper
91 100
120 24.3 11.5 34.5

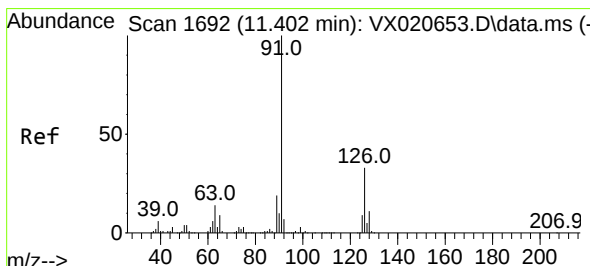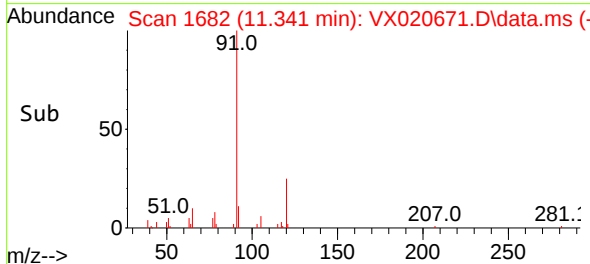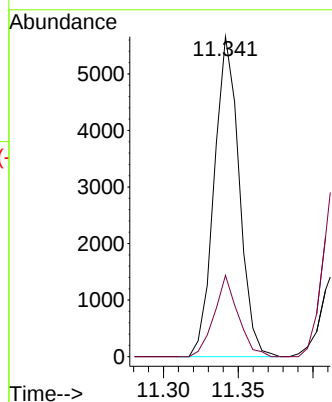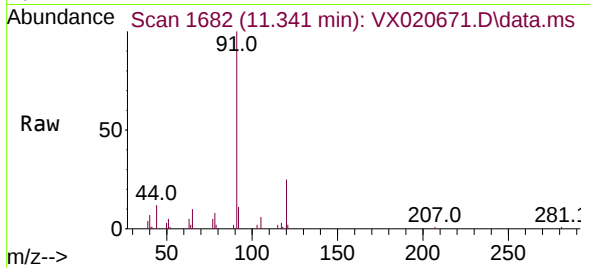

#79
2-Chlorotoluene
Concen: 0.34 ug/l
RT: 11.415 min Scan# 1694
Delta R.T. 0.013 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion: 91 Resp: 3119
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#


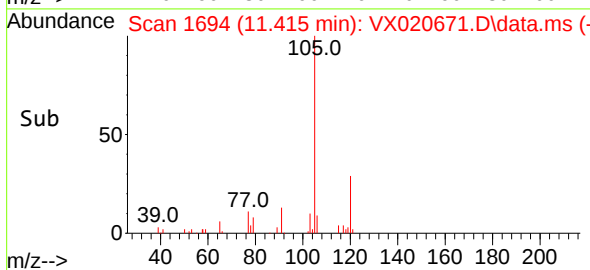

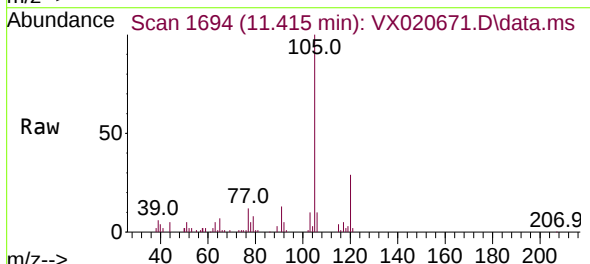


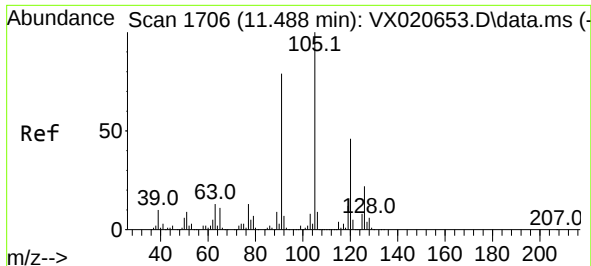

#80
1,3,5-Trimethylbenzene
Concen: 0.58 ug/l
RT: 11.488 min Scan# 1706
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion:105 Resp: 6394
Ion Ratio Lower Upper
105 100
120 45.8 23.8 71.5

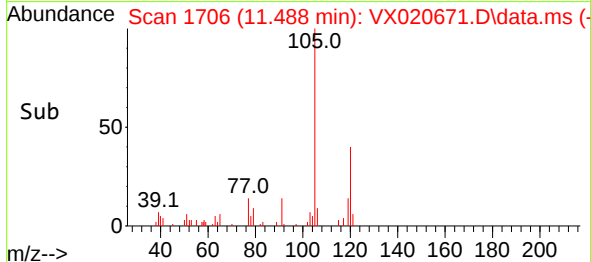

#81
trans-1,4-Dichloro-2-butene
Concen: 60.48 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. 0.067 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion: 75 Resp: 93242
Ion Ratio Lower Upper
75 100
53 0.1 74.5 111.7#
89 0.0 37.9 56.9#


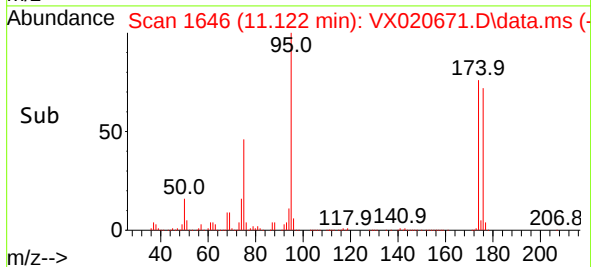

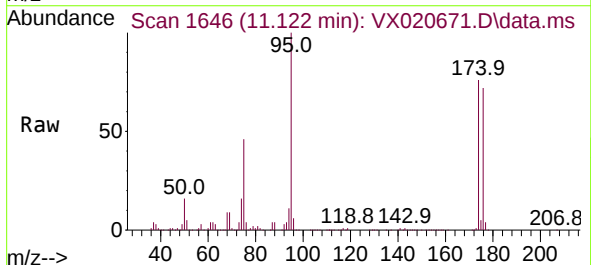




#83
tert-Butylbenzene
Concen: 0.20 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. 0.256 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion:119 Resp: 2171
Ion Ratio Lower Upper
119 100
91 29.2 27.9 83.7
134 32.2 11.3 33.9

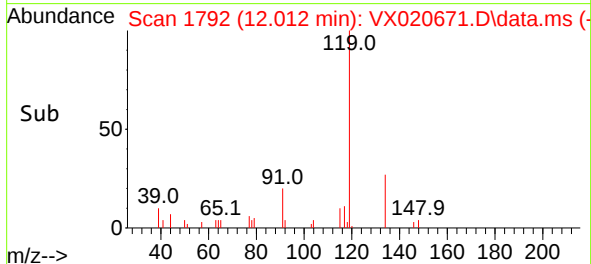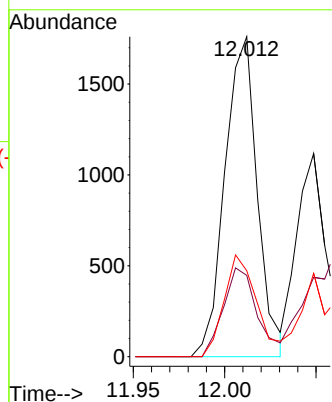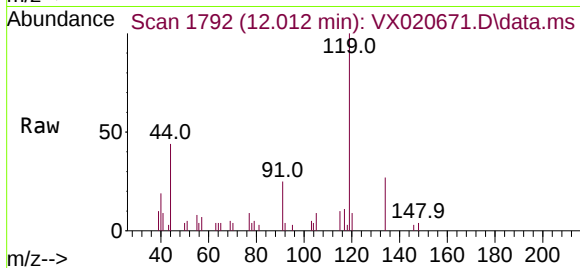

#84
1,2,4-Trimethylbenzene
Concen: 2.43 ug/l
RT: 11.787 min Scan# 1755
Delta R.T. -0.006 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion:105 Resp: 24570
Ion Ratio Lower Upper
105 100
120 43.8 22.4 67.3


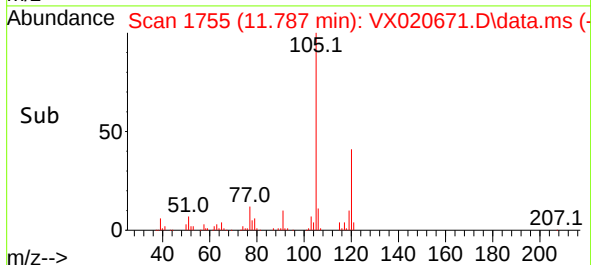

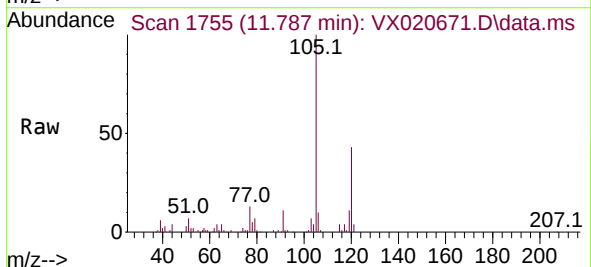


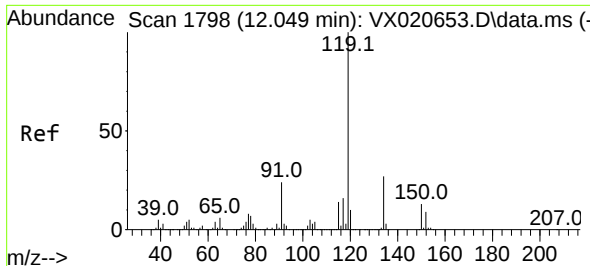

#86
p-Isopropyltoluene
Concen: 1.05 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. -0.037 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion:119 Resp: 2171
Ion Ratio Lower Upper
119 100
134 32.2 12.9 38.7
91 29.2 11.7 35.0

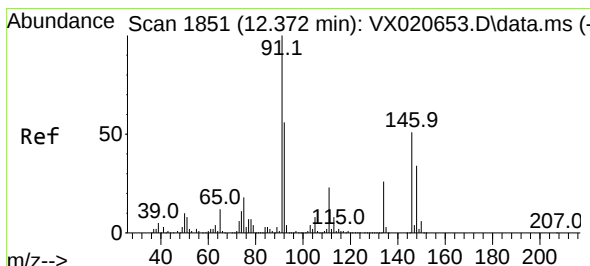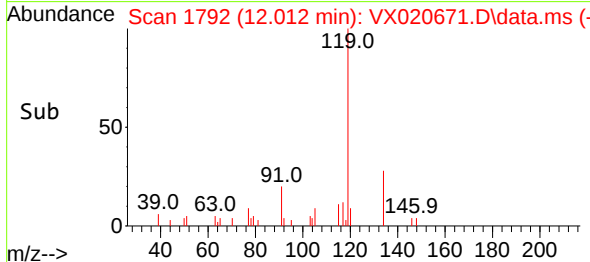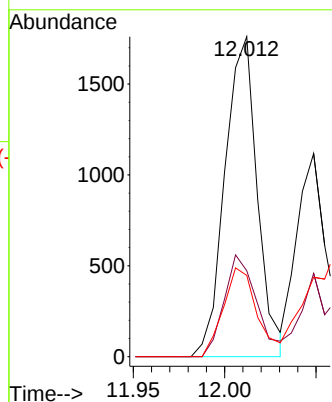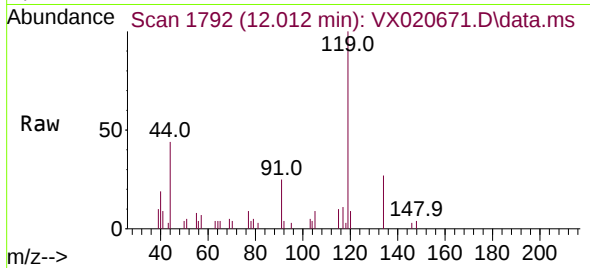

#89
n-Butylbenzene
Concen: 1.78 ug/l
RT: 12.372 min Scan# 1851
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Tgt Ion: 91 Resp: 4006
Ion Ratio Lower Upper
91 100
92 38.0 27.4 82.0
134 75.7 13.2 39.5#


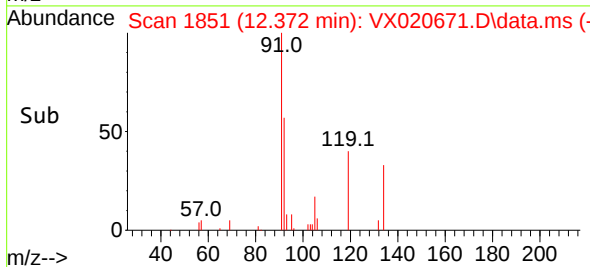

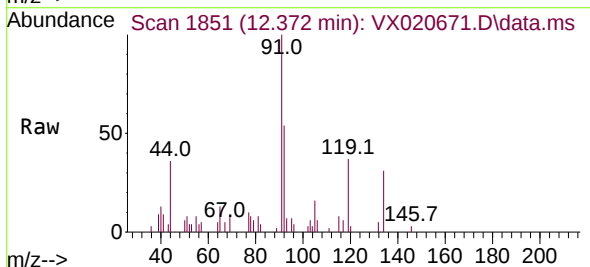




#90
Hexachloroethane
Concen: 0.26 ug/l
RT: 12.567 min Scan# 1883
Delta R.T. -0.012 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59




Instrument :
MSVOA_X
ClientSampleId :
1714-1715


Tgt Ion:117 Resp: 532
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

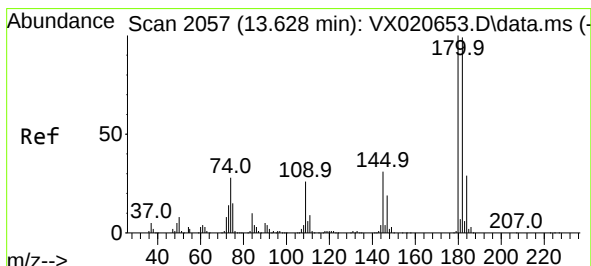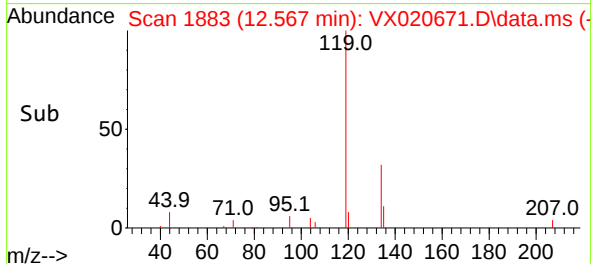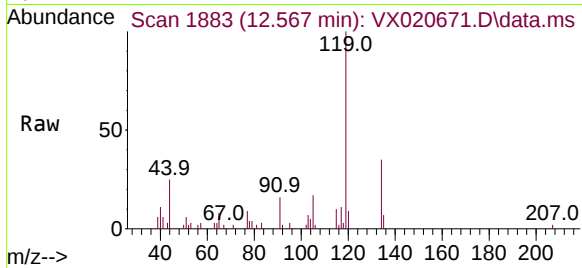

#93
1,2,4-Trichlorobenzene
Concen: 2.27 ug/l
RT: 13.628 min Scan# 2057
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59


Tgt Ion:180 Resp: 114
Ion Ratio Lower Upper
180 100
182 121.1 47.7 143.1
145 355.3 15.0 45.0#

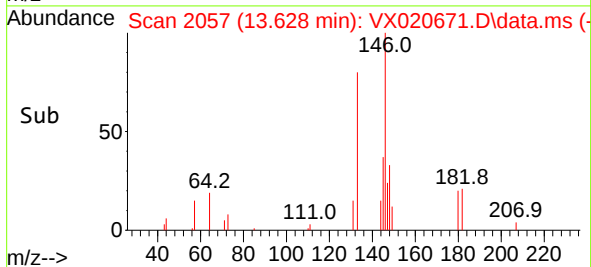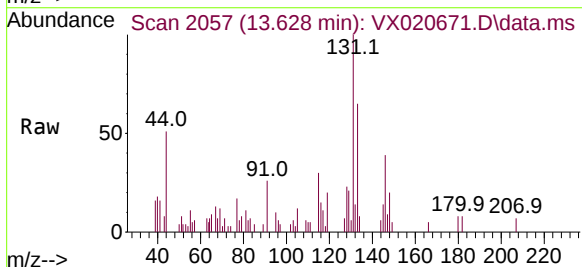

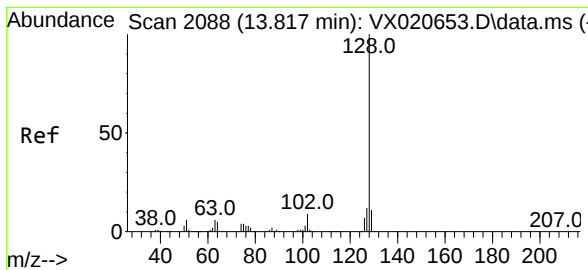

#95
Naphthalene
Concen: 41.75 ug/l
RT: 13.817 min Scan# 2088
Delta R.T. -0.000 min
Lab File: VX020671.D
Acq: 19 Jan 2021 19:59

Instrument :
MSVOA_X
ClientSampleId :
1714-1715

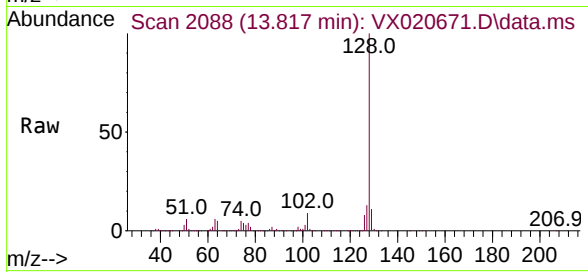

Tgt Ion:128 Resp: 572197
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 11.0 8.8 13.2

