


Dichlorodifluoromethane

Response Ratio

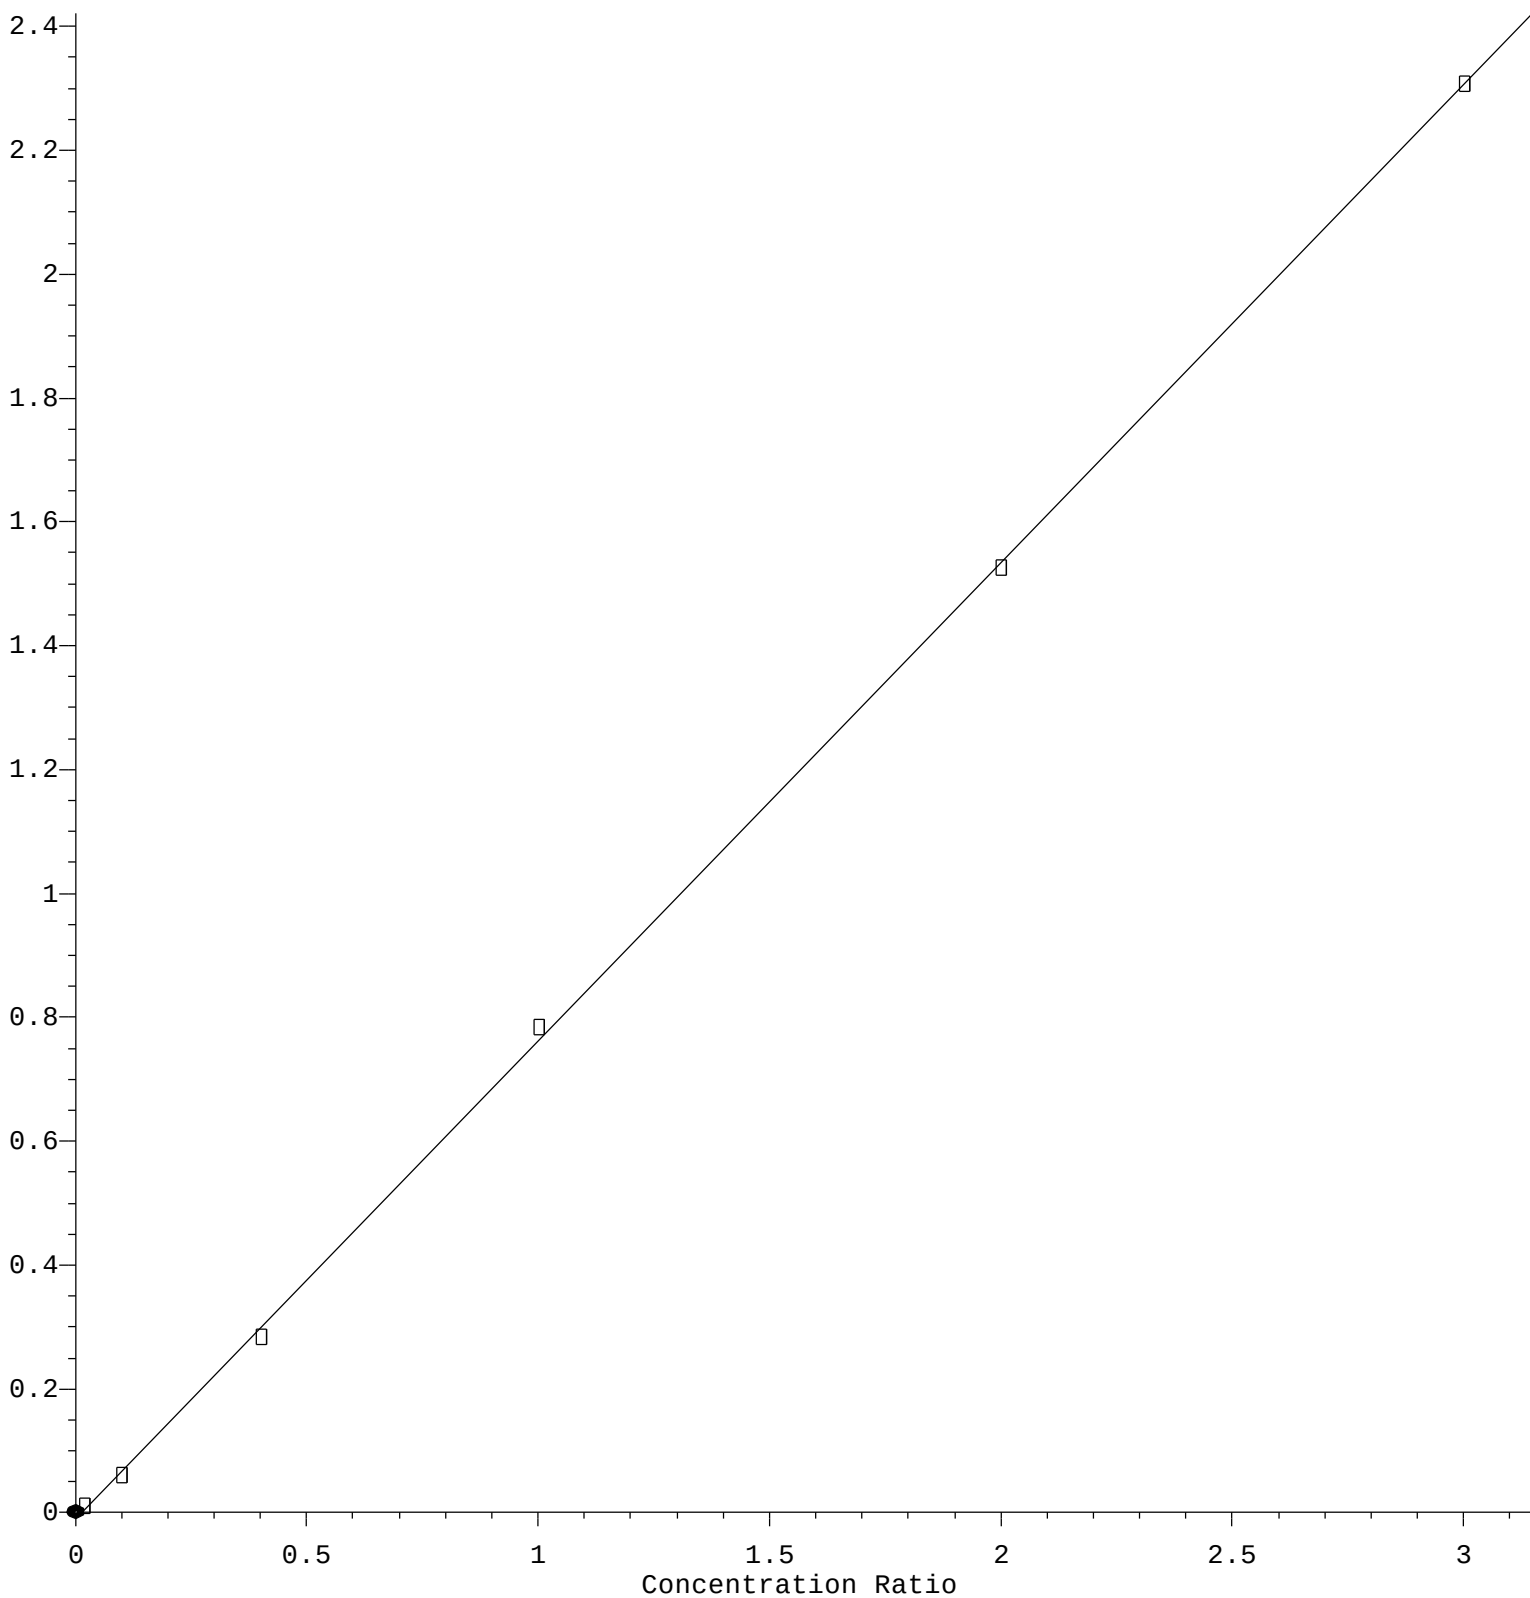

$$\text{Response} = 7.725\text{e-}001 * \text{Amt} - 1.148\text{e-}002$$


Coef of Det (r^2) = 0.999797 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M

Calibration Table Last Updated: Tue Jan 19 14:09:08 2021

Chloroethane


Response Ratio

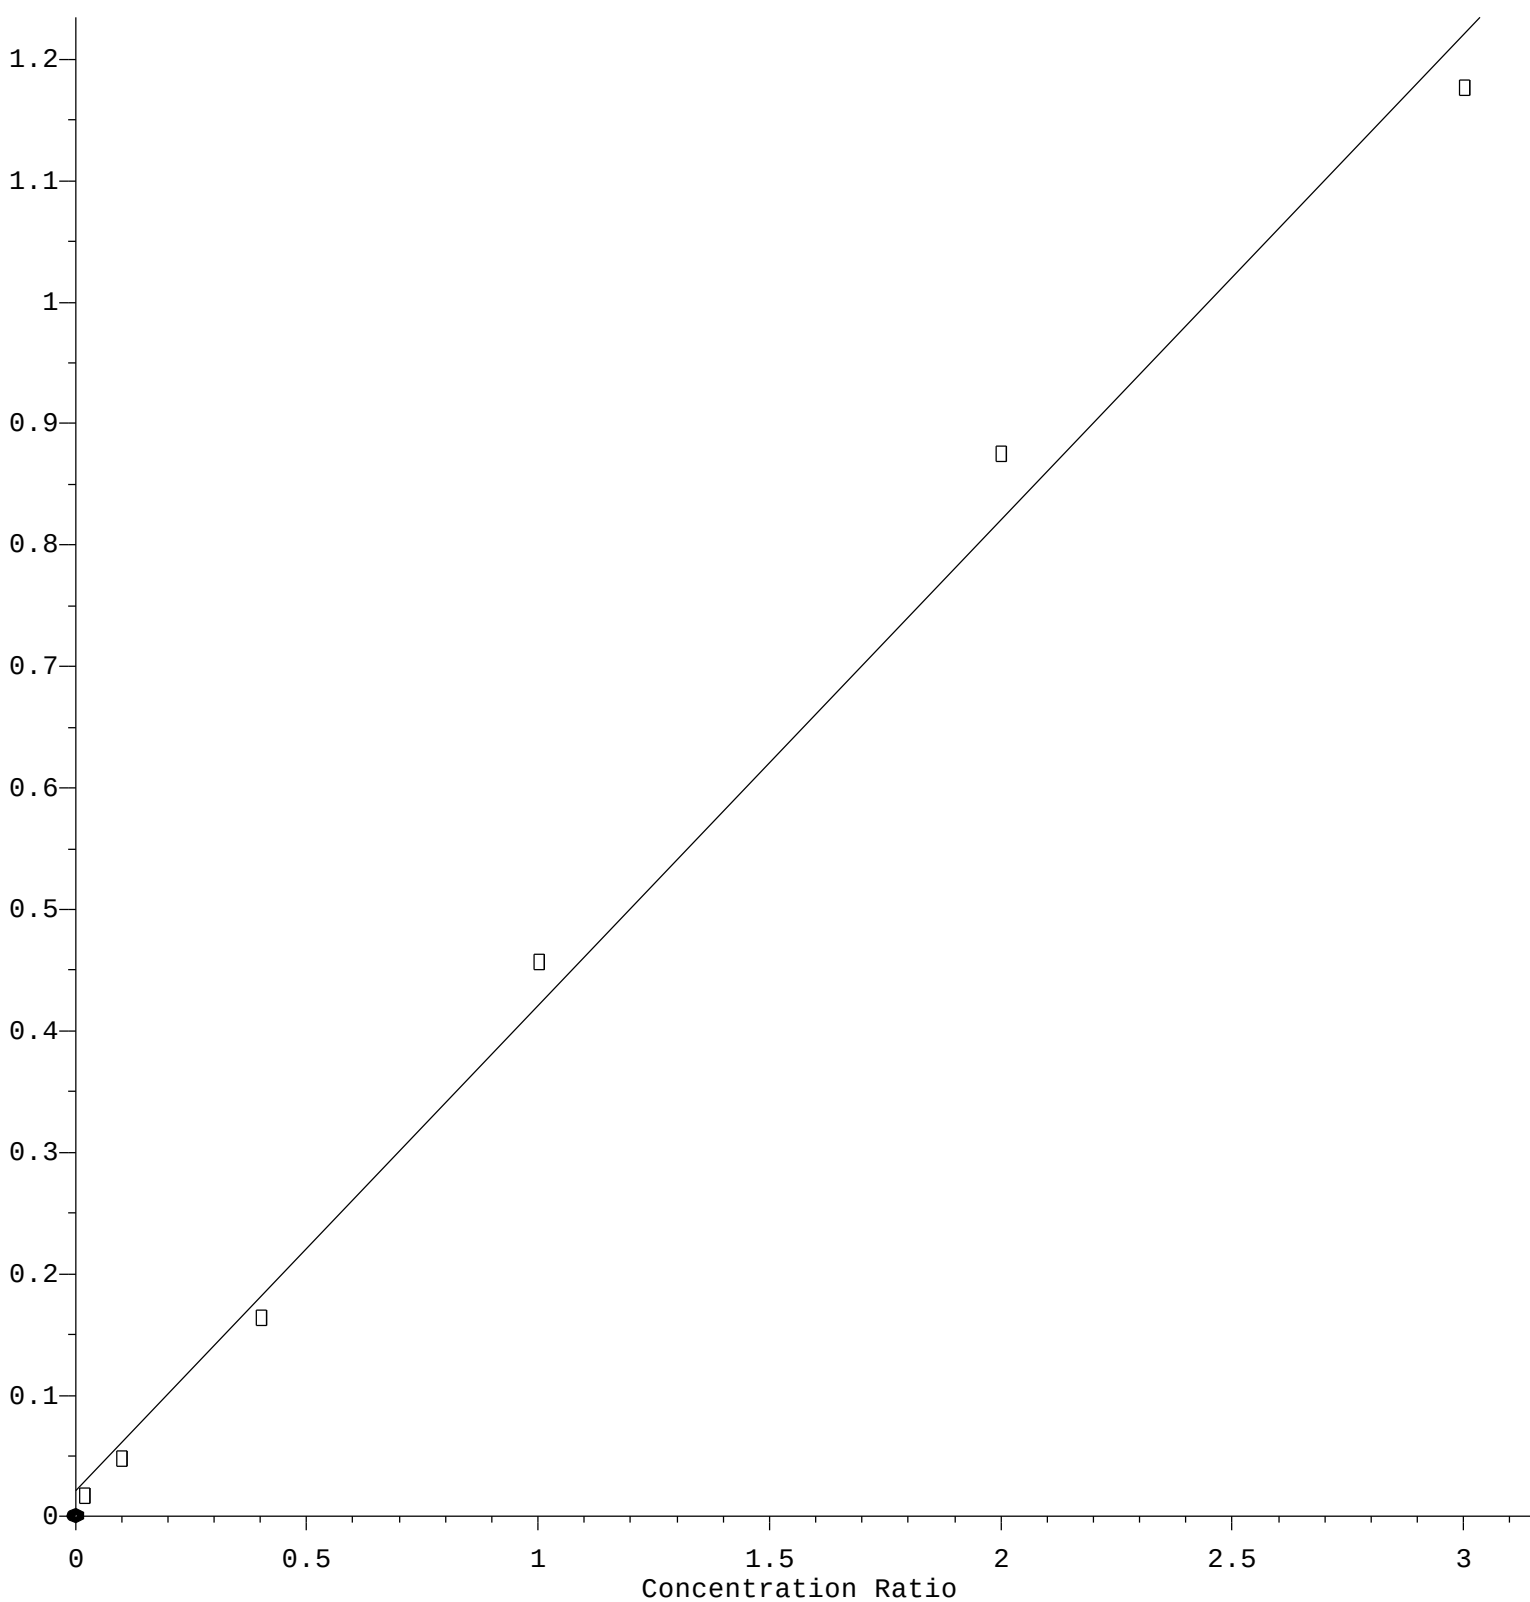

Response = $3.998e-001 * Amt + 2.126e-002$
 Coef of Det (r^2) = 0.993967 Curve Fit: Linear
 Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
 Calibration Table Last Updated: Tue Jan 19 14:09:08 2021

Acrolein


Response Ratio

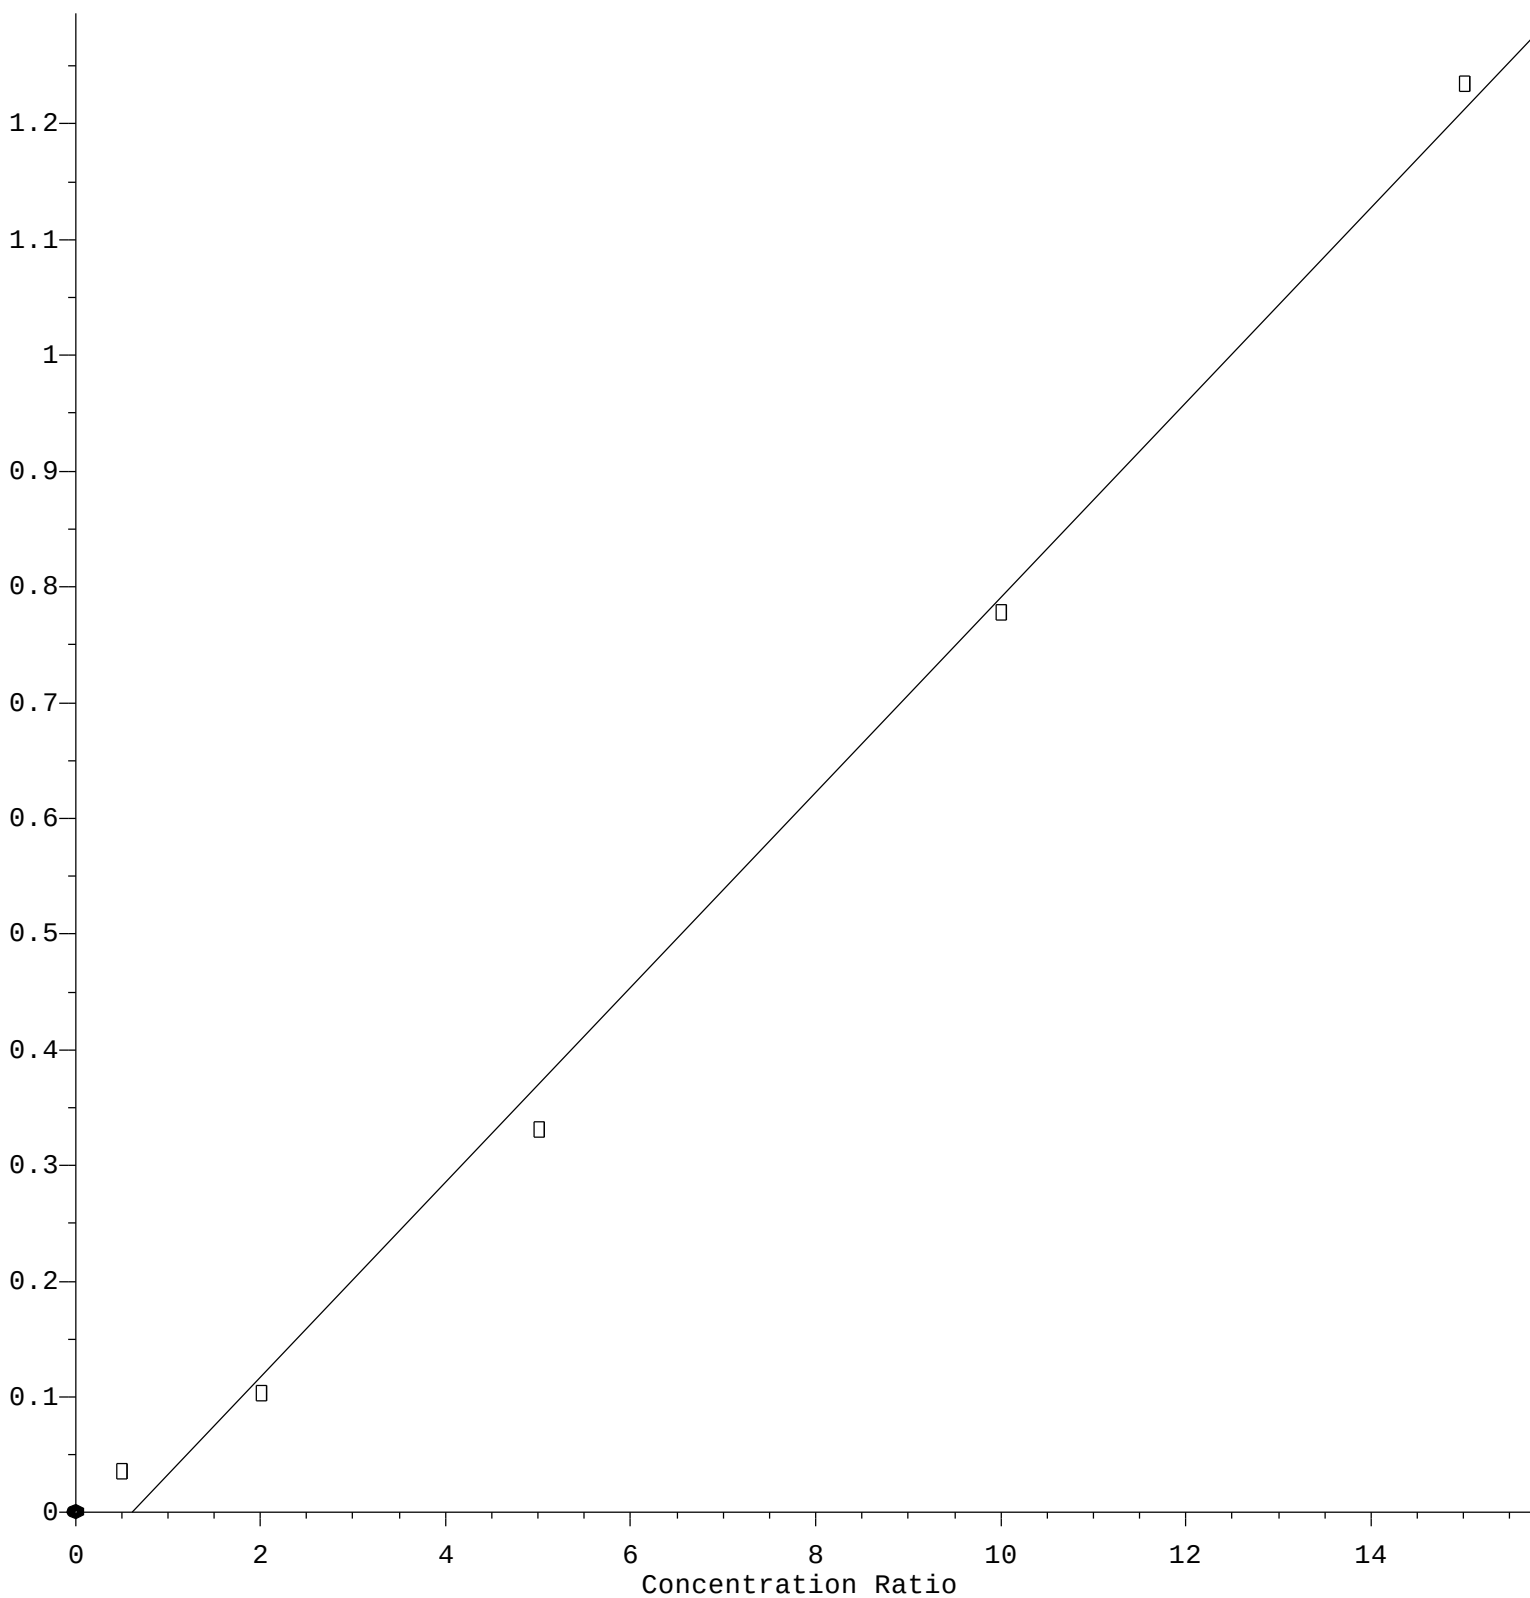

Response = $8.418 \times 10^{-2} \times \text{Amt} - 5.103 \times 10^{-2}$
Coef of Det (r^2) = 0.995744 Curve Fit: Linear
Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
Calibration Table Last Updated: Tue Jan 19 14:09:08 2021

Ethyl methacrylate

Response Ratio

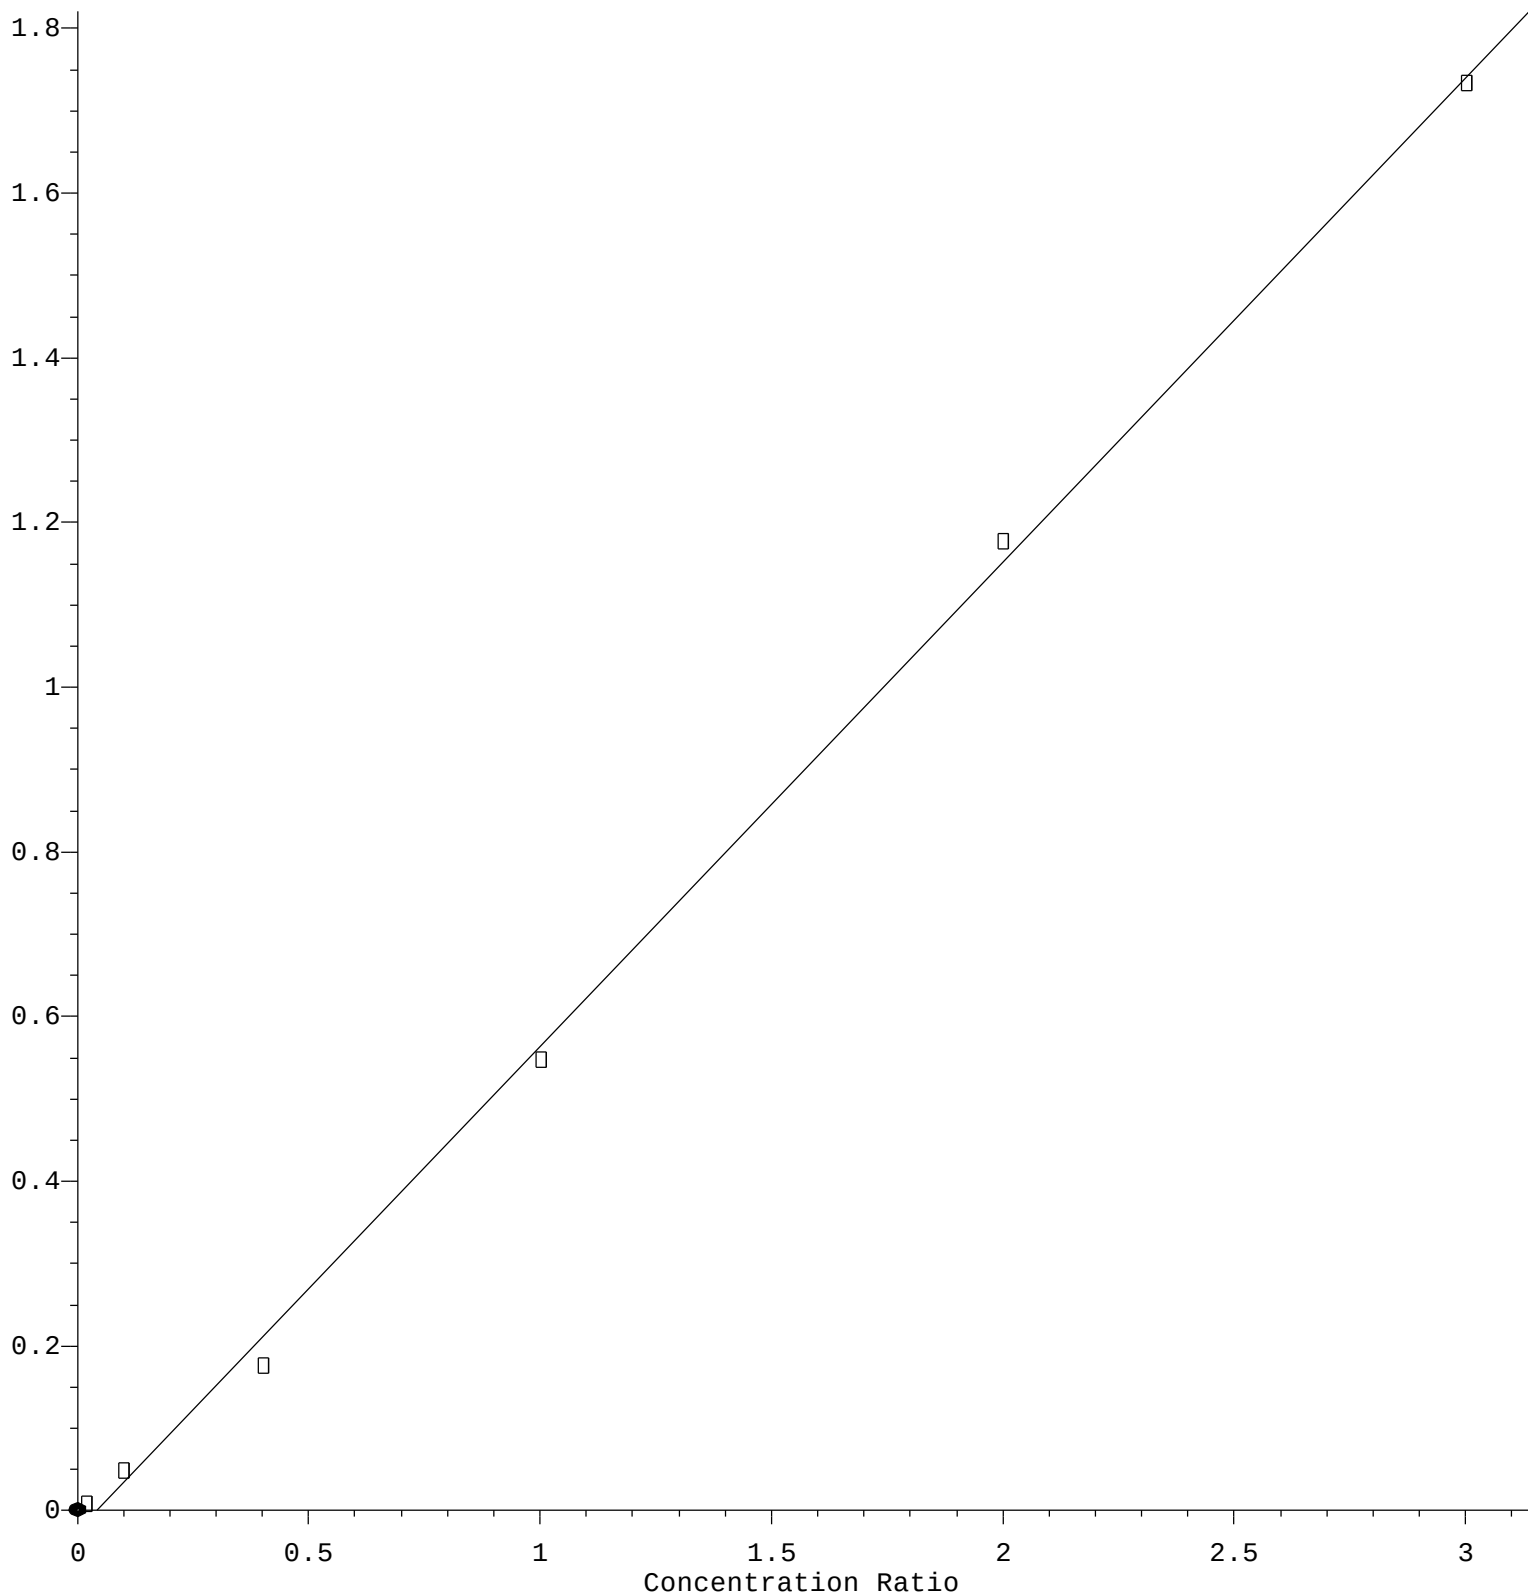

$$\text{Response} = 5.884\text{e-}001 * \text{Amt} - 2.461\text{e-}002$$


Coef of Det (r^2) = 0.998840 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M

Calibration Table Last Updated: Tue Jan 19 14:09:08 2021

Styrene


Response Ratio

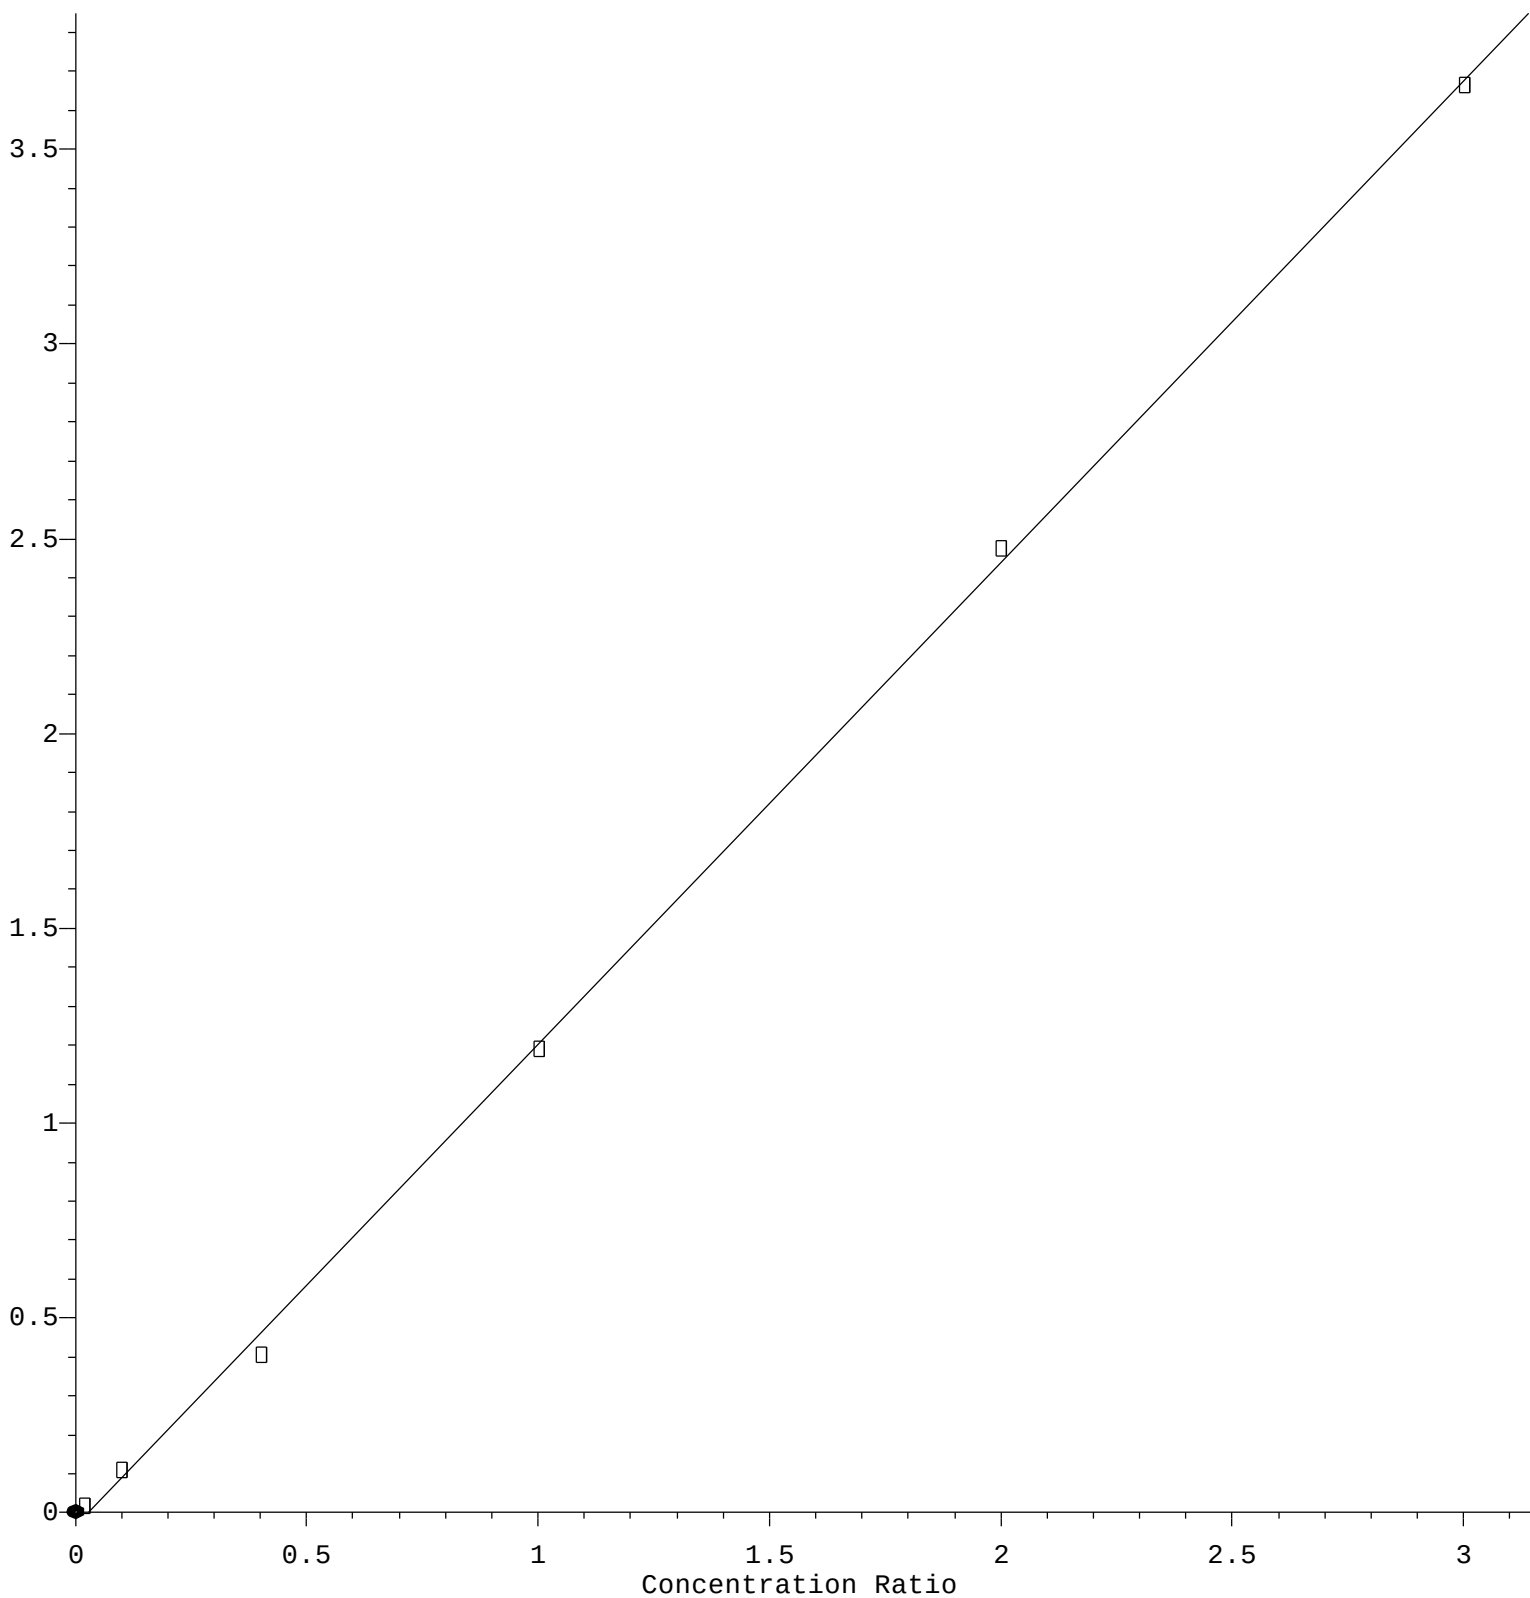

Response = 1.237e+000 * Amt - 3.507e-002
Coef of Det (r^2) = 0.999477 Curve Fit: Linear
Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
Calibration Table Last Updated: Tue Jan 19 14:09:08 2021

1,2,4-Trimethylbenzene


Response Ratio

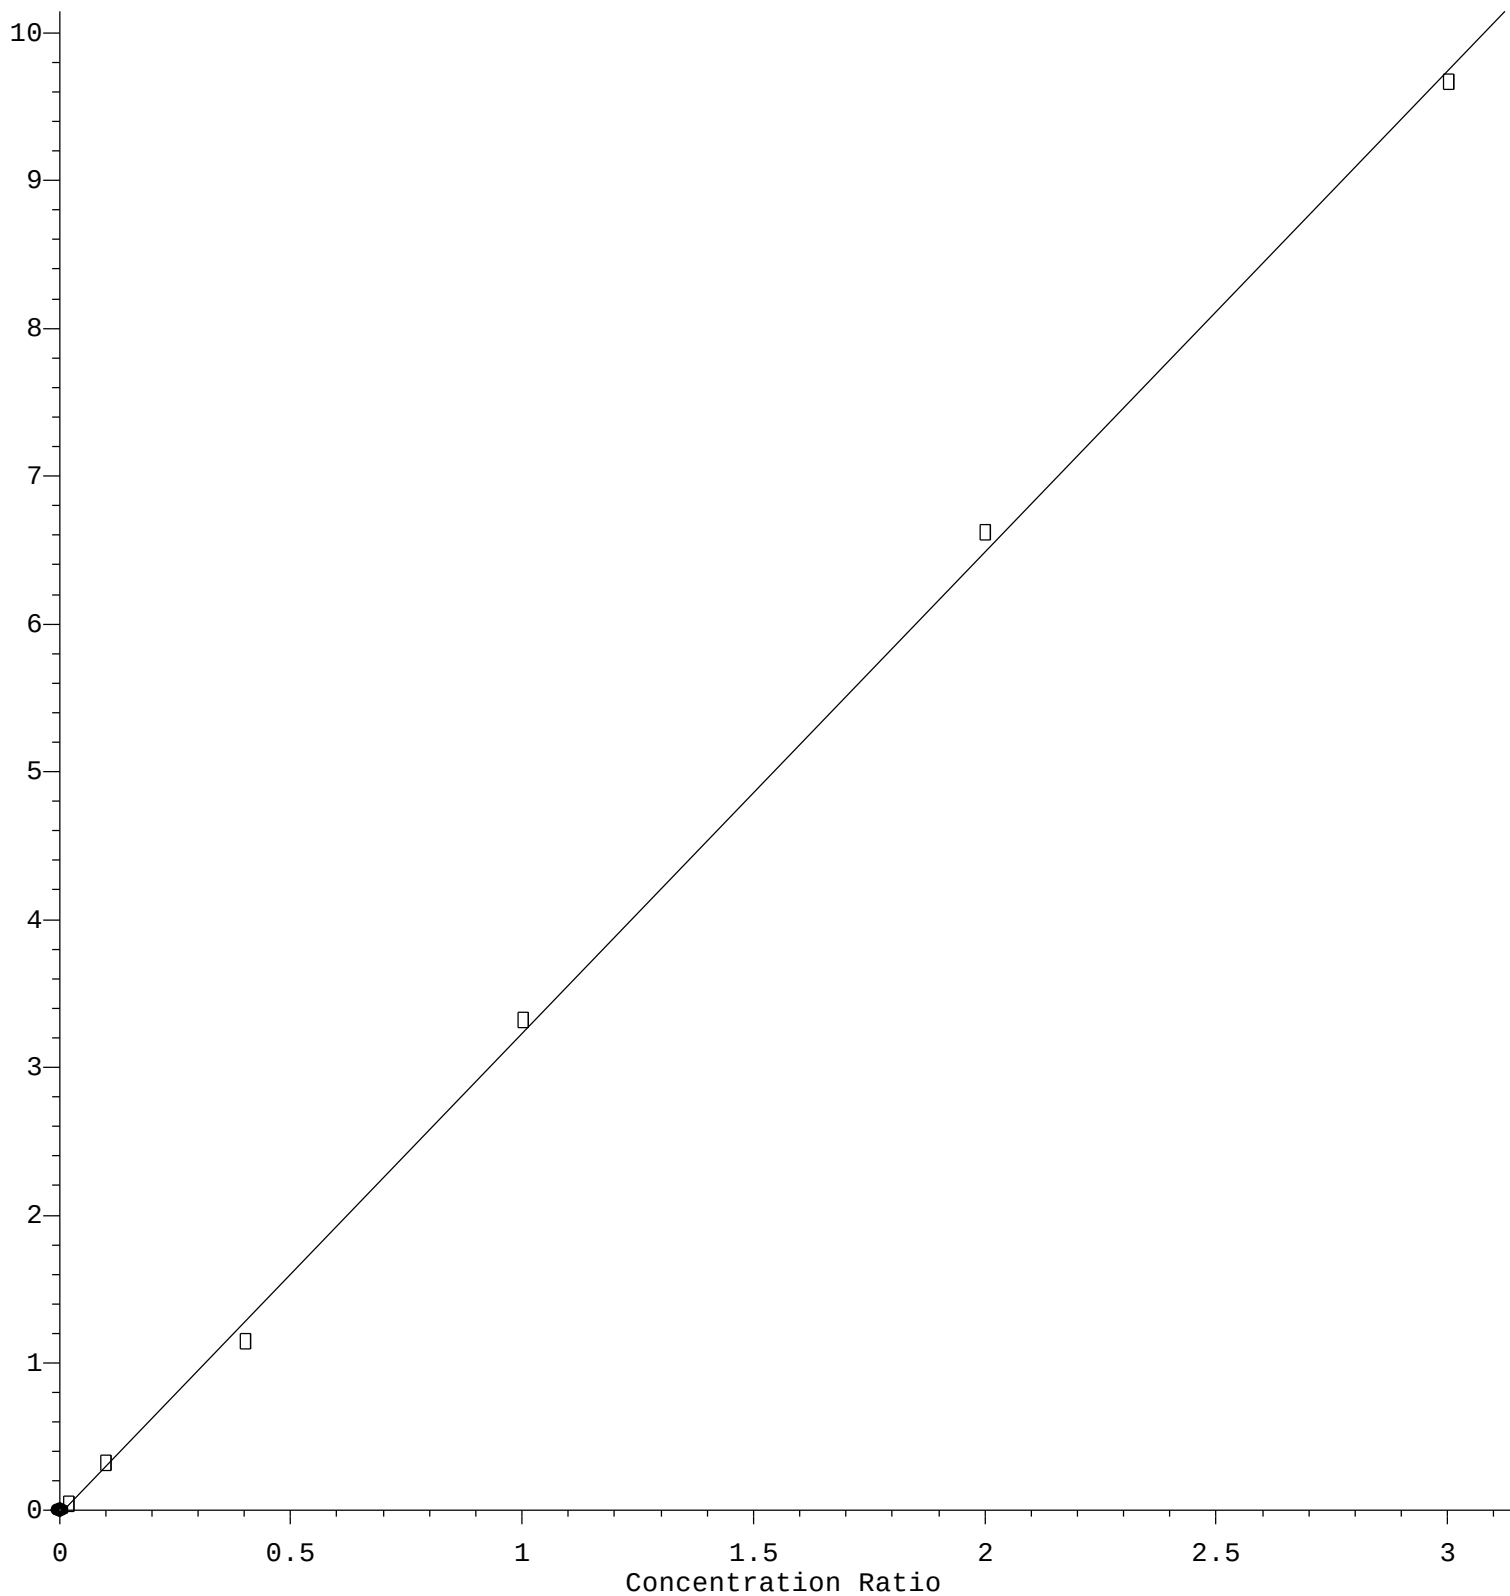

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
 Calibration Table Last Updated: Tue Jan 19 14:09:08 2021

N-amyl acetate


Response Ratio

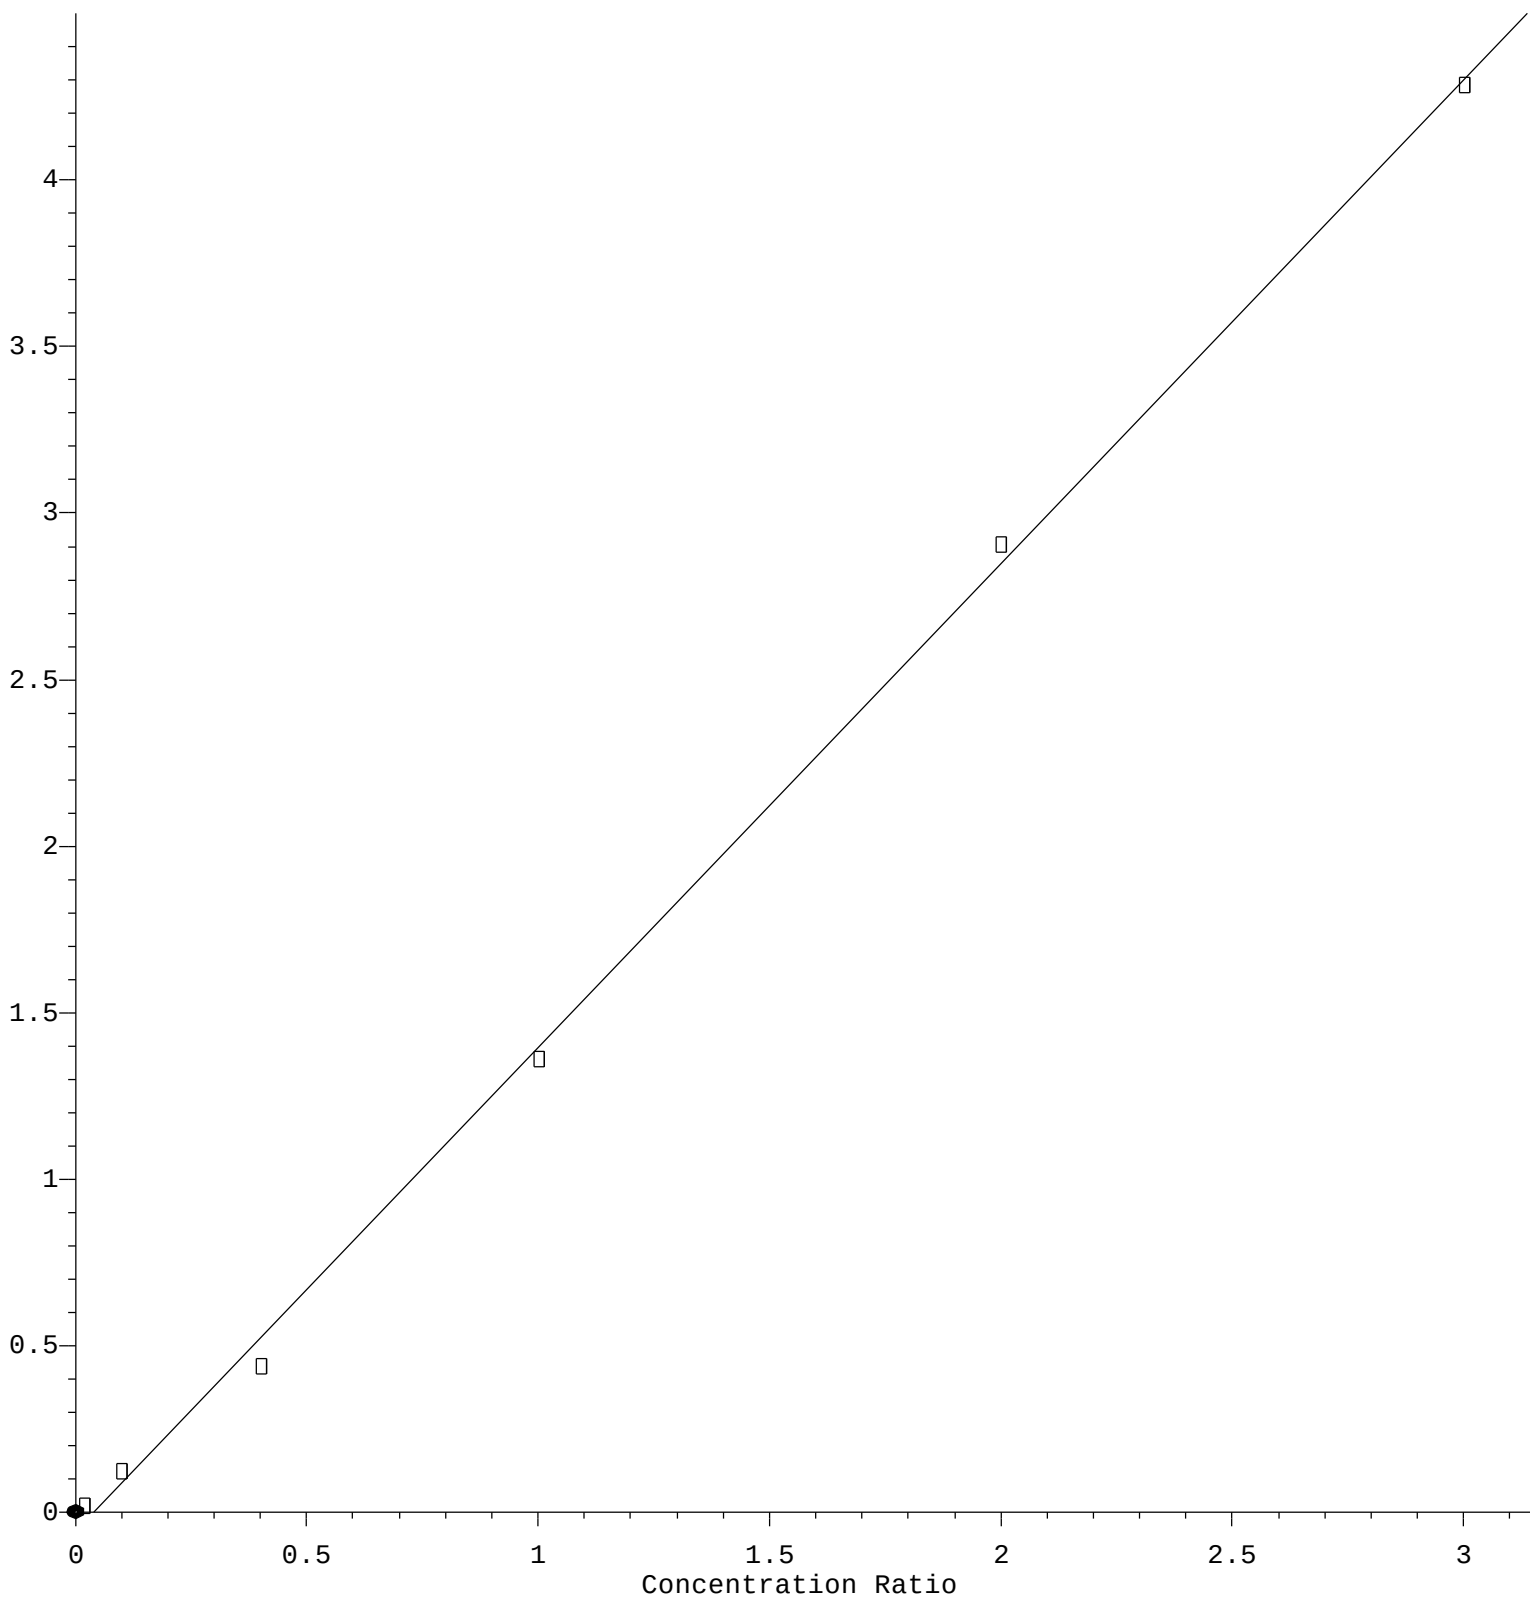

Response = 1.452e+000 * Amt - 5.628e-002
 Coef of Det (r^2) = 0.998973 Curve Fit: Linear
 Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
 Calibration Table Last Updated: Tue Jan 19 14:09:08 2021

p-Isopropyltoluene


Response Ratio

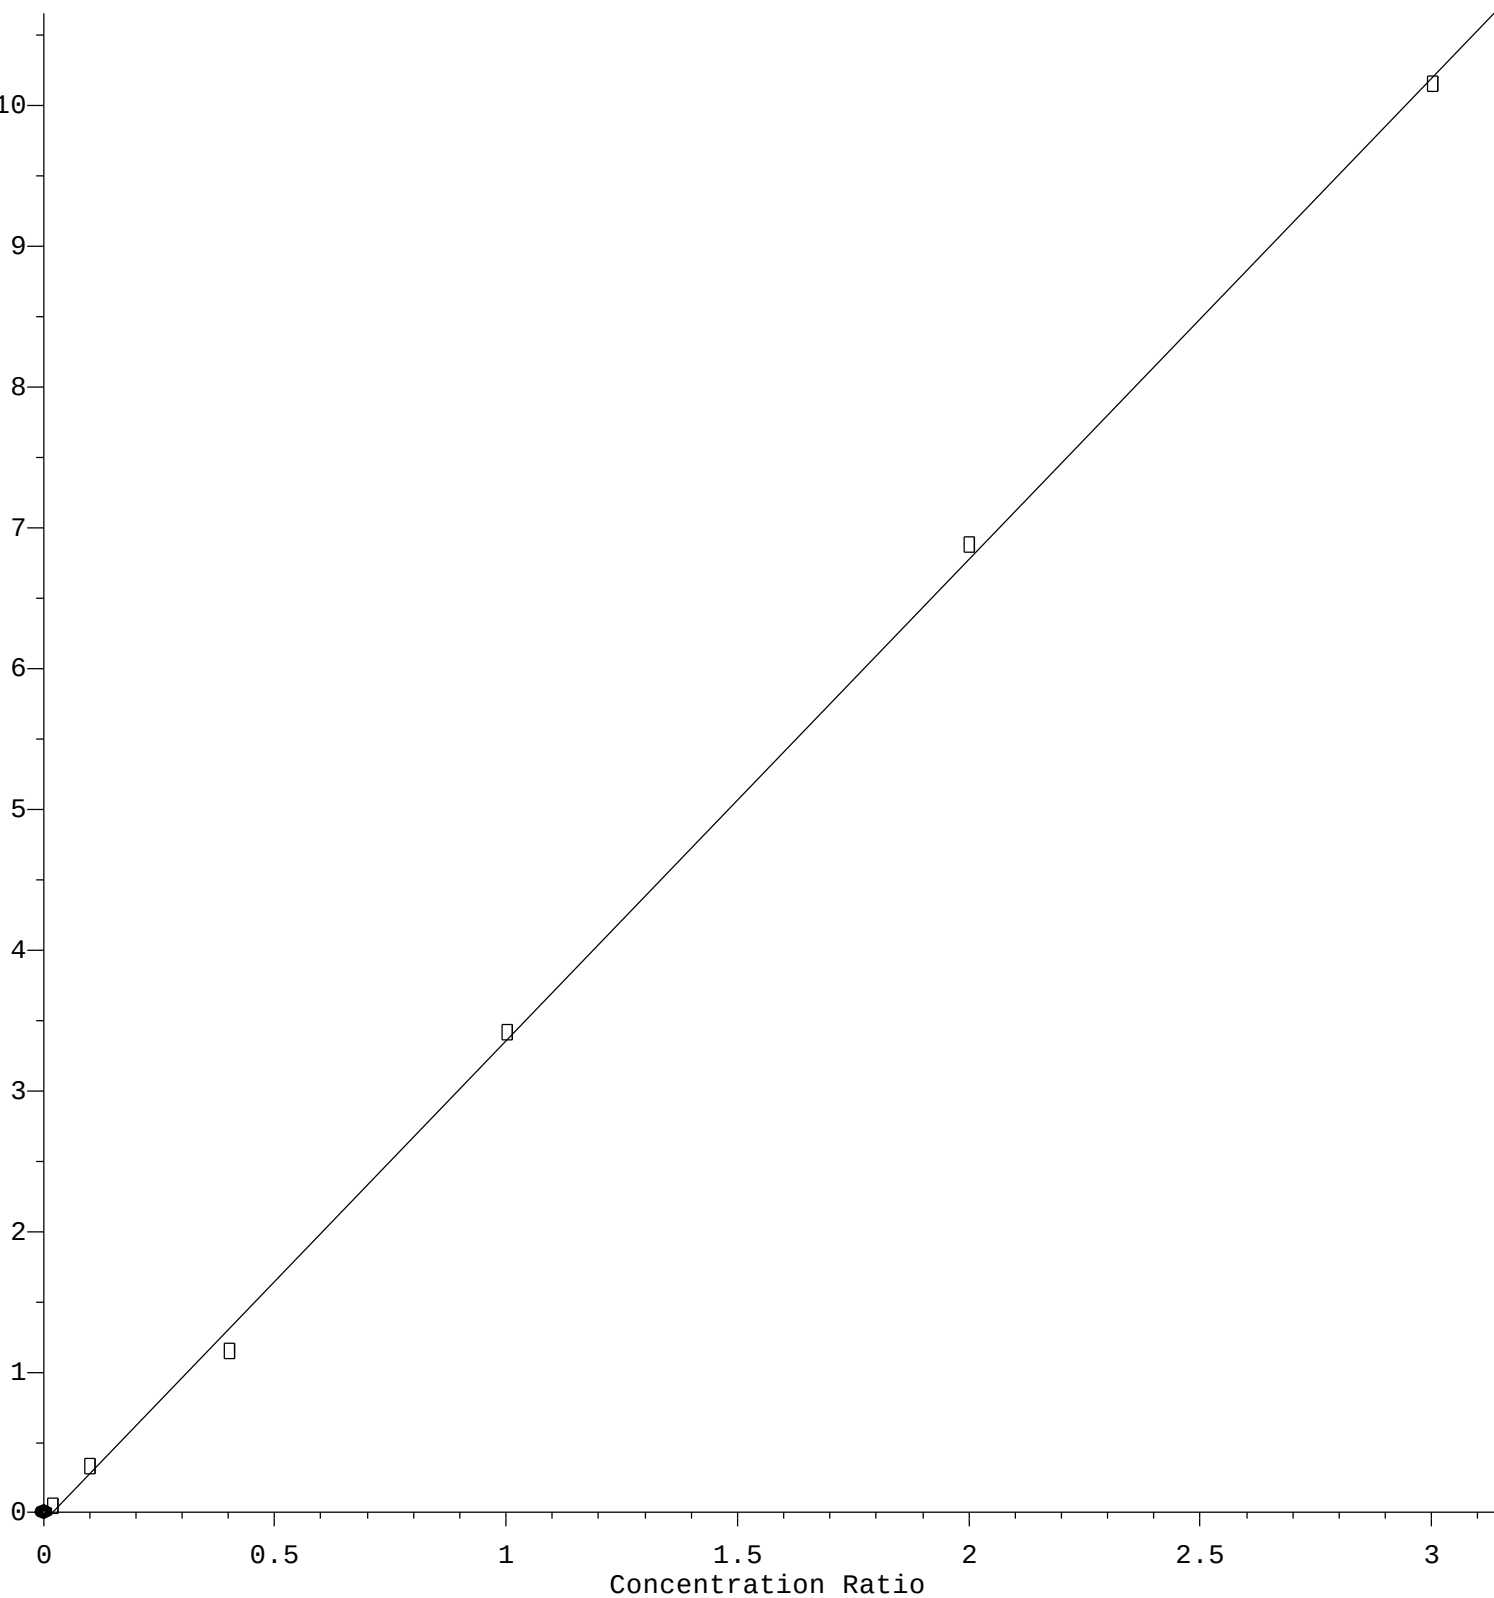

Response = 3.423e+000 * Amt - 6.028e-002
Coef of Det (r^2) = 0.999483 Curve Fit: Linear
Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
Calibration Table Last Updated: Tue Jan 19 14:09:08 2021

n-Butylbenzene


Response Ratio

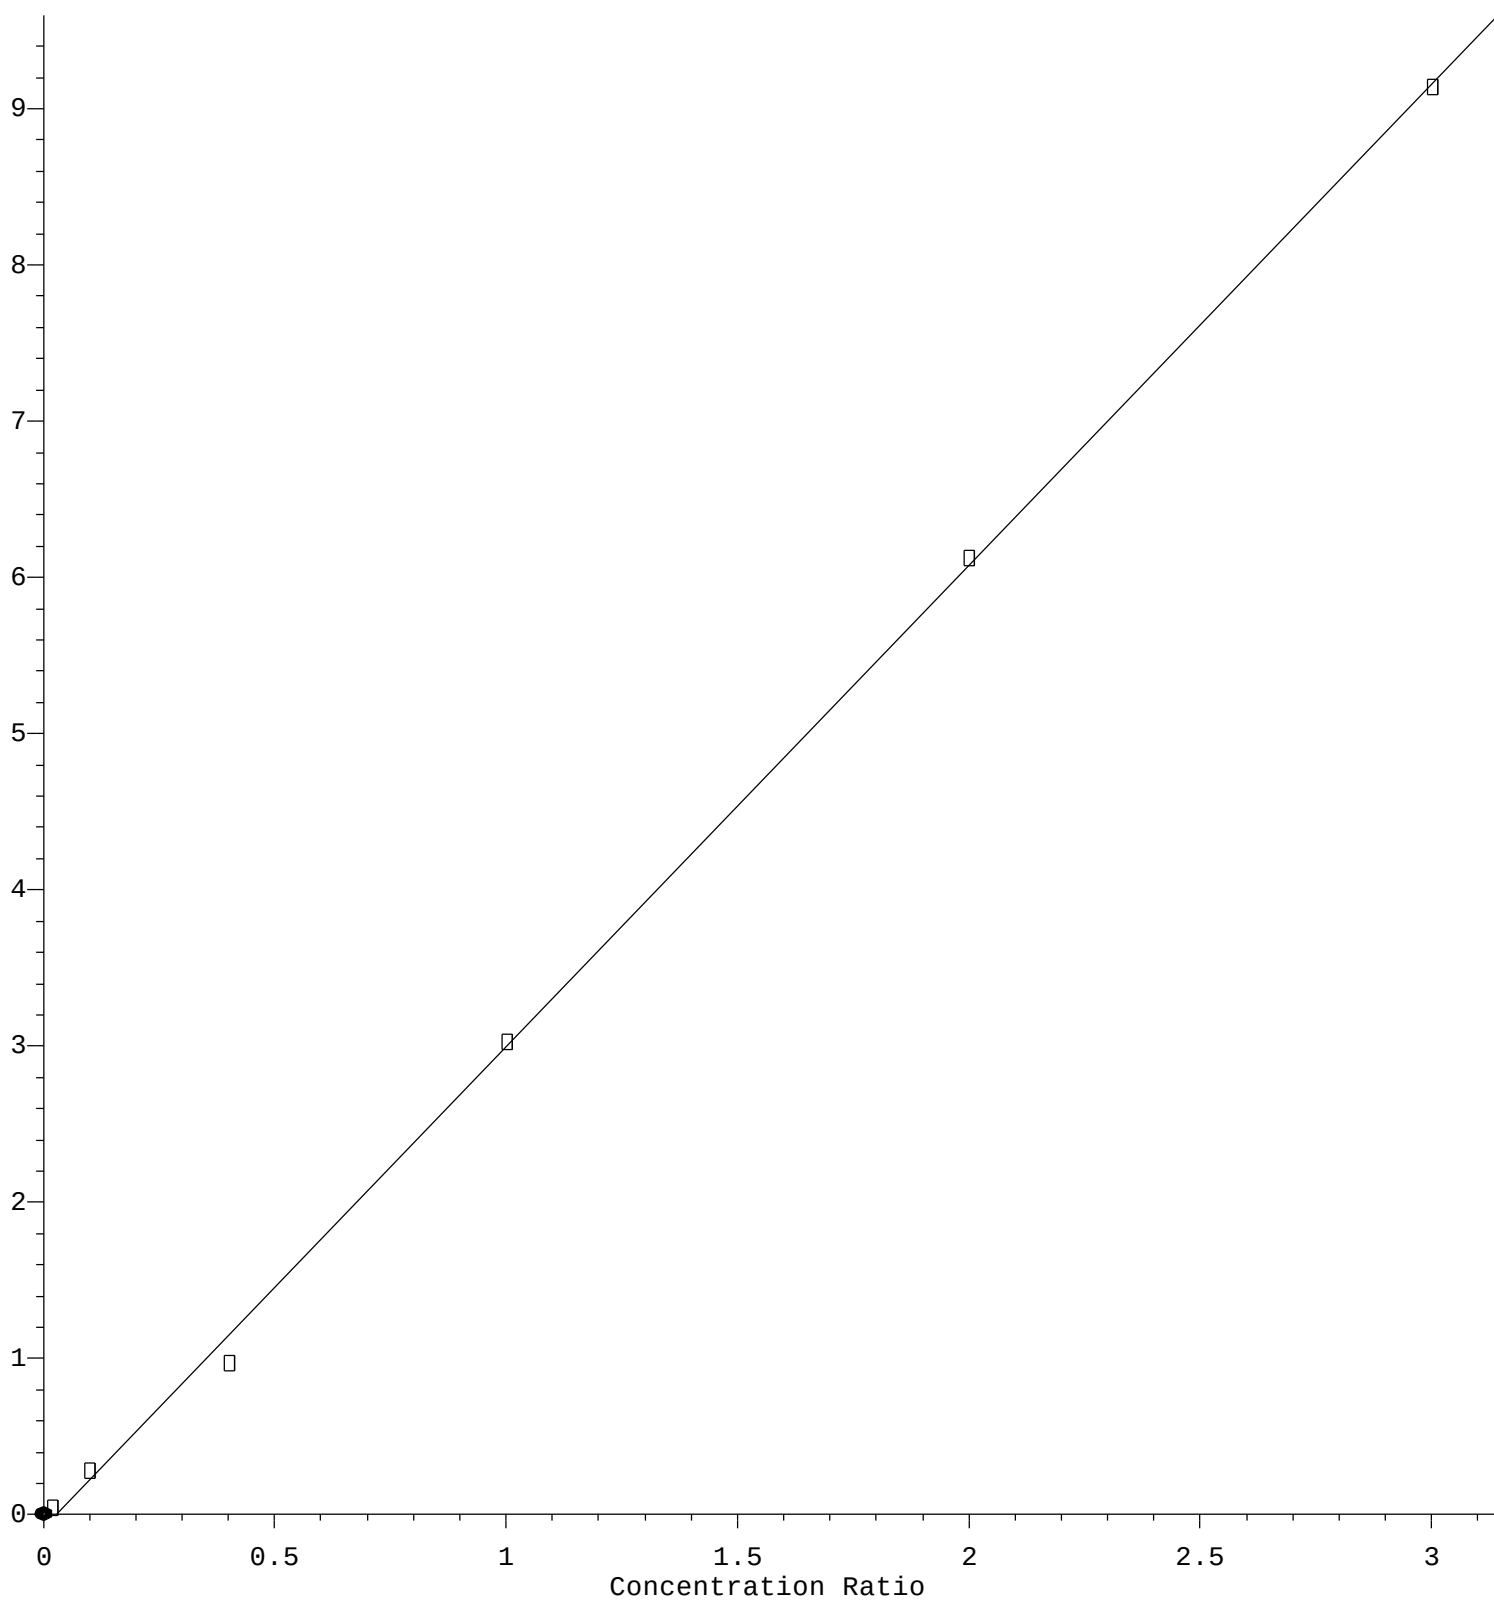

Response = 3.082e+000 * Amt - 8.813e-002
Coef of Det (r^2) = 0.999369 Curve Fit: Linear
Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
Calibration Table Last Updated: Tue Jan 19 14:09:08 2021

1,2,4-Trichlorobenzene

Response Ratio

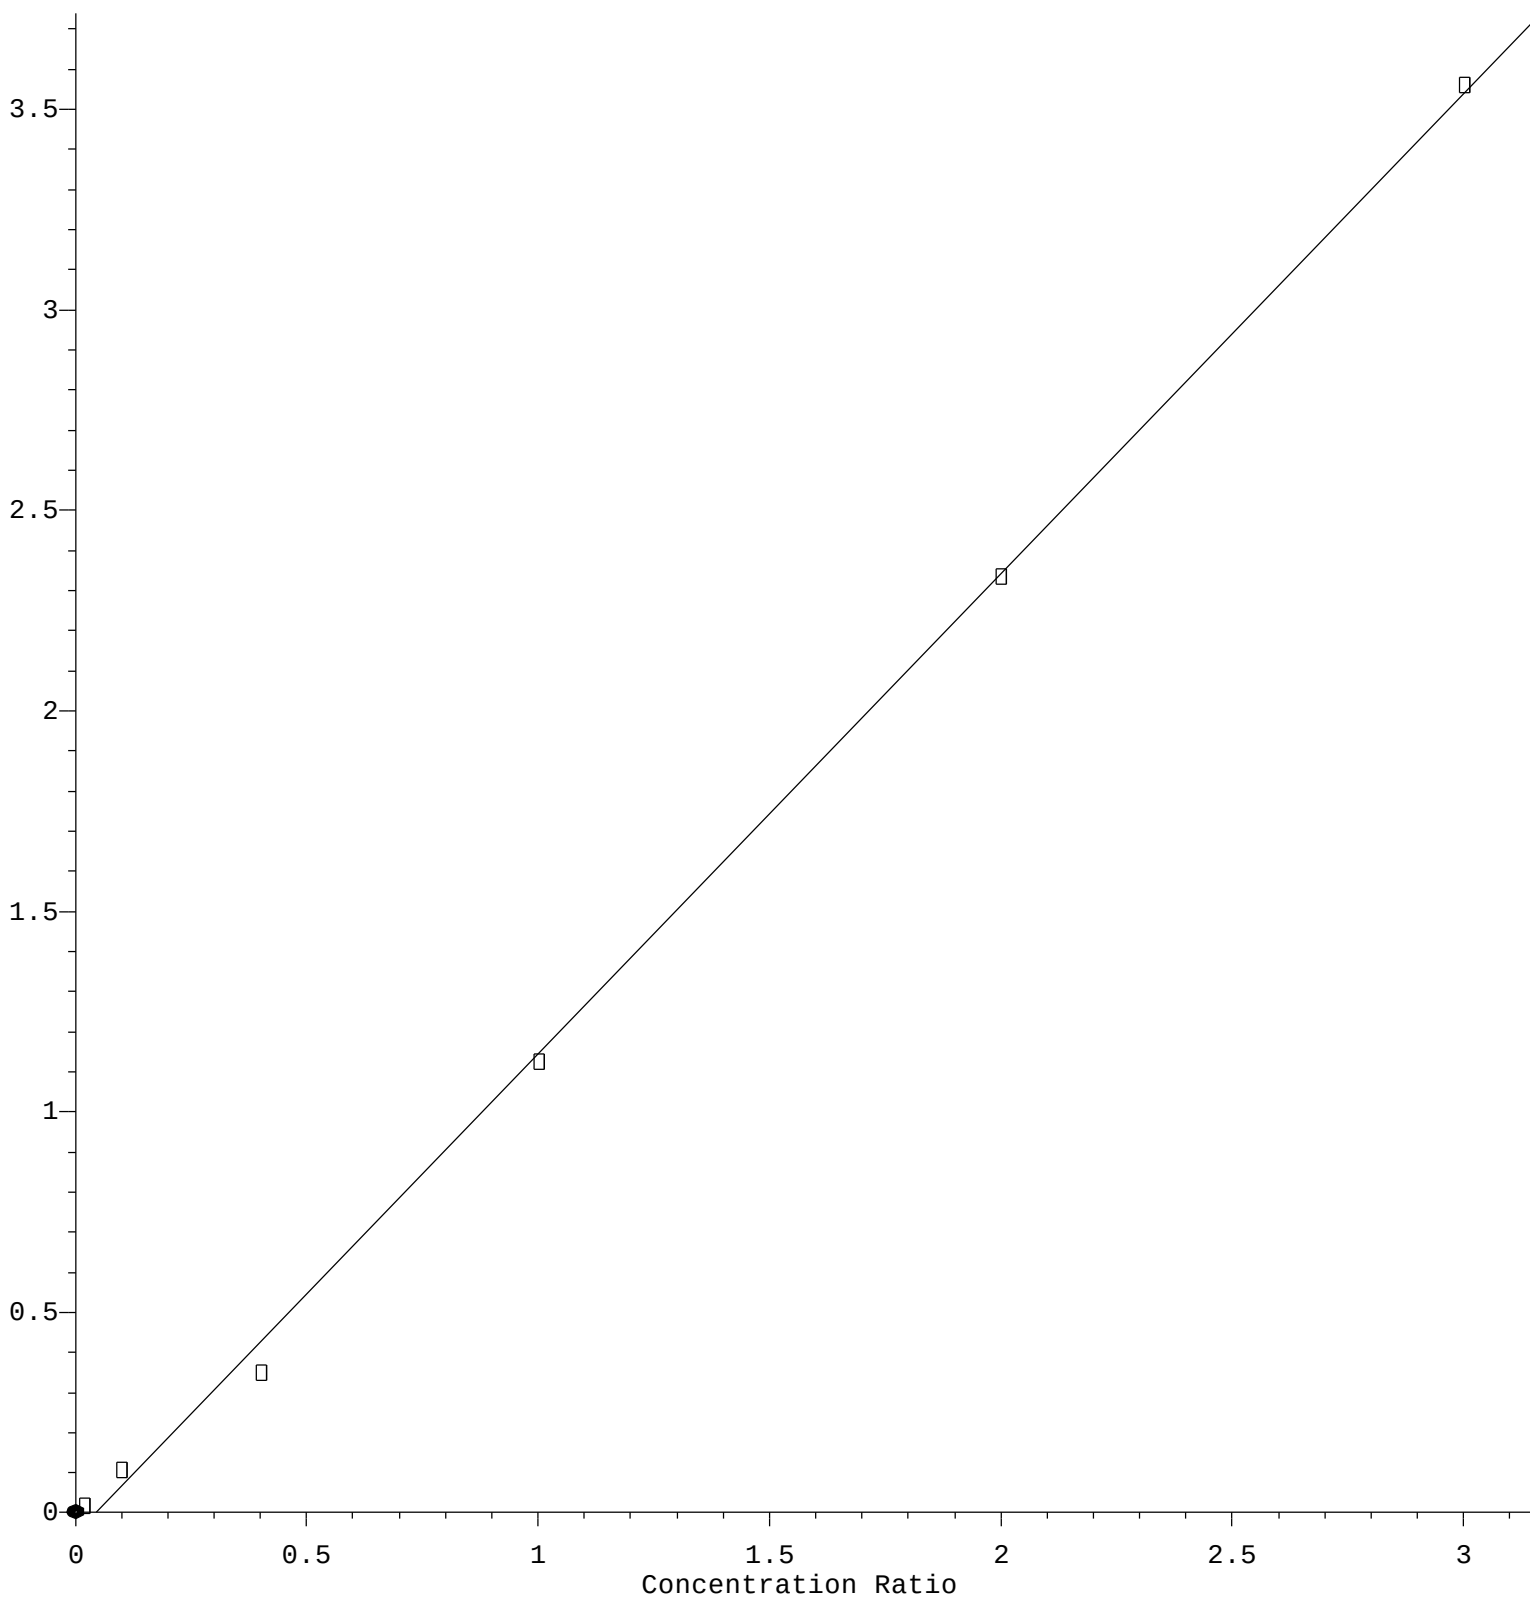

$$\text{Response} = 1.198e+000 * \text{Amt} - 5.366e-002$$


Coef of Det (r^2) = 0.998974 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M

Calibration Table Last Updated: Tue Jan 19 14:09:08 2021

Naphthalene

Response Ratio

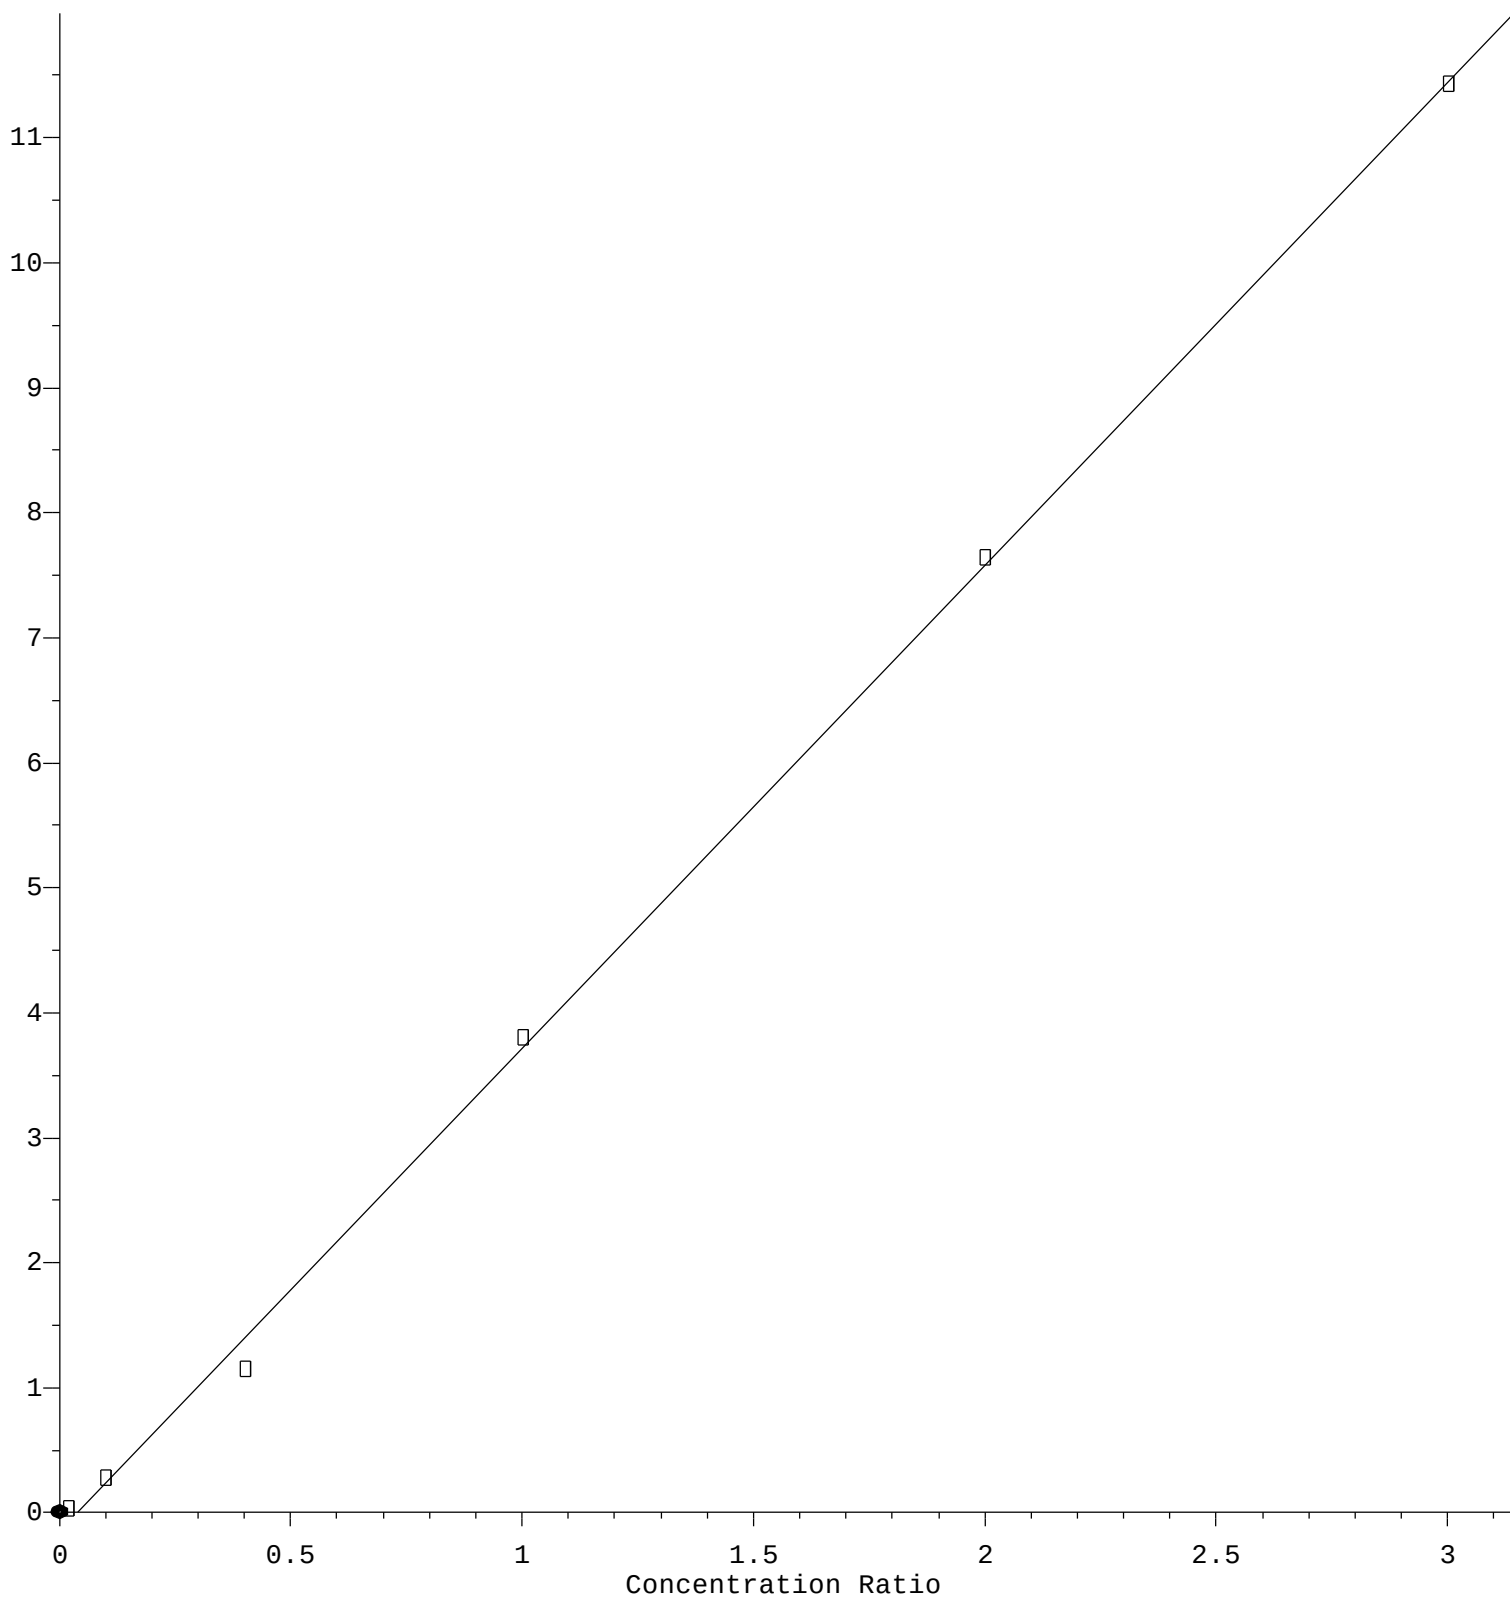

$\text{Response} = 3.868 \times 10^0 \times \text{Amt} - 1.507 \times 10^{-1}$
 Coef of Det (r^2) = 0.999191 Curve Fit: Linear
 Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
 Calibration Table Last Updated: Tue Jan 19 14:09:08 2021