


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011921\
Data File : VX020649.D
Acq On : 19 Jan 2021 09:17
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
Title : SW846 8260
Last Update : Tue Jan 19 14:09:08 2021

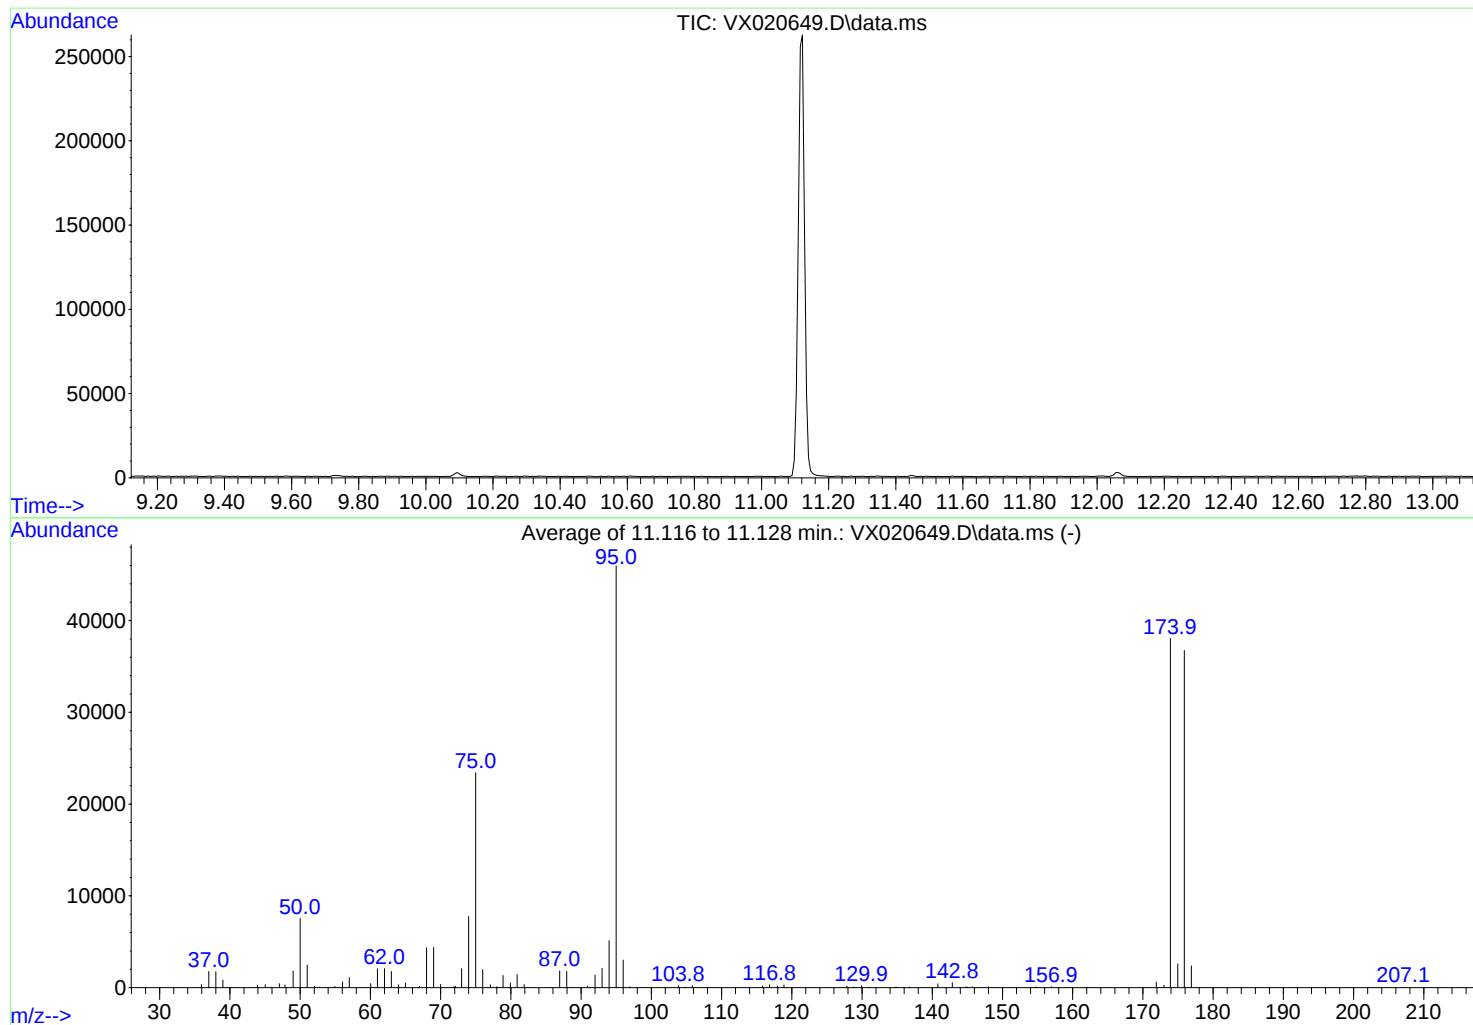

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.4	7546	PASS
75	95	30	60	50.9	23410	PASS
95	95	100	100	100.0	45965	PASS
96	95	5	9	6.5	2993	PASS
173	174	0.00	2	0.7	269	PASS
174	95	50	100	82.8	38056	PASS
175	174	5	9	6.8	2590	PASS
176	174	95	101	96.5	36731	PASS
177	176	5	9	6.5	2372	PASS