



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011923\
Data File : VX033786.D
Acq On : 19 Jan 2023 08:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Title : SW846 8260
Last Update : Wed Jan 11 14:48:42 2023

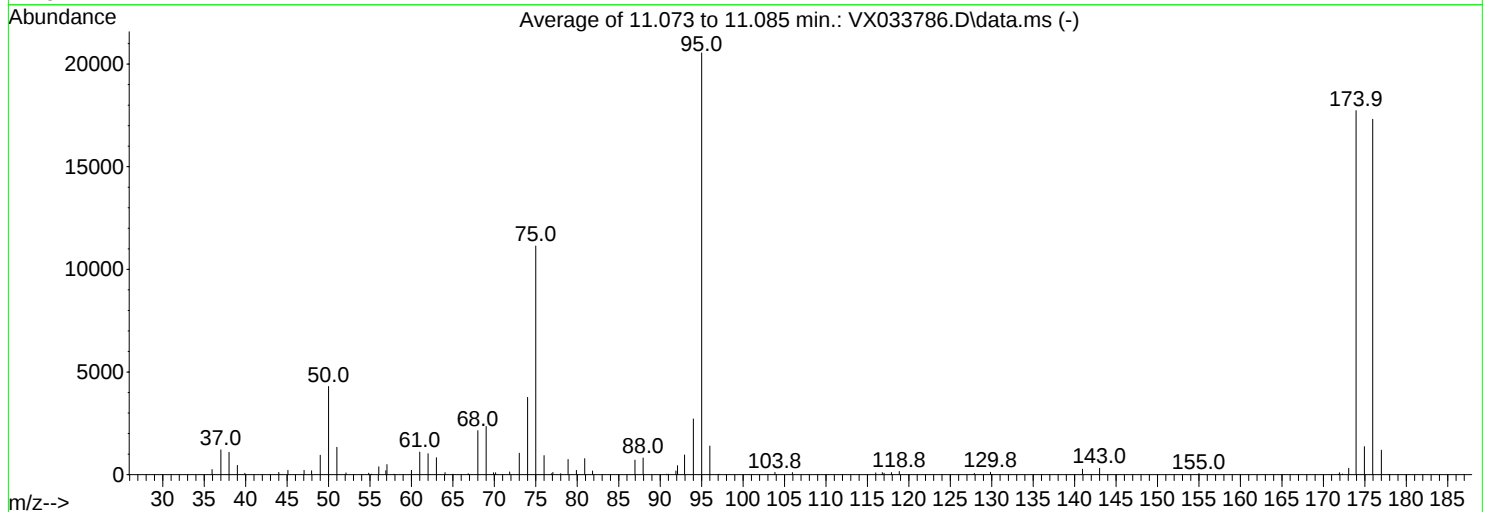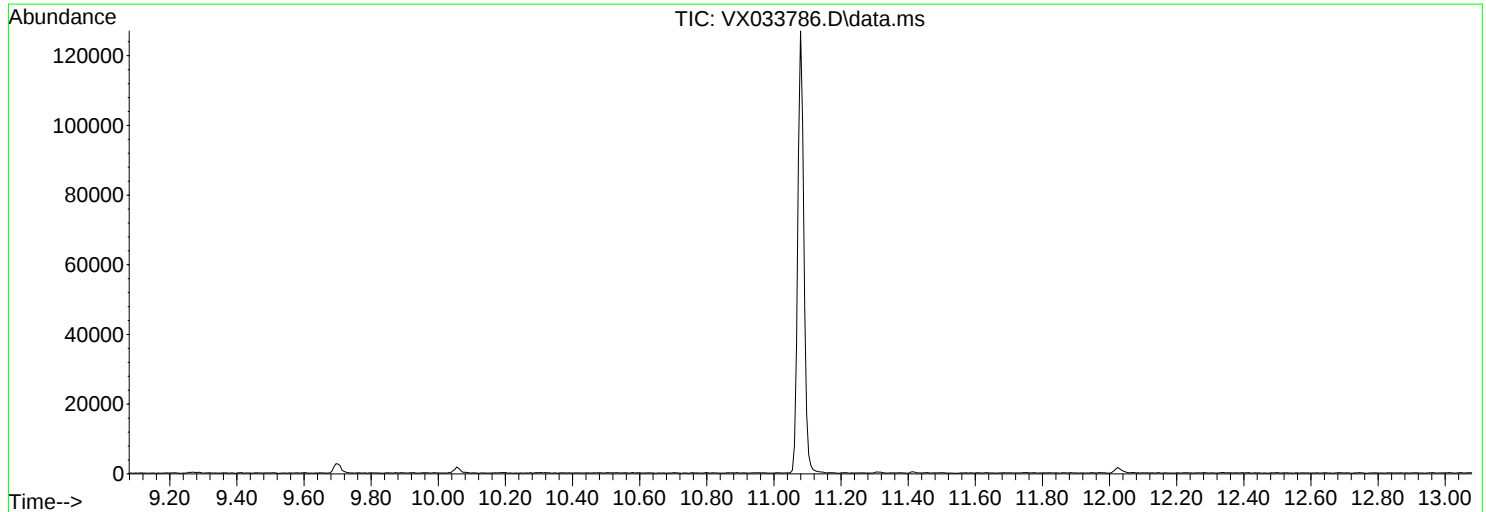

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	4296	PASS
75	95	30	60	54.2	11141	PASS
95	95	100	100	100.0	20547	PASS
96	95	5	9	6.8	1396	PASS
173	174	0.00	2	1.7	309	PASS
174	95	50	100	86.3	17731	PASS
175	174	5	9	7.7	1366	PASS
176	174	95	101	97.6	17308	PASS
177	176	5	9	6.9	1191	PASS