

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011924\
 Data File : VX039842.D
 Acq On : 19 Jan 2024 16:22
 Operator : JC/MD
 Sample : P1184-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SUMOGW-4-37-40

Quant Time: Jan 20 00:28:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 03:51:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	85885	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	157636	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	151150	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	72981	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	68134	47.358	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	94.720%		
35) Dibromofluoromethane	5.385	113	51676	48.671	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.340%		
50) Toluene-d8	8.647	98	193471	48.314	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.620%		
62) 4-Bromofluorobenzene	11.079	95	75138	47.983	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	95.960%		
Target Compounds						Qvalue
4) Vinyl Chloride	1.374	62	574	0.479	ug/l	98
11) Tert butyl alcohol	2.953	59	342	0.913	ug/l #	78
12) 1,1-Dichloroethene	2.325	96	7638	7.389	ug/l	86
16) Acetone	2.379	43	2153	2.661	ug/l	92
20) Methylene Chloride	2.788	84	392	0.320	ug/l	84
21) trans-1,2-Dichloroethene	3.099	96	2322	2.135	ug/l	85
24) 1,1-Dichloroethane	3.611	63	13312	6.232	ug/l	100
27) cis-1,2-Dichloroethene	4.489	96	91131	73.042	ug/l	87
29) Tetrahydrofuran	5.013	42	1524	2.036	ug/l	93
30) Chloroform	5.099	83	1510	0.716	ug/l	97
31) Cyclohexane	5.550	56	2325	1.224	ug/l #	9
36) 1,1-Dichloropropene	5.556	75	8282	5.011	ug/l #	46
38) Carbon Tetrachloride	5.544	117	9589	6.335	ug/l #	15
39) Methylcyclohexane	7.123	83	2632	1.326	ug/l #	1
40) Benzene	6.037	78	2391	0.511	ug/l	91
41) Methacrylonitrile	5.019	41	966	0.896	ug/l #	52
42) 1,2-Dichloroethane	6.098	62	2229	1.253	ug/l	97
44) Trichloroethene	7.123	130	187806	163.752	ug/l	97
45) 1,2-Dichloropropane	7.440	63	510	0.406	ug/l	93
48) Methyl methacrylate	7.433	41	436	0.274	ug/l #	44
49) 1,4-Dioxane	7.671	88	794	25.812	ug/l #	74
51) 4-Methyl-2-Pentanone	8.641	43	985	0.442	ug/l #	1
60) Dibromochloromethane	9.268	129	111282	99.156	ug/l #	11
64) Tetrachloroethene	9.275	164	105449	107.280	ug/l	98
65) Chlorobenzene	10.079	112	1808	0.574	ug/l	94
76) 1,2,3-Trichloropropane	11.079	75	42237	22.323	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	42237	64.678	ug/l #	5
91) 1,2-Dichlorobenzene	12.335	146	3752	1.530	ug/l	98
93) 1,2,4-Trichlorobenzene	13.591	180	2110	1.408	ug/l	98
96) 1,2,3-Trichlorobenzene	13.963	180	529	0.350	ug/l	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011924\
Data File : VX039842.D
Acq On : 19 Jan 2024 16:22
Operator : JC/MD
Sample : P1184-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40

Quant Time: Jan 20 00:28:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 03:51:26 2024
Response via : Initial Calibration

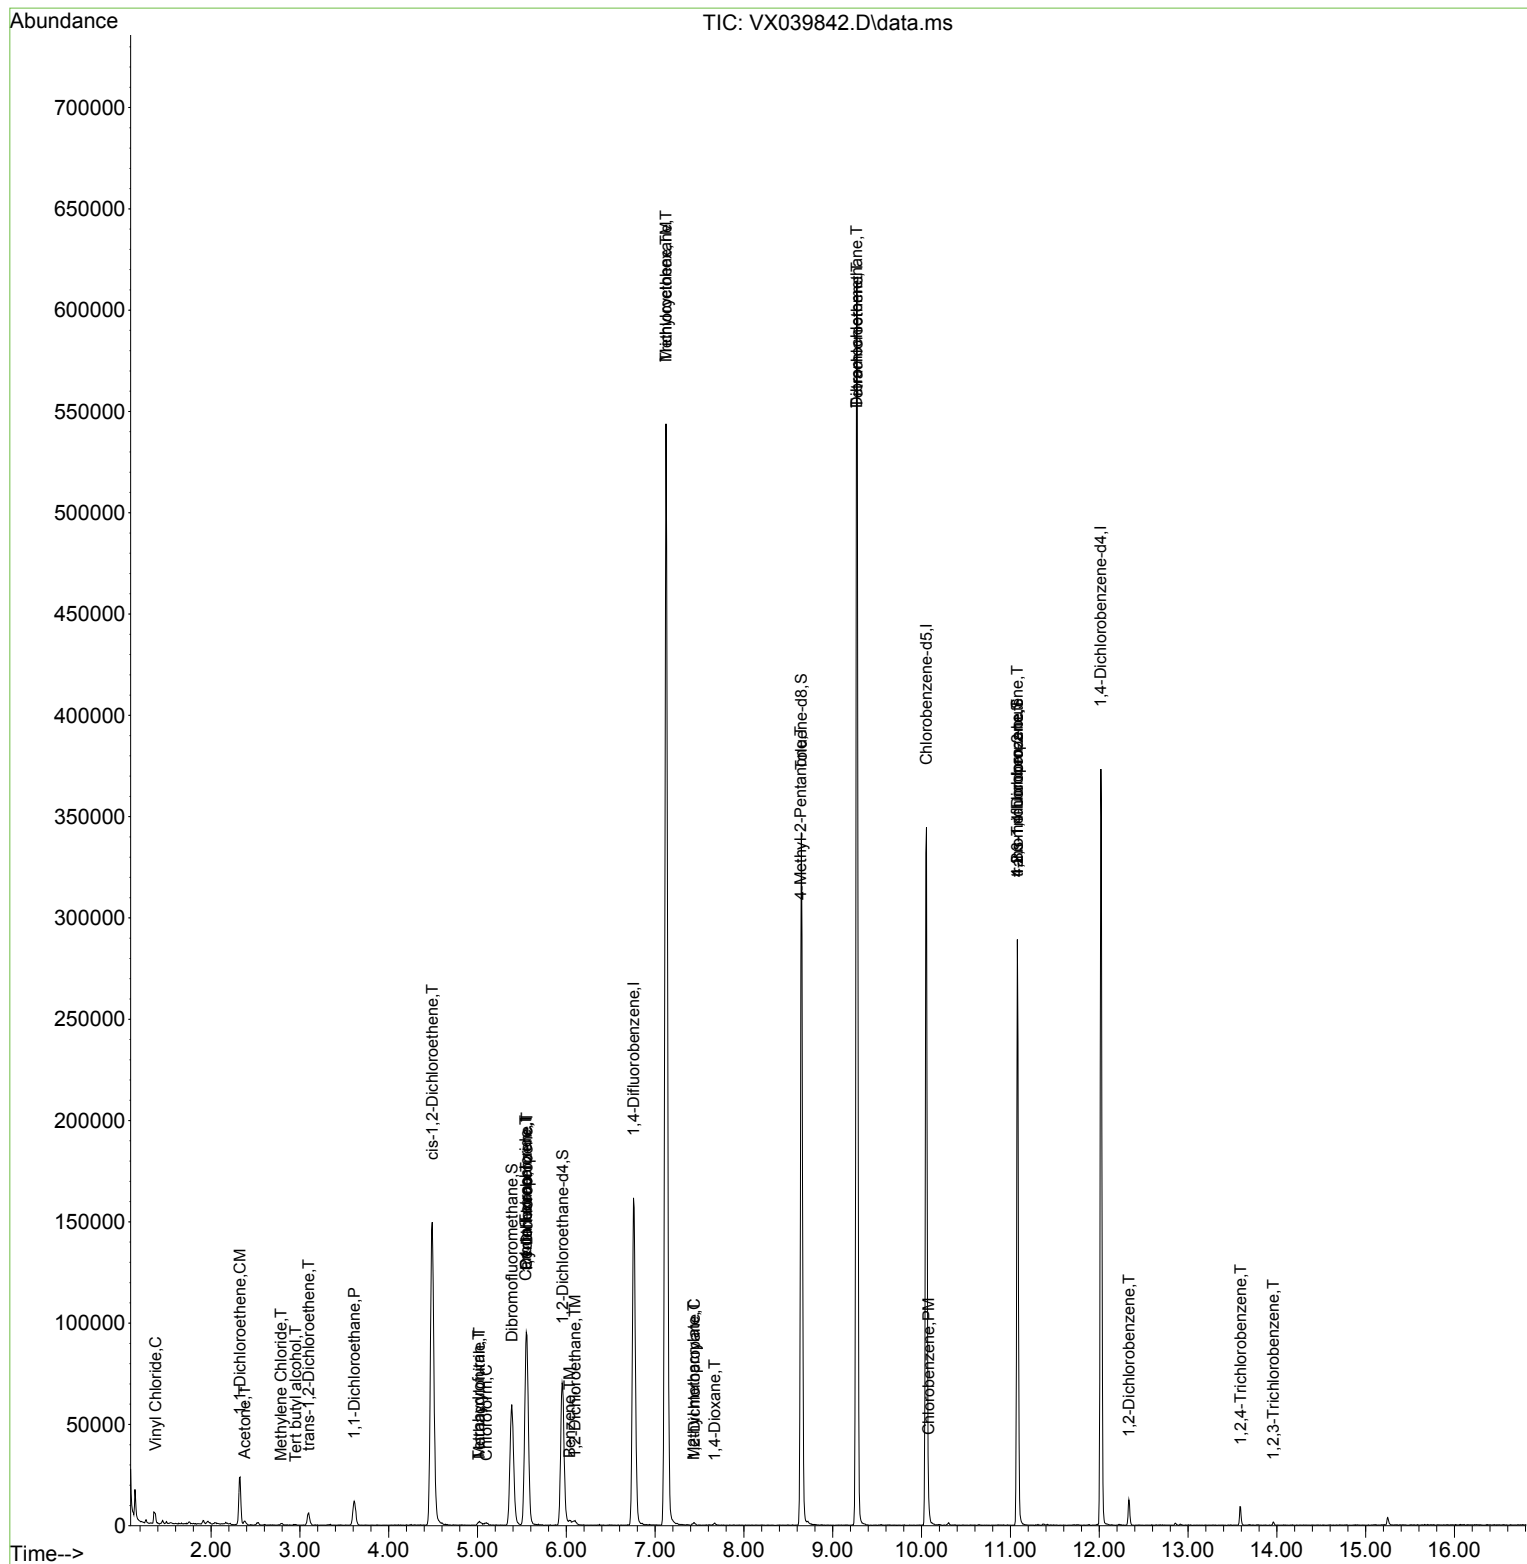



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.000 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22

Instrument :

MSVOA_X

ClientSampleId :





SUMOGW-4-37-40

Tgt Ion:168 Resp: 85885

Ion Ratio Lower Upper

168 100

99 63.6 56.6 85.0

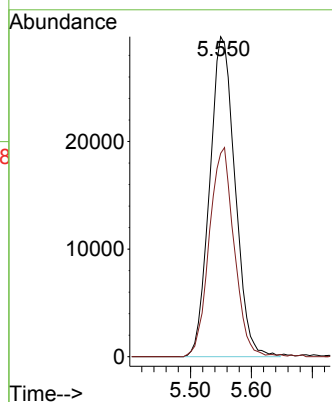

#4

Vinyl Chloride

Concen: 0.479 ug/l

RT: 1.374 min Scan# 47

Delta R.T. -0.000 min

Lab File: VX039842.D




Acq: 19 Jan 2024 16:22


Tgt Ion: 62 Resp: 574

Ion Ratio Lower Upper

62 100

64 30.3 25.4 38.0

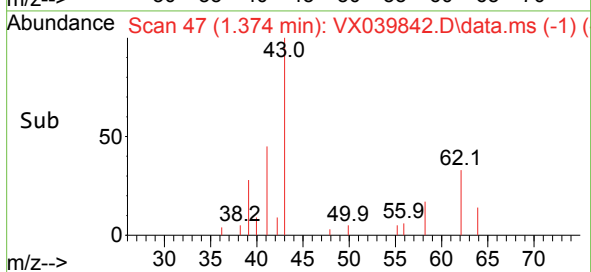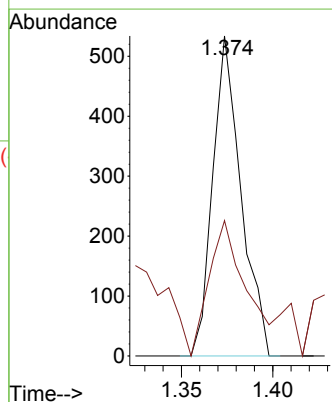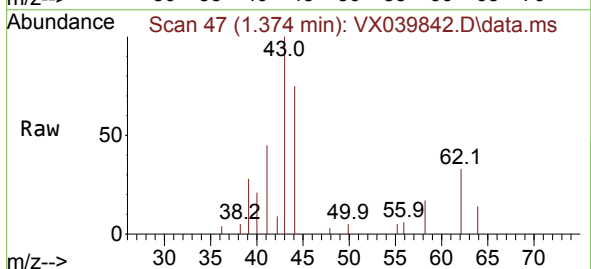

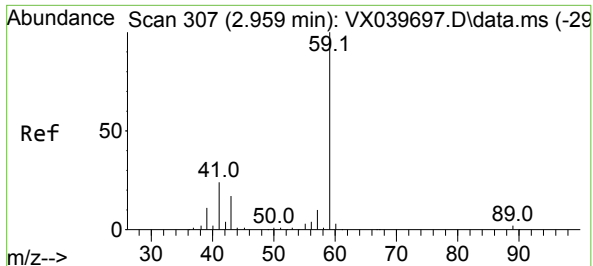

#11

Tert butyl alcohol

Concen: 0.913 ug/l

RT: 2.953 min Scan# 307

Delta R.T. -0.006 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22

Instrument :

MSVOA_X

ClientSampleId :





SUMOGW-4-37-40

Tgt Ion: 59 Resp: 342

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

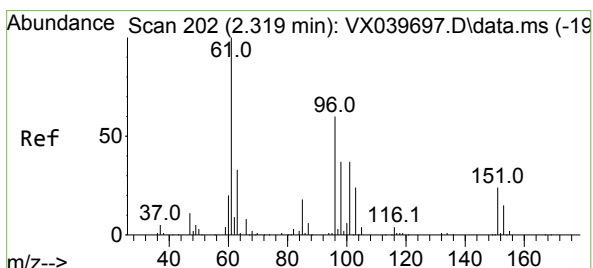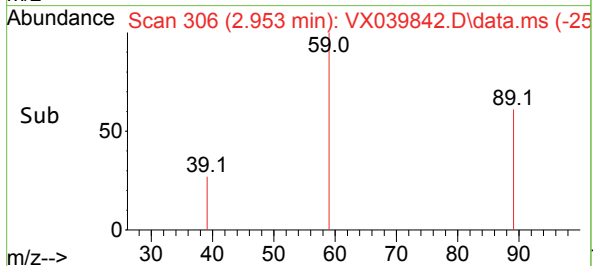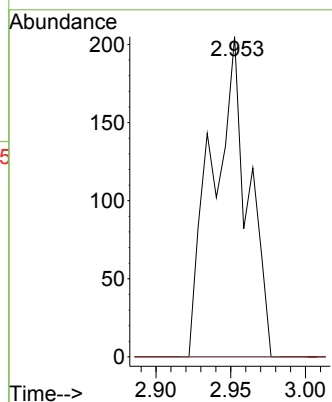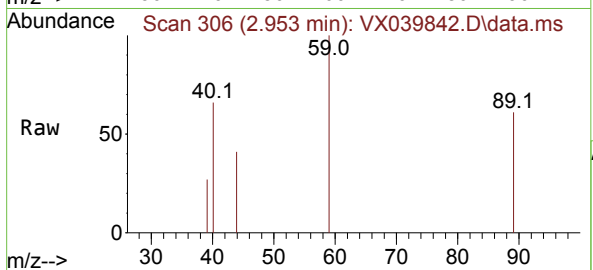

#12

1,1-Dichloroethene

Concen: 7.389 ug/l

RT: 2.325 min Scan# 203

Delta R.T. 0.006 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22




Tgt Ion: 96 Resp: 7638


Ion Ratio Lower Upper

96 100

61 155.5 144.6 216.8

98 64.8 50.4 75.6

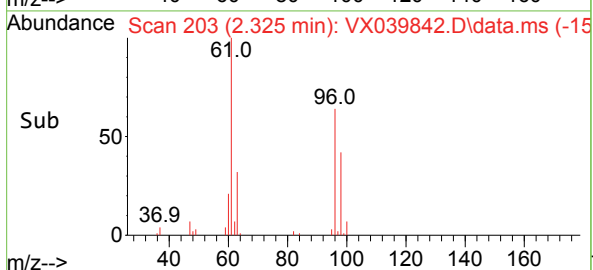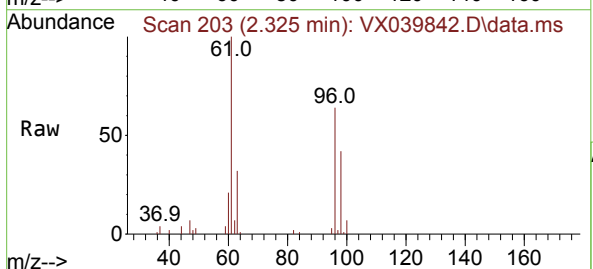

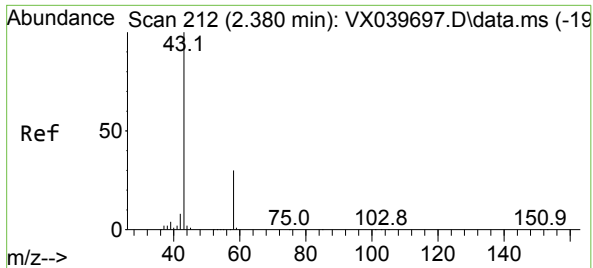

#16

Acetone

Concen: 2.661 ug/l

RT: 2.379 min Scan# 212

Delta R.T. -0.000 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22

Instrument :

MSVOA_X

ClientSampleId :





SUMOGW-4-37-40

Tgt Ion: 43 Resp: 2153

Ion Ratio Lower Upper

43 100

58 31.8 21.9 32.9

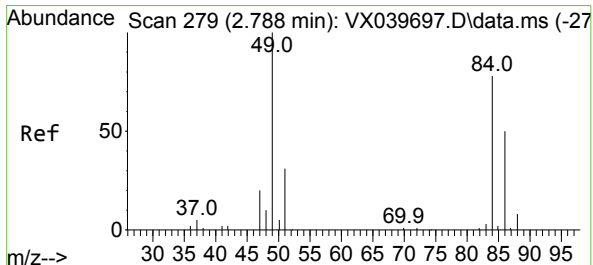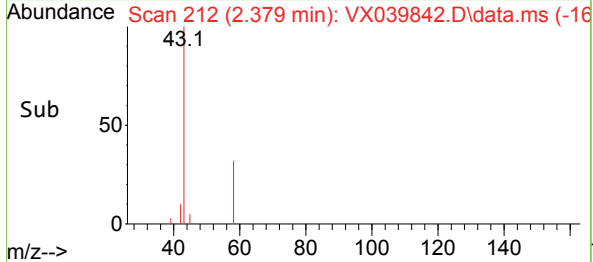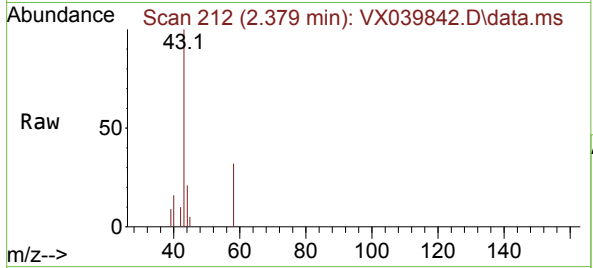

#20

Methylene Chloride

Concen: 0.320 ug/l

RT: 2.788 min Scan# 279

Delta R.T. -0.000 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22

Tgt Ion: 84 Resp: 392




Ion Ratio Lower Upper


84 100

49 152.1 103.6 155.4

51 35.7 33.8 50.6

86 70.9 49.4 74.0


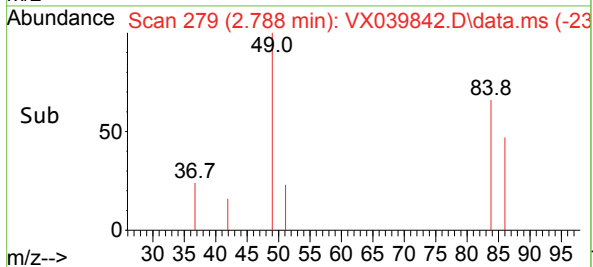
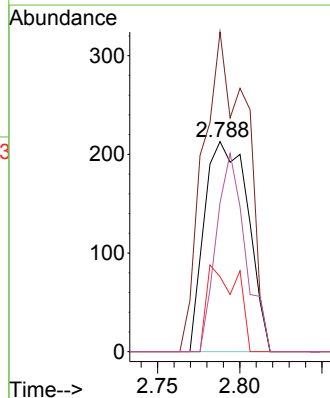
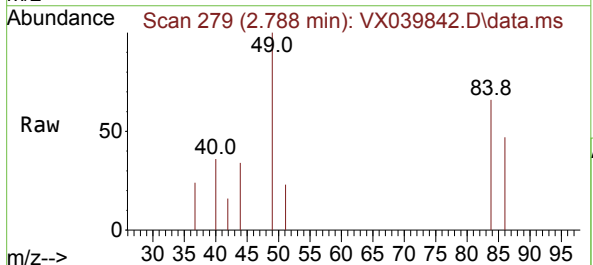




#21
trans-1,2-Dichloroethene
Concen: 2.135 ug/l
RT: 3.099 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion: 96 Resp: 2322
Ion Ratio Lower Upper
96 100
61 124.0 119.2 178.8
98 62.4 48.7 73.1

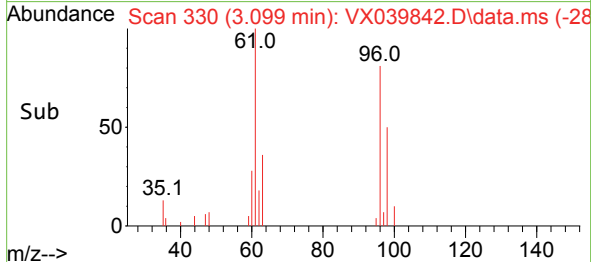

#24
1,1-Dichloroethane
Concen: 6.232 ug/l
RT: 3.611 min Scan# 414
Delta R.T. -0.000 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion: 63 Resp: 13312
Ion Ratio Lower Upper
63 100
98 6.4 3.3 9.8
100 4.2 2.1 6.5





#27

cis-1,2-Dichloroethene

Concen: 73.042 ug/l

RT: 4.489 min Scan# 51

Delta R.T. 0.006 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22

Instrument :

MSVOA_X

ClientSampleId :

SUMOGW-4-37-40





Tgt Ion: 96 Resp: 91131

Ion Ratio Lower Upper

96 100

61 132.8 0.0 312.2

98 64.2 0.0 129.0

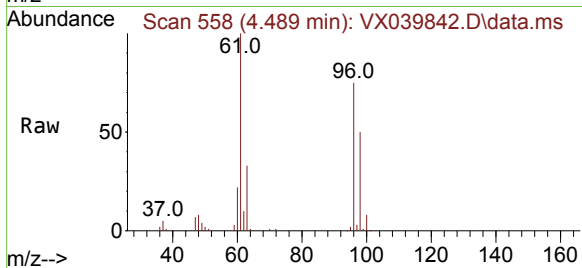

#29

Tetrahydrofuran

Concen: 2.036 ug/l

RT: 5.013 min Scan# 644

Delta R.T. 0.012 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22




Tgt Ion: 42 Resp: 1524


Ion Ratio Lower Upper

42 100

72 48.6 34.2 51.4

71 37.2 32.2 48.2



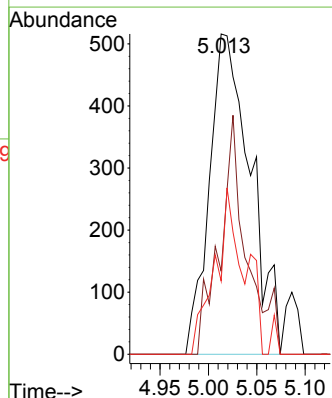
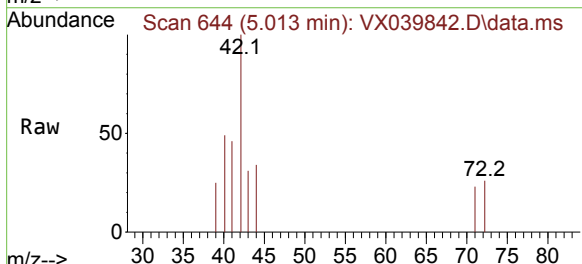




#30
Chloroform
Concen: 0.716 ug/l
RT: 5.099 min Scan# 61
Delta R.T. 0.006 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion: 83 Resp: 1510
Ion Ratio Lower Upper
83 100
85 60.6 50.3 75.5

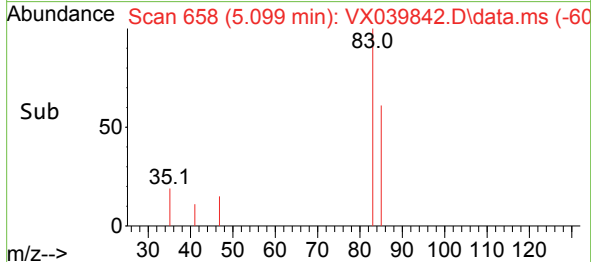

#31
Cyclohexane
Concen: 1.224 ug/l
RT: 5.550 min Scan# 732
Delta R.T. 0.079 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion: 56 Resp: 2325
Ion Ratio Lower Upper
56 100
69 156.4 23.4 35.2#
84 117.0 65.9 98.9#

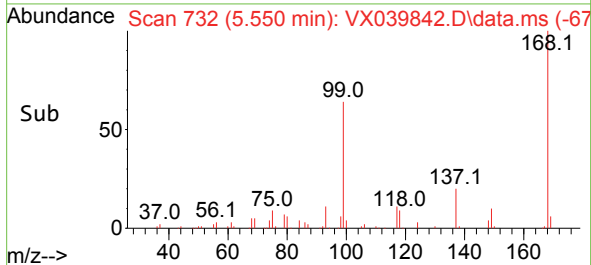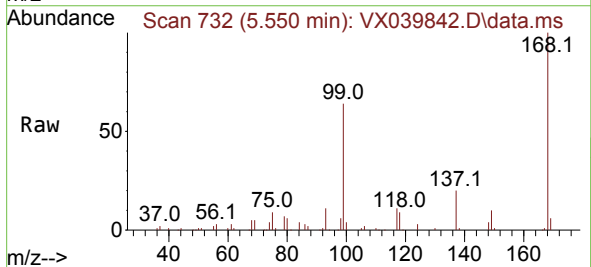



#33

1,2-Dichloroethane-d4

Concen: 47.358 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22

Instrument :

MSVOA_X

ClientSampleId :





SUMOGW-4-37-40

Tgt Ion: 65 Resp: 68134

Ion Ratio Lower Upper

65 100

67 52.0 0.0 100.2



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22




Tgt Ion: 114 Resp: 157636


Ion Ratio Lower Upper

114 100

63 21.8 0.0 45.0

88 16.0 0.0 36.6







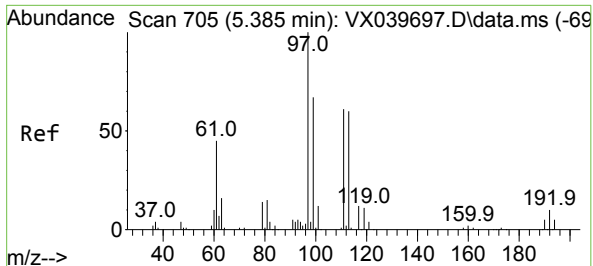

#35
Dibromofluoromethane
Concen: 48.671 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion:113 Resp: 51676
Ion Ratio Lower Upper
113 100
111 102.6 82.9 124.3
192 16.6 13.3 19.9

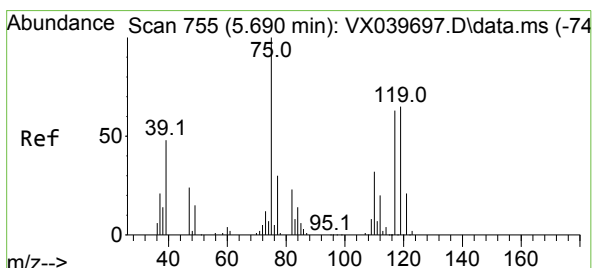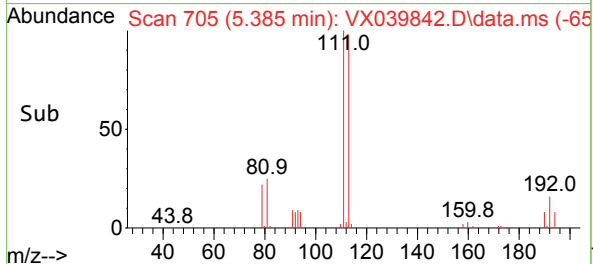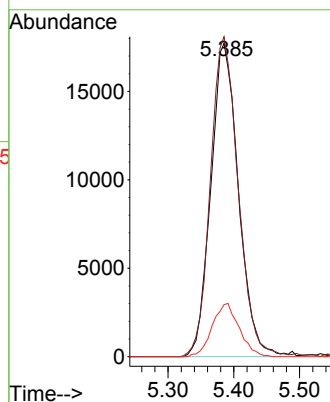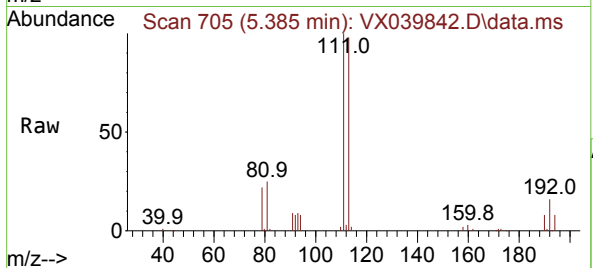

#36
1,1-Dichloropropene
Concen: 5.011 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22


Tgt Ion: 75 Resp: 8282
Ion Ratio Lower Upper
75 100
110 4.2 17.0 50.9#
77 0.0 24.7 37.1#

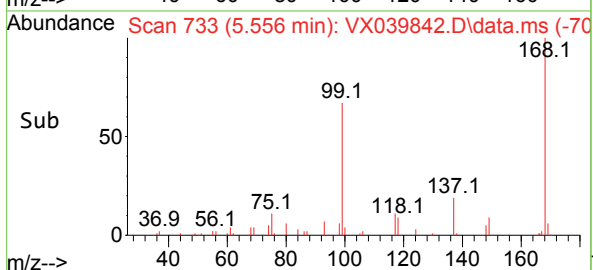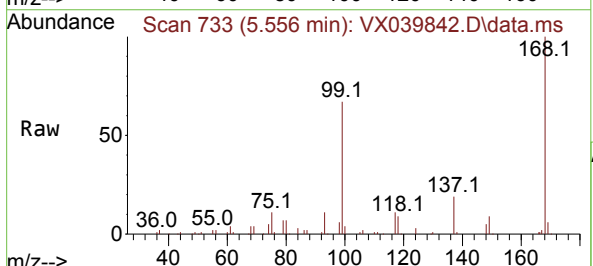






#38
Carbon Tetrachloride
Concen: 6.335 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40







Tgt Ion:117 Resp: 9589
Ion Ratio Lower Upper
117 100
119 4.7 78.2 117.2#
121 0.0 24.4 36.6#



#39
Methylcyclohexane
Concen: 1.326 ug/l
RT: 7.123 min Scan# 990
Delta R.T. -0.256 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion: 83 Resp: 2632
Ion Ratio Lower Upper
83 100
55 0.0 64.6 97.0#
98 200.9 36.7 55.1#




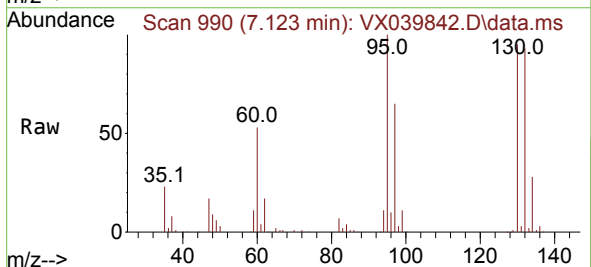


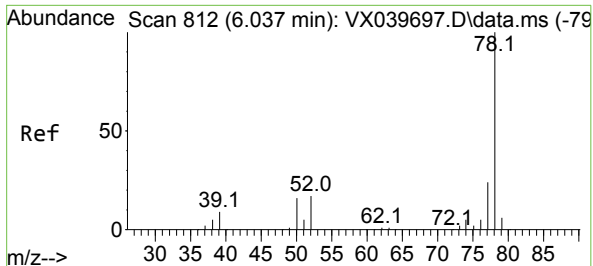

#40
Benzene
Concen: 0.511 ug/l
RT: 6.037 min Scan# 812
Delta R.T. -0.000 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion: 78 Resp: 2391
Ion Ratio Lower Upper
78 100
77 28.8 19.3 28.9

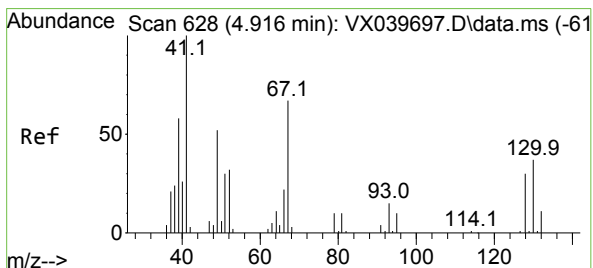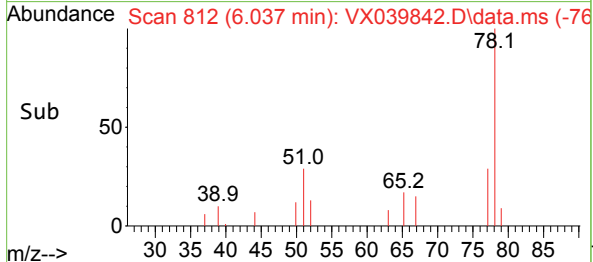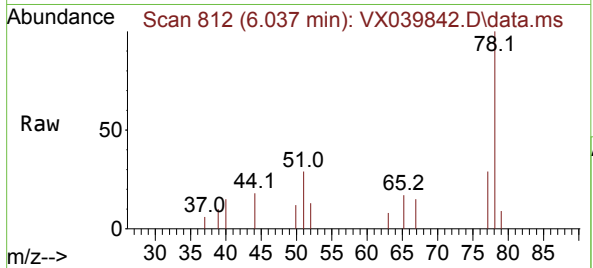

#41
Methacrylonitrile
Concen: 0.896 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.104 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion: 41 Resp: 966
Ion Ratio Lower Upper
41 100
39 52.9 45.2 67.8
67 0.0 52.6 78.8#
52 0.0 22.7 34.1#

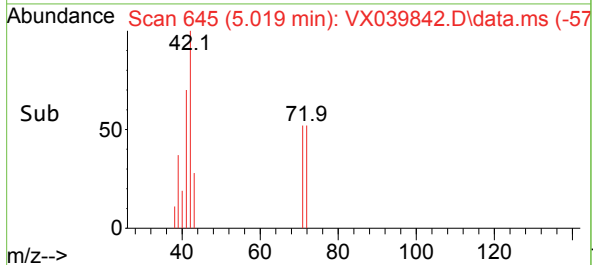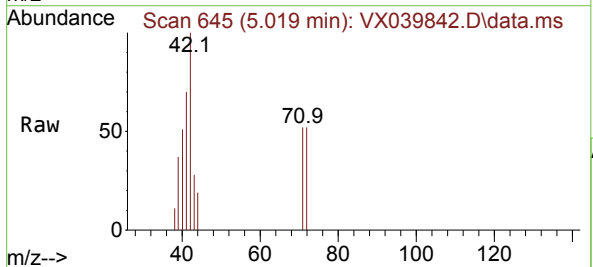

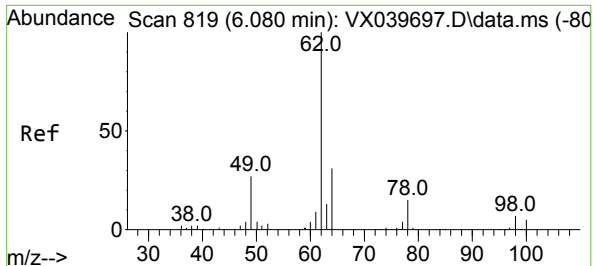

#42

1,2-Dichloroethane

Concen: 1.253 ug/l

RT: 6.098 min Scan# 819

Delta R.T. 0.018 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22

Instrument :

MSVOA_X

ClientSampleId :





SUMOGW-4-37-40

Tgt Ion: 62 Resp: 2229

Ion Ratio Lower Upper

62 100

98 7.0 0.0 16.0

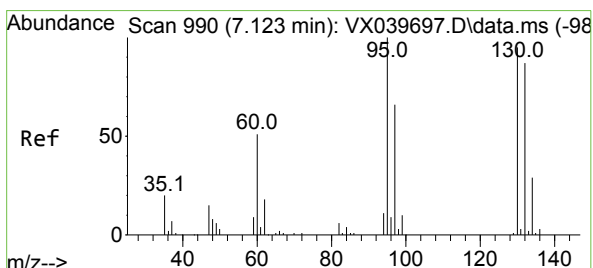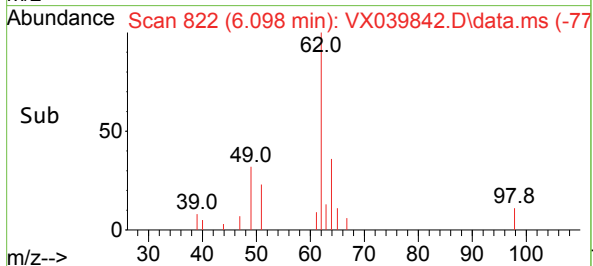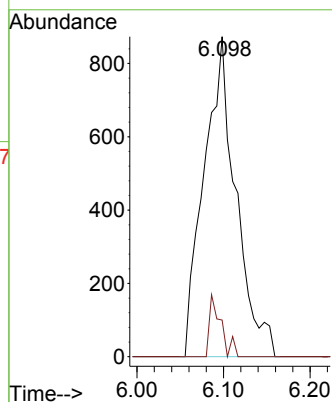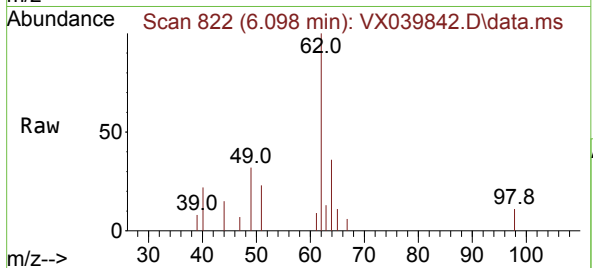

#44

Trichloroethene

Concen: 163.752 ug/l

RT: 7.123 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX039842.D




Acq: 19 Jan 2024 16:22


Tgt Ion:130 Resp: 187806

Ion Ratio Lower Upper

130 100

95 104.9 0.0 204.4


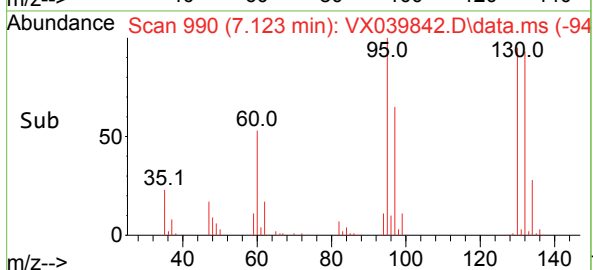

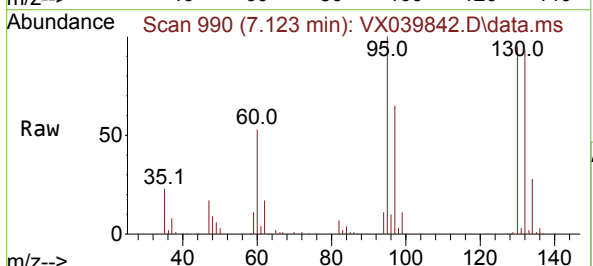




#45
1,2-Dichloropropane
Concen: 0.406 ug/l
RT: 7.440 min Scan# 1041
Delta R.T. 0.012 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion: 63 Resp: 510
Ion Ratio Lower Upper
63 100
65 26.7 24.3 36.5

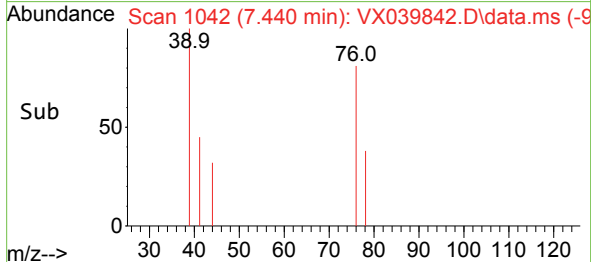

#48
Methyl methacrylate
Concen: 0.274 ug/l
RT: 7.433 min Scan# 1041
Delta R.T. -0.256 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion: 41 Resp: 436
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 72.7 47.7 71.5#


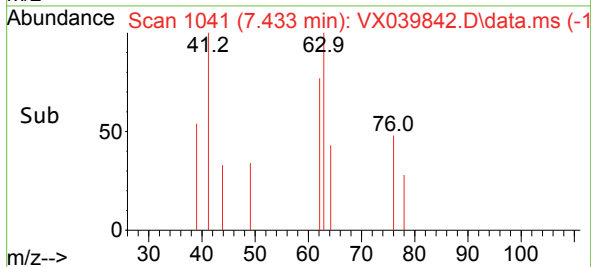

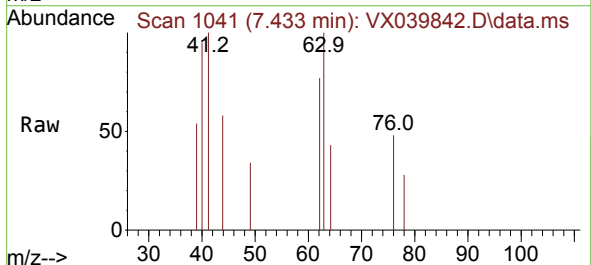




#49
1,4-Dioxane
Concen: 25.812 ug/l
RT: 7.671 min Scan# 1078
Delta R.T. 0.012 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion: 88 Resp: 794
Ion Ratio Lower Upper
88 100
43 22.5 0.0 0.0#
58 53.0 60.1 90.1#



#50
Toluene-d8
Concen: 48.314 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion: 98 Resp: 193471
Ion Ratio Lower Upper
98 100
100 64.6 53.1 79.7




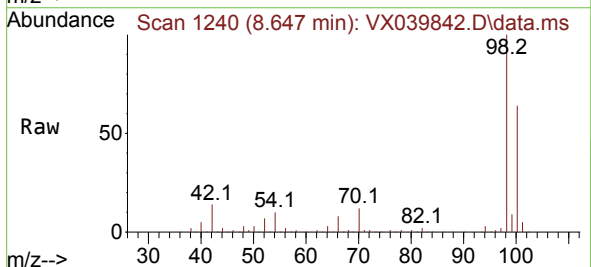




#51
4-Methyl-2-Pentanone
Concen: 0.442 ug/l
RT: 8.641 min Scan# 11
Delta R.T. 0.067 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion: 43 Resp: 985
Ion Ratio Lower Upper
43 100
58 186.5 30.4 45.6#



#60
Dibromochloromethane
Concen: 99.156 ug/l
RT: 9.268 min Scan# 1342
Delta R.T. -0.250 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion: 129 Resp: 111282
Ion Ratio Lower Upper
129 100
127 0.0 38.8 116.4#




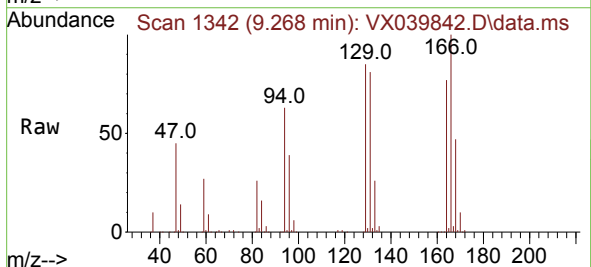




#62
4-Bromofluorobenzene
Concen: 47.983 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion: 95 Resp: 75138
Ion Ratio Lower Upper
95 100
174 69.9 0.0 135.6
176 66.8 0.0 131.0

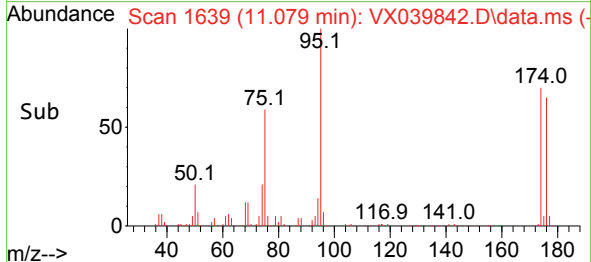

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion: 117 Resp: 151150
Ion Ratio Lower Upper
117 100
82 57.4 46.2 69.4
119 32.9 25.5 38.3









#64
Tetrachloroethene
Concen: 107.280 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion:164 Resp: 105449
Ion Ratio Lower Upper
164 100
166 127.5 102.7 154.1
129 102.1 80.4 120.6
131 99.5 76.5 114.7



#65
Chlorobenzene
Concen: 0.574 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion:112 Resp: 1808
Ion Ratio Lower Upper
112 100
114 28.5 25.7 38.5




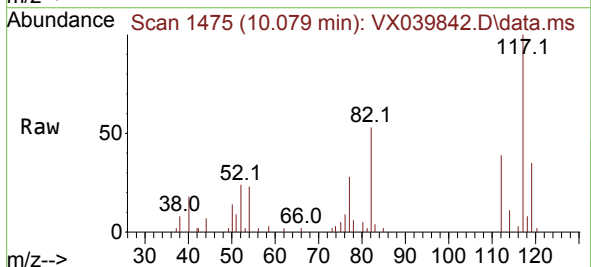




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion:152 Resp: 72981
Ion Ratio Lower Upper
152 100
115 63.8 43.3 129.9
150 156.7 0.0 345.0

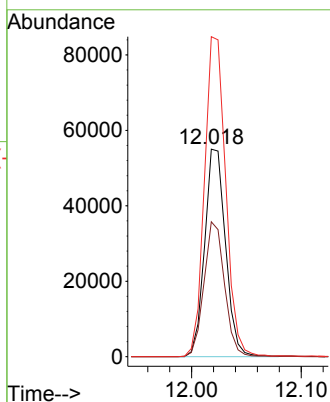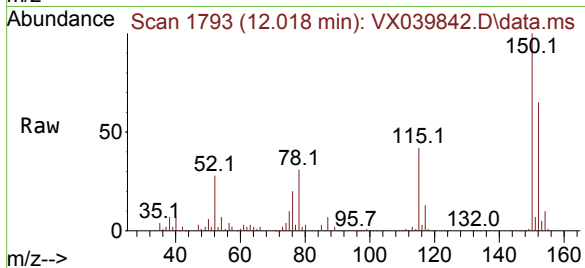

#76
1,2,3-Trichloropropane
Concen: 22.323 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion: 75 Resp: 42237
Ion Ratio Lower Upper
75 100
77 1.0 19.1 57.5#


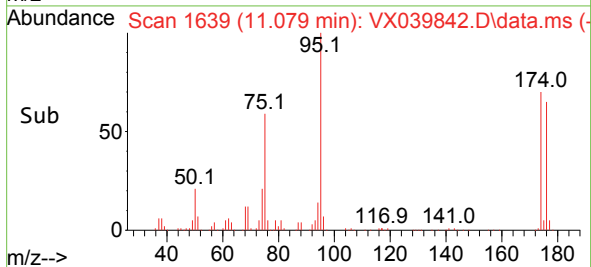
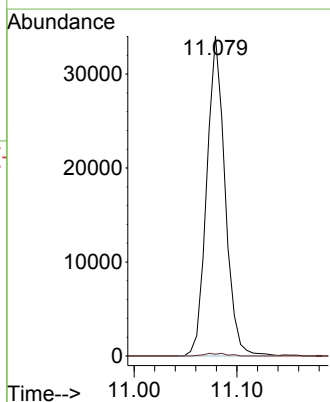
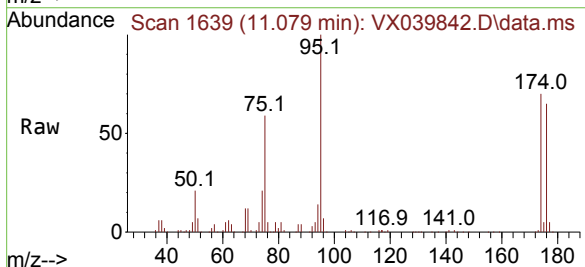




#81
trans-1,4-Dichloro-2-butene
Concen: 64.678 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22




Instrument :
MSVOA_X
ClientSampleId :
SUMOGW-4-37-40


Tgt Ion: 75 Resp: 42237
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#



#91
1,2-Dichlorobenzene
Concen: 1.530 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.000 min
Lab File: VX039842.D
Acq: 19 Jan 2024 16:22

Tgt Ion: 146 Resp: 3752
Ion Ratio Lower Upper
146 100
111 46.3 22.4 67.0
148 61.4 31.6 95.0





#93

1,2,4-Trichlorobenzene

Concen: 1.408 ug/l

RT: 13.591 min Scan# 2050

Delta R.T. 0.006 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22

Instrument :

MSVOA_X

ClientSampleId :

SUMOGW-4-37-40





Tgt Ion:180 Resp: 2110

Ion Ratio Lower Upper

180 100

182 94.7 48.3 144.8

145 38.4 18.0 54.0

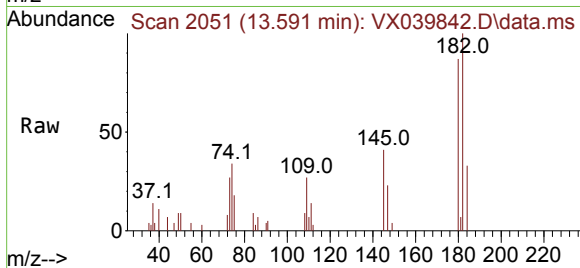

#96

1,2,3-Trichlorobenzene

Concen: 0.350 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX039842.D

Acq: 19 Jan 2024 16:22

Tgt Ion:180 Resp: 529

Ion Ratio Lower Upper

180 100

182 70.3 46.9 140.6

145 26.5 17.8 53.5

