

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012020\
 Data File : VX014670.D
 Acq On : 20 Jan 2020 15:07
 Operator : JC/SP
 Sample : L1173-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 0052-DECANT-H2O-COMP-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	43	rBV	1307138	1550119	70.68%	11.803%
2	1.600	109	117	122	rVB7	30990	64680	2.95%	0.492%
3	2.430	248	253	257	rVB	20693	30086	1.37%	0.229%
4	5.478	740	753	765	rBV2	247150	720862	32.87%	5.489%
5	5.642	770	780	796	rVB	434572	1226405	55.92%	9.338%
6	6.045	838	846	859	rBV	287299	734333	33.48%	5.591%
7	6.843	965	977	987	rBV	681881	1590053	72.50%	12.107%
8	8.709	1276	1283	1293	rBV	1397105	2193293	100.00%	16.700%
9	10.105	1506	1512	1520	rBV	1419609	1880632	85.74%	14.319%
10	11.129	1674	1680	1688	rBV	1123688	1432055	65.29%	10.904%
11	12.074	1829	1835	1841	rBV	1390879	1711007	78.01%	13.028%


Sum of corrected areas: 13133525

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012020\
Data File : VX014670.D
Acq On : 20 Jan 2020 15:07
Operator : JC/SP
Sample : L1173-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
0052-DECANT-H2O-COMP-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

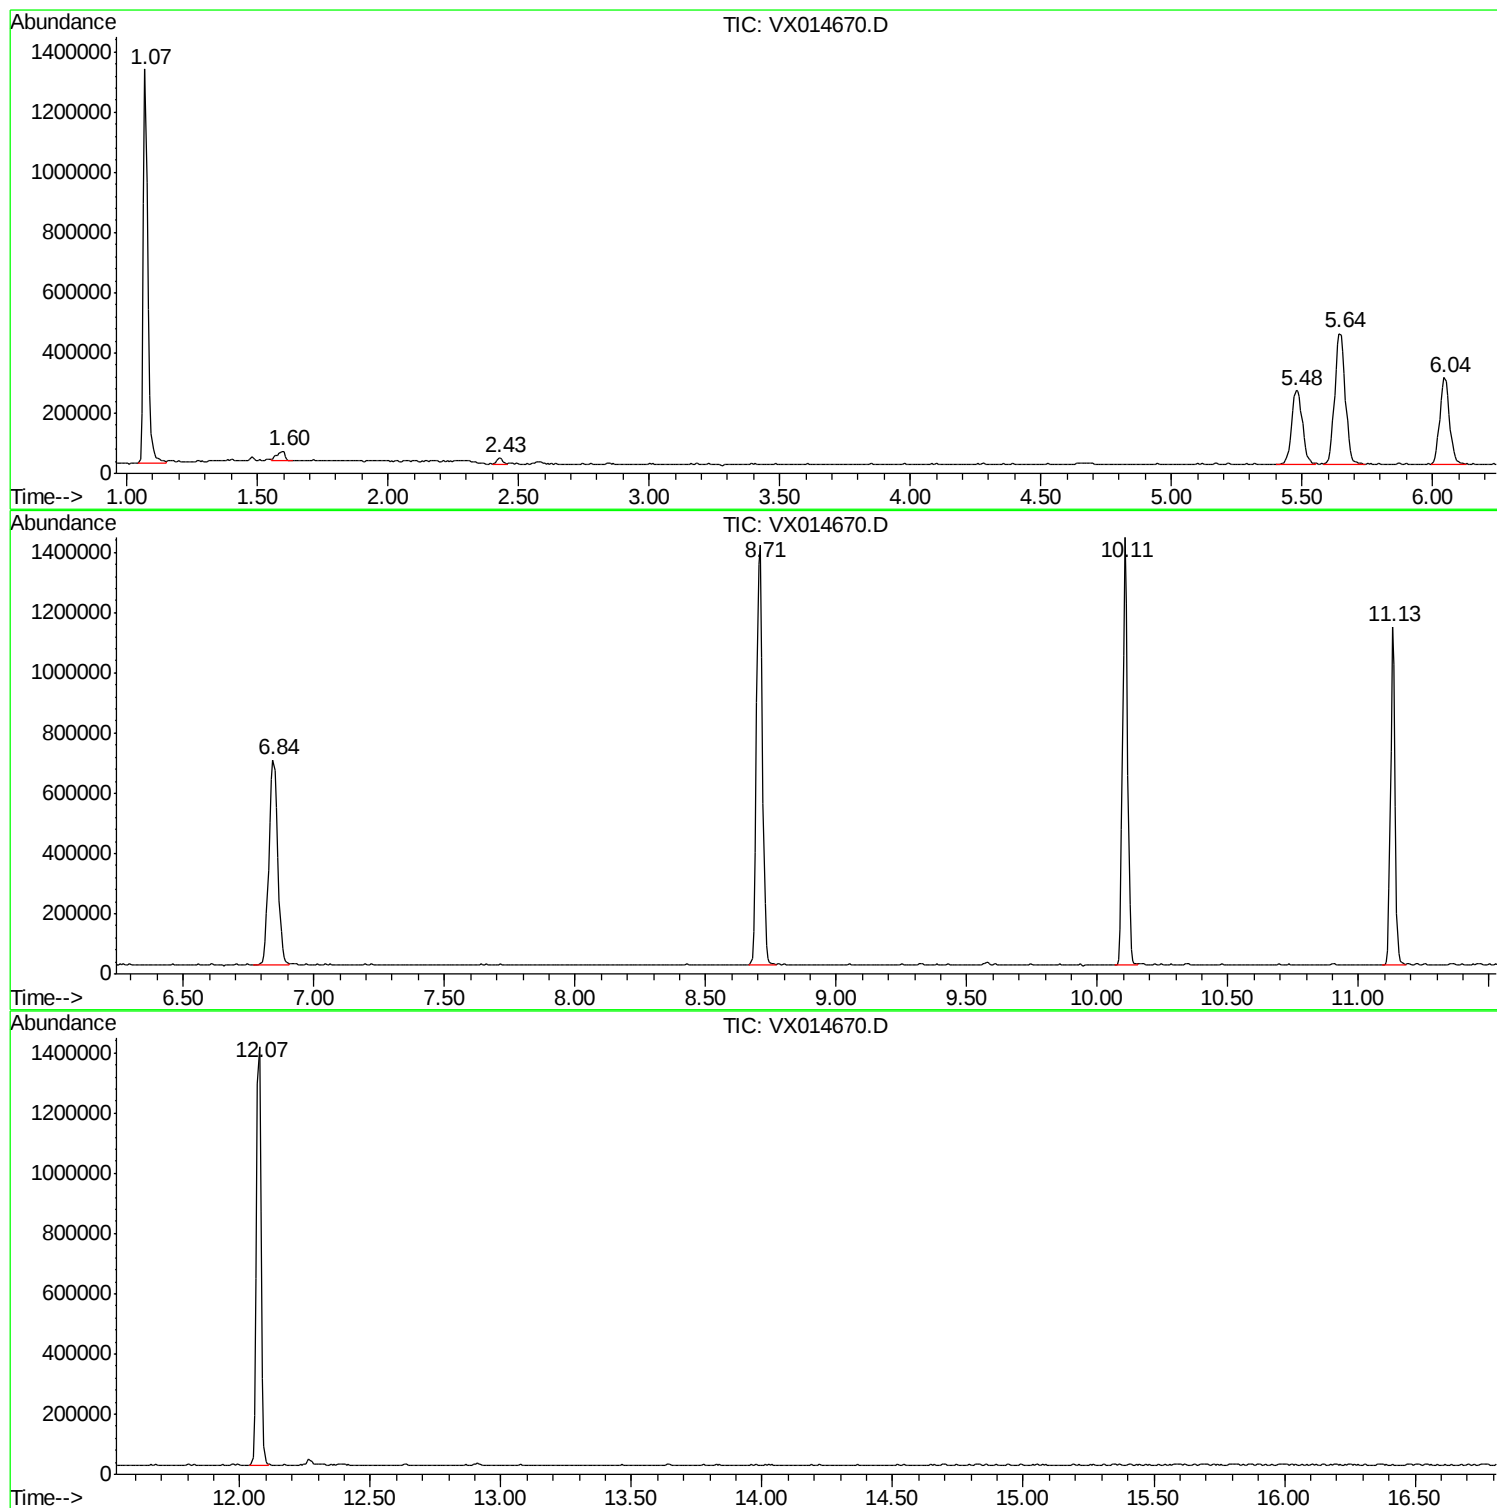

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX012020\
Data File : VX014670.D
Acq On : 20 Jan 2020 15:07
Operator : JC/SP
Sample : L1173-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
0052-DECANT-H2O-COMP-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX012020\
Data File : VX014670.D
Acq On : 20 Jan 2020 15:07
Operator : JC/SP
Sample : L1173-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
0052-DECANT-H2O-COMP-4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc