


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012021\
Data File : VX020674.D
Acq On : 20 Jan 2021 09:26
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
Title : SW846 8260
Last Update : Tue Jan 19 14:09:08 2021

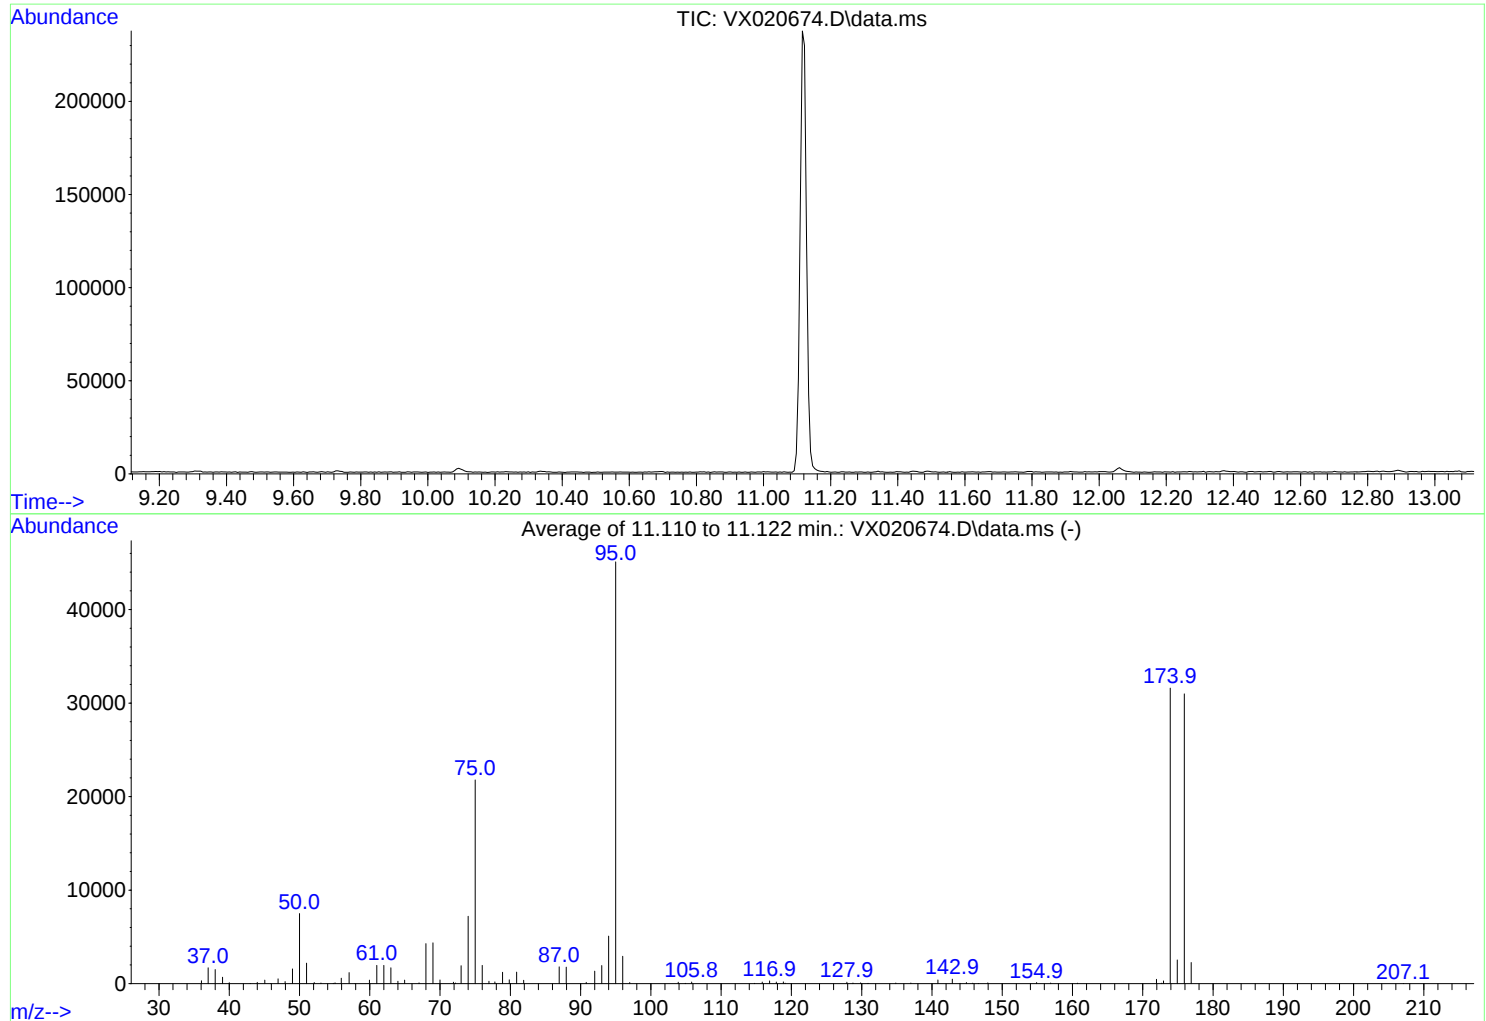

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	7500	PASS
75	95	30	60	48.3	21773	PASS
95	95	100	100	100.0	45101	PASS
96	95	5	9	6.5	2918	PASS
173	174	0.00	2	0.9	290	PASS
174	95	50	100	70.1	31595	PASS
175	174	5	9	8.0	2533	PASS
176	174	95	101	98.1	30987	PASS
177	176	5	9	7.3	2259	PASS