

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012022\
 Data File : VX026524.D
 Acq On : 20 Jan 2022 11:28
 Operator : JC/MD
 Sample : VX0120WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0120WBL01

Quant Time: Jan 21 04:01:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	142676	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	240501	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	211754	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	87702	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	95690	48.011	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	96.020%
35) Dibromofluoromethane	5.391	113	75913	48.879	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.760%
50) Toluene-d8	8.653	98	280583	50.134	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.260%
62) 4-Bromofluorobenzene	11.079	95	99996	50.296	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012022\
Data File : VX026524.D
Acq On : 20 Jan 2022 11:28
Operator : JC/MD
Sample : VX0120WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0120WBL01

Quant Time: Jan 21 04:01:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration




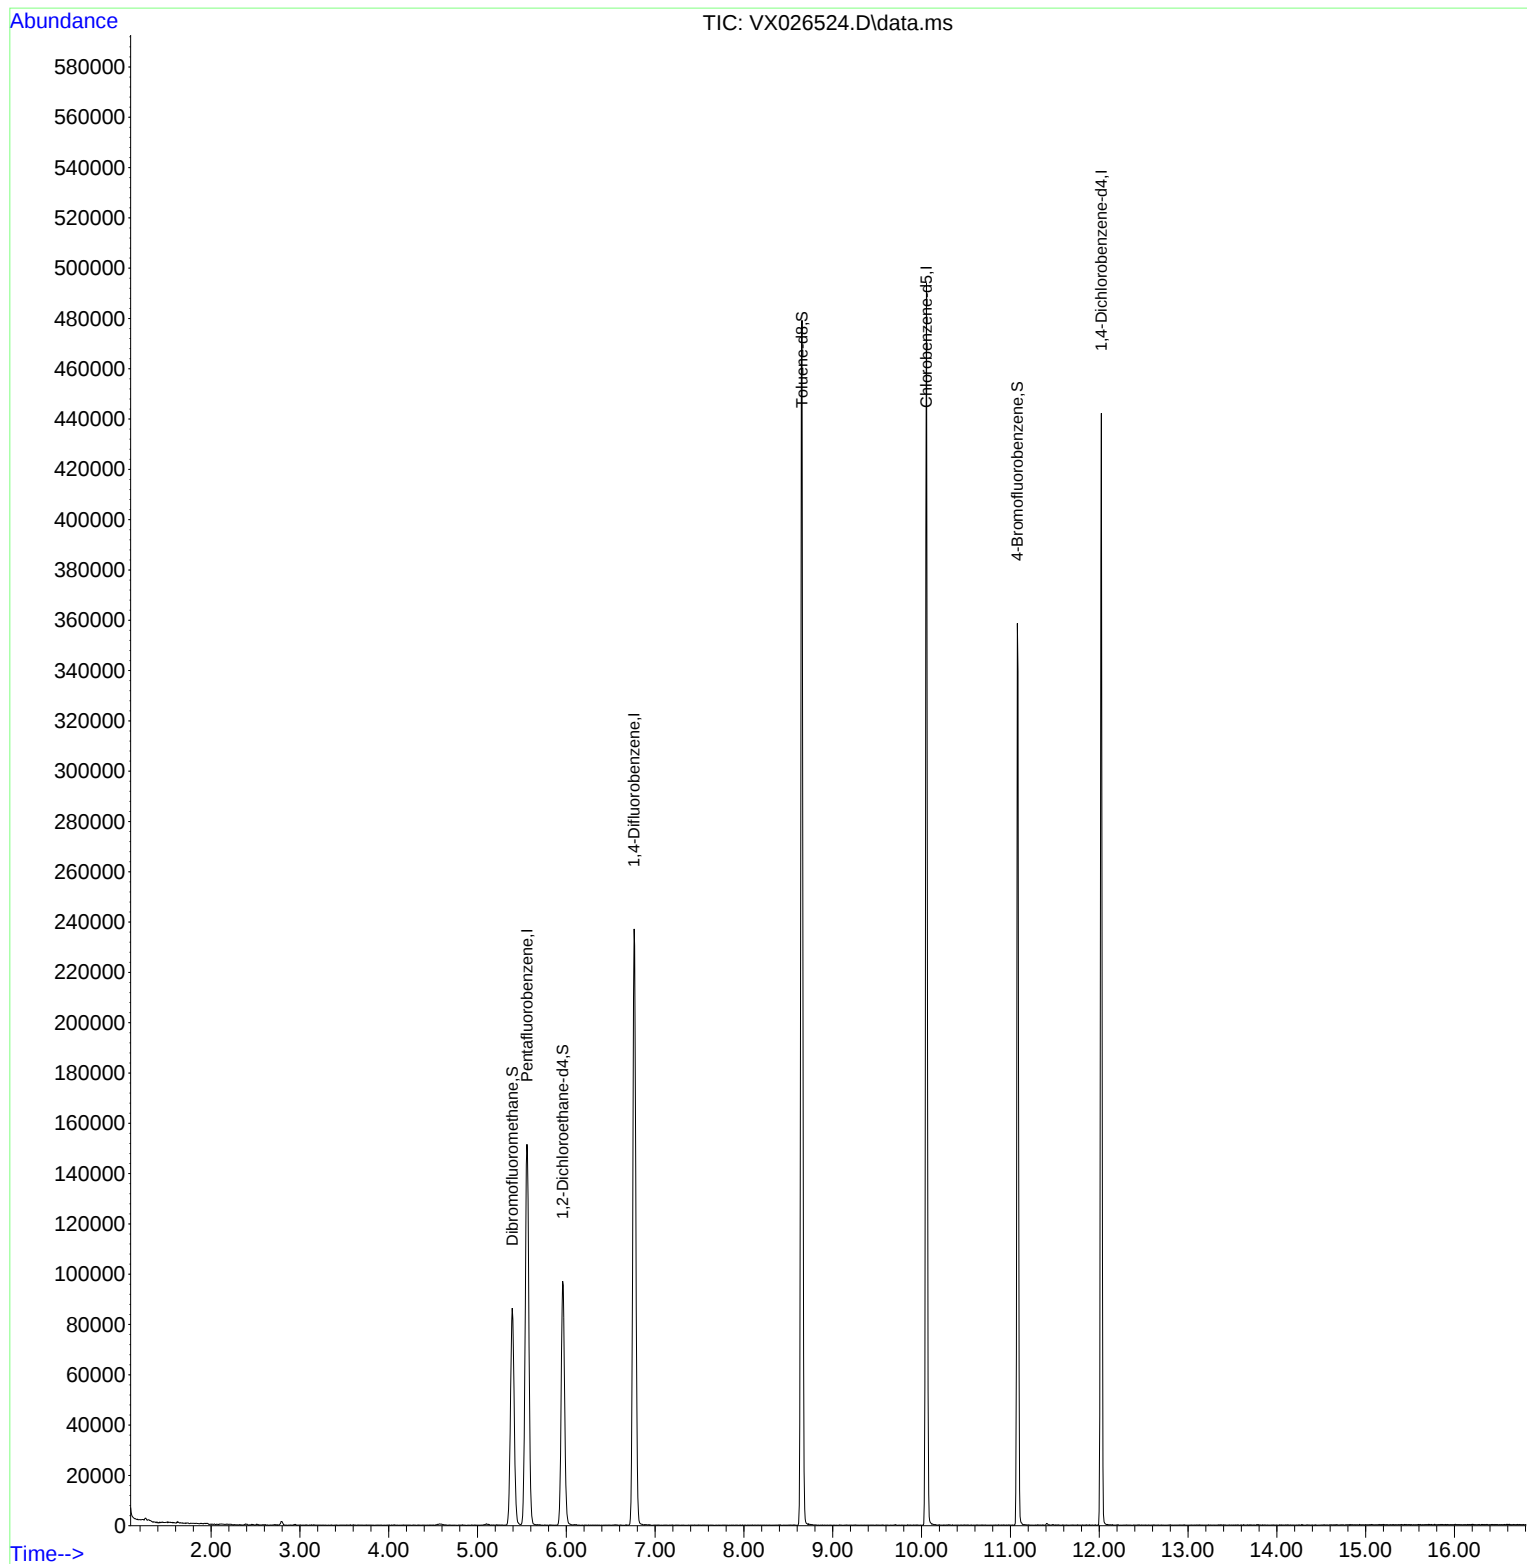


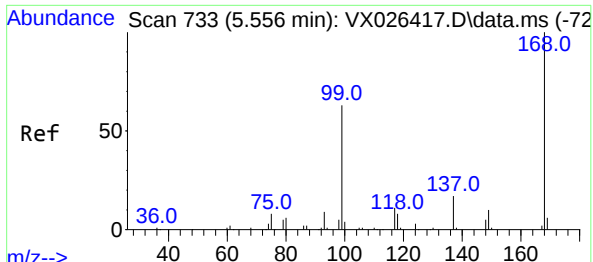

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX026524.D
Acq: 20 Jan 2022 11:28




Instrument :
MSVOA_X
ClientSampleId :
VX0120WBL01


Tgt Ion:168 Resp: 142676
Ion Ratio Lower Upper
168 100
99 64.2 50.3 75.5

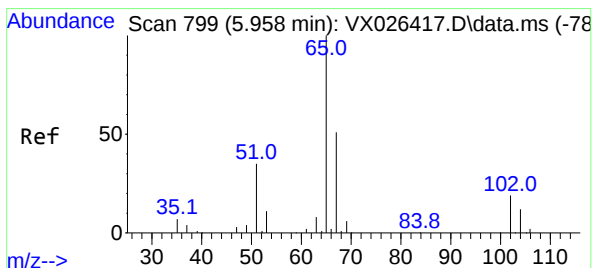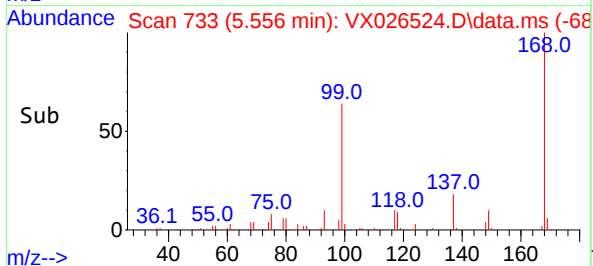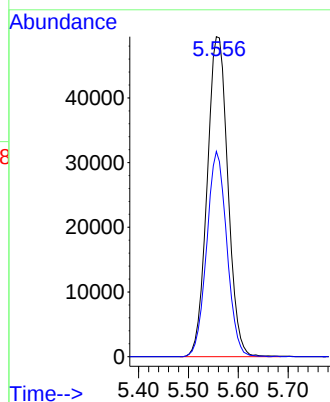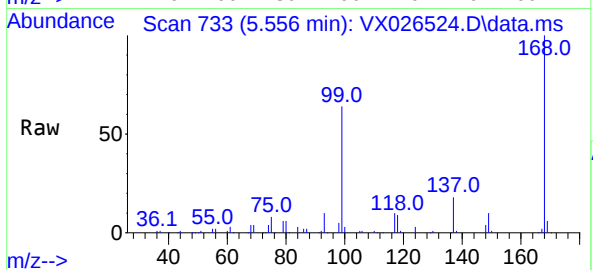

#33
1,2-Dichloroethane-d4
Concen: 48.011 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX026524.D
Acq: 20 Jan 2022 11:28

Tgt Ion: 65 Resp: 95690
Ion Ratio Lower Upper
65 100
67 51.2 0.0 100.8


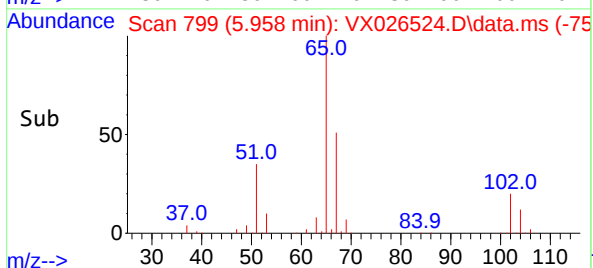
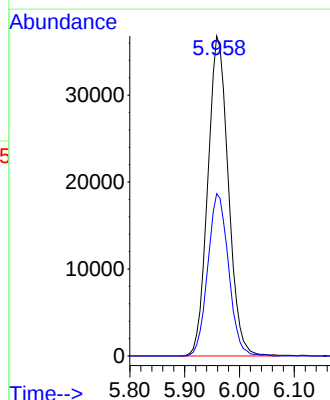
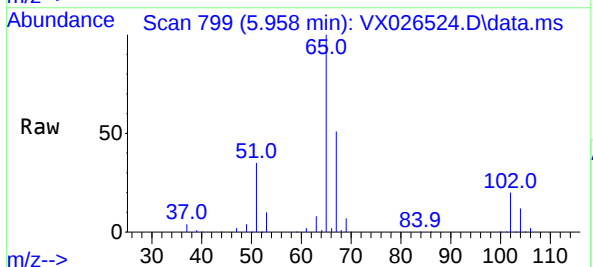


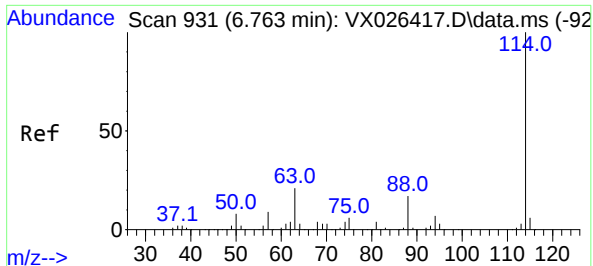

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX026524.D
Acq: 20 Jan 2022 11:28




Instrument :
MSVOA_X
ClientSampleId :
VX0120WBL01


Tgt Ion:114 Resp: 240501
Ion Ratio Lower Upper
114 100
63 21.4 0.0 42.8
88 16.6 0.0 33.0

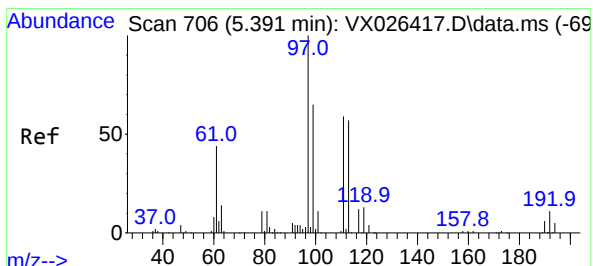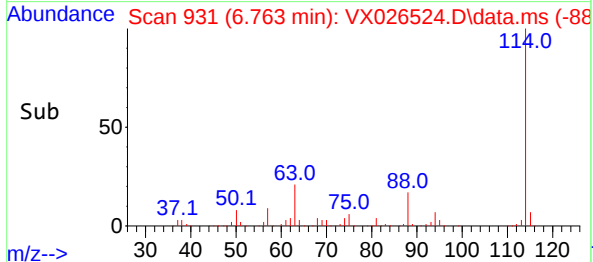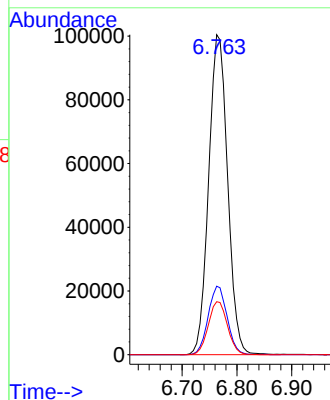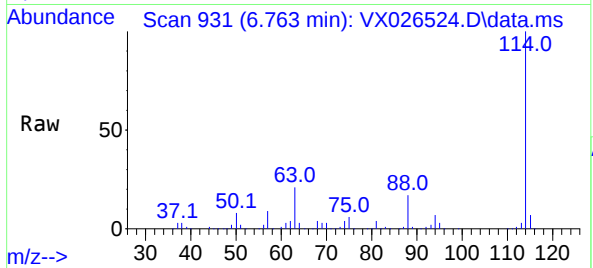

#35
Dibromofluoromethane
Concen: 48.879 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026524.D
Acq: 20 Jan 2022 11:28

Tgt Ion:113 Resp: 75913
Ion Ratio Lower Upper
113 100
111 101.4 81.2 121.8
192 18.7 15.0 22.4


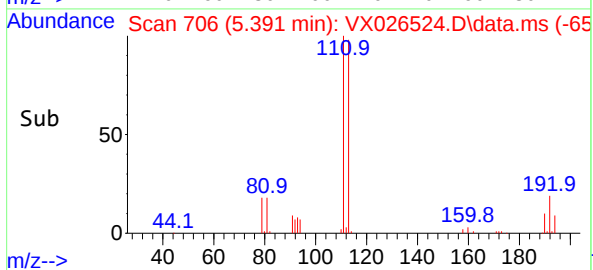
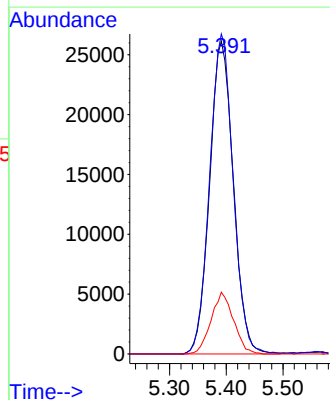
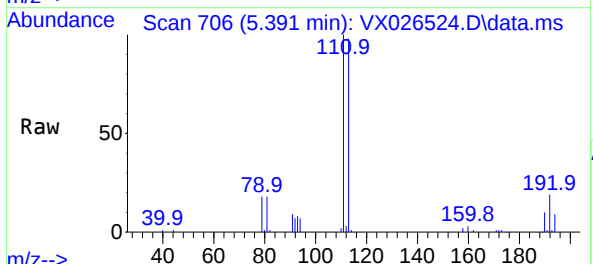


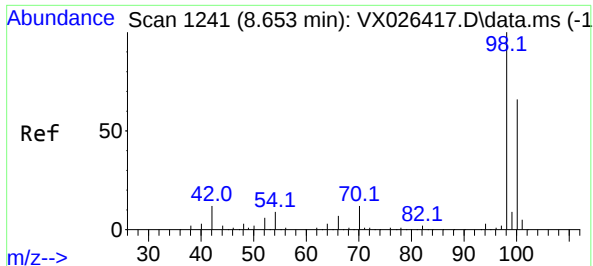

#50
Toluene-d8
Concen: 50.134 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026524.D
Acq: 20 Jan 2022 11:28




Instrument :
MSVOA_X
ClientSampleId :
VX0120WBL01


Tgt Ion: 98 Resp: 280583
Ion Ratio Lower Upper
98 100
100 66.5 53.2 79.8

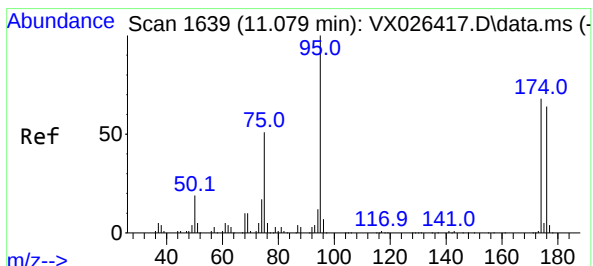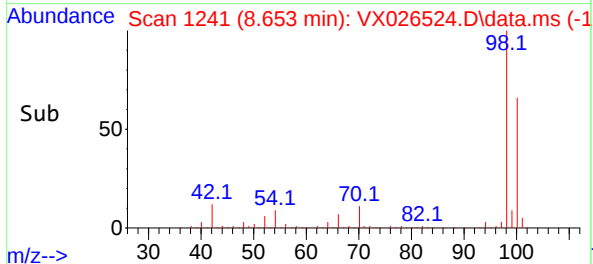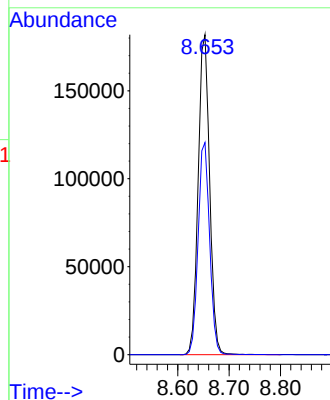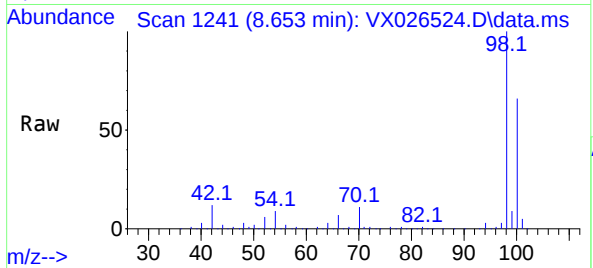

#62
4-Bromofluorobenzene
Concen: 50.296 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026524.D
Acq: 20 Jan 2022 11:28

Tgt Ion: 95 Resp: 99996
Ion Ratio Lower Upper
95 100
174 73.7 0.0 148.6
176 70.8 0.0 141.4


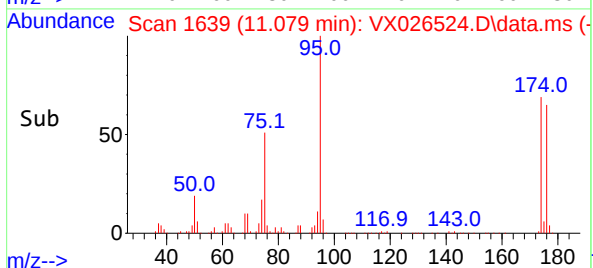
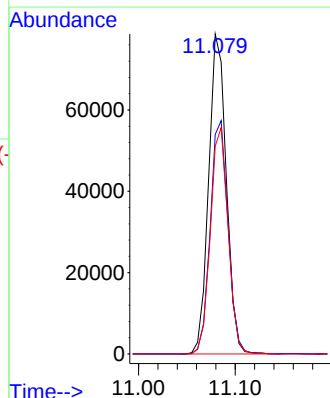
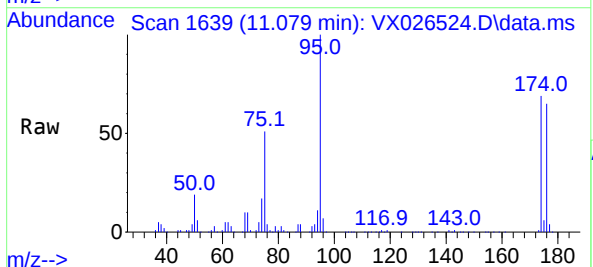


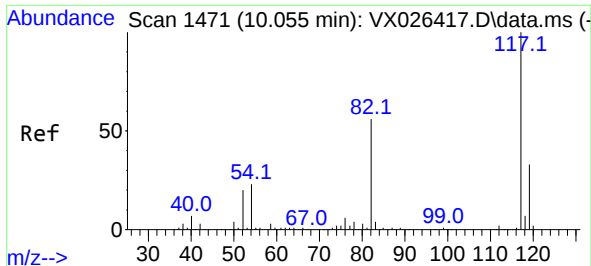

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026524.D
Acq: 20 Jan 2022 11:28

Instrument :
MSVOA_X
ClientSampleId :
VX0120WBL01

Tgt Ion:117 Resp: 211754
Ion Ratio Lower Upper
117 100
82 56.0 45.2 67.8
119 32.1 26.2 39.2

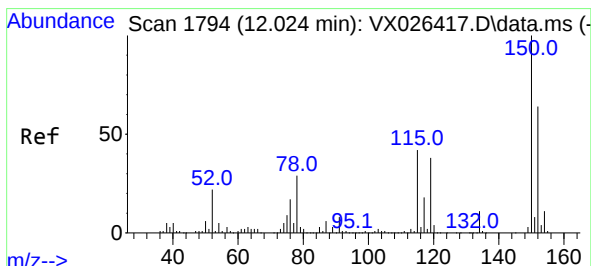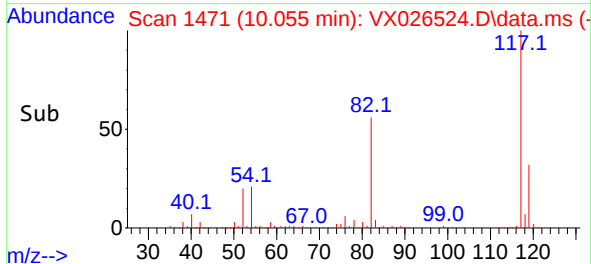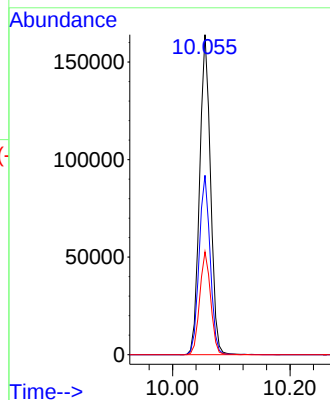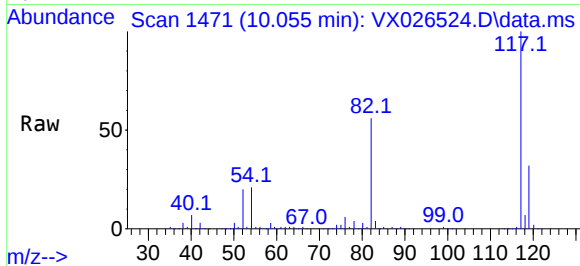

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026524.D
Acq: 20 Jan 2022 11:28

Tgt Ion:152 Resp: 87702
Ion Ratio Lower Upper
152 100
115 61.0 44.2 132.6
150 158.1 0.0 348.2

