

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012022\
 Data File : VX026533.D
 Acq On : 20 Jan 2022 18:12
 Operator : JC/MD
 Sample : N1099-09
 Misc : 5.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-09

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M

Title : SW846 8260

Signal : TIC: VX026533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.721	261	268	277	rBV2	4208	9758	1.55%	0.290%
2	5.397	694	707	721	rBV2	66452	202620	32.10%	6.027%
3	5.556	721	733	751	rVB	128388	367647	58.24%	10.936%
4	5.964	789	800	817	rBV	80552	216059	34.23%	6.427%
5	6.763	920	931	944	rBV	195220	473548	75.02%	14.086%
6	8.653	1234	1241	1250	rBV	393994	631236	100.00%	18.776%
7	10.055	1465	1471	1483	rBV	370488	546333	86.55%	16.251%
8	11.085	1634	1640	1651	rBV	303294	408644	64.74%	12.155%
9	12.024	1789	1794	1805	rVB	391256	506028	80.16%	15.052%




Sum of corrected areas: 3361873

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012022\
Data File : VX026533.D
Acq On : 20 Jan 2022 18:12
Operator : JC/MD
Sample : N1099-09
Misc : 5.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VACLOT-BACKFILL-TILCON-09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

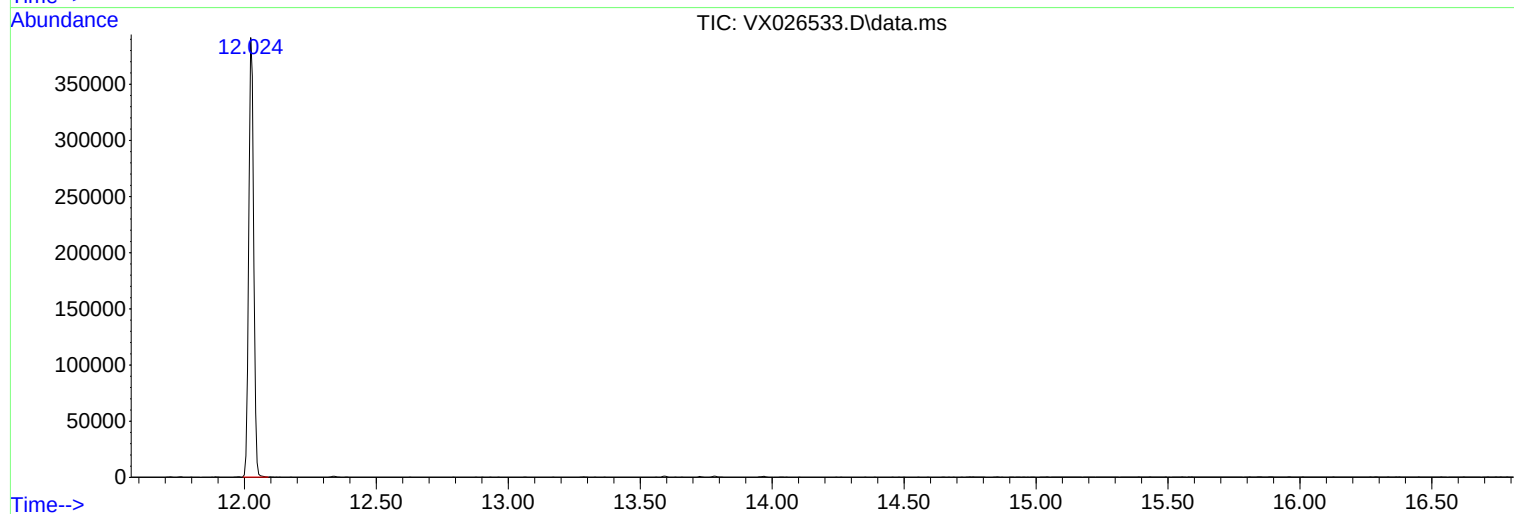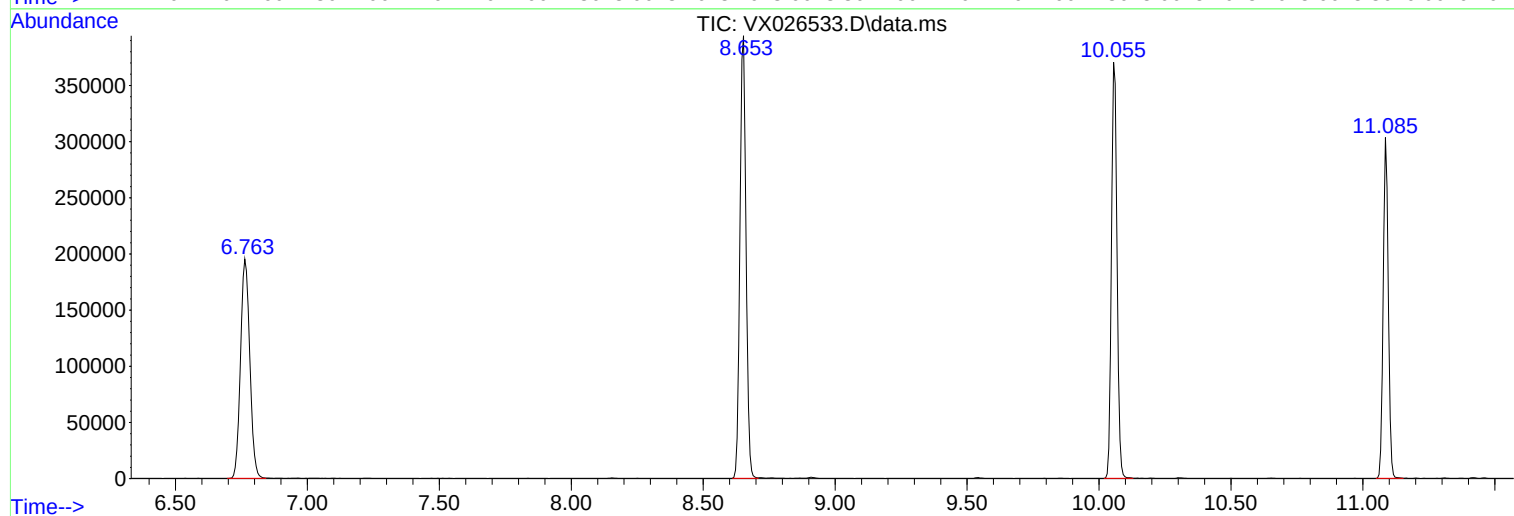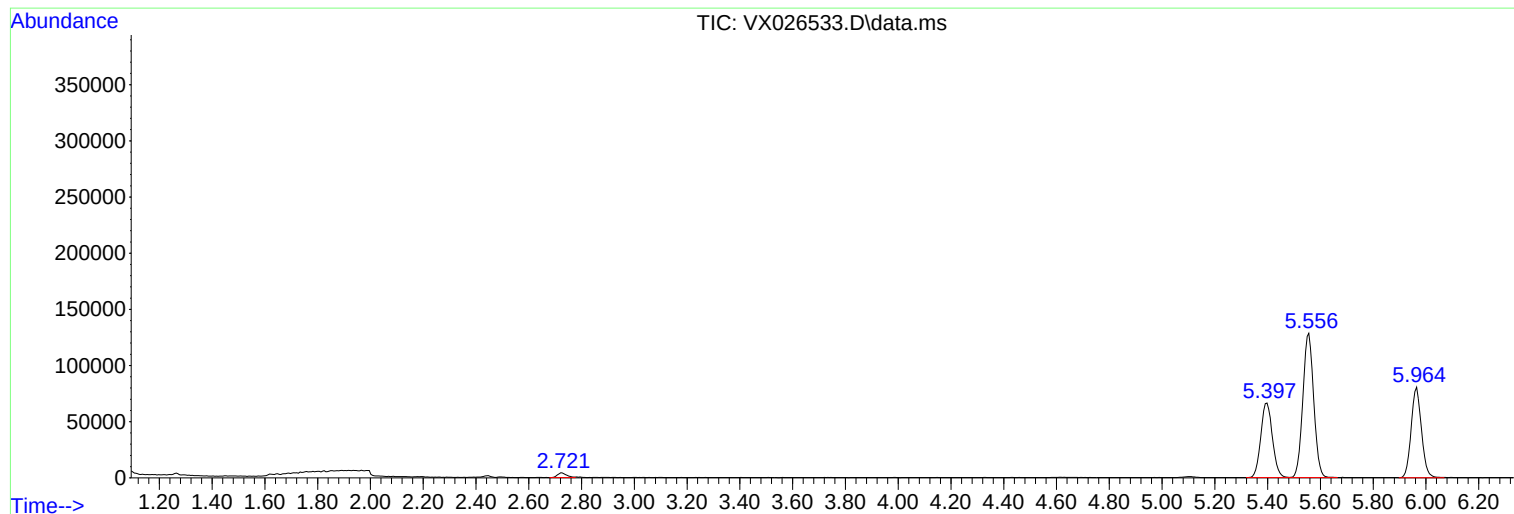

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012022\
Data File : VX026533.D
Acq On : 20 Jan 2022 18:12
Operator : JC/MD
Sample : N1099-09
Misc : 5.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VACLOT-BACKFILL-TILCON-09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012022\
Data File : VX026533.D
Acq On : 20 Jan 2022 18:12
Operator : JC/MD
Sample : N1099-09
Misc : 5.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VACLOT-BACKFILL-TILCON-09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc