
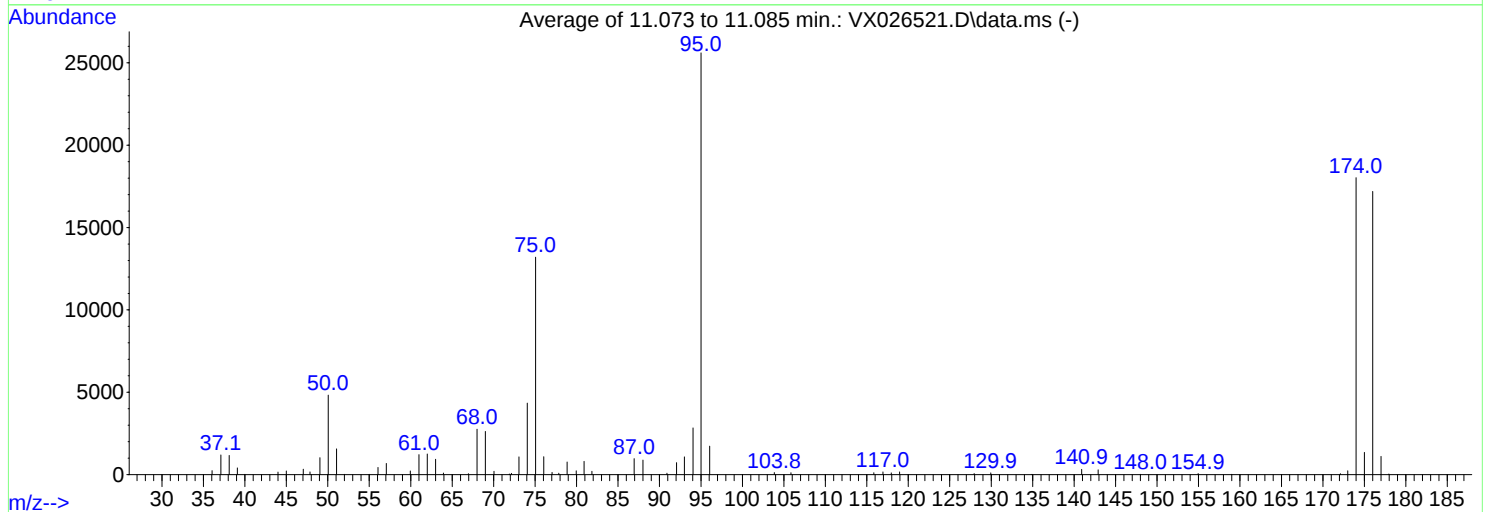


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012022\
 Data File : VX026521.D
 Acq On : 20 Jan 2022 09:58
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Title : SW846 8260
 Last Update : Tue Jan 11 14:45:13 2022

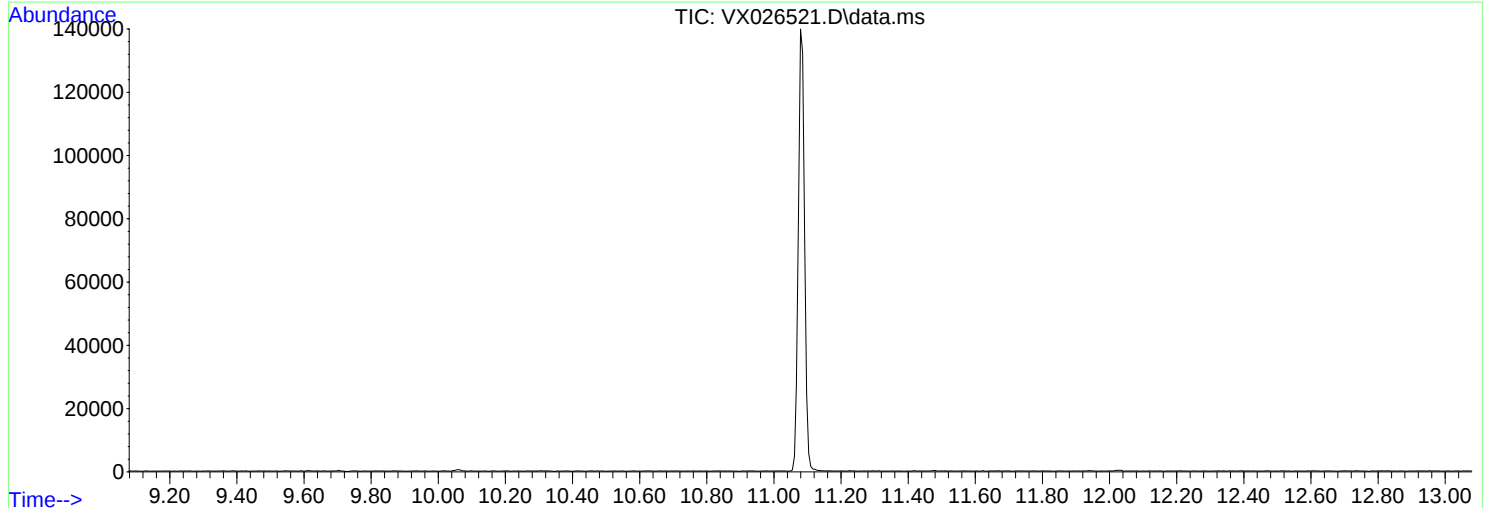

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	4824	PASS
75	95	30	60	51.5	13198	PASS
95	95	100	100	100.0	25605	PASS
96	95	5	9	6.8	1732	PASS
173	174	0.00	2	1.3	232	PASS
174	95	50	100	70.4	18032	PASS
175	174	5	9	7.5	1355	PASS
176	174	95	101	95.3	17192	PASS
177	176	5	9	6.4	1104	PASS