

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX012119\
 Data File : VX007168.D
 Acq On : 21 Jan 2019 19:20
 Operator : JC/SP
 Sample : K1195-05DL 5X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SS038MW013-190116DL

Quant Time: Jan 22 00:09:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 08 14:06:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	566581	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	875103	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	833056	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	426774	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	304601	51.44	ug/l	0.00
Spiked Amount			Recovery	=	102.88%	
35) Dibromofluoromethane	5.51	113	271202	48.39	ug/l	0.00
Spiked Amount			Recovery	=	96.78%	
50) Toluene-d8	8.71	98	1055287	51.45	ug/l	0.00
Spiked Amount			Recovery	=	102.90%	
62) 4-Bromofluorobenzene	11.13	95	386214	54.01	ug/l	0.00
Spiked Amount			Recovery	=	108.02%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
4) Vinyl Chloride	1.40	62	1375	0.236	ug/l	99
11) Tert butyl alcohol	3.07	59	398	0.285	ug/l #	5
13) Acrolein	2.31	56	372	3.694	ug/l #	1
16) Acetone	2.44	43	1262	0.431	ug/l #	78
18) Methyl Acetate	2.77	43	1976	0.233	ug/l	93
20) Methylene Chloride	2.86	84	1210	Below Cal	#	68
29) Tetrahydrofuran	5.12	42	747	0.274	ug/l #	44
36) 1,1-Dichloropropene	5.66	75	34963	4.595	ug/l #	49
38) Carbon Tetrachloride	5.66	117	51217	6.691	ug/l #	15
39) Methylcyclohexane	7.46	83	2489	0.257	ug/l	90
40) Benzene	6.15	78	14798	0.637	ug/l	96
49) 1,4-Dioxane	7.71	88	225	Below Cal	#	60
65) Chlorobenzene	10.13	112	549813	30.260	ug/l	98
73) Isopropylbenzene	11.02	105	32561	1.082	ug/l	100
76) 1,2,3-Trichloropropane	11.13	75	188156	21.756	ug/l #	40
78) n-propylbenzene	11.36	91	26189	0.793	ug/l	99
79) 2-Chlorotoluene	11.36	91	26189	1.317	ug/l #	38
81) trans-1,4-Dichloro-2-buten	11.13	75	188156	64.473	ug/l #	10
82) 4-Chlorotoluene	11.36	91	26189	1.137	ug/l #	42
83) tert-Butylbenzene	11.77	119	28042	1.118	ug/l	87
85) sec-Butylbenzene	11.94	105	50980	1.701	ug/l	99
86) p-Isopropyltoluene	12.23	119	129462	4.831	ug/l	97
88) 1,4-Dichlorobenzene	12.10	146	3300	0.377	ug/l #	1
89) n-Butylbenzene	12.39	91	6232	0.273	ug/l #	63
90) Hexachloroethane	12.70	117	58671	15.824	ug/l #	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012119\
Data File : VX007168.D
Acq On : 21 Jan 2019 19:20
Operator : JC/SP
Sample : K1195-05DL 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SS038MW013-190116DL

Quant Time: Jan 22 00:09:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 08 14:06:59 2019
Response via : Initial Calibration

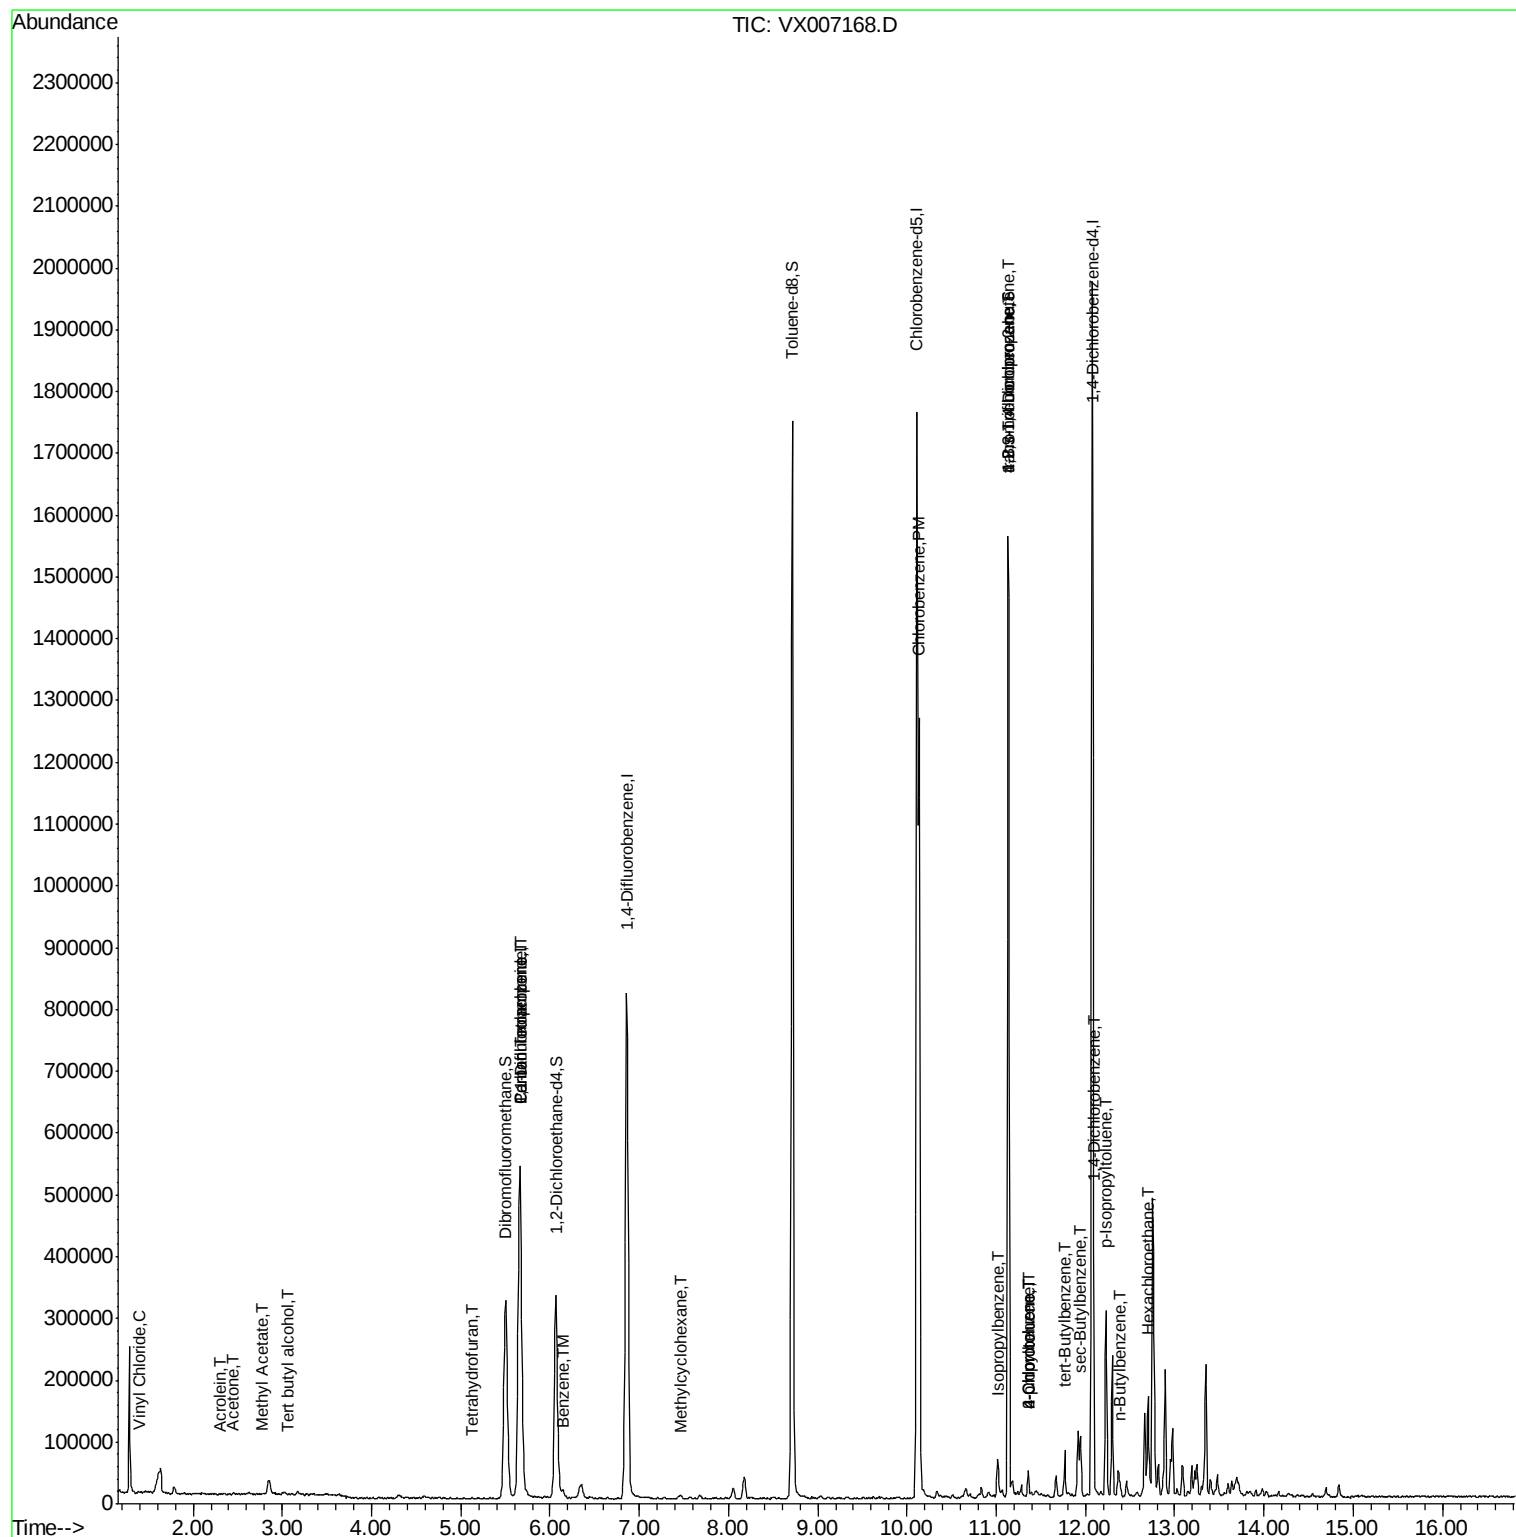



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :


SS038MW013-190116DL

Tot Ion:168 Resp: 566581

Ion Ratio Lower Upper

168 100

99 49.0 41.8 62.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

200000

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

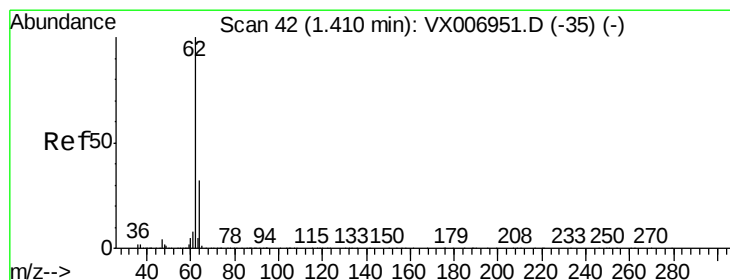

#4

Vinyl Chloride

Concen: 0.236 ug/l

RT: 1.40 min Scan# 41

Delta R.T. -0.01 min

Lab File: VX007168.D


Acq: 21 Jan 2019 19:20

Tgt Ion: 62 Resp: 1375

Ion Ratio Lower Upper

62 100

64 30.8 25.1 37.7

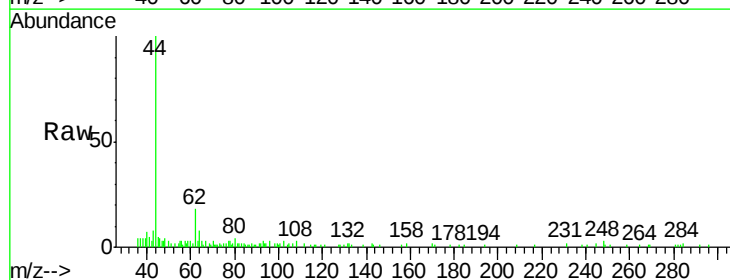

Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 63.90 (63.60 to 64.60): VX0

1.40

1000

800

600


400


200

0

Time-->

1.35 1.40 1.45






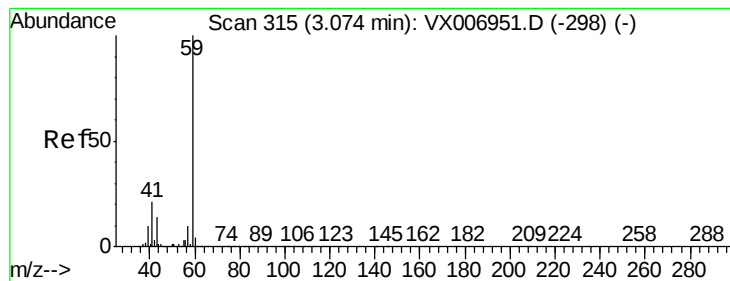


#11

Tert butyl alcohol
Concen: 0.285 ug/l
RT: 3.07 min Scan# 314
Delta R.T. -0.01 min
Lab File: VX007168.D
Acq: 21 Jan 2019 19:20

Instrument :
MSVOA_X
ClientSampleId :
SS038MW013-190116DL




Tot Ion: 59 Resp: 398
Ion Ratio Lower Upper
59 100
57 46.5 8.5 12.7#

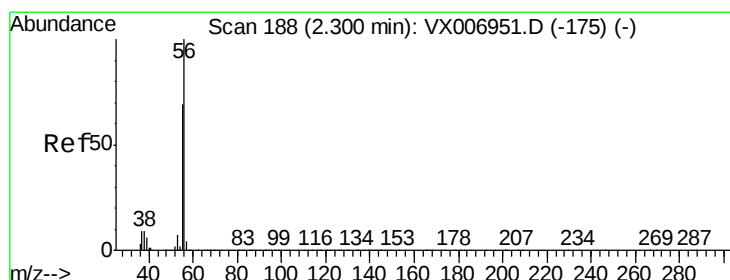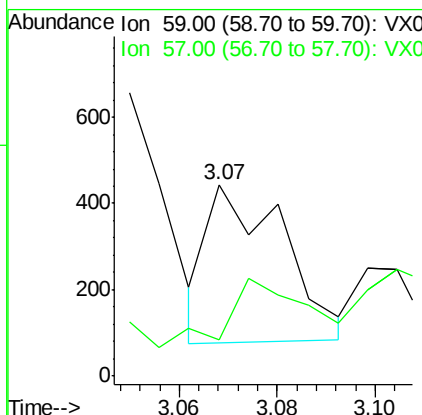


#13

Acrolein
Concen: 3.694 ug/l
RT: 2.31 min Scan# 189
Delta R.T. 0.01 min
Lab File: VX007168.D
Acq: 21 Jan 2019 19:20

Tgt Ion: 56 Resp: 372
Ion Ratio Lower Upper
56 100
55 171.2 58.2 87.4#

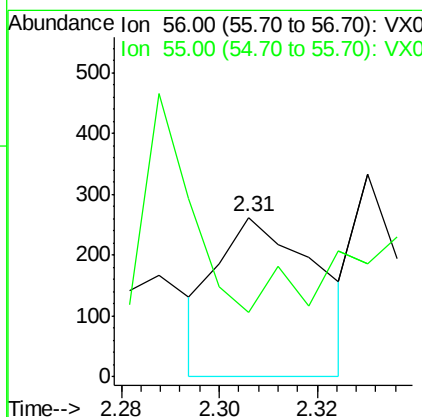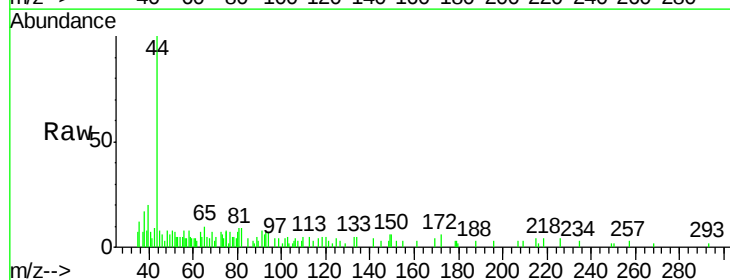

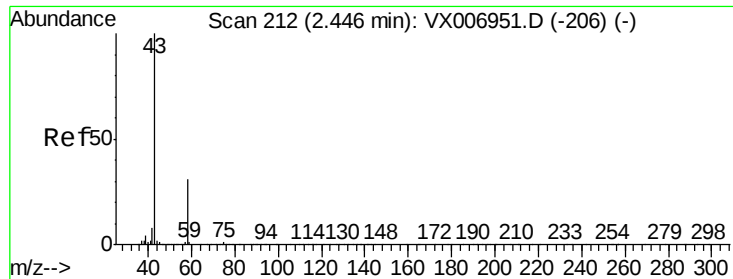

#16

Acetone

Concen: 0.431 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :





SS038MW013-190116DL

Tot Ion: 43 Resp: 1262

Ion Ratio Lower Upper

43 100

58 18.9 25.0 37.6#

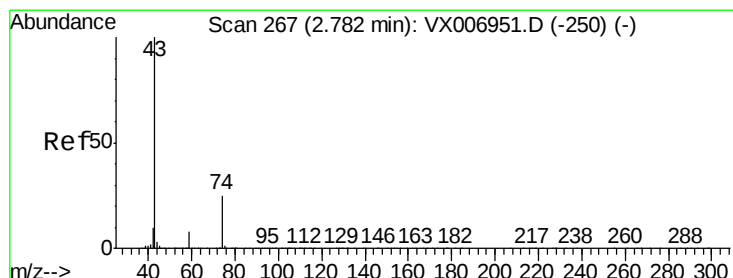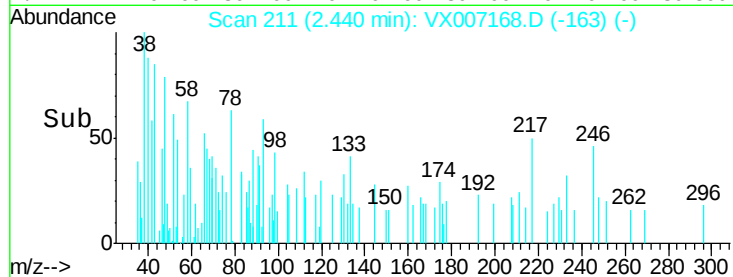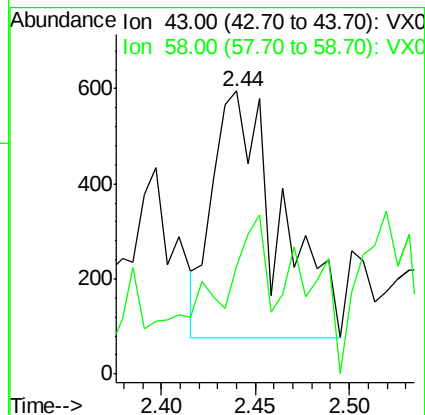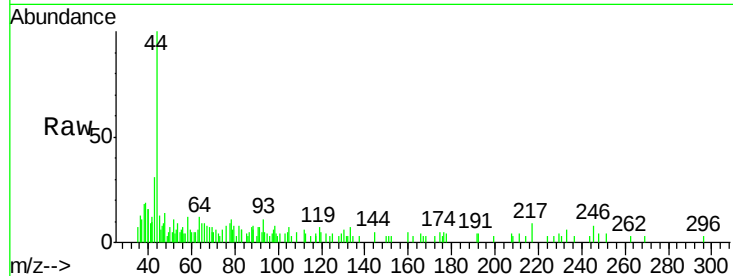

#18

Methyl Acetate

Concen: 0.233 ug/l

RT: 2.77 min Scan# 265

Delta R.T. -0.01 min

Lab File: VX007168.D




Acq: 21 Jan 2019 19:20


Tgt Ion: 43 Resp: 1976

Ion Ratio Lower Upper

43 100

74 26.7 18.6 28.0


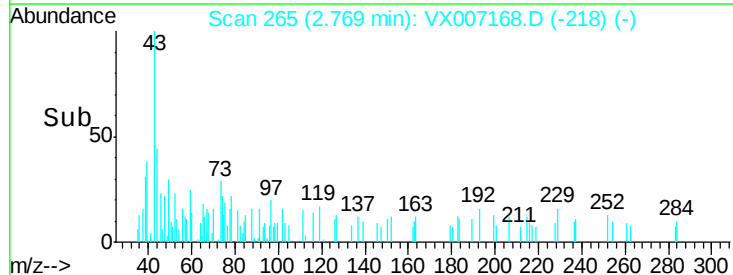
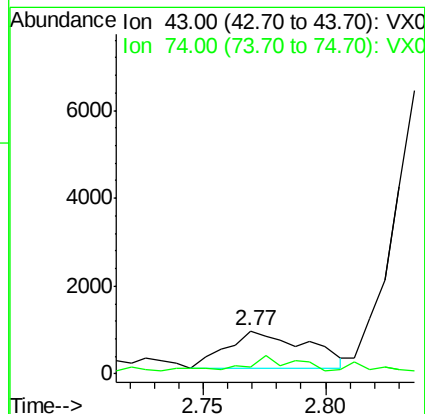
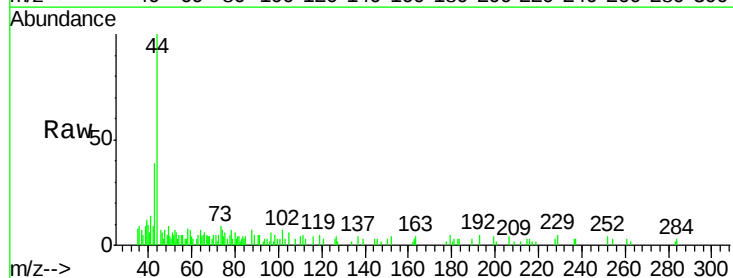




#20
Methvlene Chloride
Concen: Below Cal
RT: 2.86 min Scan# 280
Delta R.T. 0.00 min
Lab File: VX007168.D
Acq: 21 Jan 2019 19:20




Instrument :
MSVOA_X
ClientSampleId :
SS038MW013-190116DL


Tot Ion: 84 Resp: 1210
Ion Ratio Lower Upper
84 100
49 79.0 91.8 137.6#
51 51.7 28.5 42.7#
86 87.2 50.2 75.2#

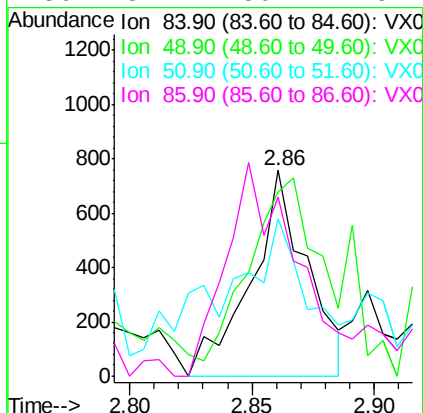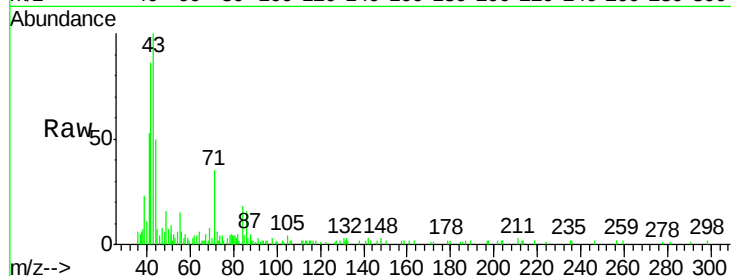

#29
Tetrahydrofuran
Concen: 0.274 ug/l
RT: 5.12 min Scan# 651
Delta R.T. -0.03 min
Lab File: VX007168.D
Acq: 21 Jan 2019 19:20

Tgt Ion: 42 Resp: 747
Ion Ratio Lower Upper
42 100
72 18.6 38.9 58.3#
71 0.0 36.2 54.4#

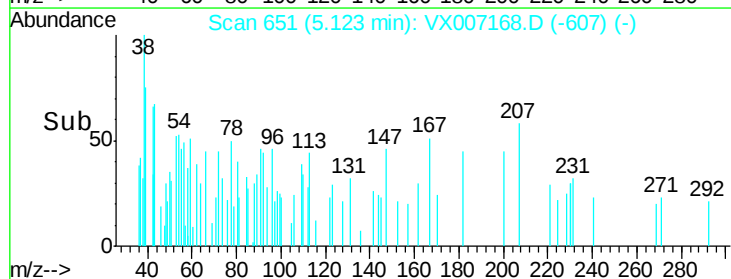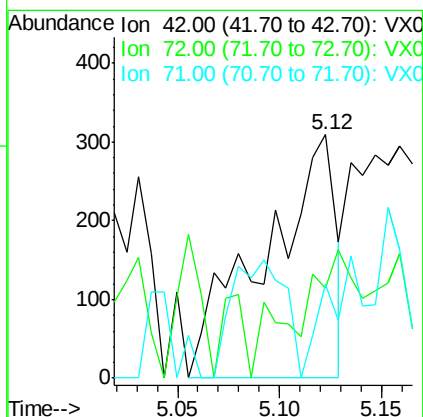



#33

1,2-Dichloroethane-d4

Concen: 51.442 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :


SS038MW013-190116DL

Tot Ion: 65 Resp: 304601

Ion Ratio Lower Upper




65 100

67 52.3 0.0 105.0

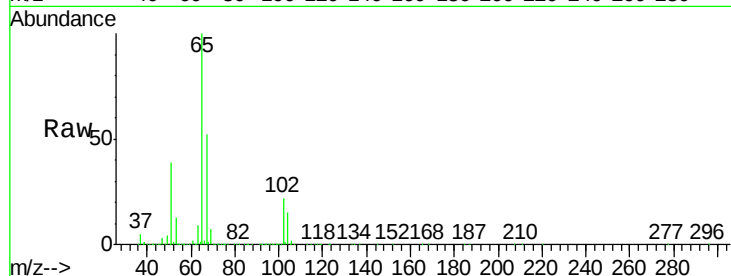

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

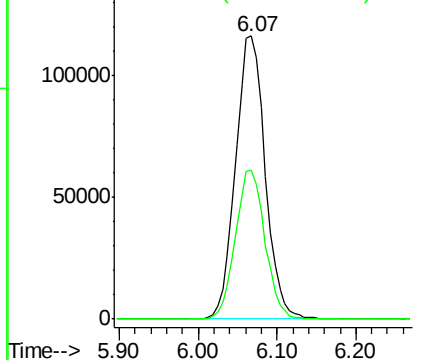

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20


Tgt Ion: 114 Resp: 875103

Ion Ratio Lower Upper

114 100

63 18.2 0.0 34.8



88 14.2 0.0 28.8




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

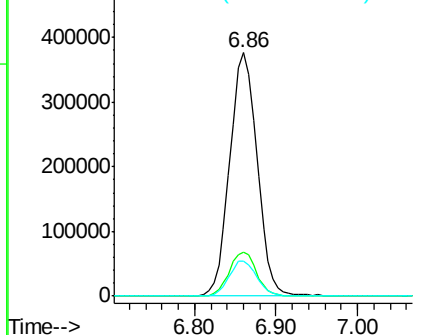



#35

Dibromofluoromethane

Concen: 48.393 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :

SS038MW013-190116DL


Tot Ion:113 Resp: 271202

Ion Ratio Lower Upper

113 100

111 103.2 81.6 122.4




192 22.0 16.7 25.1

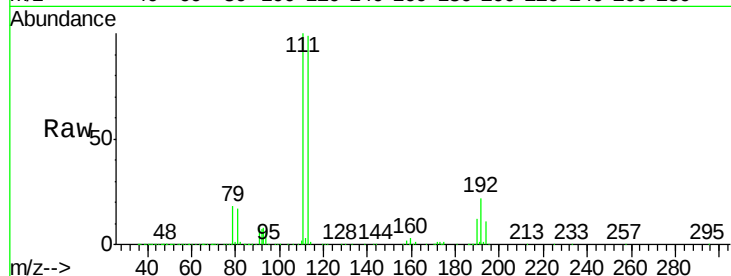

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

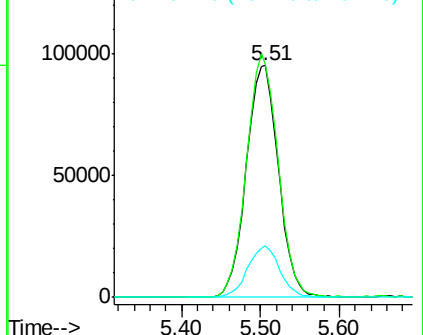

#36

1,1-Dichloropropene

Concen: 4.595 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20


Tgt Ion: 75 Resp: 34963

Ion Ratio Lower Upper

75 100

110 11.3 20.2 60.5#



77 0.0 24.8 37.2#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

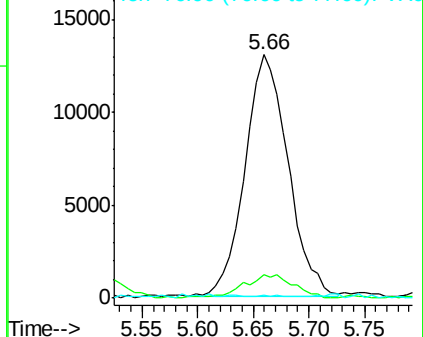



#38

Carbon Tetrachloride

Concen: 6.691 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.12 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :

SS038MW013-190116DL


Tot Ion:117 Resp: 51217

Ion Ratio Lower Upper

117 100

119 5.8 79.4 119.2#




121 0.0 24.0 36.0#

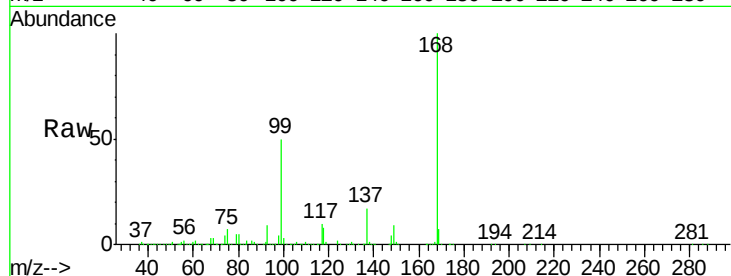

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

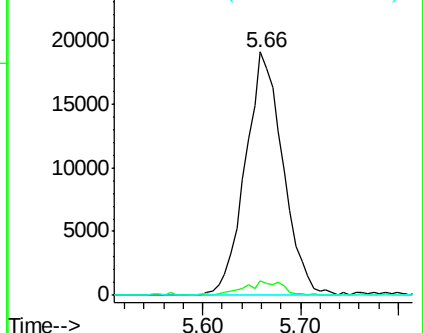

#39

Methylcyclohexane

Concen: 0.257 ug/l

RT: 7.46 min Scan# 1034

Delta R.T. -0.01 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20


Tgt Ion: 83 Resp: 2489

Ion Ratio Lower Upper

83 100

55 60.8 54.9 82.3



98 40.4 37.9 56.9




Abundance Ion 83.00 (82.70 to 83.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 98.00 (97.70 to 98.70): VX0

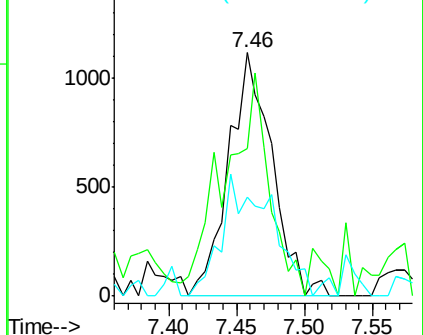



#40

Benzene

Concen: 0.637 ug/l

RT: 6.15 min Scan# 819

Delta R.T. 0.01 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :


SS038MW013-190116DL

Tot Ion: 78 Resp: 14798

Ion Ratio Lower Upper




78 100

77 21.9 19.2 28.8

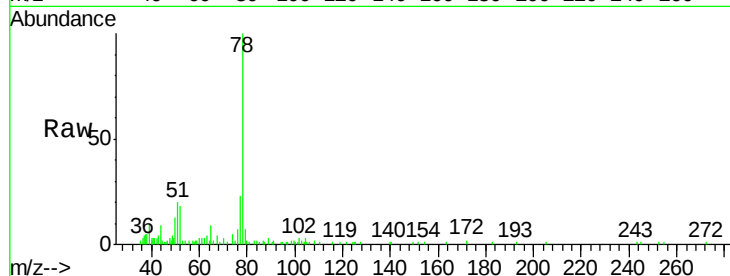

Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0

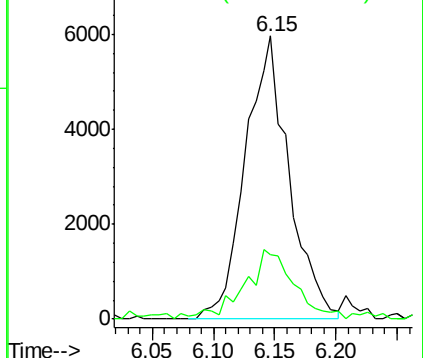

#49

1,4-Dioxane

Concen: Below Cal

RT: 7.71 min Scan# 1076

Delta R.T. -0.04 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20


Tgt Ion: 88 Resp: 225

Ion Ratio Lower Upper

88 100

43 82.7 22.2 33.4#



58 73.3 51.0 76.4




Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

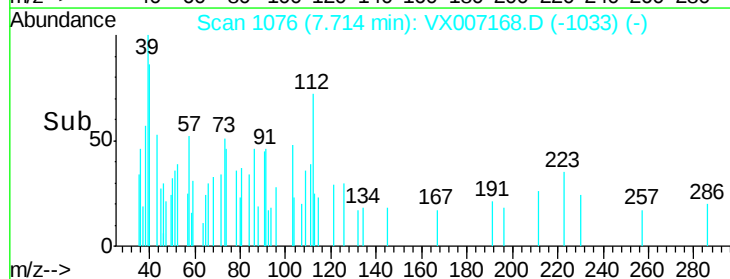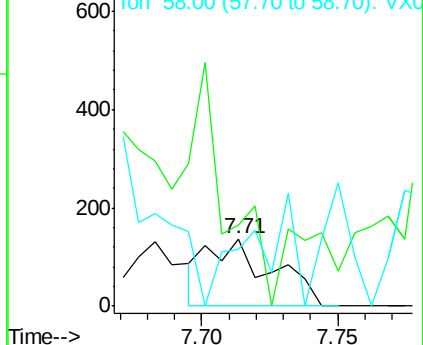



#50

Toluene-d8

Concen: 51.445 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :





SS038MW013-190116DL

Tot Ion: 98 Resp: 1055287

Ion Ratio Lower Upper

98 100

100 64.1 52.0 78.0

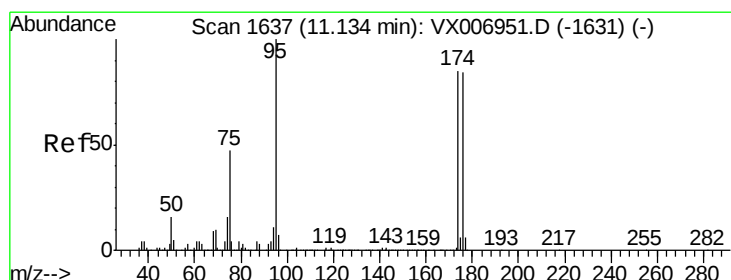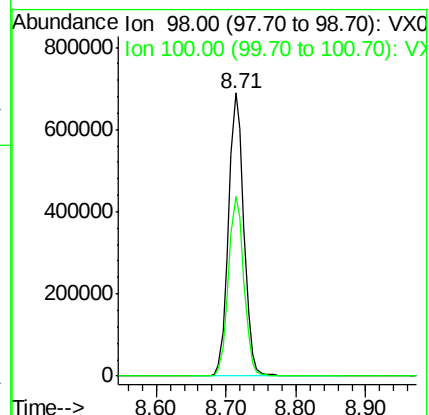

#62

4-Bromofluorobenzene

Concen: 54.007 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20




Tgt Ion: 95 Resp: 386214


Ion Ratio Lower Upper

95 100

174 92.1 0.0 182.2

176 91.6 0.0 178.8



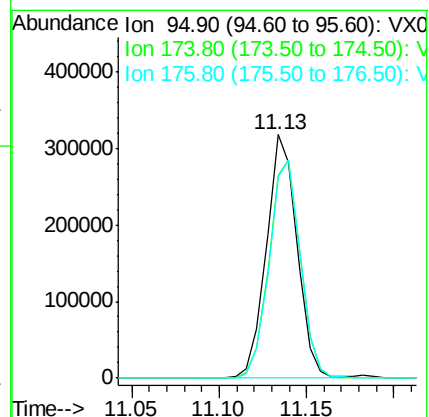





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.01 min
Lab File: VX007168.D
Acq: 21 Jan 2019 19:20




Instrument :
MSVOA_X
ClientSampleId :
SS038MW013-190116DL


Tot Ion:117 Resp: 833056
Ion Ratio Lower Upper
117 100
82 51.0 41.0 61.6
119 31.9 25.4 38.0

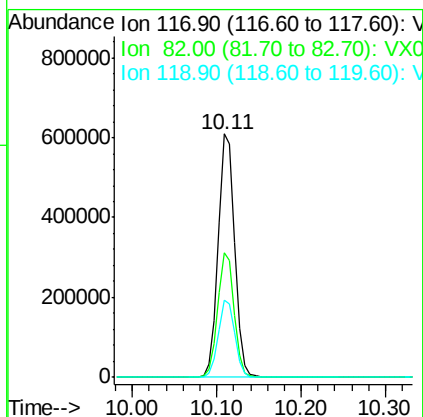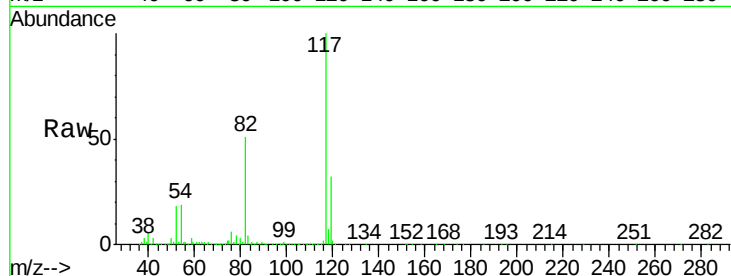

#65
Chlorobenzene
Concen: 30.260 ug/l
RT: 10.13 min Scan# 1473
Delta R.T. -0.01 min
Lab File: VX007168.D
Acq: 21 Jan 2019 19:20

Tgt Ion:112 Resp: 549813
Ion Ratio Lower Upper
112 100
114 33.2 25.7 38.5

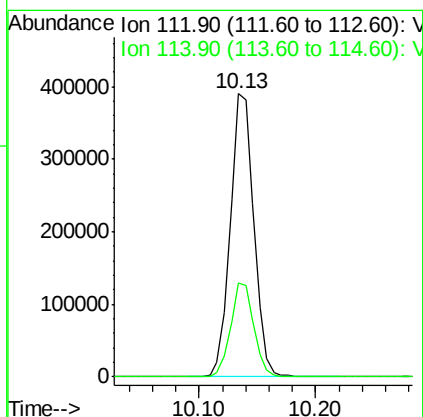

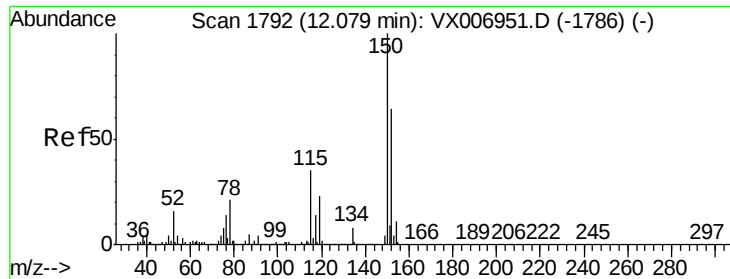

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :

SS038MW013-190116DL


Tot Ion:152 Resp: 426774

Ion Ratio Lower Upper

152 100

115 55.2 39.1 117.2




150 156.8 0.0 344.8

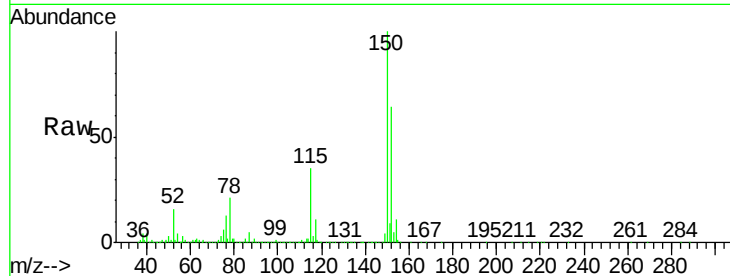

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

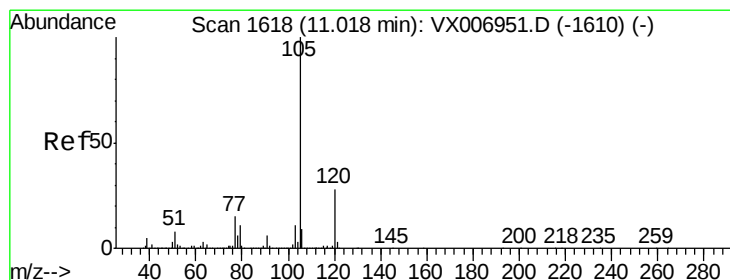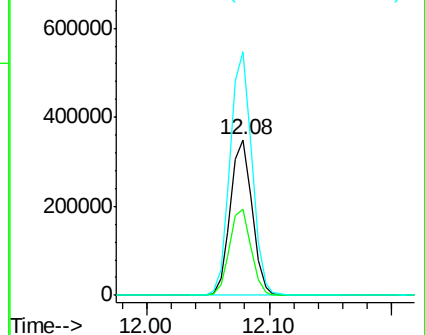

#73

Isopropylbenzene

Concen: 1.082 ug/l

RT: 11.02 min Scan# 1618

Delta R.T. -0.00 min

Lab File: VX007168.D


Acq: 21 Jan 2019 19:20

Tgt Ion:105 Resp: 32561

Ion Ratio Lower Upper



105 100


120 28.3 14.1 42.4



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

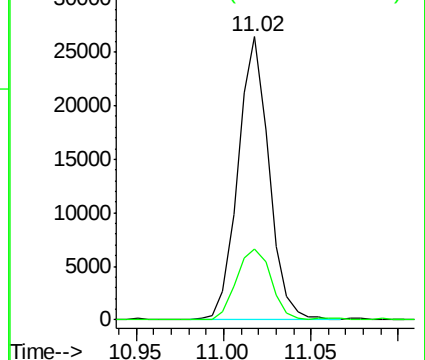

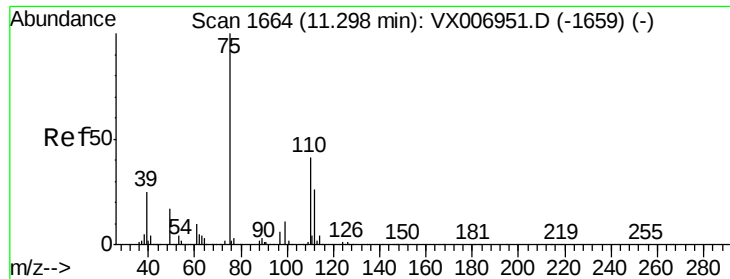

#76

1,2,3-Trichloropropane

Concen: 21.756 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :


SS038MW013-190116DL

Tot Ion: 75 Resp: 188156

Ion Ratio Lower Upper




75 100

77 1.5 18.5 55.5#

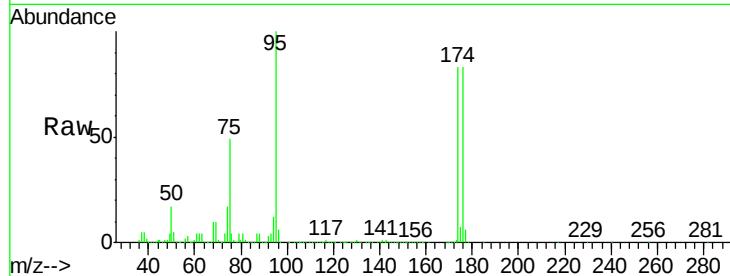

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

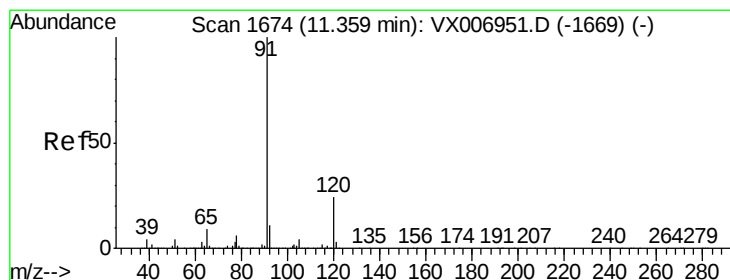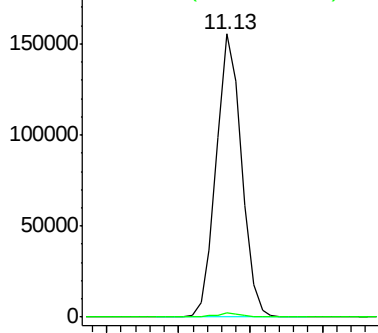

#78

n-propylbenzene

Concen: 0.793 ug/l

RT: 11.36 min Scan# 1674

Delta R.T. -0.00 min

Lab File: VX007168.D


Acq: 21 Jan 2019 19:20

Tgt Ion: 91 Resp: 26189

Ion Ratio Lower Upper



91 100


120 25.0 12.7 38.0



Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 120.00 (119.70 to 120.70): V

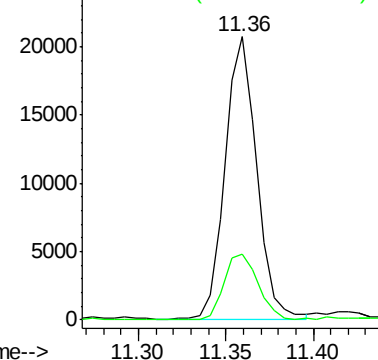



#79

2-Chlorotoluene

Concen: 1.317 ug/l

RT: 11.36 min Scan# 1674

Delta R.T. -0.06 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :


SS038MW013-190116DL

Tot Ion: 91 Resp: 26189

Ion Ratio Lower Upper




91 100

126 0.3 18.6 56.0#



Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 125.90 (125.60 to 126.60): V

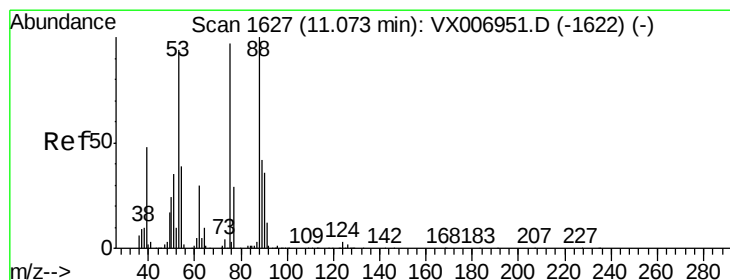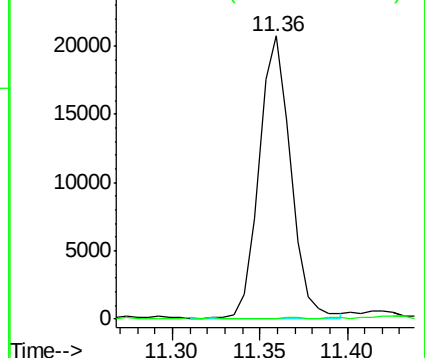

#81

trans-1,4-Dichloro-2-butene

Concen: 64.473 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20


Tgt Ion: 75 Resp: 188156

Ion Ratio Lower Upper

75 100

53 0.2 79.7 119.5#



89 0.2 38.0 57.0#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0



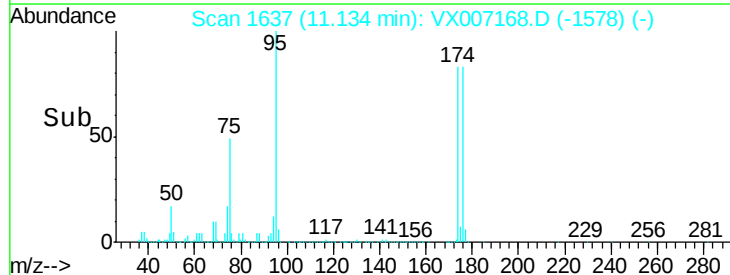
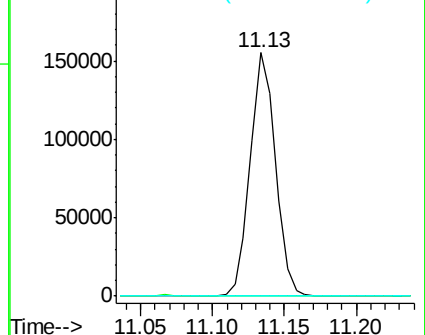


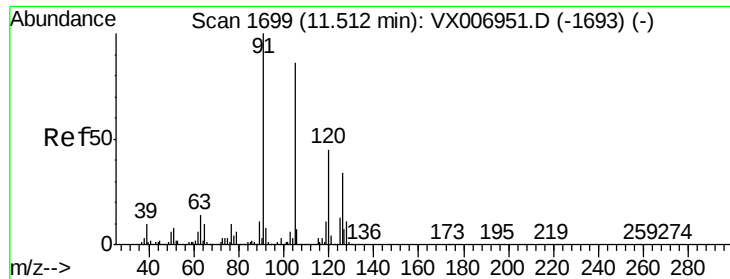

#82
4-Chlorotoluene
Concen: 1.137 ug/l
RT: 11.36 min Scan# 1674
Delta R.T. -0.15 min
Lab File: VX007168.D
Acq: 21 Jan 2019 19:20




Instrument :
MSVOA_X
ClientSampleId :
SS038MW013-190116DL


Tot Ion: 91 Resp: 26189
Ion Ratio Lower Upper
91 100
126 0.3 16.3 48.9#

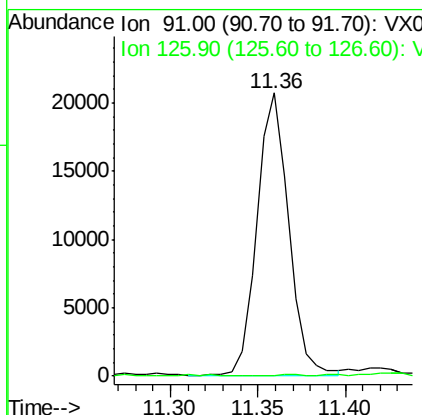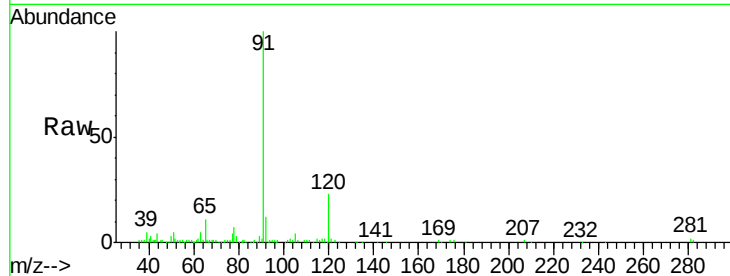

#83
tert-Butylbenzene
Concen: 1.118 ug/l
RT: 11.77 min Scan# 1741
Delta R.T. -0.00 min
Lab File: VX007168.D
Acq: 21 Jan 2019 19:20

Tgt Ion: 119 Resp: 28042
Ion Ratio Lower Upper
119 100
91 67.4 27.7 83.1
134 26.7 11.9 35.5

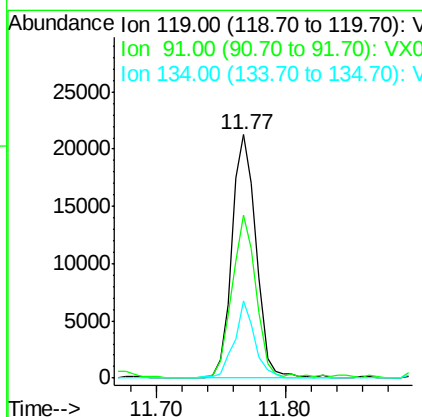

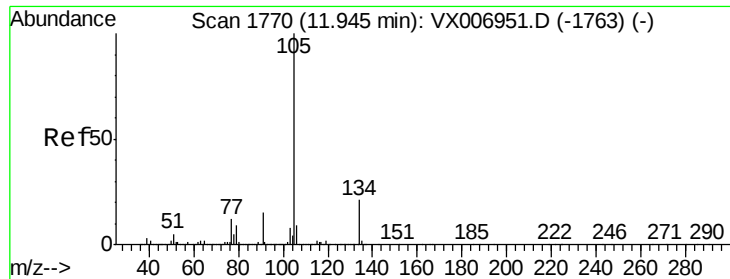

#85

sec-Butylbenzene

Concen: 1.701 ug/l

RT: 11.94 min Scan# 1770

Delta R.T. -0.00 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :


SS038MW013-190116DL

Tot Ion:105 Resp: 50980

Ion Ratio Lower Upper




105 100

134 21.0 10.7 31.9

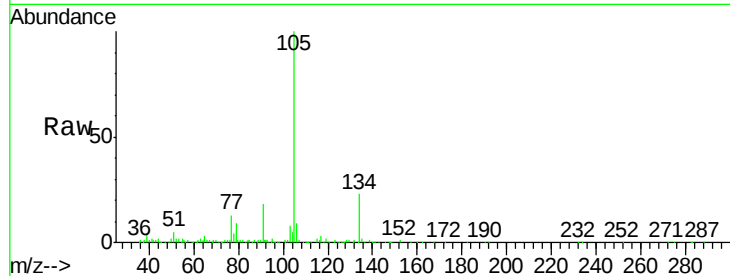

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 134.00 (133.70 to 134.70): V

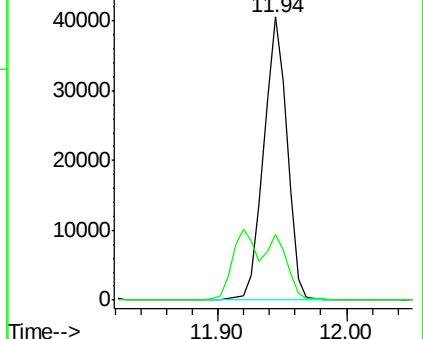

#86

p-Isopropyltoluene

Concen: 4.831 ug/l

RT: 12.23 min Scan# 1817

Delta R.T. 0.17 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20


Tgt Ion:119 Resp: 129462

Ion Ratio Lower Upper

119 100

134 29.0 14.0 41.9



91 24.7 11.3 33.9




Abundance Ion 119.00 (118.70 to 119.70): V

Ion 134.00 (133.70 to 134.70): V

Ion 91.00 (90.70 to 91.70): V

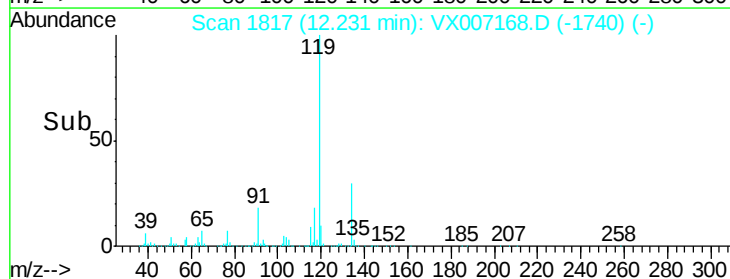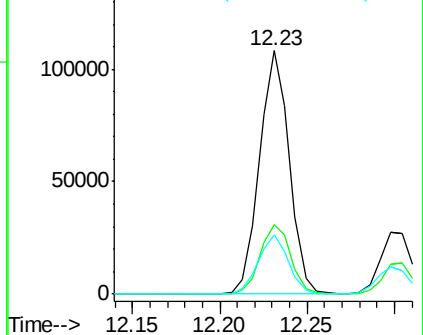



#88

1,4-Dichlorobenzene

Concen: 0.377 ug/l

RT: 12.10 min Scan# 1795

Delta R.T. -0.00 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :

SS038MW013-190116DL


Tot Ion:146 Resp: 3300

Ion Ratio Lower Upper

146 100

111 206.1 18.1 54.1#




148 111.7 31.9 95.9#

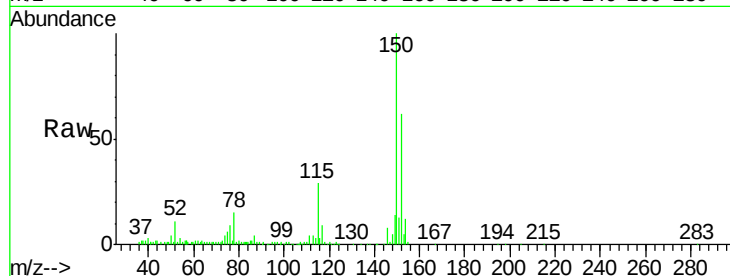

Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V

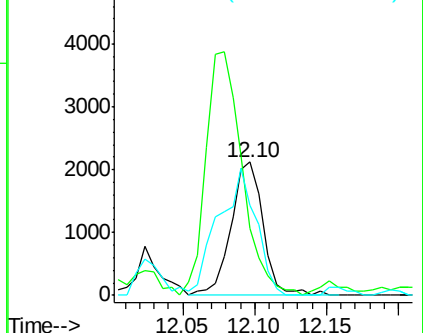

#89

n-Butylbenzene

Concen: 0.273 ug/l

RT: 12.39 min Scan# 1843

Delta R.T. -0.00 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20


Tgt Ion: 91 Resp: 6232

Ion Ratio Lower Upper

91 100

92 33.6 26.8 80.4



134 0.0 14.4 43.2#




Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 92.00 (91.70 to 92.70): VX0

Ion 134.00 (133.70 to 134.70): V

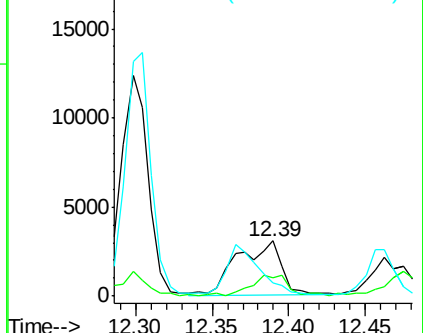

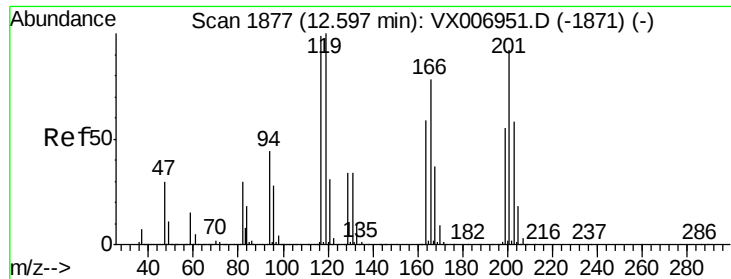

#90

Hexachloroethane

Concen: 15.824 ug/l

RT: 12.70 min Scan# 1894

Delta R.T. 0.10 min

Lab File: VX007168.D

Acq: 21 Jan 2019 19:20

Instrument :

MSVOA_X

ClientSampleId :

SS038MW013-190116DL

Tot Ion:117 Resp: 58671

Ion Ratio Lower Upper

117 100

201 0.1 42.9 128.7#

