

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012119\
 Data File : VX007161.D
 Acq On : 21 Jan 2019 16:15
 Operator : JC/SP
 Sample : K1198-09
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP01-20190115

Quant Time: Jan 25 03:39:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 08 14:06:59 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	552981	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	858125	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	808543	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	404362	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	296769	51.35	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.70%	
35) Dibromofluoromethane	5.50	113	262877	47.84	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.68%	
50) Toluene-d8	8.71	98	1028827	51.15	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.30%	
62) 4-Bromofluorobenzene	11.13	95	373559	53.27	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.54%	
Target Compounds						
52) Toluene	8.79	92	5362	0.366	ug/l	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012119\
Data File : VX007161.D
Acq On : 21 Jan 2019 16:15
Operator : JC/SP
Sample : K1198-09
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP01-20190115

Quant Time: Jan 25 03:39:23 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 08 14:06:59 2019
Response via : Initial Calibration

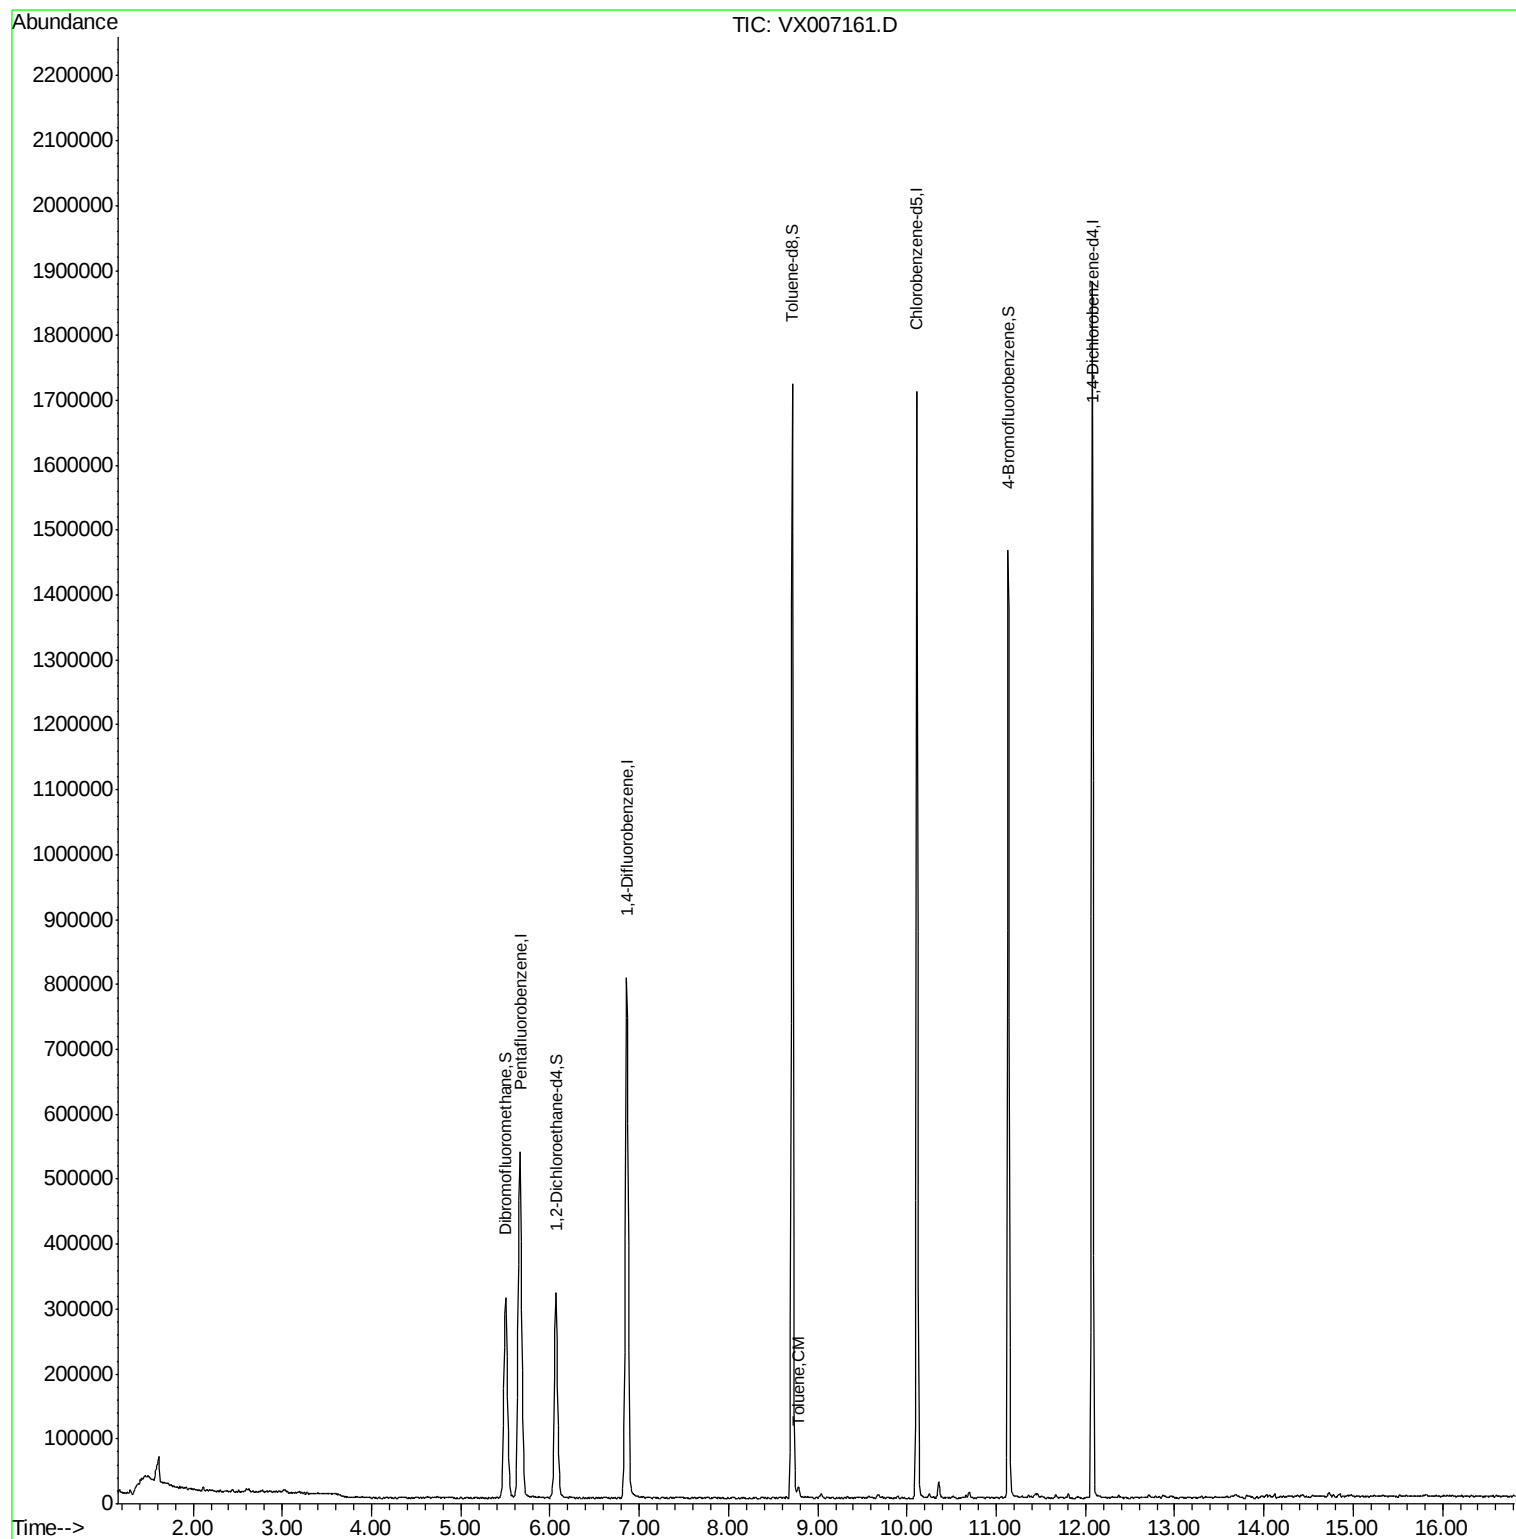

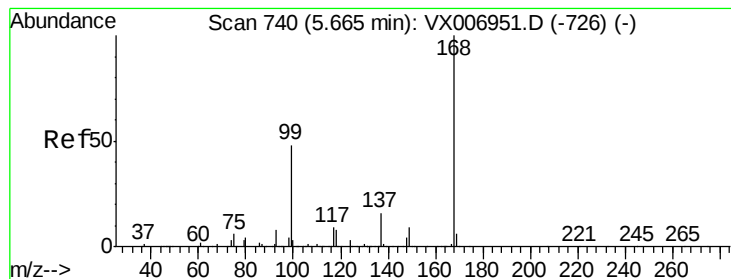

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.01 min

Lab File: VX007161.D

Acq: 21 Jan 2019 16:15

Instrument :

MSVOA_X

ClientSampleId :


DUP01-20190115

Tot Ion:168 Resp: 552981

Ion Ratio Lower Upper

168 100

99 48.1 41.8 62.8

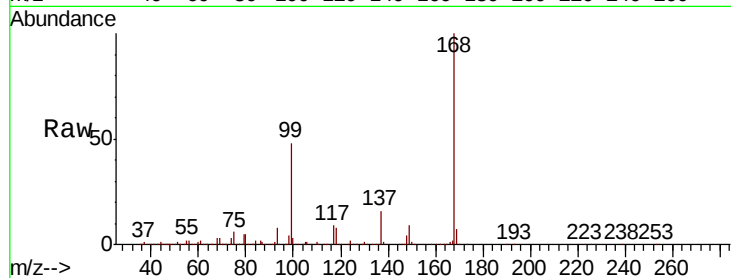

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

200000



150000

100000

50000

0

Time--> 5.50 5.60 5.70 5.80

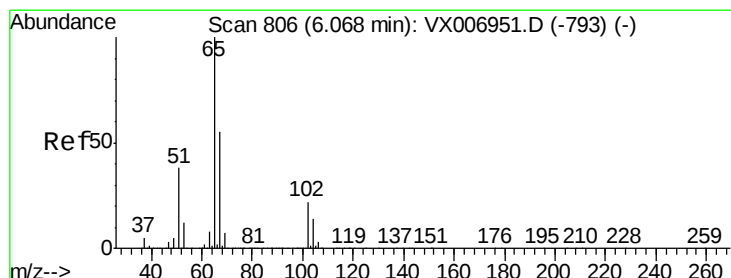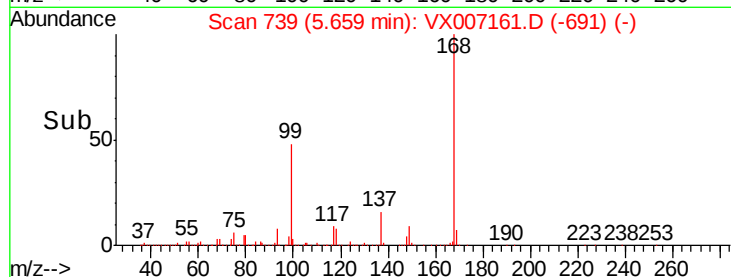

#33

1,2-Dichloroethane-d4

Concen: 51.352 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.01 min

Lab File: VX007161.D


Acq: 21 Jan 2019 16:15

Tgt Ion: 65 Resp: 296769

Ion Ratio Lower Upper

65 100

67 53.5 0.0 105.0

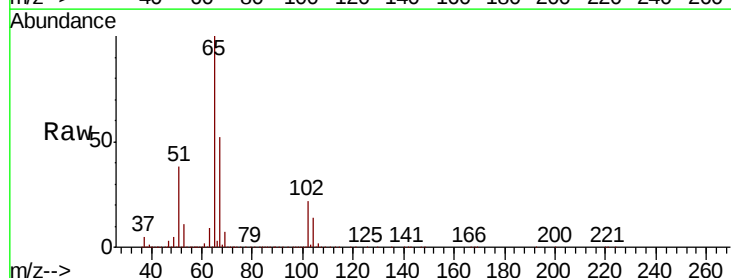

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.06

120000

100000

80000


60000


40000

20000

0

Time--> 5.90 6.00 6.10 6.20

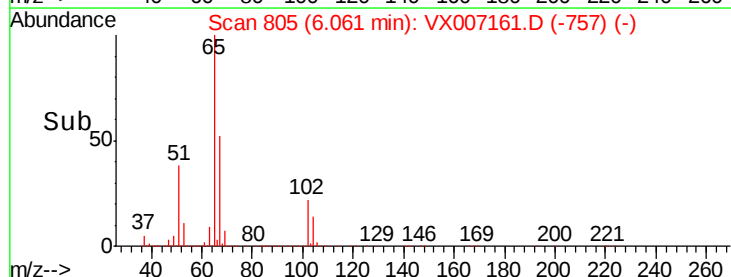

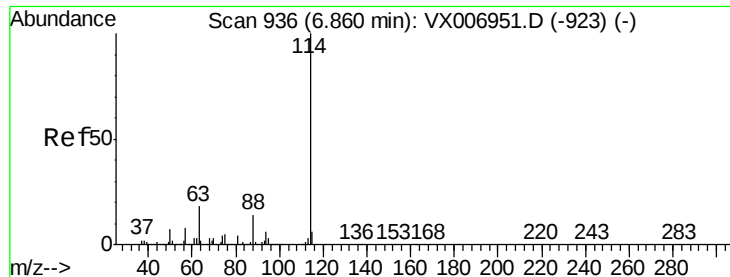

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX007161.D

Acq: 21 Jan 2019 16:15

Instrument :

MSVOA_X

ClientSampleId :

DUP01-20190115


Tot Ion:114 Resp: 858125

Ion Ratio Lower Upper

114 100

63 18.4 0.0 34.8




88 15.6 0.0 28.8

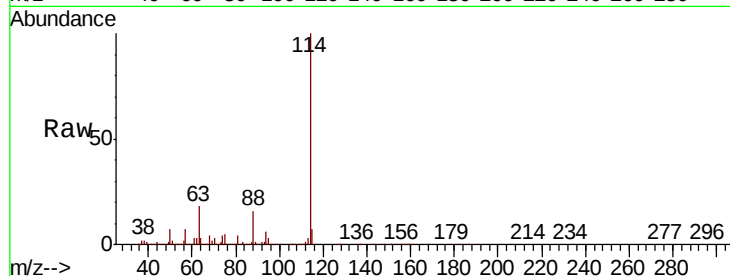

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

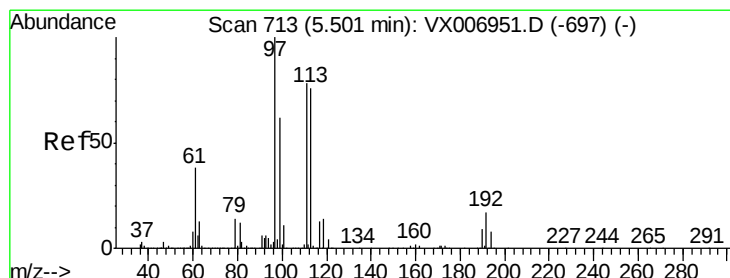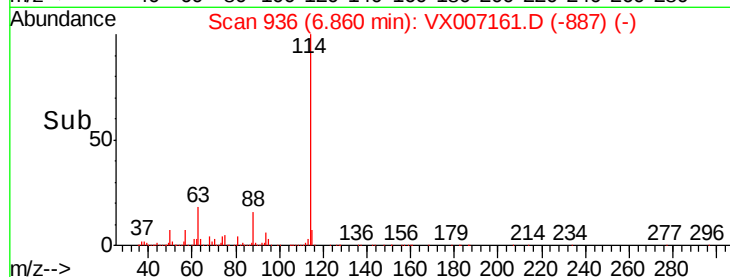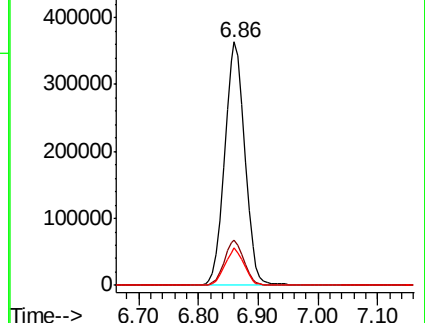

#35

Dibromofluoromethane

Concen: 47.836 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX007161.D

Acq: 21 Jan 2019 16:15


Tgt Ion:113 Resp: 262877

Ion Ratio Lower Upper

113 100

111 102.1 81.6 122.4



192 22.6 16.7 25.1

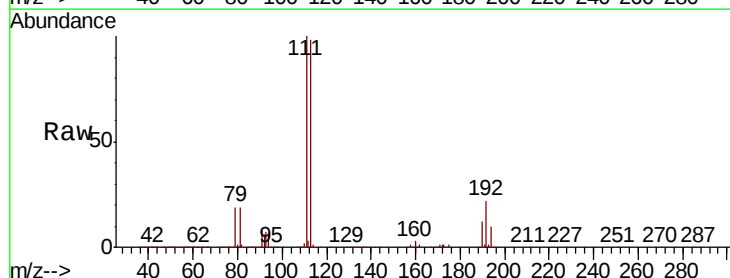


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

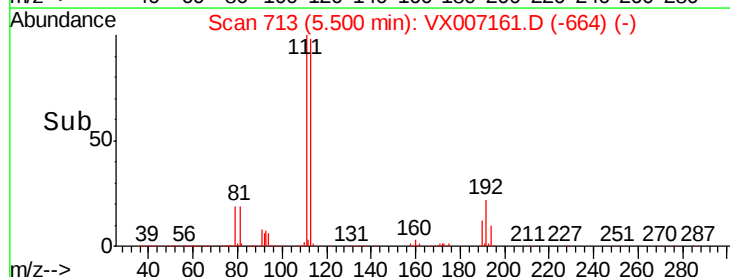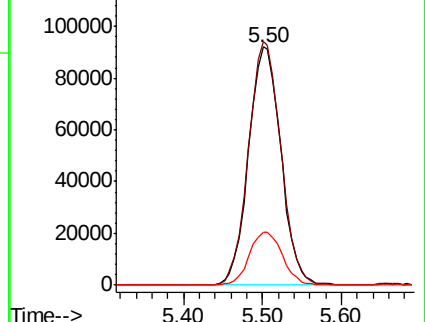

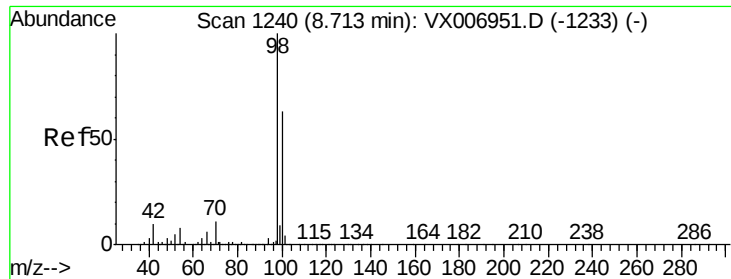

#50

Toluene-d8

Concen: 51.148 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX007161.D

Acq: 21 Jan 2019 16:15

Instrument :

MSVOA_X

ClientSampleId :





DUP01-20190115

Tot Ion: 98 Resp: 1028827

Ion Ratio Lower Upper

98 100

100 63.4 52.0 78.0

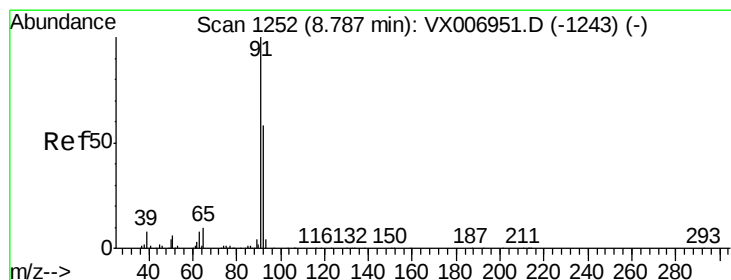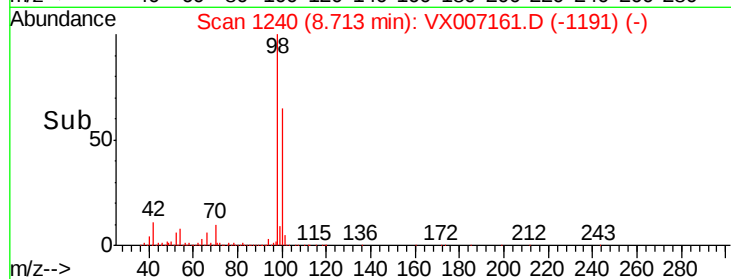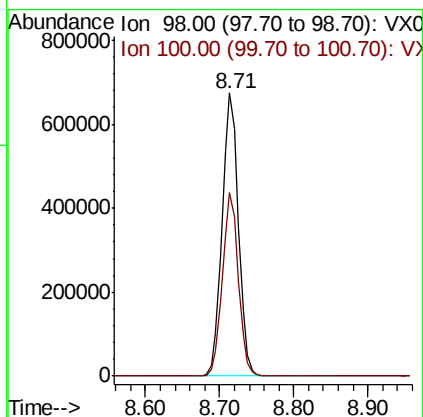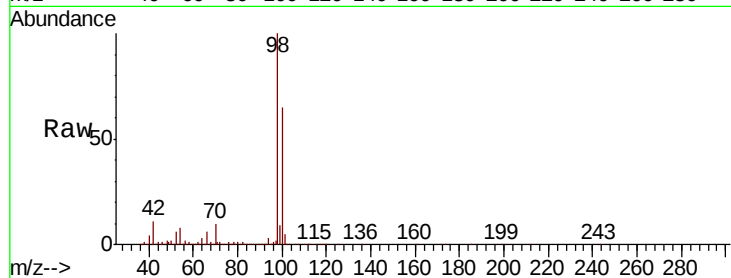

#52

Toluene

Concen: 0.366 ug/l

RT: 8.79 min Scan# 1252

Delta R.T. -0.00 min

Lab File: VX007161.D




Acq: 21 Jan 2019 16:15


Tgt Ion: 92 Resp: 5362

Ion Ratio Lower Upper

92 100

91 186.3 137.6 206.4

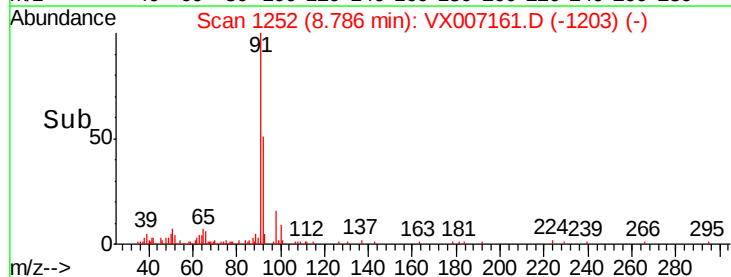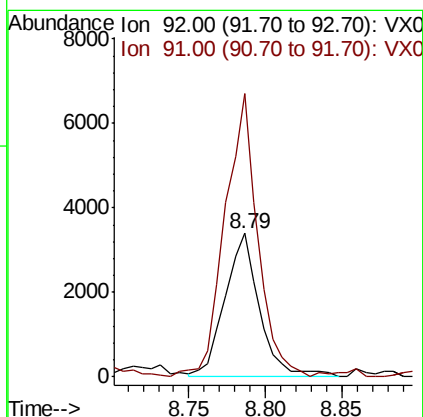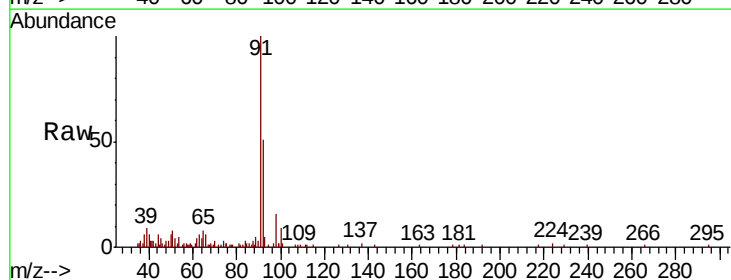

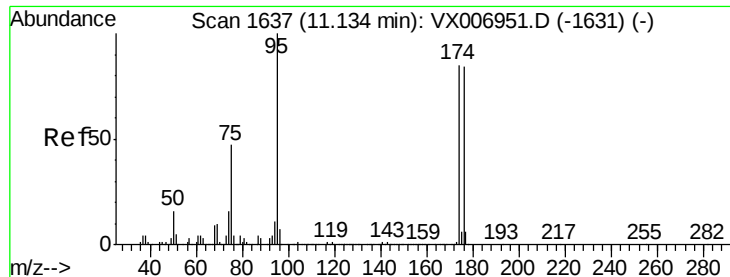

#62

4-Bromofluorobenzene

Concen: 53.270 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX007161.D

Acq: 21 Jan 2019 16:15

Instrument :

MSVOA_X

ClientSampleId :

DUP01-20190115


Tot Ion: 95 Resp: 373559

Ion Ratio Lower Upper

95 100

174 91.6 0.0 182.2




176 89.9 0.0 178.8

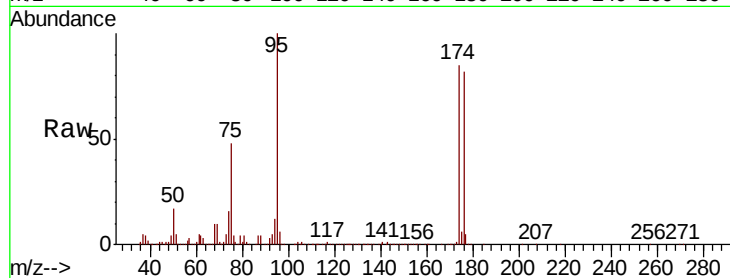

Abundance Ion 94.90 (94.60 to 95.60): VX006951.D (-1631) (-)

Ion 173.80 (173.50 to 174.50): VX006951.D (-1631) (-)

Ion 175.80 (175.50 to 176.50): VX006951.D (-1631) (-)

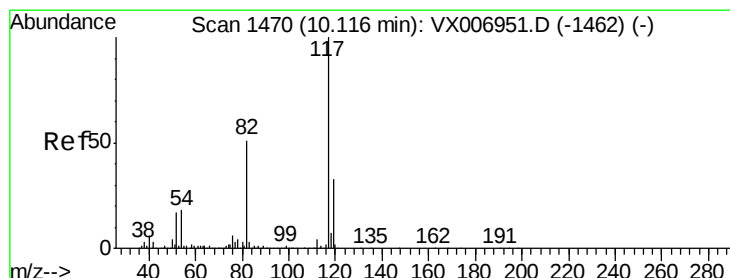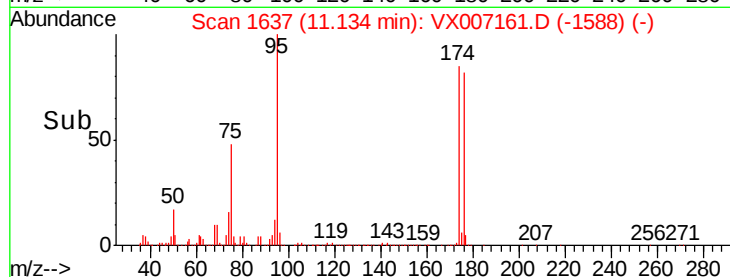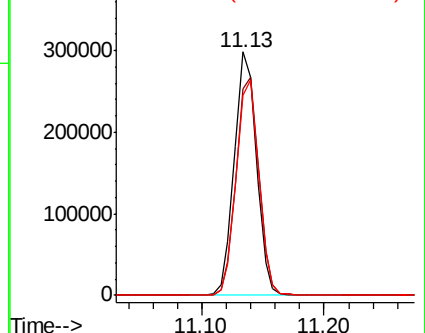

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.01 min

Lab File: VX007161.D

Acq: 21 Jan 2019 16:15


Tgt Ion: 117 Resp: 808543

Ion Ratio Lower Upper

117 100

82 51.8 41.0 61.6



119 32.7 25.4 38.0

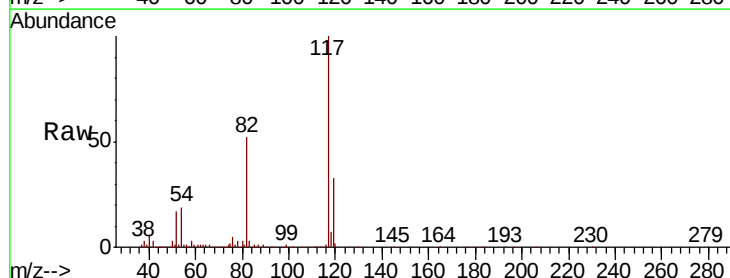


Abundance Ion 116.90 (116.60 to 117.60): VX006951.D (-1462) (-)

Ion 82.00 (81.70 to 82.70): VX006951.D (-1462) (-)

Ion 118.90 (118.60 to 119.60): VX006951.D (-1462) (-)

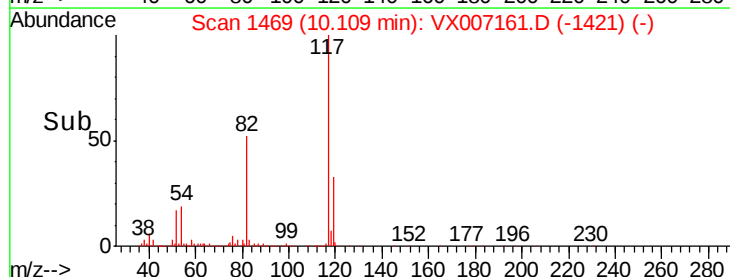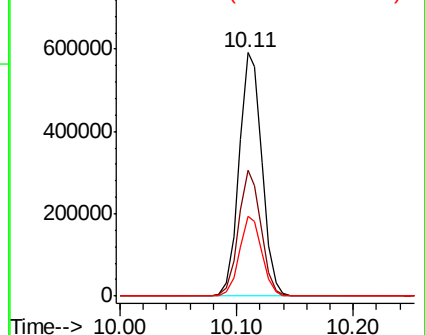

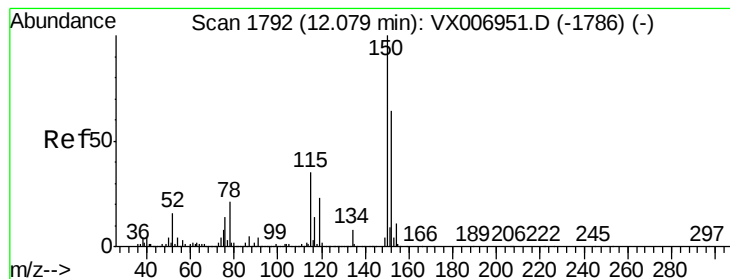

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX007161.D

Acq: 21 Jan 2019 16:15

Instrument :

MSVOA_X

ClientSampleId :

DUP01-20190115


Tot Ion:152 Resp: 404362

Ion Ratio Lower Upper

152 100

115 54.0 39.1 117.2

150 155.9 0.0 344.8

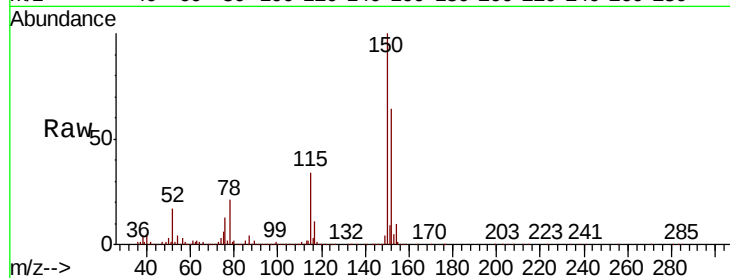

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

