

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012119\  
 Data File : VX007165.D  
 Acq On : 21 Jan 2019 18:01  
 Operator : JC/SP  
 Sample : K1199-21  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SA-TW528-4246

Quant Time: Jan 22 10:55:03 2019  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Jan 08 14:06:59 2019  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 5.67  | 168  | 527812   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 6.86  | 114  | 815386   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 10.11 | 117  | 779787   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 12.08 | 152  | 390655   | 50.00 | ug/l  | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|-------|------|----------|-------|---------|----------|
| 33) 1,2-Dichloroethane-d4   | 6.07  | 65   | 285967   | 51.84 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 103.68% |          |
| 35) Dibromofluoromethane    | 5.50  | 113  | 255903   | 49.01 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 98.02%  |          |
| 50) Toluene-d8              | 8.71  | 98   | 987581   | 51.67 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 103.34% |          |
| 62) 4-Bromofluorobenzene    | 11.13 | 95   | 359397   | 53.94 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 107.88% |          |


| Target Compounds | Qvalue |
|------------------|--------|
|------------------|--------|


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012119\  
Data File : VX007165.D  
Acq On : 21 Jan 2019 18:01  
Operator : JC/SP  
Sample : K1199-21  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW528-4246

Quant Time: Jan 22 10:55:03 2019  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260  
QLast Update : Tue Jan 08 14:06:59 2019  
Response via : Initial Calibration

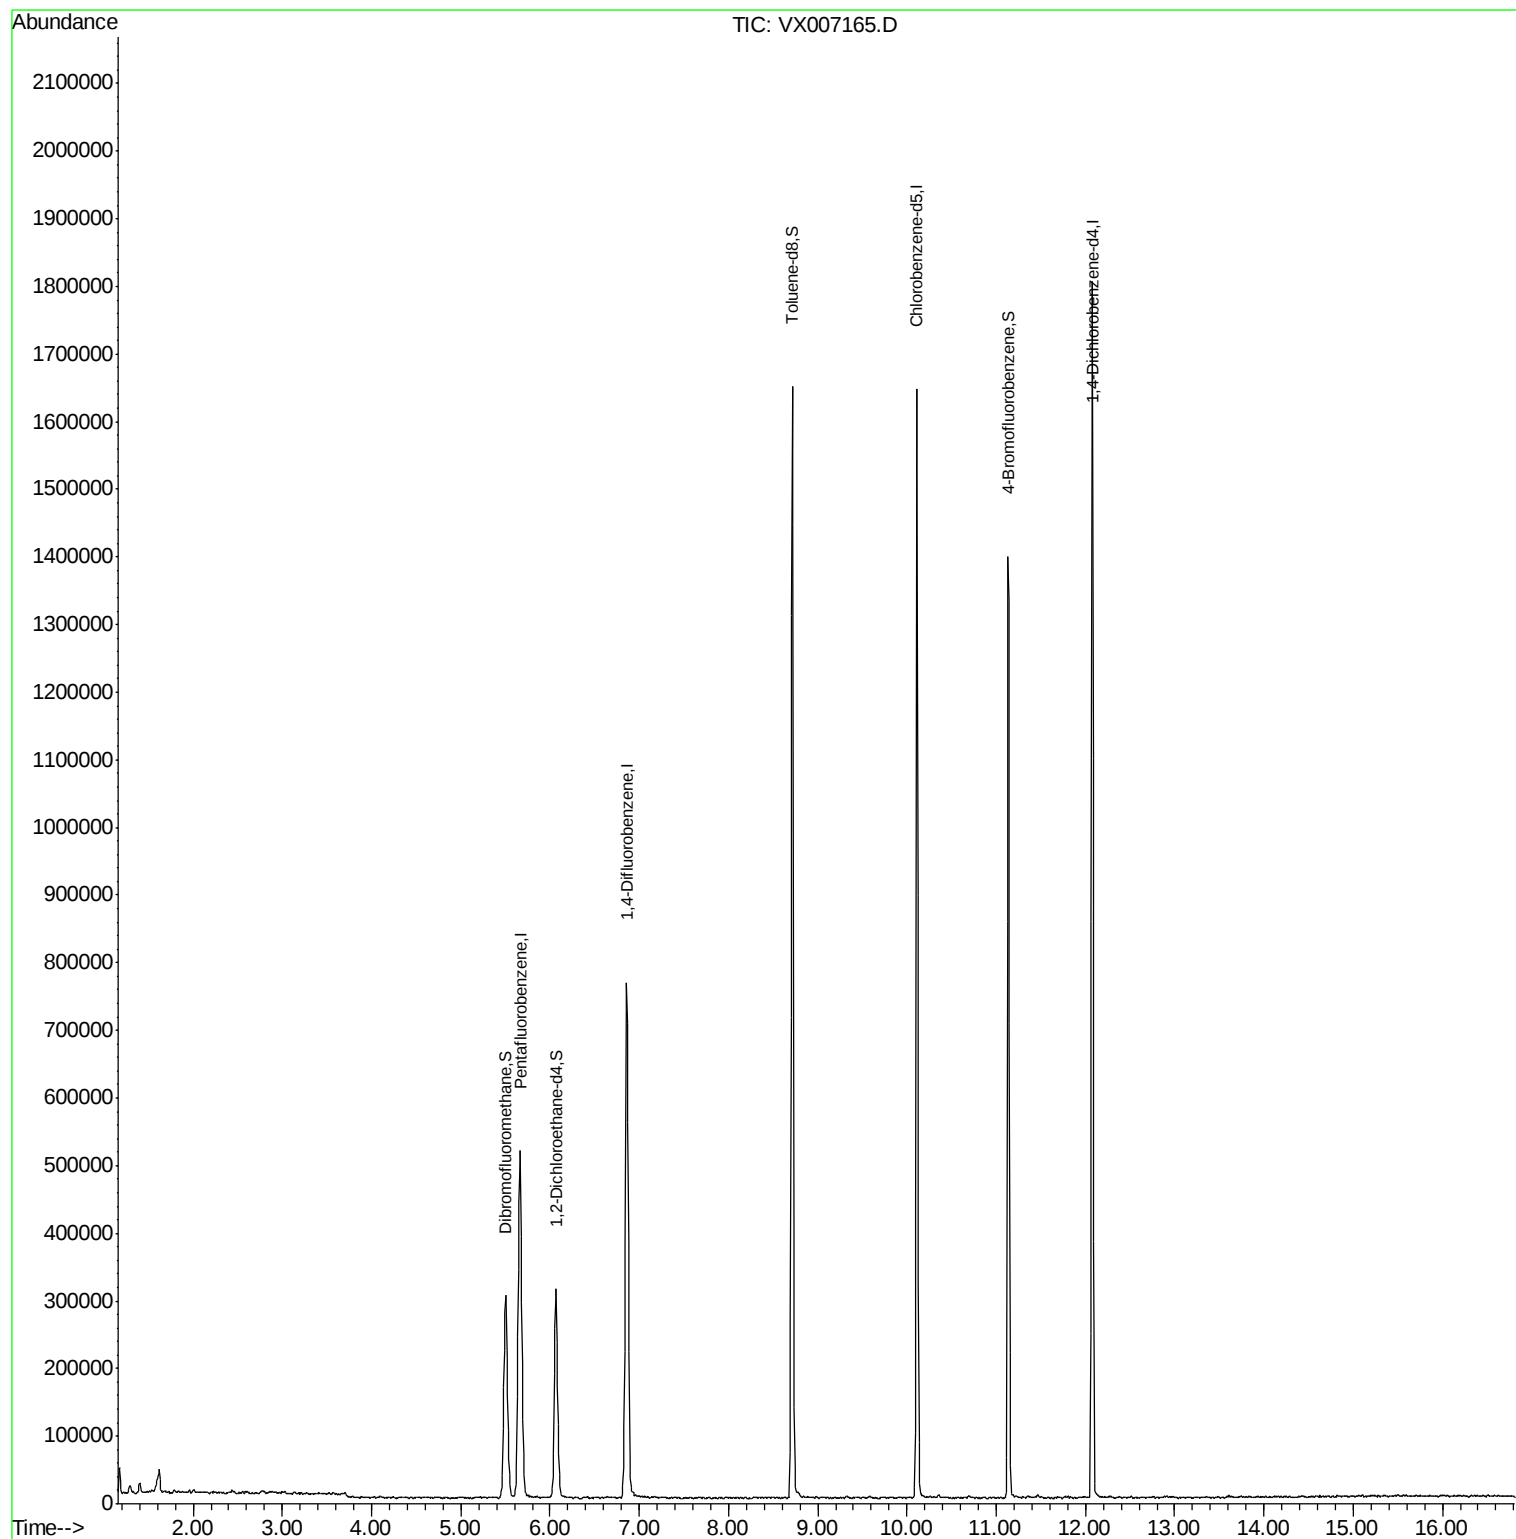

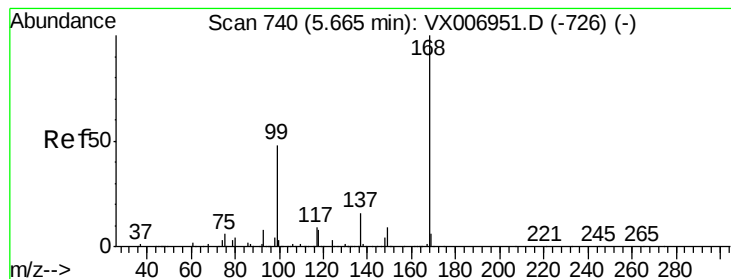

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX007165.D

Acq: 21 Jan 2019 18:01

Instrument :

MSVOA\_X

ClientSampleId :


SA-TW528-4246

Tot Ion:168 Resp: 527812

Ion Ratio Lower Upper

168 100

99 49.5 41.8 62.8

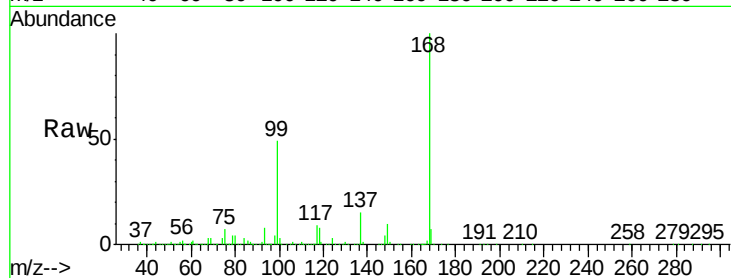

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

200000



150000

100000

50000

0

Time-->

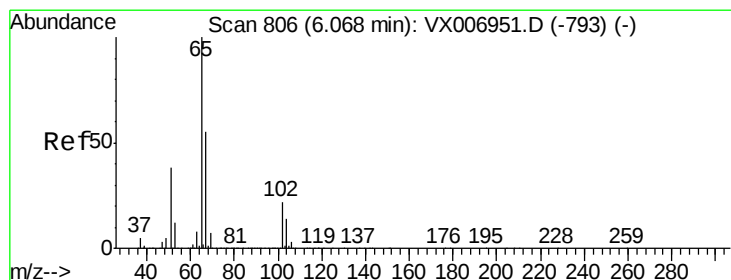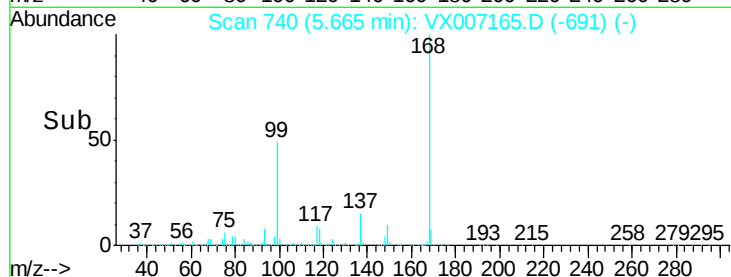

#33

1,2-Dichloroethane-d4

Concen: 51.842 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX007165.D


Acq: 21 Jan 2019 18:01

Tgt Ion: 65 Resp: 285967

Ion Ratio Lower Upper

65 100

67 53.4 0.0 105.0

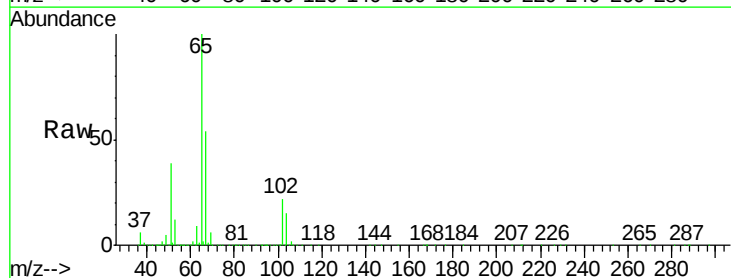

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

120000

100000

80000


60000


40000

20000

0

Time-->

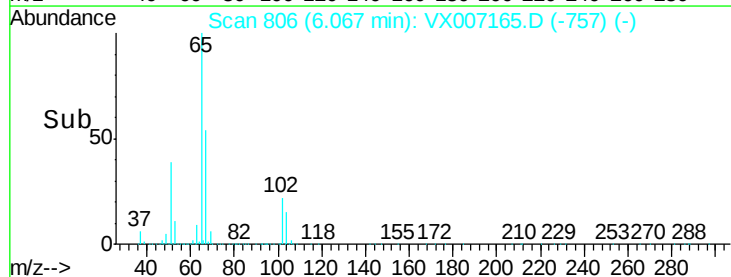

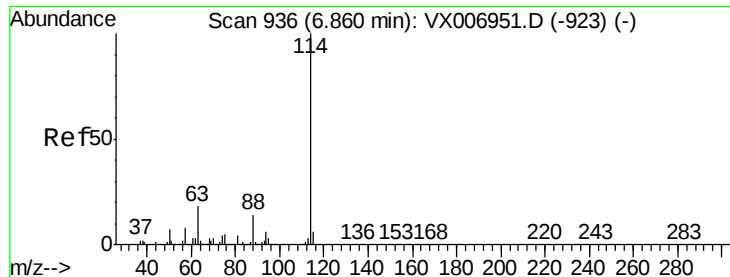

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX007165.D

Acq: 21 Jan 2019 18:01

Instrument :

MSVOA\_X

ClientSampleId :

SA-TW528-4246


Tot Ion:114 Resp: 815386

Ion Ratio Lower Upper

114 100

63 18.2 0.0 34.8




88 14.9 0.0 28.8

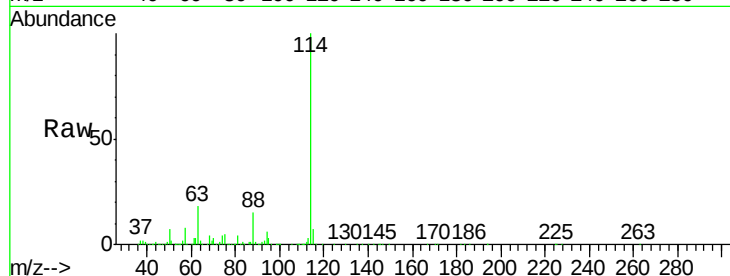

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

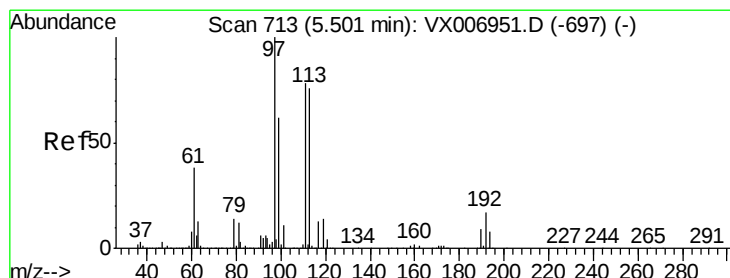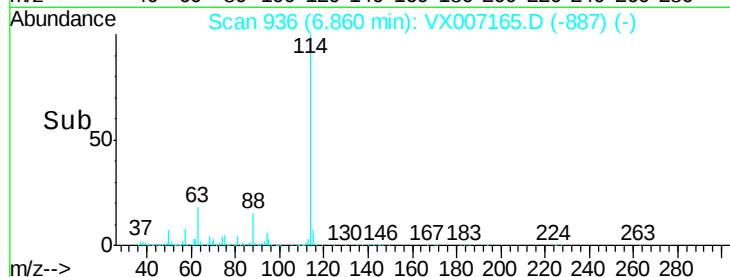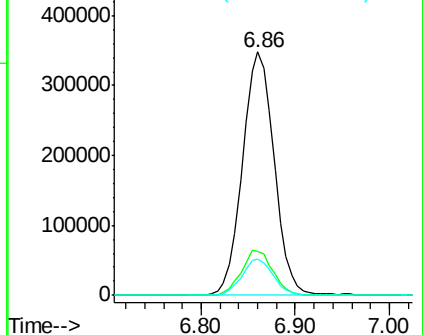

#35

Dibromofluoromethane

Concen: 49.008 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX007165.D

Acq: 21 Jan 2019 18:01


Tgt Ion:113 Resp: 255903

Ion Ratio Lower Upper

113 100

111 101.0 81.6 122.4



192 21.8 16.7 25.1

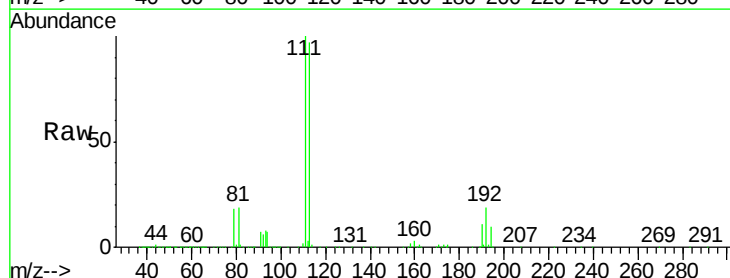


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

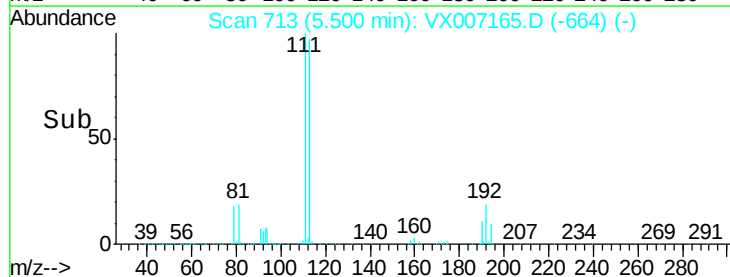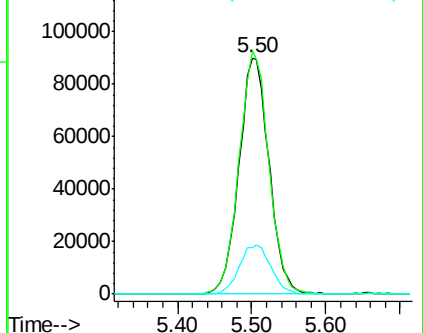

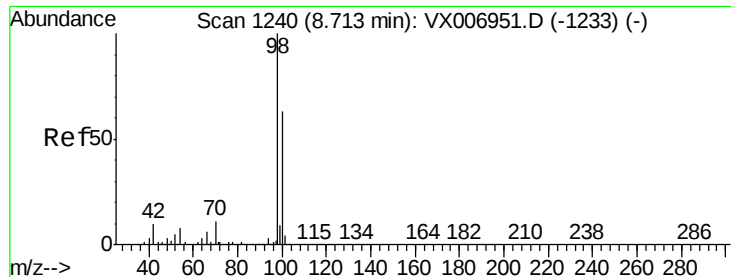

#50

Toluene-d8

Concen: 51.671 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX007165.D

Acq: 21 Jan 2019 18:01

Instrument :

MSVOA\_X

ClientSampleId :


SA-TW528-4246

Tot Ion: 98 Resp: 987581

Ion Ratio Lower Upper




98 100

100 64.6 52.0 78.0

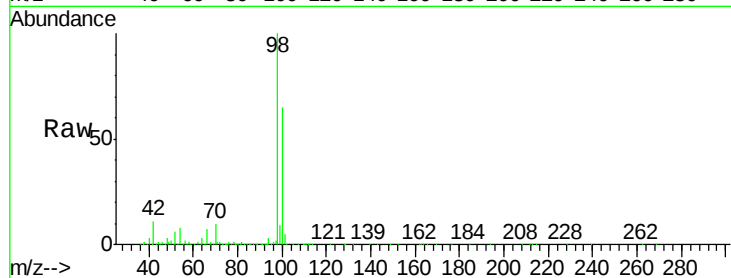

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

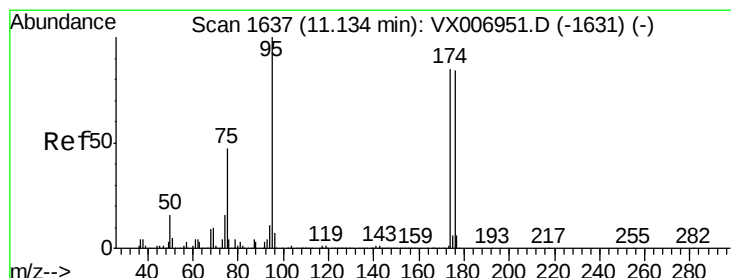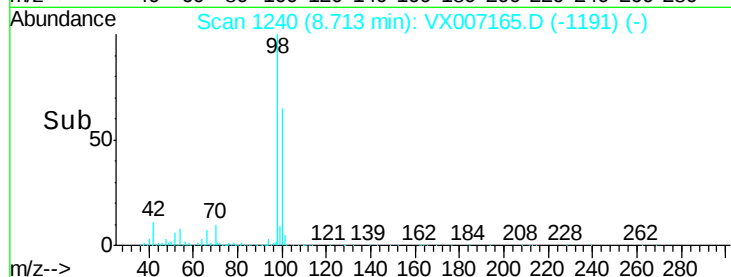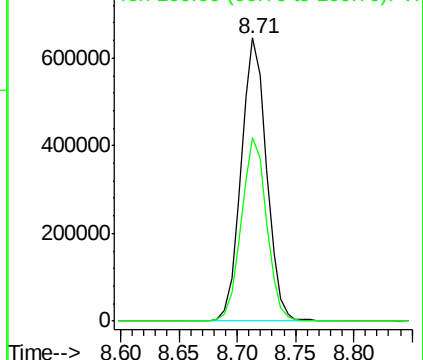

#62

4-Bromofluorobenzene

Concen: 53.937 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX007165.D

Acq: 21 Jan 2019 18:01


Tgt Ion: 95 Resp: 359397

Ion Ratio Lower Upper

95 100

174 91.7 0.0 182.2



176 89.7 0.0 178.8

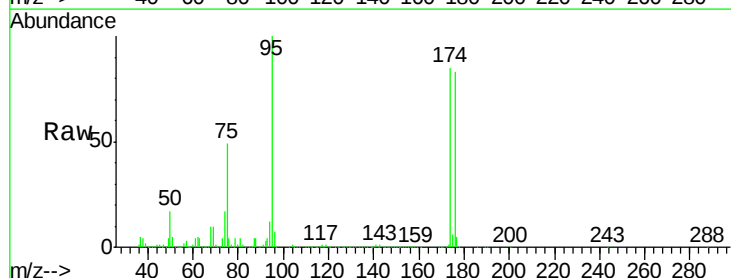


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

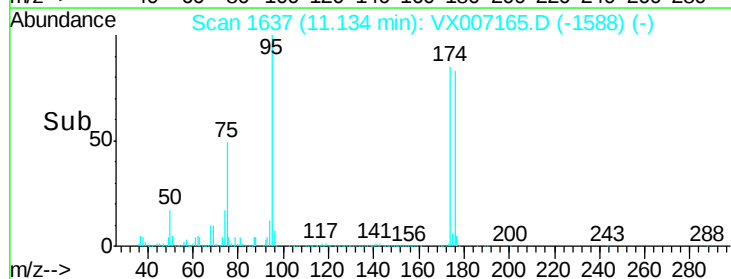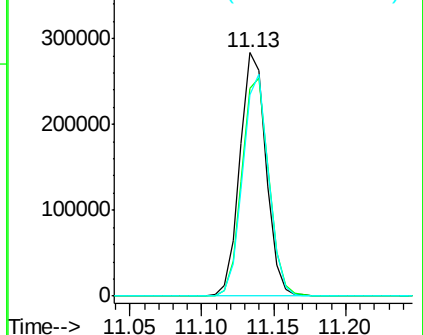

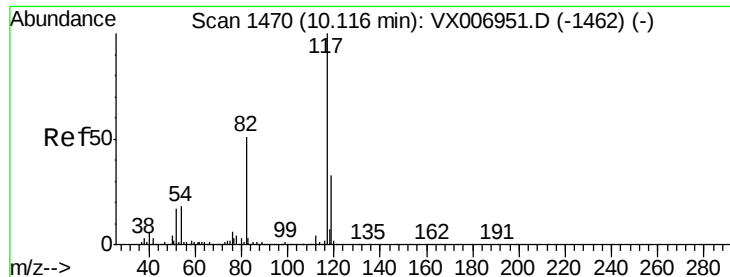

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.01 min

Lab File: VX007165.D

Acq: 21 Jan 2019 18:01

Instrument :

MSVOA\_X

ClientSampleId :

SA-TW528-4246


Tot Ion:117 Resp: 779787

Ion Ratio Lower Upper

117 100

82 52.4 41.0 61.6




119 32.8 25.4 38.0

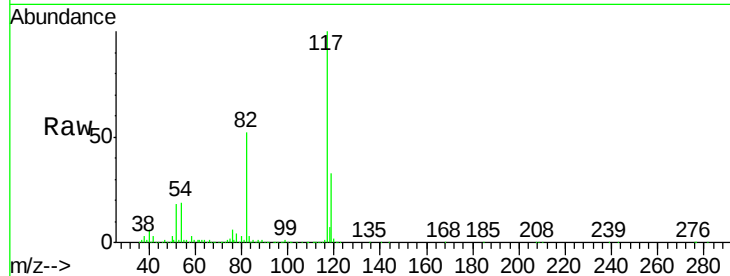

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

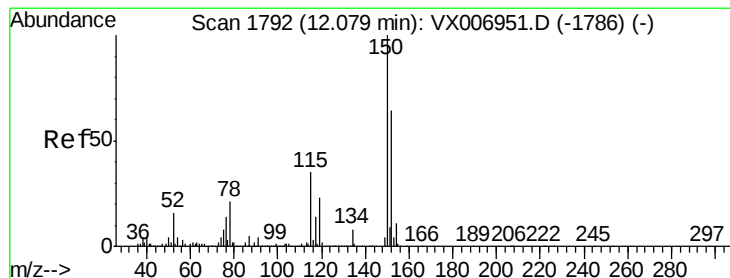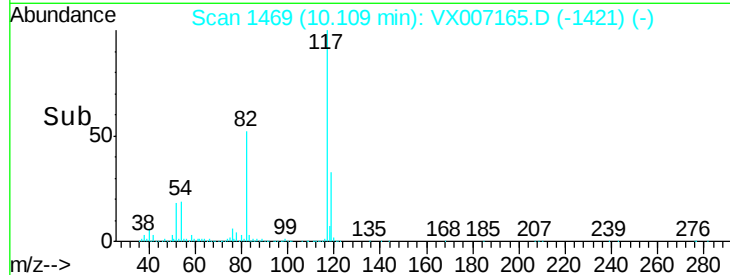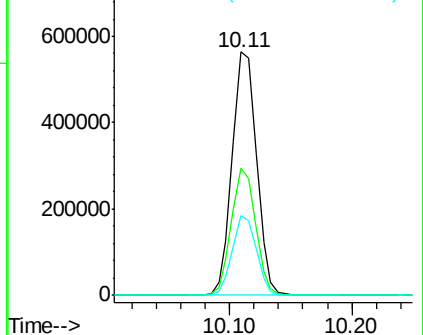

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX007165.D

Acq: 21 Jan 2019 18:01


Tgt Ion:152 Resp: 390655

Ion Ratio Lower Upper

152 100

115 54.7 39.1 117.2

150 157.7 0.0 344.8

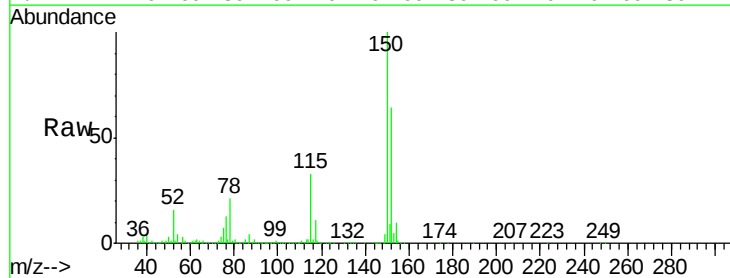

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

