

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012119\  
Data File : VX007156.D  
Acq On : 21 Jan 2019 14:03  
Operator : JC/SP  
Sample : K1198-04  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW517-3337

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.629       | 66            | 78          | 83           | rVB2     | 36837          | 92465         | 3.58%           | 0.646%        |
| 2         | 5.501       | 702           | 713         | 726          | rBV2     | 309798         | 890251        | 34.48%          | 6.219%        |
| 3         | 5.665       | 728           | 740         | 753          | rVV      | 519558         | 1471883       | 57.00%          | 10.283%       |
| 4         | 6.068       | 795           | 806         | 823          | rBV      | 318737         | 835703        | 32.36%          | 5.838%        |
| 5         | 6.860       | 925           | 936         | 947          | rBV      | 782662         | 1839254       | 71.23%          | 12.849%       |
| 6         | 8.714       | 1233          | 1240        | 1248         | rBV      | 1690080        | 2582274       | 100.00%         | 18.040%       |
| 7         | 8.787       | 1248          | 1252        | 1256         | rVB2     | 16872          | 26662         | 1.03%           | 0.186%        |
| 8         | 9.335       | 1334          | 1342        | 1349         | rBV      | 44531          | 68776         | 2.66%           | 0.480%        |
| 9         | 10.110      | 1464          | 1469        | 1478         | rBV      | 1700871        | 2283781       | 88.44%          | 15.955%       |
| 10        | 11.134      | 1631          | 1637        | 1651         | rBV      | 1478467        | 1880151       | 72.81%          | 13.135%       |
| 11        | 12.079      | 1786          | 1792        | 1800         | rBV      | 1852136        | 2343088       | 90.74%          | 16.369%       |


Sum of corrected areas: 14314288

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012119\  
Data File : VX007156.D  
Acq On : 21 Jan 2019 14:03  
Operator : JC/SP  
Sample : K1198-04  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW517-3337

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

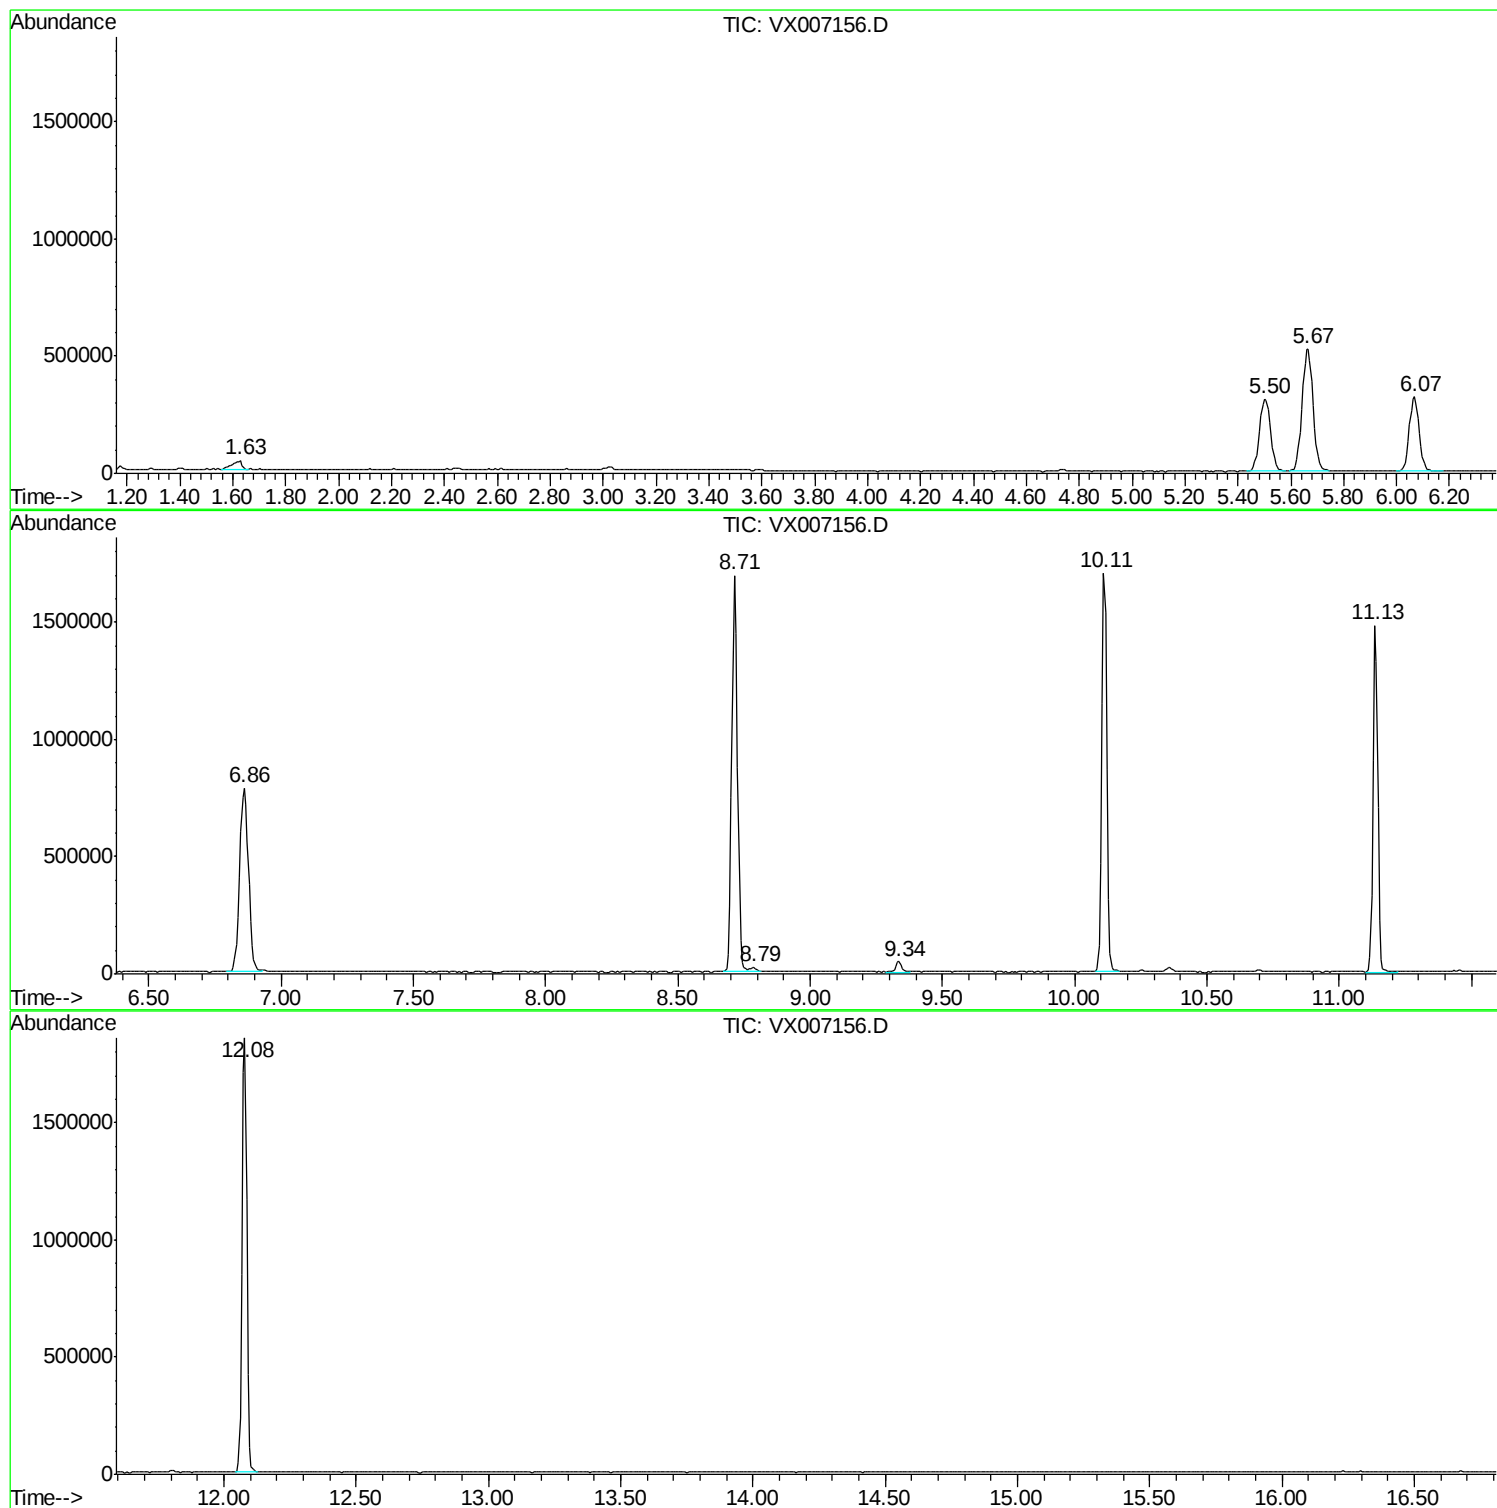

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX012119\  
Data File : VX007156.D  
Acq On : 21 Jan 2019 14:03  
Operator : JC/SP  
Sample : K1198-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW517-3337

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX012119\  
Data File : VX007156.D  
Acq On : 21 Jan 2019 14:03  
Operator : JC/SP  
Sample : K1198-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW517-3337

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |