

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
 Data File : VX044684.D
 Acq On : 21 Jan 2025 16:33
 Operator :
 Sample : Q1131-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 22 01:38:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 22 01:17:07 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	299309	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	252062	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	99259	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	126420	48.941	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	97.880%		
7) Chloroethane-d5	1.648	69	27157	40.809	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.620%		
11) 1,1-Dichloroethene-d2	2.294	65	45398	46.550	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.100%		
21) 2-Butanone-d5	4.452	46	142765	110.253	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	110.250%		
24) Chloroform-d	5.050	84	215361	50.443	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.880%		
26) 1,2-Dichloroethane-d4	5.946	65	139449	49.522	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.040%		
32) Benzene-d6	5.964	84	445936	53.011	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	106.020%		
36) 1,2-Dichloropropane-d6	7.299	67	144928	54.507	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	109.020%		
41) Toluene-d8	8.641	98	389458	51.788	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.580%		
43) trans-1,3-Dichloroprop...	8.945	79	70412	51.671	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	103.340%		
47) 2-Hexanone-d5	9.384	63	87572	114.641	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	114.640%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	179088	55.875	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	111.760%		
66) 1,2-Dichlorobenzene-d4	12.317	152	116103	54.430	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.860%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	8.945	75	3363	1.130	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044684.D
Acq On : 21 Jan 2025 16:33
Operator :
Sample : Q1131-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 22 01:38:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 22 01:17:07 2025
Response via : Initial Calibration

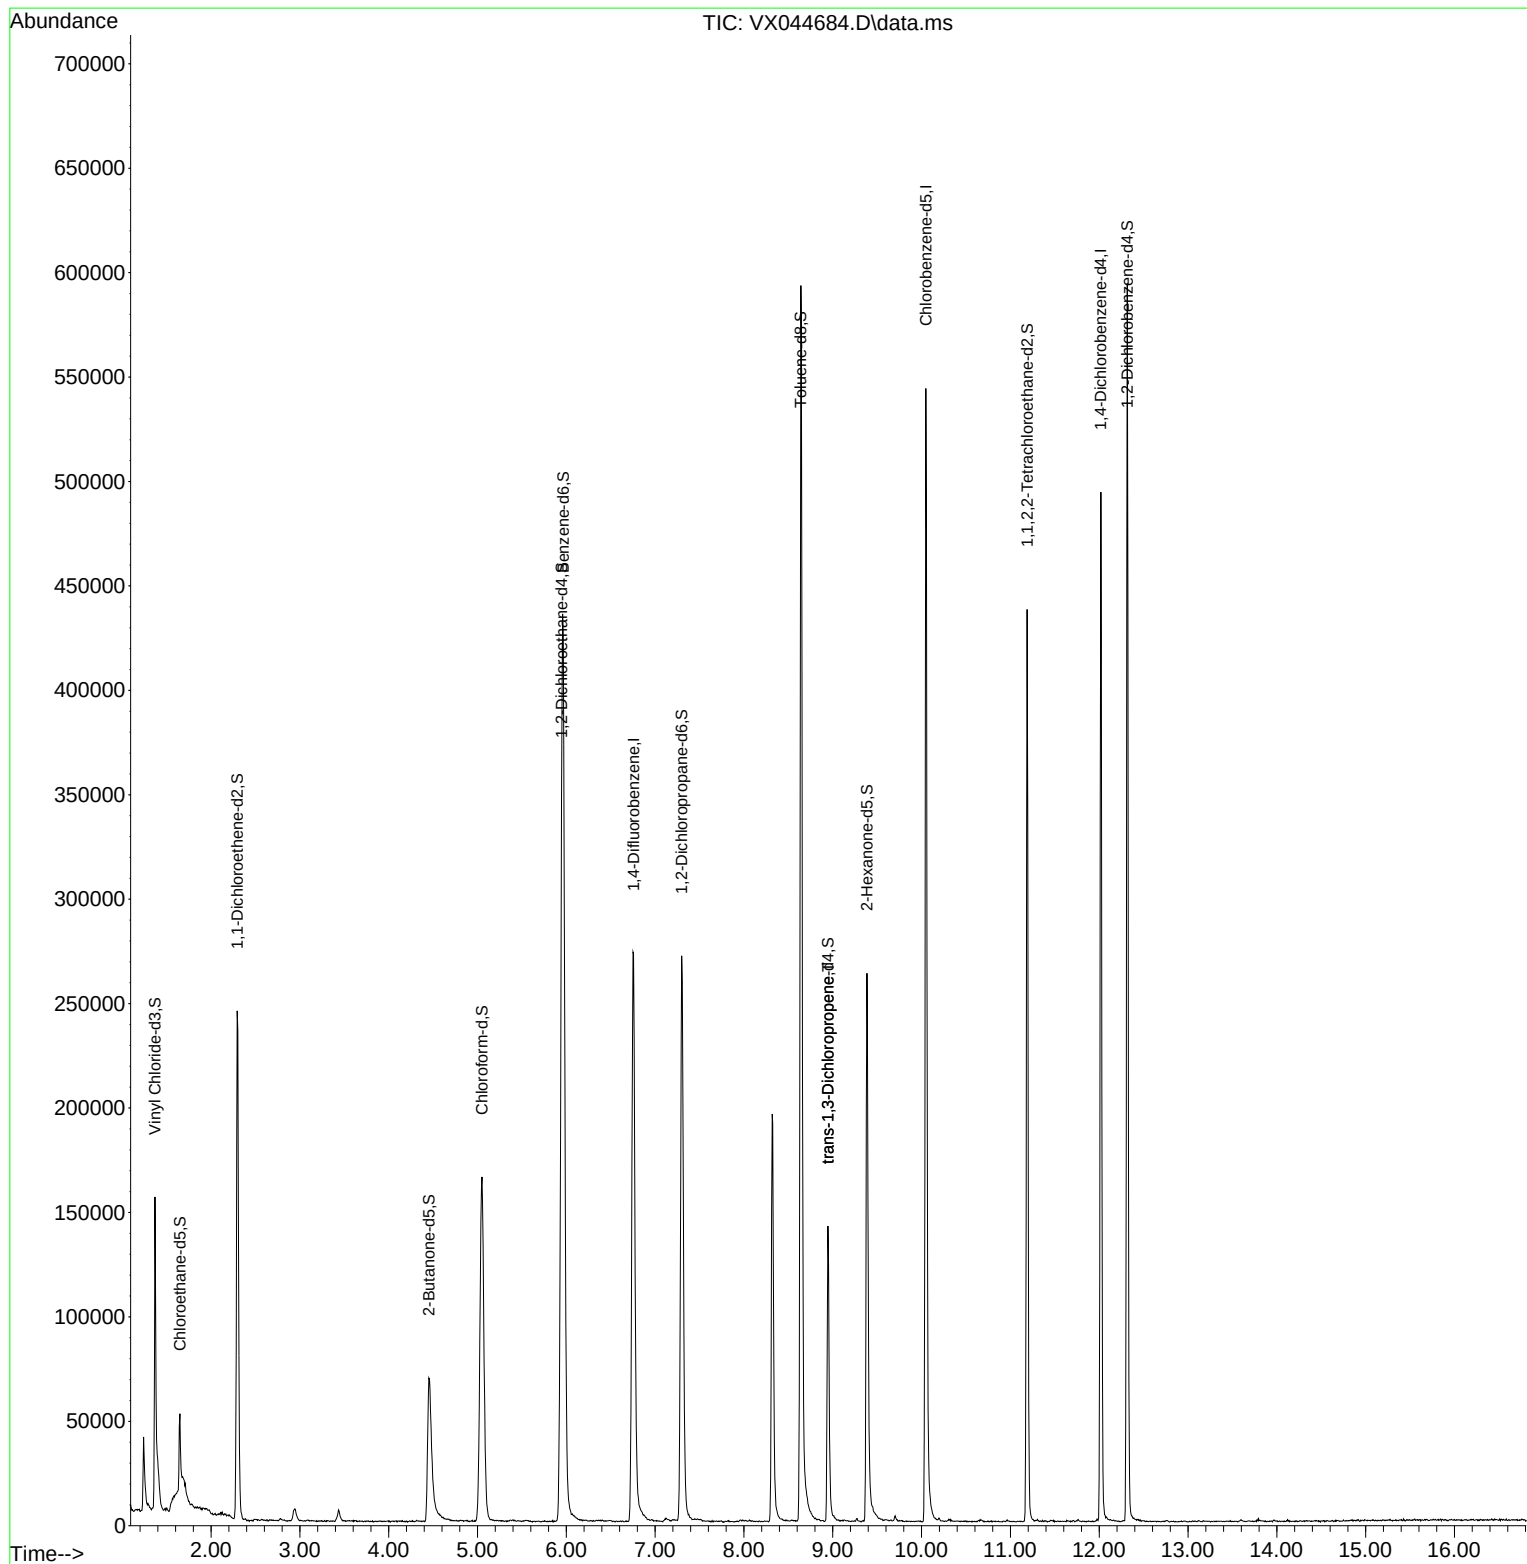

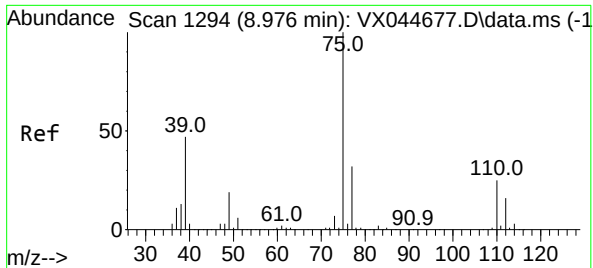

#44
 trans-1,3-Dichloropropene
 Concen: 1.130 ug/L
 RT: 8.945 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VX044684.D
 Acq: 21 Jan 2025 16:33

Instrument :
 MSVOA_X
 ClientSampleId :

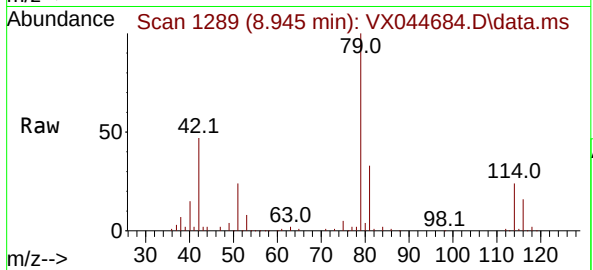

Tgt Ion:	75	Resp:	3363
Ion Ratio	Lower	Upper	
75	100		
77	39.3	22.4	41.6

