

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
 Data File : VX044682.D
 Acq On : 21 Jan 2025 15:39
 Operator : JC/MD
 Sample : VX0121WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK751

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Title : VOC Analysis

Signal : TIC: VX044682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	39	rBV2	31655	56791	5.12%	0.770%
2	1.368	43	46	63	rVB	112637	179256	16.17%	2.430%
3	1.648	89	92	97	rBV	22450	30370	2.74%	0.412%
4	2.288	192	197	207	rVB	186415	299098	26.98%	4.055%
5	2.422	217	219	220	rVB2	550	267	0.02%	0.004%
6	2.459	220	225	227	rBV3	1447	2093	0.19%	0.028%
7	2.941	298	304	311	rBV3	4987	12533	1.13%	0.170%
8	3.166	339	341	343	rBV2	899	697	0.06%	0.009%
9	3.190	343	345	349	rBV5	831	1141	0.10%	0.015%
10	3.294	359	362	364	rBV4	596	820	0.07%	0.011%
11	3.343	369	370	376	rVB5	506	809	0.07%	0.011%
12	3.428	376	384	395	rBV4	5826	15364	1.39%	0.208%
13	3.556	403	405	407	rBV3	767	582	0.05%	0.008%
14	3.636	417	418	420	rVB2	655	415	0.04%	0.006%
15	3.733	431	434	435	rBV2	697	703	0.06%	0.010%
16	3.812	445	447	450	rBV3	395	517	0.05%	0.007%
17	3.892	458	460	462	rBV2	555	383	0.03%	0.005%
18	4.239	514	517	519	rVB4	460	446	0.04%	0.006%
19	4.257	519	520	521	rBV	572	379	0.03%	0.005%
20	4.288	524	525	528	rVB2	736	505	0.05%	0.007%
21	4.459	543	553	570	rBV	60492	206091	18.59%	2.794%
22	4.879	620	622	623	rBV	420	355	0.03%	0.005%
23	4.922	627	629	631	rVV2	550	327	0.03%	0.004%
24	5.044	635	649	666	rBV	136940	432974	39.06%	5.870%
25	5.653	747	749	752	rVB2	455	465	0.04%	0.006%
26	5.739	762	763	765	rVB	497	317	0.03%	0.004%
27	5.763	765	767	769	rBV2	346	359	0.03%	0.005%
28	5.818	774	776	777	rVB	579	315	0.03%	0.004%
29	5.836	777	779	783	rBV3	473	590	0.05%	0.008%
30	5.952	786	798	823	rBV2	368403	1108597	100.00%	15.031%
31	6.263	847	849	850	rBV2	721	488	0.04%	0.007%
32	6.287	850	853	854	rBV	361	393	0.04%	0.005%
33	6.531	892	893	895	rVB	535	259	0.02%	0.004%
34	6.562	895	898	899	rVB2	470	292	0.03%	0.004%
35	6.611	904	906	908	rBV3	486	448	0.04%	0.006%
36	6.751	920	929	945	rBV	237291	588220	53.06%	7.975%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
 Data File : VX044682.D
 Acq On : 21 Jan 2025 15:39
 Operator : JC/MD
 Sample : VX0121WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK751

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Title : VOC Analysis

37	7.299	1010	1019	1038	rBV	220713	501993	45.28%	6.806%
38	7.696	1078	1084	1086	rBV4	594	955	0.09%	0.013%
39	7.873	1112	1113	1115	rBV2	599	402	0.04%	0.005%
40	7.934	1122	1123	1126	rVB2	532	506	0.05%	0.007%
41	7.964	1126	1128	1129	rBV	880	632	0.06%	0.009%
42	8.190	1163	1165	1166	rVB2	439	260	0.02%	0.004%
43	8.208	1166	1168	1169	rBV2	532	272	0.02%	0.004%
44	8.318	1180	1186	1204	rBV	160230	281452	25.39%	3.816%
45	8.641	1233	1239	1273	rVB	488361	855842	77.20%	11.604%
46	8.897	1280	1281	1284	rBV2	696	634	0.06%	0.009%
47	8.946	1284	1289	1309	rVV	107994	180458	16.28%	2.447%
48	9.244	1336	1338	1339	rBV	491	315	0.03%	0.004%
49	9.269	1339	1342	1347	rBV5	1514	2417	0.22%	0.033%
50	9.391	1356	1362	1379	rBV	204978	385863	34.81%	5.232%
51	9.708	1410	1414	1419	rVB5	1669	3287	0.30%	0.045%
52	9.958	1453	1455	1458	rBV2	325	341	0.03%	0.005%
53	9.982	1458	1459	1460	rBV	481	269	0.02%	0.004%
54	10.049	1464	1470	1486	rBV	428055	636958	57.46%	8.636%
55	10.305	1510	1512	1516	rVB4	1477	1183	0.11%	0.016%
56	10.421	1530	1531	1534	rBV3	563	276	0.02%	0.004%
57	10.598	1556	1560	1562	rBV5	470	862	0.08%	0.012%
58	10.646	1566	1568	1570	rBV3	1078	1114	0.10%	0.015%
59	10.756	1584	1586	1588	rBV	477	375	0.03%	0.005%
60	10.854	1601	1602	1605	rBV2	615	671	0.06%	0.009%
61	11.012	1626	1628	1631	rVB3	712	821	0.07%	0.011%
62	11.049	1631	1634	1635	rBV2	576	598	0.05%	0.008%
63	11.110	1642	1644	1647	rVB3	426	440	0.04%	0.006%
64	11.134	1647	1648	1651	rVB2	469	380	0.03%	0.005%
65	11.189	1651	1657	1669	rBV	358329	479781	43.28%	6.505%
66	11.415	1690	1694	1697	rBV3	499	636	0.06%	0.009%
67	11.457	1697	1701	1704	rBV4	1660	2139	0.19%	0.029%
68	11.561	1714	1718	1719	rBV3	656	786	0.07%	0.011%
69	11.610	1724	1726	1731	rVV3	486	628	0.06%	0.009%
70	11.713	1741	1743	1745	rBV3	667	568	0.05%	0.008%
71	11.762	1748	1751	1754	rVB4	1669	2237	0.20%	0.030%
72	11.860	1765	1767	1770	rBV3	418	470	0.04%	0.006%
73	11.975	1782	1786	1788	rBV3	2470	3413	0.31%	0.046%
74	12.018	1788	1793	1803	rVV	379481	485833	43.82%	6.587%
75	12.317	1837	1842	1858	rBV	436340	569116	51.34%	7.716%
76	12.689	1899	1903	1904	rBV3	398	401	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
 Data File : VX044682.D
 Acq On : 21 Jan 2025 15:39
 Operator : JC/MD
 Sample : VX0121WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK751

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Title : VOC Analysis

77	12.719	1907	1908	1910	rBV2	375	290	0.03%	0.004%
78	12.798	1917	1921	1923	rBV3	530	629	0.06%	0.009%
79	12.847	1925	1929	1932	rBV3	526	829	0.07%	0.011%
80	12.890	1935	1936	1939	rVB2	548	349	0.03%	0.005%
81	12.914	1939	1940	1942	rBV	415	332	0.03%	0.005%
82	13.116	1969	1973	1982	rVB6	1476	2754	0.25%	0.037%
83	13.256	1993	1996	1999	rBV3	469	516	0.05%	0.007%
84	13.286	1999	2001	2004	rBV3	421	456	0.04%	0.006%
85	13.372	2011	2015	2016	rBV3	727	726	0.07%	0.010%
86	13.420	2022	2023	2025	rBV2	532	325	0.03%	0.004%
87	13.451	2026	2028	2029	rVB2	508	316	0.03%	0.004%
88	13.487	2032	2034	2039	rBV4	456	762	0.07%	0.010%
89	13.536	2039	2042	2044	rBV3	523	563	0.05%	0.008%
90	13.597	2047	2052	2058	rVB6	1801	3563	0.32%	0.048%
91	13.737	2073	2075	2076	rBV2	302	265	0.02%	0.004%
92	13.780	2078	2082	2089	rVV2	3415	6476	0.58%	0.088%
93	13.902	2100	2102	2103	rBV	701	600	0.05%	0.008%
94	13.963	2109	2112	2117	rBV5	2202	3178	0.29%	0.043%
95	14.377	2177	2180	2182	rBV4	493	485	0.04%	0.007%
96	14.420	2186	2187	2191	rBV3	359	314	0.03%	0.004%
97	14.603	2213	2217	2219	rBV4	510	725	0.07%	0.010%
98	15.292	2327	2330	2332	rBV4	789	943	0.09%	0.013%
99	15.597	2379	2380	2381	rBV	564	256	0.02%	0.003%
100	16.115	2463	2465	2467	rBV2	764	656	0.06%	0.009%

Sum of corrected areas: 7375551




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044682.D
Acq On : 21 Jan 2025 15:39
Operator : JC/MD
Sample : VX0121WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK751

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

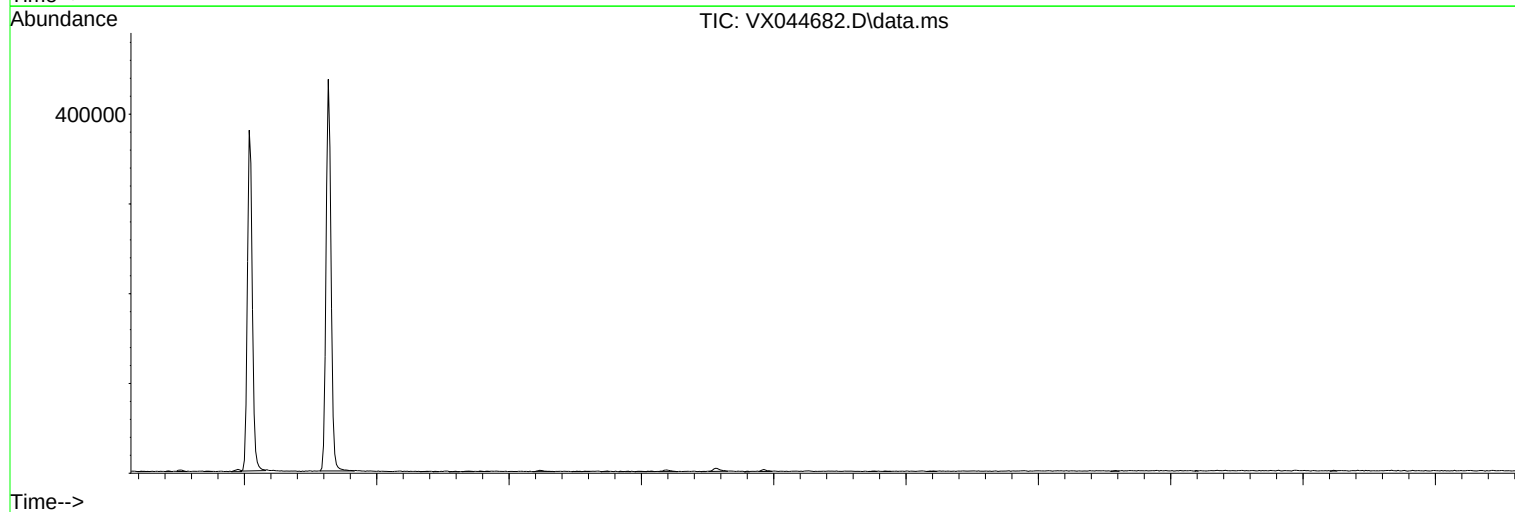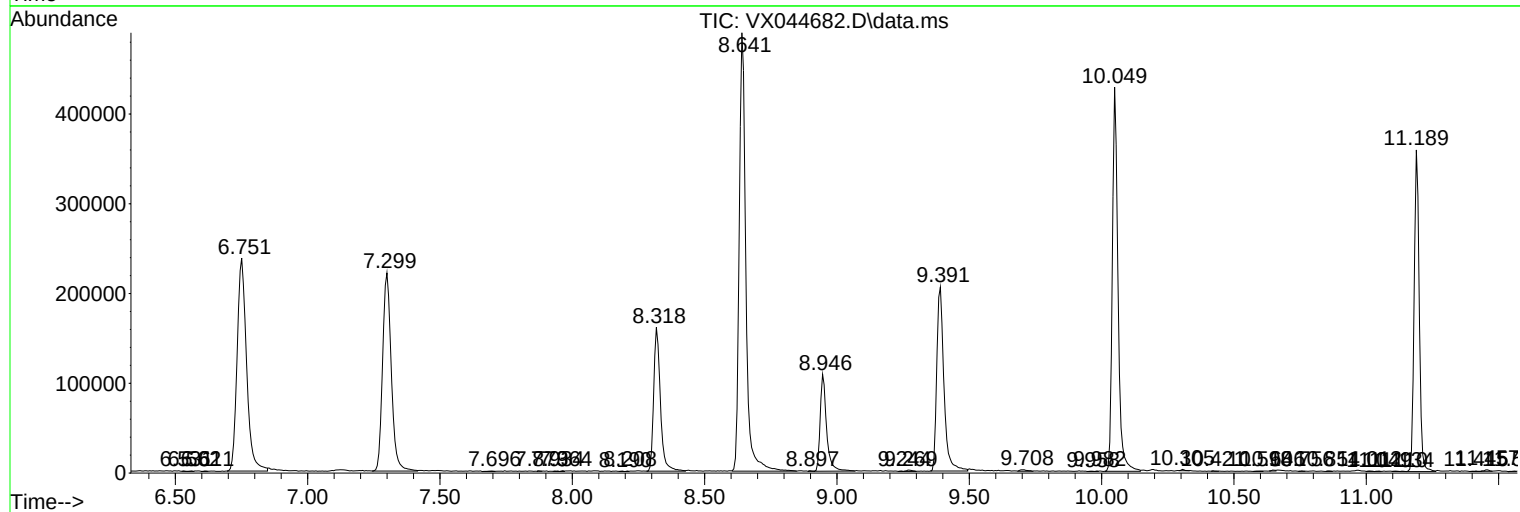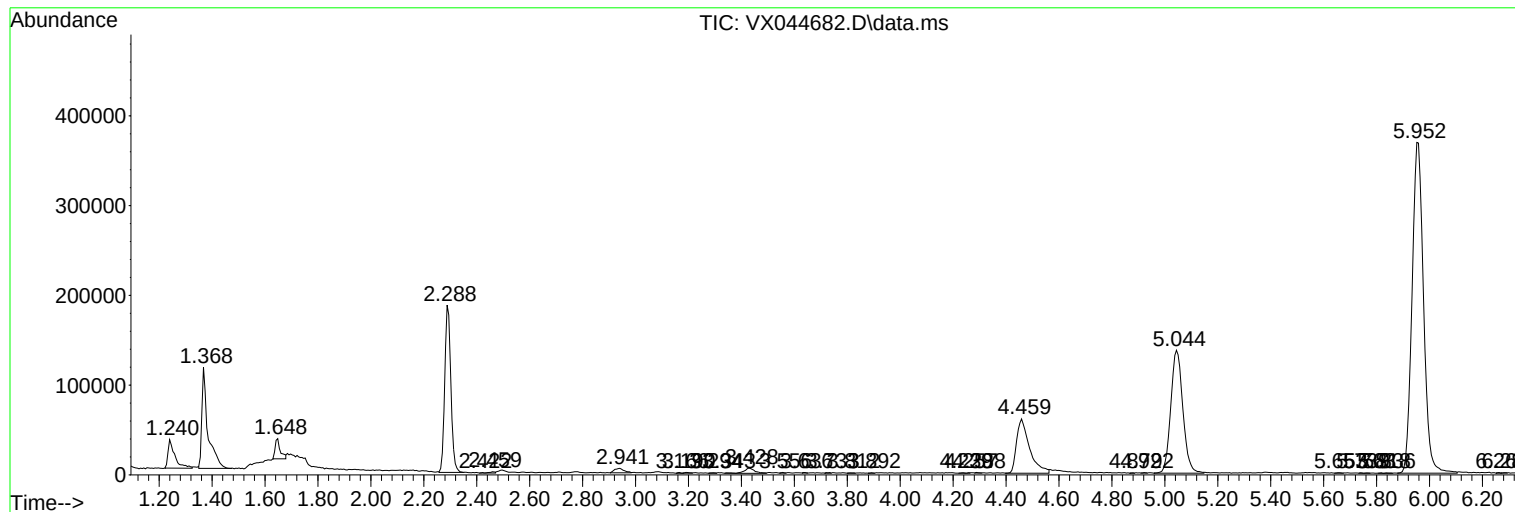

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044682.D
Acq On : 21 Jan 2025 15:39
Operator : JC/MD
Sample : VX0121WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK751

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044682.D
Acq On : 21 Jan 2025 15:39
Operator : JC/MD
Sample : VX0121WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK751

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
