

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
 Data File : VX044683.D
 Acq On : 21 Jan 2025 16:10
 Operator : JC/MD
 Sample : Q1131-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 JNLE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Title : VOC Analysis

Signal : TIC: VX044683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV	31670	45559	5.96%	0.765%
2	1.368	42	46	62	rVV	104276	167884	21.95%	2.819%
3	1.496	64	67	71	rVB2	6823	8589	1.12%	0.144%
4	1.648	88	92	96	rBV	22014	31339	4.10%	0.526%
5	2.294	192	198	207	rVV	161365	257302	33.63%	4.320%
6	2.386	209	213	217	rBV2	1968	3400	0.44%	0.057%
7	2.496	228	231	236	rVB2	2316	3589	0.47%	0.060%
8	2.563	236	242	244	rBV5	423	818	0.11%	0.014%
9	2.703	263	265	269	rVB2	447	461	0.06%	0.008%
10	2.782	273	278	282	rBV3	1619	2785	0.36%	0.047%
11	2.941	297	304	310	rBV2	3918	9385	1.23%	0.158%
12	3.032	315	319	323	rBV4	377	568	0.07%	0.010%
13	3.105	323	331	332	rBV5	2018	4787	0.63%	0.080%
14	3.337	366	369	370	rBV	538	441	0.06%	0.007%
15	3.434	378	385	393	rBV3	3972	9587	1.25%	0.161%
16	3.605	407	413	418	rBV3	853	1573	0.21%	0.026%
17	3.697	427	428	431	rVB2	400	375	0.05%	0.006%
18	3.739	431	435	436	rBV2	489	672	0.09%	0.011%
19	3.965	468	472	473	rBV3	501	767	0.10%	0.013%
20	4.154	500	503	506	rBV2	506	601	0.08%	0.010%
21	4.227	513	515	517	rBV3	368	390	0.05%	0.007%
22	4.398	540	543	545	rBV3	433	579	0.08%	0.010%
23	4.459	545	553	583	rVV	55749	203968	26.66%	3.425%
24	4.891	622	624	629	rBV3	721	1167	0.15%	0.020%
25	5.044	637	649	669	rBV	97557	314270	41.08%	5.277%
26	5.221	675	678	679	rVB2	560	447	0.06%	0.008%
27	5.251	679	683	685	rBV3	388	419	0.05%	0.007%
28	5.306	687	692	695	rVB2	696	1049	0.14%	0.018%
29	5.379	697	704	706	rBV6	1152	2035	0.27%	0.034%
30	5.452	710	716	722	rBV4	1384	3298	0.43%	0.055%
31	5.666	745	751	755	rVV6	1072	2417	0.32%	0.041%
32	5.818	773	776	778	rBV2	374	401	0.05%	0.007%
33	5.958	785	799	818	rBV2	251846	764996	100.00%	12.845%
34	6.275	848	851	854	rVB3	416	585	0.08%	0.010%
35	6.342	856	862	864	rBV3	736	1174	0.15%	0.020%
36	6.385	868	869	872	rVB2	546	435	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
 Data File : VX044683.D
 Acq On : 21 Jan 2025 16:10
 Operator : JC/MD
 Sample : Q1131-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 JNLE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Title : VOC Analysis

37	6.586	900	902	905	rBV2	341	383	0.05%	0.006%
38	6.672	913	916	918	rBV2	449	601	0.08%	0.010%
39	6.751	920	929	952	rBV	147282	376804	49.26%	6.327%
40	7.123	982	990	998	rBV9	2589	6866	0.90%	0.115%

41	7.300	1011	1019	1035	rBV	156594	354398	46.33%	5.951%
42	7.476	1046	1048	1051	rVB4	506	446	0.06%	0.007%
43	7.647	1072	1076	1078	rBV3	342	454	0.06%	0.008%
44	7.818	1100	1104	1108	rBV4	1014	1982	0.26%	0.033%
45	7.982	1123	1131	1136	rBV7	953	2913	0.38%	0.049%

46	8.232	1169	1172	1176	rBV2	379	446	0.06%	0.007%
47	8.269	1176	1178	1180	rVB2	552	519	0.07%	0.009%
48	8.318	1180	1186	1201	rBV	115914	207982	27.19%	3.492%
49	8.476	1208	1212	1215	rVB4	544	723	0.09%	0.012%
50	8.580	1224	1229	1233	rBV5	1713	3655	0.48%	0.061%

51	8.641	1233	1239	1249	rBV	340151	580963	75.94%	9.755%
52	8.946	1284	1289	1306	rBV	79164	136956	17.90%	2.300%
53	9.153	1320	1323	1328	rBV3	1586	2264	0.30%	0.038%
54	9.269	1335	1342	1348	rVB3	5061	8470	1.11%	0.142%
55	9.385	1356	1361	1380	rVV	211779	401962	52.54%	6.749%

56	9.513	1380	1382	1388	rVB3	2039	3200	0.42%	0.054%
57	9.610	1395	1398	1402	rVB3	1113	1466	0.19%	0.025%
58	9.860	1435	1439	1441	rBV4	632	851	0.11%	0.014%
59	9.927	1446	1450	1451	rBV3	313	389	0.05%	0.007%
60	10.049	1465	1470	1489	rVV	281687	437472	57.19%	7.345%

61	10.195	1490	1494	1502	rVV3	3821	6915	0.90%	0.116%
62	10.305	1506	1512	1518	rVV3	3681	6408	0.84%	0.108%
63	10.537	1548	1550	1553	rBV3	463	556	0.07%	0.009%
64	10.567	1553	1555	1558	rVB	454	412	0.05%	0.007%
65	10.647	1562	1568	1574	rBV5	4802	10953	1.43%	0.184%

66	10.799	1589	1593	1594	rBV3	1356	1628	0.21%	0.027%
67	10.896	1606	1609	1611	rBV3	523	518	0.07%	0.009%
68	10.964	1611	1620	1626	rBV2	4904	9441	1.23%	0.159%
69	11.012	1626	1628	1630	rVB2	494	409	0.05%	0.007%
70	11.153	1648	1651	1652	rBV2	563	507	0.07%	0.009%

71	11.189	1652	1657	1670	rVV	373327	508457	66.47%	8.537%
72	11.305	1673	1676	1681	rVB4	2291	3469	0.45%	0.058%
73	11.348	1681	1683	1686	rBV3	583	692	0.09%	0.012%
74	11.451	1697	1700	1710	rVB3	5150	8184	1.07%	0.137%
75	11.707	1740	1742	1745	rBV2	631	831	0.11%	0.014%

76	11.756	1746	1750	1755	rVB3	5189	7095	0.93%	0.119%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
 Data File : VX044683.D
 Acq On : 21 Jan 2025 16:10
 Operator : JC/MD
 Sample : Q1131-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 JNLE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Title : VOC Analysis

77	11.976	1782	1786	1788	rBV3	3906	5489	0.72%	0.092%
78	12.018	1788	1793	1808	rVB	319796	423251	55.33%	7.107%
79	12.232	1823	1828	1831	rBV3	1915	3561	0.47%	0.060%
80	12.317	1837	1842	1853	rBV	414517	544493	71.18%	9.142%
81	12.890	1932	1936	1937	rBV3	582	607	0.08%	0.010%
82	13.116	1970	1973	1978	rBV4	2613	3684	0.48%	0.062%
83	13.219	1988	1990	1991	rBV2	508	432	0.06%	0.007%
84	13.274	1997	1999	2000	rBV2	398	393	0.05%	0.007%
85	13.451	2025	2028	2029	rBV2	507	463	0.06%	0.008%
86	13.591	2048	2051	2056	rBV4	3793	5097	0.67%	0.086%
87	13.780	2077	2082	2093	rBV2	4954	9267	1.21%	0.156%
88	13.933	2103	2107	2108	rBV3	573	651	0.09%	0.011%
89	13.963	2108	2112	2116	rVV4	3015	4421	0.58%	0.074%
90	14.030	2122	2123	2127	rBV4	584	516	0.07%	0.009%
91	14.122	2137	2138	2140	rBV	733	561	0.07%	0.009%
92	14.268	2160	2162	2165	rVB2	518	509	0.07%	0.009%
93	14.615	2217	2219	2221	rVB2	701	495	0.06%	0.008%
94	14.676	2227	2229	2233	rBV4	384	555	0.07%	0.009%
95	15.225	2317	2319	2322	rBV3	744	836	0.11%	0.014%
96	15.304	2331	2332	2339	rVB6	821	1157	0.15%	0.019%
97	15.609	2380	2382	2384	rBV2	862	554	0.07%	0.009%
98	15.938	2434	2436	2437	rBV	668	469	0.06%	0.008%
99	16.036	2450	2452	2455	rBV3	706	669	0.09%	0.011%
100	16.615	2545	2547	2550	rBV3	634	872	0.11%	0.015%

Sum of corrected areas: 5955754




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044683.D
Acq On : 21 Jan 2025 16:10
Operator : JC/MD
Sample : Q1131-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JNLE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

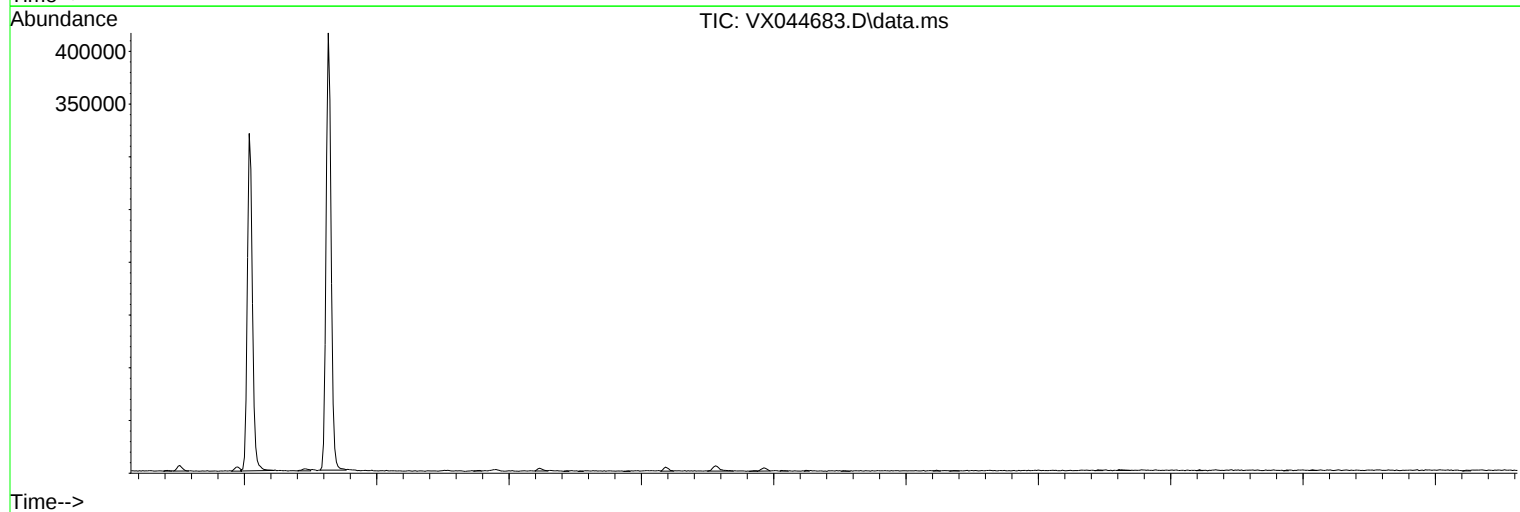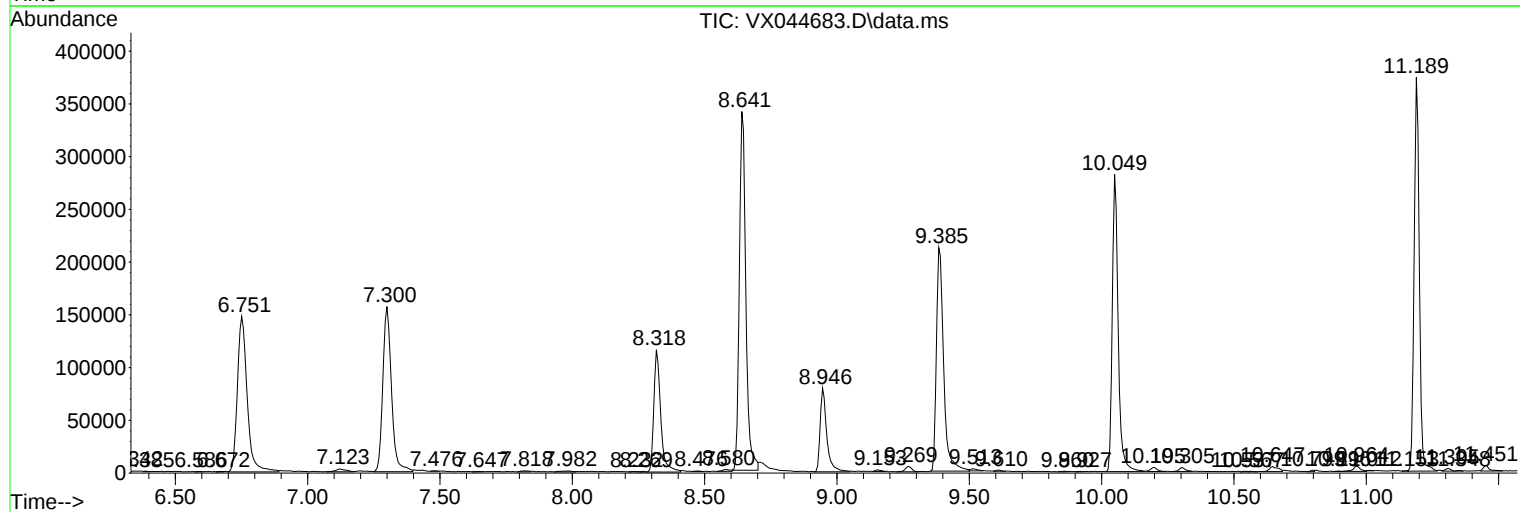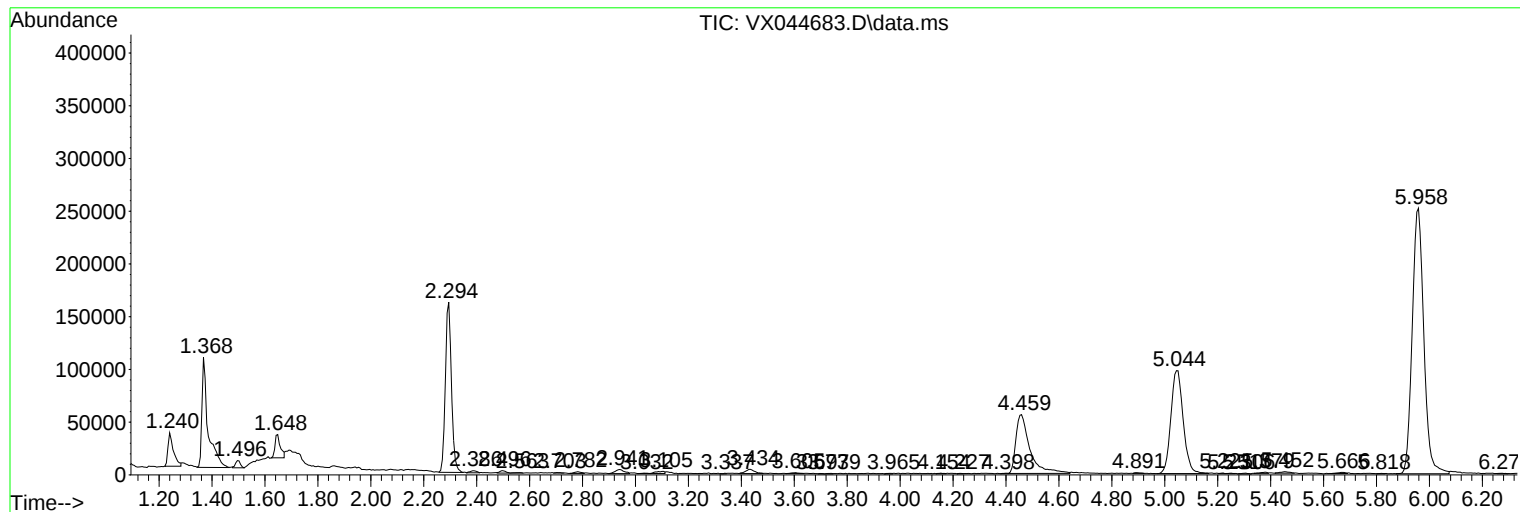

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044683.D
Acq On : 21 Jan 2025 16:10
Operator : JC/MD
Sample : Q1131-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JNLE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044683.D
Acq On : 21 Jan 2025 16:10
Operator : JC/MD
Sample : Q1131-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JNLE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc