

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
 Data File : VX044684.D
 Acq On : 21 Jan 2025 16:33
 Operator : JC/MD
 Sample : Q1131-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM012125WMA.M
 Title : VOC Analysis

Signal : TIC: VX044684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	32	rBV	35134	48389	3.71%	0.542%
2	1.367	43	46	62	rVB	150107	202613	15.54%	2.270%
3	1.648	89	92	96	rBV	36482	43672	3.35%	0.489%
4	2.294	192	198	209	rVB	243570	390965	29.99%	4.381%
5	2.483	227	229	230	rBV2	877	780	0.06%	0.009%
6	2.940	298	304	313	rVB2	5708	14734	1.13%	0.165%
7	3.276	358	359	362	rVB3	638	501	0.04%	0.006%
8	3.434	378	385	394	rBV2	5536	12148	0.93%	0.136%
9	3.751	435	437	439	rBV2	394	335	0.03%	0.004%
10	3.855	451	454	456	rBV2	313	360	0.03%	0.004%
11	4.026	481	482	483	rBV	485	336	0.03%	0.004%
12	4.087	488	492	493	rVB3	566	690	0.05%	0.008%
13	4.105	493	495	497	rBV2	532	609	0.05%	0.007%
14	4.196	508	510	512	rVB2	564	499	0.04%	0.006%
15	4.233	514	516	518	rVV2	406	331	0.03%	0.004%
16	4.312	527	529	533	rVV3	552	561	0.04%	0.006%
17	4.452	544	552	577	rBV	68831	237833	18.25%	2.665%
18	4.812	607	611	613	rBV4	564	723	0.06%	0.008%
19	5.050	638	650	665	rBV	164886	515923	39.58%	5.781%
20	5.623	743	744	746	rBV2	455	459	0.04%	0.005%
21	5.665	749	751	753	rBV	345	399	0.03%	0.004%
22	5.739	760	763	764	rBV2	401	420	0.03%	0.005%
23	5.757	764	766	768	rVV3	610	456	0.03%	0.005%
24	5.867	782	784	785	rBV	493	335	0.03%	0.004%
25	5.958	788	799	815	rBV2	434305	1303536	100.00%	14.606%
26	6.568	896	899	901	rBV4	531	703	0.05%	0.008%
27	6.635	908	910	912	rVB	463	361	0.03%	0.004%
28	6.751	920	929	957	rBV	272781	703927	54.00%	7.887%
29	7.123	984	990	999	rBV9	1874	5509	0.42%	0.062%
30	7.299	1011	1019	1038	rBV	270421	606795	46.55%	6.799%
31	7.641	1073	1075	1077	rVB3	726	410	0.03%	0.005%
32	7.659	1077	1078	1081	rBV2	531	594	0.05%	0.007%
33	7.793	1097	1100	1102	rVV2	456	656	0.05%	0.007%
34	7.824	1102	1105	1108	rVB5	695	828	0.06%	0.009%
35	7.921	1116	1121	1124	rBV6	567	836	0.06%	0.009%
36	7.958	1124	1127	1130	rVV4	850	1352	0.10%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
 Data File : VX044684.D
 Acq On : 21 Jan 2025 16:33
 Operator : JC/MD
 Sample : Q1131-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Title : VOC Analysis

37	8.013	1134	1136	1140	rVV4	637	894	0.07%	0.010%
38	8.061	1142	1144	1147	rVB4	695	663	0.05%	0.007%
39	8.171	1160	1162	1165	rBV3	454	455	0.03%	0.005%
40	8.317	1180	1186	1203	rBV	195010	347184	26.63%	3.890%
41	8.641	1233	1239	1265	rBV	591193	1030480	79.05%	11.546%
42	8.945	1284	1289	1299	rBV	141214	218177	16.74%	2.445%
43	9.220	1331	1334	1336	rBV2	328	333	0.03%	0.004%
44	9.275	1339	1343	1348	rBB4	1331	1555	0.12%	0.017%
45	9.342	1350	1354	1356	rBV3	790	980	0.08%	0.011%
46	9.384	1356	1361	1383	rBV	262336	443809	34.05%	4.973%
47	9.701	1410	1413	1420	rVB3	2583	3510	0.27%	0.039%
48	10.049	1465	1470	1487	rBV	542325	796265	61.09%	8.922%
49	10.573	1555	1556	1559	rBV3	529	591	0.05%	0.007%
50	10.640	1564	1567	1569	rBV4	654	733	0.06%	0.008%
51	10.658	1569	1570	1571	rBV	770	412	0.03%	0.005%
52	10.780	1587	1590	1591	rBV3	469	330	0.03%	0.004%
53	10.817	1593	1596	1597	rBV2	327	345	0.03%	0.004%
54	10.921	1611	1613	1614	rBV	408	377	0.03%	0.004%
55	10.963	1617	1620	1621	rBV3	942	746	0.06%	0.008%
56	11.079	1637	1639	1641	rBV	353	363	0.03%	0.004%
57	11.189	1652	1657	1670	rVV	436629	570328	43.75%	6.390%
58	11.305	1674	1676	1680	rVV3	1092	1046	0.08%	0.012%
59	11.335	1680	1681	1684	rVB2	430	342	0.03%	0.004%
60	11.360	1684	1685	1688	rBV2	709	524	0.04%	0.006%
61	11.390	1688	1690	1691	rVV	522	466	0.04%	0.005%
62	11.421	1694	1695	1698	rBV3	301	416	0.03%	0.005%
63	11.451	1698	1700	1701	rVV2	792	633	0.05%	0.007%
64	11.634	1729	1730	1731	rBV	659	359	0.03%	0.004%
65	11.707	1740	1742	1745	rVB3	665	758	0.06%	0.008%
66	11.744	1745	1748	1749	rVV2	555	538	0.04%	0.006%
67	11.762	1749	1751	1757	rVV4	1139	1564	0.12%	0.018%
68	11.811	1757	1759	1761	rVV3	393	365	0.03%	0.004%
69	11.975	1780	1786	1788	rBV4	1391	1874	0.14%	0.021%
70	12.018	1788	1793	1802	rBV	492407	629189	48.27%	7.050%
71	12.317	1837	1842	1853	rBV	592409	749881	57.53%	8.402%
72	12.481	1868	1869	1873	rBV3	404	583	0.04%	0.007%
73	12.762	1911	1915	1920	rVB5	736	1309	0.10%	0.015%
74	12.811	1920	1923	1925	rBV4	367	474	0.04%	0.005%
75	13.115	1972	1973	1978	rVB4	555	714	0.05%	0.008%
76	13.170	1981	1982	1985	rBV2	584	546	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
 Data File : VX044684.D
 Acq On : 21 Jan 2025 16:33
 Operator : JC/MD
 Sample : Q1131-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Title : VOC Analysis

77	13.268	1996	1998	2000	rBV3	313	347	0.03%	0.004%
78	13.475	2030	2032	2035	rVB2	523	367	0.03%	0.004%
79	13.676	2061	2065	2066	rBV2	426	494	0.04%	0.006%
80	13.792	2080	2084	2085	rBV3	1514	1501	0.12%	0.017%
81	13.896	2099	2101	2104	rBV3	350	433	0.03%	0.005%
82	13.975	2110	2114	2117	rBV4	863	1460	0.11%	0.016%
83	14.030	2121	2123	2125	rBV2	380	351	0.03%	0.004%
84	14.121	2134	2138	2140	rVV5	915	921	0.07%	0.010%
85	14.158	2142	2144	2146	rBV2	364	358	0.03%	0.004%
86	14.262	2159	2161	2165	rBV3	473	586	0.04%	0.007%
87	14.487	2196	2198	2199	rVB	603	431	0.03%	0.005%
88	14.505	2199	2201	2203	rBV2	646	804	0.06%	0.009%
89	14.566	2209	2211	2215	rBV3	500	634	0.05%	0.007%
90	14.627	2218	2221	2223	rVB2	684	702	0.05%	0.008%
91	14.646	2223	2224	2226	rBV	501	411	0.03%	0.005%
92	14.749	2239	2241	2244	rBV3	597	418	0.03%	0.005%
93	14.865	2259	2260	2263	rBV3	452	477	0.04%	0.005%
94	14.944	2272	2273	2274	rBV	658	367	0.03%	0.004%
95	14.987	2279	2280	2285	rVV3	639	792	0.06%	0.009%
96	15.188	2311	2313	2315	rBV3	565	574	0.04%	0.006%
97	15.426	2350	2352	2355	rVB2	1035	880	0.07%	0.010%
98	15.463	2355	2358	2359	rBV2	714	570	0.04%	0.006%
99	15.865	2422	2424	2427	rBV3	731	916	0.07%	0.010%
100	16.511	2528	2530	2531	rVB	848	430	0.03%	0.005%




Sum of corrected areas: 8924913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044684.D
Acq On : 21 Jan 2025 16:33
Operator : JC/MD
Sample : Q1131-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

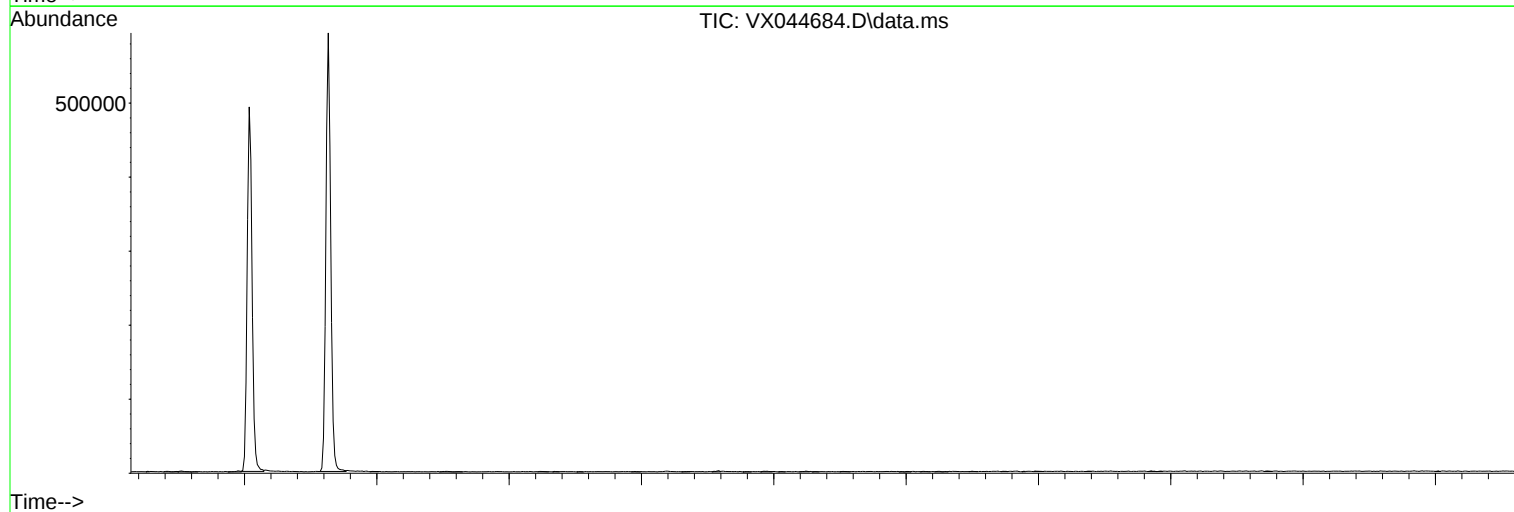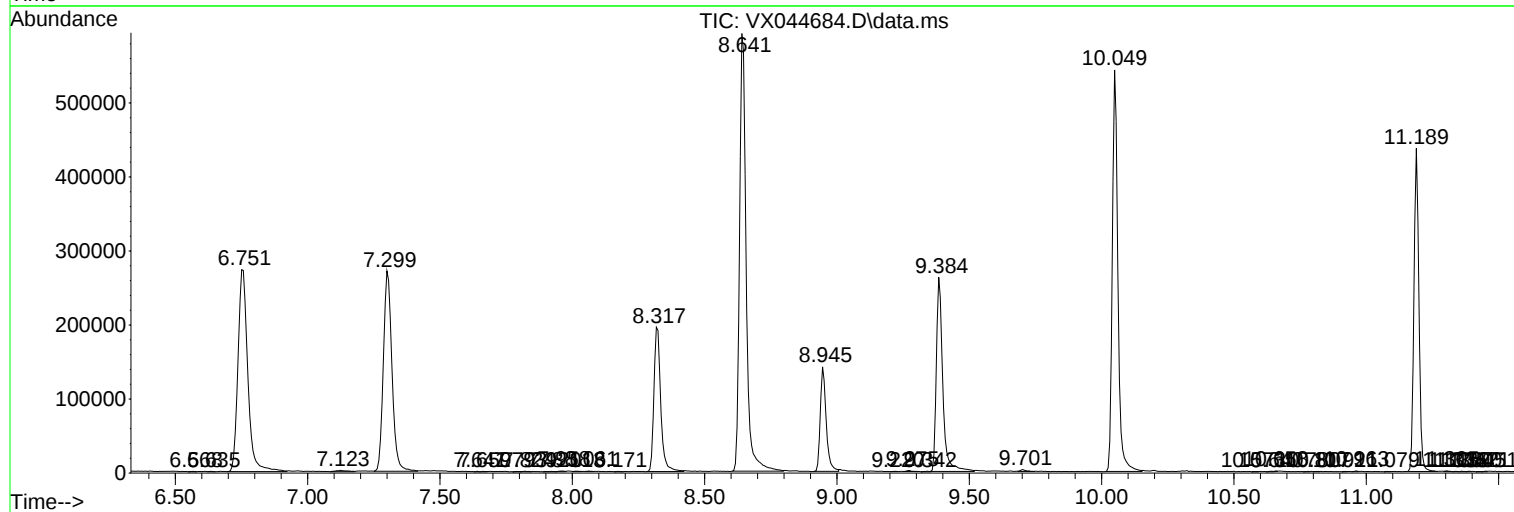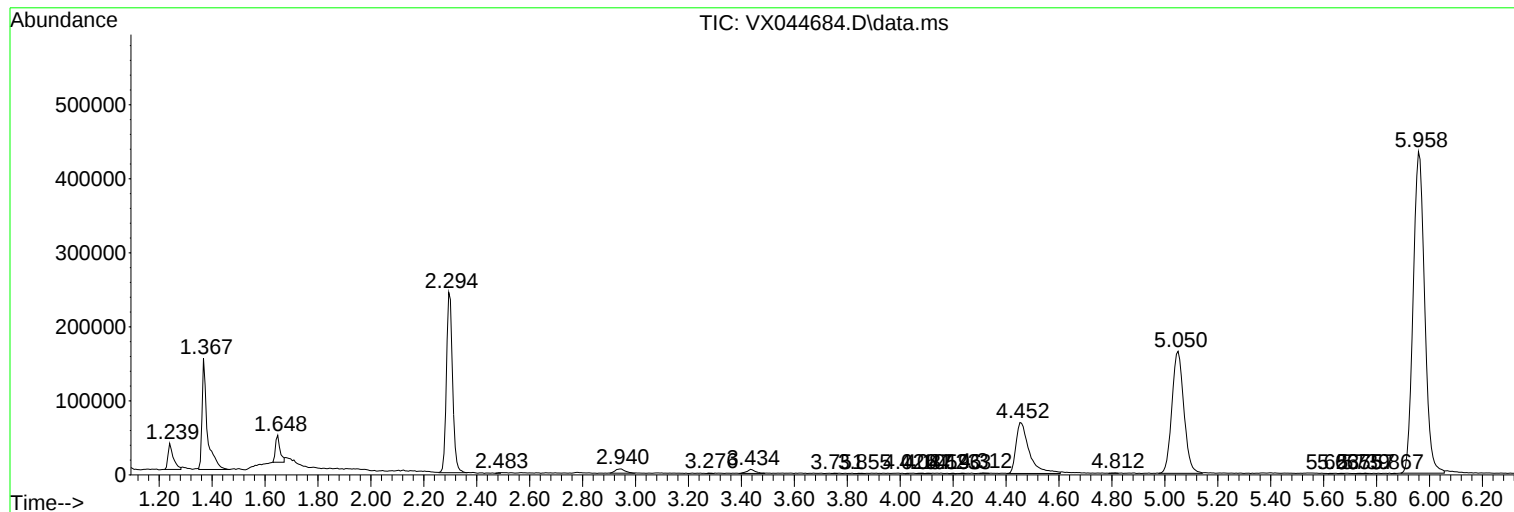

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044684.D
Acq On : 21 Jan 2025 16:33
Operator : JC/MD
Sample : Q1131-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044684.D
Acq On : 21 Jan 2025 16:33
Operator : JC/MD
Sample : Q1131-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc