
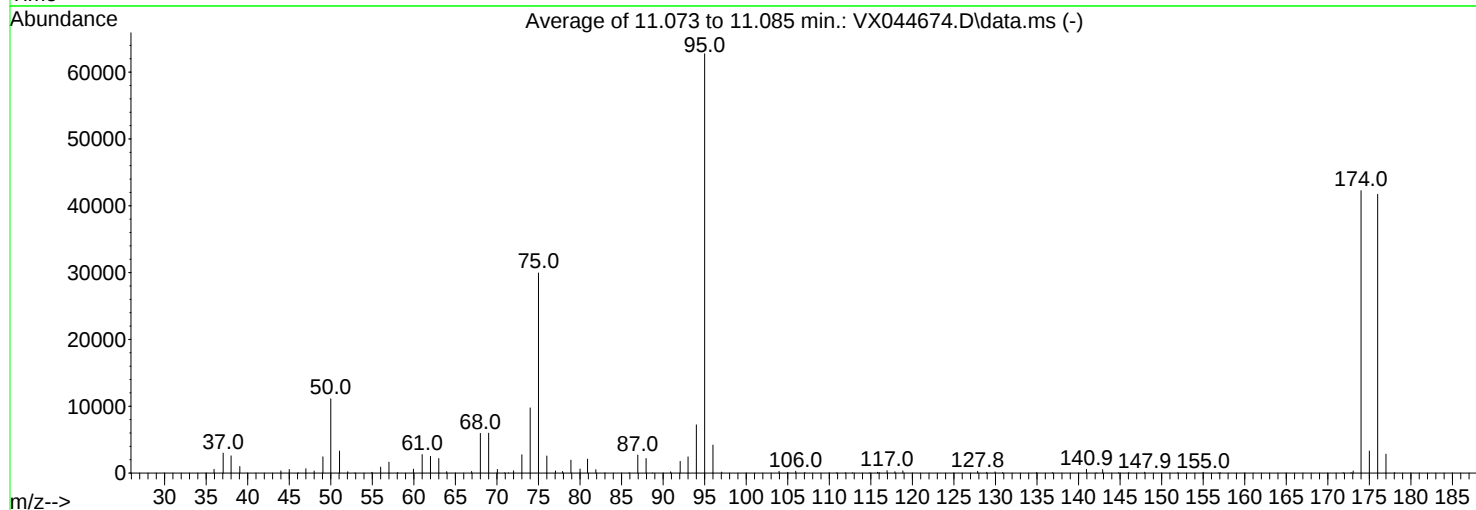


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012125\
Data File : VX044674.D
Acq On : 21 Jan 2025 10:23
Operator : JC/MD
Sample : BFB712
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB712

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM012125WMA.M
Title : VOC Analysis
Last Update : Thu Jan 23 00:51:10 2025

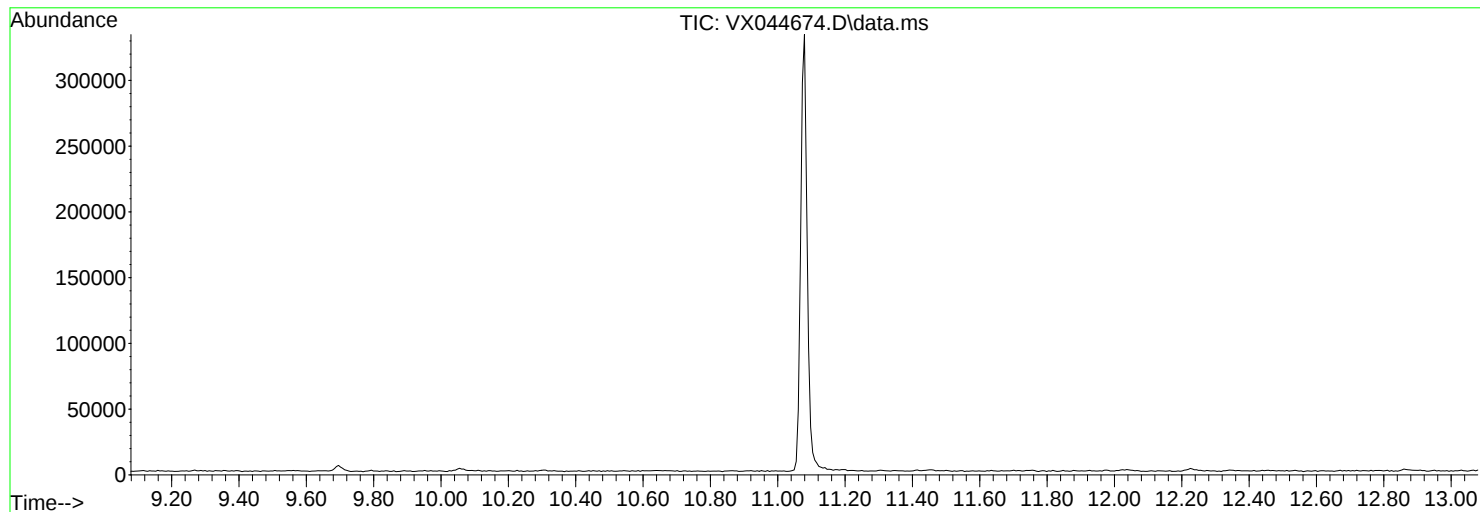

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	11114	PASS
75	95	30	80	47.7	29947	PASS
95	95	100	100	100.0	62755	PASS
96	95	5	9	6.7	4199	PASS
173	174	0.00	2	0.7	310	PASS
174	95	50	120	67.4	42267	PASS
175	174	5	9	7.8	3304	PASS
176	174	95	101	98.7	41720	PASS
177	176	5	9	6.8	2829	PASS

m/z	Abundance
38.10	63.0
39.10	122.0
40.00	1307.0
41.00	242.0
42.10	122.0
43.00	204.0
44.00	542.0
54.90	184.0
56.00	57.0
57.20	95.0
67.20	63.0
69.10	63.0
83.10	66.0
83.90	58.0
91.00	61.0

Instrument :
MSVOA_X
ClientSampleId :
BFB712

m/z	Abundance
36.00	687.0
37.10	3499.0
38.00	3203.0
39.10	1342.0
40.10	1345.0
41.00	170.0
42.00	161.0
43.00	204.0
44.00	1021.0
45.00	697.0
47.00	751.0
48.00	376.0
49.10	3006.0
50.00	13120.0
51.00	3711.0
52.00	292.0
55.00	314.0
56.00	1010.0
57.00	1935.0
58.00	93.0
60.00	604.0
61.00	3192.0
62.00	2993.0
63.00	2438.0
63.90	251.0
67.00	316.0
68.00	6335.0
69.00	6524.0
70.00	658.0
71.40	79.0
72.00	435.0
73.00	3182.0
74.00	10802.0
75.00	32896.0
76.00	2947.0
77.10	341.0
78.10	175.0
78.90	2012.0
80.00	746.0
80.90	2346.0
81.90	586.0
86.90	2972.0
87.90	2499.0
90.90	254.0
92.10	1762.0
93.00	2781.0
94.00	7757.0
95.00	68368.0
96.00	4601.0
97.10	221.0
104.00	243.0
105.00	156.0
105.90	270.0
107.10	83.0
110.00	58.0
110.90	60.0
111.90	75.0
112.80	90.0
115.80	230.0
116.90	354.0
117.90	245.0
118.90	376.0
127.80	218.0
128.90	147.0
130.00	194.0
130.90	92.0
134.90	76.0
136.80	102.0
140.90	604.0
142.90	575.0
146.00	66.0
148.00	114.0
152.00	83.0
155.00	126.0
156.80	96.0
171.90	52.0
173.10	387.0
174.00	39656.0
175.00	3098.0
176.00	39256.0
177.00	2826.0
178.00	116.0

Instrument :
MSVOA_X
ClientSampleId :
BFB712

m/z	Abundance
35.90	647.0
37.00	3531.0
38.00	3002.0
39.00	1227.0
40.00	1275.0
41.00	157.0
42.00	66.0
43.10	189.0
44.10	879.0
45.00	528.0
46.10	81.0
47.00	761.0
48.00	417.0
49.00	2640.0
50.00	12708.0
51.10	3791.0
52.00	170.0
55.00	338.0
56.00	1072.0
57.00	2093.0
58.10	100.0
60.00	688.0
61.00	3086.0
62.00	2952.0
63.00	2499.0
64.00	235.0
66.90	204.0
68.00	7340.0
69.00	7316.0
70.00	561.0
72.00	370.0
73.00	3108.0
74.00	11651.0
75.00	35992.0
76.00	2728.0
77.00	403.0
77.90	300.0
78.90	2387.0
80.00	692.0
80.90	2426.0
81.90	693.0
83.10	127.0
86.00	71.0
87.00	3352.0
88.00	2572.0
90.90	333.0
92.00	2186.0
93.00	2791.0
94.00	8629.0
95.00	73760.0
96.00	5059.0
97.10	122.0
104.00	292.0
105.00	67.0
106.00	367.0
107.00	106.0
110.90	116.0
112.00	64.0
112.80	74.0
114.80	50.0
116.00	282.0
116.90	444.0
117.90	274.0
118.80	362.0
127.80	324.0
129.00	106.0
130.00	185.0
130.80	80.0
134.90	80.0
136.90	130.0
140.90	613.0
143.00	647.0
144.80	86.0
146.00	92.0
147.90	188.0
151.90	62.0
155.00	140.0
157.00	95.0
171.80	92.0
173.00	542.0
174.00	51336.0
175.00	4128.0
176.00	49848.0
177.00	3243.0

Instrument :
MSVOA_X
ClientSampleId :
BFB712

m/z	Abundance
36.00	351.0
37.00	1956.0
38.00	1711.0
39.10	748.0
40.00	1172.0
41.10	109.0
41.80	85.0
43.10	118.0
44.00	720.0
45.10	402.0
47.10	444.0
47.90	148.0
49.00	1660.0
50.00	7515.0
51.00	2389.0
52.10	156.0
52.90	54.0
55.00	244.0
56.00	798.0
57.00	1164.0
58.10	57.0
59.90	486.0
61.00	2028.0
61.90	1555.0
63.00	1603.0
64.00	178.0
67.00	215.0
68.00	4155.0
69.00	4260.0
70.10	417.0
70.90	69.0
72.00	243.0
73.00	1942.0
74.00	6822.0
75.00	20952.0
76.00	1996.0
77.00	237.0
77.80	234.0
78.90	1412.0
79.90	398.0
80.90	1475.0
81.90	277.0
82.90	91.0
85.80	59.0
87.00	1757.0
88.00	1485.0
88.70	106.0
90.90	173.0
92.00	1324.0
93.00	1712.0
94.00	5262.0
95.00	46136.0
96.00	2938.0
97.00	120.0
103.80	283.0
105.00	128.0
106.00	191.0
107.00	58.0
115.80	134.0
117.00	333.0
117.80	122.0
118.80	277.0
127.90	237.0
129.00	118.0
129.80	193.0
130.90	61.0
135.00	108.0
141.00	473.0
142.20	75.0
142.80	362.0
144.80	87.0
146.10	70.0
148.00	127.0
155.00	109.0
157.10	85.0
171.80	64.0
172.80	244.0
174.00	35808.0
175.00	2685.0
176.00	36056.0
177.00	2418.0
178.10	64.0

Instrument :
MSVOA_X
ClientSampleId :
BFB712