

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012219\
 Data File : VX007175.D
 Acq On : 22 Jan 2019 12:23
 Operator : JC/SP
 Sample : K1215-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB04-20190117

Quant Time: Jan 23 00:42:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 08 14:06:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	585459	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	896223	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	839138	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	410284	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	311064	50.84	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.68%	
35) Dibromofluoromethane	5.50	113	278823	48.58	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.16%	
50) Toluene-d8	8.71	98	1065076	50.70	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.40%	
62) 4-Bromofluorobenzene	11.13	95	378880	51.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.46%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012219\
Data File : VX007175.D
Acq On : 22 Jan 2019 12:23
Operator : JC/SP
Sample : K1215-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB04-20190117

Quant Time: Jan 23 00:42:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 08 14:06:59 2019
Response via : Initial Calibration

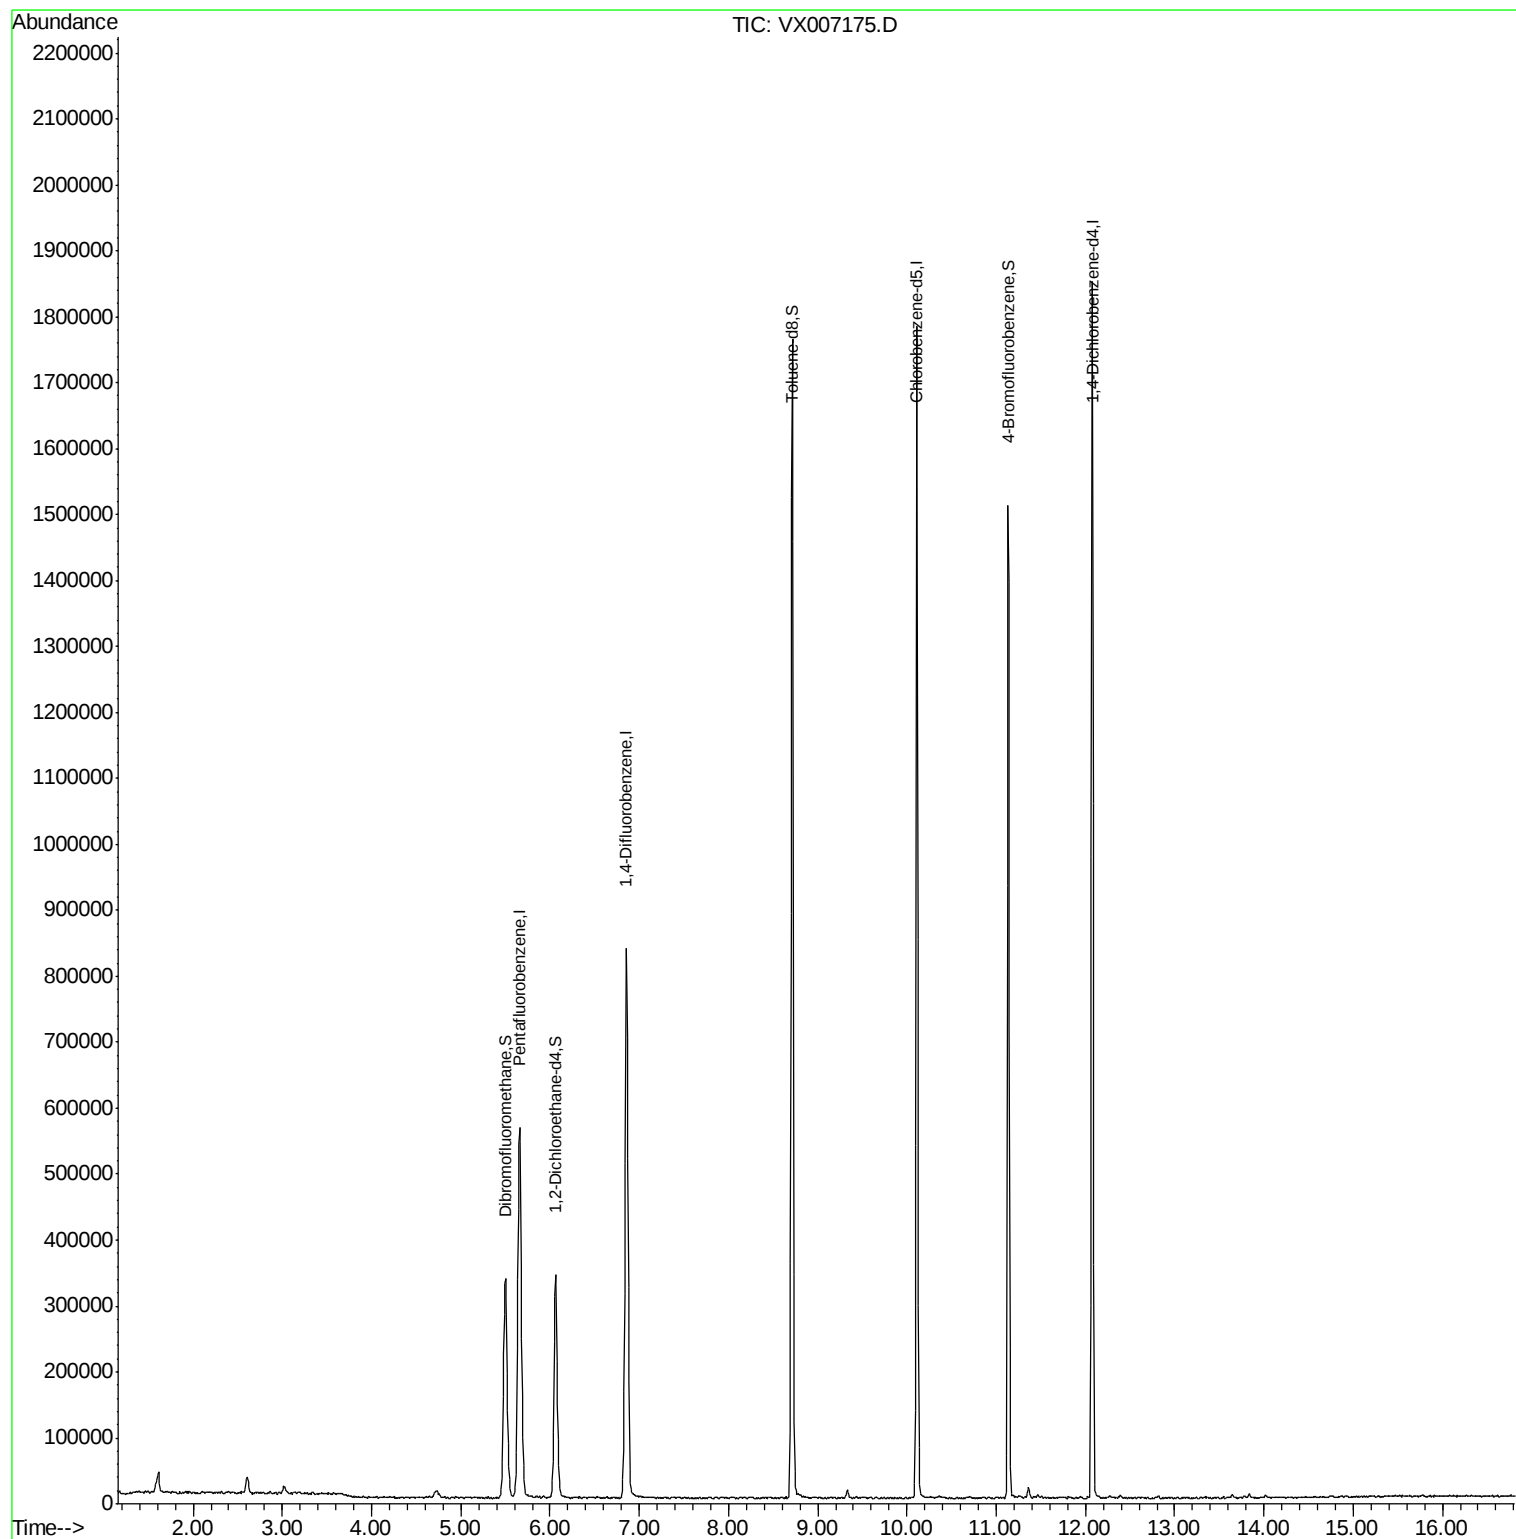

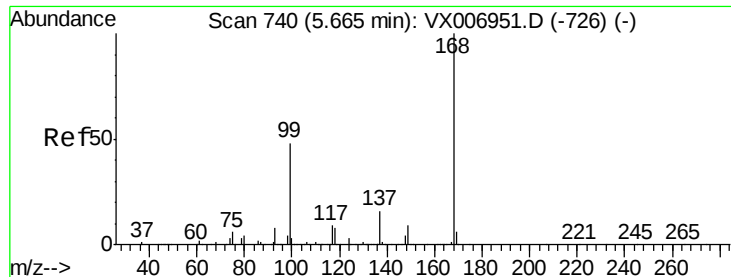

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.01 min

Lab File: VX007175.D

Acq: 22 Jan 2019 12:23

Instrument :

MSVOA_X

ClientSampleId :


EB04-20190117

Tot Ion:168 Resp: 585459

Ion Ratio Lower Upper

168 100

99 50.1 41.8 62.8

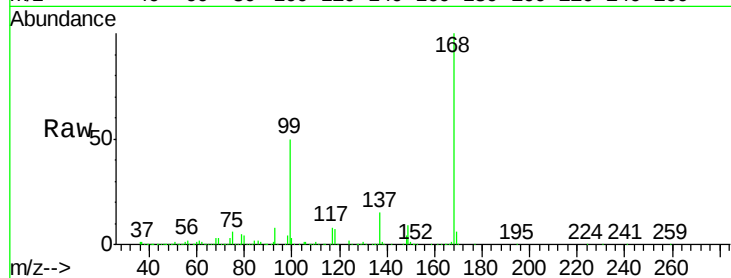

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

200000



150000

100000

50000

0

Time--> 5.50 5.60 5.70 5.80

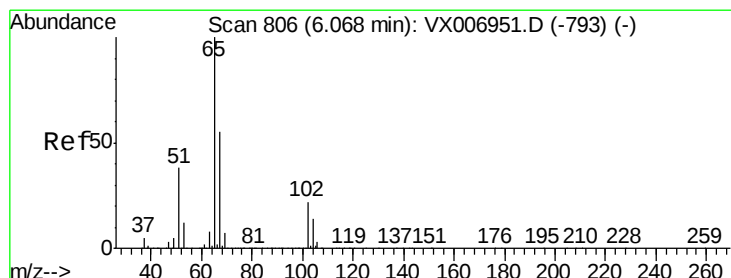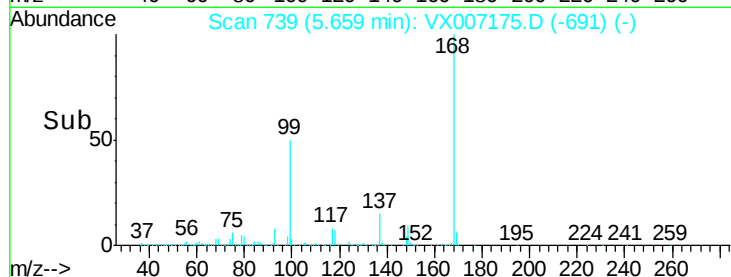

#33

1,2-Dichloroethane-d4

Concen: 50.840 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.01 min

Lab File: VX007175.D


Acq: 22 Jan 2019 12:23

Tgt Ion: 65 Resp: 311064

Ion Ratio Lower Upper

65 100

67 52.9 0.0 105.0

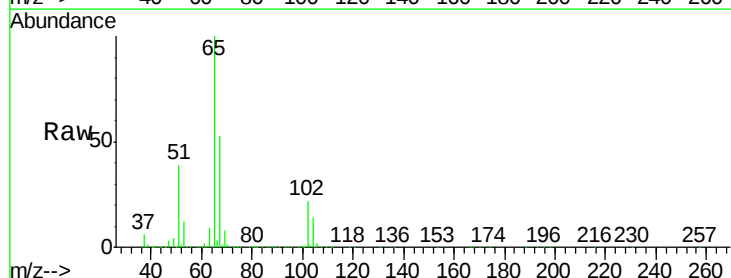

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0


6.06


100000

50000

0

Time--> 5.90 6.00 6.10 6.20

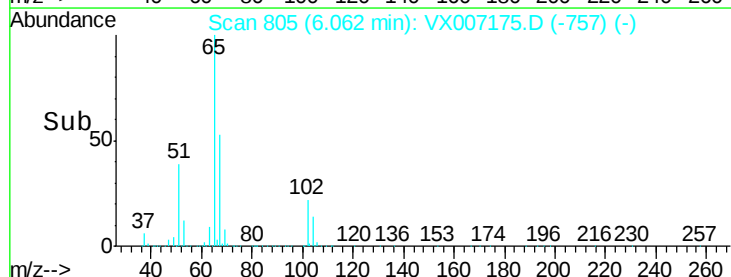

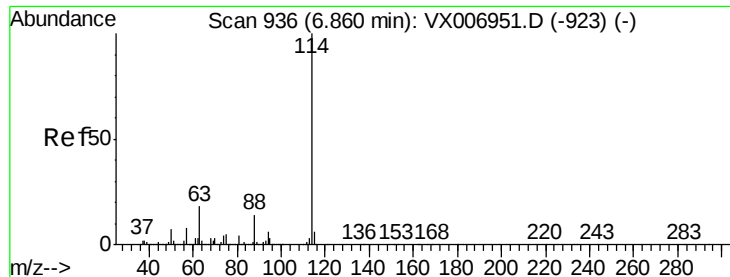

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX007175.D

Acq: 22 Jan 2019 12:23

Instrument :

MSVOA_X

ClientSampleId :

EB04-20190117


Tot Ion:114 Resp: 896223

Ion Ratio Lower Upper

114 100

63 17.8 0.0 34.8




88 14.3 0.0 28.8

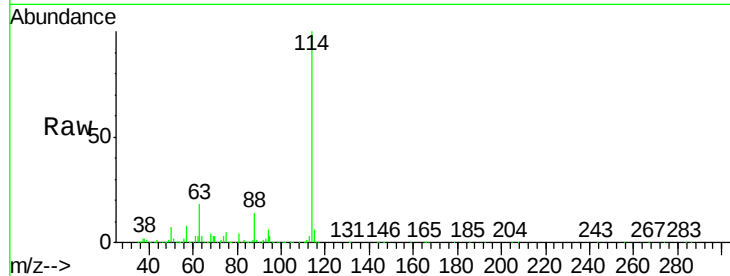

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

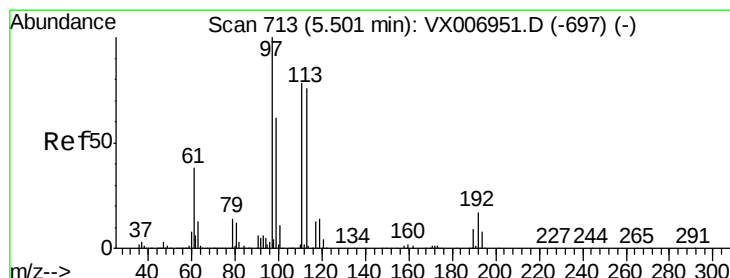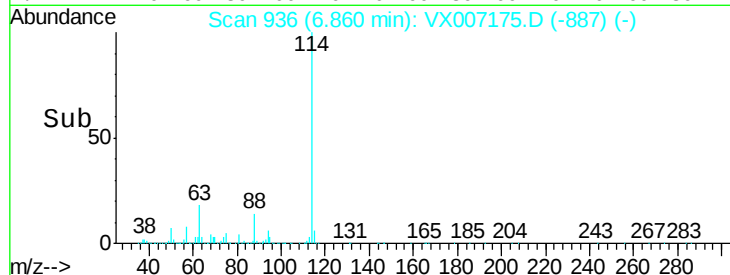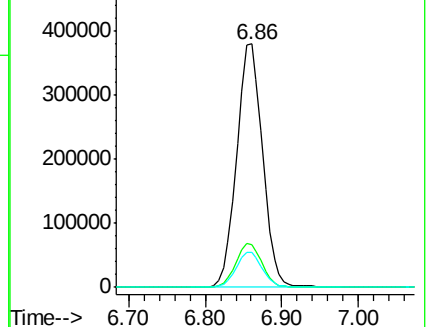

#35

Dibromofluoromethane

Concen: 48.581 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX007175.D

Acq: 22 Jan 2019 12:23


Tgt Ion:113 Resp: 278823

Ion Ratio Lower Upper

113 100

111 102.5 81.6 122.4



192 22.8 16.7 25.1

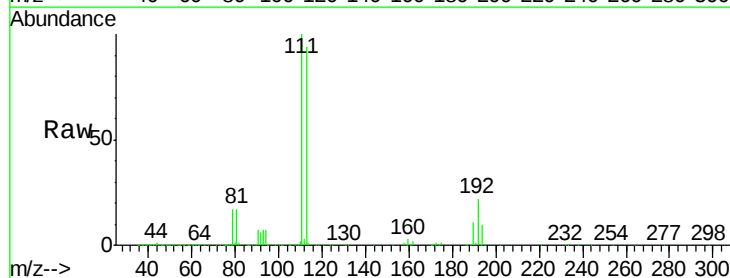


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

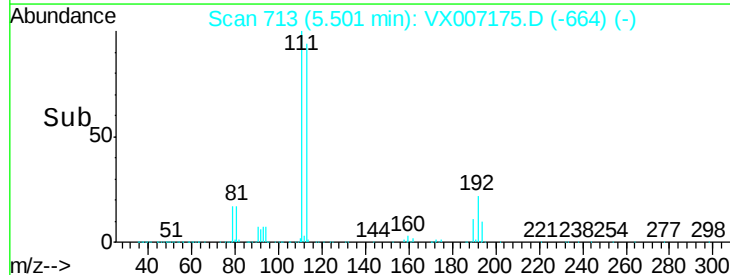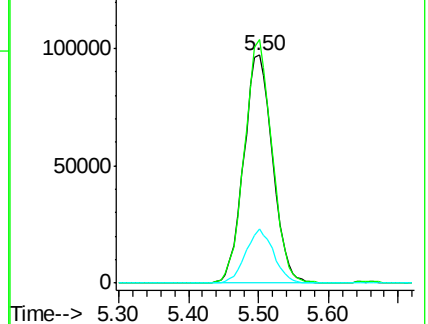

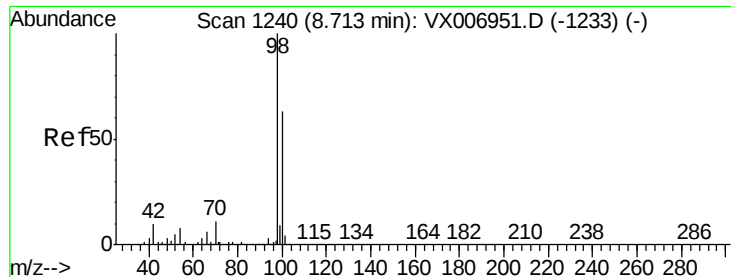

#50

Toluene-d8

Concen: 50.699 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX007175.D

Acq: 22 Jan 2019 12:23

Instrument :

MSVOA_X

ClientSampleId :





EB04-20190117

Tot Ion: 98 Resp: 1065076

Ion Ratio Lower Upper

98 100

100 64.2 52.0 78.0

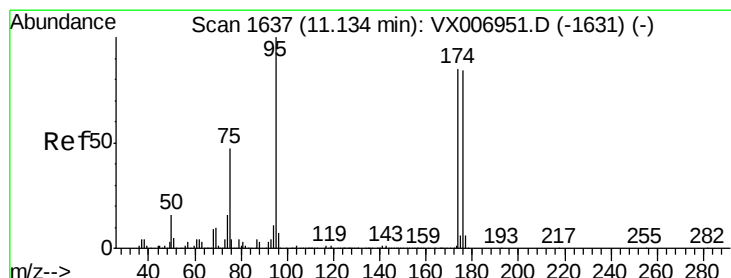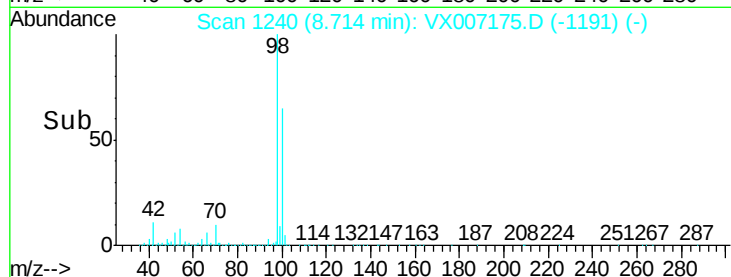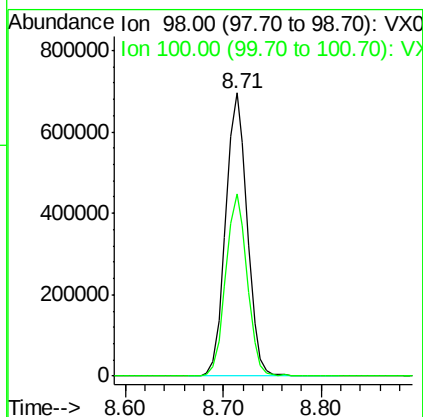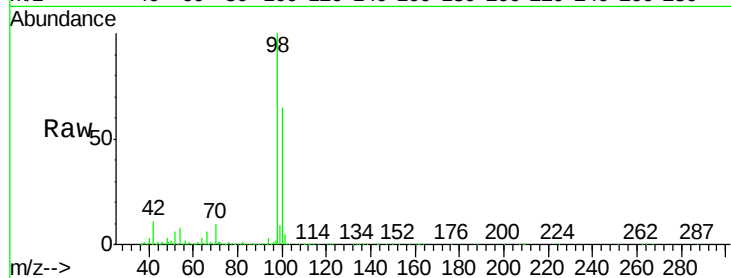

#62

4-Bromofluorobenzene

Concen: 51.732 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX007175.D

Acq: 22 Jan 2019 12:23




Tgt Ion: 95 Resp: 378880


Ion Ratio Lower Upper

95 100

174 93.3 0.0 182.2

176 90.7 0.0 178.8


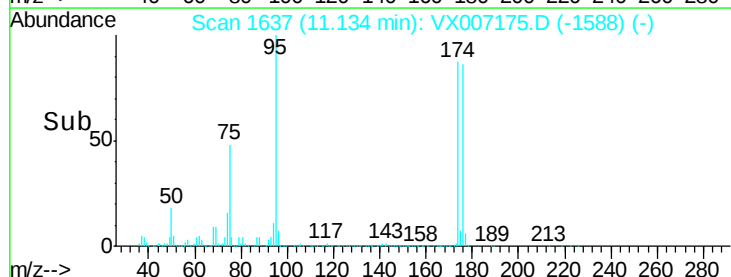
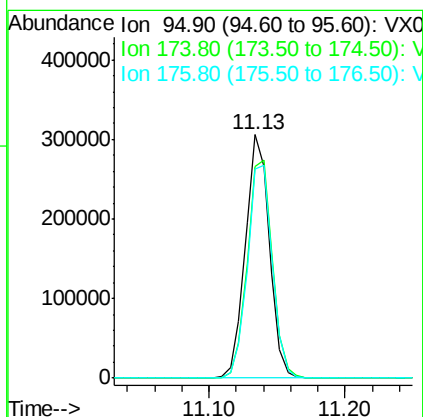
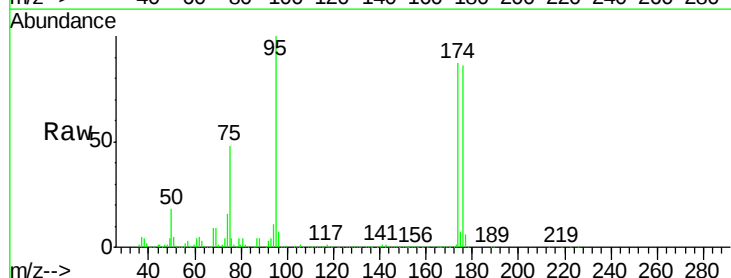


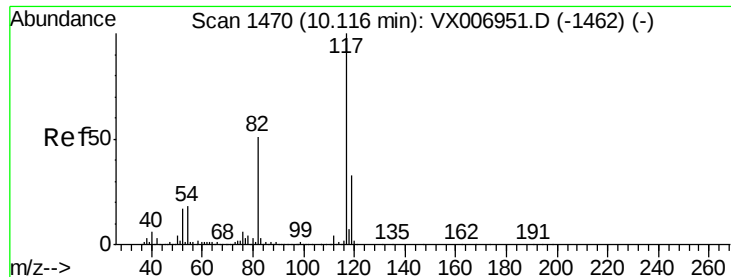

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.11 min Scan# 1469
 Delta R.T. -0.01 min
 Lab File: VX007175.D
 Acq: 22 Jan 2019 12:23

Instrument :
 MSVOA_X
 ClientSampleId :
 EB04-20190117

Tot Ion	Ratio	Lower	Upper
117	100		
82	50.0	41.0	61.6
119	32.1	25.4	38.0

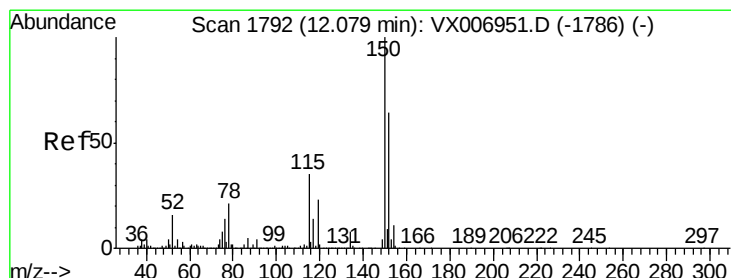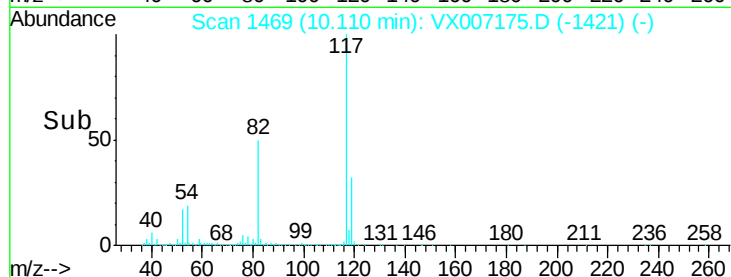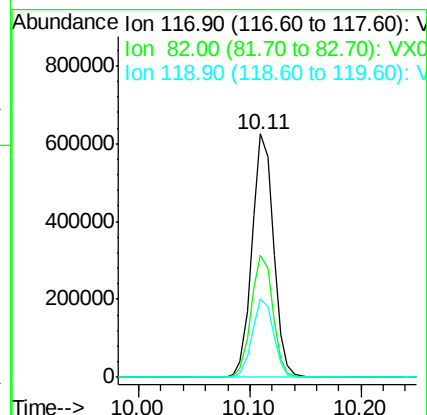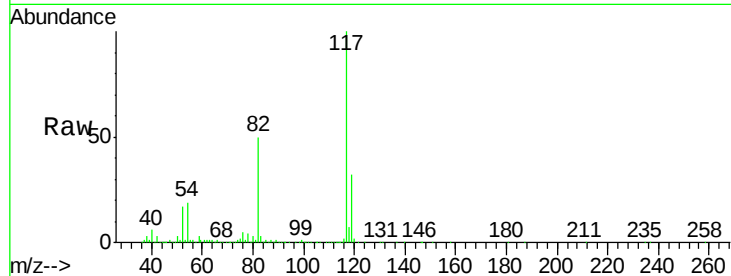

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.08 min Scan# 1792
 Delta R.T. 0.00 min
 Lab File: VX007175.D
 Acq: 22 Jan 2019 12:23

Tgt Ion	Ratio	Lower	Upper
152	100		
115	55.0	39.1	117.2
150	157.1	0.0	344.8

