

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012219\  
 Data File : VX007188.D  
 Acq On : 22 Jan 2019 18:08  
 Operator : JC/SP  
 Sample : K1214-11  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SA-TW531-2327

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.282       | 16            | 21          | 26           | rBV3     | 23054          | 42126         | 1.71%           | 0.314%        |
| 2         | 1.623       | 66            | 77          | 81           | rVB3     | 31097          | 73378         | 2.98%           | 0.546%        |
| 3         | 2.617       | 234           | 240         | 247          | rVB      | 40770          | 75328         | 3.06%           | 0.561%        |
| 4         | 5.507       | 702           | 714         | 726          | rBV      | 290259         | 825623        | 33.50%          | 6.148%        |
| 5         | 5.665       | 728           | 740         | 755          | rVV      | 491207         | 1381618       | 56.05%          | 10.289%       |
| 6         | 6.068       | 796           | 806         | 817          | rBV      | 299305         | 781754        | 31.72%          | 5.822%        |
| 7         | 6.860       | 924           | 936         | 948          | rBV      | 743068         | 1744145       | 70.76%          | 12.989%       |
| 8         | 8.713       | 1232          | 1240        | 1250         | rBV      | 1624806        | 2464776       | 100.00%         | 18.355%       |
| 9         | 10.110      | 1463          | 1469        | 1479         | rBV      | 1548531        | 2154884       | 87.43%          | 16.047%       |
| 10        | 11.134      | 1632          | 1637        | 1648         | rBV      | 1356178        | 1730884       | 70.22%          | 12.890%       |
| 11        | 12.079      | 1786          | 1792        | 1801         | rBV      | 1701290        | 2153823       | 87.38%          | 16.039%       |


Sum of corrected areas: 13428339

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012219\  
Data File : VX007188.D  
Acq On : 22 Jan 2019 18:08  
Operator : JC/SP  
Sample : K1214-11  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW531-2327

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

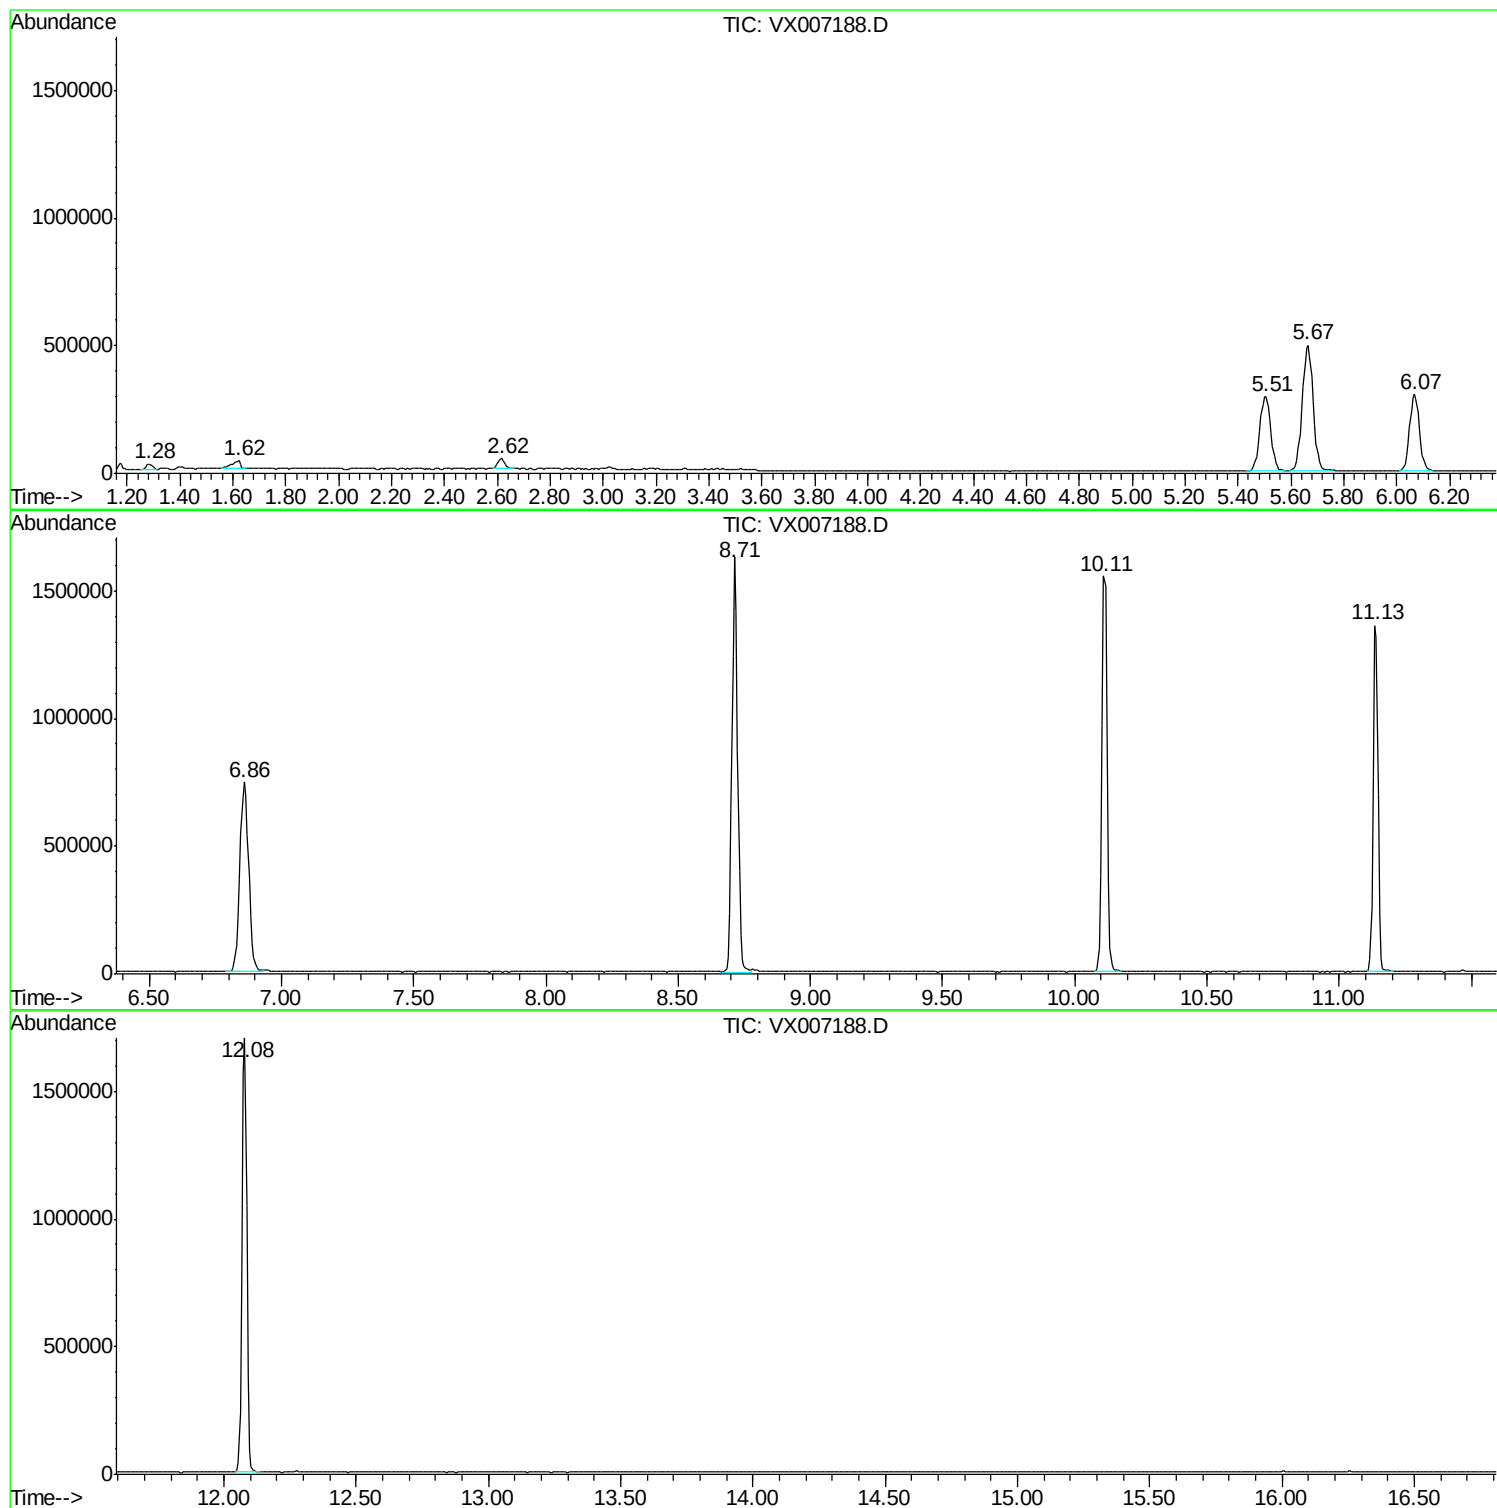

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX012219\  
Data File : VX007188.D  
Acq On : 22 Jan 2019 18:08  
Operator : JC/SP  
Sample : K1214-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW531-2327

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX012219\  
Data File : VX007188.D  
Acq On : 22 Jan 2019 18:08  
Operator : JC/SP  
Sample : K1214-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW531-2327

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |