




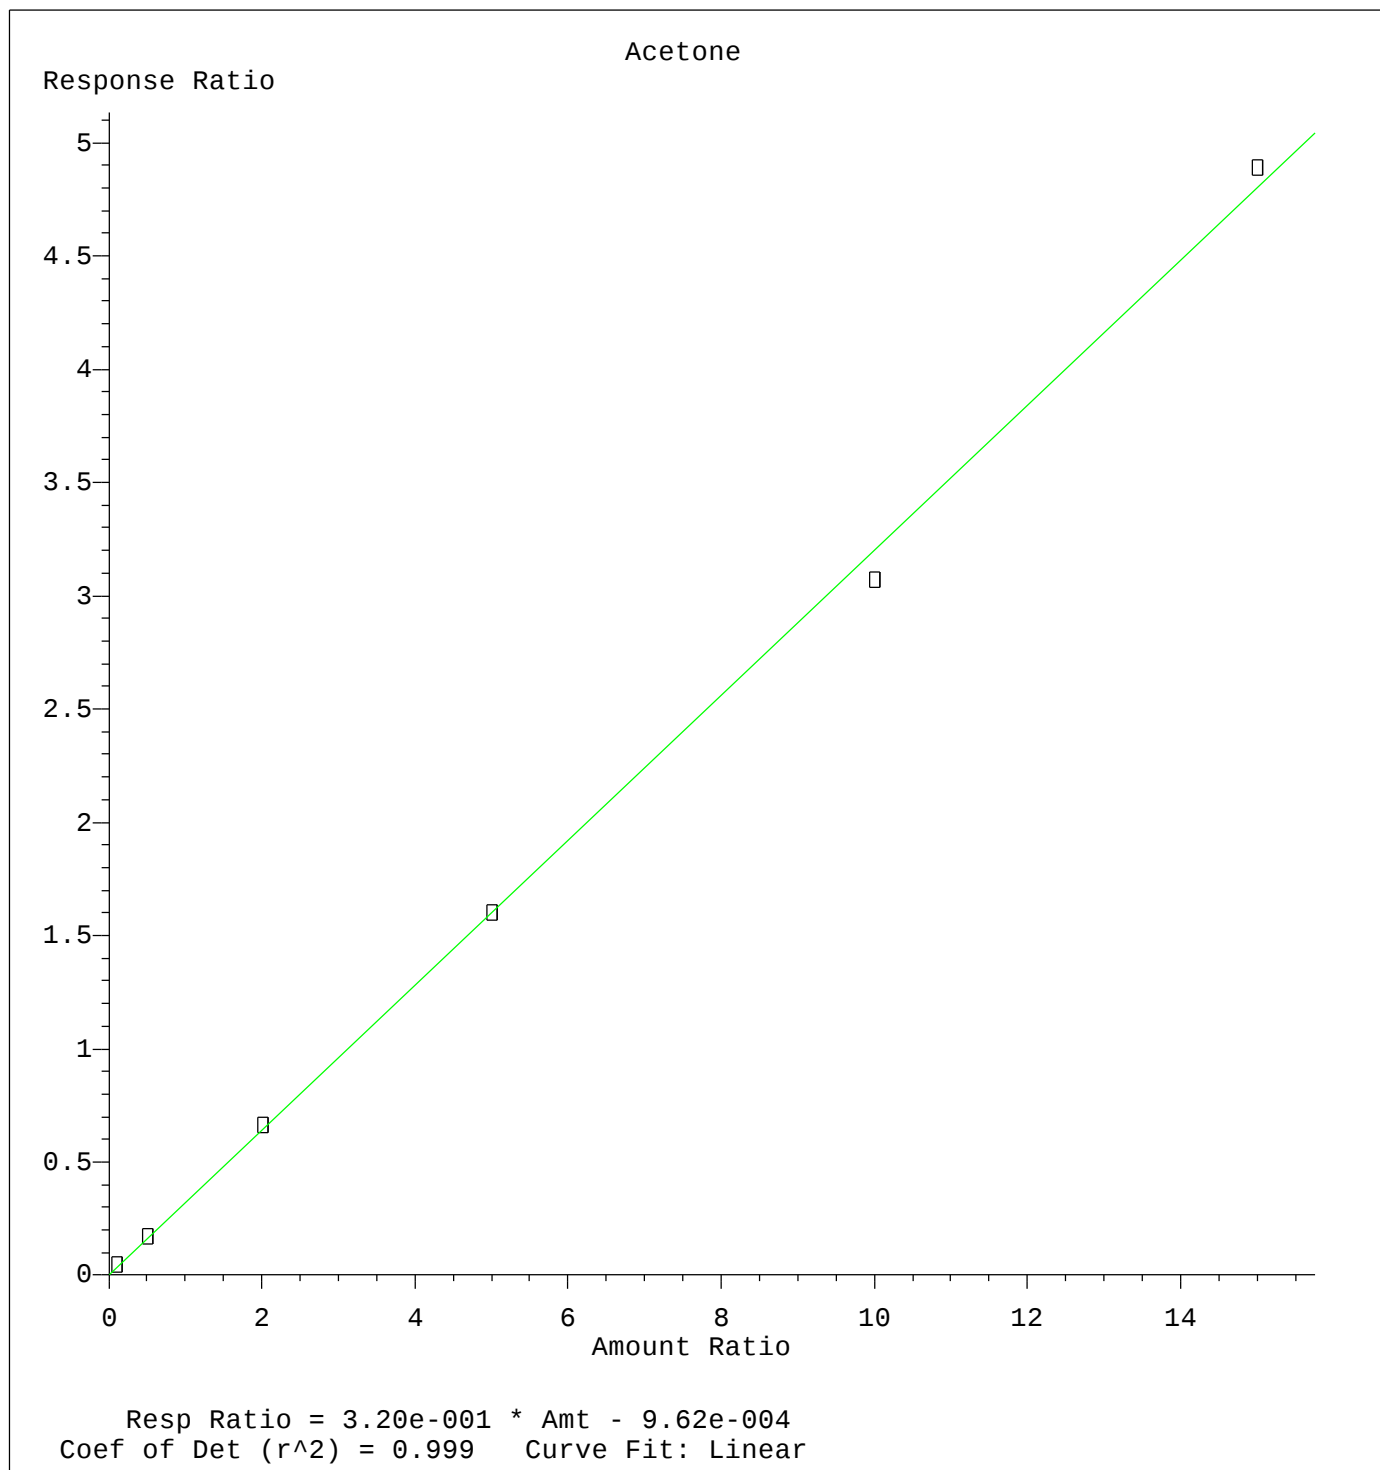

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Calibration Table Last Updated: Wed Jan 22 12:35:15 2020

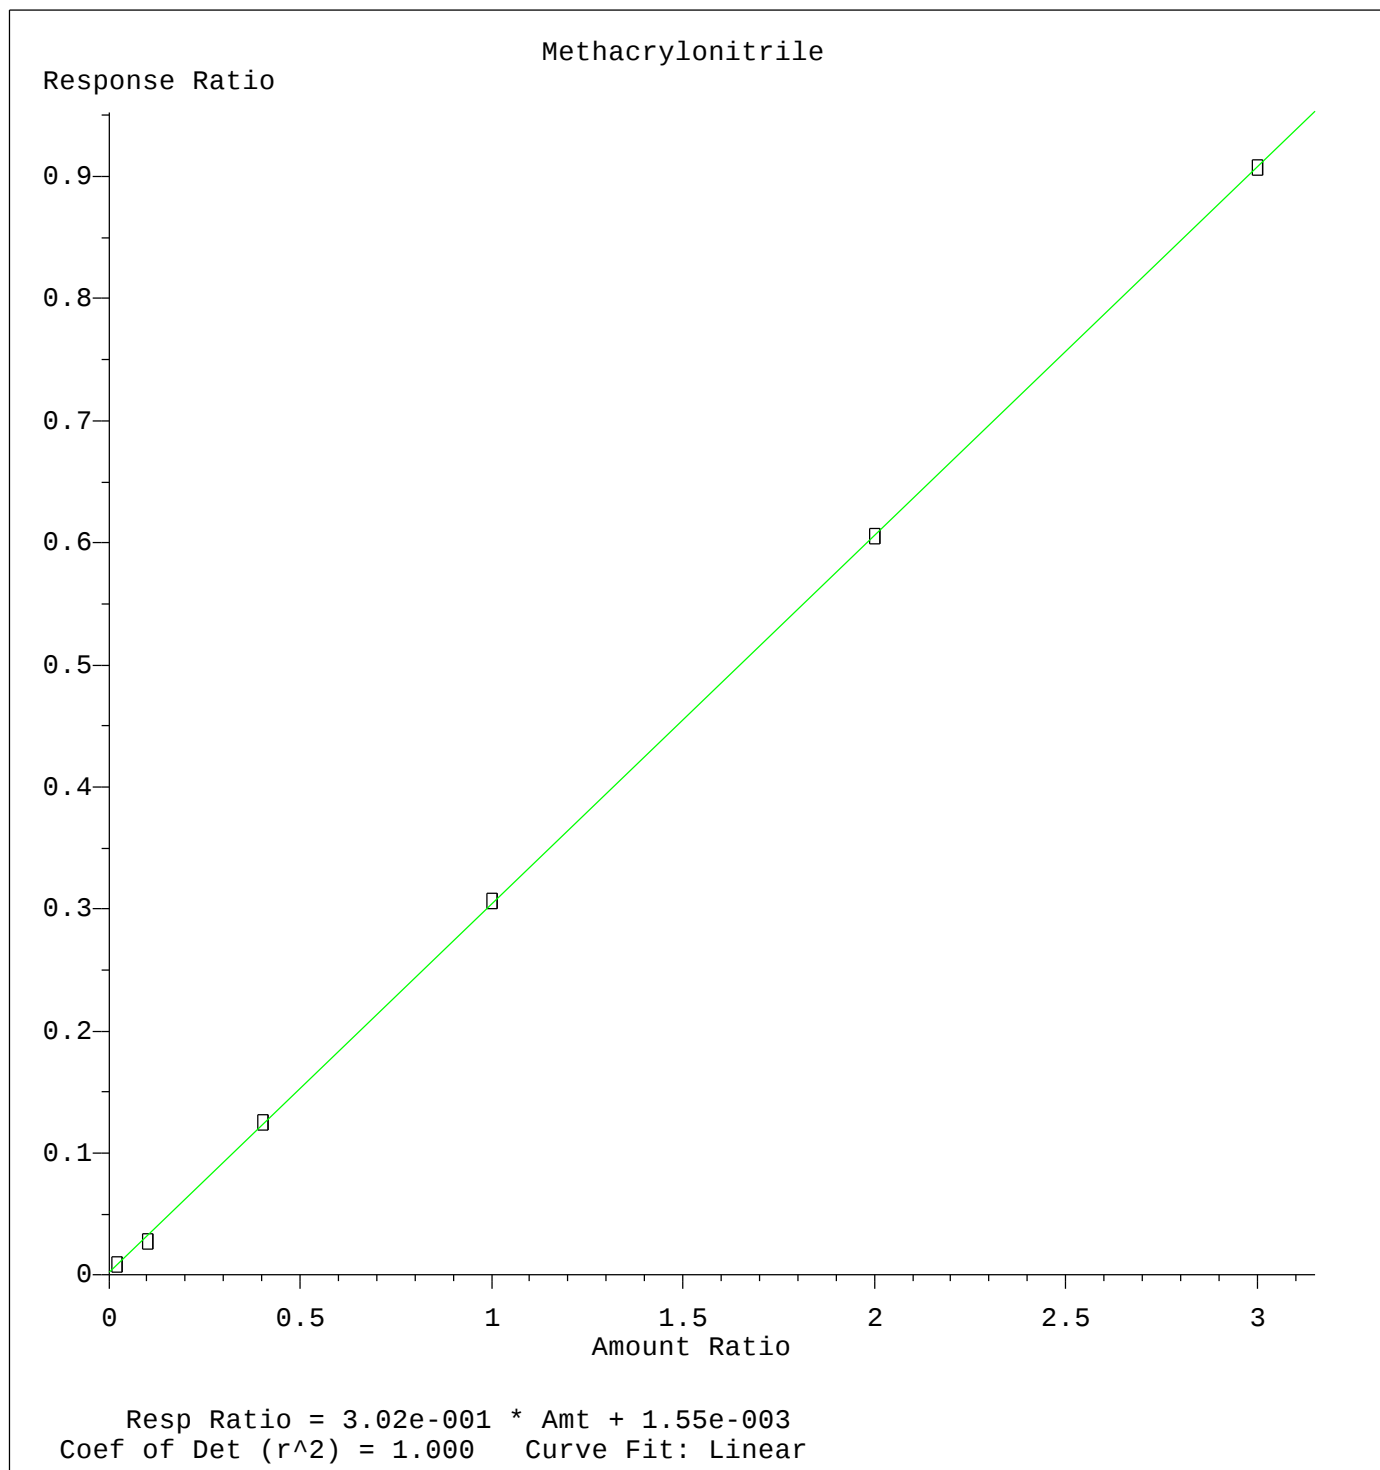


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Calibration Table Last Updated: Wed Jan 22 12:35:15 2020

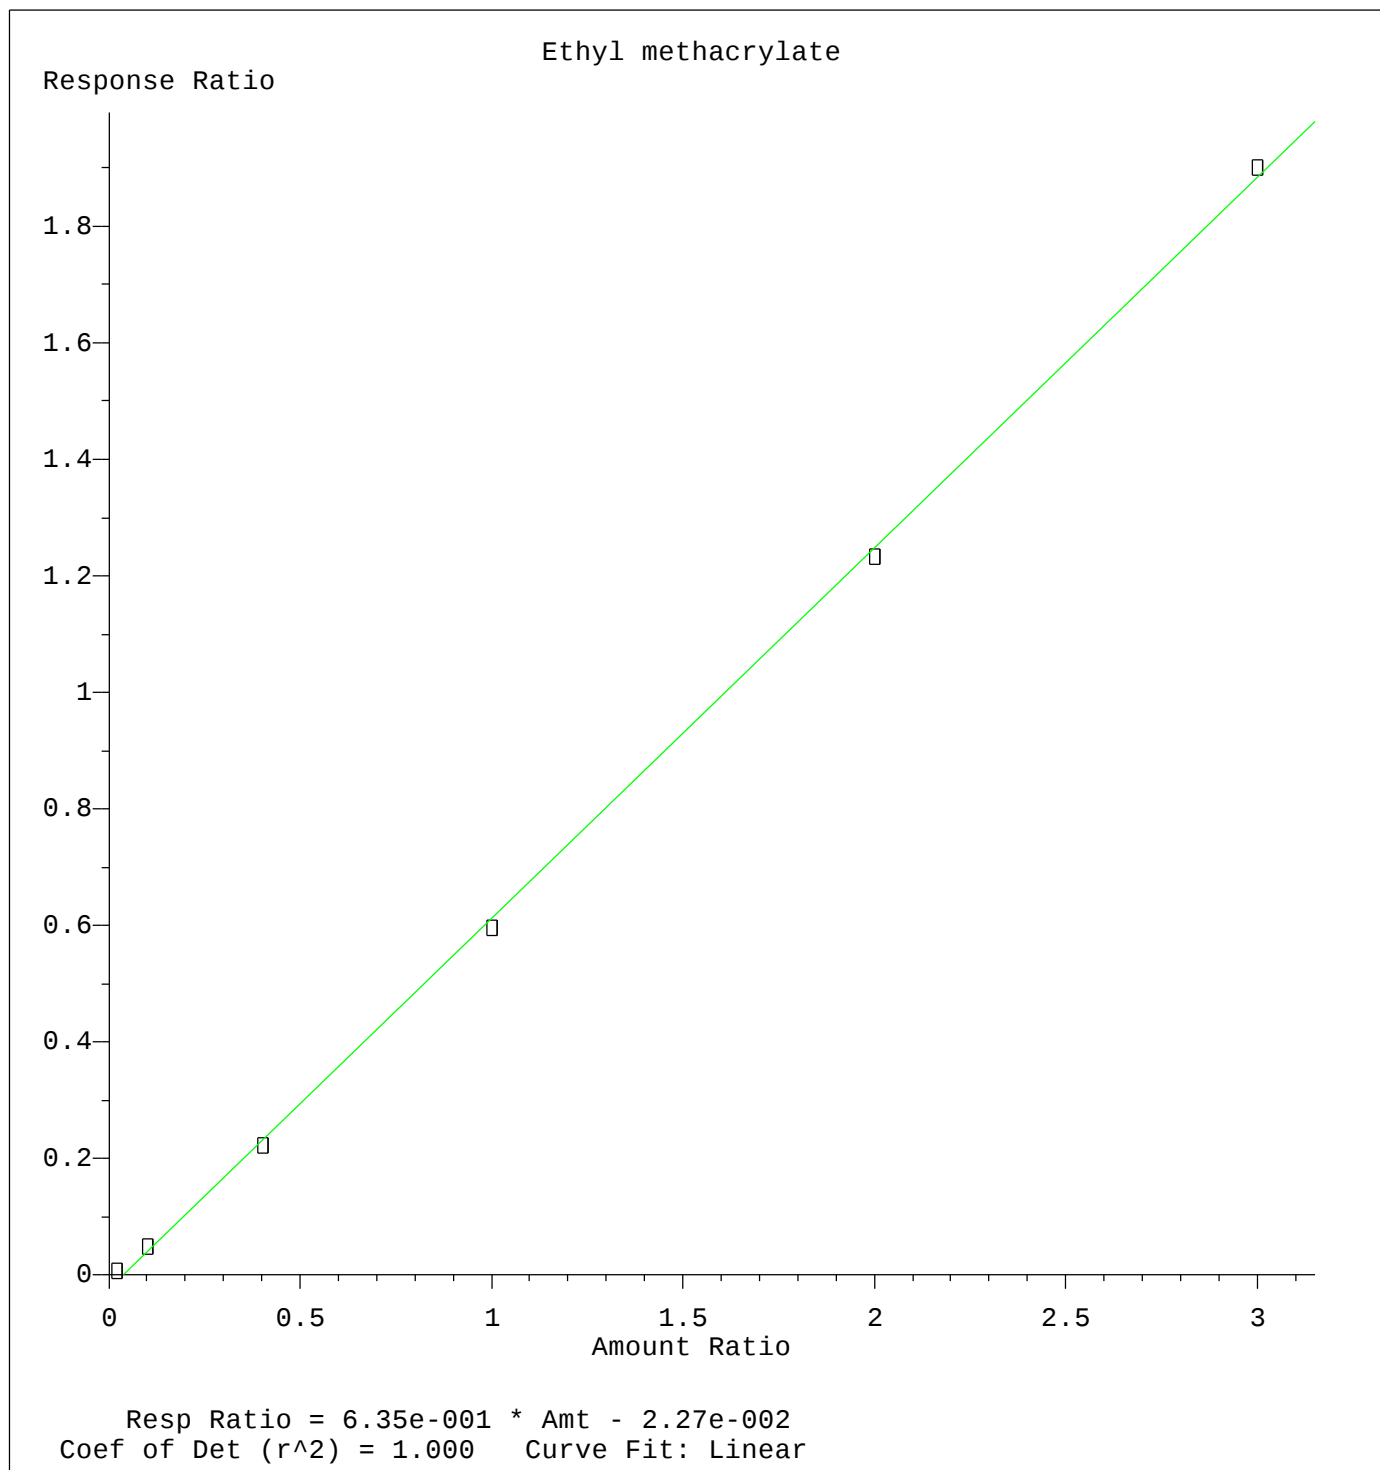

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Calibration Table Last Updated: Wed Jan 22 12:35:15 2020

Naphthalene

Response Ratio

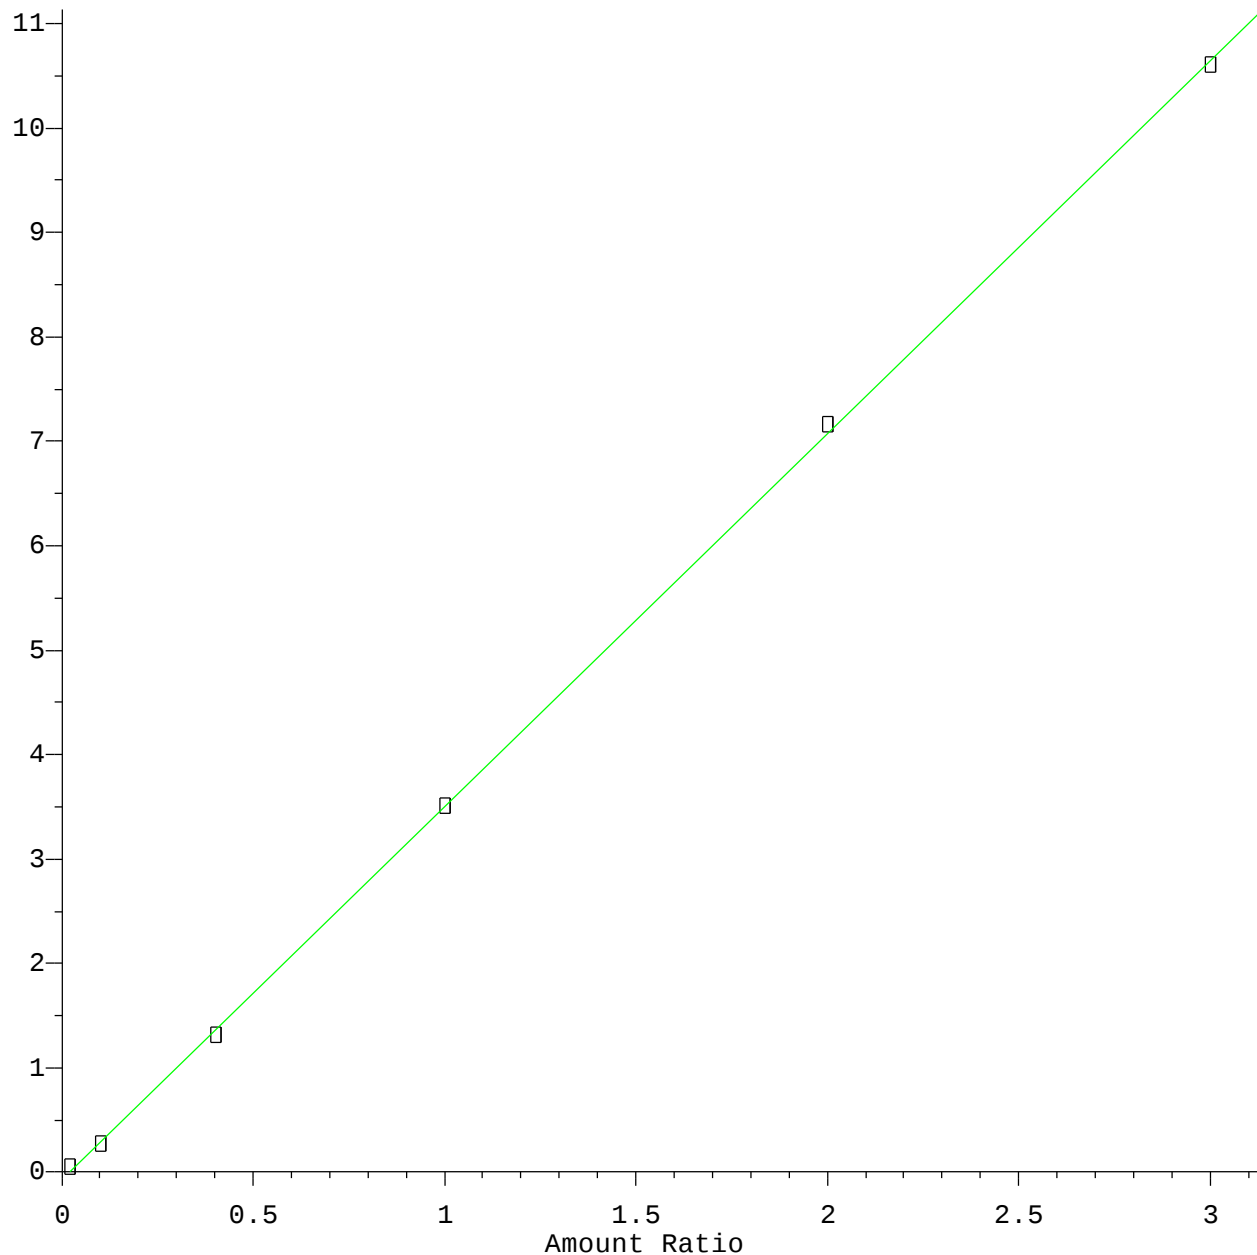


Resp Ratio = 3.57e+000 * Amt - 6.65e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Calibration Table Last Updated: Wed Jan 22 12:35:15 2020

Dichlorodifluoromethane

Response Ratio

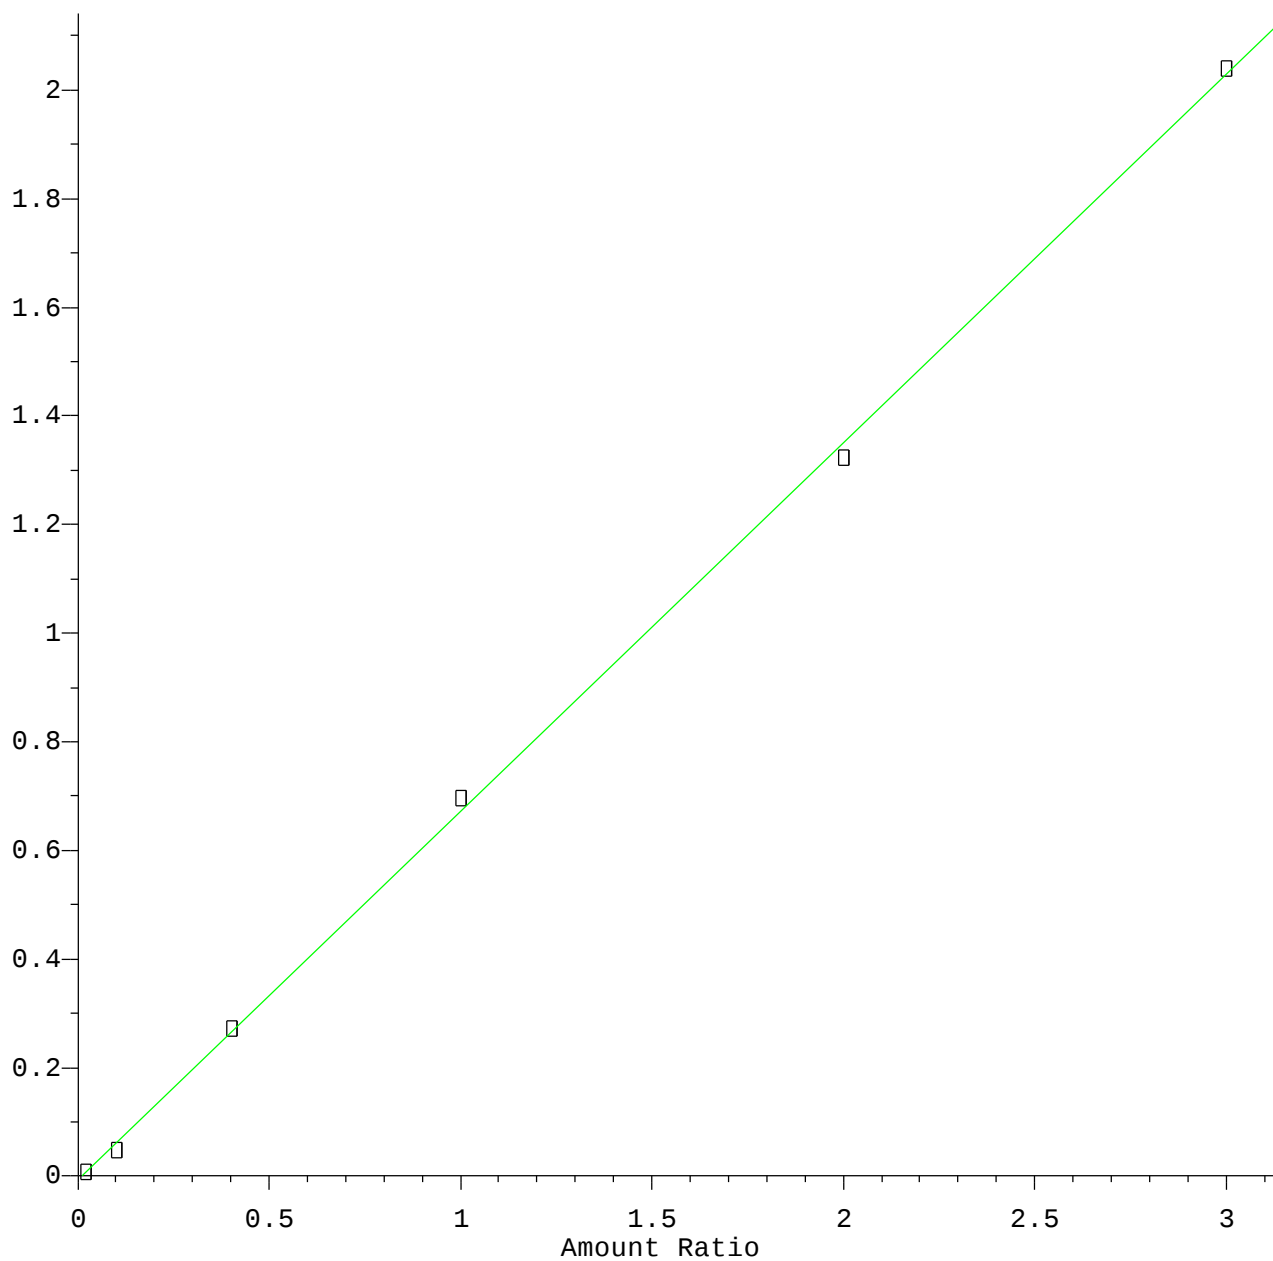


Resp Ratio = $6.78 \times 10^{-1} \times \text{Amt} - 7.21 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Calibration Table Last Updated: Wed Jan 22 12:35:15 2020

Chloroethane

Response Ratio

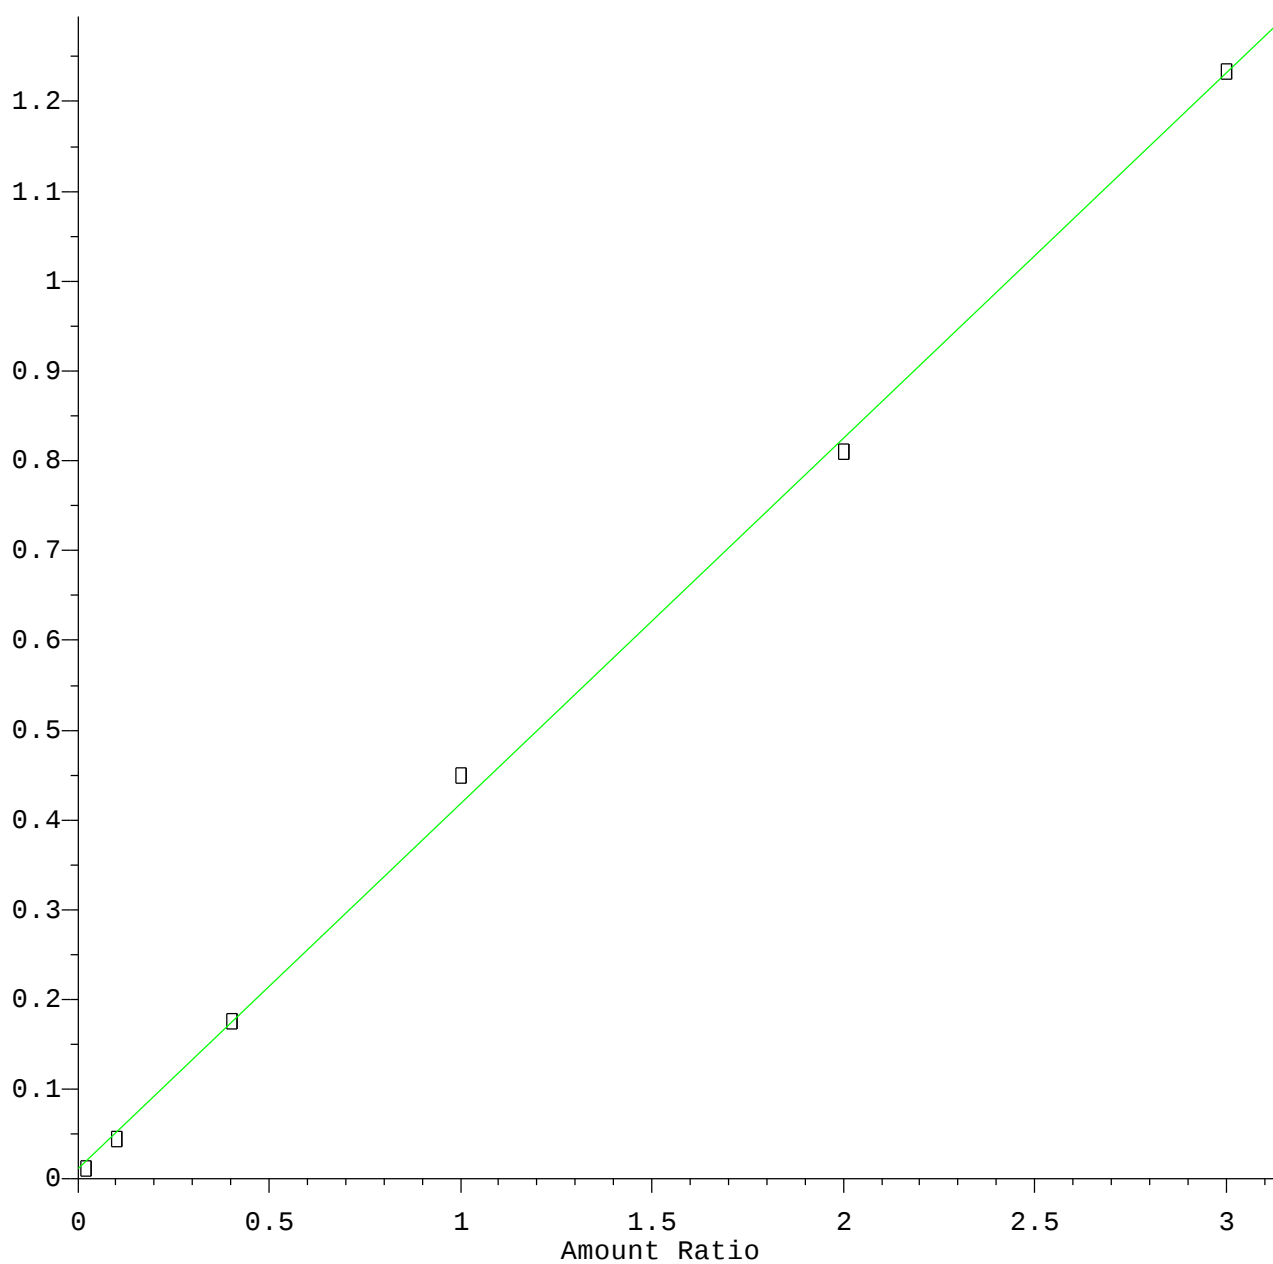

Resp Ratio = $4.07 \times 10^{-1} \times \text{Amt} + 1.16 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Calibration Table Last Updated: Wed Jan 22 12:35:15 2020