


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX012220\
 Data File : VX014679.D
 Acq On : 22 Jan 2020 09:48
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
 Title : SW846 8260
 Last Update : Wed Jan 22 12:35:15 2020

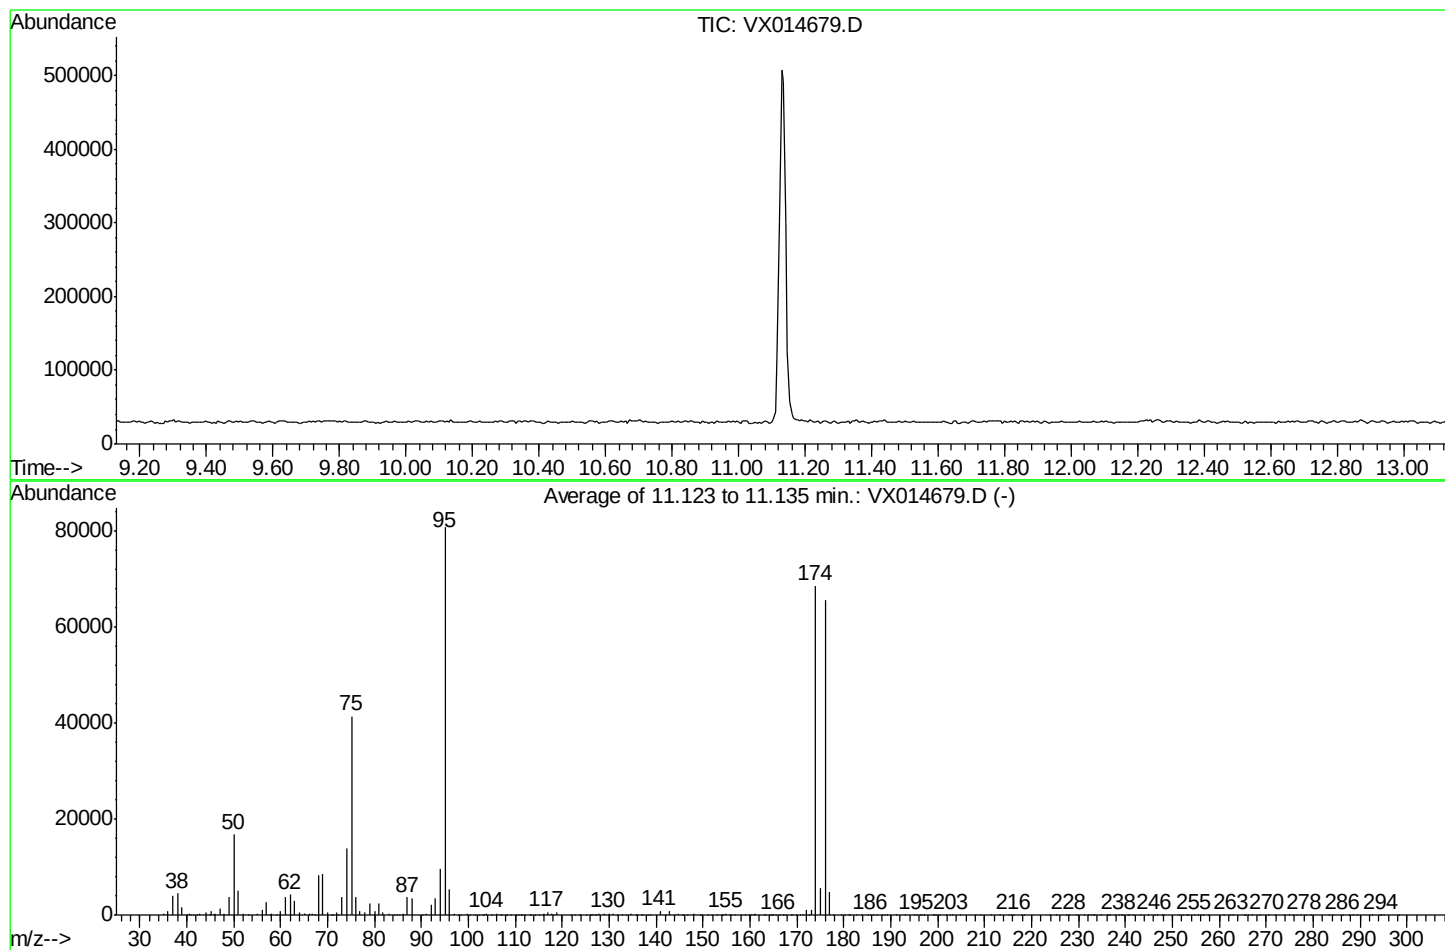

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1671

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	16761	PASS
75	95	30	60	51.2	41351	PASS
95	95	100	100	100.0	80690	PASS
96	95	5	9	6.5	5272	PASS
173	174	0.00	2	1.6	1082	PASS
174	95	50	100	84.9	68472	PASS
175	174	5	9	8.0	5502	PASS
176	174	95	101	95.8	65573	PASS
177	176	5	9	7.2	4704	PASS