


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012221\
 Data File : VX020705.D
 Acq On : 22 Jan 2021 10:10
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011921W.M
 Title : SW846 8260
 Last Update : Tue Jan 19 14:09:08 2021

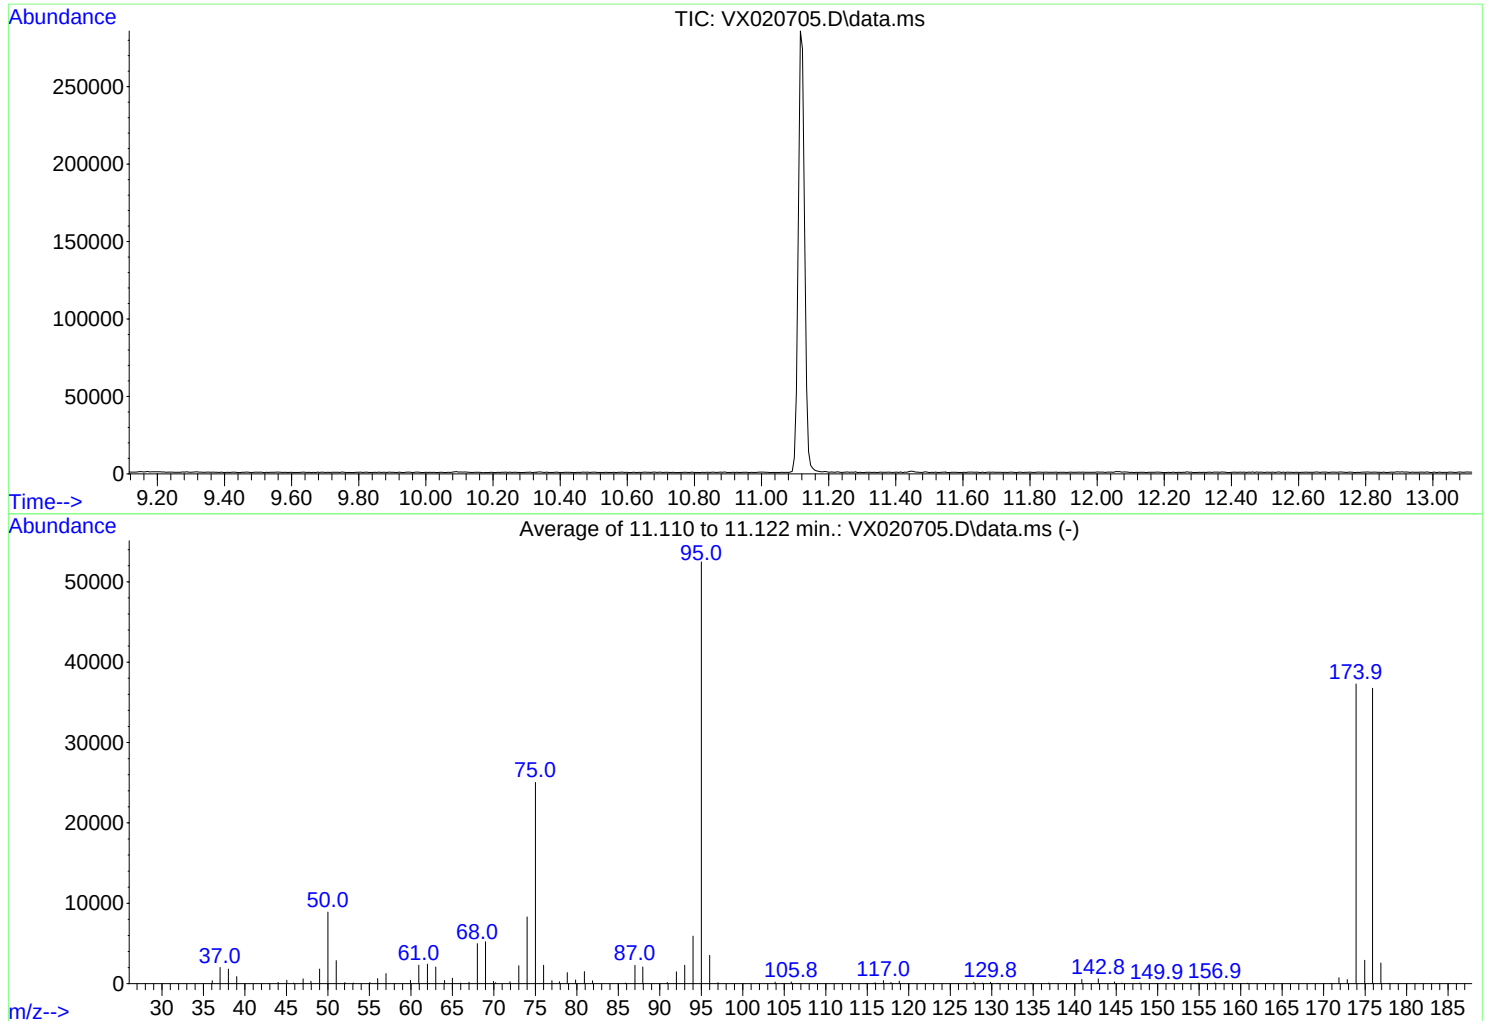

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	8902	PASS
75	95	30	60	47.7	25048	PASS
95	95	100	100	100.0	52485	PASS
96	95	5	9	6.7	3523	PASS
173	174	0.00	2	1.4	507	PASS
174	95	50	100	71.1	37299	PASS
175	174	5	9	7.8	2915	PASS
176	174	95	101	98.6	36763	PASS
177	176	5	9	7.0	2570	PASS