

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012224\
 Data File : VX039890.D
 Acq On : 22 Jan 2024 17:38
 Operator : JC/MD
 Sample : P1215-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-195-TB-20240117

Quant Time: Jan 23 00:20:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 03:51:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	77102	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	143016	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	135729	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	63938	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	61662	47.742	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	95.480%
35) Dibromofluoromethane	5.385	113	47765	49.586	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.180%
50) Toluene-d8	8.647	98	173310	47.704	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.400%
62) 4-Bromofluorobenzene	11.079	95	67484	47.501	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012224\
Data File : VX039890.D
Acq On : 22 Jan 2024 17:38
Operator : JC/MD
Sample : P1215-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-195-TB-20240117


Quant Time: Jan 23 00:20:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 03:51:26 2024
Response via : Initial Calibration

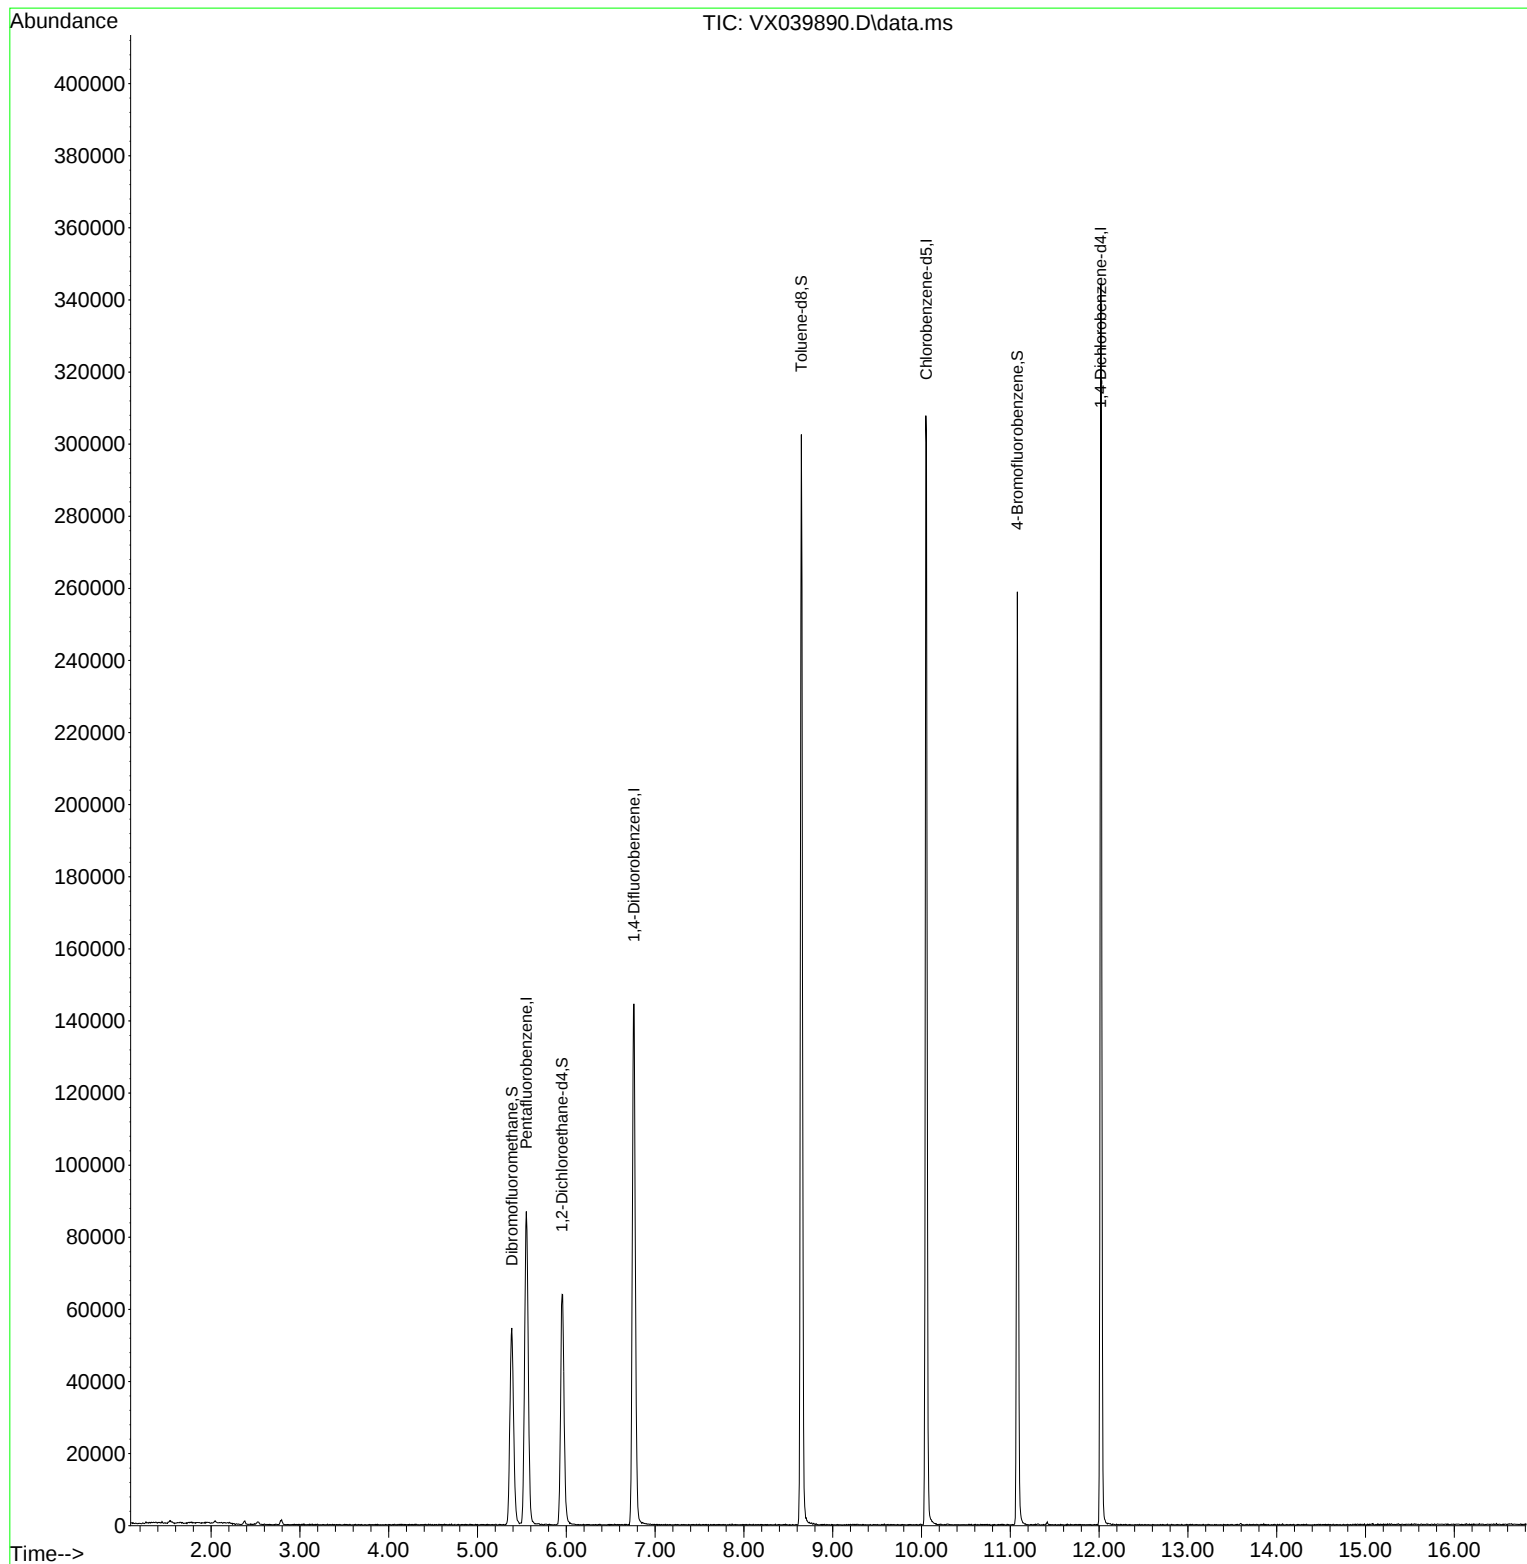



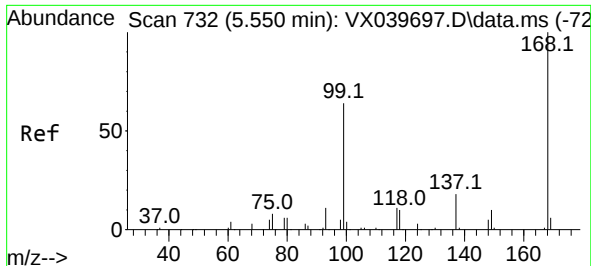


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.000 min
Lab File: VX039890.D
Acq: 22 Jan 2024 17:38

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-195-TB-20240117



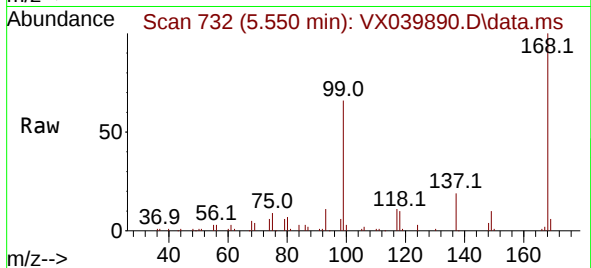



Tgt Ion:168 Resp: 77102
Ion Ratio Lower Upper
168 100
99 66.3 56.6 85.0

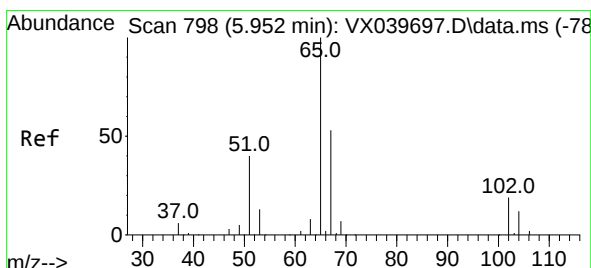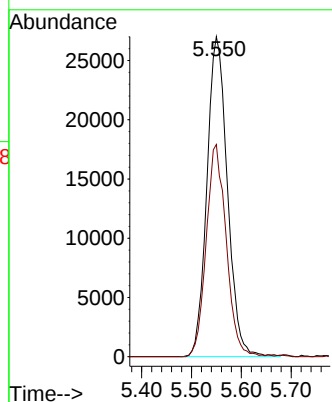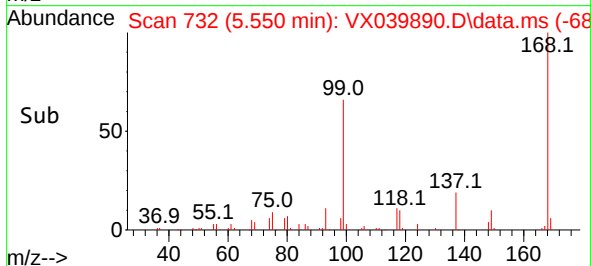

#33
1,2-Dichloroethane-d4
Concen: 47.742 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX039890.D
Acq: 22 Jan 2024 17:38

Tgt Ion: 65 Resp: 61662
Ion Ratio Lower Upper
65 100
67 52.4 0.0 100.2


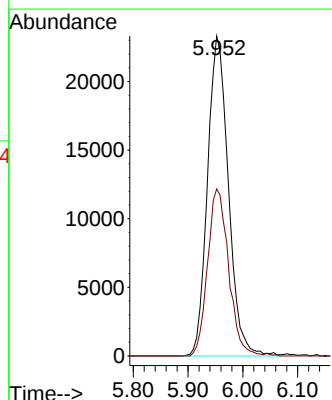
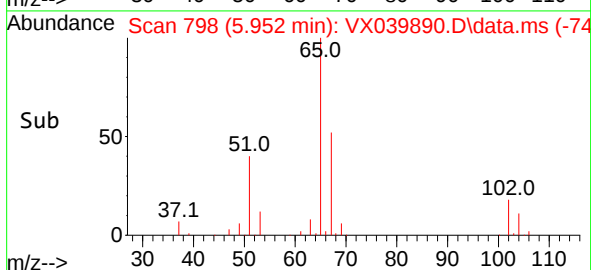
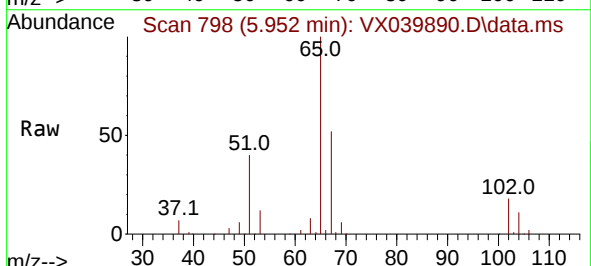


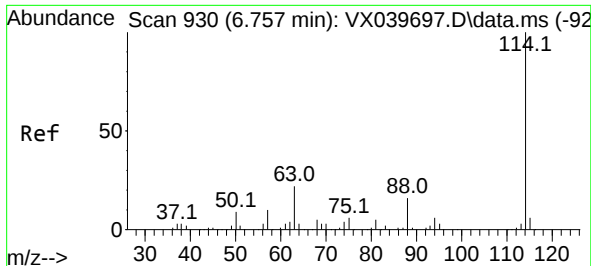

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX039890.D
Acq: 22 Jan 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-195-TB-20240117


Tgt Ion:114 Resp: 143016
Ion Ratio Lower Upper
114 100
63 21.1 0.0 45.0
88 15.2 0.0 36.6

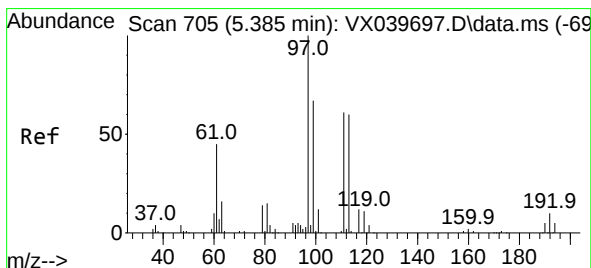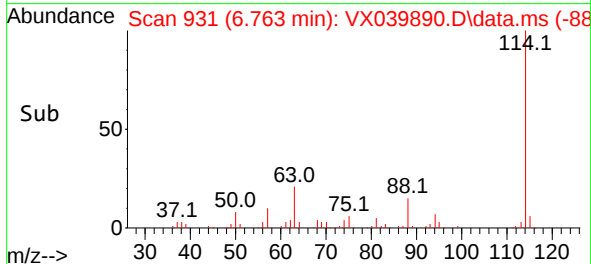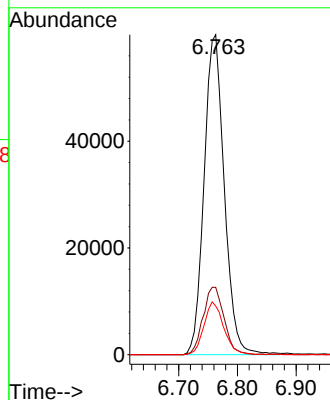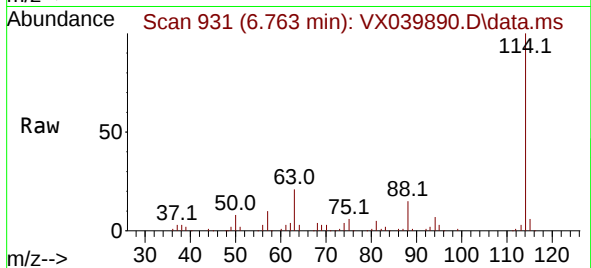

#35
Dibromofluoromethane
Concen: 49.586 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039890.D
Acq: 22 Jan 2024 17:38

Tgt Ion:113 Resp: 47765
Ion Ratio Lower Upper
113 100
111 101.7 82.9 124.3
192 16.5 13.3 19.9


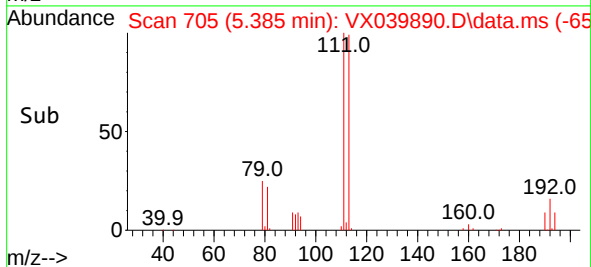
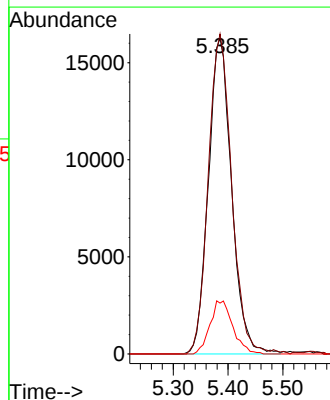
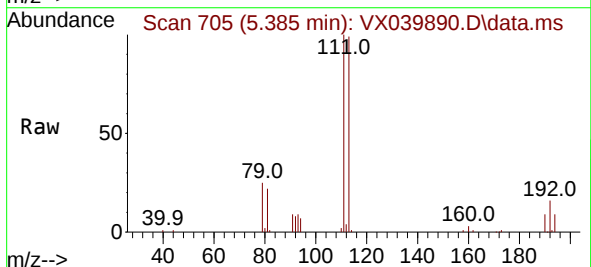


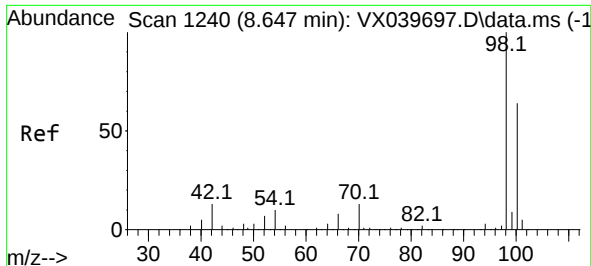

#50
Toluene-d8
Concen: 47.704 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX039890.D
Acq: 22 Jan 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-195-TB-20240117


Tgt Ion: 98 Resp: 173310
Ion Ratio Lower Upper
98 100
100 64.7 53.1 79.7

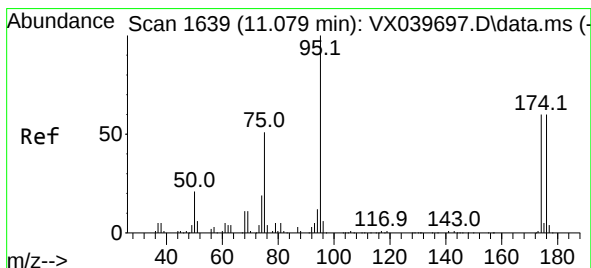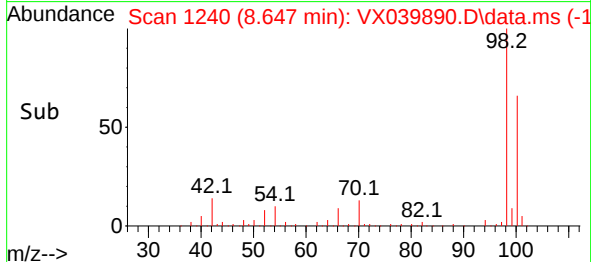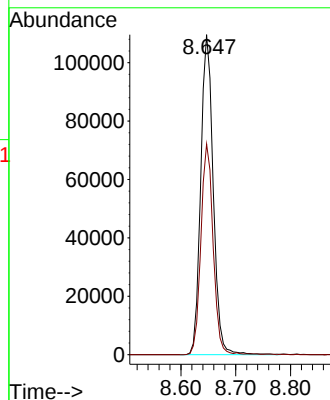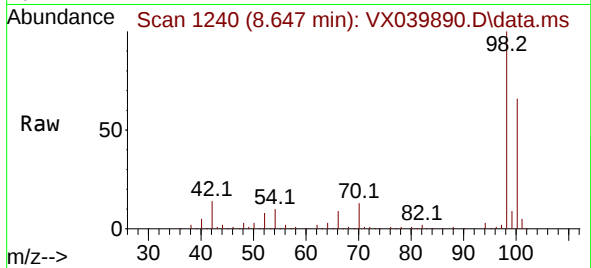

#62
4-Bromofluorobenzene
Concen: 47.501 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX039890.D
Acq: 22 Jan 2024 17:38

Tgt Ion: 95 Resp: 67484
Ion Ratio Lower Upper
95 100
174 69.6 0.0 135.6
176 67.0 0.0 131.0


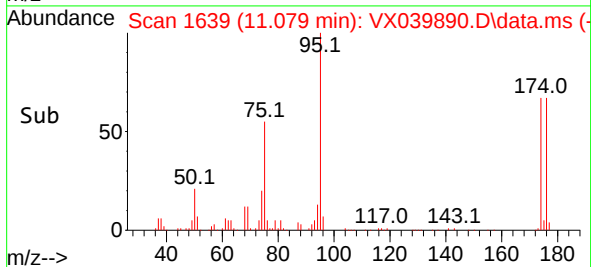
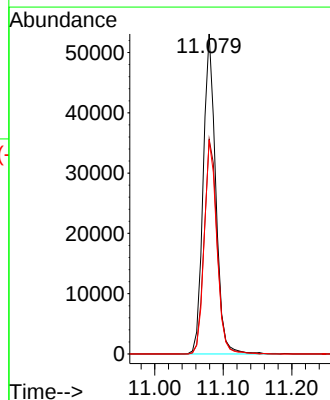
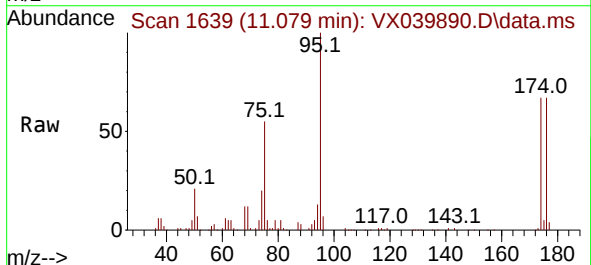


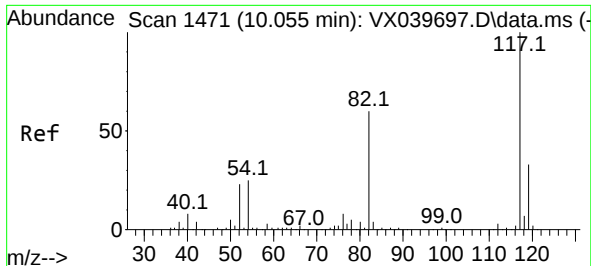

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX039890.D
Acq: 22 Jan 2024 17:38

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-195-TB-20240117

Tgt Ion:117 Resp: 135729
Ion Ratio Lower Upper
117 100
82 57.6 46.2 69.4
119 32.0 25.5 38.3

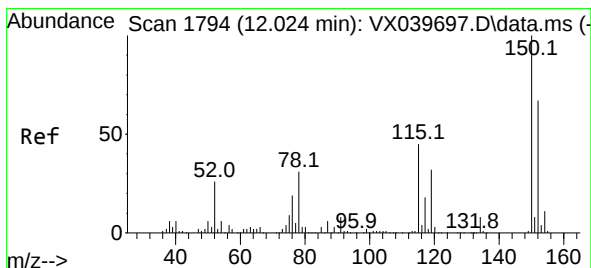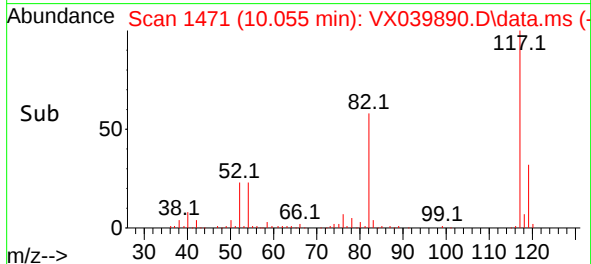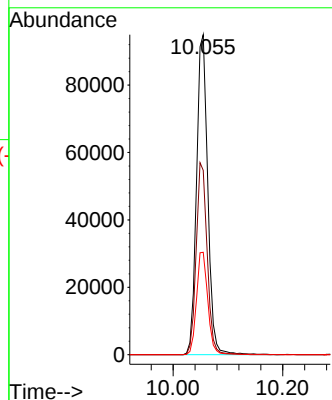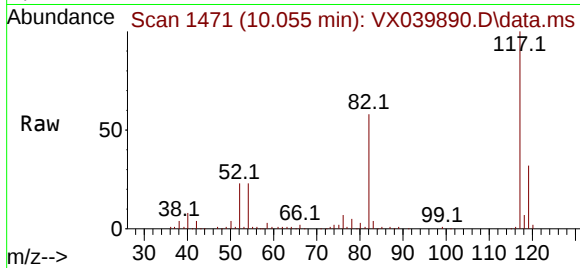

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX039890.D
Acq: 22 Jan 2024 17:38

Tgt Ion:152 Resp: 63938
Ion Ratio Lower Upper
152 100
115 65.3 43.3 129.9
150 160.4 0.0 345.0

