
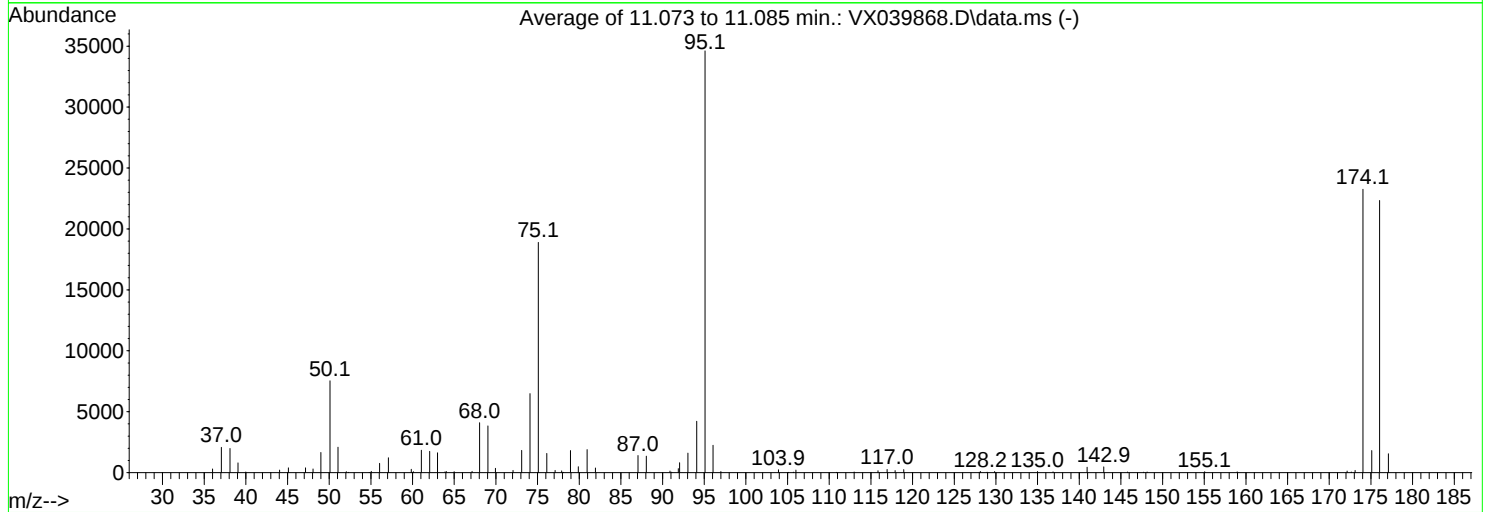


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012224\
Data File : VX039868.D
Acq On : 22 Jan 2024 08:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 03:51:26 2024

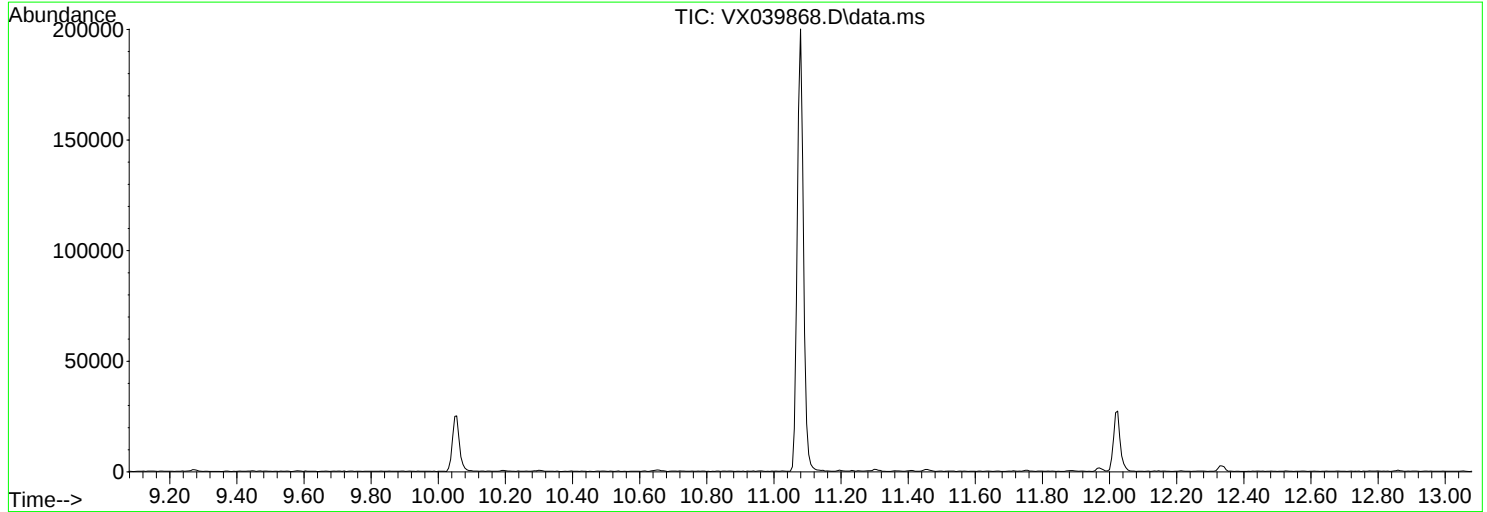

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	7541	PASS
75	95	30	60	54.6	18900	PASS
95	95	100	100	100.0	34616	PASS
96	95	5	9	6.5	2247	PASS
173	174	0.00	2	0.8	189	PASS
174	95	50	100	67.2	23261	PASS
175	174	5	9	7.8	1806	PASS
176	174	95	101	96.0	22339	PASS
177	176	5	9	6.9	1552	PASS