

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012225\
 Data File : VX044695.D
 Acq On : 22 Jan 2025 14:39
 Operator : JC/MD
 Sample : Q1131-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 23 00:52:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 23 00:51:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.750	114	238881	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	199974	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	78572	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	83176	40.345	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.700%
7) Chloroethane-d5	1.648	69	15496	29.176	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	58.360%#
11) 1,1-Dichloroethene-d2	2.294	65	26654	34.244	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.480%
21) 2-Butanone-d5	4.452	46	107191	103.721	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.720%
24) Chloroform-d	5.043	84	138313	40.592	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.180%
26) 1,2-Dichloroethane-d4	5.946	65	87902	39.113	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.220%
32) Benzene-d6	5.958	84	288437	43.219	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.440%
36) 1,2-Dichloropropane-d6	7.299	67	93400	44.277	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.560%
41) Toluene-d8	8.640	98	250265	41.947	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.900%
43) trans-1,3-Dichloroprop...	8.945	79	42582	39.388	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.780%
47) 2-Hexanone-d5	9.384	63	63258	104.381	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.380%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	120889	47.541	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.080%
66) 1,2-Dichlorobenzene-d4	12.316	152	73426	43.486	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.980%
Target Compounds						
61) 1,2,3-Trichloropropane	12.018	75	10407	6.748	ug/L	Qvalue # 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012225\
Data File : VX044695.D
Acq On : 22 Jan 2025 14:39
Operator : JC/MD
Sample : Q1131-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 23 00:52:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 23 00:51:10 2025
Response via : Initial Calibration

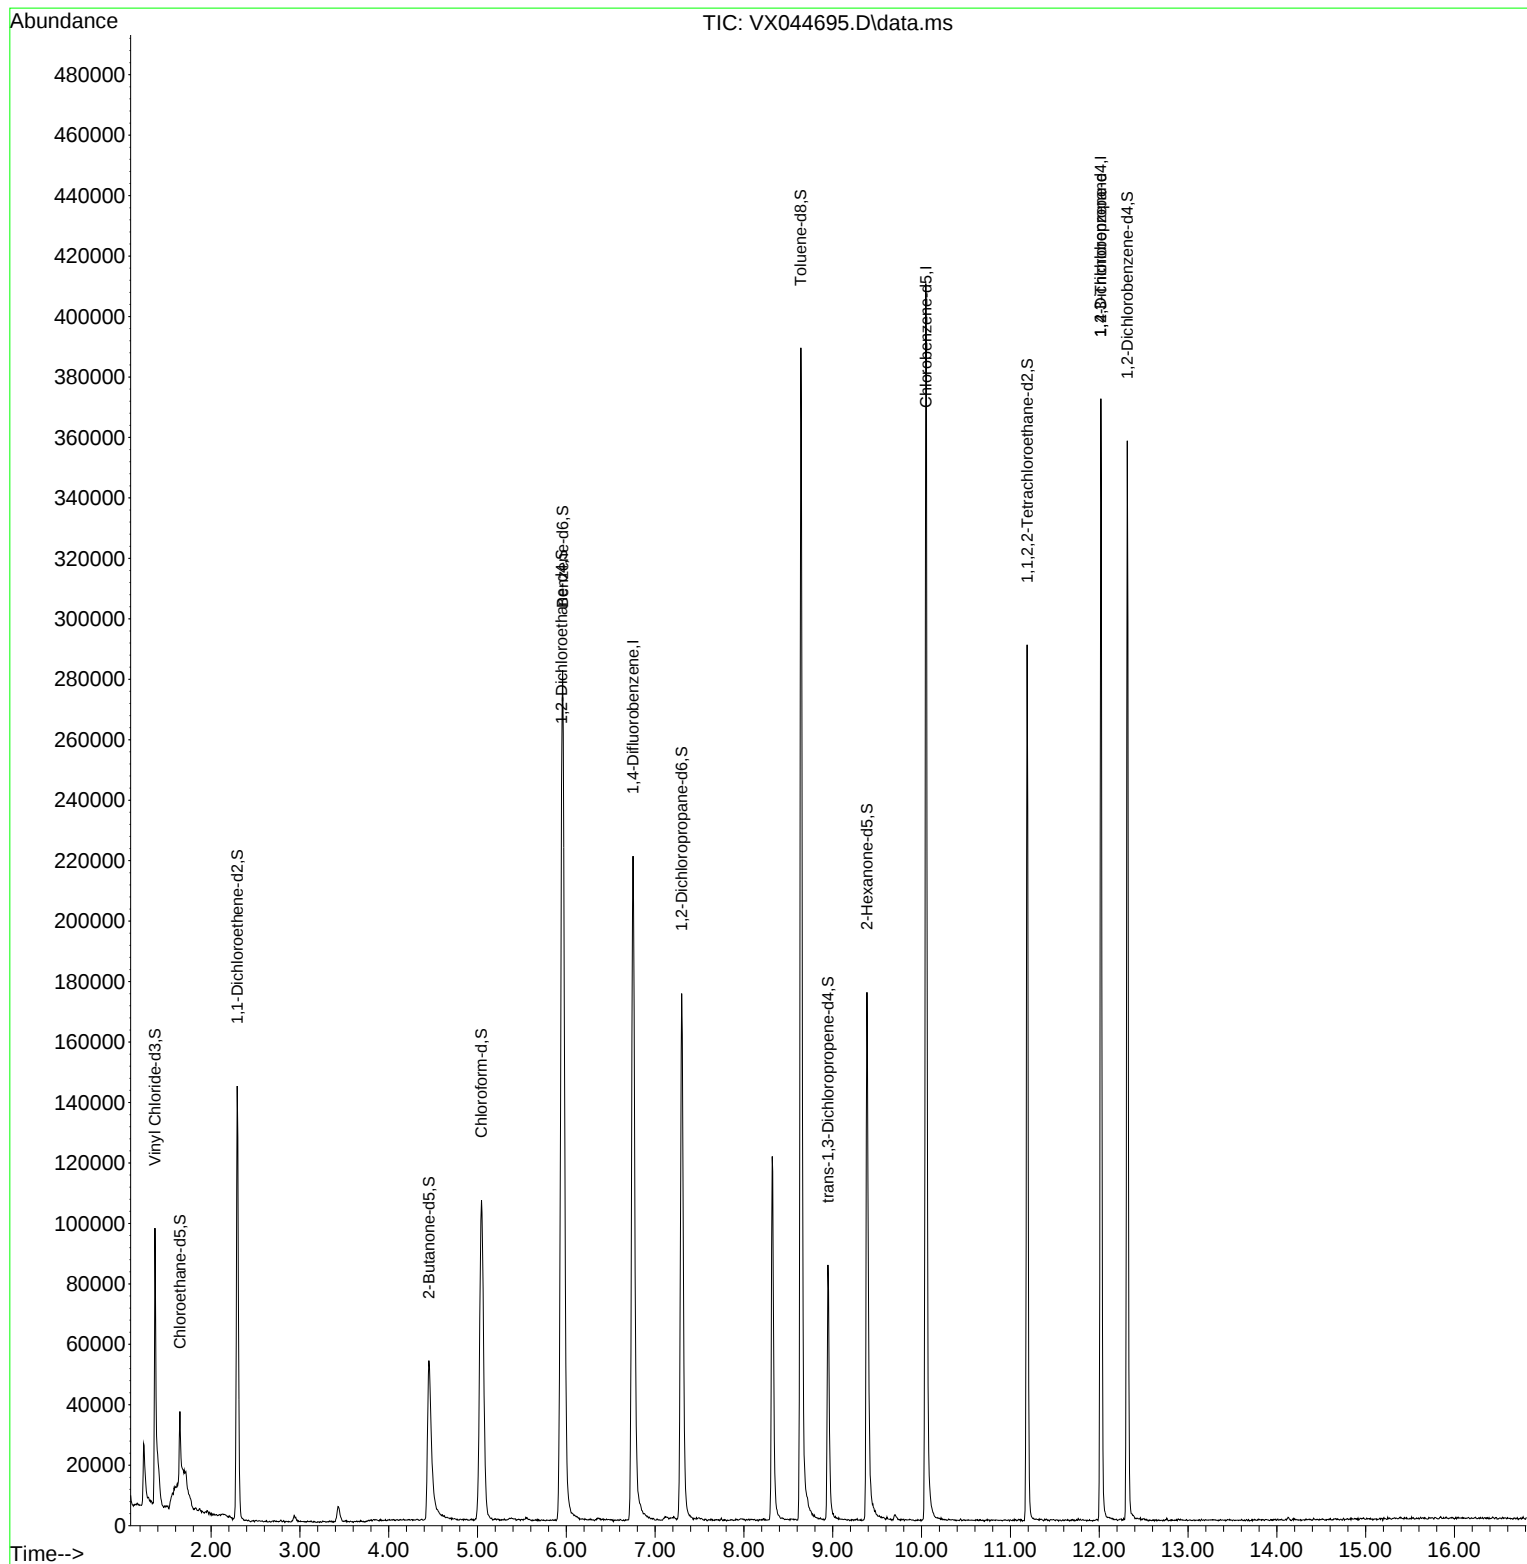

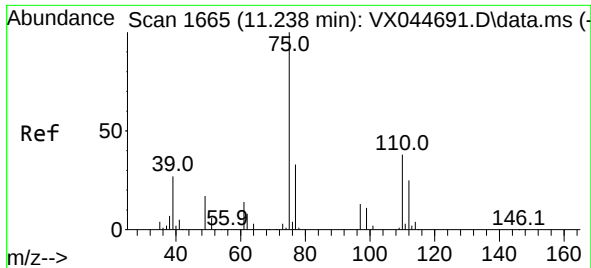

#61
 1,2,3-Trichloropropane
 Concen: 6.748 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX044695.D
 Acq: 22 Jan 2025 14:39

Instrument :
 MSVOA_X
 ClientSampleId :

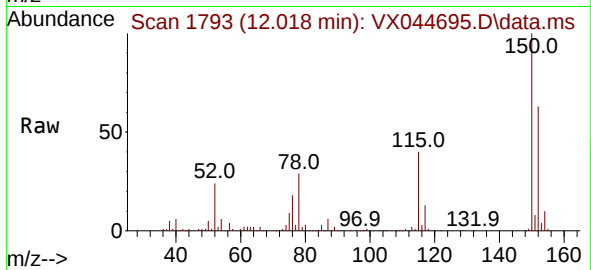

Tgt Ion: 75 Resp: 10407
 Ion Ratio Lower Upper
 75 100
 77 32.5 25.8 38.6
 110 2.9 30.8 46.2#

