

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012225\
 Data File : VX044696.D
 Acq On : 22 Jan 2025 15:09
 Operator : JC/MD
 Sample : Q1130-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 23 00:52:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 23 00:51:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.750	114	228477	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	189148	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	70263	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	92259	46.789	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.580%
7) Chloroethane-d5	1.648	69	17431	34.314	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	68.620%#
11) 1,1-Dichloroethene-d2	2.294	65	30976	41.609	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.220%
21) 2-Butanone-d5	4.452	46	121692	123.114	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	123.110%
24) Chloroform-d	5.043	84	155993	47.865	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.720%
26) 1,2-Dichloroethane-d4	5.946	65	99100	46.104	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.200%
32) Benzene-d6	5.964	84	327428	51.870	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.740%
36) 1,2-Dichloropropane-d6	7.299	67	106018	53.135	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	106.280%
41) Toluene-d8	8.640	98	279108	49.459	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.920%
43) trans-1,3-Dichloroprop...	8.945	79	49329	48.240	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.480%
47) 2-Hexanone-d5	9.384	63	71177	124.171	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	124.170%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	136034	56.559	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	113.120%
66) 1,2-Dichlorobenzene-d4	12.316	152	78598	52.054	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.100%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	12.018	75	9503	6.891	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012225\
Data File : VX044696.D
Acq On : 22 Jan 2025 15:09
Operator : JC/MD
Sample : Q1130-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 23 00:52:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012125WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 23 00:51:10 2025
Response via : Initial Calibration

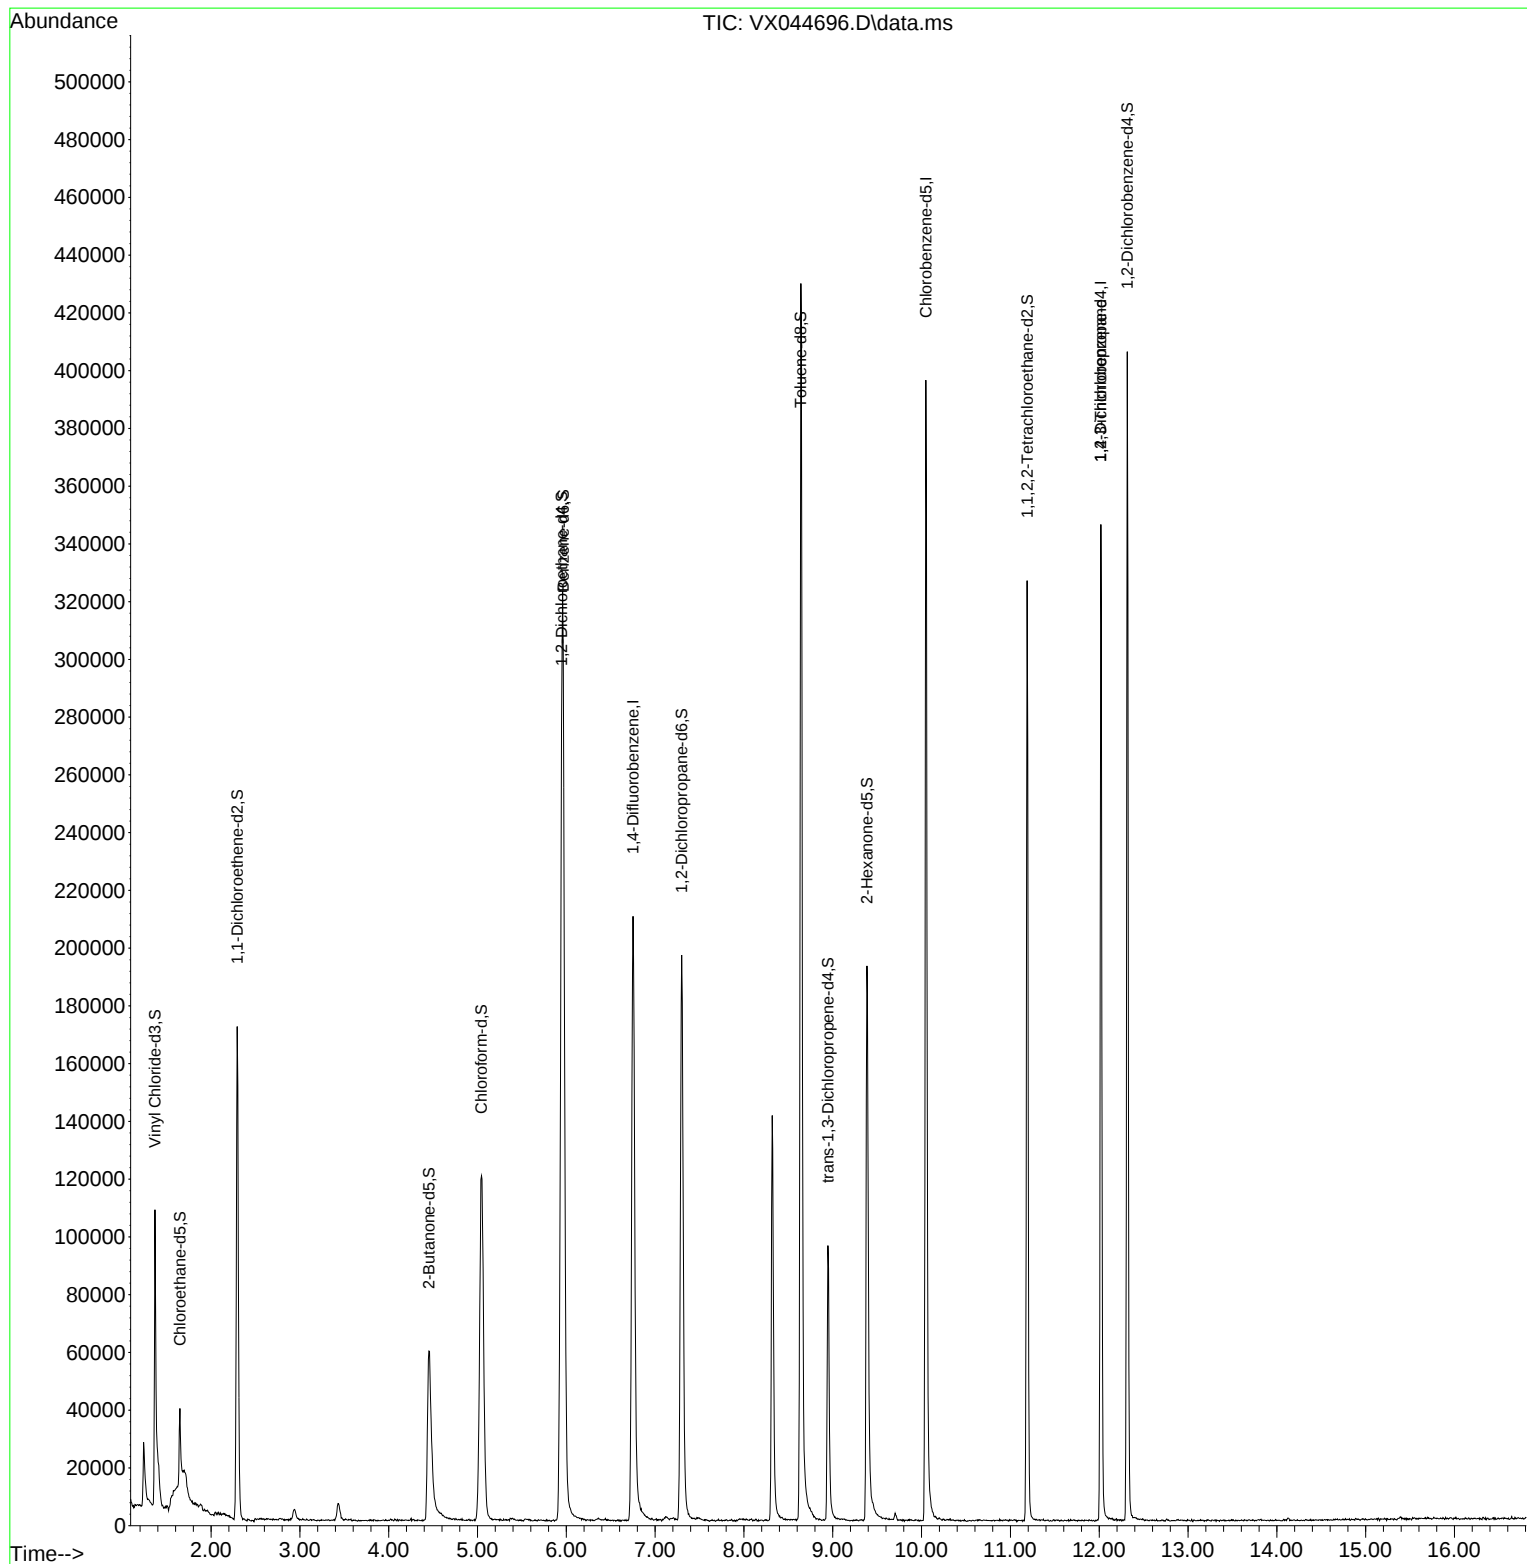

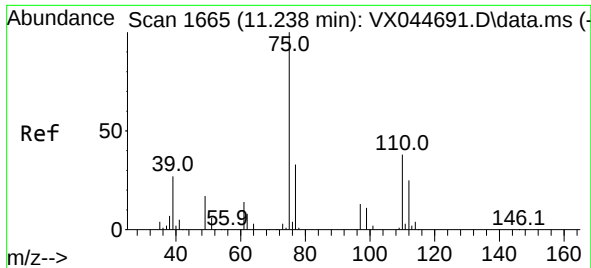

#61
 1,2,3-Trichloropropane
 Concen: 6.891 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX044696.D
 Acq: 22 Jan 2025 15:09

Instrument :
 MSVOA_X
 ClientSampleId :

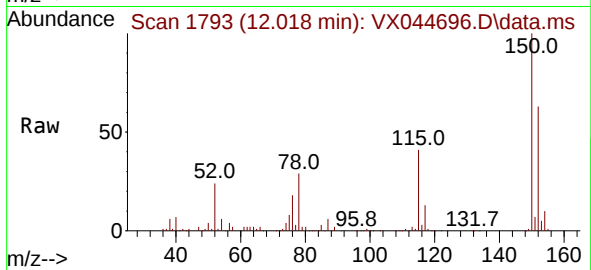

Tgt Ion: 75 Resp: 9503
 Ion Ratio Lower Upper
 75 100
 77 33.4 25.8 38.6
 110 2.5 30.8 46.2#

