
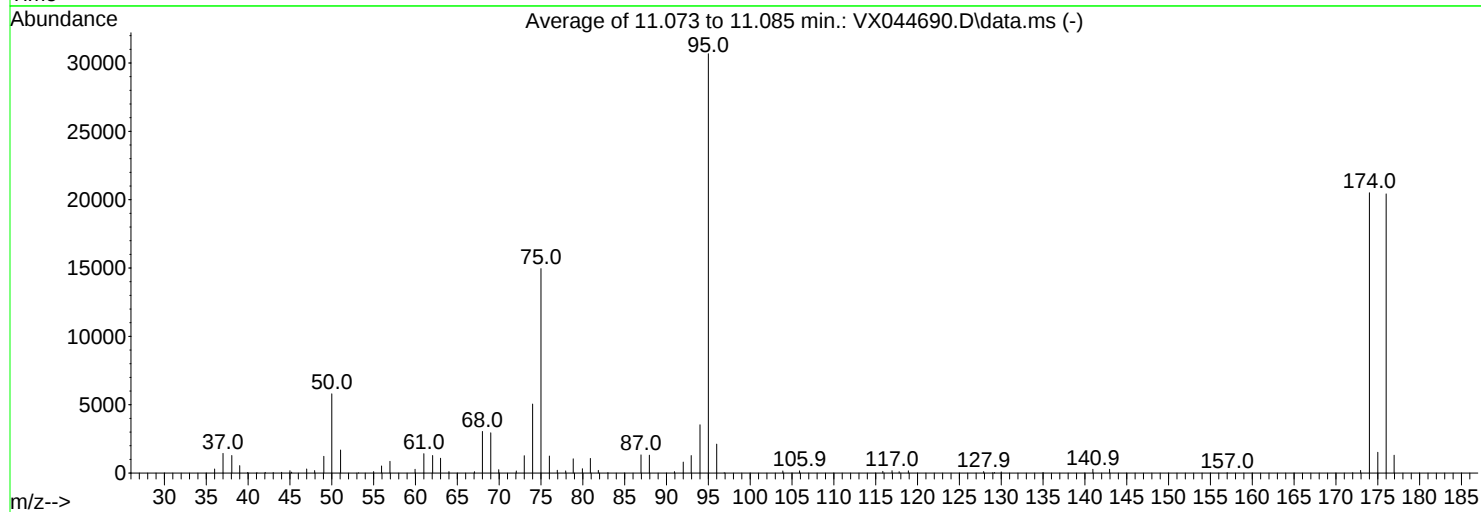


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012225\
Data File : VX044690.D
Acq On : 22 Jan 2025 09:38
Operator : JC/MD
Sample : BFB713
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB713

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXL012125WMA.M
Title : VOC Analysis
Last Update : Thu Jan 23 00:51:10 2025

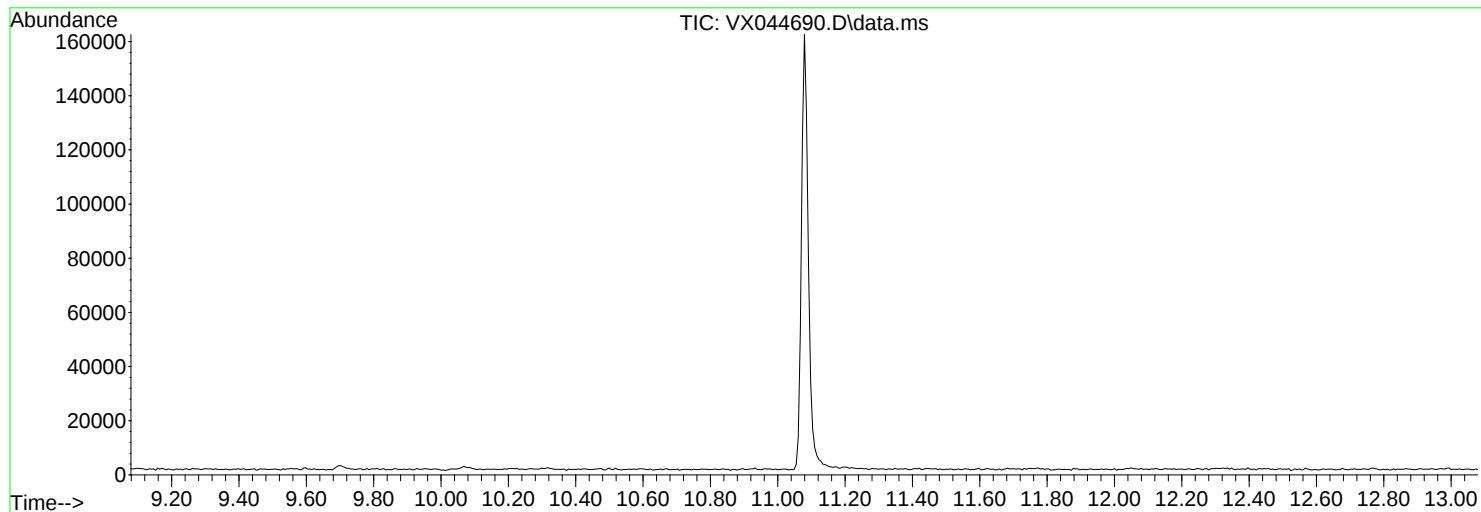

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	5797	PASS
75	95	30	80	48.8	14958	PASS
95	95	100	100	100.0	30677	PASS
96	95	5	9	6.9	2117	PASS
173	174	0.00	2	0.9	192	PASS
174	95	50	120	66.8	20506	PASS
175	174	5	9	7.4	1521	PASS
176	174	95	101	99.6	20422	PASS
177	176	5	9	6.4	1307	PASS

m/z	Abundance
38.90	101.0
40.00	1095.0
41.10	88.0
42.90	82.0
44.00	550.0
91.00	62.0

Instrument :
MSVOA_X
ClientSampleId :
BFB713

m/z	Abundance
36.00	282.0
37.00	1573.0
38.10	1256.0
39.00	775.0
40.00	1106.0
41.00	122.0
42.10	78.0
43.10	138.0
44.00	592.0
45.00	289.0
46.90	315.0
48.00	178.0
49.10	1120.0
50.00	5447.0
51.10	1503.0
55.00	63.0
55.90	424.0
57.00	949.0
60.00	223.0
61.00	1460.0
62.10	1184.0
63.00	1126.0
64.00	108.0
67.00	99.0
68.00	2991.0
69.00	2779.0
70.00	247.0
72.10	185.0
73.00	1277.0
74.00	4476.0
75.00	13777.0
76.00	1280.0
77.10	207.0
78.00	157.0
78.90	1013.0
80.00	208.0
80.90	948.0
81.90	188.0
83.00	88.0
86.90	1181.0
87.90	1339.0
91.00	166.0
92.00	658.0
93.00	1324.0
94.00	3164.0
95.00	27352.0
96.00	1942.0
103.90	187.0
105.90	214.0
115.80	98.0
117.00	234.0
117.90	65.0
118.90	139.0
127.80	82.0
129.00	80.0
130.10	64.0
135.00	52.0
140.90	174.0
143.00	121.0
172.90	199.0
174.00	16325.0
175.00	1283.0
176.00	15642.0
177.00	1115.0

Instrument :
MSVOA_X
ClientSampleId :
BFB713

m/z	Abundance
36.00	312.0
37.00	1562.0
38.00	1354.0
39.10	723.0
39.90	1154.0
41.10	130.0
43.20	147.0
43.90	588.0
45.00	235.0
47.00	292.0
47.80	204.0
49.00	1498.0
50.00	6495.0
51.00	1919.0
53.20	59.0
55.00	114.0
55.90	568.0
56.90	907.0
59.90	379.0
61.00	1484.0
62.00	1439.0
63.10	1165.0
64.00	130.0
67.10	135.0
68.00	3514.0
69.00	3367.0
69.90	273.0
72.00	113.0
73.00	1445.0
74.00	6119.0
75.00	18208.0
76.00	1343.0
76.90	257.0
77.80	155.0
78.90	1287.0
80.00	353.0
80.90	1291.0
81.80	206.0
87.00	1467.0
88.00	1426.0
90.90	208.0
92.00	945.0
93.00	1372.0
94.00	4040.0
95.00	35472.0
96.00	2582.0
96.90	72.0
103.90	165.0
105.90	179.0
115.80	173.0
116.80	150.0
117.80	102.0
118.90	231.0
127.90	203.0
129.20	113.0
130.00	110.0
135.00	63.0
141.00	383.0
142.90	374.0
157.00	59.0
172.90	160.0
174.00	24168.0
175.00	1746.0
176.00	24136.0
177.00	1548.0

Instrument :
MSVOA_X
ClientSampleId :
BFB713

m/z	Abundance
36.00	296.0
37.00	1182.0
38.00	1244.0
39.00	440.0
40.00	1151.0
41.10	92.0
42.00	67.0
43.00	69.0
44.10	644.0
45.20	205.0
47.10	289.0
48.00	162.0
49.00	1059.0
50.00	5448.0
51.00	1637.0
55.00	149.0
56.00	567.0
57.00	724.0
59.90	235.0
61.00	1313.0
62.00	1233.0
62.90	963.0
64.00	88.0
67.10	73.0
68.00	2623.0
69.00	2696.0
70.00	231.0
72.00	169.0
73.00	1090.0
74.00	4557.0
75.00	12889.0
76.00	1112.0
76.90	160.0
78.00	161.0
78.80	826.0
79.90	400.0
80.90	972.0
81.90	191.0
87.00	1341.0
88.00	1162.0
90.90	133.0
92.00	810.0
92.90	1148.0
94.00	3388.0
95.00	29208.0
96.00	1827.0
103.80	110.0
106.00	104.0
115.90	113.0
117.00	140.0
117.70	142.0
118.90	127.0
128.00	58.0
129.90	94.0
140.90	279.0
143.00	341.0
172.00	62.0
173.00	216.0
174.00	21024.0
175.00	1533.0
176.00	21488.0
176.90	1259.0

Instrument :
MSVOA_X
ClientSampleId :
BFB713