

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012323\
 Data File : VX033838.D
 Acq On : 23 Jan 2023 10:53
 Operator : JC/MD
 Sample : VX0123WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0123WBL01

Quant Time: Jan 24 00:35:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 11 14:48:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	158425	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	229035	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	205440	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	96377	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	75849	45.471	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	90.940%
35) Dibromofluoromethane	5.385	113	70803	49.785	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.560%
50) Toluene-d8	8.647	98	260275	50.229	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.460%
62) 4-Bromofluorobenzene	11.079	95	87794	45.634	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.260%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012323\
Data File : VX033838.D
Acq On : 23 Jan 2023 10:53
Operator : JC/MD
Sample : VX0123WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0123WBL01

Quant Time: Jan 24 00:35:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 11 14:48:42 2023
Response via : Initial Calibration




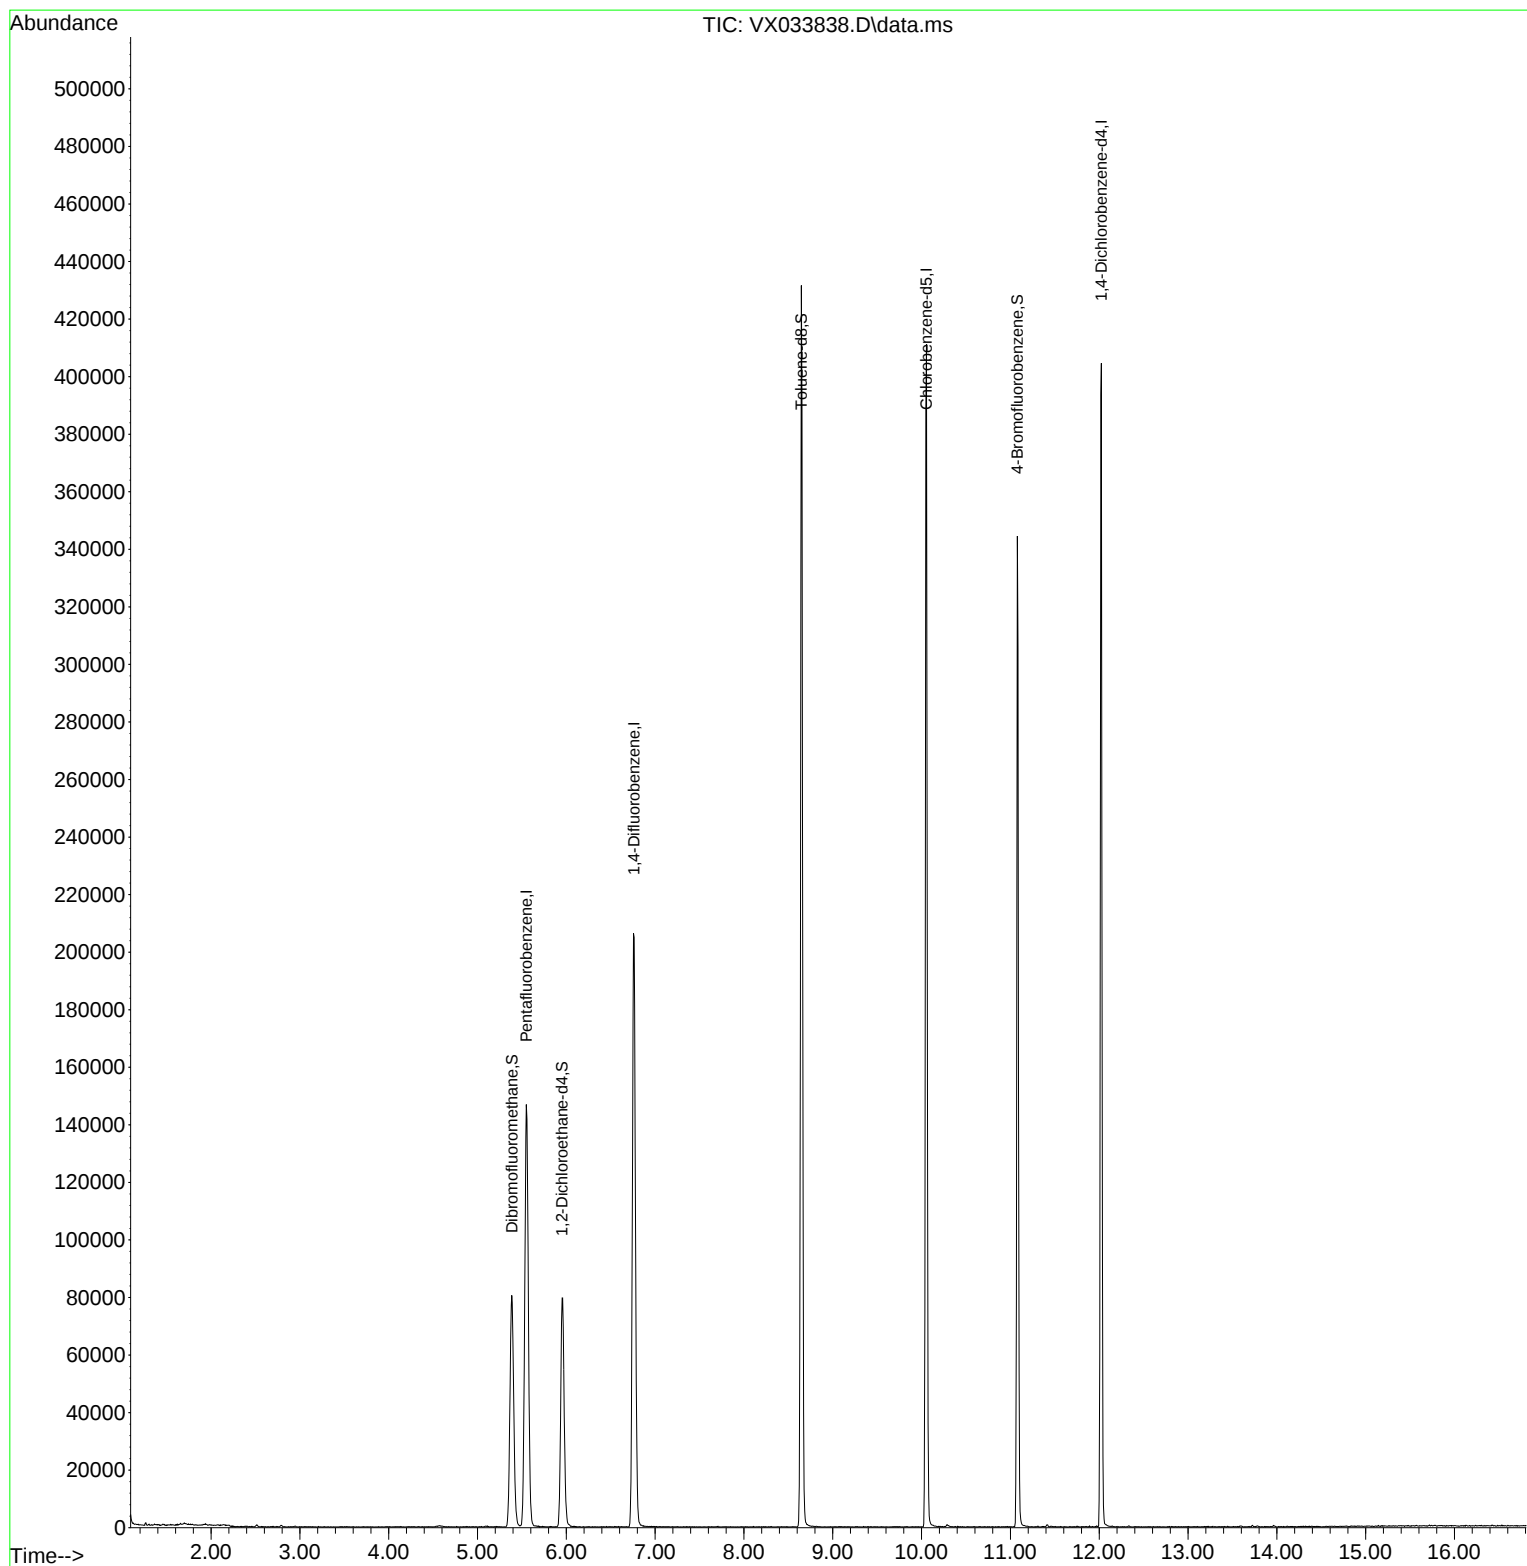


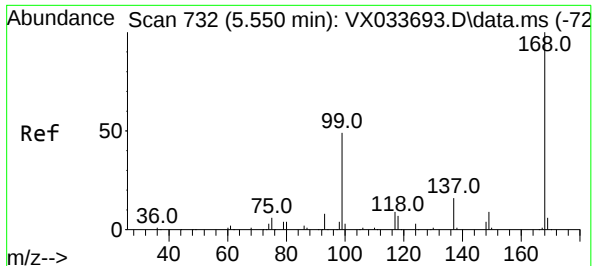

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX033838.D
Acq: 23 Jan 2023 10:53




Instrument :
MSVOA_X
ClientSampleId :
VX0123WBL01


Tgt Ion:168 Resp: 158425
Ion Ratio Lower Upper
168 100
99 47.3 39.6 59.4

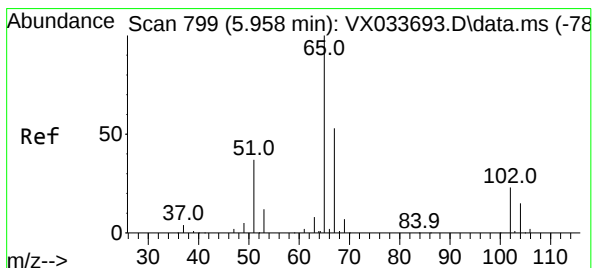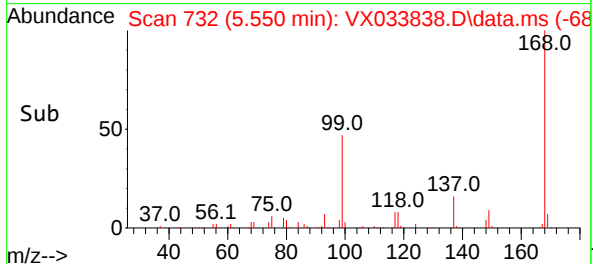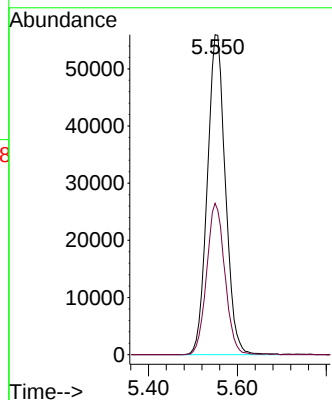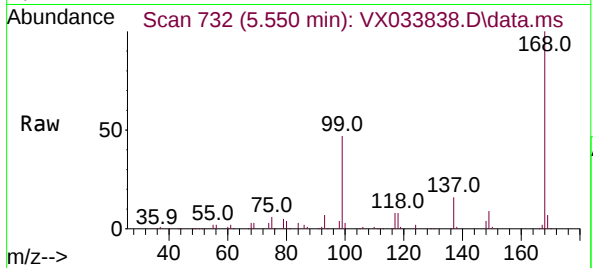

#33
1,2-Dichloroethane-d4
Concen: 45.471 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX033838.D
Acq: 23 Jan 2023 10:53

Tgt Ion: 65 Resp: 75849
Ion Ratio Lower Upper
65 100
67 54.1 0.0 104.8


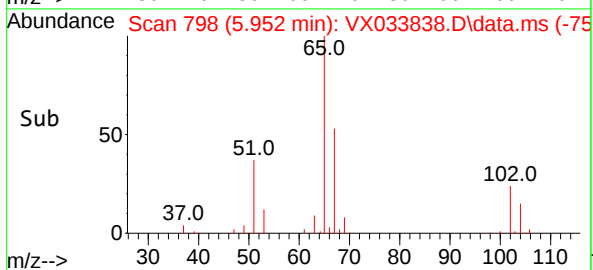
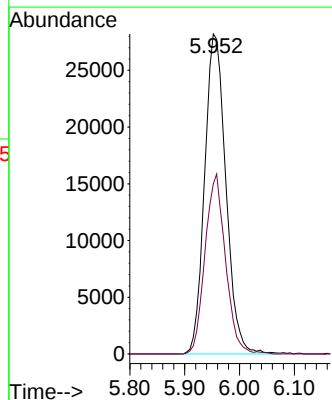
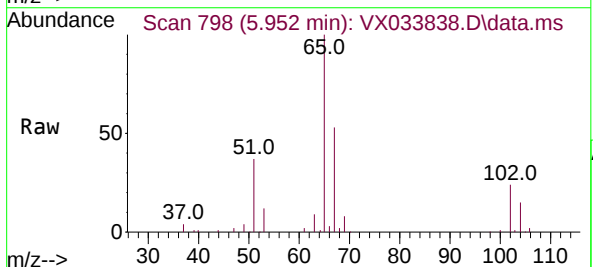


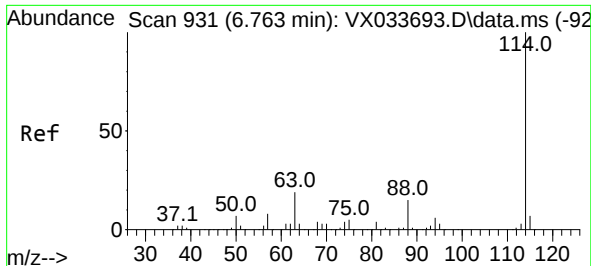

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX033838.D
Acq: 23 Jan 2023 10:53




Instrument :
MSVOA_X
ClientSampleId :
VX0123WBL01


Tgt Ion:114 Resp: 229035
Ion Ratio Lower Upper
114 100
63 18.4 0.0 37.4
88 15.1 0.0 30.6

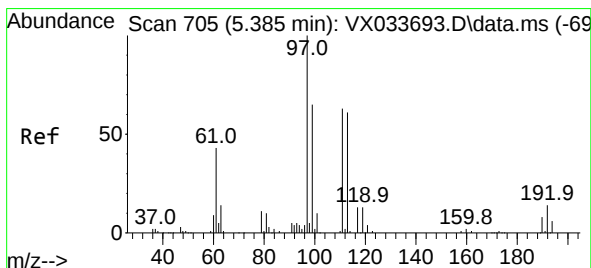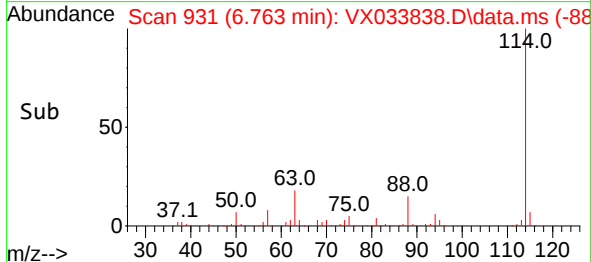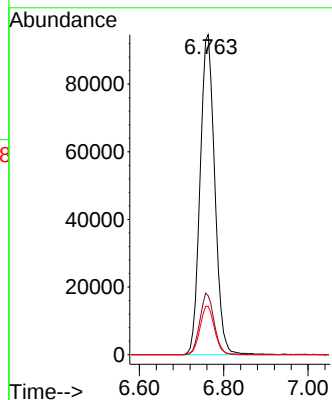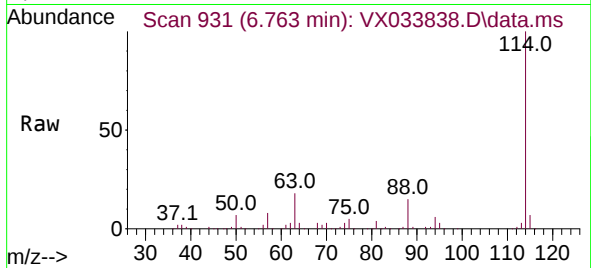

#35
Dibromofluoromethane
Concen: 49.785 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX033838.D
Acq: 23 Jan 2023 10:53

Tgt Ion:113 Resp: 70803
Ion Ratio Lower Upper
113 100
111 103.6 83.0 124.6
192 24.6 19.0 28.4


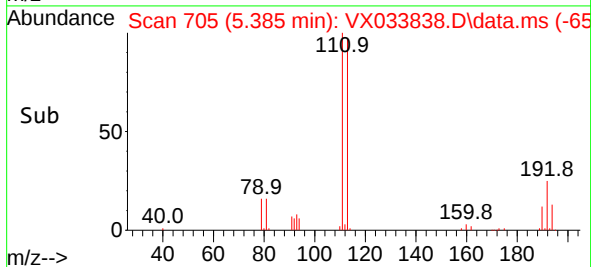
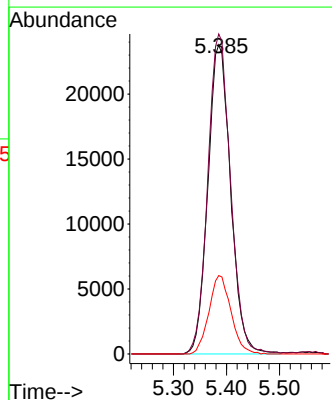
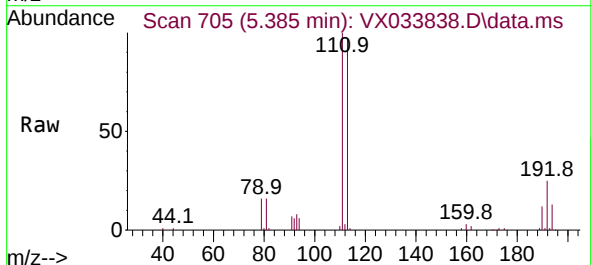


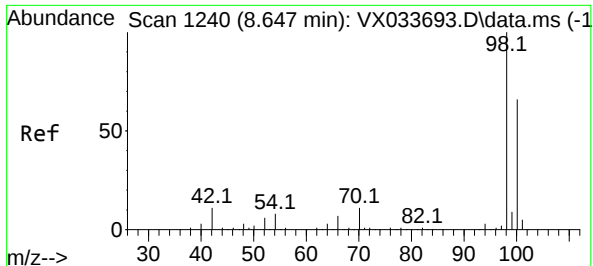

#50
Toluene-d8
Concen: 50.229 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033838.D
Acq: 23 Jan 2023 10:53




Instrument :
MSVOA_X
ClientSampleId :
VX0123WBL01


Tgt Ion: 98 Resp: 260275
Ion Ratio Lower Upper
98 100
100 67.2 53.6 80.4

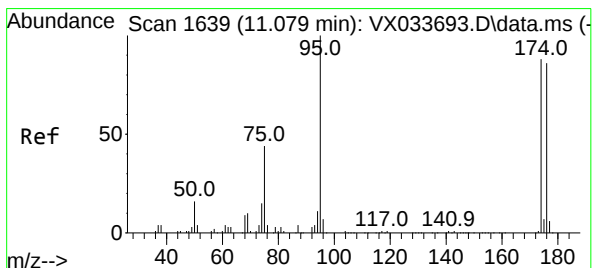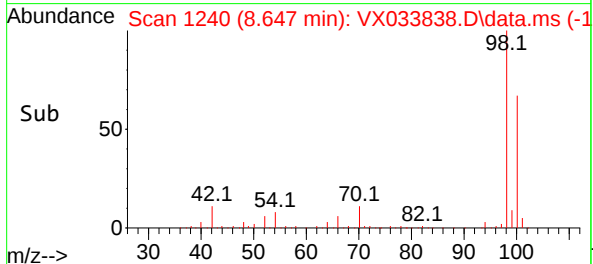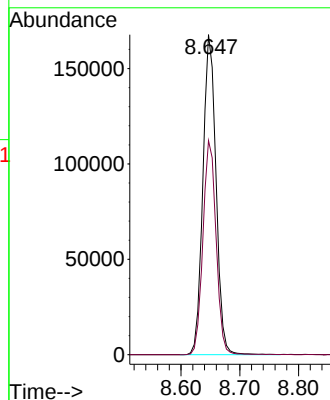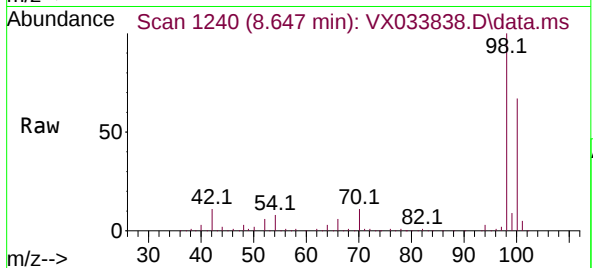

#62
4-Bromofluorobenzene
Concen: 45.634 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX033838.D
Acq: 23 Jan 2023 10:53

Tgt Ion: 95 Resp: 87794
Ion Ratio Lower Upper
95 100
174 97.1 0.0 184.4
176 94.5 0.0 178.8


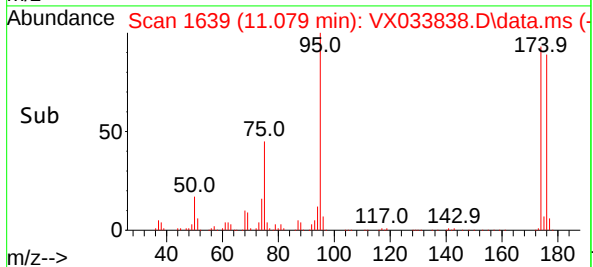
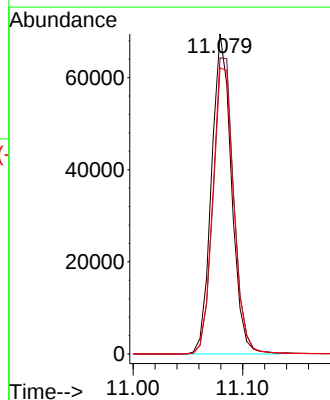
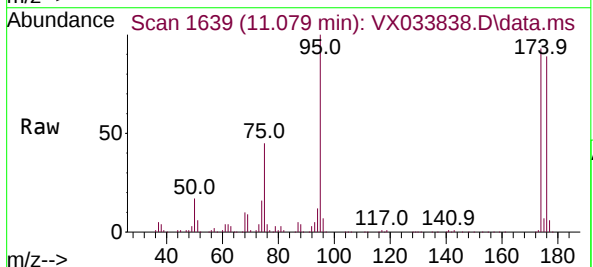


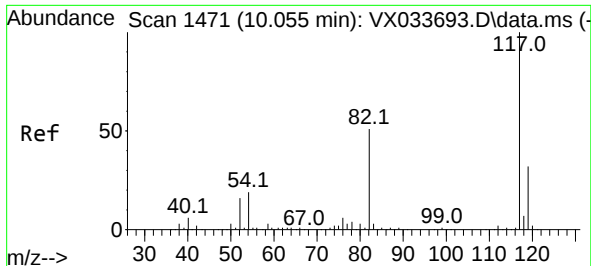

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033838.D
Acq: 23 Jan 2023 10:53

Instrument :
MSVOA_X
ClientSampleId :
VX0123WBL01

Tgt Ion:117 Resp: 205440
Ion Ratio Lower Upper
117 100
82 51.2 40.6 60.8
119 31.7 25.6 38.4

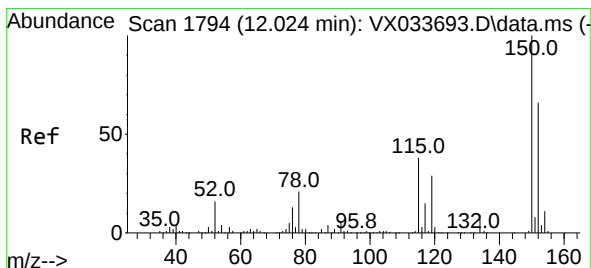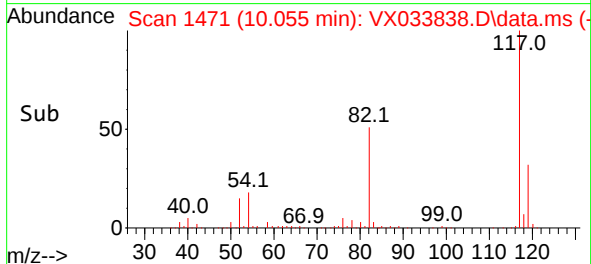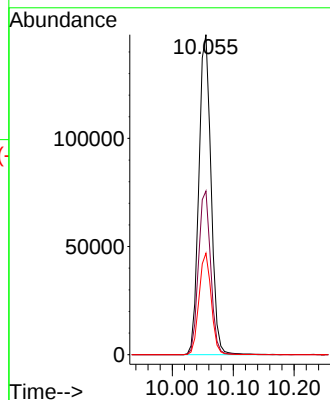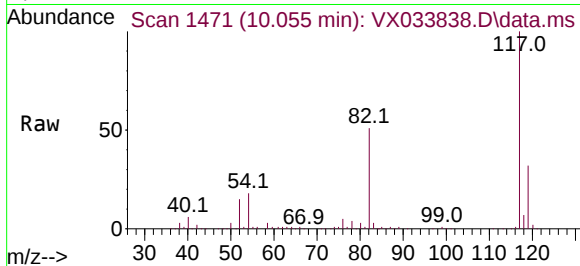

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX033838.D
Acq: 23 Jan 2023 10:53

Tgt Ion:152 Resp: 96377
Ion Ratio Lower Upper
152 100
115 53.5 38.7 116.1
150 156.0 0.0 348.2

