


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012323\
Data File : VX033835.D
Acq On : 23 Jan 2023 08:49
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Title : SW846 8260
Last Update : Wed Jan 11 14:48:42 2023

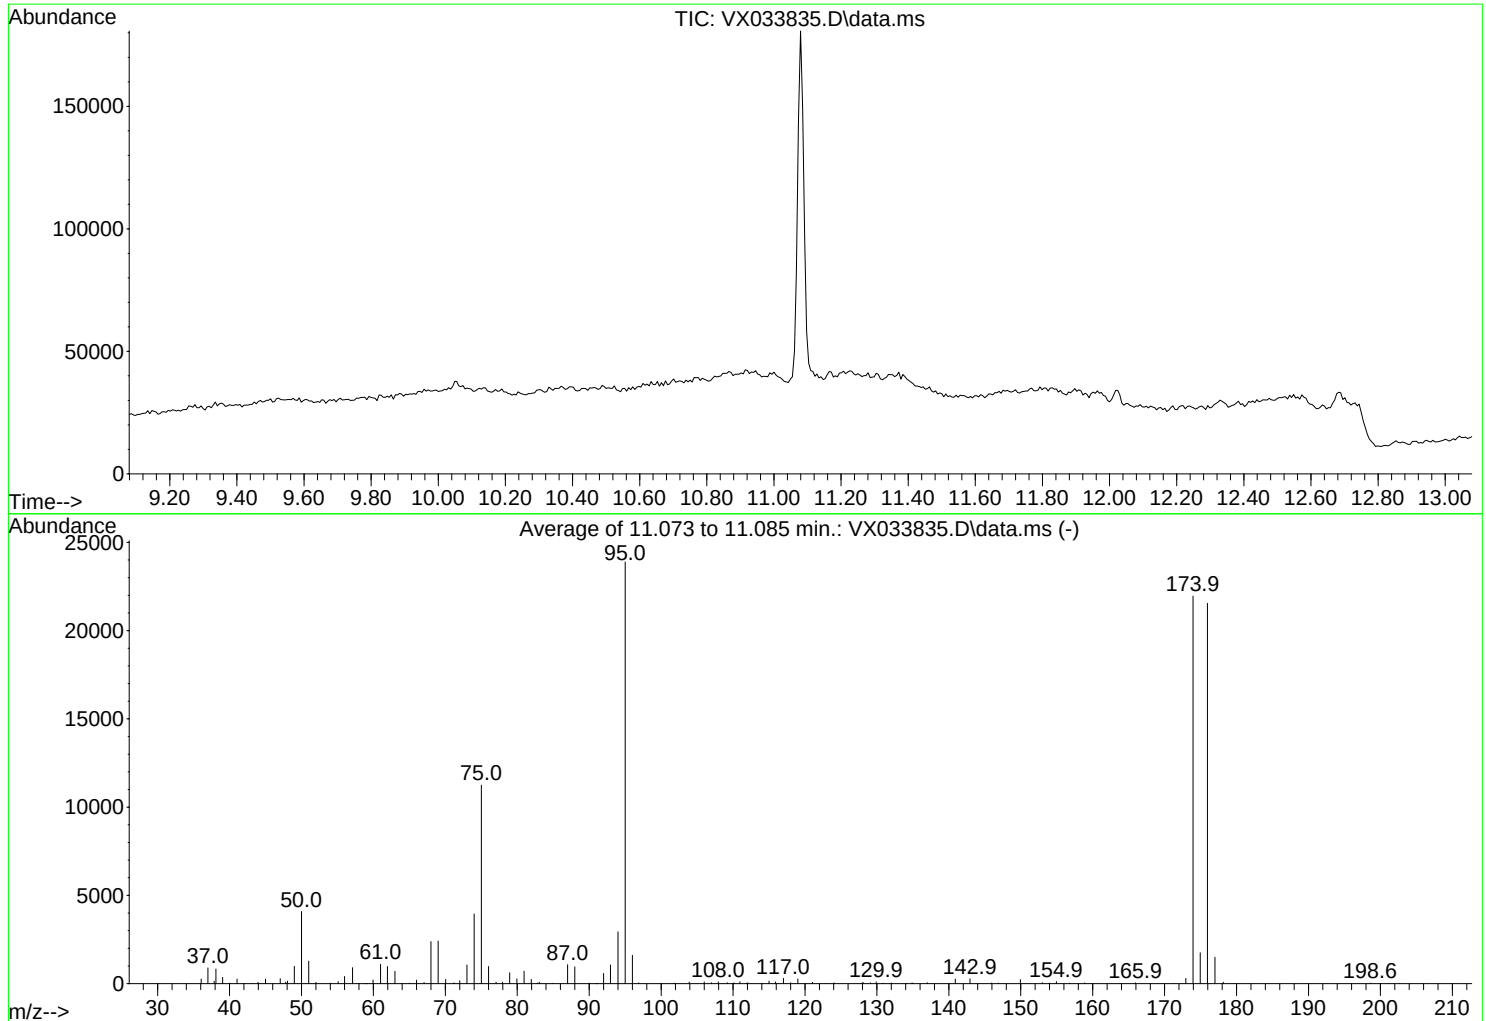

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	4092	PASS
75	95	30	60	47.1	11246	PASS
95	95	100	100	100.0	23897	PASS
96	95	5	9	6.7	1604	PASS
173	174	0.00	2	1.4	301	PASS
174	95	50	100	91.9	21955	PASS
175	174	5	9	8.0	1751	PASS
176	174	95	101	98.1	21544	PASS
177	176	5	9	6.9	1492	PASS