
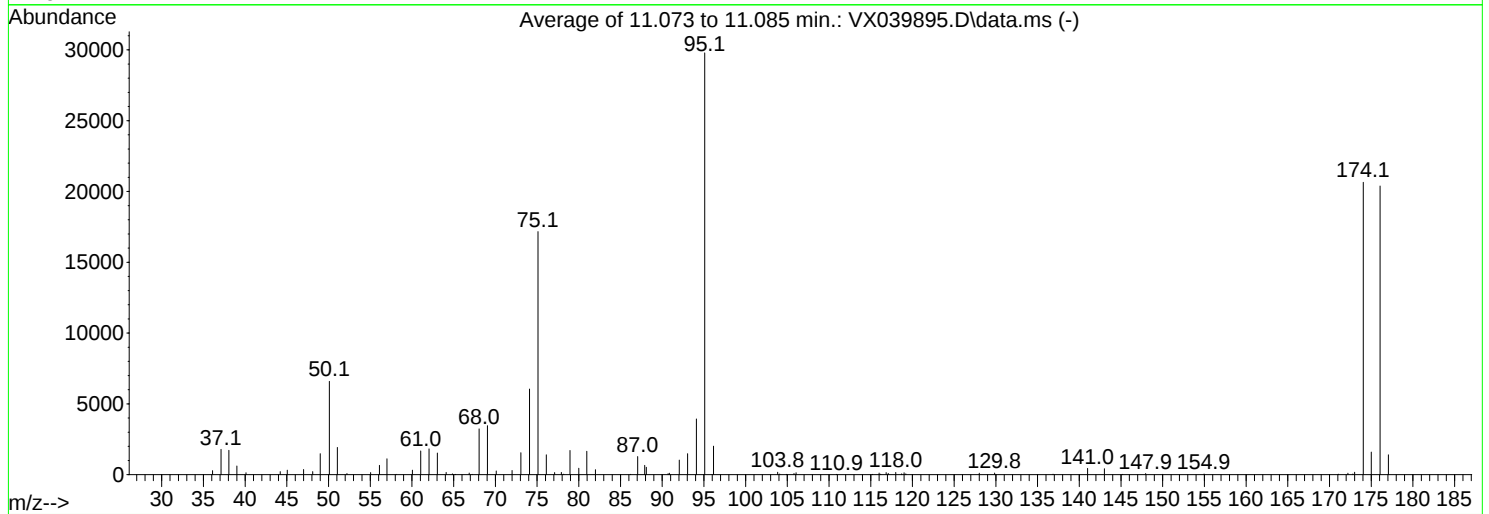


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012324\
Data File : VX039895.D
Acq On : 23 Jan 2024 08:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 03:51:26 2024

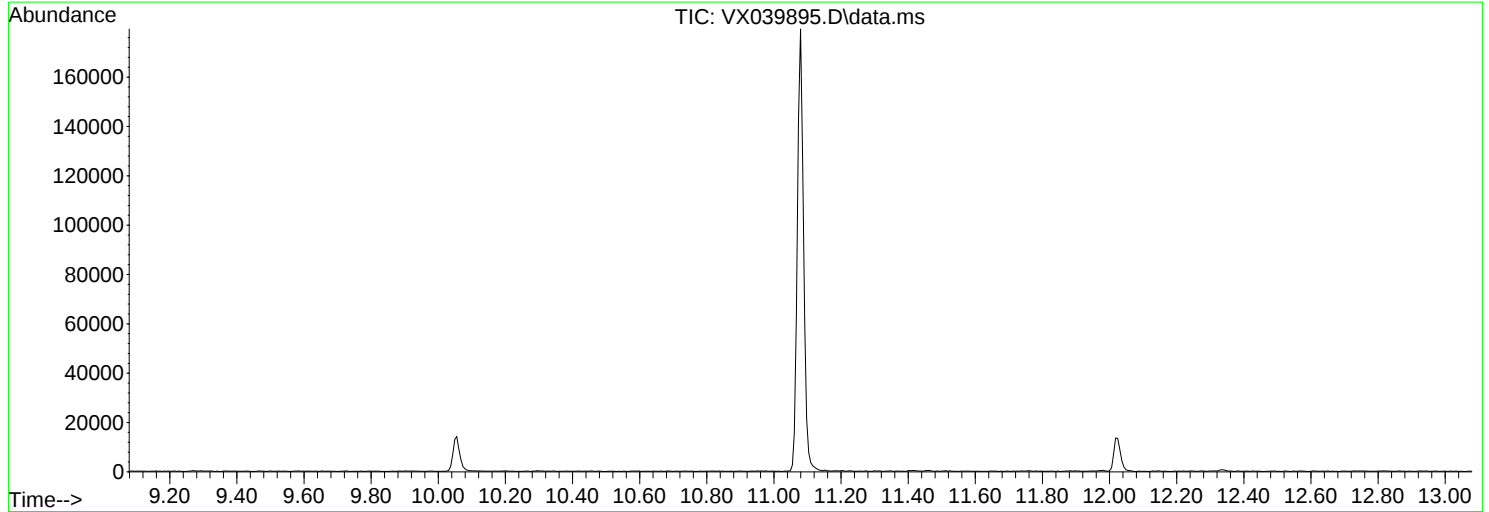

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	6589	PASS
75	95	30	60	57.6	17169	PASS
95	95	100	100	100.0	29792	PASS
96	95	5	9	6.7	2007	PASS
173	174	0.00	2	0.8	167	PASS
174	95	50	100	69.3	20651	PASS
175	174	5	9	7.7	1595	PASS
176	174	95	101	98.7	20392	PASS
177	176	5	9	6.9	1401	PASS