
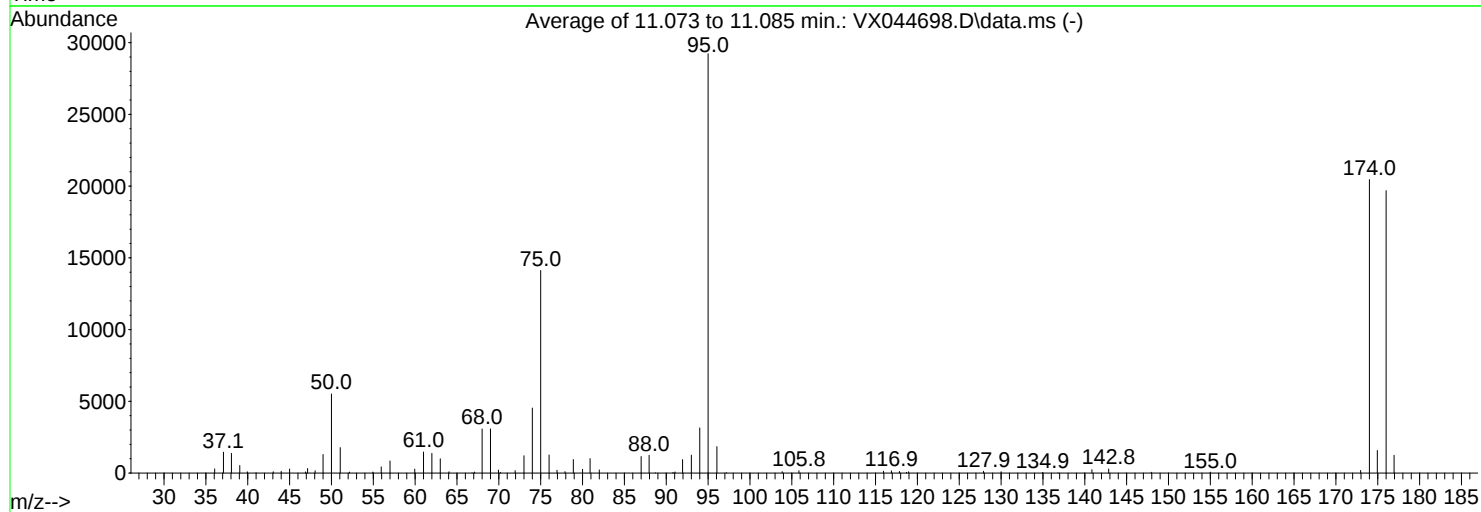


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012325\
Data File : VX044698.D
Acq On : 23 Jan 2025 07:54
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011625W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Jan 17 01:21:41 2025

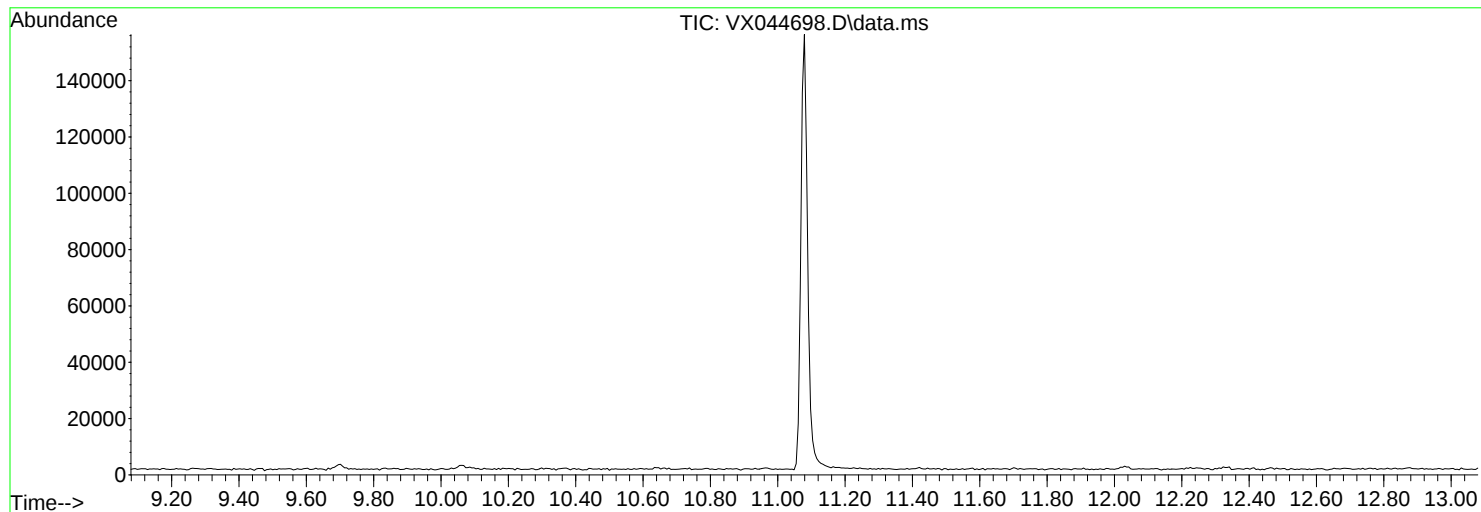

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	5515	PASS
75	95	30	60	48.3	14121	PASS
95	95	100	100	100.0	29227	PASS
96	95	5	9	6.3	1845	PASS
173	174	0.00	2	0.9	183	PASS
174	95	50	100	70.0	20459	PASS
175	174	5	9	7.7	1577	PASS
176	174	95	101	96.2	19685	PASS
177	176	5	9	6.3	1242	PASS