

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012419\
 Data File : VX007207.D
 Acq On : 24 Jan 2019 16:49
 Operator : JC/SP
 Sample : K1016-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TR-05-RO-4-012319

Quant Time: Jan 25 02:24:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 08 14:06:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	540237	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	838536	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	788973	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	380861	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	291665	51.66	ug/l	0.00
Spiked Amount						
			Recovery	=	103.32%	
35) Dibromofluoromethane	5.51	113	260163	48.45	ug/l	0.00
Spiked Amount						
			Recovery	=	96.90%	
50) Toluene-d8	8.71	98	1006348	51.20	ug/l	0.00
Spiked Amount						
			Recovery	=	102.40%	
62) 4-Bromofluorobenzene	11.13	95	353976	51.66	ug/l	0.00
Spiked Amount						
			Recovery	=	103.32%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	2.45	43	29004	10.391	ug/l	97
18) Methyl Acetate	2.78	43	19160	2.370	ug/l	99
20) Methylene Chloride	2.86	84	182366	34.172	ug/l	96
25) 2-Butanone	4.70	43	7822	1.959	ug/l	94
43) Isopropyl Acetate	6.46	43	29110	2.361	ug/l	98
95) Naphthalene	13.83	128	49483	1.803	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012419\
Data File : VX007207.D
Acq On : 24 Jan 2019 16:49
Operator : JC/SP
Sample : K1016-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TR-05-RO-4-012319

Quant Time: Jan 25 02:24:28 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 08 14:06:59 2019
Response via : Initial Calibration

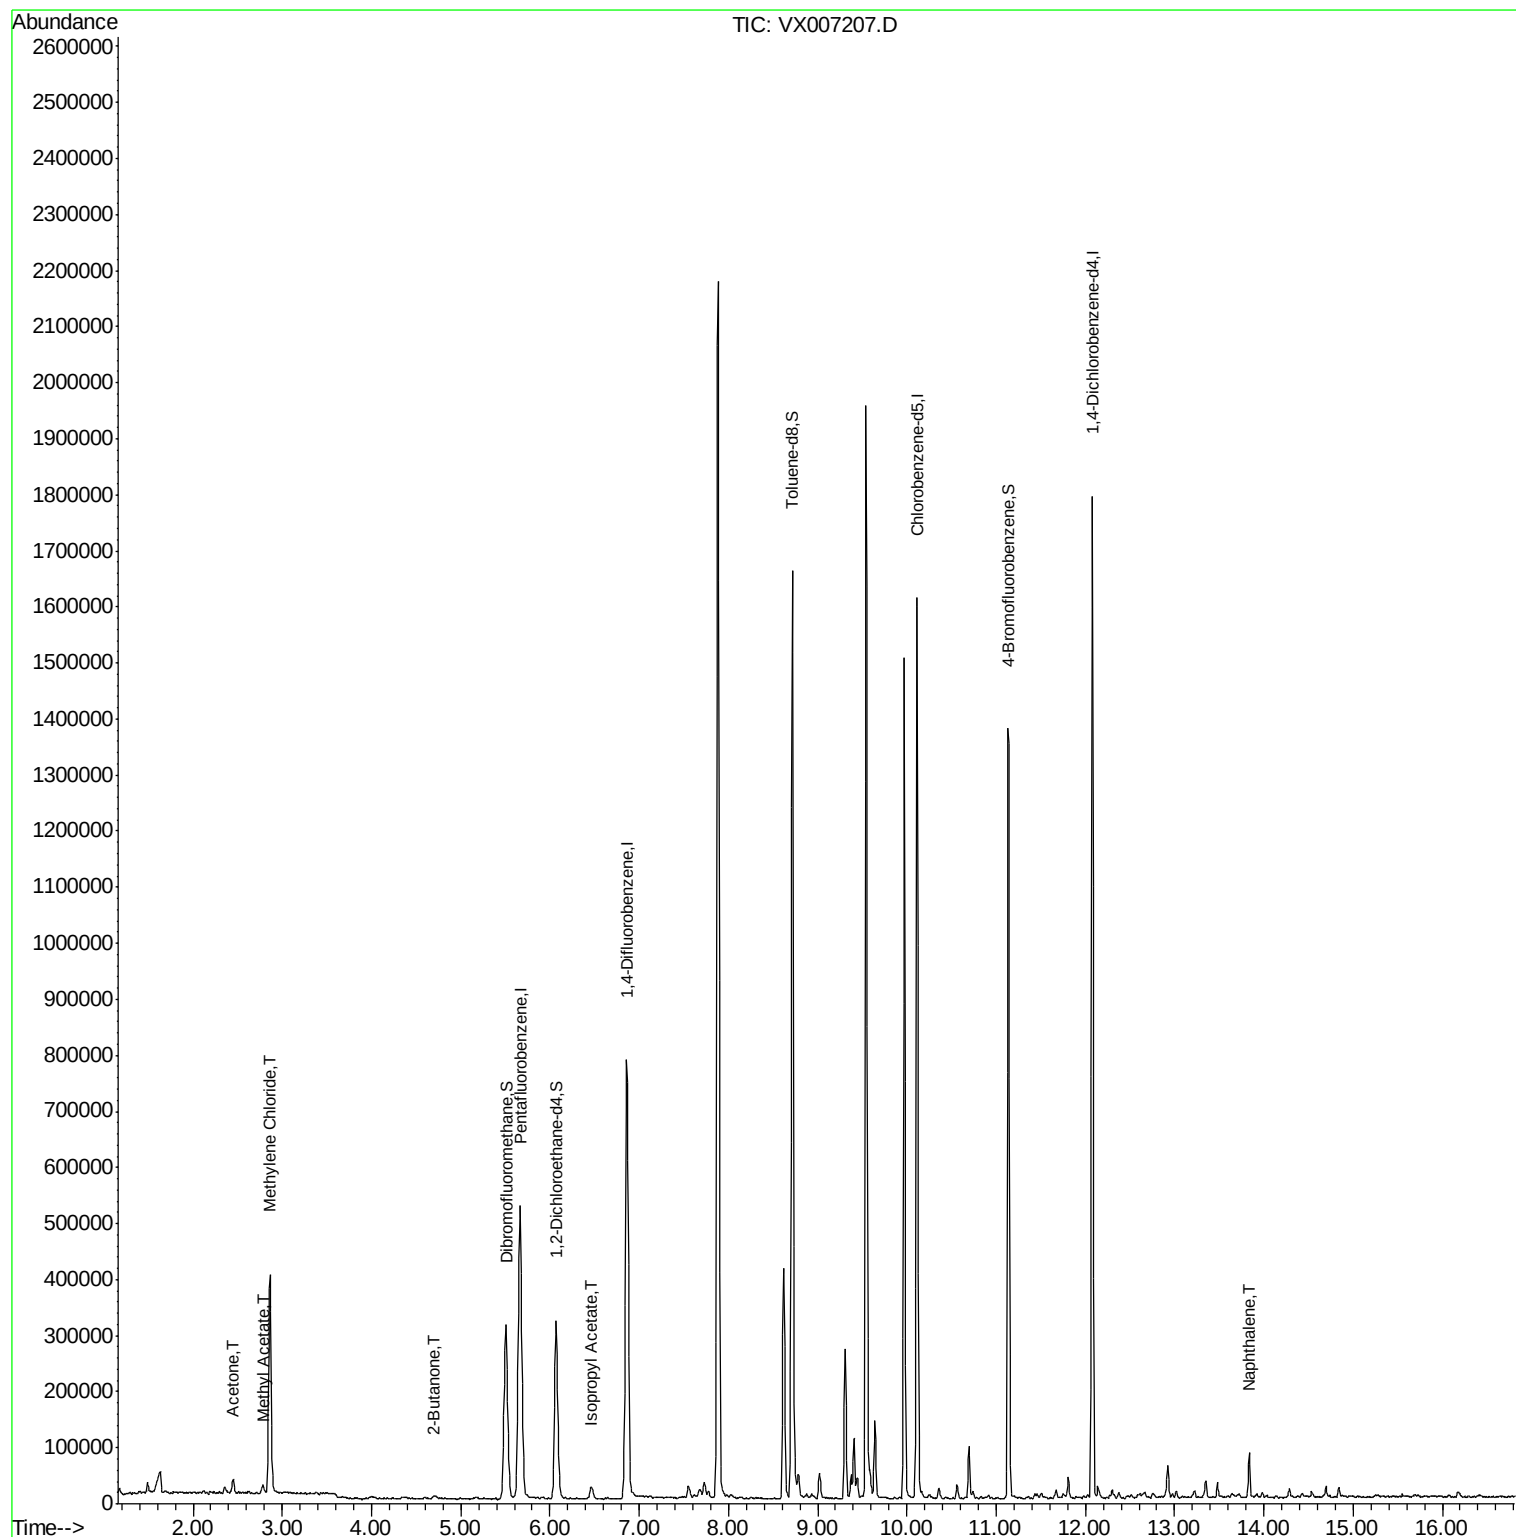

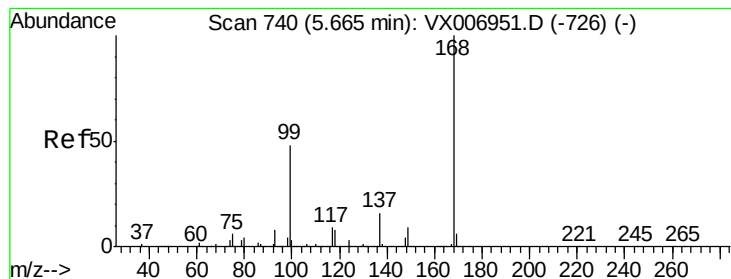

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX007207.D

Acq: 24 Jan 2019 16:49

Instrument :

MSVOA_X

ClientSampleId :


TR-05-RO-4-012319

Tot Ion:168 Resp: 540237

Ion Ratio Lower Upper

168 100

99 49.6 41.8 62.8

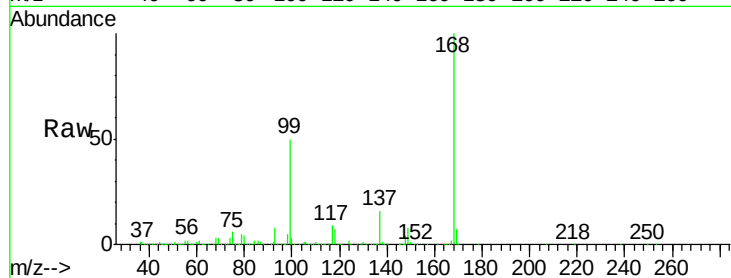

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

200000



150000

100000

50000

0

Time--> 5.50 5.60 5.70 5.80

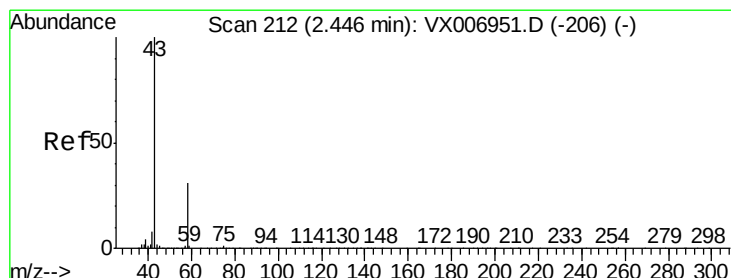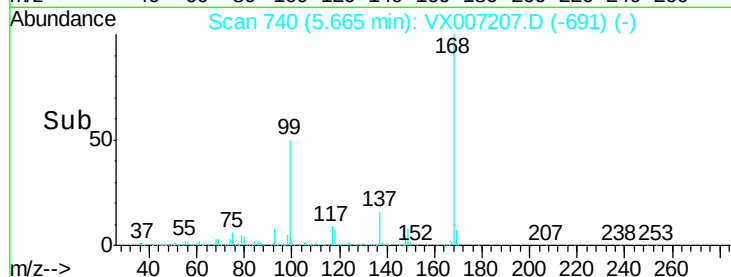

#16

Acetone

Concen: 10.391 ug/l

RT: 2.45 min Scan# 212

Delta R.T. 0.00 min

Lab File: VX007207.D


Acq: 24 Jan 2019 16:49

Tgt Ion: 43 Resp: 29004

Ion Ratio Lower Upper

43 100

58 29.4 25.0 37.6

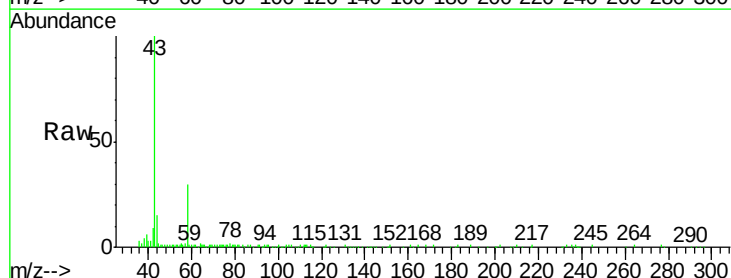

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.45

20000


15000


10000

5000

0

Time--> 2.35 2.40 2.45 2.50




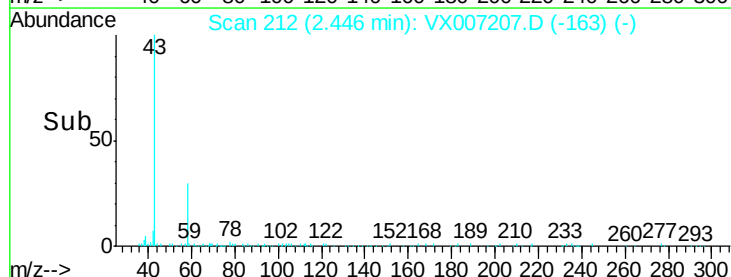


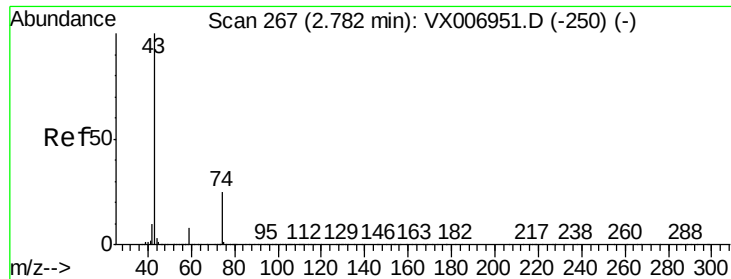

#18
Methyl Acetate
Concen: 2.370 ug/l
RT: 2.78 min Scan# 267
Delta R.T. 0.00 min
Lab File: VX007207.D
Acq: 24 Jan 2019 16:49




Instrument :
MSVOA_X
ClientSampleId :
TR-05-RO-4-012319


Tot Ion: 43 Resp: 19160
Ion Ratio Lower Upper
43 100
74 22.6 18.6 28.0

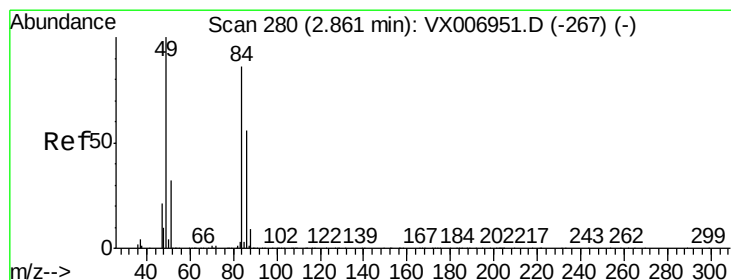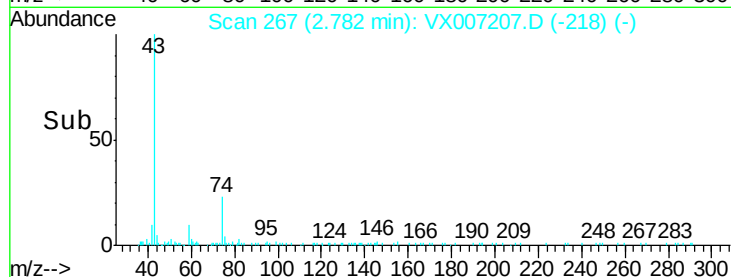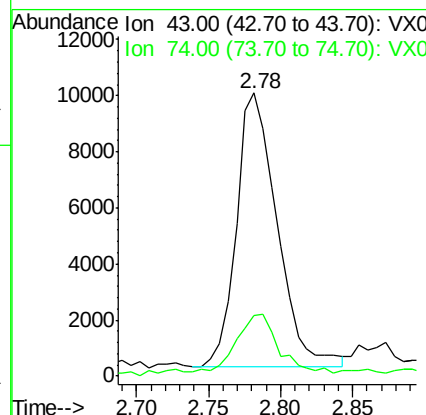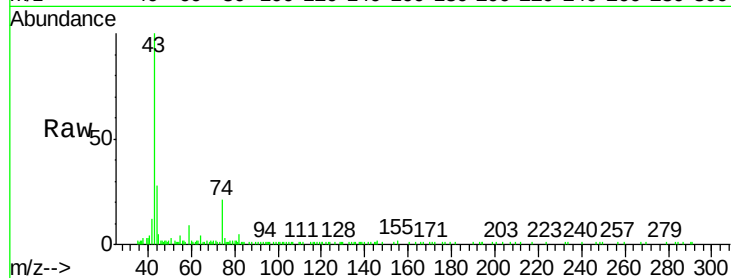

#20
Methylene Chloride
Concen: 34.172 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.00 min
Lab File: VX007207.D
Acq: 24 Jan 2019 16:49

Tgt Ion: 84 Resp: 182366
Ion Ratio Lower Upper
84 100
49 119.8 91.8 137.6
51 35.5 28.5 42.7
86 65.5 50.2 75.2


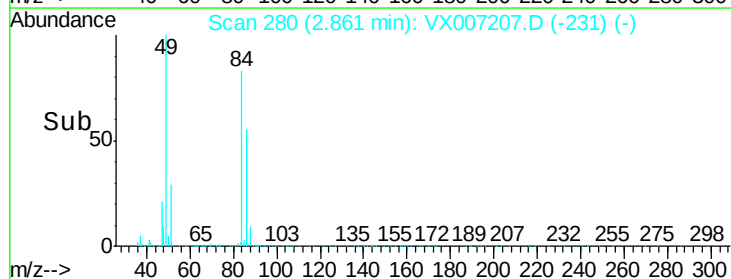
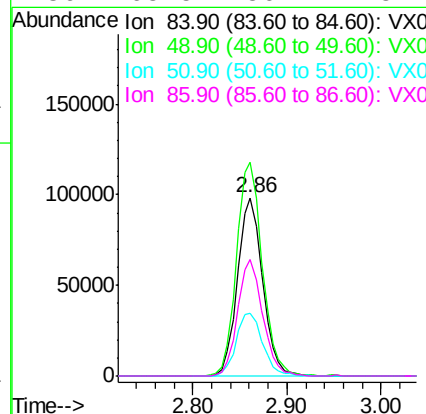
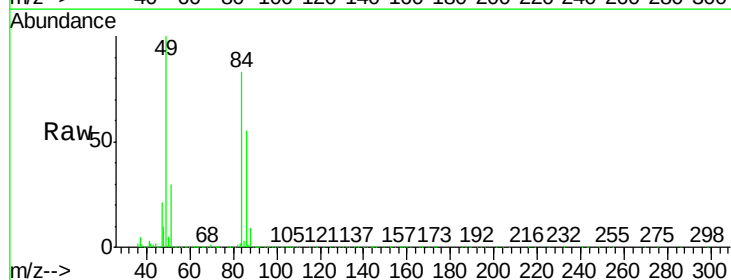


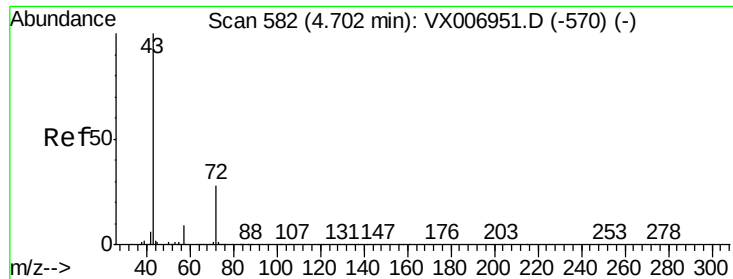

#25
2-Butanone
Concen: 1.959 ug/l
RT: 4.70 min Scan# 581
Delta R.T. -0.01 min
Lab File: VX007207.D
Acq: 24 Jan 2019 16:49




Instrument :
MSVOA_X
ClientSampleId :
TR-05-RO-4-012319


Tot Ion: 43 Resp: 7822
Ion Ratio Lower Upper
43 100
72 24.9 22.4 33.6

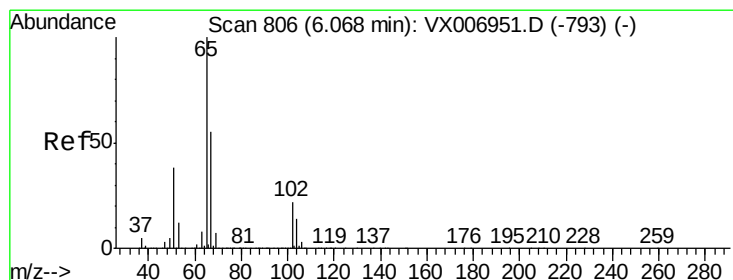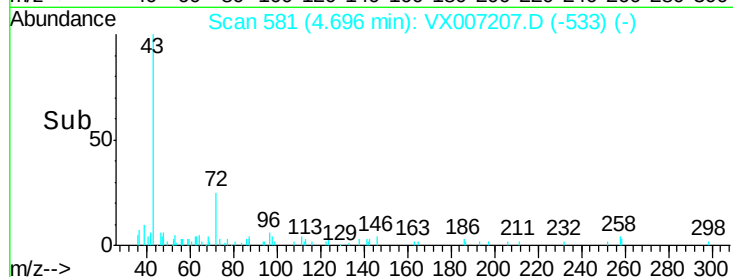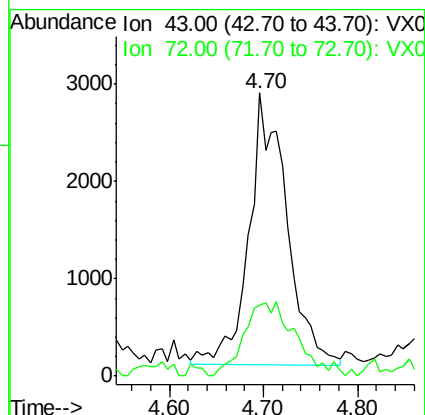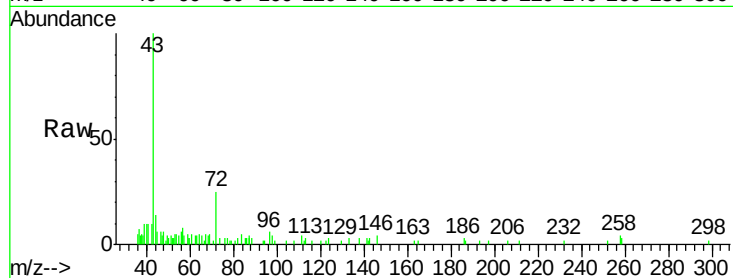

#33
1,2-Dichloroethane-d4
Concen: 51.659 ug/l
RT: 6.07 min Scan# 806
Delta R.T. 0.00 min
Lab File: VX007207.D
Acq: 24 Jan 2019 16:49

Tgt Ion: 65 Resp: 291665
Ion Ratio Lower Upper
65 100
67 54.4 0.0 105.0

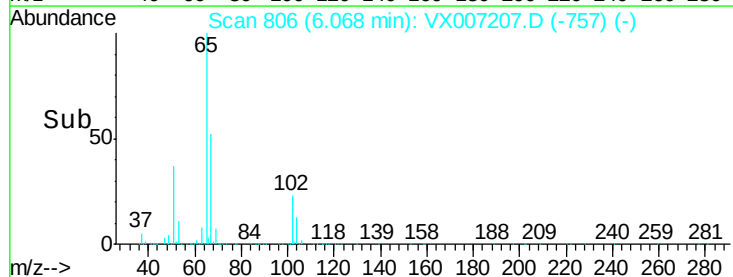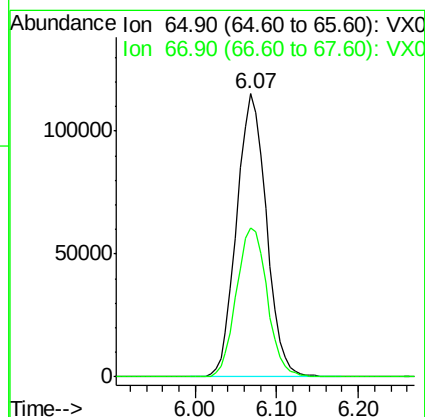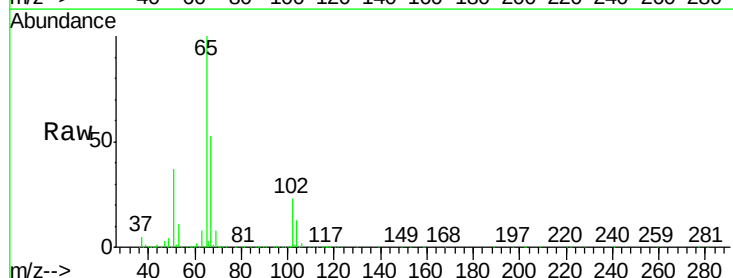

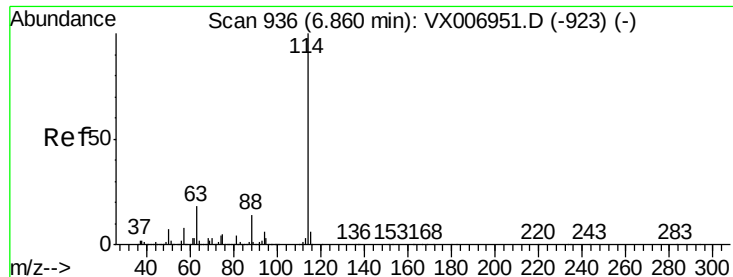

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX007207.D

Acq: 24 Jan 2019 16:49

Instrument :

MSVOA_X

ClientSampleId :

TR-05-RO-4-012319


Tot Ion:114 Resp: 838536

Ion Ratio Lower Upper

114 100

63 18.8 0.0 34.8




88 14.5 0.0 28.8

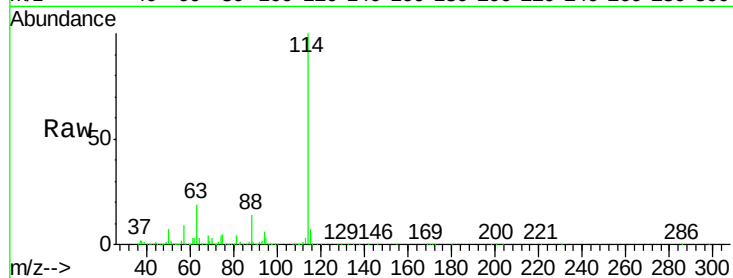

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

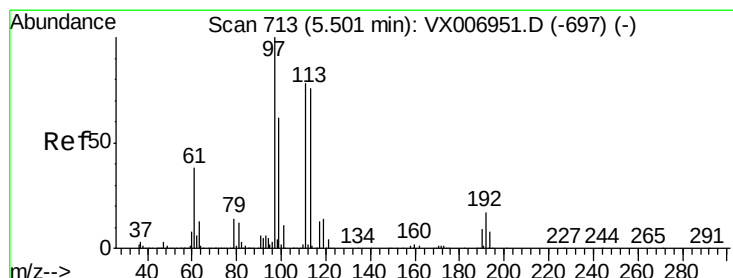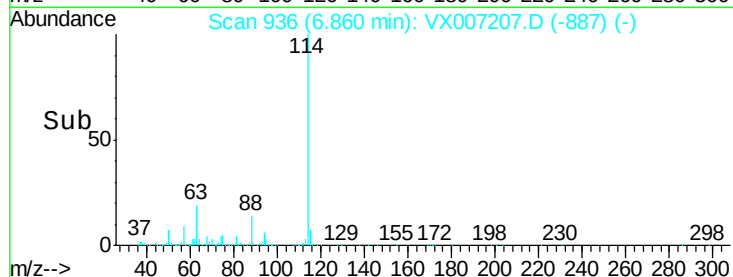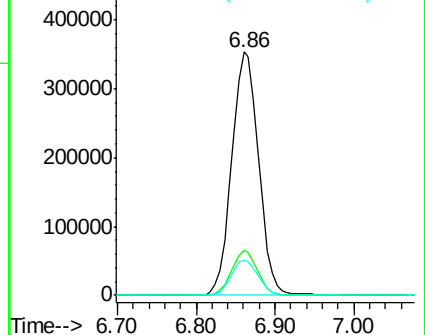

#35

Dibromofluoromethane

Concen: 48.448 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX007207.D

Acq: 24 Jan 2019 16:49


Tgt Ion:113 Resp: 260163

Ion Ratio Lower Upper

113 100

111 101.5 81.6 122.4



192 22.6 16.7 25.1

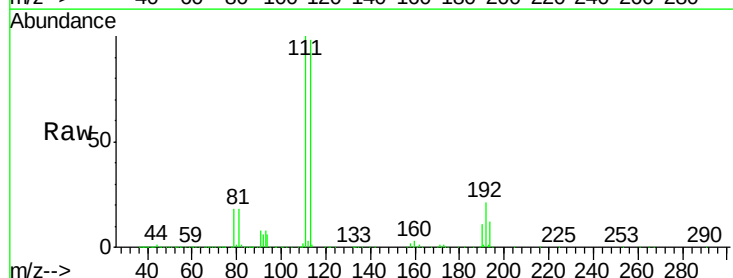


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

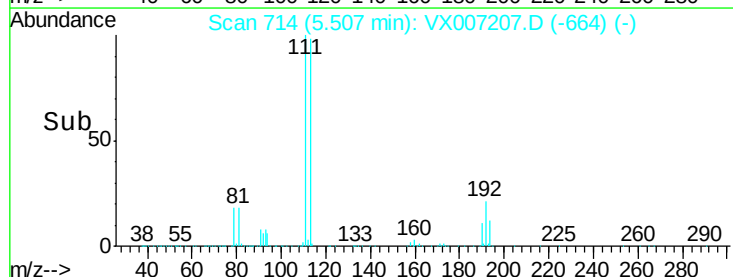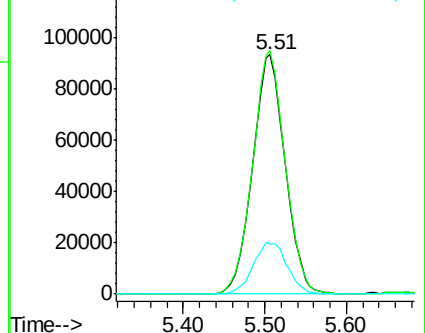

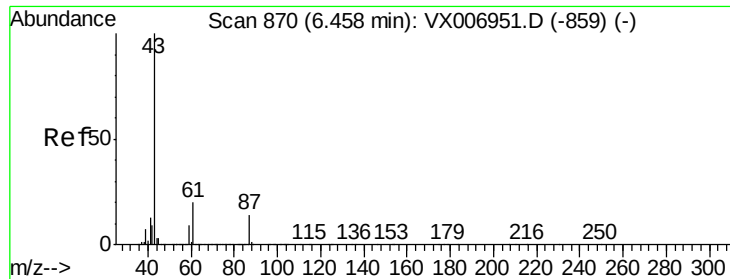

#43

Isopropyl Acetate

Concen: 2.361 ug/l

RT: 6.46 min Scan# 870

Delta R.T. 0.00 min

Lab File: VX007207.D

Acq: 24 Jan 2019 16:49

Instrument :

MSVOA_X

ClientSampleId :

TR-05-RO-4-012319


Tot Ion: 43 Resp: 29110

Ion Ratio Lower Upper

43 100

61 20.9 16.8 25.2




87 13.9 12.4 18.6

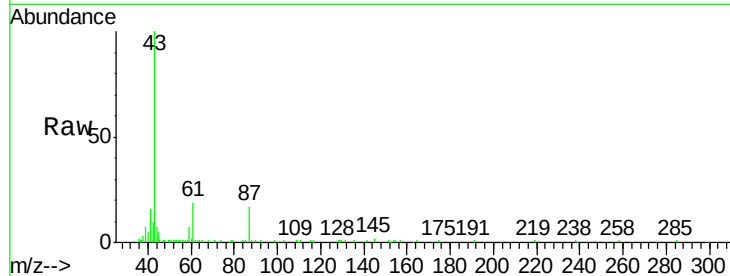

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

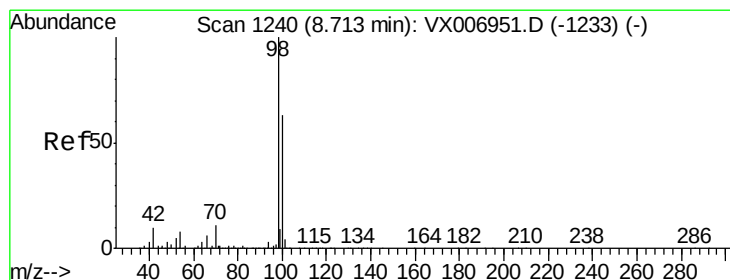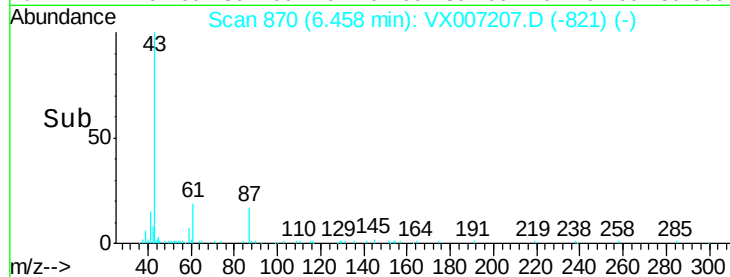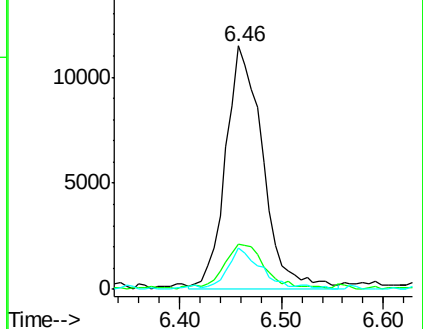

#50

Toluene-d8

Concen: 51.199 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX007207.D


Acq: 24 Jan 2019 16:49

Tgt Ion: 98 Resp: 1006348

Ion Ratio Lower Upper



98 100


100 64.0 52.0 78.0

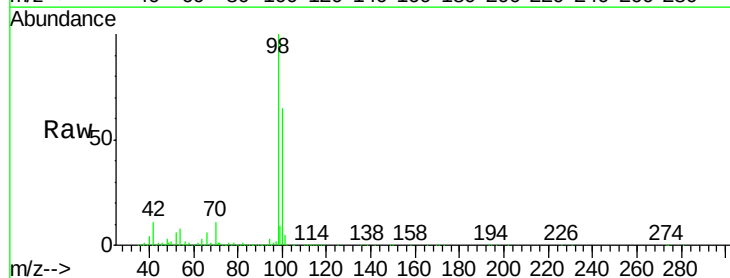

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

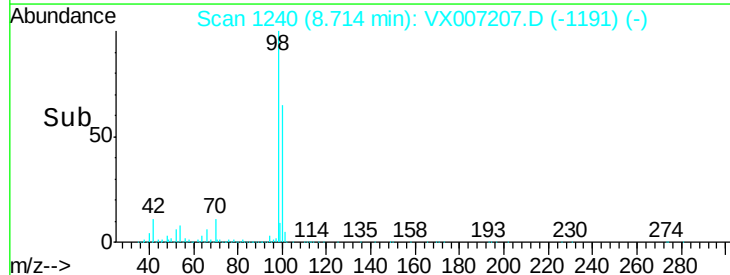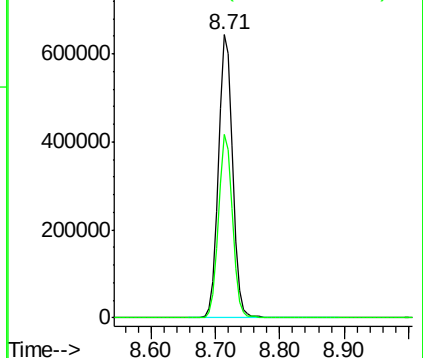

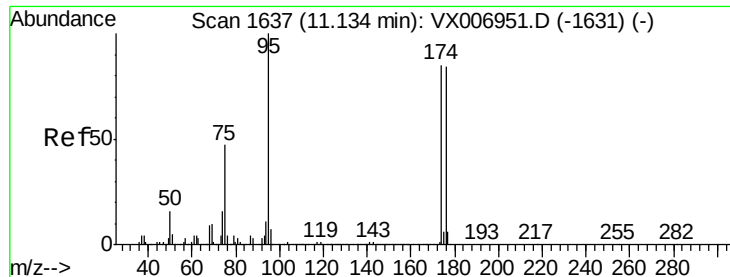

#62

4-Bromofluorobenzene

Concen: 51.657 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX007207.D

Acq: 24 Jan 2019 16:49

Instrument :

MSVOA_X

ClientSampleId :

TR-05-RO-4-012319


Tot Ion: 95 Resp: 353976

Ion Ratio Lower Upper

95 100

174 92.2 0.0 182.2




176 90.5 0.0 178.8

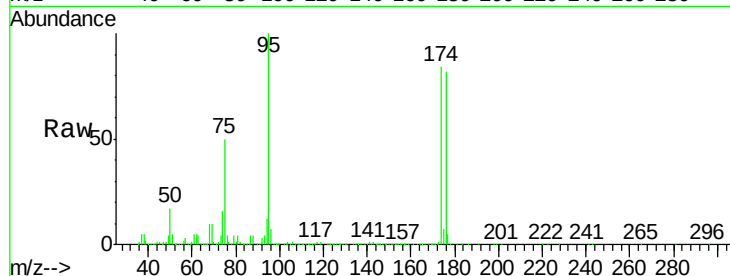

Abundance Ion 94.90 (94.60 to 95.60): VX006951.D (-1631) (-)

Ion 173.80 (173.50 to 174.50): VX006951.D (-1631) (-)

Ion 175.80 (175.50 to 176.50): VX006951.D (-1631) (-)

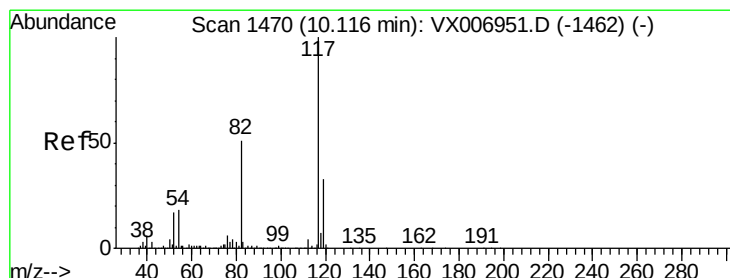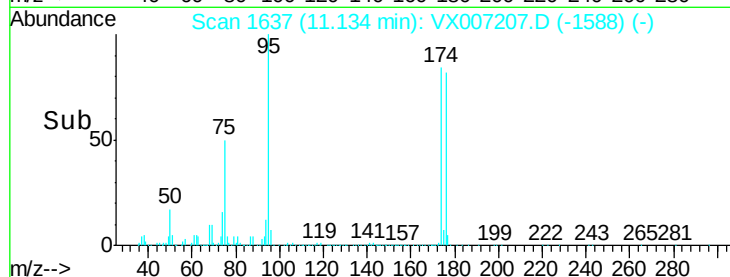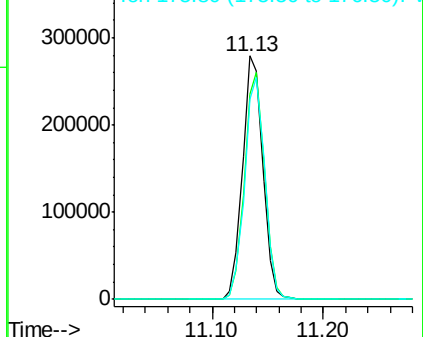

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1470

Delta R.T. 0.00 min

Lab File: VX007207.D

Acq: 24 Jan 2019 16:49


Tgt Ion: 117 Resp: 788973

Ion Ratio Lower Upper

117 100

82 50.3 41.0 61.6



119 32.0 25.4 38.0

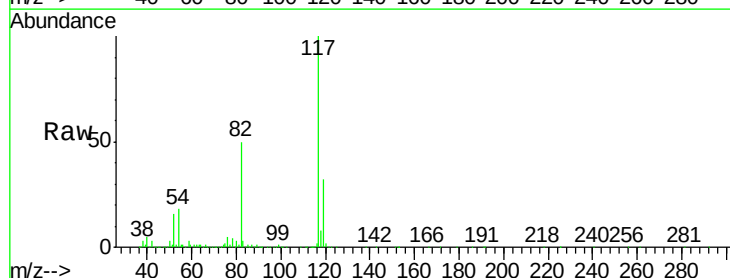


Abundance Ion 116.90 (116.60 to 117.60): VX006951.D (-1462) (-)

Ion 82.00 (81.70 to 82.70): VX006951.D (-1462) (-)

Ion 118.90 (118.60 to 119.60): VX006951.D (-1462) (-)

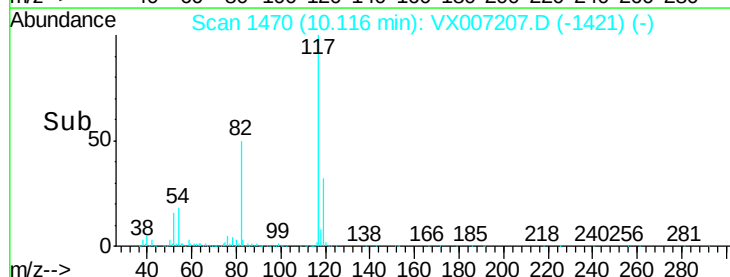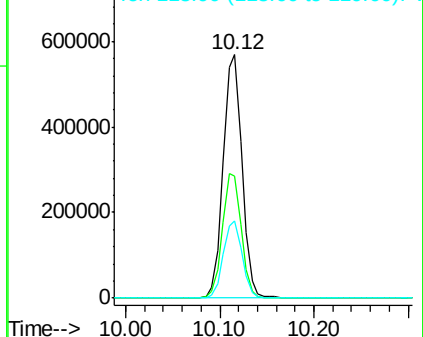

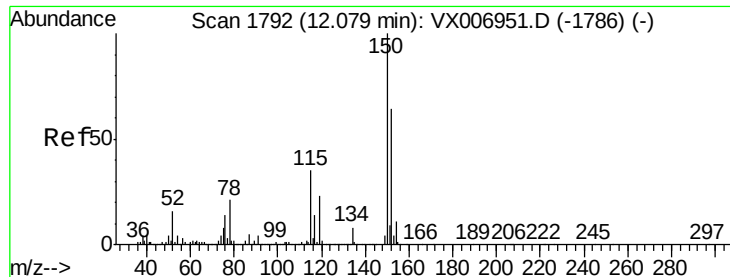

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX007207.D

Acq: 24 Jan 2019 16:49

Instrument :

MSVOA_X

ClientSampleId :

TR-05-RO-4-012319


Tot Ion:152 Resp: 380861

Ion Ratio Lower Upper

152 100

115 54.5 39.1 117.2




150 155.1 0.0 344.8

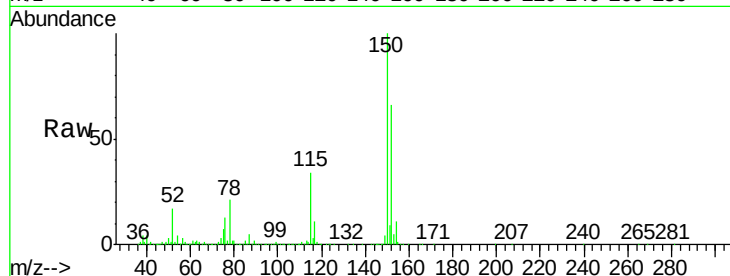

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

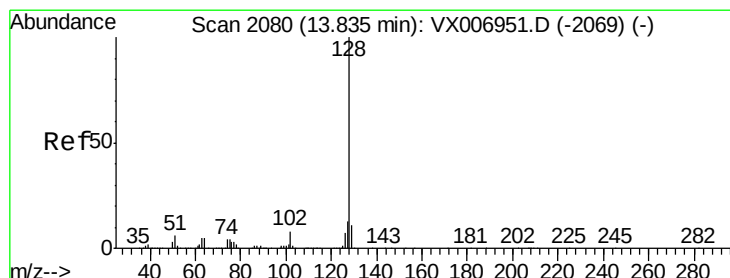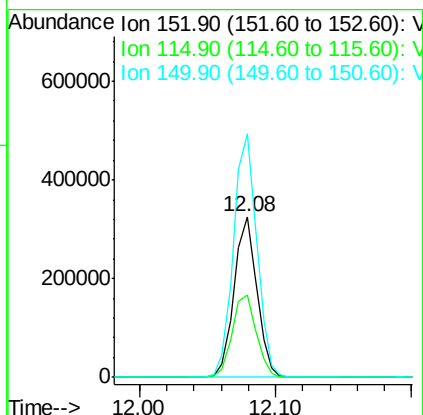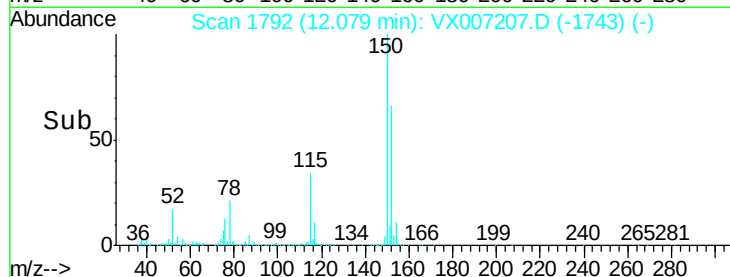

#95

Naphthalene

Concen: 1.803 ug/l

RT: 13.83 min Scan# 2080

Delta R.T. 0.00 min

Lab File: VX007207.D

Acq: 24 Jan 2019 16:49


Tgt Ion:128 Resp: 49483

Ion Ratio Lower Upper

128 100

127 12.7 10.1 15.1

129 11.4 8.6 13.0

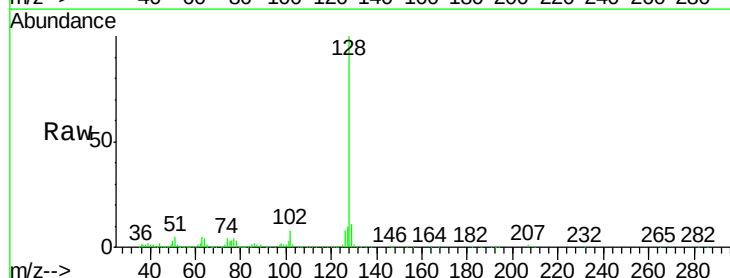

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

