

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012420\
 Data File : VX014706.D
 Acq On : 24 Jan 2020 18:52
 Operator : JC/SP
 Sample : L1173-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 0049-DECANT-H2O-COMP-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	45	rBV	1091685	1319053	64.62%	11.061%
2	1.271	59	63	68	rVB	20441	25702	1.26%	0.216%
3	1.600	110	117	120	rVB9	27064	49543	2.43%	0.415%
4	2.430	248	253	257	rBV	13802	23204	1.14%	0.195%
5	5.490	745	755	770	rBV2	232201	658759	32.27%	5.524%
6	5.655	770	782	792	rBV	404323	1130829	55.40%	9.483%
7	6.057	837	848	858	rBV	259705	680255	33.32%	5.704%
8	6.849	967	978	988	rBV	627980	1473714	72.20%	12.358%
9	8.709	1276	1283	1294	rBV	1312808	2041277	100.00%	17.118%
10	10.111	1507	1513	1519	rBV	1219457	1717376	84.13%	14.402%
11	11.135	1675	1681	1688	rBV	992632	1272381	62.33%	10.670%
12	12.074	1829	1835	1844	rBV	1223778	1511782	74.06%	12.677%
13	12.269	1863	1867	1871	rBV	14481	21053	1.03%	0.177%


Sum of corrected areas: 11924928

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012420\
Data File : VX014706.D
Acq On : 24 Jan 2020 18:52
Operator : JC/SP
Sample : L1173-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
0049-DECANT-H2O-COMP-1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

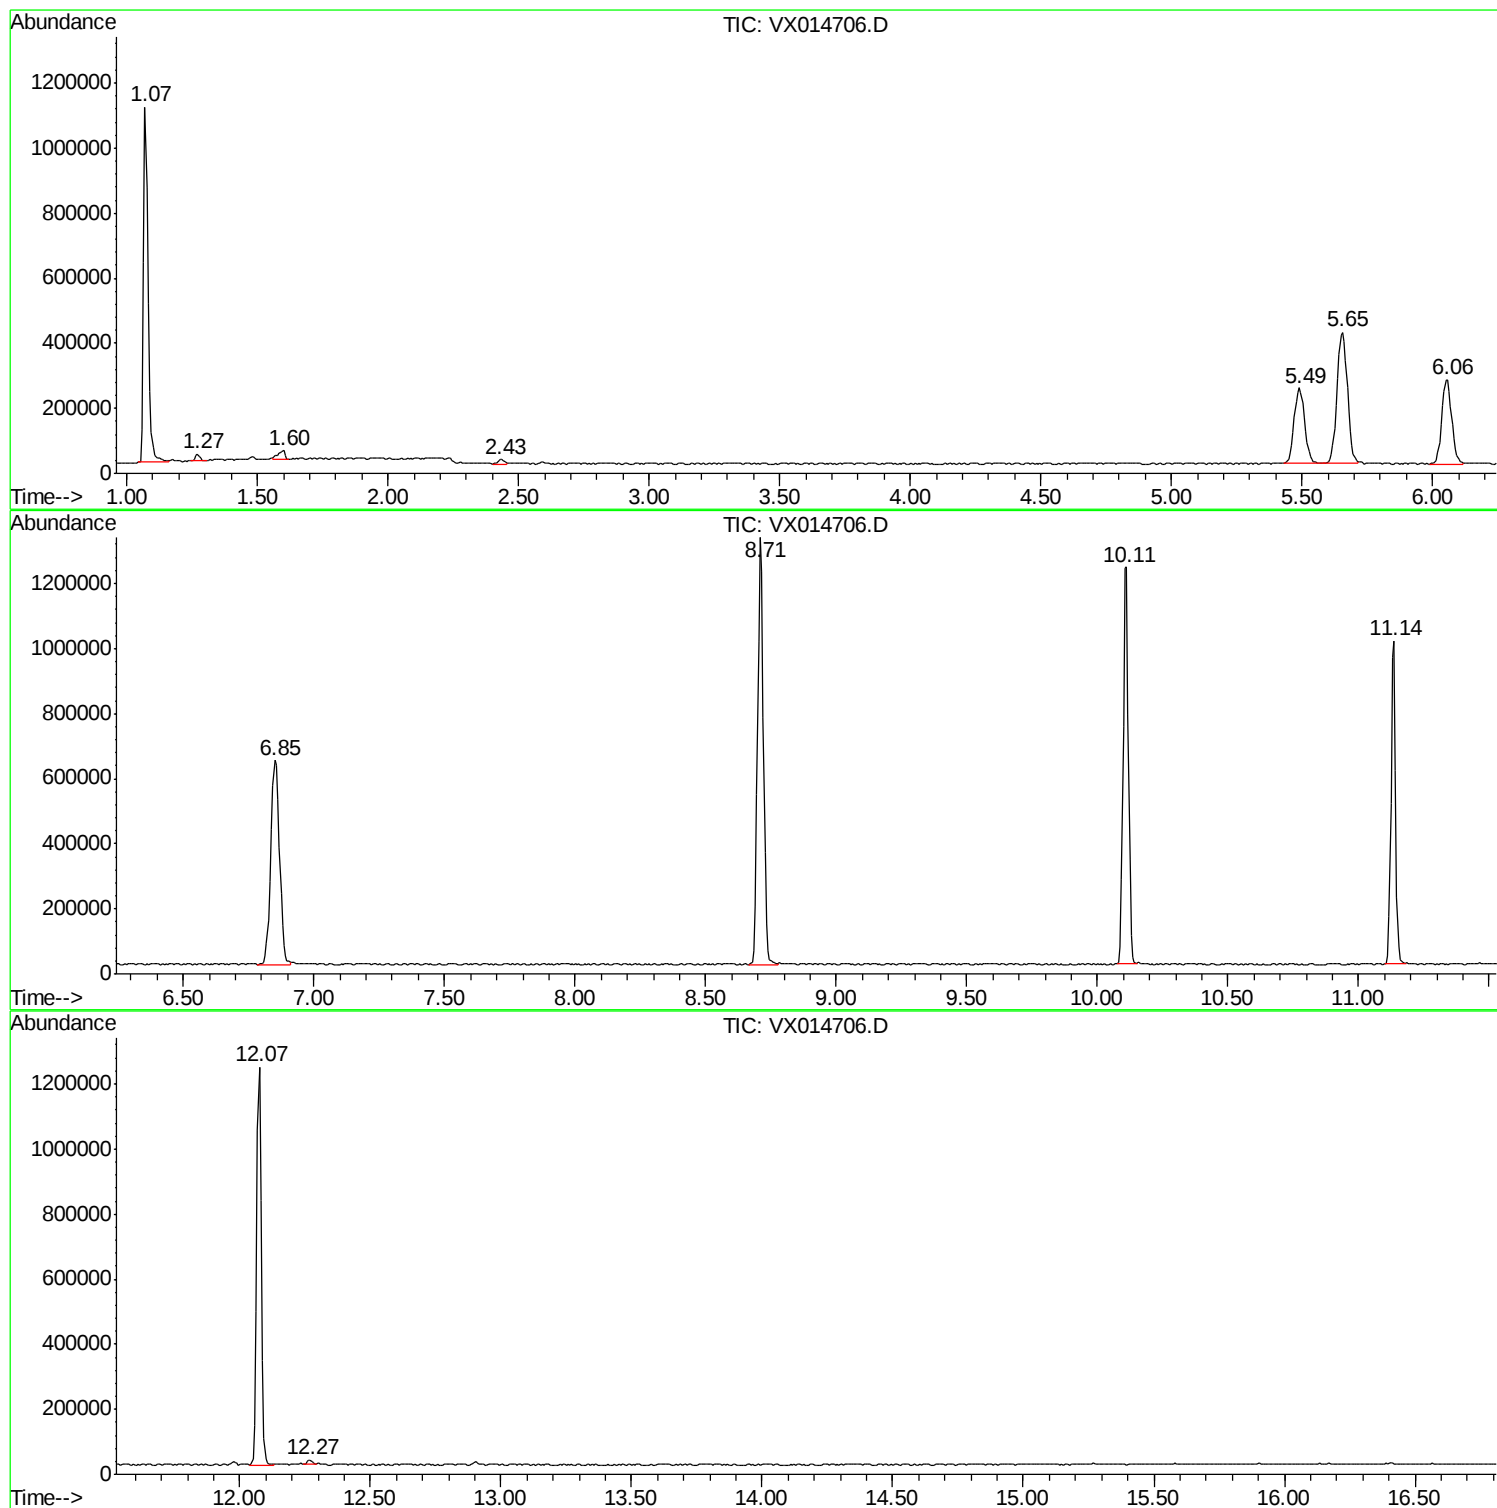

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX012420\
Data File : VX014706.D
Acq On : 24 Jan 2020 18:52
Operator : JC/SP
Sample : L1173-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
0049-DECANT-H2O-COMP-1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX012420\
Data File : VX014706.D
Acq On : 24 Jan 2020 18:52
Operator : JC/SP
Sample : L1173-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
0049-DECANT-H2O-COMP-1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc