

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012422\
 Data File : VX026551.D
 Acq On : 24 Jan 2022 11:08
 Operator : JC/MD
 Sample : VX0124WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0124WBL01

Quant Time: Jan 25 03:24:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	138033	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	230322	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	203942	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	85397	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	90979	47.183	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.360%
35) Dibromofluoromethane	5.385	113	71974	48.391	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.780%
50) Toluene-d8	8.653	98	270232	50.419	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.840%
62) 4-Bromofluorobenzene	11.079	95	95520	50.168	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012422\
Data File : VX026551.D
Acq On : 24 Jan 2022 11:08
Operator : JC/MD
Sample : VX0124WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0124WBL01

Quant Time: Jan 25 03:24:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration




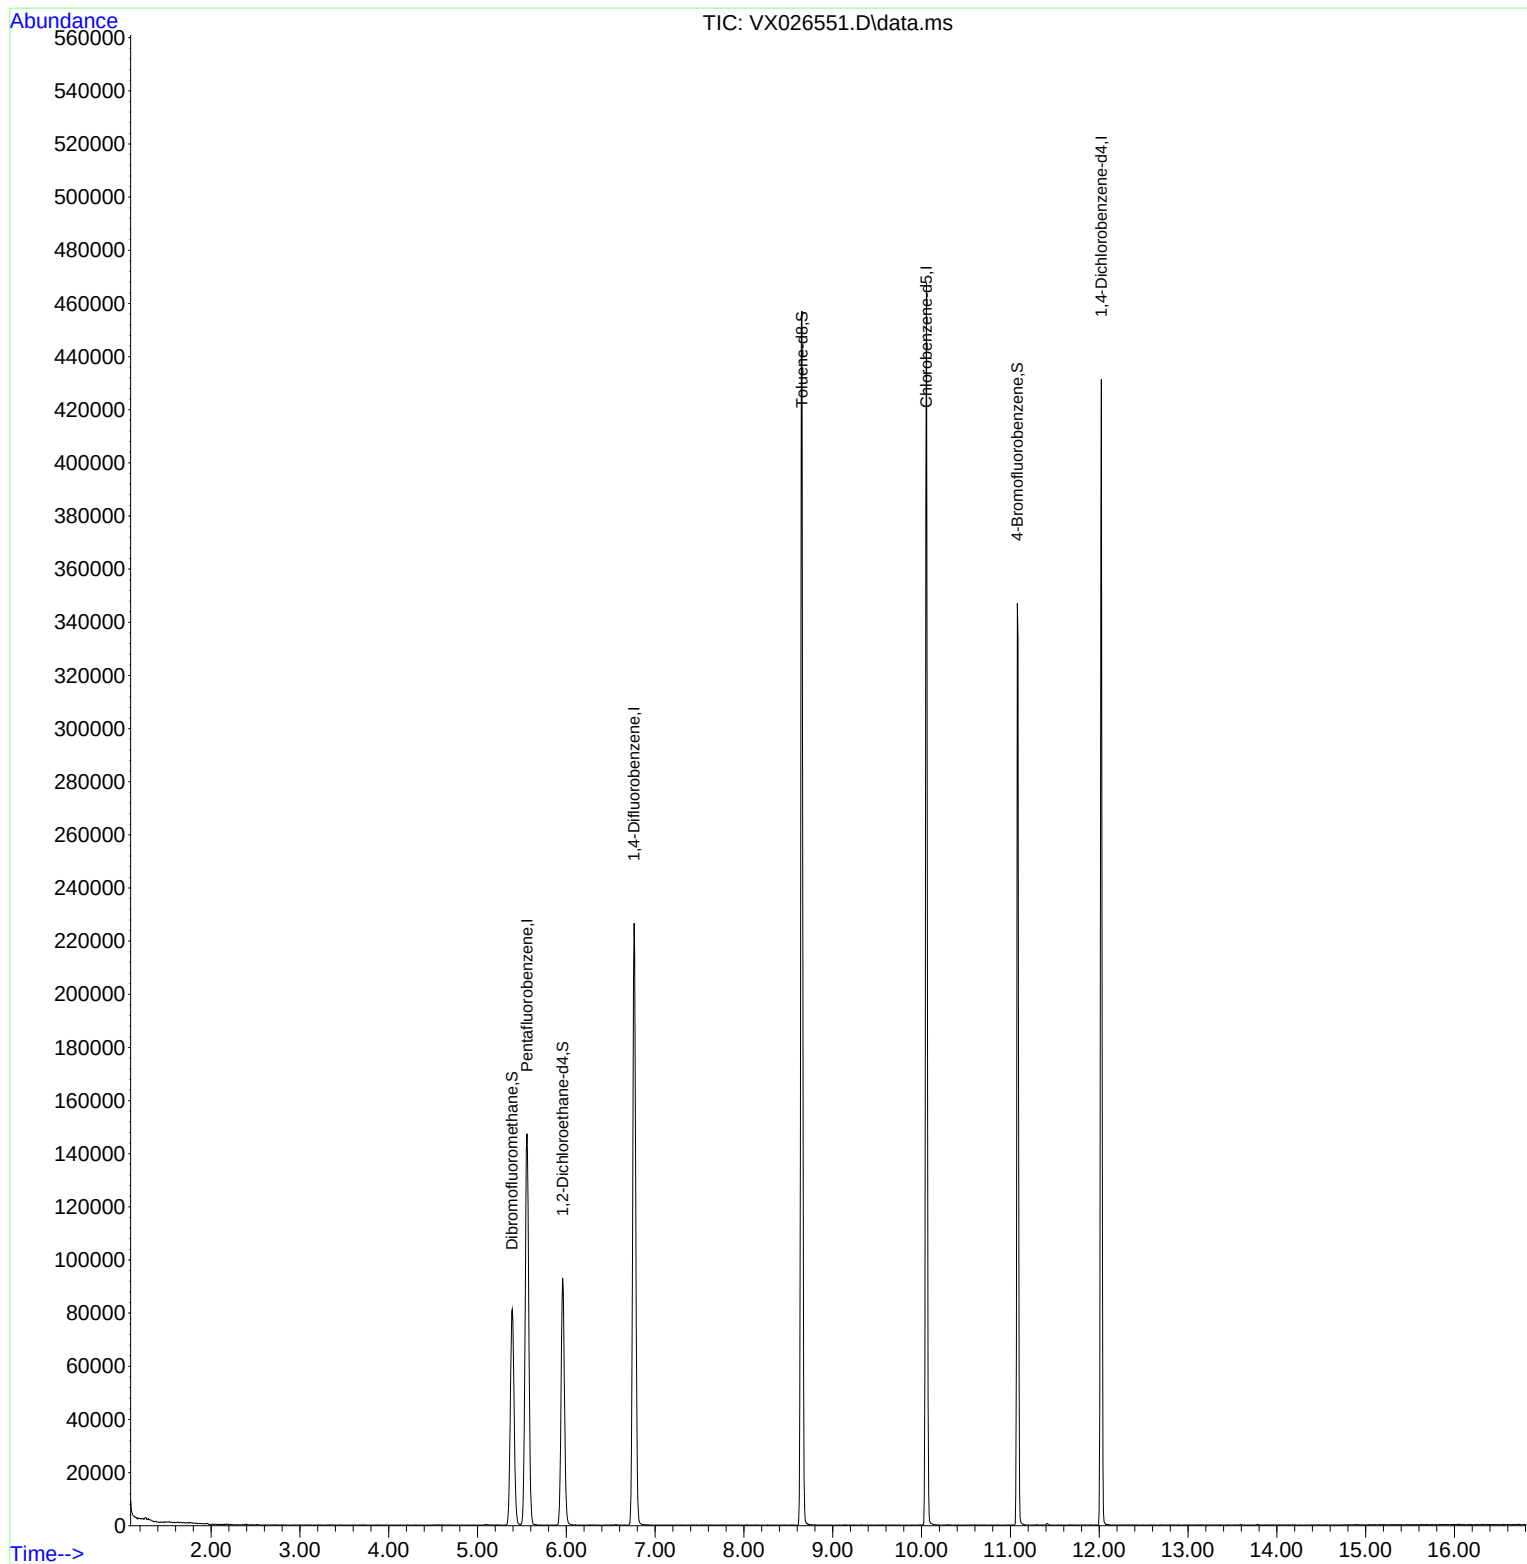


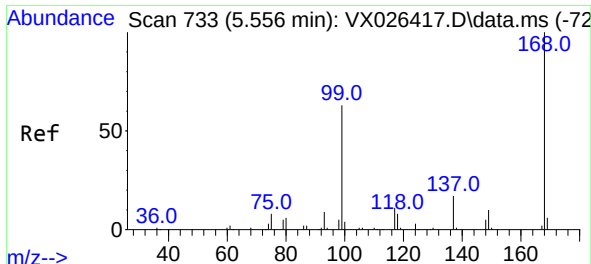

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX026551.D
Acq: 24 Jan 2022 11:08




Instrument :
MSVOA_X
ClientSampleId :
VX0124WBL01


Tgt Ion:168 Resp: 138033
Ion Ratio Lower Upper
168 100
99 60.8 50.3 75.5

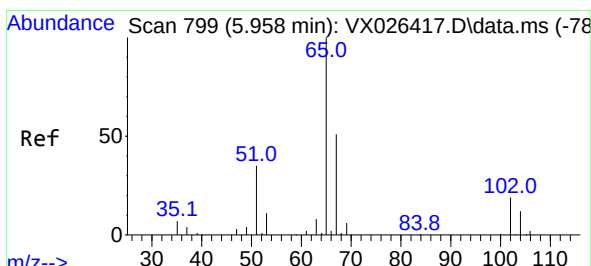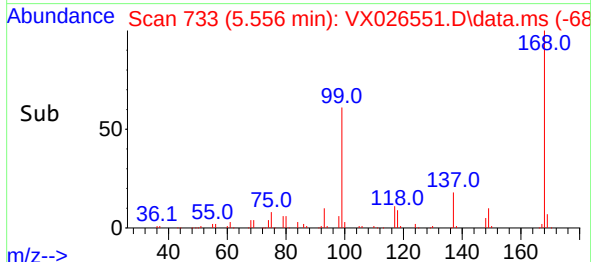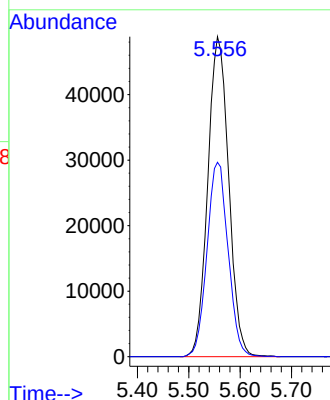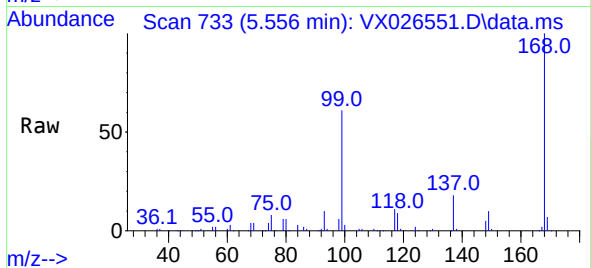

#33
1,2-Dichloroethane-d4
Concen: 47.183 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX026551.D
Acq: 24 Jan 2022 11:08

Tgt Ion: 65 Resp: 90979
Ion Ratio Lower Upper
65 100
67 51.4 0.0 100.8


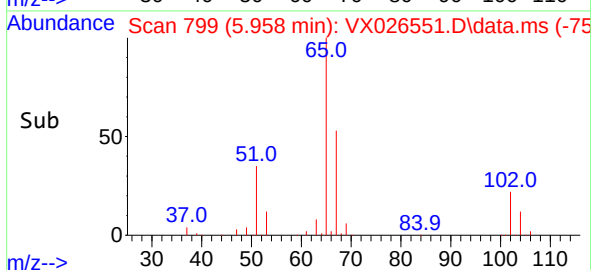
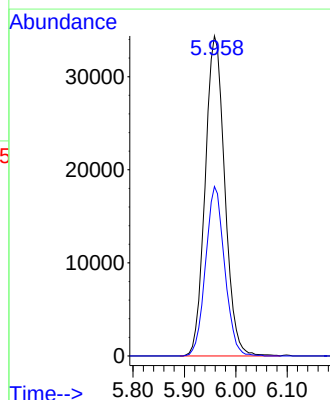
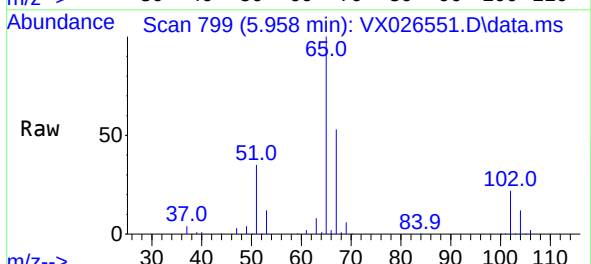


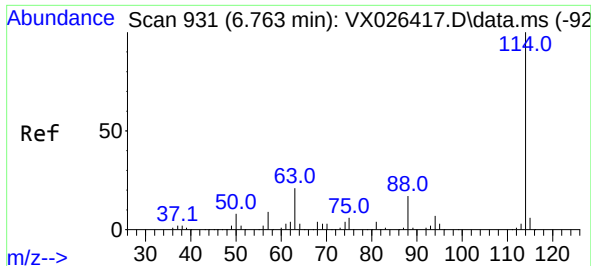

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX026551.D
Acq: 24 Jan 2022 11:08




Instrument :
MSVOA_X
ClientSampleId :
VX0124WBL01


Tgt Ion:114 Resp: 230322
Ion Ratio Lower Upper
114 100
63 21.4 0.0 42.8
88 16.7 0.0 33.0

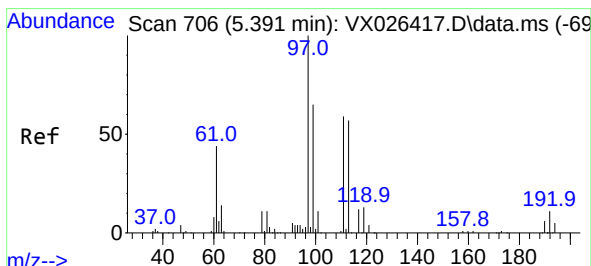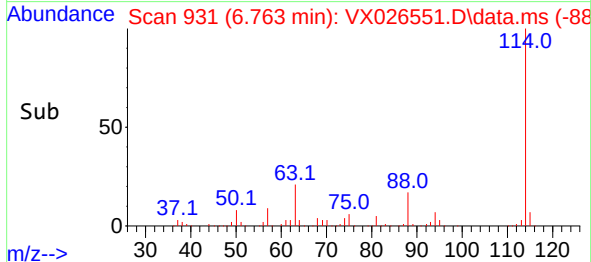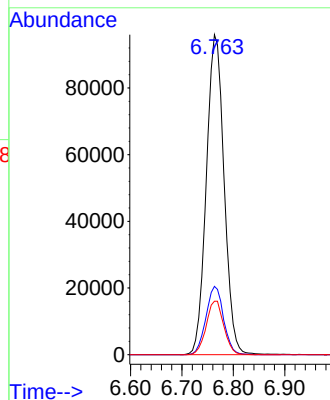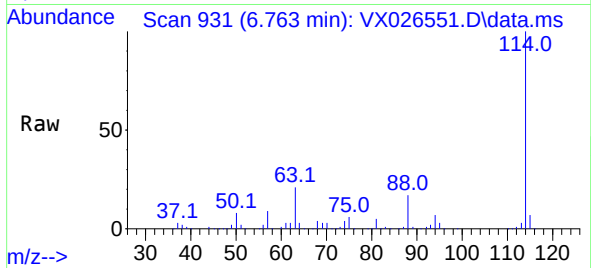

#35
Dibromofluoromethane
Concen: 48.391 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX026551.D
Acq: 24 Jan 2022 11:08

Tgt Ion:113 Resp: 71974
Ion Ratio Lower Upper
113 100
111 104.2 81.2 121.8
192 19.4 15.0 22.4


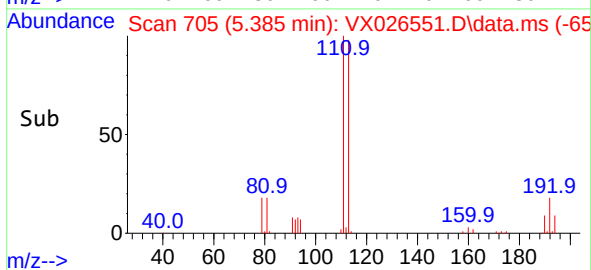
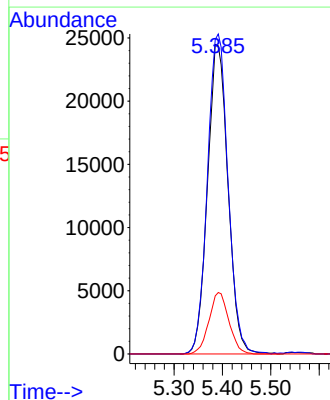
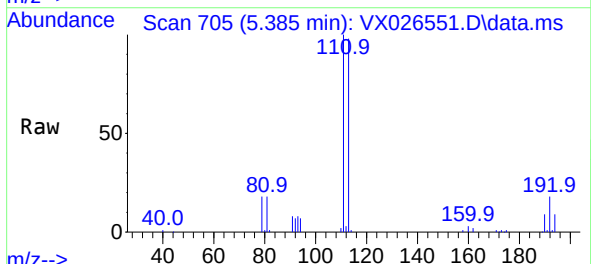


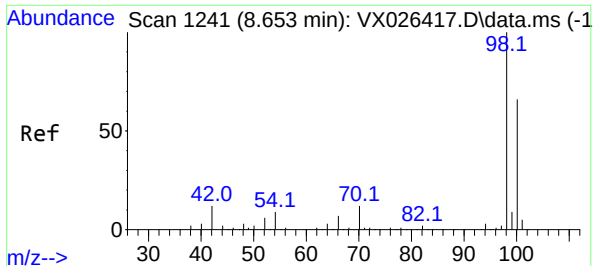

#50
Toluene-d8
Concen: 50.419 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026551.D
Acq: 24 Jan 2022 11:08




Instrument :
MSVOA_X
ClientSampleId :
VX0124WBL01


Tgt Ion: 98 Resp: 270232
Ion Ratio Lower Upper
98 100
100 66.0 53.2 79.8

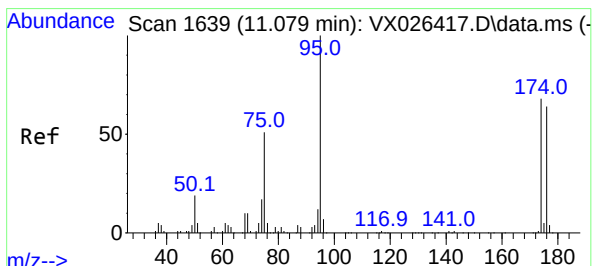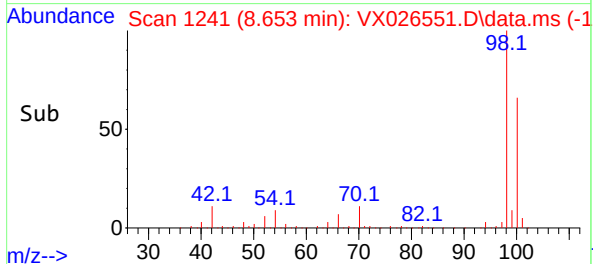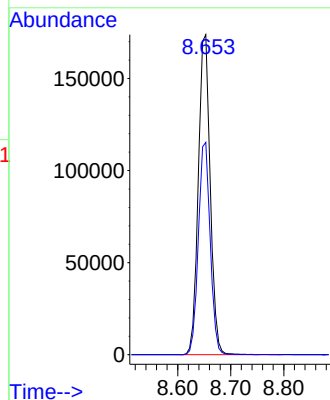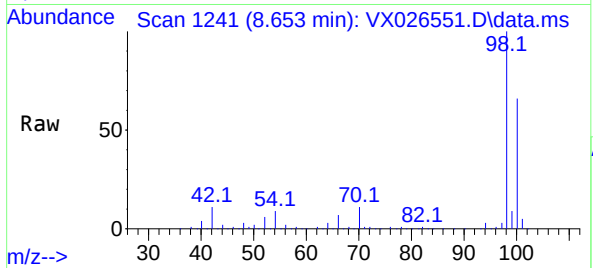

#62
4-Bromofluorobenzene
Concen: 50.168 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026551.D
Acq: 24 Jan 2022 11:08

Tgt Ion: 95 Resp: 95520
Ion Ratio Lower Upper
95 100
174 74.0 0.0 148.6
176 72.7 0.0 141.4


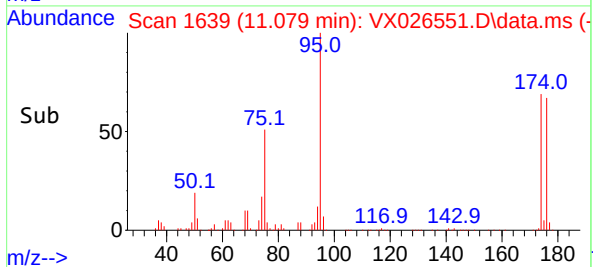
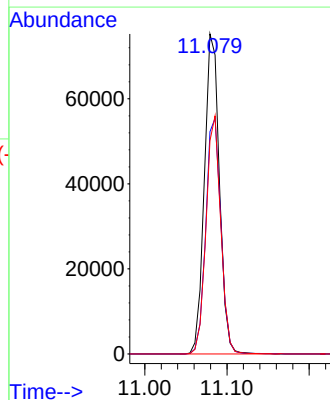
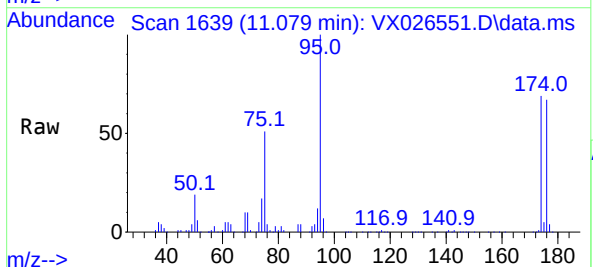


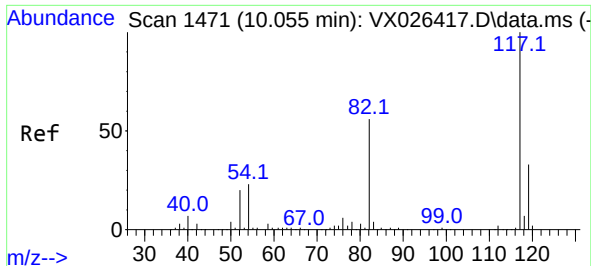

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026551.D
Acq: 24 Jan 2022 11:08

Instrument :
MSVOA_X
ClientSampleId :
VX0124WBL01

Tgt Ion:117 Resp: 203942
Ion Ratio Lower Upper
117 100
82 56.4 45.2 67.8
119 31.6 26.2 39.2

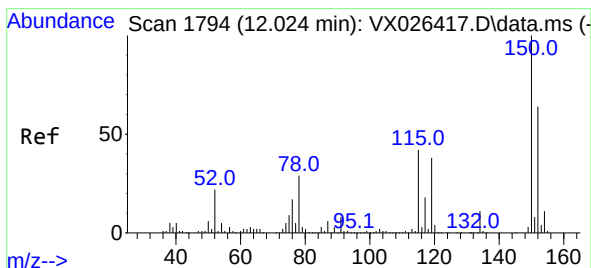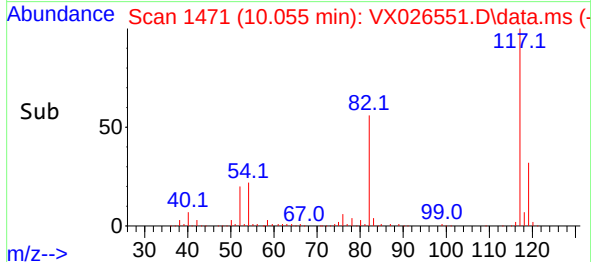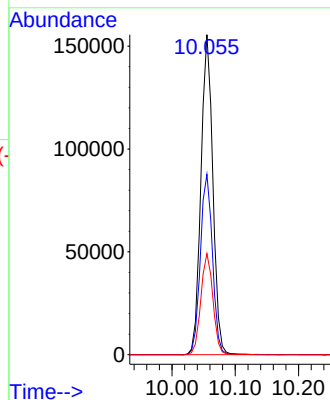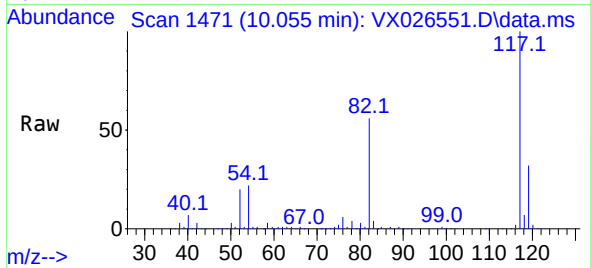

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026551.D
Acq: 24 Jan 2022 11:08

Tgt Ion:152 Resp: 85397
Ion Ratio Lower Upper
152 100
115 61.0 44.2 132.6
150 155.5 0.0 348.2

