

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012423\
 Data File : VX033867.D
 Acq On : 24 Jan 2023 14:25
 Operator : JC/MD
 Sample : 01260-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-21

Quant Time: Jan 25 03:16:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 11 14:48:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	155547	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	227847	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	203321	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	99018	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	75927	46.360	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.720%
35) Dibromofluoromethane	5.385	113	69269	48.960	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.920%
50) Toluene-d8	8.647	98	260432	50.521	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	101.040%
62) 4-Bromofluorobenzene	11.079	95	90137	47.096	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.200%
Target Compounds						
					Qvalue	
16) Acetone	2.386	43	18818	20.231	ug/l	98
17) Carbon Disulfide	2.514	76	250	1.897	ug/l #	76
18) Methyl Acetate	2.709	43	1691	0.740	ug/l	93
20) Methylene Chloride	2.794	84	5430	1.377	ug/l	86
24) 1,1-Dichloroethane	3.605	63	575	0.219	ug/l #	81
25) 2-Butanone	4.586	43	2859	2.672	ug/l	96
31) Cyclohexane	5.556	56	2288	0.949	ug/l #	1
32) 1,1,1-Trichloroethane	5.385	97	1600	0.696	ug/l #	50
36) 1,1-Dichloropropene	5.550	75	9327	4.517	ug/l #	49
37) Ethyl Acetate	4.714	43	20470	7.988	ug/l	99
38) Carbon Tetrachloride	5.556	117	13375	6.254	ug/l #	16
43) Isopropyl Acetate	6.336	43	90398	27.732	ug/l	98
44) Trichloroethene	7.135	130	871	0.518	ug/l	89
48) Methyl methacrylate	7.610	41	2539	1.546	ug/l #	16
49) 1,4-Dioxane	7.793	88	133	3.662	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	65986	32.961	ug/l #	50
53) t-1,3-Dichloropropene	8.951	75	547	0.270	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	31609	13.899	ug/l #	61
56) Ethyl methacrylate	9.244	69	499	0.230	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	3775	1.513	ug/l #	43
59) 2-Hexanone	9.482	43	50264	36.073	ug/l #	50
60) Dibromochloromethane	9.275	129	323	0.203	ug/l #	11
64) Tetrachloroethene	9.275	164	374	Below Cal	#	83
73) Isopropylbenzene	10.969	105	20	Below Cal	#	48
74) N-amyl acetate	10.817	43	549	0.211	ug/l #	42
76) 1,2,3-Trichloropropane	11.079	75	41347	22.727	ug/l #	34
79) 2-Chlorotoluene	11.360	91	21	Below Cal	#	39
81) trans-1,4-Dichloro-2-b...	11.079	75	41347	70.632	ug/l #	8
82) 4-Chlorotoluene	11.451	91	108	Below Cal	#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012423\
Data File : VX033867.D
Acq On : 24 Jan 2023 14:25
Operator : JC/MD
Sample : 01260-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-21

Quant Time: Jan 25 03:16:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 11 14:48:42 2023
Response via : Initial Calibration

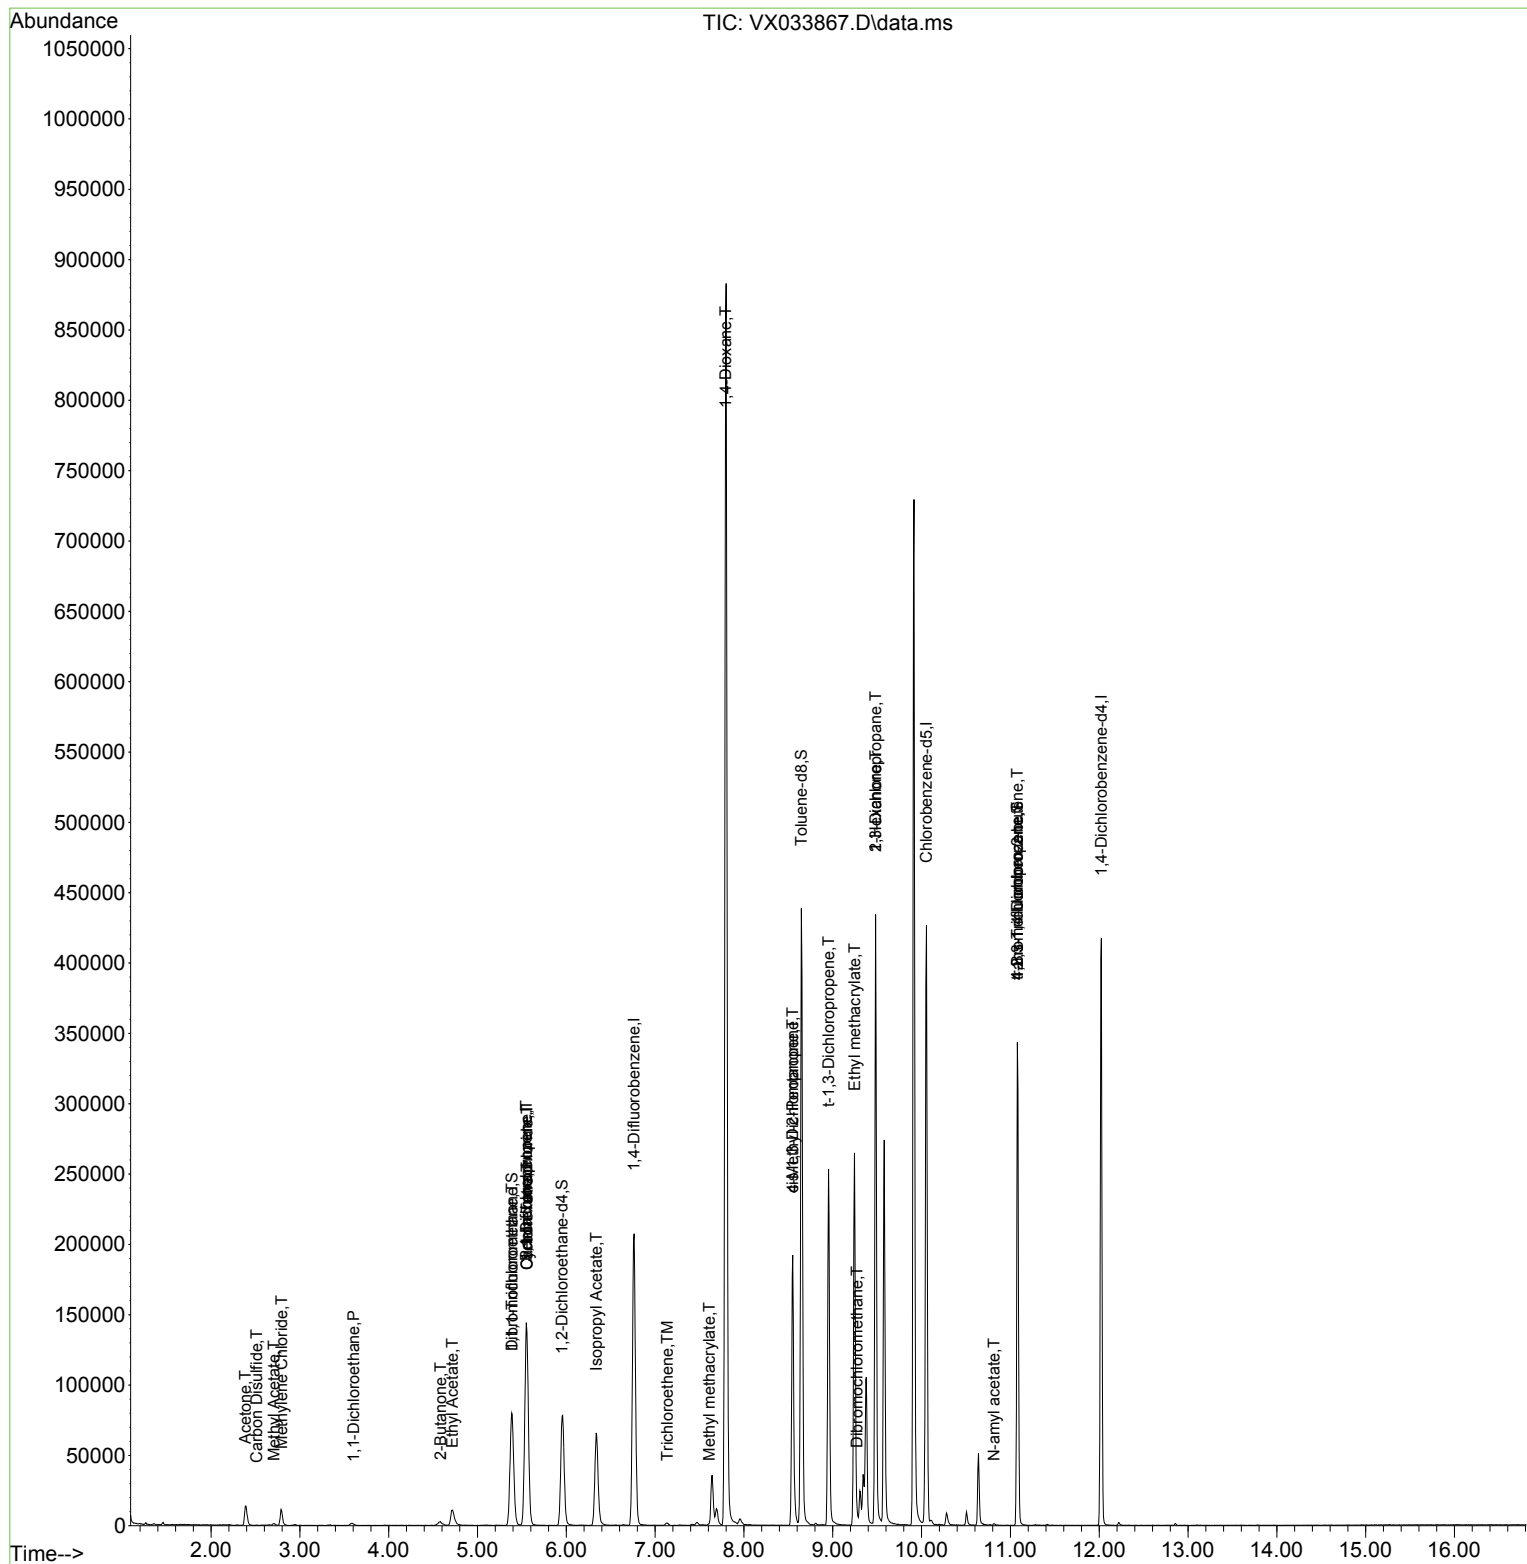



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.000 min

Lab File: VX033867.D

Acq: 24 Jan 2023 14:25

Instrument :

MSVOA_X

ClientSampleId :





TP-21

Tgt Ion:168 Resp: 155547

Ion Ratio Lower Upper

168 100

99 47.2 39.6 59.4

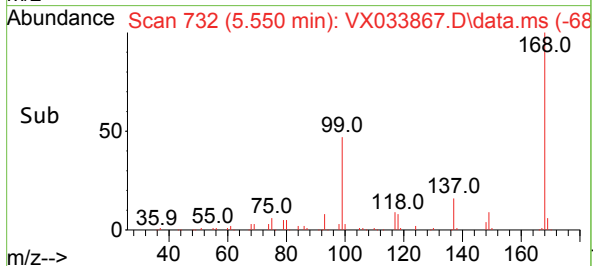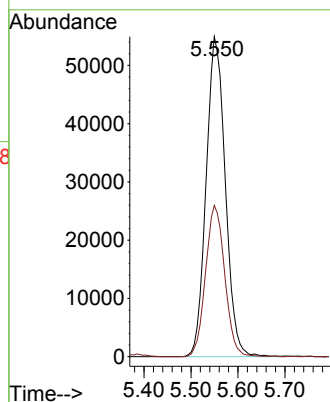

#16

Acetone

Concen: 20.231 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.013 min

Lab File: VX033867.D




Acq: 24 Jan 2023 14:25


Tgt Ion: 43 Resp: 18818

Ion Ratio Lower Upper

43 100

58 27.3 22.6 33.8


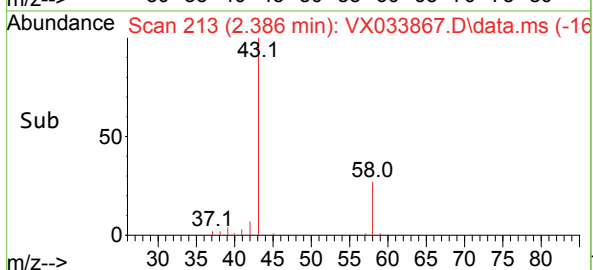

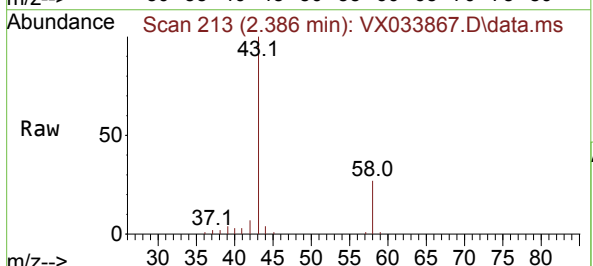


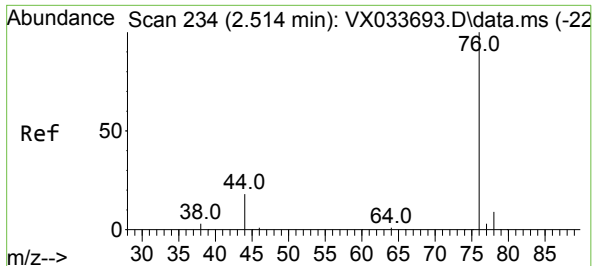

#17
Carbon Disulfide
Concen: 1.897 ug/l
RT: 2.514 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25




Instrument :
MSVOA_X
ClientSampleId :
TP-21


Tgt Ion: 76 Resp: 250
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.6#

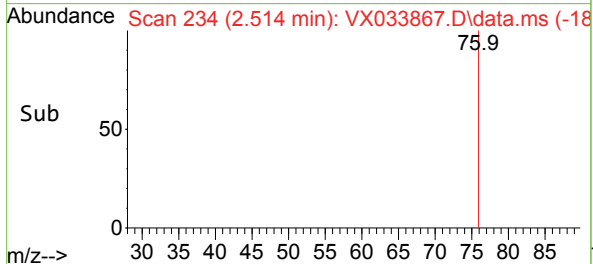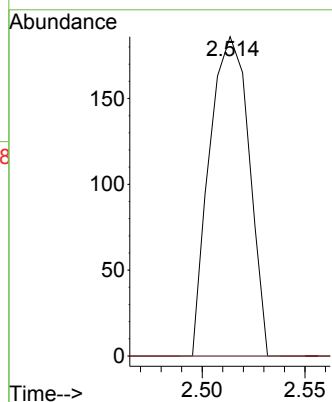

#18
Methyl Acetate
Concen: 0.740 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Tgt Ion: 43 Resp: 1691
Ion Ratio Lower Upper
43 100
74 19.4 18.2 27.4


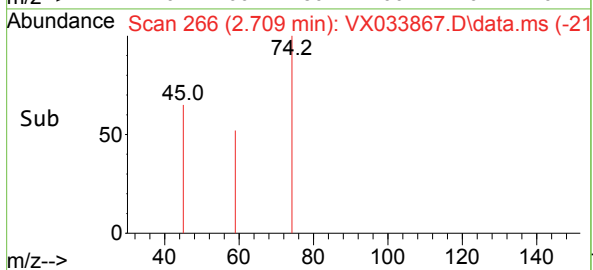
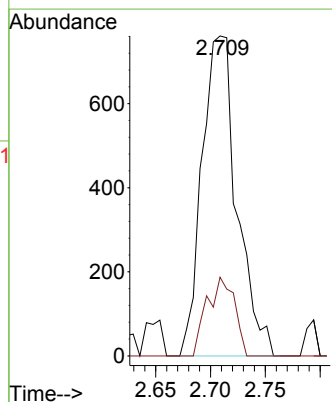
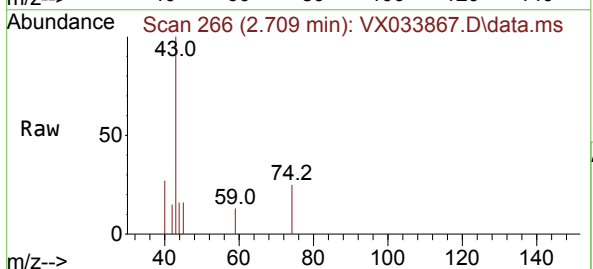




#20
Methylene Chloride
Concen: 1.377 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25




Instrument :
MSVOA_X
ClientSampleId :
TP-21


Tgt Ion:	84	Resp:	5430
Ion	Ratio	Lower	Upper
84	100		
49	104.9	101.1	151.7
51	34.5	31.0	46.6
86	57.8	52.6	79.0

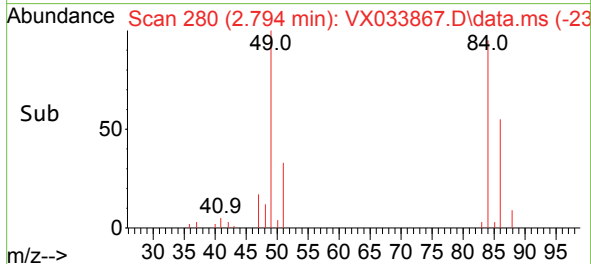

#24
1,1-Dichloroethane
Concen: 0.219 ug/l
RT: 3.605 min Scan# 413
Delta R.T. -0.006 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Tgt Ion:	63	Resp:	575
Ion	Ratio	Lower	Upper
63	100		
98	0.0	3.8	11.2#
100	0.0	2.4	7.2#









#25
2-Butanone
Concen: 2.672 ug/l
RT: 4.586 min Scan# 51
Delta R.T. 0.018 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25




Instrument :
MSVOA_X
ClientSampleId :
TP-21


Tgt Ion: 43 Resp: 2859
Ion Ratio Lower Upper
43 100
72 22.2 19.4 29.2

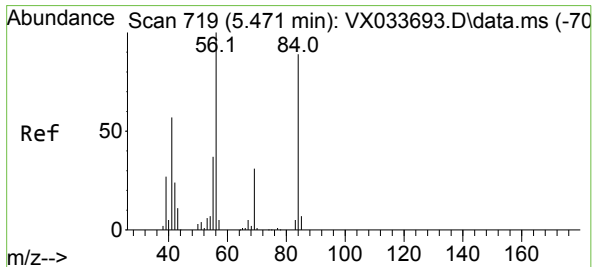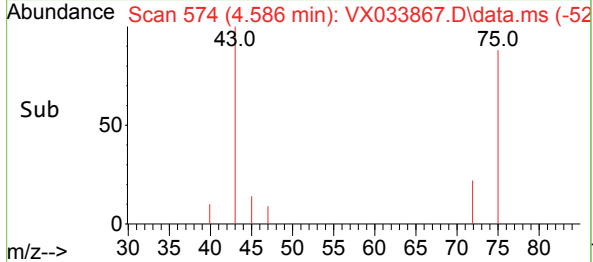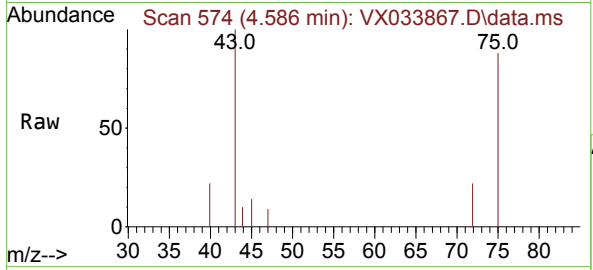

#31
Cyclohexane
Concen: 0.949 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.085 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Tgt Ion: 56 Resp: 2288
Ion Ratio Lower Upper
56 100
69 180.9 24.6 37.0#
84 166.3 71.0 106.6#


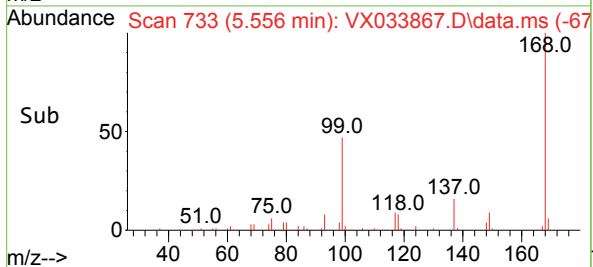

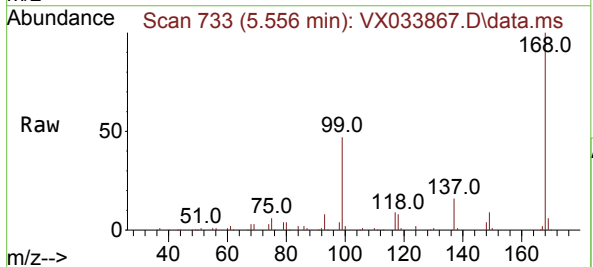


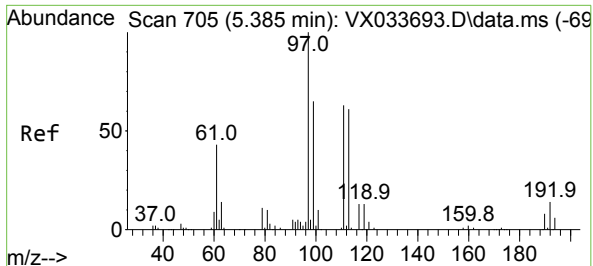

#32
 1,1,1-Trichloroethane
 Concen: 0.696 ug/l
 RT: 5.385 min Scan# 705
 Delta R.T. -0.000 min
 Lab File: VX033867.D
 Acq: 24 Jan 2023 14:25




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-21


Tgt Ion: 97 Resp: 1600
 Ion Ratio Lower Upper
 97 100
 99 0.0 52.3 78.5#
 61 43.4 35.2 52.8

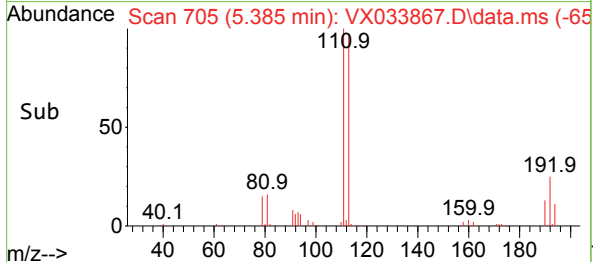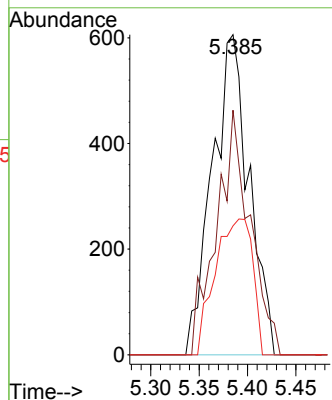

#33
 1,2-Dichloroethane-d4
 Concen: 46.360 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. -0.006 min
 Lab File: VX033867.D
 Acq: 24 Jan 2023 14:25

Tgt Ion: 65 Resp: 75927
 Ion Ratio Lower Upper
 65 100
 67 53.0 0.0 104.8

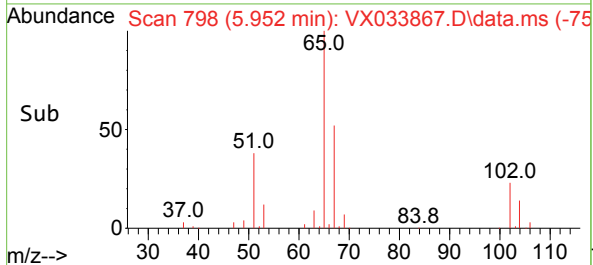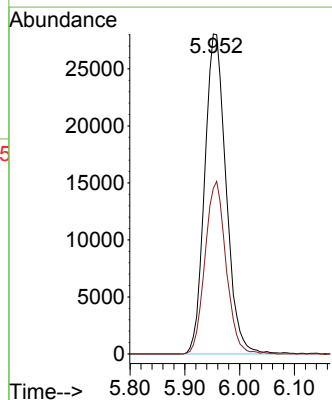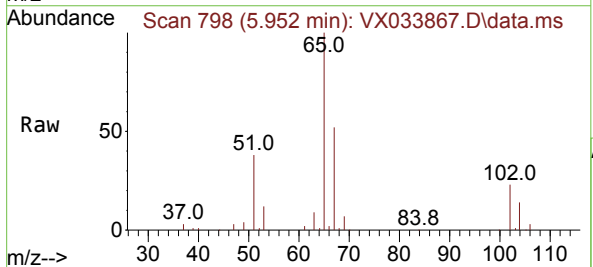



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. -0.000 min

Lab File: VX033867.D

Acq: 24 Jan 2023 14:25

Instrument :

MSVOA_X

ClientSampleId :

TP-21





Tgt Ion:114 Resp: 227847

Ion Ratio Lower Upper

114 100

63 18.4 0.0 37.4

88 14.5 0.0 30.6



#35

Dibromofluoromethane

Concen: 48.960 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.000 min

Lab File: VX033867.D

Acq: 24 Jan 2023 14:25




Tgt Ion:113 Resp: 69269


Ion Ratio Lower Upper

113 100

111 102.9 83.0 124.6

192 24.8 19.0 28.4


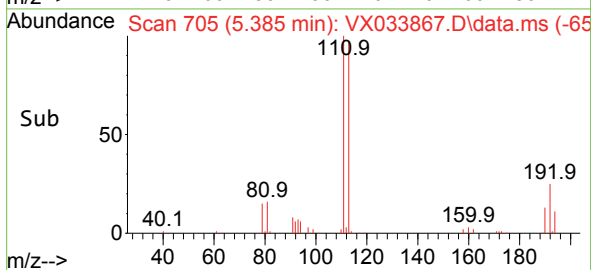




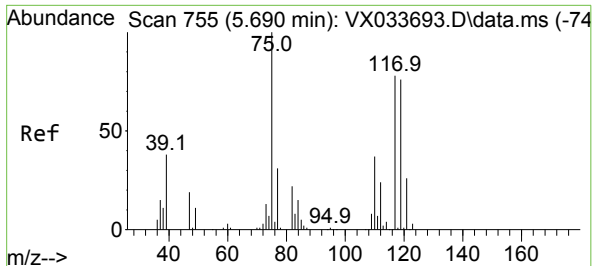

#36
1,1-Dichloropropene
Concen: 4.517 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.141 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25




Instrument :
MSVOA_X
ClientSampleId :
TP-21


Tgt Ion: 75 Resp: 9327
Ion Ratio Lower Upper
75 100
110 9.8 18.8 56.4#
77 0.0 25.1 37.7#

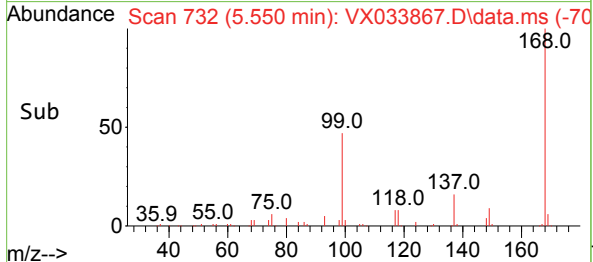

#37
Ethyl Acetate
Concen: 7.988 ug/l
RT: 4.714 min Scan# 595
Delta R.T. -0.001 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Tgt Ion: 43 Resp: 20470
Ion Ratio Lower Upper
43 100
61 14.8 11.1 16.7
70 10.6 8.5 12.7

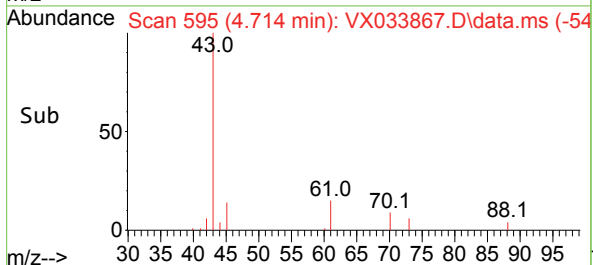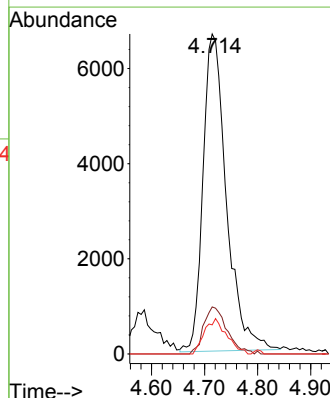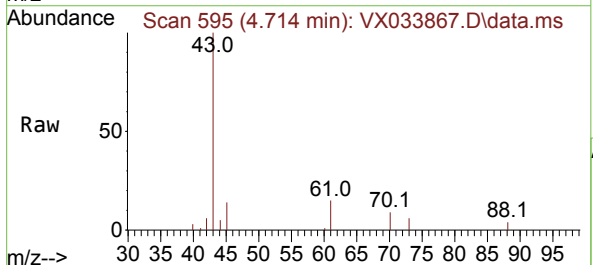

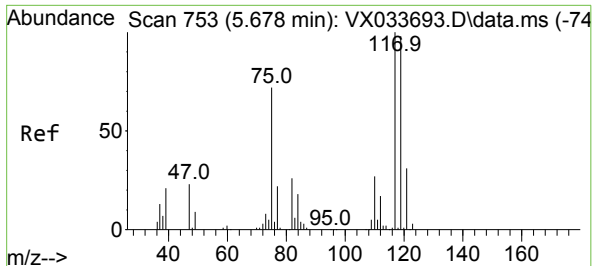

#38

Carbon Tetrachloride

Concen: 6.254 ug/l

RT: 5.556 min Scan# 71

Delta R.T. -0.122 min

Lab File: VX033867.D


Acq: 24 Jan 2023 14:25

Instrument :

MSVOA_X

ClientSampleId :

TP-21






Tgt Ion:117 Resp: 13375

Ion Ratio Lower Upper

117 100

119 6.1 78.0 117.0#

121 0.0 24.4 36.6#

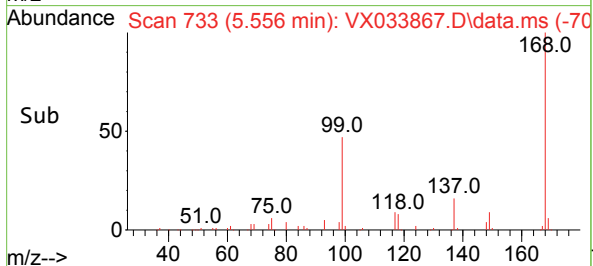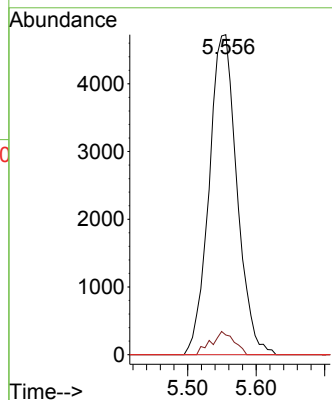

#43

Isopropyl Acetate

Concen: 27.732 ug/l

RT: 6.336 min Scan# 861

Delta R.T. -0.000 min

Lab File: VX033867.D

Acq: 24 Jan 2023 14:25




Tgt Ion: 43 Resp: 90398


Ion Ratio Lower Upper

43 100

61 20.7 15.7 23.5

87 13.7 10.6 15.8


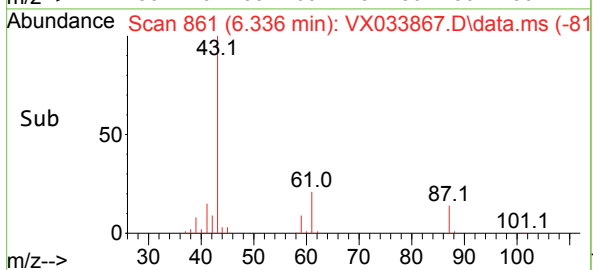
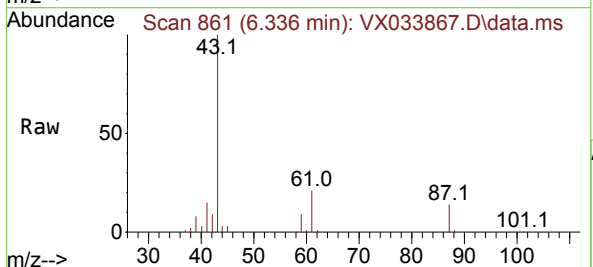
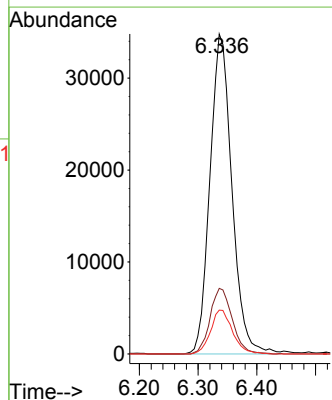


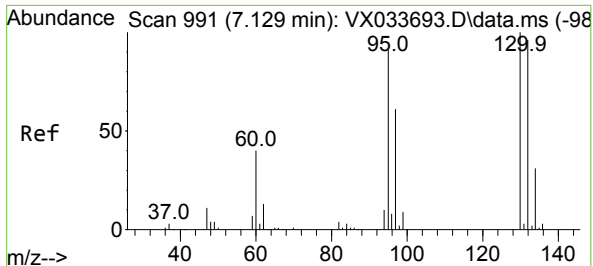

#44
Trichloroethene
Concen: 0.518 ug/l
RT: 7.135 min Scan# 991
Delta R.T. 0.006 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25




Instrument :
MSVOA_X
ClientSampleId :
TP-21


Tgt Ion:130 Resp: 871
Ion Ratio Lower Upper
130 100
95 101.9 0.0 182.6

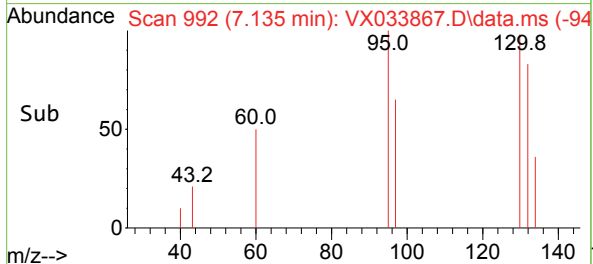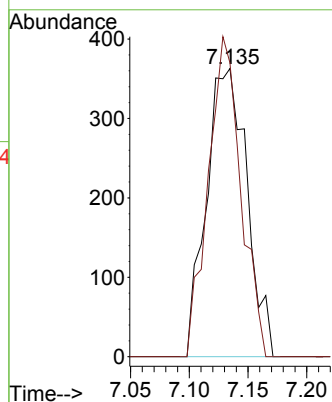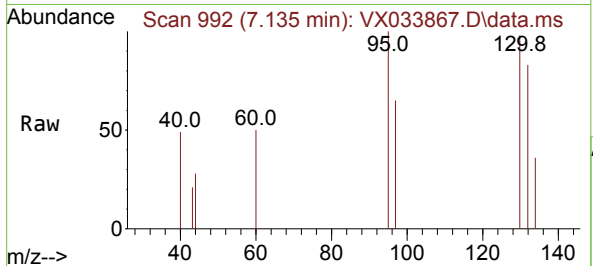

#48
Methyl methacrylate
Concen: 1.546 ug/l
RT: 7.610 min Scan# 1070
Delta R.T. -0.080 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Tgt Ion: 41 Resp: 2539
Ion Ratio Lower Upper
41 100
69 0.0 63.1 94.7#
39 0.0 43.2 64.8#

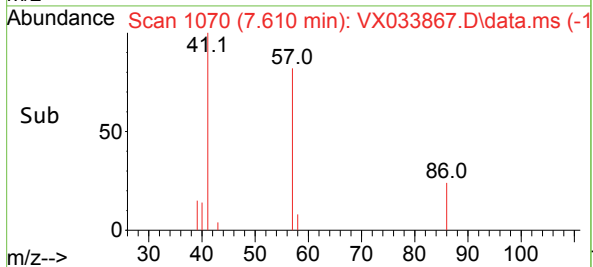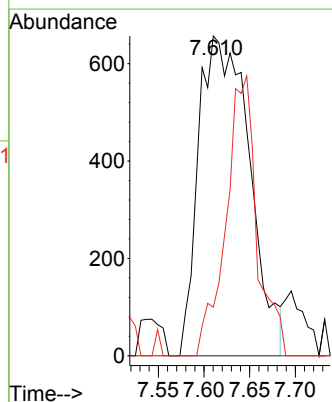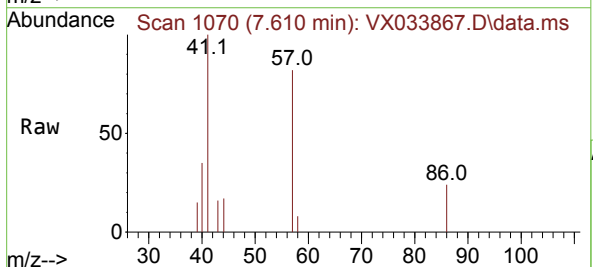



#49

1,4-Dioxane

Concen: 3.662 ug/l

RT: 7.793 min Scan# 1100

Delta R.T. 0.055 min

Lab File: VX033867.D

Acq: 24 Jan 2023 14:25

Instrument :

MSVOA_X

ClientSampleId :

TP-21





Tgt Ion: 88 Resp: 133

Ion Ratio Lower Upper

88 100

43 626218.0 0.0 0.0#

58 2569.2 56.5 84.7#

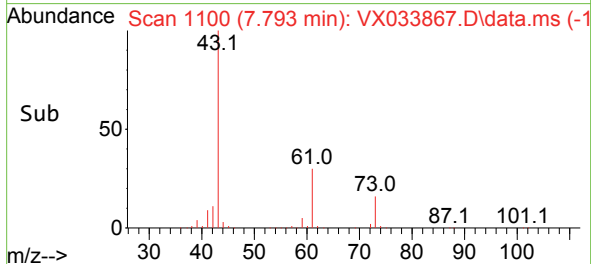

#50

Toluene-d8

Concen: 50.521 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX033867.D




Acq: 24 Jan 2023 14:25


Tgt Ion: 98 Resp: 260432

Ion Ratio Lower Upper

98 100

100 66.8 53.6 80.4









#51
4-Methyl-2-Pentanone
Concen: 32.961 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.025 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25




Instrument :
MSVOA_X
ClientSampleId :
TP-21


Tgt Ion: 43 Resp: 65986
Ion Ratio Lower Upper
43 100
58 8.6 31.2 46.8#

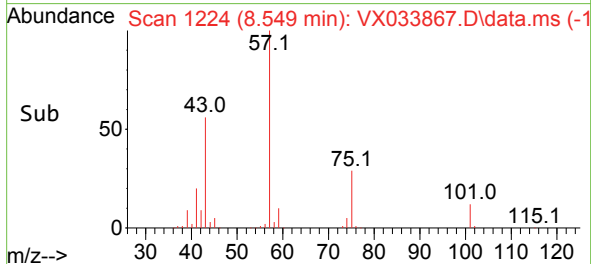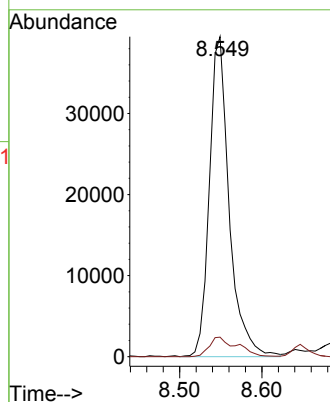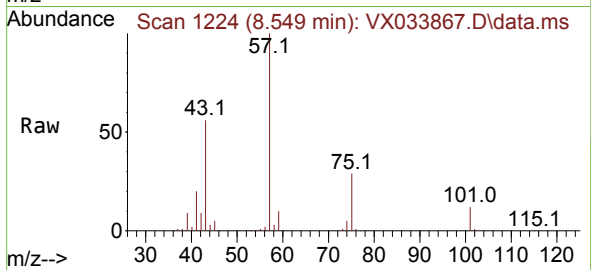

#53
t-1,3-Dichloropropene
Concen: 0.270 ug/l
RT: 8.951 min Scan# 1290
Delta R.T. -0.025 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Tgt Ion: 75 Resp: 547
Ion Ratio Lower Upper
75 100
77 0.0 25.5 38.3#









#54
 cis-1,3-Dichloropropene
 Concen: 13.899 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX033867.D
 Acq: 24 Jan 2023 14:25




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-21


Tgt Ion: 75 Resp: 31609
 Ion Ratio Lower Upper
 75 100
 77 0.3 25.0 37.6#
 39 29.8 38.6 58.0#

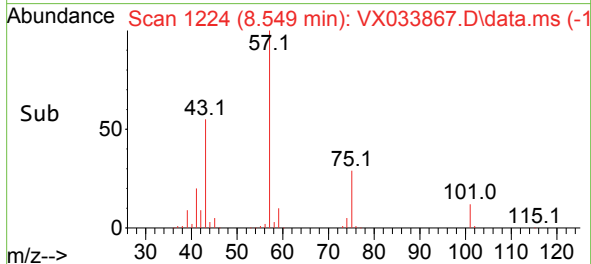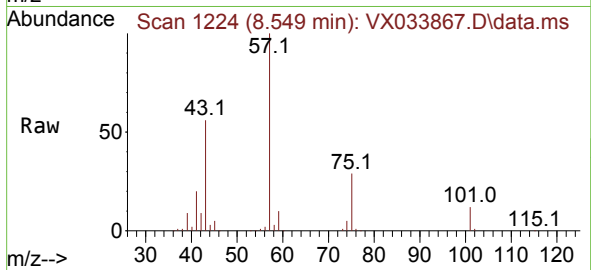

#56
 Ethyl methacrylate
 Concen: 0.230 ug/l
 RT: 9.244 min Scan# 1338
 Delta R.T. 0.128 min
 Lab File: VX033867.D
 Acq: 24 Jan 2023 14:25

Tgt Ion: 69 Resp: 499
 Ion Ratio Lower Upper
 69 100
 41 7823.4 55.1 82.7#
 39 3148.9 28.5 42.7#

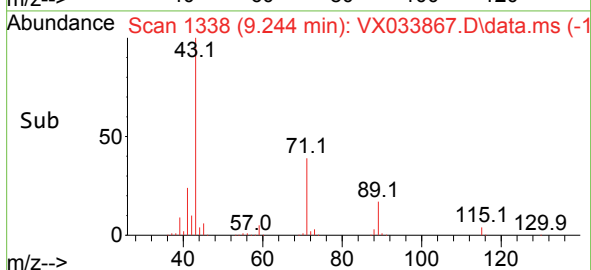



#57

1,3-Dichloropropane

Concen: 1.513 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.176 min

Lab File: VX033867.D

Acq: 24 Jan 2023 14:25

Instrument :

MSVOA_X

ClientSampleId :





TP-21

Tgt Ion: 76 Resp: 3775

Ion Ratio Lower Upper

76 100

78 0.0 25.6 38.4#

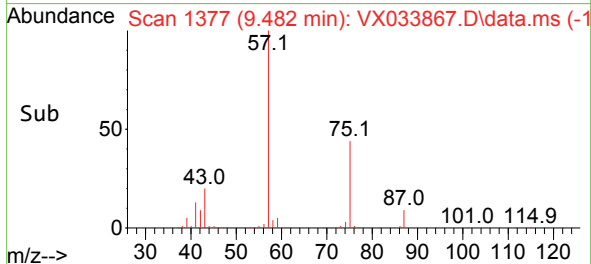

#59

2-Hexanone

Concen: 36.073 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.048 min

Lab File: VX033867.D




Acq: 24 Jan 2023 14:25


Tgt Ion: 43 Resp: 50264

Ion Ratio Lower Upper

43 100

58 19.0 27.4 82.0#


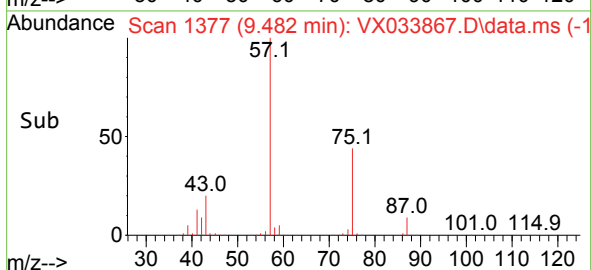






#60
Dibromochloromethane
Concen: 0.203 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.244 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25




Instrument :
MSVOA_X
ClientSampleId :
TP-21


Tgt Ion:129 Resp: 323
Ion Ratio Lower Upper
129 100
127 0.0 38.8 116.3#

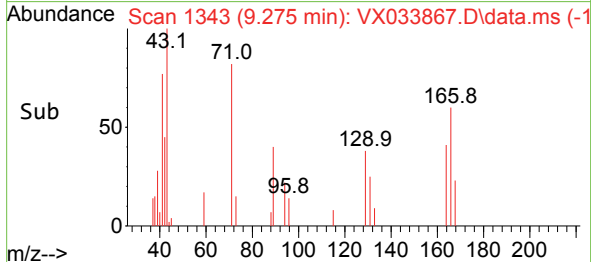

#62
4-Bromofluorobenzene
Concen: 47.096 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Tgt Ion: 95 Resp: 90137
Ion Ratio Lower Upper
95 100
174 94.9 0.0 184.4
176 92.8 0.0 178.8


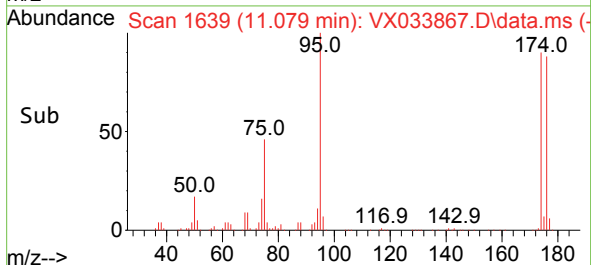
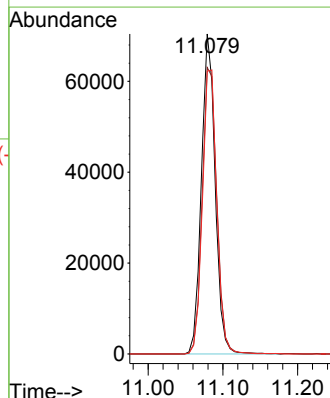





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25




Instrument :
MSVOA_X
ClientSampleId :
TP-21


Tgt Ion:117	Resp: 203321
Ion Ratio	Lower Upper
117 100	
82 50.4	40.6 60.8
119 32.8	25.6 38.4

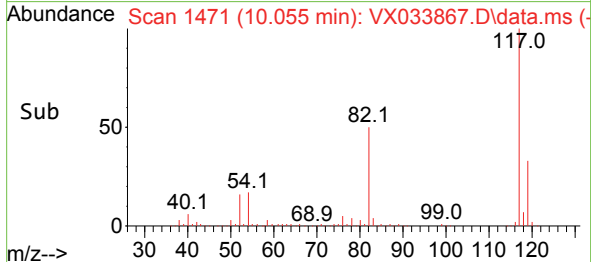

#64
Tetrachloroethene
Concen: Below Cal
RT: 9.275 min Scan# 1343
Delta R.T. -0.000 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Tgt	Ion:164	Resp:	374
Ion	Ratio	Lower	Upper
164	100		
166	145.6	100.2	150.2
129	92.0	69.2	103.8
131	59.9	67.2	100.8#




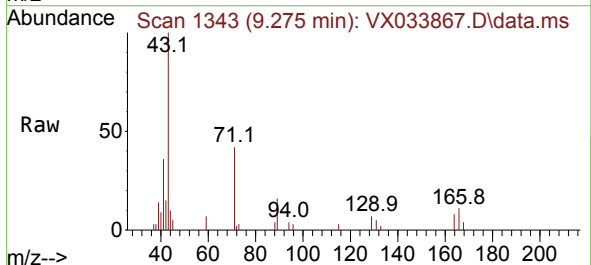




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25




Instrument :
MSVOA_X
ClientSampleId :
TP-21


Tgt Ion:152 Resp: 99018
Ion Ratio Lower Upper
152 100
115 53.2 38.7 116.1
150 157.9 0.0 348.2

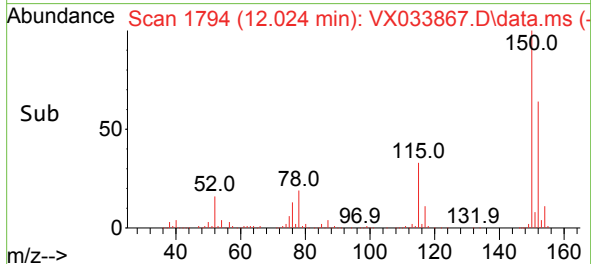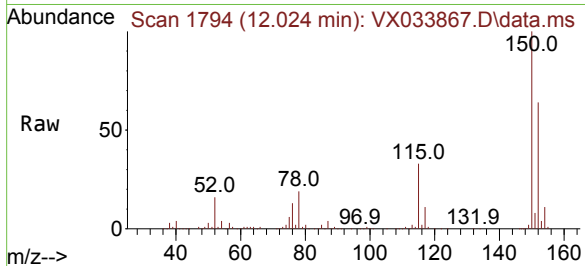

#73
Isopropylbenzene
Concen: Below Cal
RT: 10.969 min Scan# 1621
Delta R.T. 0.005 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Tgt Ion:105 Resp: 20
Ion Ratio Lower Upper
105 100
120 0.0 13.6 40.8#

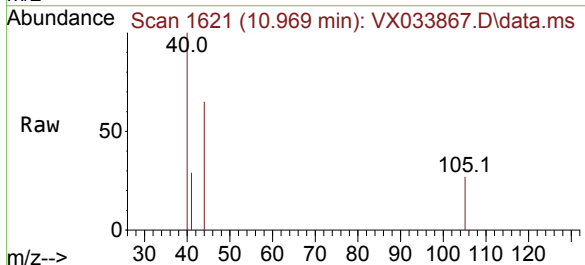



#74

N-amy1 acetate

Concen: 0.211 ug/l

RT: 10.817 min Scan# 1

Delta R.T. -0.025 min

Lab File: VX033867.D

Acq: 24 Jan 2023 14:25

Instrument :

MSVOA_X

ClientSampleId :

TP-21

Tgt Ion: 43 Resp: 549





Ion Ratio Lower Upper

43 100

70 0.0 34.8 52.2#

55 0.0 19.4 29.0#

61 0.0 19.4 29.2#

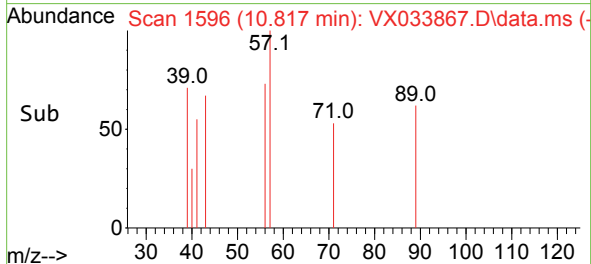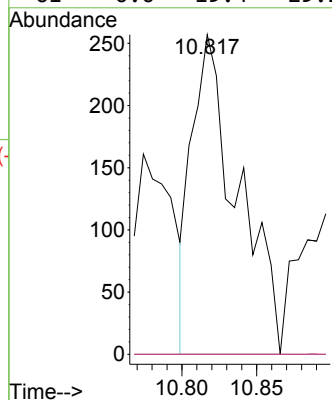

#76

1,2,3-Trichloropropane

Concen: 22.727 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX033867.D




Acq: 24 Jan 2023 14:25


Tgt Ion: 75 Resp: 41347

Ion Ratio Lower Upper

75 100

77 1.2 21.8 65.4#


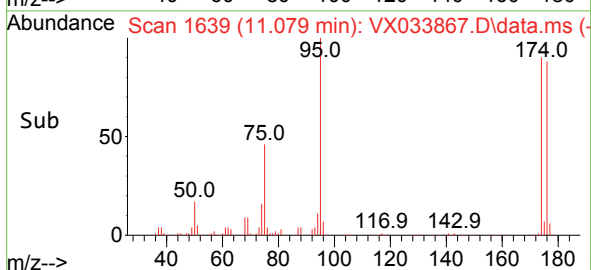
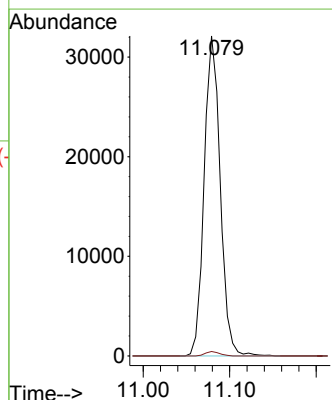





#79
2-Chlorotoluene
Concen: Below Cal
RT: 11.360 min Scan# 1685
Delta R.T. -0.006 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25




Instrument :
MSVOA_X
ClientSampleId :
TP-21


Tgt Ion: 91 Resp: 21
Ion Ratio Lower Upper
91 100
126 0.0 18.1 54.1#

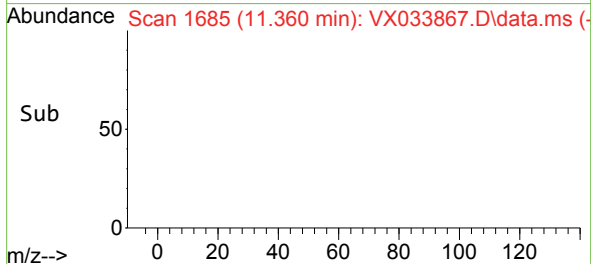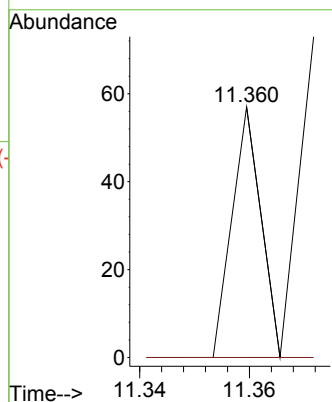

#81
trans-1,4-Dichloro-2-butene
Concen: 70.632 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Tgt Ion: 75 Resp: 41347
Ion Ratio Lower Upper
75 100
53 0.0 83.0 124.6#
89 0.0 37.7 56.5#

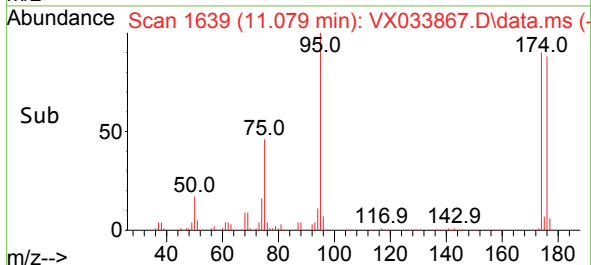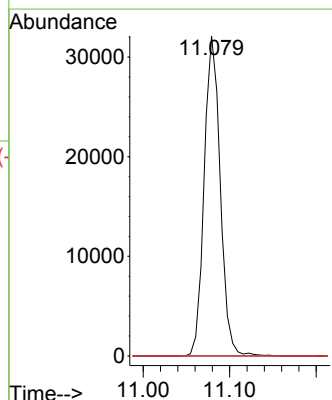



#82
4-Chlorotoluene
Concen: Below Cal
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033867.D
Acq: 24 Jan 2023 14:25

Instrument :
MSVOA_X
ClientSampleId :
TP-21

Tgt Ion: 91 Resp: 108
Ion Ratio Lower Upper
91 100
126 0.0 15.8 47.4#

