

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012423\
 Data File : VX033870.D
 Acq On : 24 Jan 2023 16:21
 Operator : JC/MD
 Sample : 01260-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-26

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
 Title : SW846 8260

Signal : TIC: VX033870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.386	206	213	223	rBV	14622	27264	1.75%	0.300%
2	2.788	272	279	291	rVB	10908	21418	1.37%	0.236%
3	4.715	587	595	610	rVV	10529	32457	2.08%	0.357%
4	5.385	693	705	721	rBV2	77457	224990	14.43%	2.477%
5	5.550	721	732	751	rVB	137773	396171	25.41%	4.362%
6	5.958	787	799	818	rBV	77129	209540	13.44%	2.307%
7	6.336	849	861	881	rBV	64694	169791	10.89%	1.870%
8	6.763	921	931	947	rBV	201454	482540	30.95%	5.313%
9	7.641	1064	1075	1080	rBV	35214	67549	4.33%	0.744%
10	7.690	1080	1083	1093	rVV	12223	22559	1.45%	0.248%
11	7.799	1093	1101	1122	rVV	879238	1559046	100.00%	17.167%
12	8.549	1217	1224	1234	rBV	191147	311951	20.01%	3.435%
13	8.647	1234	1240	1255	rVB	415843	669525	42.94%	7.372%
14	8.952	1284	1290	1309	rBV	254772	387566	24.86%	4.268%
15	9.244	1332	1338	1345	rBV	281177	402580	25.82%	4.433%
16	9.305	1345	1348	1351	rVV	25019	37364	2.40%	0.411%
17	9.342	1351	1354	1356	rVV	42634	56460	3.62%	0.622%
18	9.378	1356	1360	1369	rVV	111380	172250	11.05%	1.897%
19	9.482	1372	1377	1388	rVV	467395	613831	39.37%	6.759%
20	9.580	1388	1393	1410	rVB	300387	411489	26.39%	4.531%
21	9.915	1442	1448	1463	rBV	844601	1142140	73.26%	12.576%
22	10.055	1464	1471	1477	rVV	413382	583904	37.45%	6.429%
23	10.281	1503	1508	1521	rBV	10645	15916	1.02%	0.175%
24	10.506	1541	1545	1555	rBV	11392	15756	1.01%	0.173%
25	10.640	1559	1567	1579	rBV	71622	95521	6.13%	1.052%
26	11.079	1634	1639	1648	rBV	338686	435920	27.96%	4.800%
27	12.024	1788	1794	1806	rBV	390629	516156	33.11%	5.684%




Sum of corrected areas: 9081654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012423\
Data File : VX033870.D
Acq On : 24 Jan 2023 16:21
Operator : JC/MD
Sample : 01260-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

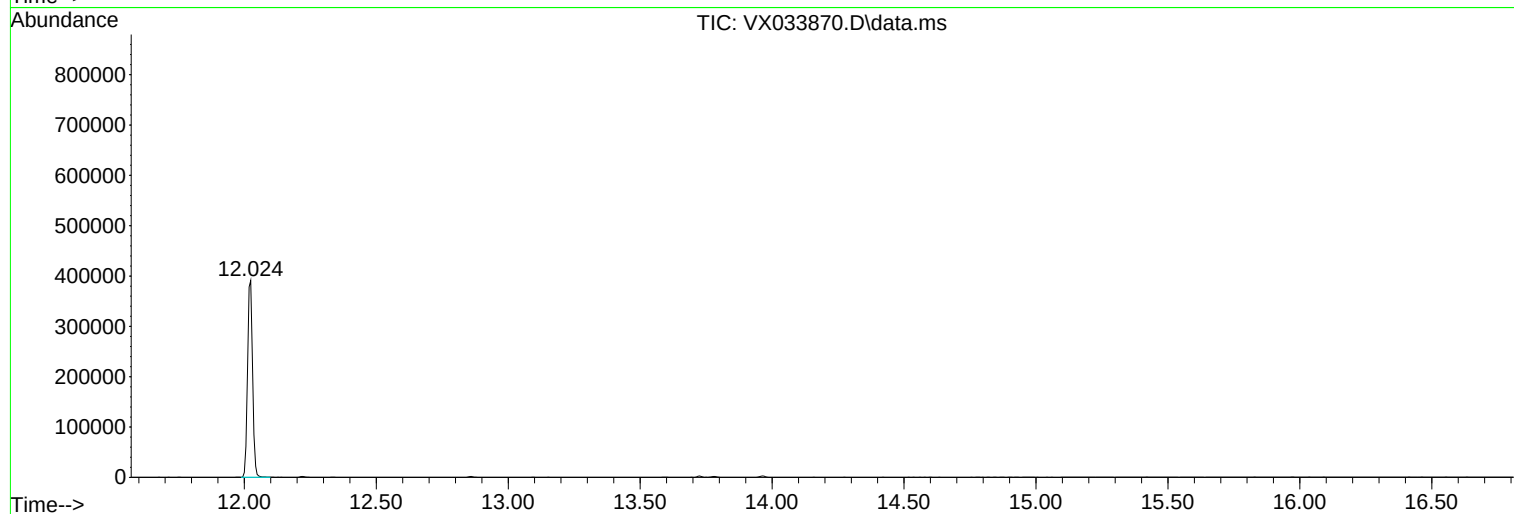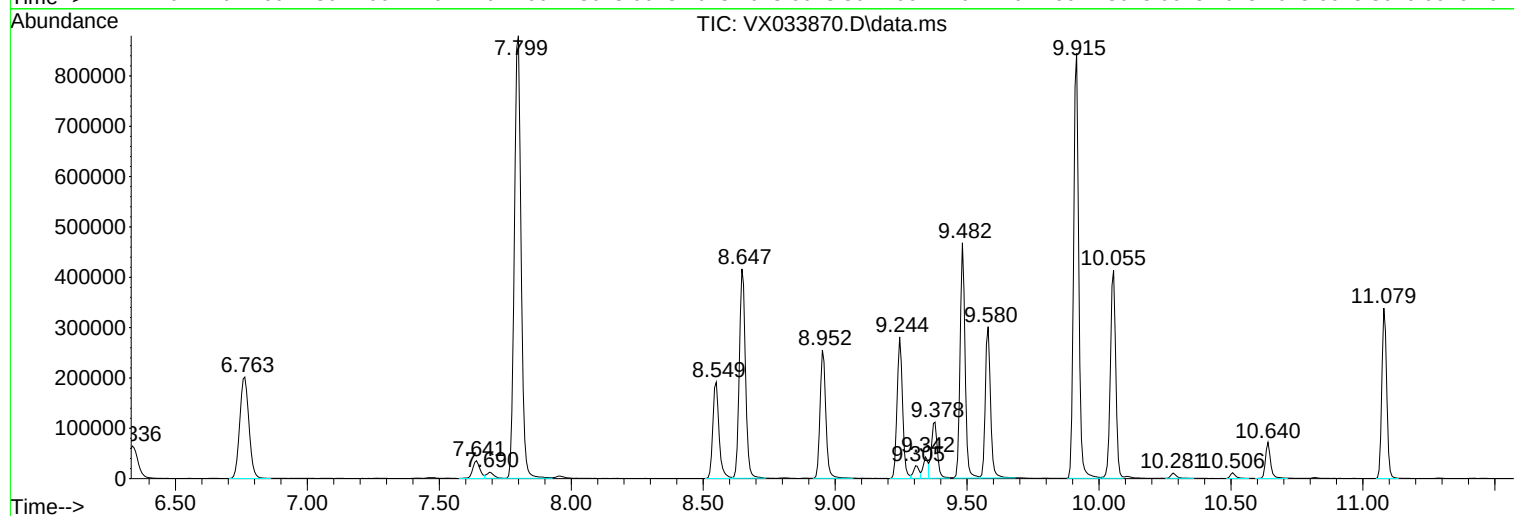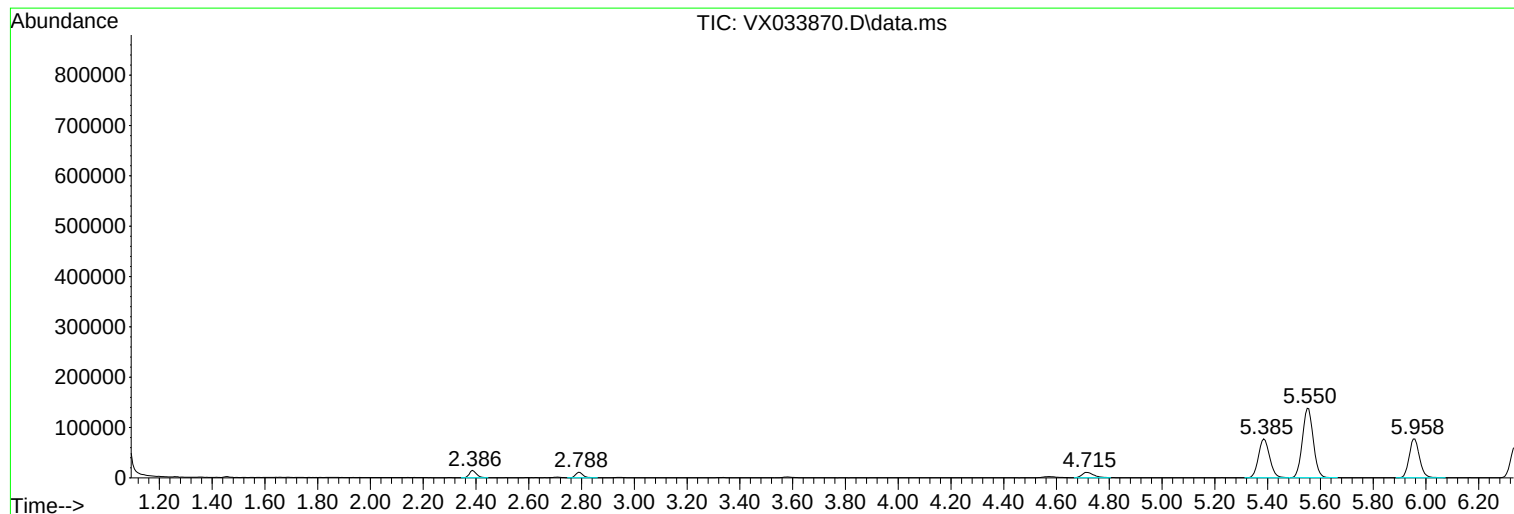

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012423\
Data File : VX033870.D
Acq On : 24 Jan 2023 16:21
Operator : JC/MD
Sample : 01260-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012423\
Data File : VX033870.D
Acq On : 24 Jan 2023 16:21
Operator : JC/MD
Sample : 01260-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------