
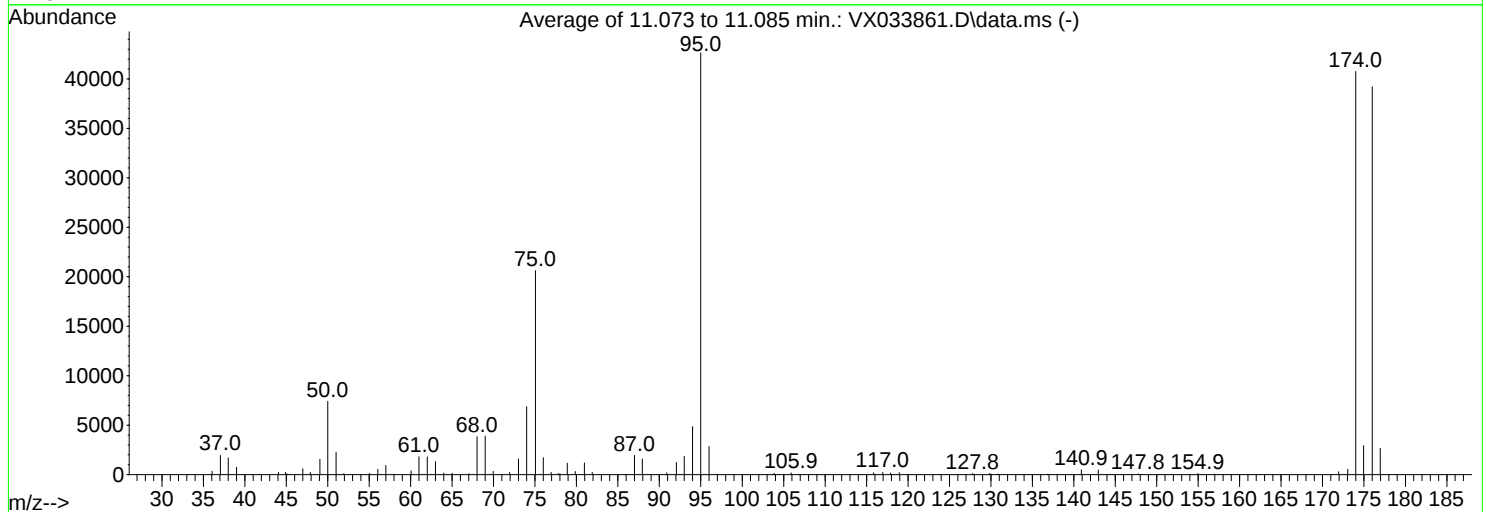


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012423\
Data File : VX033861.D
Acq On : 24 Jan 2023 08:40
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Title : SW846 8260
Last Update : Wed Jan 11 14:48:42 2023

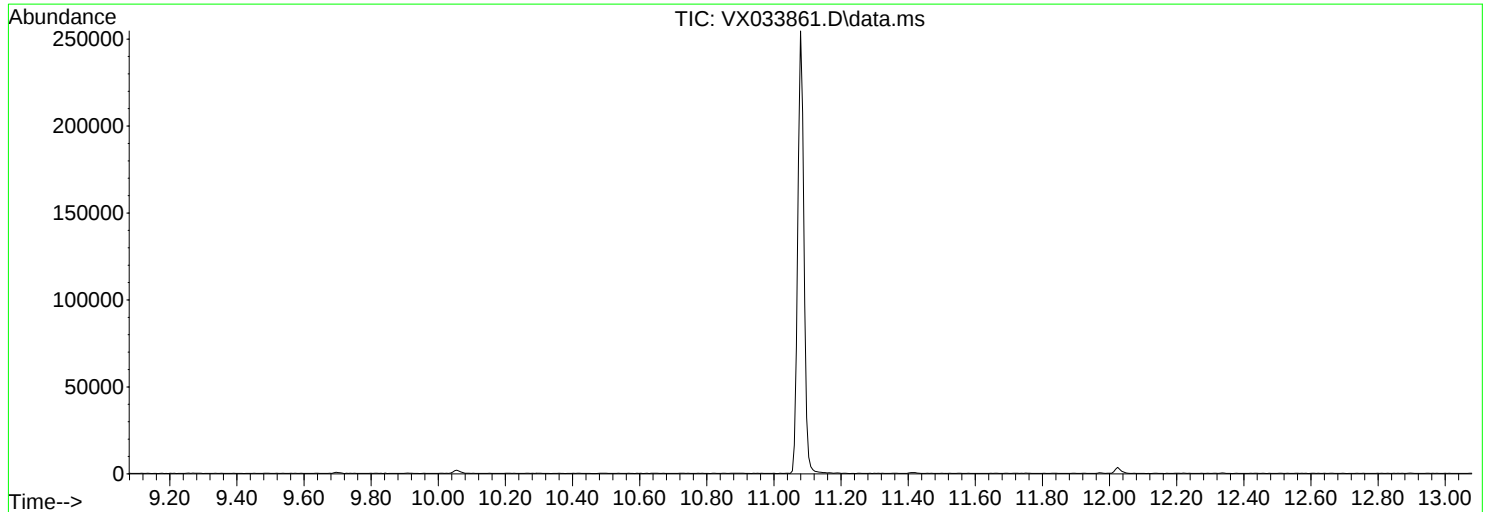

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	7400	PASS
75	95	30	60	48.4	20627	PASS
95	95	100	100	100.0	42632	PASS
96	95	5	9	6.7	2854	PASS
173	174	0.00	2	1.3	528	PASS
174	95	50	100	95.6	40749	PASS
175	174	5	9	7.2	2920	PASS
176	174	95	101	96.2	39200	PASS
177	176	5	9	6.8	2663	PASS