
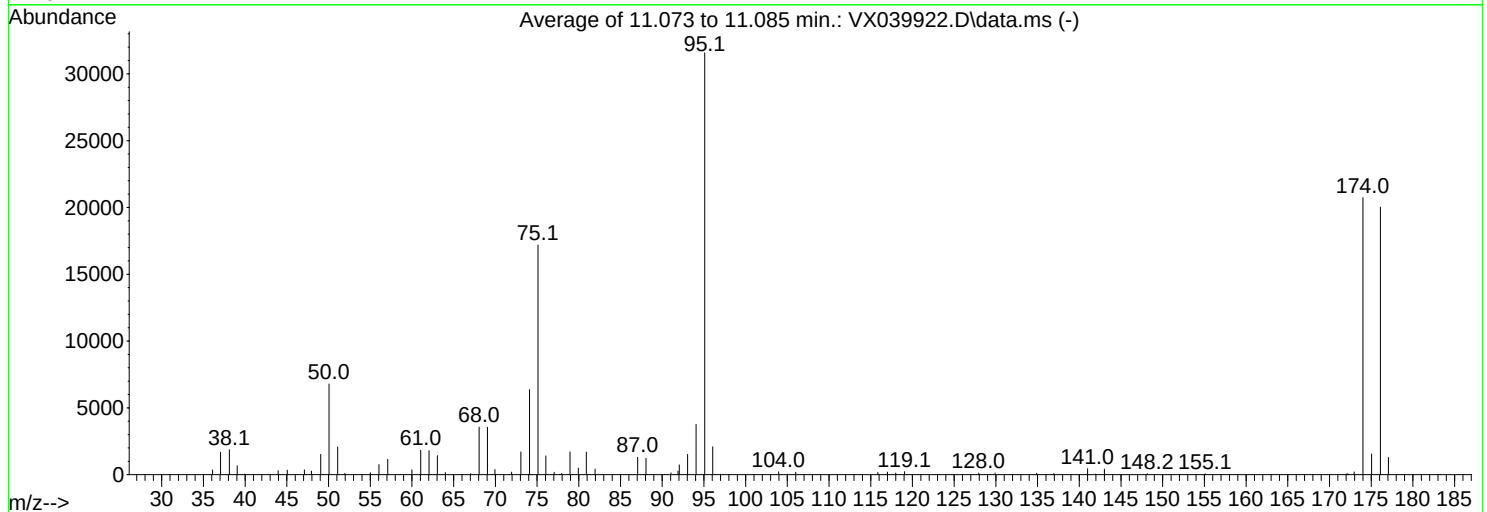


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012424\
Data File : VX039922.D
Acq On : 24 Jan 2024 09:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 03:51:26 2024

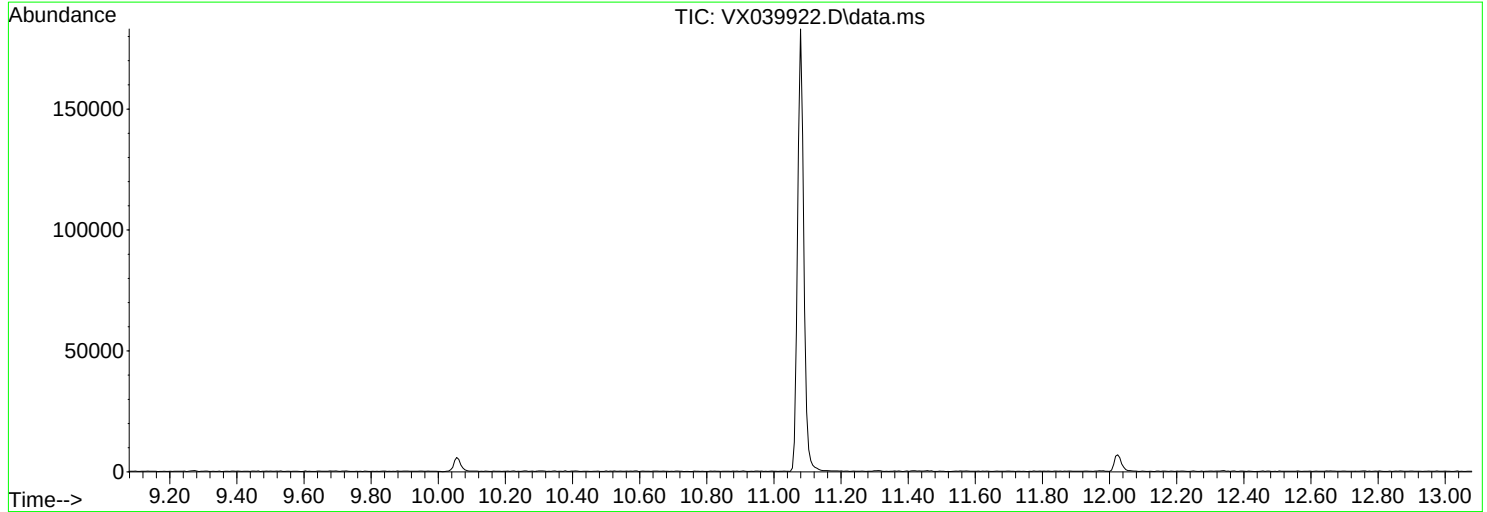

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.5	6788	PASS
75	95	30	60	54.4	17185	PASS
95	95	100	100	100.0	31573	PASS
96	95	5	9	6.6	2080	PASS
173	174	0.00	2	1.0	198	PASS
174	95	50	100	65.7	20732	PASS
175	174	5	9	7.5	1549	PASS
176	174	95	101	96.6	20022	PASS
177	176	5	9	6.4	1280	PASS