


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012519\  
Data File : VX007215.D  
Acq On : 25 Jan 2019 08:29  
Operator : JC/SP  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA\_F\METHODS\82F011519S.M  
Title : SW846 8260  
Last Update : Wed Jan 16 04:51:59 2019

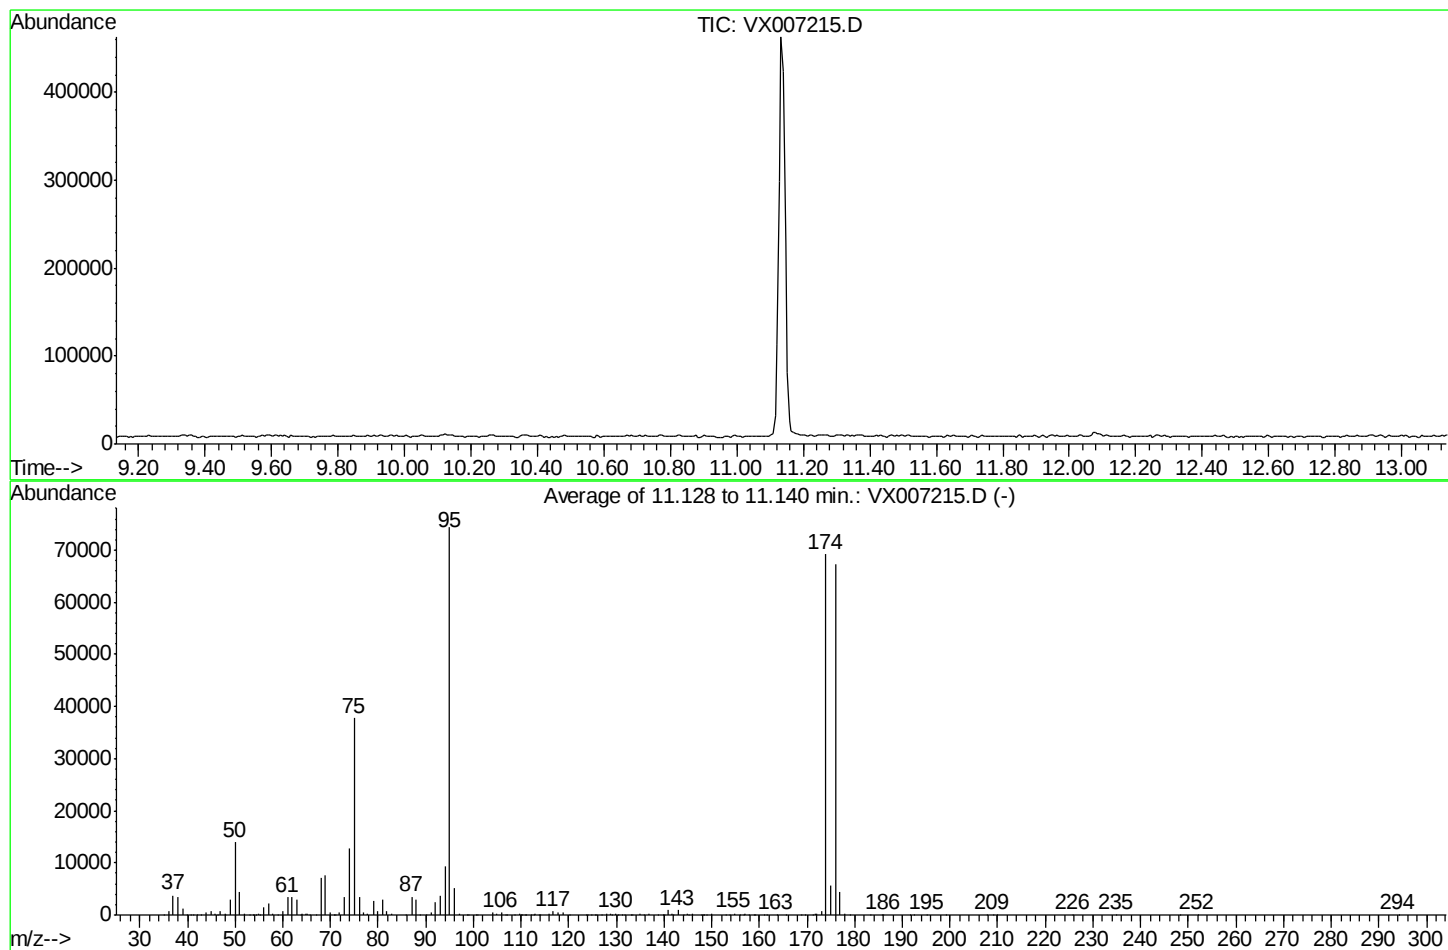

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.8      | 13968   | PASS             |
| 75          | 95           | 30           | 60           | 50.7      | 37726   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 74389   | PASS             |
| 96          | 95           | 5            | 9            | 7.0       | 5172    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.2       | 813     | PASS             |
| 174         | 95           | 50           | 100          | 93.0      | 69170   | PASS             |
| 175         | 174          | 5            | 9            | 8.1       | 5630    | PASS             |
| 176         | 174          | 95           | 101          | 97.4      | 67341   | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 4419    | PASS             |