

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012521\
 Data File : VX020730.D
 Acq On : 25 Jan 2021 17:22
 Operator : JC/SP
 Sample : M1189-09 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 41052

Quant Time: Jan 27 11:55:42 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:38:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.629	168	314792	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	539540	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.097	117	518974	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.060	152	236074	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	213761	49.79	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	99.58%		
35) Dibromofluoromethane	5.464	113	181644	49.15	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	98.30%		
50) Toluene-d8	8.695	98	670664	49.50	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	99.00%		
62) 4-Bromofluorobenzene	11.122	95	247939	47.12	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	94.24%		
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.184	85	175	1.23	ug/l #	42
5) Bromomethane	1.629	94	698	0.33	ug/l	97
11) Tert butyl alcohol	2.989	59	5740	7.16	ug/l #	73
16) Acetone	2.416	43	215834	132.58	ug/l	99
17) Carbon Disulfide	2.550	76	1222	1.02	ug/l	97
20) Methylene Chloride	2.830	84	1117	0.27	ug/l #	90
25) 2-Butanone	4.635	43	2748	1.08	ug/l #	78
29) Tetrahydrofuran	5.104	42	424	0.26	ug/l #	60
31) Cyclohexane	5.623	56	6222	1.08	ug/l #	1
36) 1,1-Dichloropropene	5.623	75	24912	4.60	ug/l #	49
37) Ethyl Acetate	4.806	43	2147	0.42	ug/l #	74
38) Carbon Tetrachloride	5.623	117	32895	5.78	ug/l #	16
40) Benzene	6.104	78	5057	0.32	ug/l #	88
52) Toluene	8.762	92	133976	13.36	ug/l	98
67) Ethyl Benzene	10.232	91	16318	0.84	ug/l	93
68) m/p-Xylenes	10.341	106	23874	3.29	ug/l	98
69) o-Xylene	10.683	106	12960	1.90	ug/l	95
74) N-amyl acetate	10.896	43	124	2.03	ug/l #	1
76) 1,2,3-Trichloropropane	11.116	75	122212	22.32	ug/l #	39
78) n-propylbenzene	11.341	91	10563	0.54	ug/l	95
79) 2-Chlorotoluene	11.414	91	5833	0.48	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.487	105	14366	0.99	ug/l	95
81) trans-1,4-Dichloro-2-b...	11.116	75	122212	62.55	ug/l #	12
83) tert-Butylbenzene	11.792	119	7015	0.50	ug/l #	52
84) 1,2,4-Trimethylbenzene	11.792	105	58534	3.98	ug/l	100
85) sec-Butylbenzene	11.926	105	5013	0.31	ug/l	89
86) p-Isopropyltoluene	12.006	119	5966	0.39	ug/l	97
89) n-Butylbenzene	12.371	91	11176	0.83	ug/l #	46
90) Hexachloroethane	12.591	117	1773	0.65	ug/l #	9
95) Naphthalene	13.816	128	24247	4.13	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012521\
Data File : VX020730.D
Acq On : 25 Jan 2021 17:22
Operator : JC/SP
Sample : M1189-09 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
41052

Quant Time: Jan 27 11:55:42 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:38:15 2021
Response via : Initial Calibration




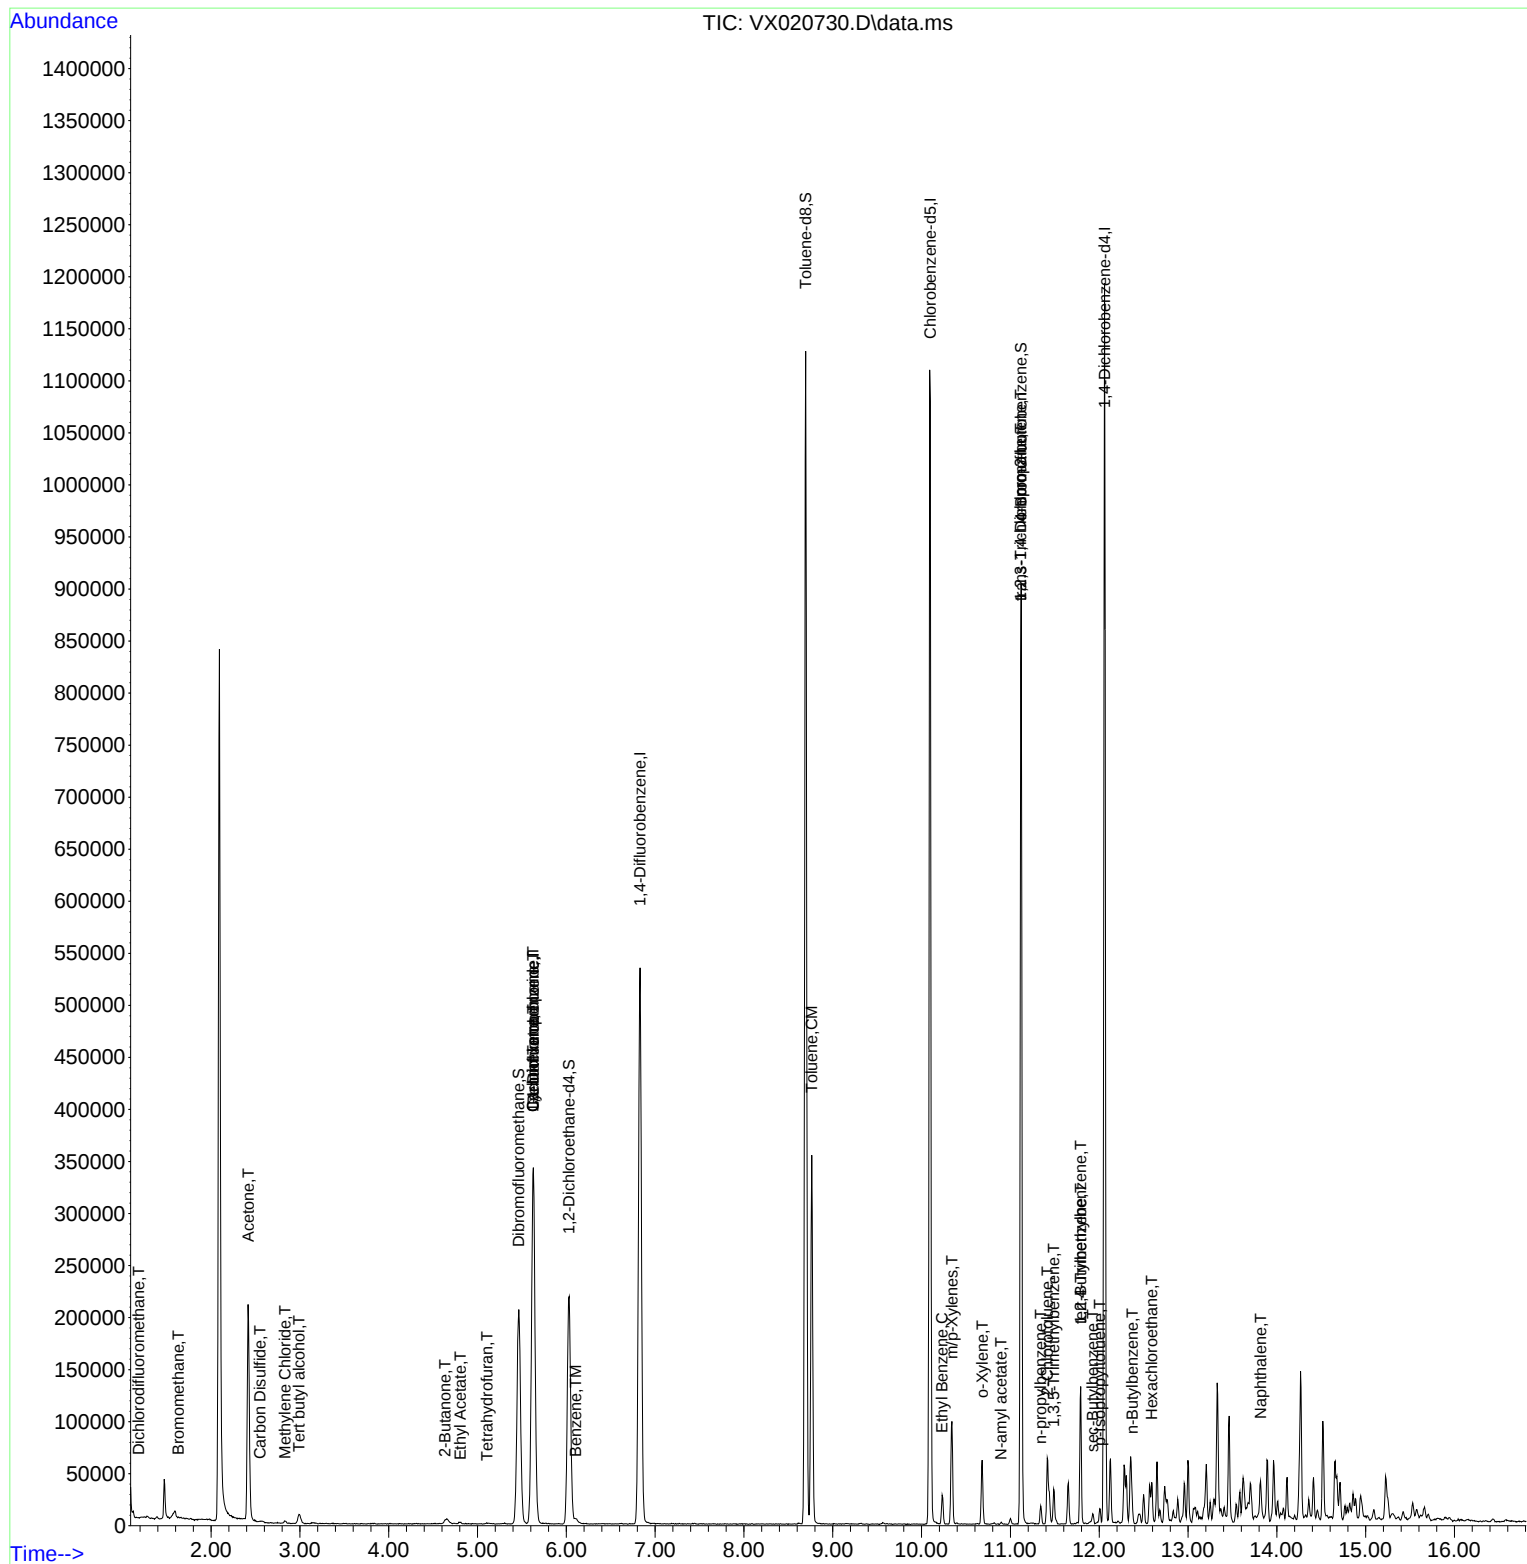




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.000 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampleId :
41052


Tgt Ion:168 Resp: 314792
Ion Ratio Lower Upper
168 100
99 61.2 45.8 68.6

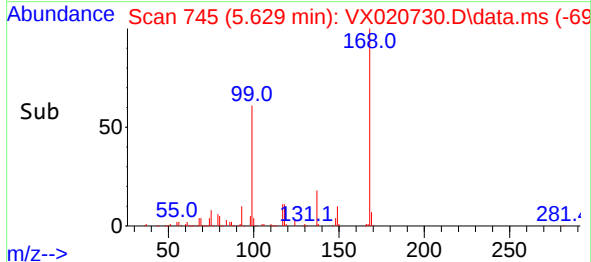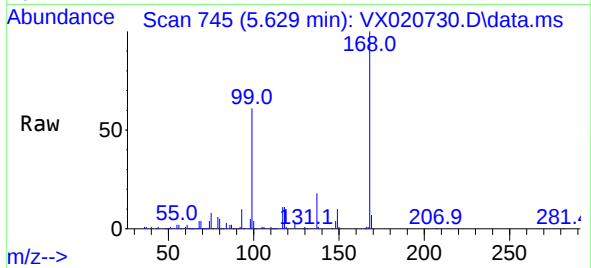

#2
Dichlorodifluoromethane
Concen: 1.23 ug/l
RT: 1.184 min Scan# 16
Delta R.T. -0.001 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 85 Resp: 175
Ion Ratio Lower Upper
85 100
87 0.0 16.4 49.2#


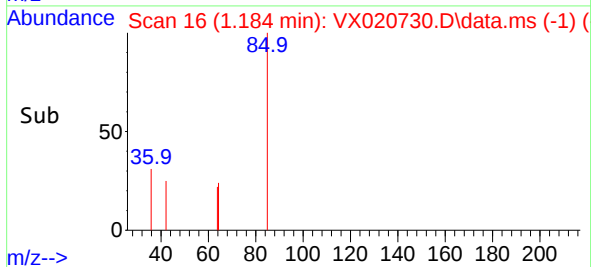

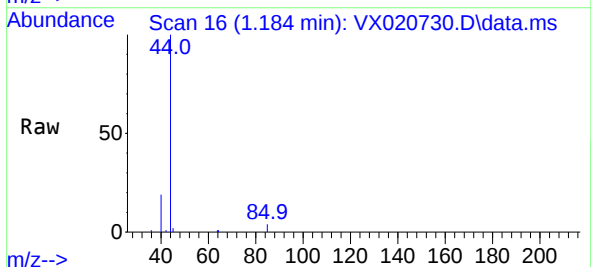


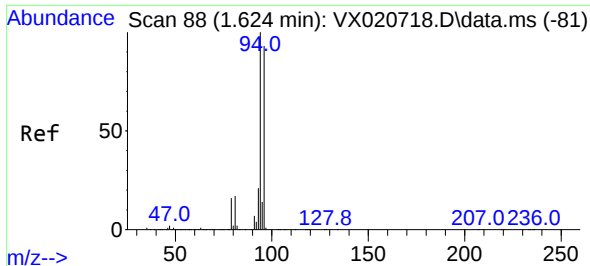

#5
Bromomethane
Concen: 0.33 ug/l
RT: 1.629 min Scan# 89
Delta R.T. 0.005 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampleId :
41052


Tgt Ion: 94 Resp: 698
Ion Ratio Lower Upper
94 100
96 92.5 76.4 114.6

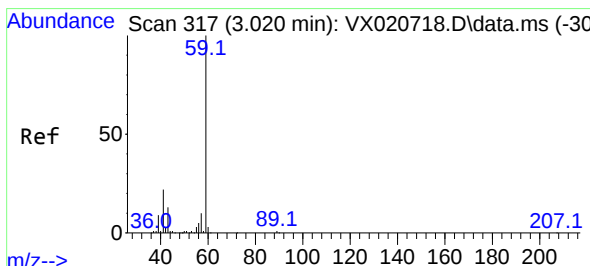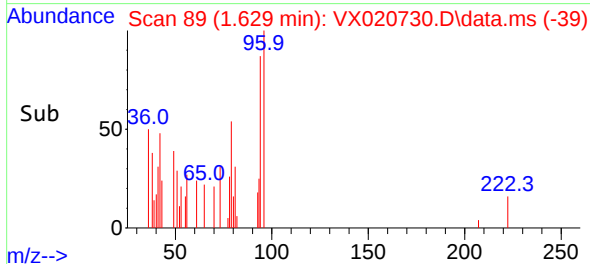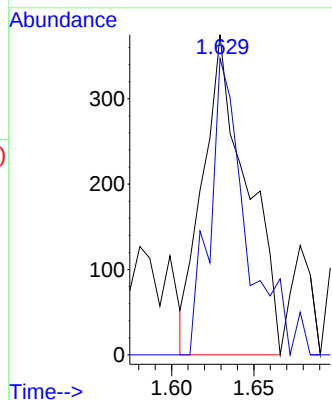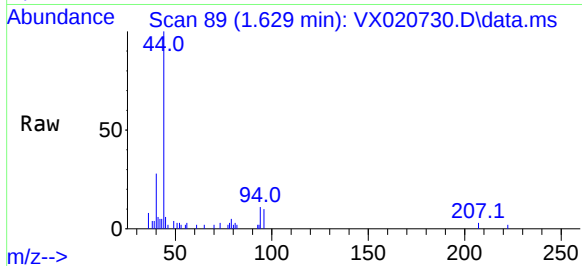

#11
Tert butyl alcohol
Concen: 7.16 ug/l
RT: 2.989 min Scan# 312
Delta R.T. -0.031 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 59 Resp: 5740
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#


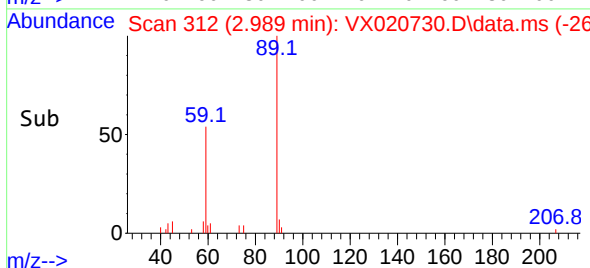
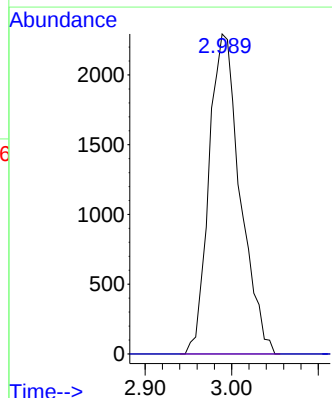
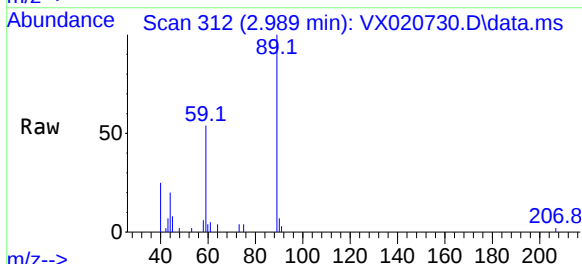




#16
Acetone
Concen: 132.58 ug/l
RT: 2.416 min Scan# 218
Delta R.T. -0.006 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampleId :
41052


Tgt Ion: 43 Resp: 215834
Ion Ratio Lower Upper
43 100
58 35.6 27.8 41.8

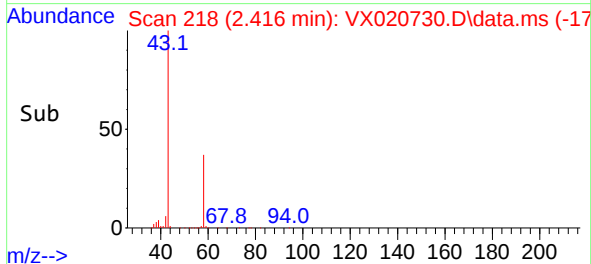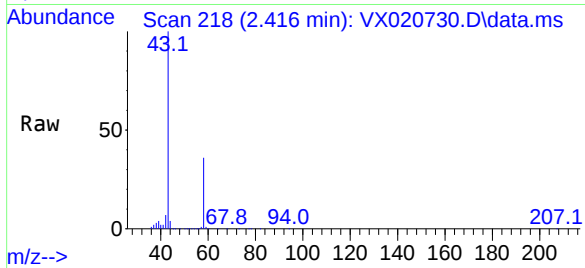

#17
Carbon Disulfide
Concen: 1.02 ug/l
RT: 2.550 min Scan# 240
Delta R.T. 0.006 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 76 Resp: 1222
Ion Ratio Lower Upper
76 100
78 10.1 7.2 10.8

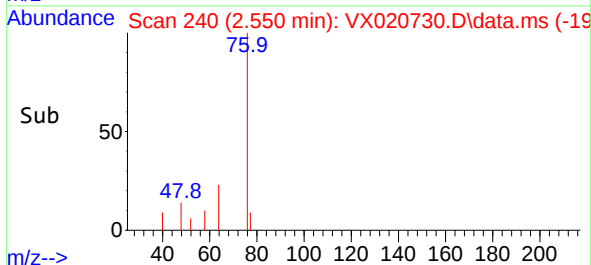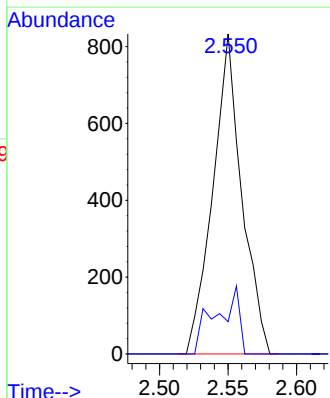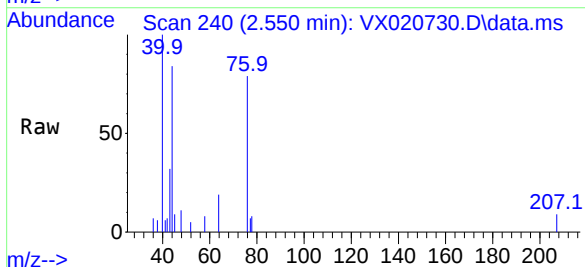

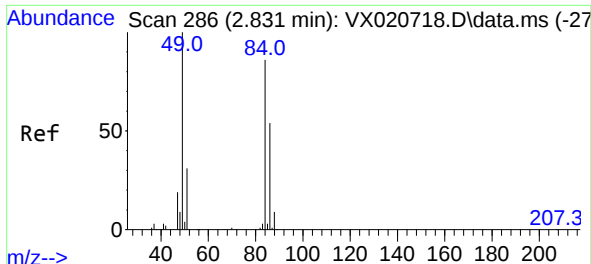

#20

Methylene Chloride

Concen: 0.27 ug/l

RT: 2.830 min Scan# 286

Delta R.T. -0.001 min

Lab File: VX020730.D

Acq: 25 Jan 2021 17:22

Instrument :
MSVOA_X
ClientSampled :
41052

Tgt Ion: 84 Resp: 1117


Ion Ratio Lower Upper

84 100




49 117.6 88.6 132.8

51 44.0 27.0 40.6#

86 54.2 50.3 75.5

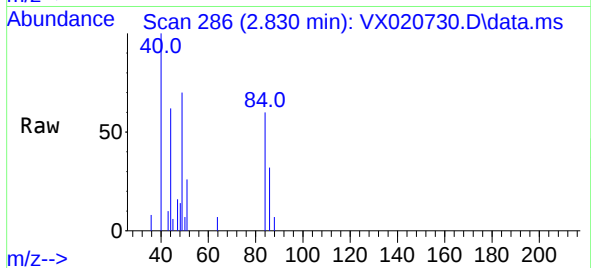

Abundance

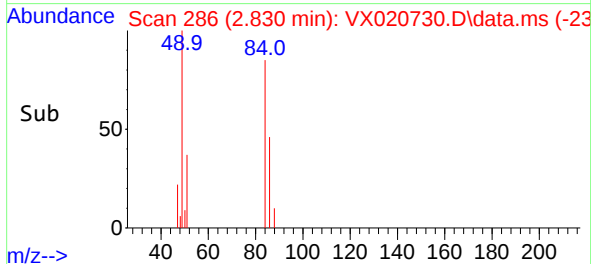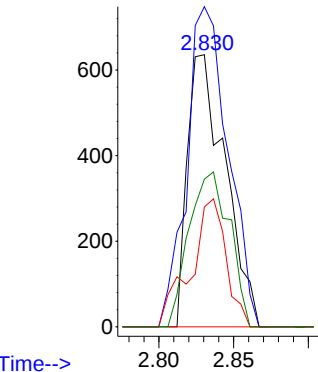

#25

2-Butanone

Concen: 1.08 ug/l

RT: 4.635 min Scan# 582

Delta R.T. -0.000 min

Lab File: VX020730.D


Acq: 25 Jan 2021 17:22

Tgt Ion: 43 Resp: 2748



Ion Ratio Lower Upper


43 100

72 17.6 23.7 35.5#

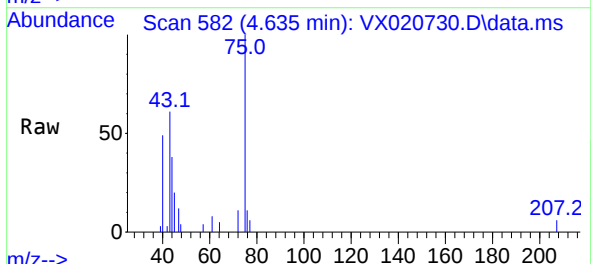

Abundance



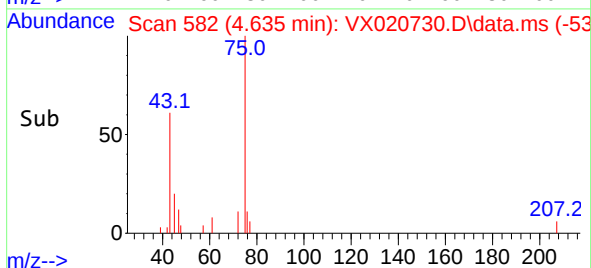
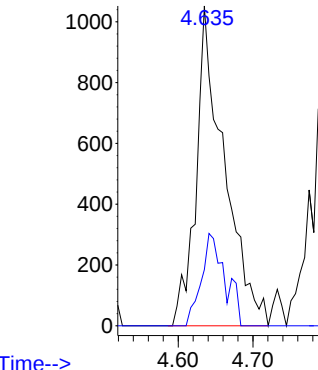




#29
Tetrahydrofuran
Concen: 0.26 ug/l
RT: 5.104 min Scan# 659
Delta R.T. 0.018 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampled :
41052


Tgt Ion: 42 Resp: 424
Ion Ratio Lower Upper
42 100
72 18.9 41.7 62.5#
71 25.9 38.4 57.6#

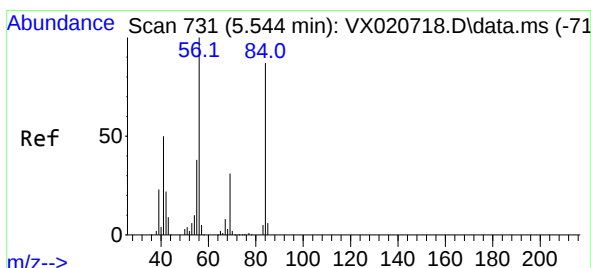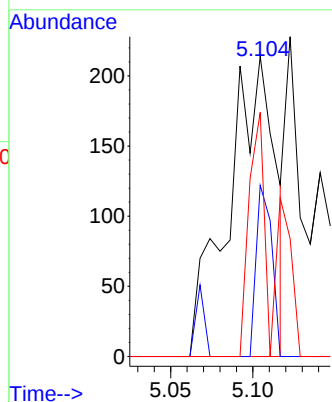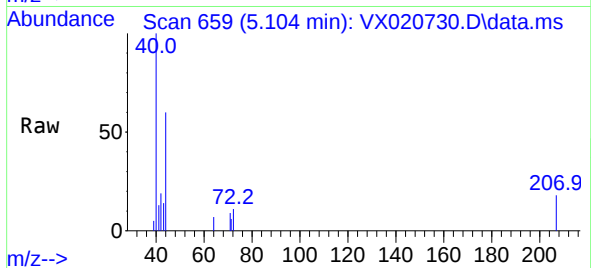

#31
Cyclohexane
Concen: 1.08 ug/l
RT: 5.623 min Scan# 744
Delta R.T. 0.079 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 56 Resp: 6222
Ion Ratio Lower Upper
56 100
69 196.3 25.3 37.9#
84 174.1 71.4 107.0#


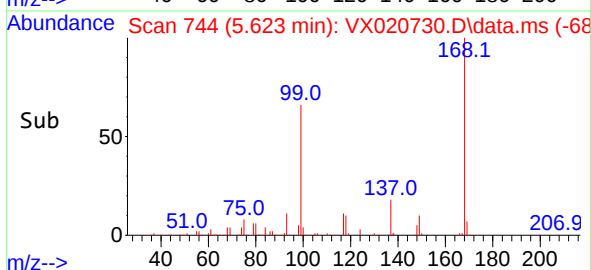
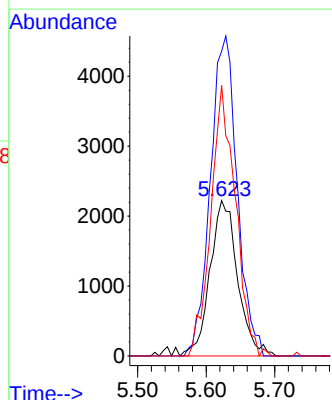



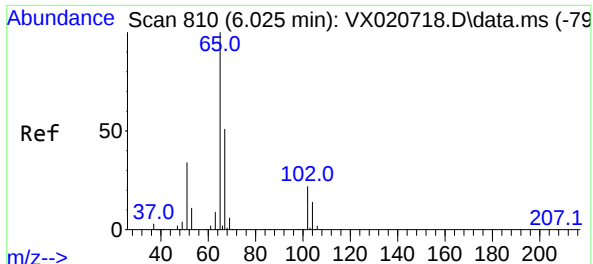

#33
1,2-Dichloroethane-d4
Concen: 49.79 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.006 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampleId :
41052


Tgt Ion: 65 Resp: 213761
Ion Ratio Lower Upper
65 100
67 52.8 0.0 105.4

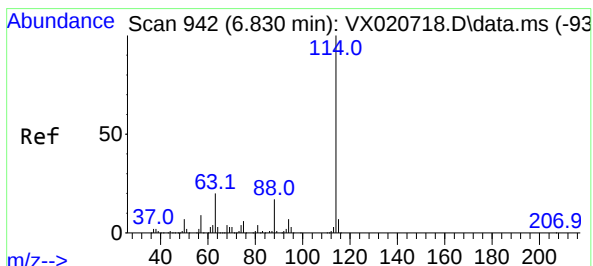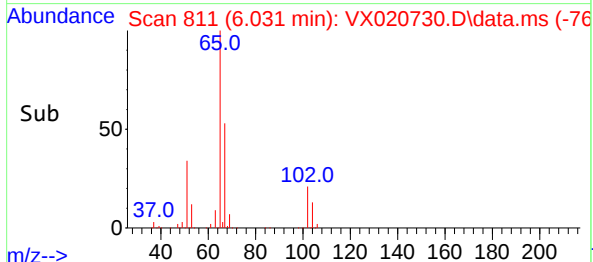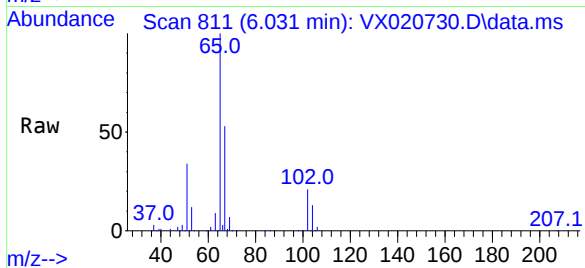

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.830 min Scan# 942
Delta R.T. -0.000 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 114 Resp: 539540
Ion Ratio Lower Upper
114 100
63 20.4 0.0 40.8
88 16.4 0.0 32.8


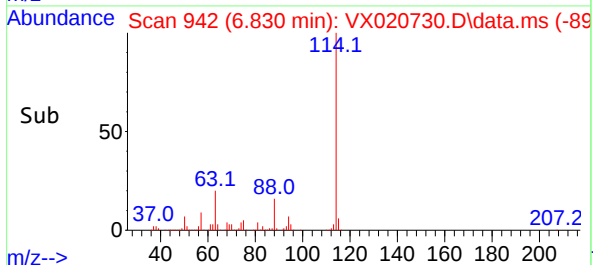

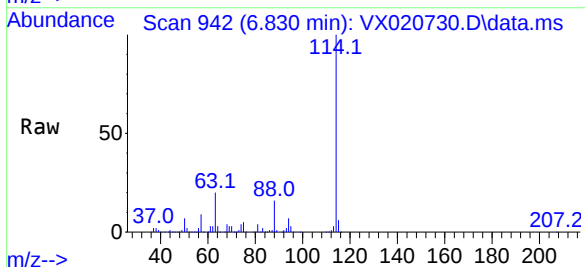


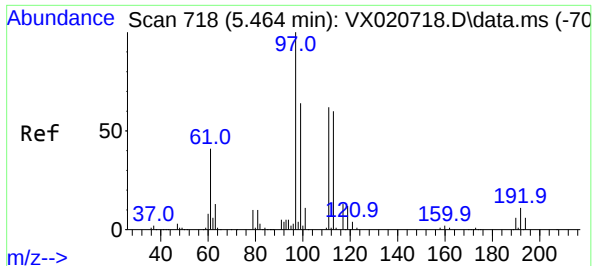

#35
Dibromofluoromethane
Concen: 49.15 ug/l
RT: 5.464 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampleId :
41052


Tgt Ion:113 Resp: 181644
Ion Ratio Lower Upper
113 100
111 103.0 81.9 122.9
192 19.3 16.7 25.1

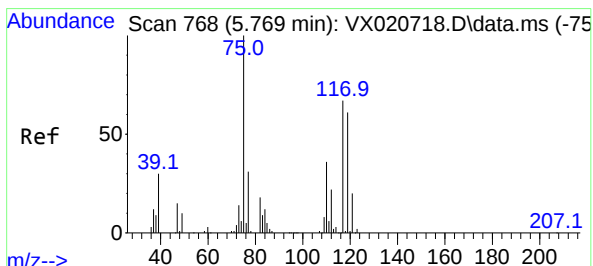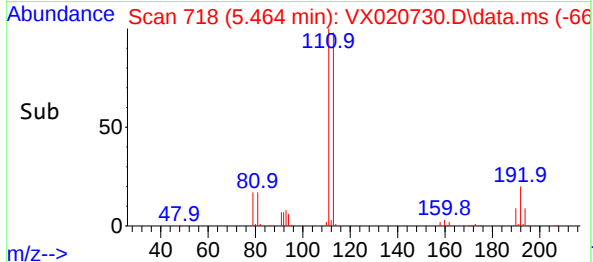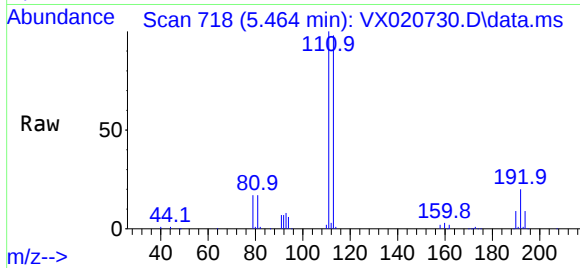

#36
1,1-Dichloropropene
Concen: 4.60 ug/l
RT: 5.623 min Scan# 744
Delta R.T. -0.146 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 75 Resp: 24912
Ion Ratio Lower Upper
75 100
110 9.0 18.1 54.4#
77 0.0 25.3 37.9#

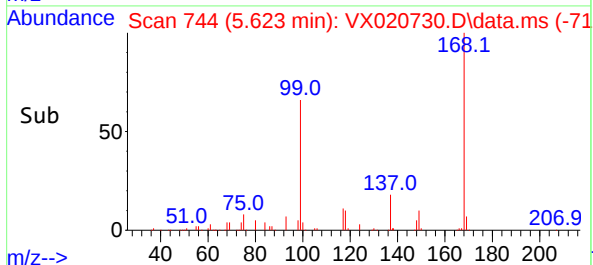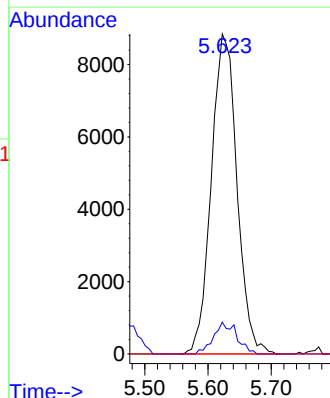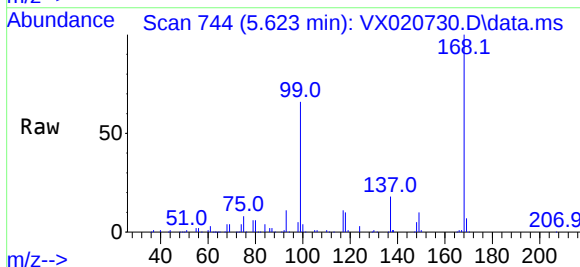

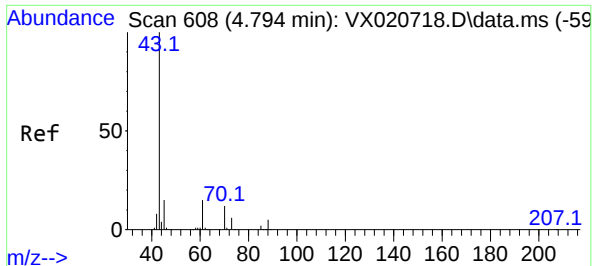

#37

Ethyl Acetate

Concen: 0.42 ug/l

RT: 4.806 min Scan# 610

Delta R.T. 0.012 min





Lab File: VX020730.D

Acq: 25 Jan 2021 17:22

Instrument :
MSVOA_X
ClientSampleId :
41052

Tgt Ion: 43 Resp: 2147

Ion	Ratio	Lower	Upper
43	100		
61	7.6	12.8	19.2#
70	0.0	10.5	15.7#

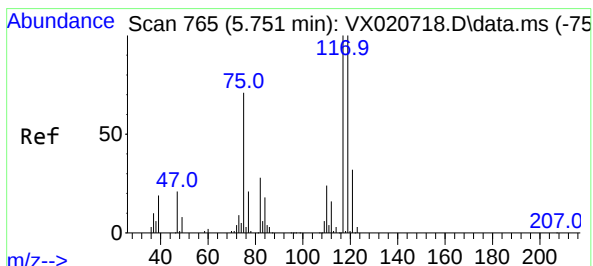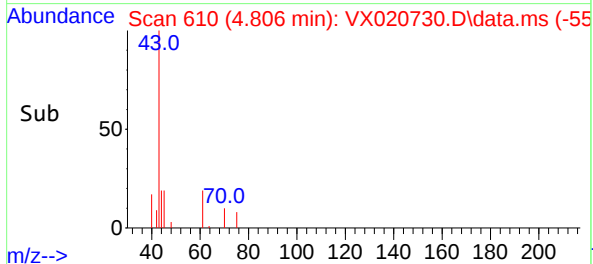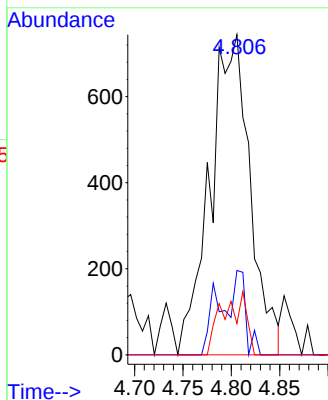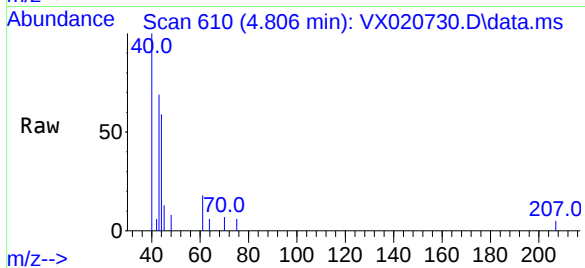

#38

Carbon Tetrachloride

Concen: 5.78 ug/l

RT: 5.623 min Scan# 744




Delta R.T. -0.128 min


Lab File: VX020730.D

Acq: 25 Jan 2021 17:22

Tgt Ion: 117 Resp: 32895

Ion	Ratio	Lower	Upper
117	100		
119	4.6	76.2	114.2#
121	0.0	24.8	37.2#


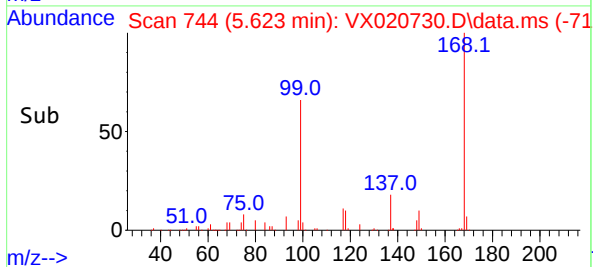
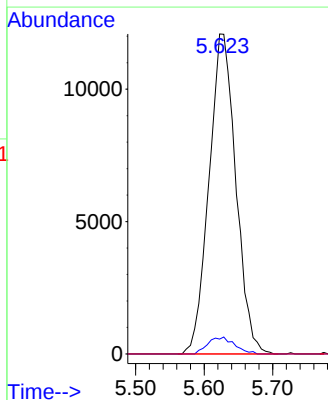
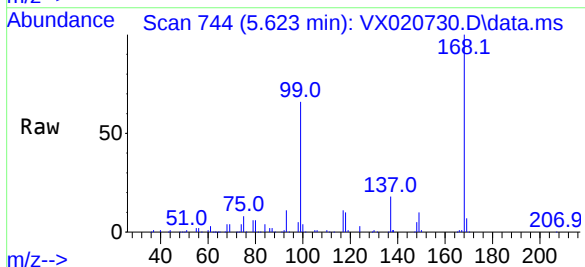




#40
Benzene
Concen: 0.32 ug/l
RT: 6.104 min Scan# 823
Delta R.T. -0.007 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampleId :
41052


Tgt Ion: 78 Resp: 5057
Ion Ratio Lower Upper
78 100
77 18.0 18.9 28.3#

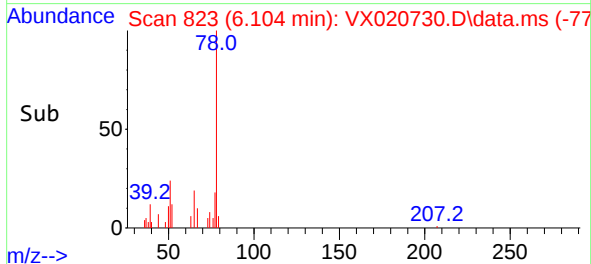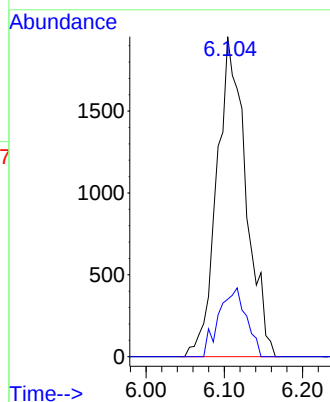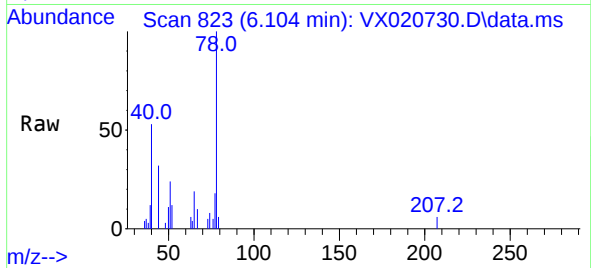

#50
Toluene-d8
Concen: 49.50 ug/l
RT: 8.695 min Scan# 1248
Delta R.T. -0.001 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 98 Resp: 670664
Ion Ratio Lower Upper
98 100
100 65.8 51.9 77.9


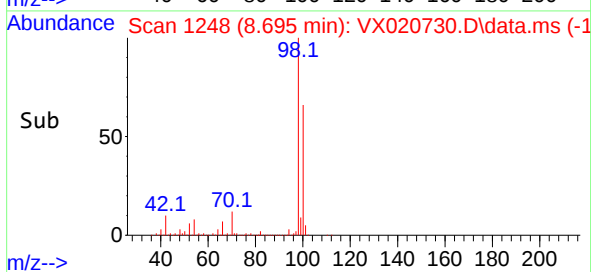




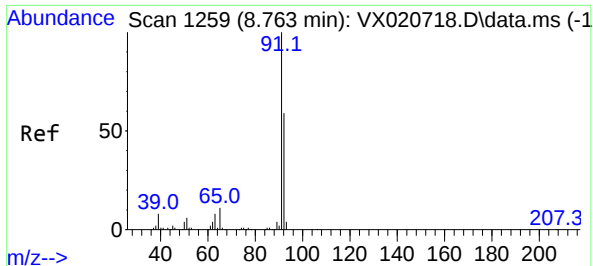

#52
Toluene
Concen: 13.36 ug/l
RT: 8.762 min Scan# 1259
Delta R.T. -0.001 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampled :
41052


Tgt Ion: 92 Resp: 133976
Ion Ratio Lower Upper
92 100
91 168.7 137.1 205.7

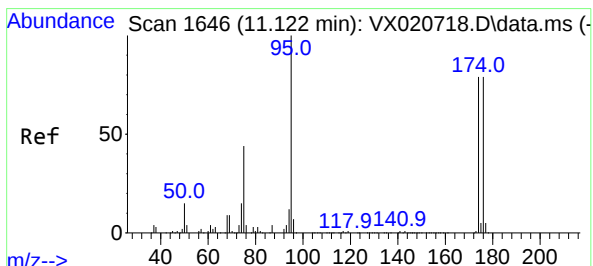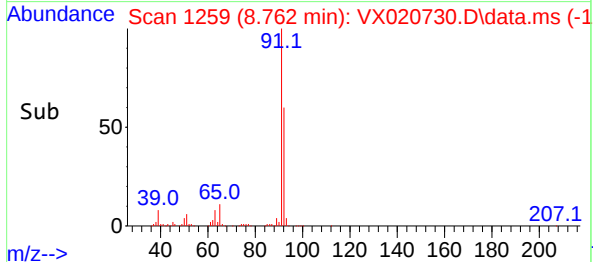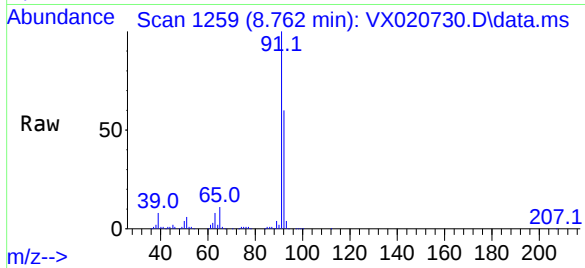

#62
4-Bromofluorobenzene
Concen: 47.12 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.000 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 95 Resp: 247939
Ion Ratio Lower Upper
95 100
174 75.1 0.0 154.6
176 74.4 0.0 155.8


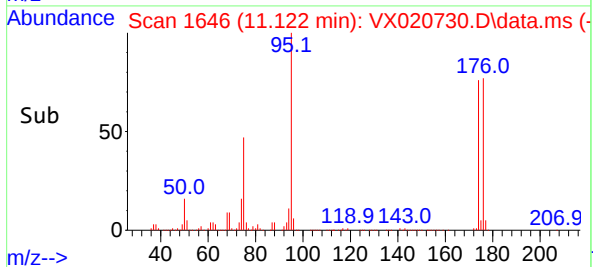

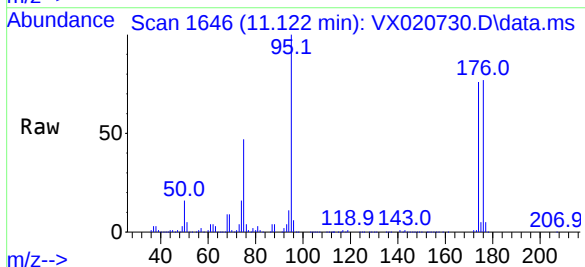




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.097 min Scan# 1478
Delta R.T. 0.005 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampled :
41052


Tgt Ion:117 Resp: 518974
Ion Ratio Lower Upper
117 100
82 57.5 47.4 71.2
119 32.0 26.6 39.8

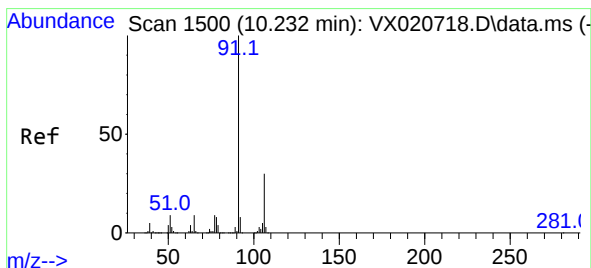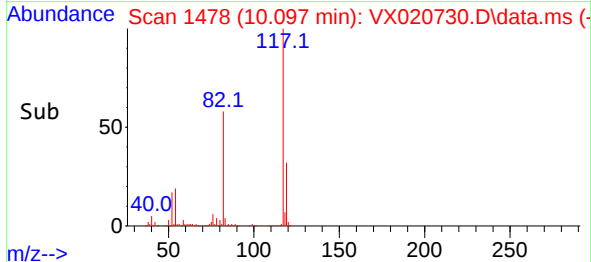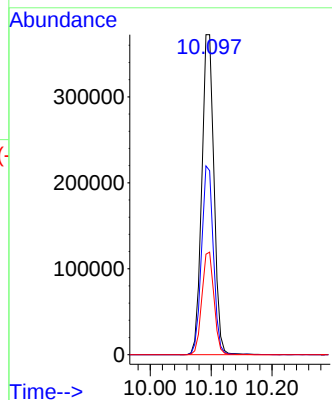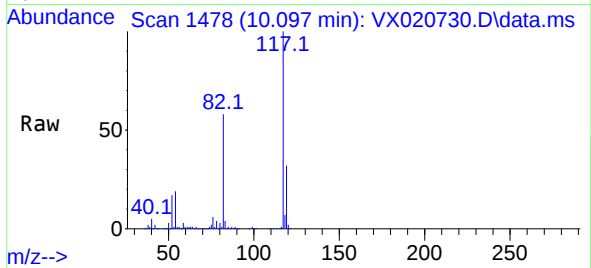

#67
Ethyl Benzene
Concen: 0.84 ug/l
RT: 10.232 min Scan# 1500
Delta R.T. -0.000 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 91 Resp: 16318
Ion Ratio Lower Upper
91 100
106 27.1 24.6 37.0


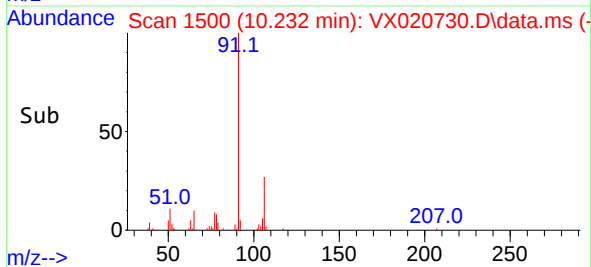
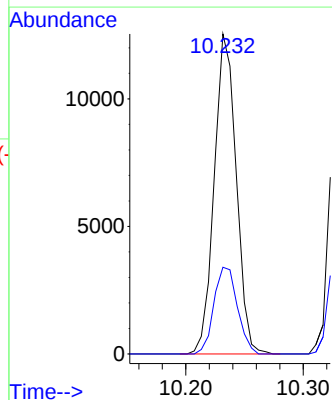
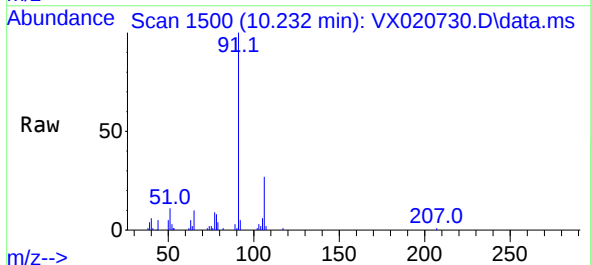




#68
m/p-Xylenes
Concen: 3.29 ug/l
RT: 10.341 min Scan# 1518
Delta R.T. -0.001 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampled :
41052


Tgt Ion:106 Resp: 23874
Ion Ratio Lower Upper
106 100
91 205.8 162.8 244.2

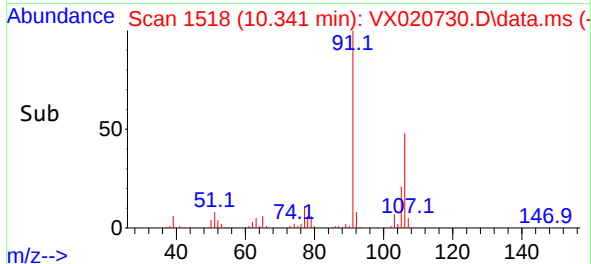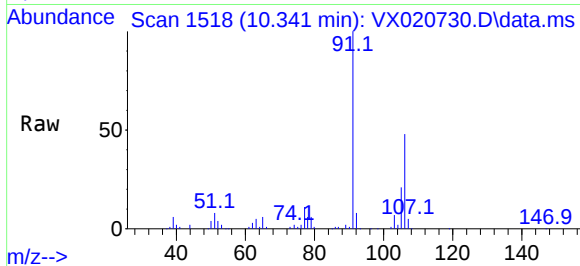

#69
o-Xylene
Concen: 1.90 ug/l
RT: 10.683 min Scan# 1574
Delta R.T. -0.000 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion:106 Resp: 12960
Ion Ratio Lower Upper
106 100
91 223.4 108.1 324.2


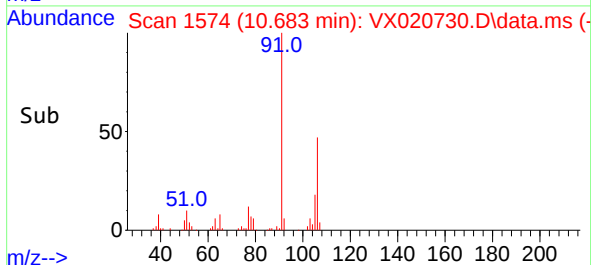
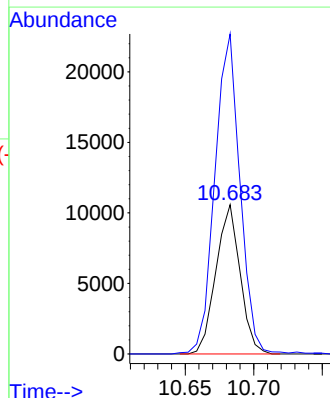
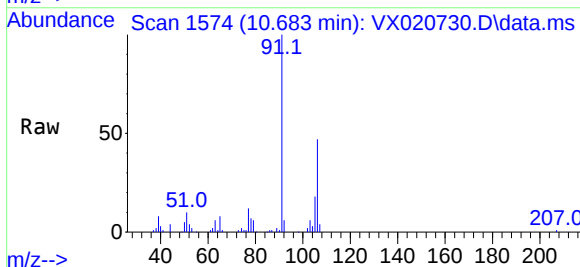




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.060 min Scan# 1800
Delta R.T. -0.001 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampleId :
41052


Tgt Ion:152 Resp: 236074
Ion Ratio Lower Upper
152 100
115 61.6 41.1 123.3
150 158.6 0.0 349.0

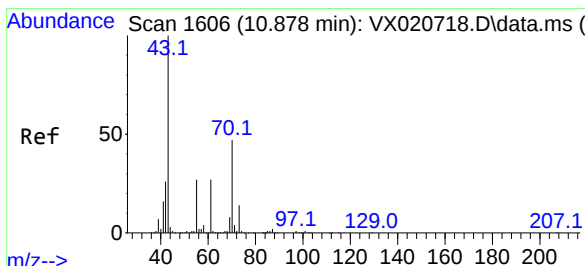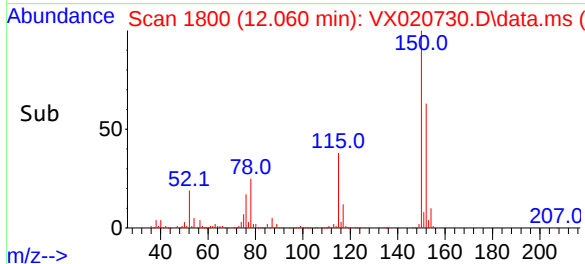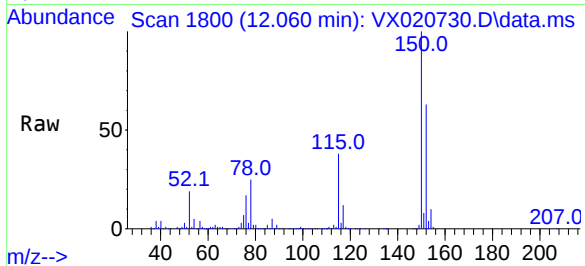

#74
N-ethyl acetate
Concen: 2.03 ug/l
RT: 10.896 min Scan# 1609
Delta R.T. 0.018 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 43 Resp: 124
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.6#
55 275.0 21.5 32.3#
61 0.0 22.1 33.1#


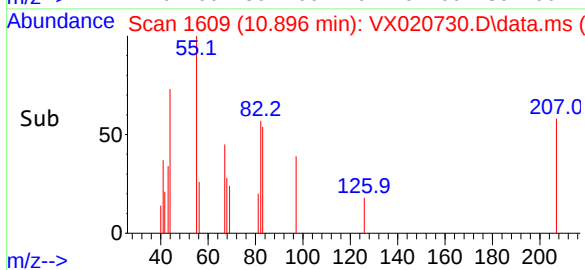

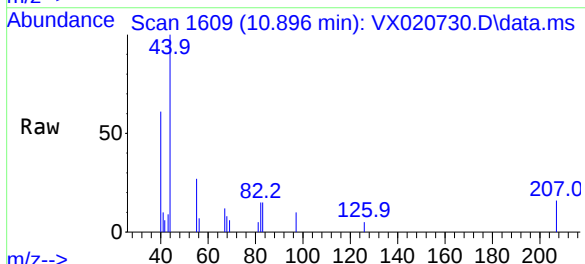


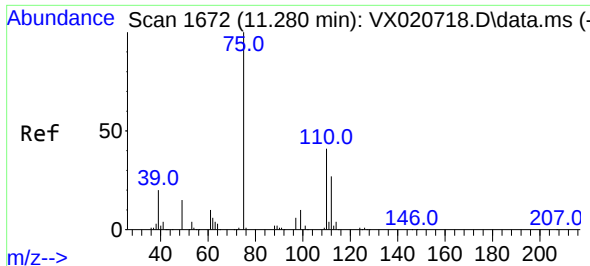

#76
1,2,3-Trichloropropane
Concen: 22.32 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. -0.164 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampled :
41052


Tgt Ion: 75 Resp: 122212
Ion Ratio Lower Upper
75 100
77 1.2 19.1 57.5#

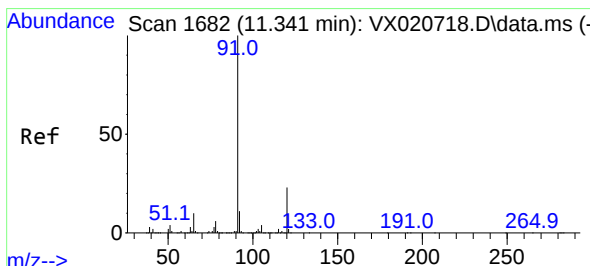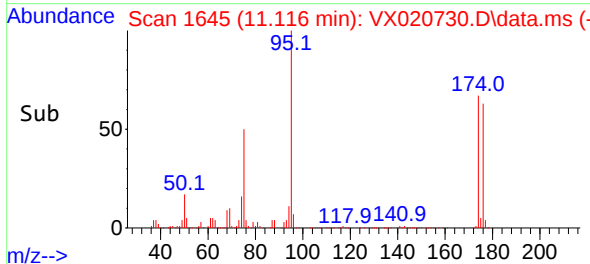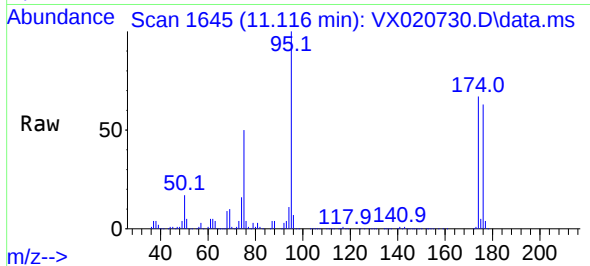

#78
n-propylbenzene
Concen: 0.54 ug/l
RT: 11.341 min Scan# 1682
Delta R.T. 0.000 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 91 Resp: 10563
Ion Ratio Lower Upper
91 100
120 20.8 11.5 34.5


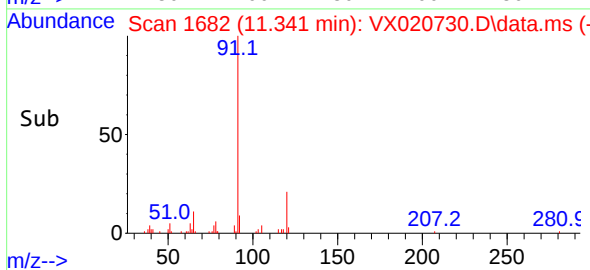

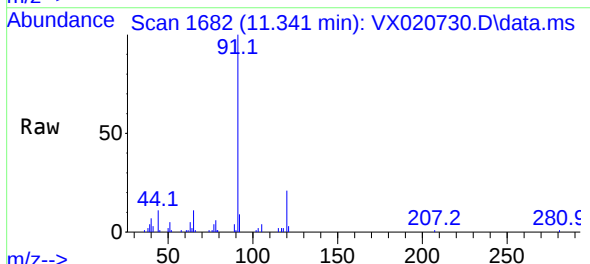




#79
2-Chlorotoluene
Concen: 0.48 ug/l
RT: 11.414 min Scan# 1694
Delta R.T. 0.012 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampled :
41052


Tgt Ion: 91 Resp: 5833
Ion Ratio Lower Upper
91 100
126 1.5 16.6 49.8#

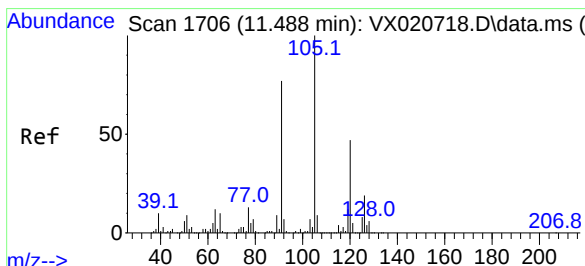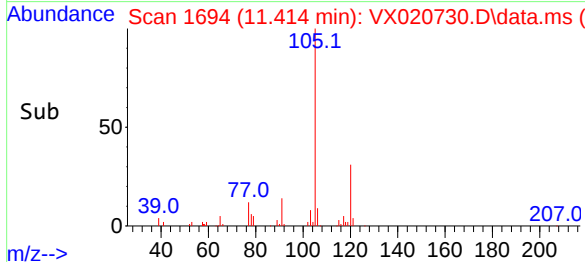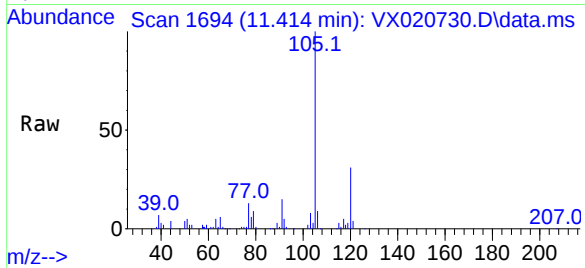

#80
1,3,5-Trimethylbenzene
Concen: 0.99 ug/l
RT: 11.487 min Scan# 1706
Delta R.T. -0.001 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 105 Resp: 14366
Ion Ratio Lower Upper
105 100
120 44.4 23.8 71.5


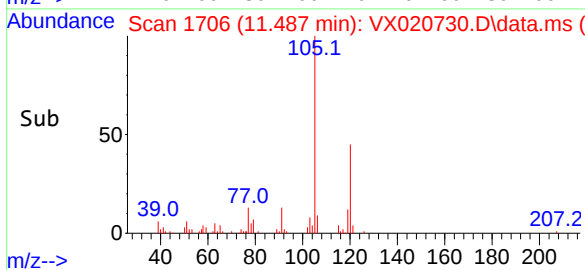

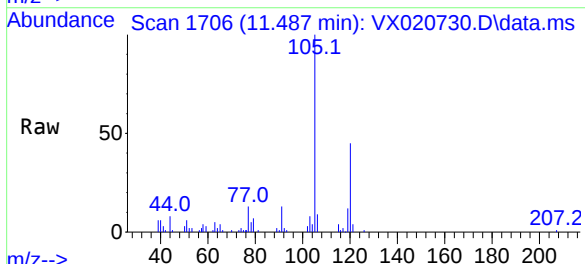




#81
trans-1,4-Dichloro-2-butene
Concen: 62.55 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. 0.061 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampled :
41052


Tgt Ion: 75 Resp: 122212
Ion Ratio Lower Upper
75 100
53 0.1 74.5 111.7#
89 0.0 37.9 56.9#

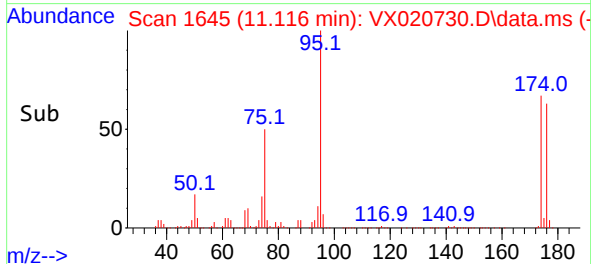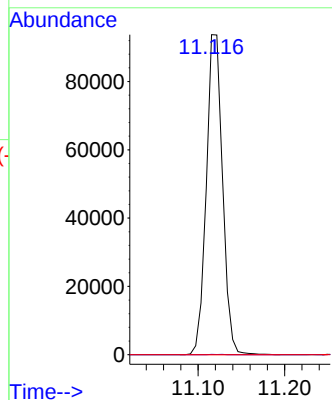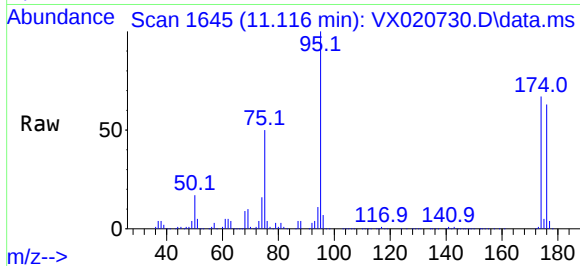

#83
tert-Butylbenzene
Concen: 0.50 ug/l
RT: 11.792 min Scan# 1756
Delta R.T. 0.042 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 119 Resp: 7015
Ion Ratio Lower Upper
119 100
91 91.2 27.9 83.7#
134 0.0 11.3 33.9#


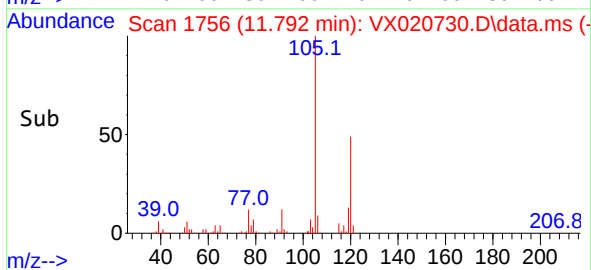
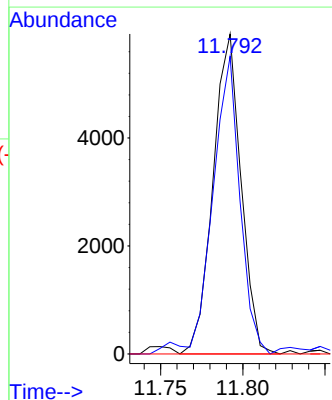
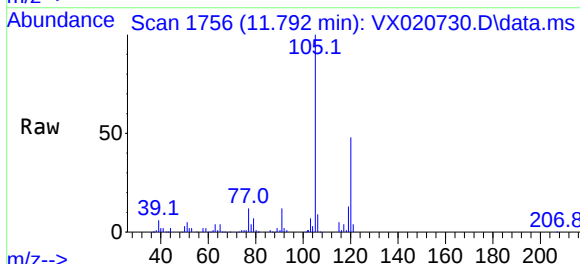




#84
1,2,4-Trimethylbenzene
Concen: 3.98 ug/l
RT: 11.792 min Scan# 1756
Delta R.T. -0.001 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampled :
41052


Tgt Ion:105 Resp: 58534
Ion Ratio Lower Upper
105 100
120 44.8 22.4 67.3

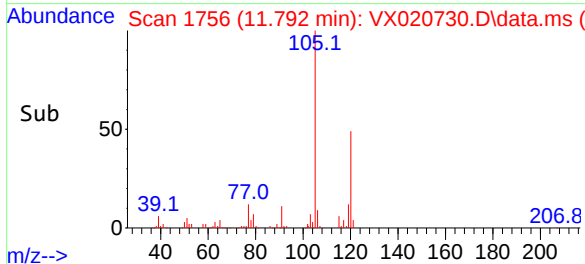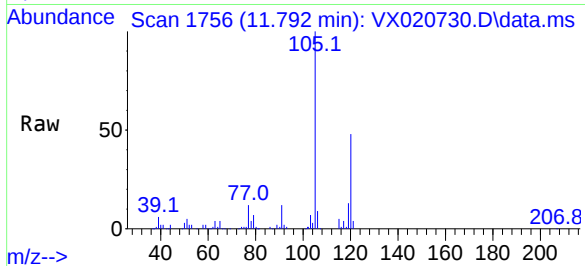

#85
sec-Butylbenzene
Concen: 0.31 ug/l
RT: 11.926 min Scan# 1778
Delta R.T. -0.001 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion:105 Resp: 5013
Ion Ratio Lower Upper
105 100
134 25.0 10.0 29.8


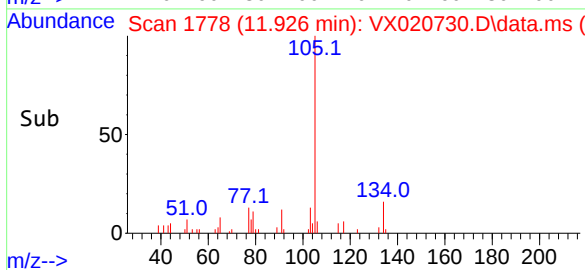

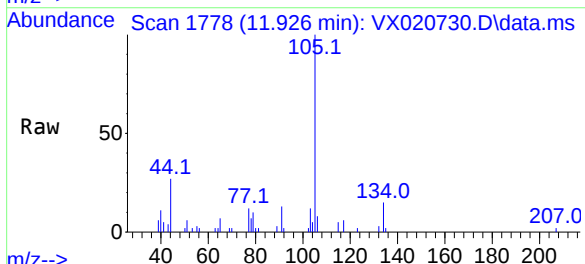




#86
p-Isopropyltoluene
Concen: 0.39 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.043 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22




Instrument :
MSVOA_X
ClientSampleId :
41052


Tgt Ion:119 Resp: 5966
Ion Ratio Lower Upper
119 100
134 26.4 12.9 38.7
91 25.5 11.7 35.0

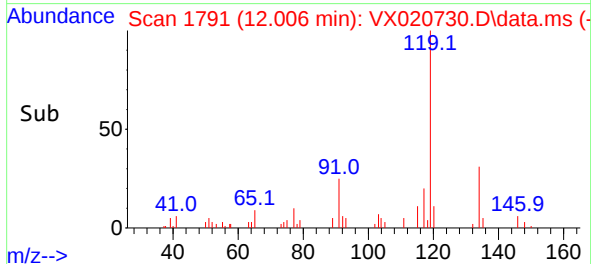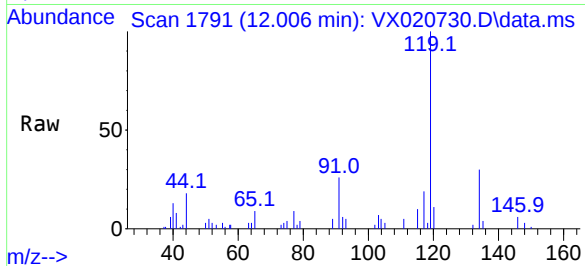

#89
n-Butylbenzene
Concen: 0.83 ug/l
RT: 12.371 min Scan# 1851
Delta R.T. -0.001 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion: 91 Resp: 11176
Ion Ratio Lower Upper
91 100
92 39.1 27.4 82.0
134 88.9 13.2 39.5#


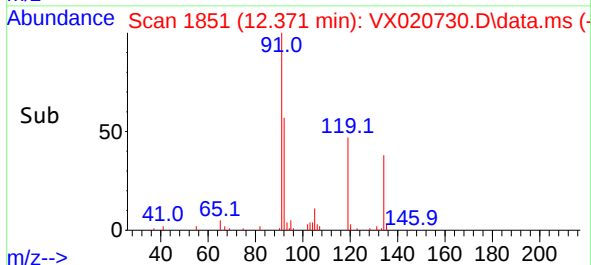
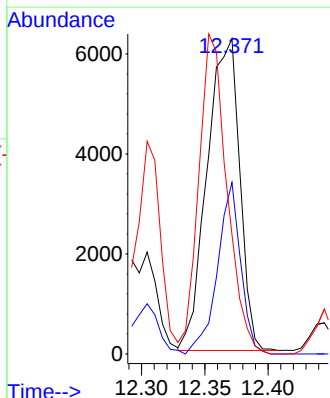
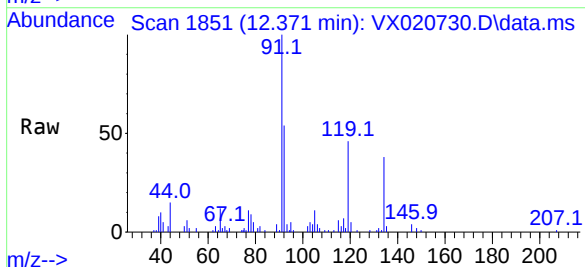




#90
Hexachloroethane
Concen: 0.65 ug/l
RT: 12.591 min Scan# 1887
Delta R.T. 0.012 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Instrument :
MSVOA_X
ClientSampled :
41052

Tgt Ion:117 Resp: 1773
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

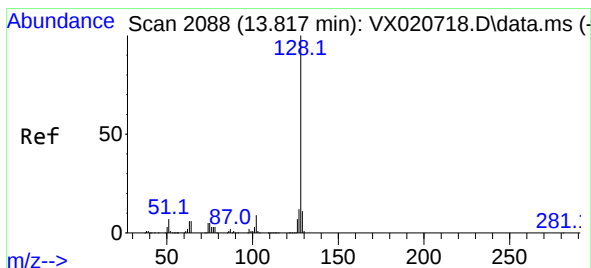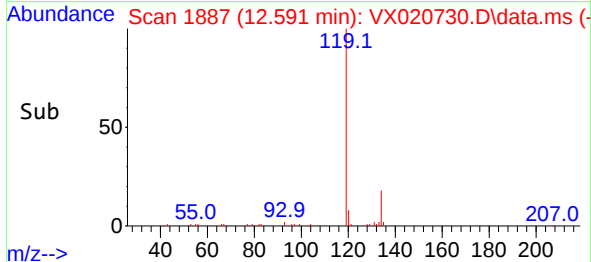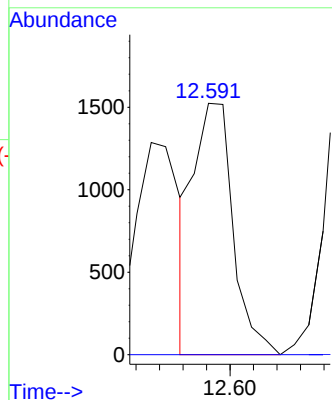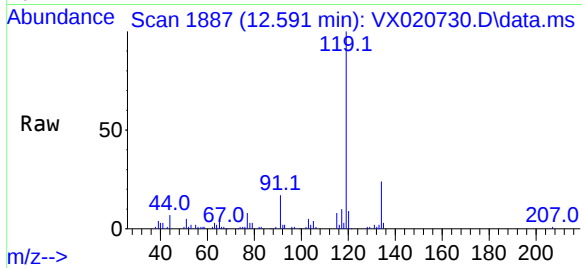

#95
Naphthalene
Concen: 4.13 ug/l
RT: 13.816 min Scan# 2088
Delta R.T. -0.001 min
Lab File: VX020730.D
Acq: 25 Jan 2021 17:22

Tgt Ion:128 Resp: 24247
Ion Ratio Lower Upper
128 100
127 12.3 10.3 15.5
129 12.9 8.8 13.2

