
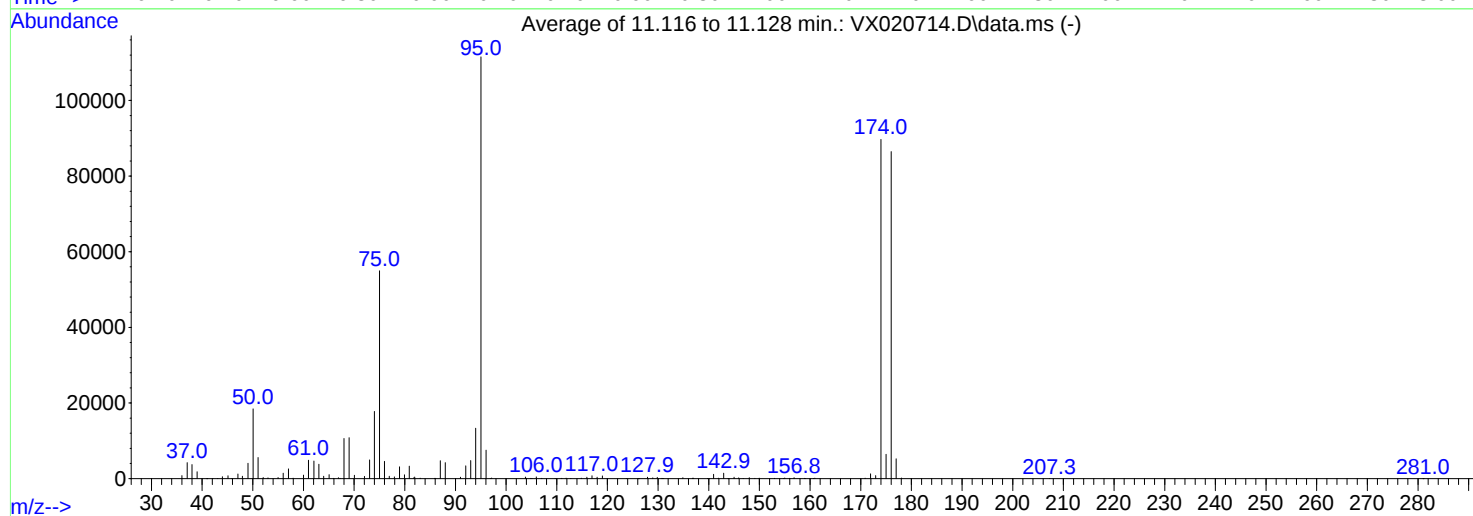


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012521\
 Data File : VX020714.D
 Acq On : 25 Jan 2021 09:32
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Title : SW846 8260
 Last Update : Mon Jan 25 13:38:15 2021

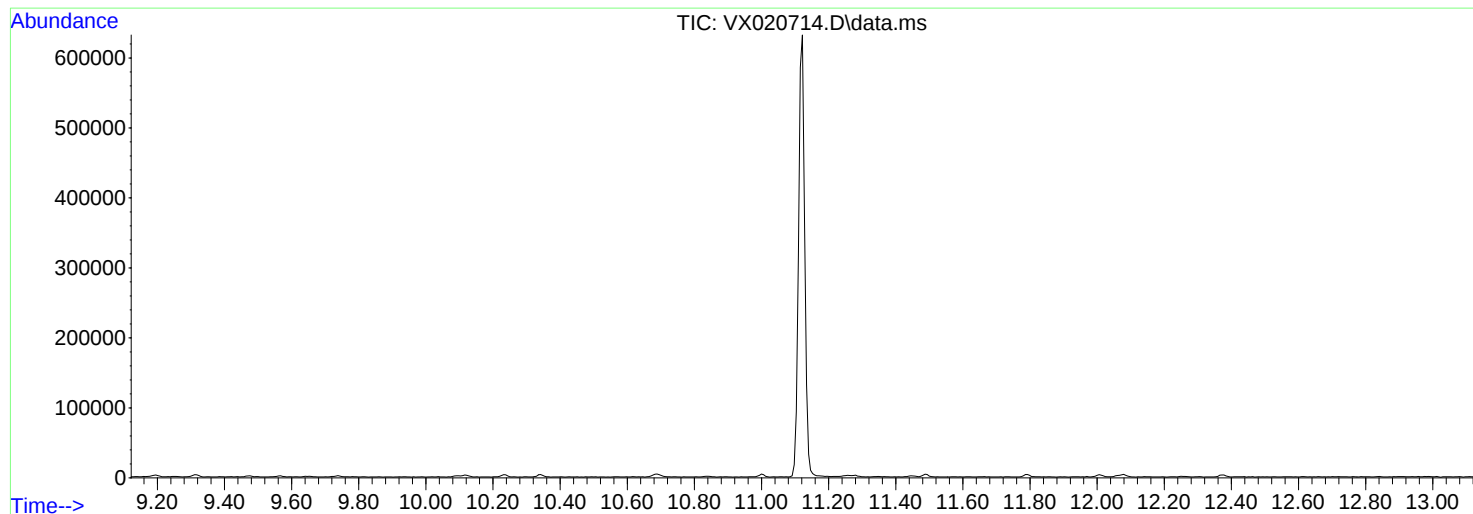

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	18458	PASS
75	95	30	60	49.3	54957	PASS
95	95	100	100	100.0	111531	PASS
96	95	5	9	6.8	7531	PASS
173	174	0.00	2	0.9	817	PASS
174	95	50	100	80.4	89709	PASS
175	174	5	9	7.2	6435	PASS
176	174	95	101	96.4	86464	PASS
177	176	5	9	6.1	5253	PASS