

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012523\
 Data File : VX033891.D
 Acq On : 25 Jan 2023 16:34
 Operator : JC/MD
 Sample : 01308-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 22-MW-2I

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M

Title : SW846 8260

Signal : TIC: VX033891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.940	297	304	313	rVB	3465	7773	1.16%	0.202%
2	4.562	560	570	583	rVB2	10306	34406	5.12%	0.895%
3	5.385	693	705	721	rBV2	78922	233624	34.78%	6.075%
4	5.550	721	732	748	rVV	144625	410754	61.15%	10.680%
5	5.958	789	799	813	rBV	79659	215418	32.07%	5.601%
6	6.763	921	931	952	rBV	206880	500242	74.48%	13.007%
7	7.129	982	991	1009	rBV	96288	212102	31.58%	5.515%
8	8.647	1234	1240	1253	rBV	437006	671661	100.00%	17.464%
9	10.055	1465	1471	1484	rBV	408076	574195	85.49%	14.930%
10	11.079	1634	1639	1648	rBV	344459	444953	66.25%	11.569%
11	12.024	1788	1794	1803	rBV	418508	540802	80.52%	14.062%




Sum of corrected areas: 3845930

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012523\
Data File : VX033891.D
Acq On : 25 Jan 2023 16:34
Operator : JC/MD
Sample : 01308-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
22-MW-2I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

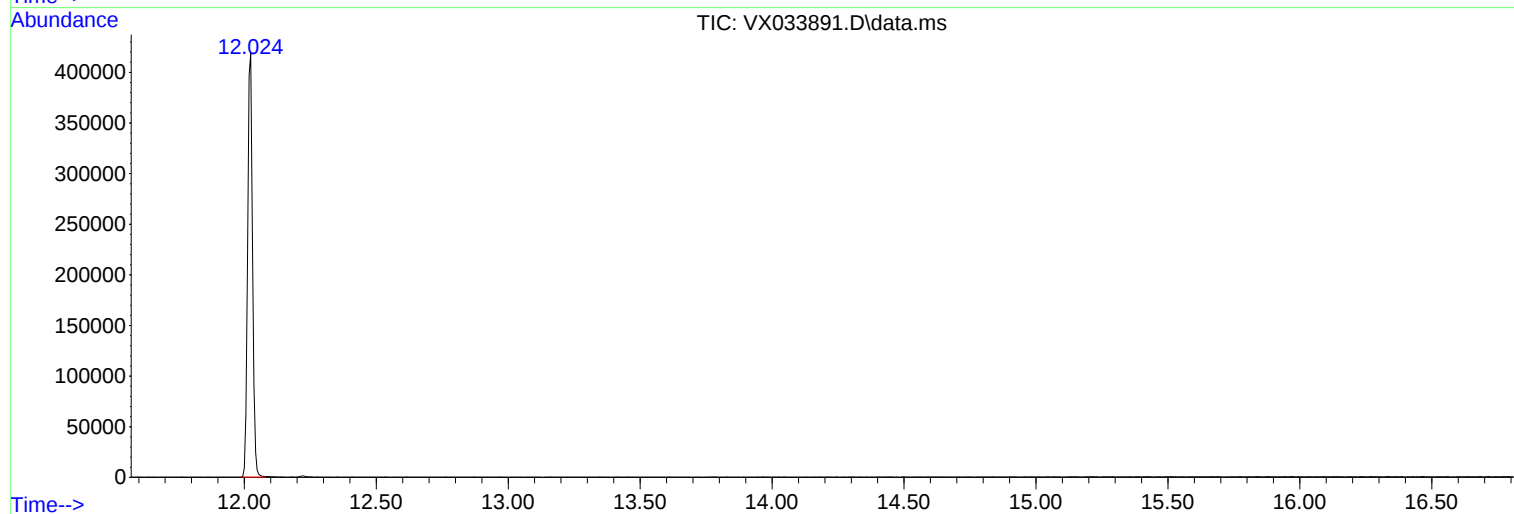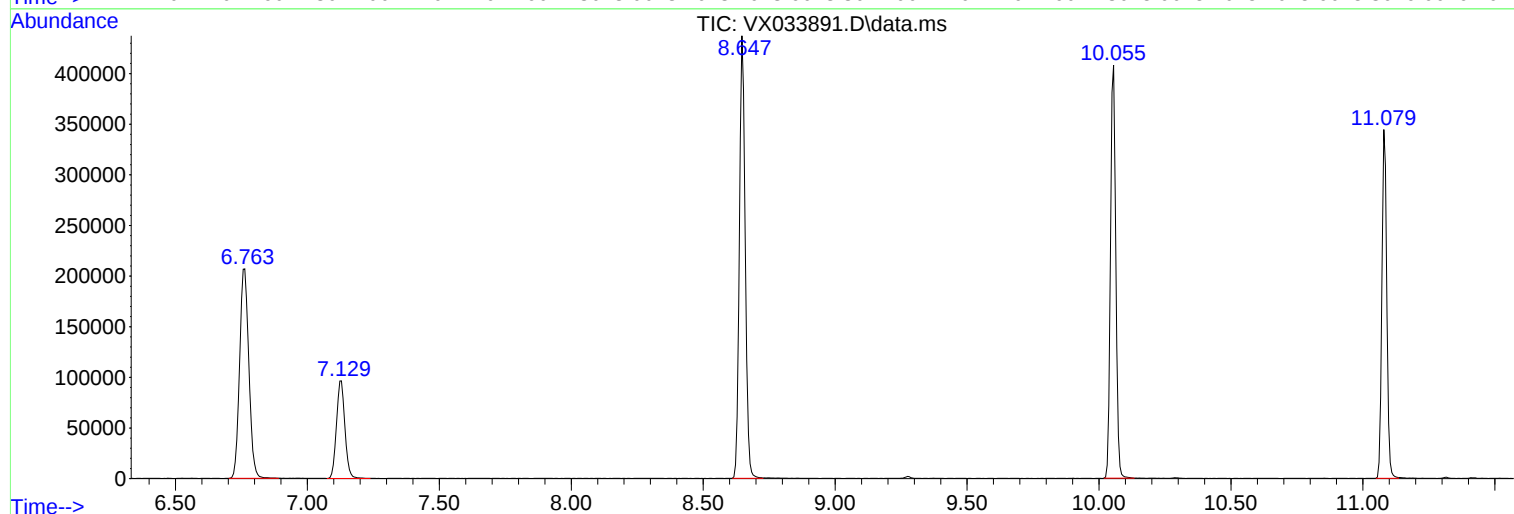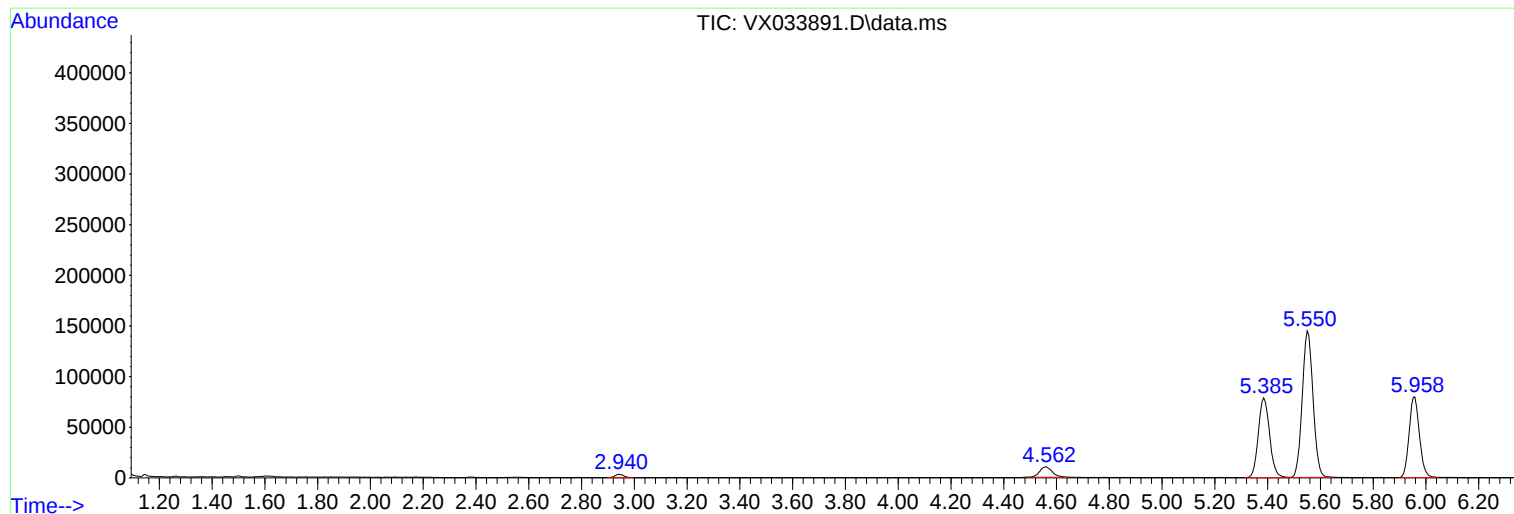

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012523\
Data File : VX033891.D
Acq On : 25 Jan 2023 16:34
Operator : JC/MD
Sample : 01308-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
22-MW-2I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012523\
Data File : VX033891.D
Acq On : 25 Jan 2023 16:34
Operator : JC/MD
Sample : 01308-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
22-MW-2I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------