
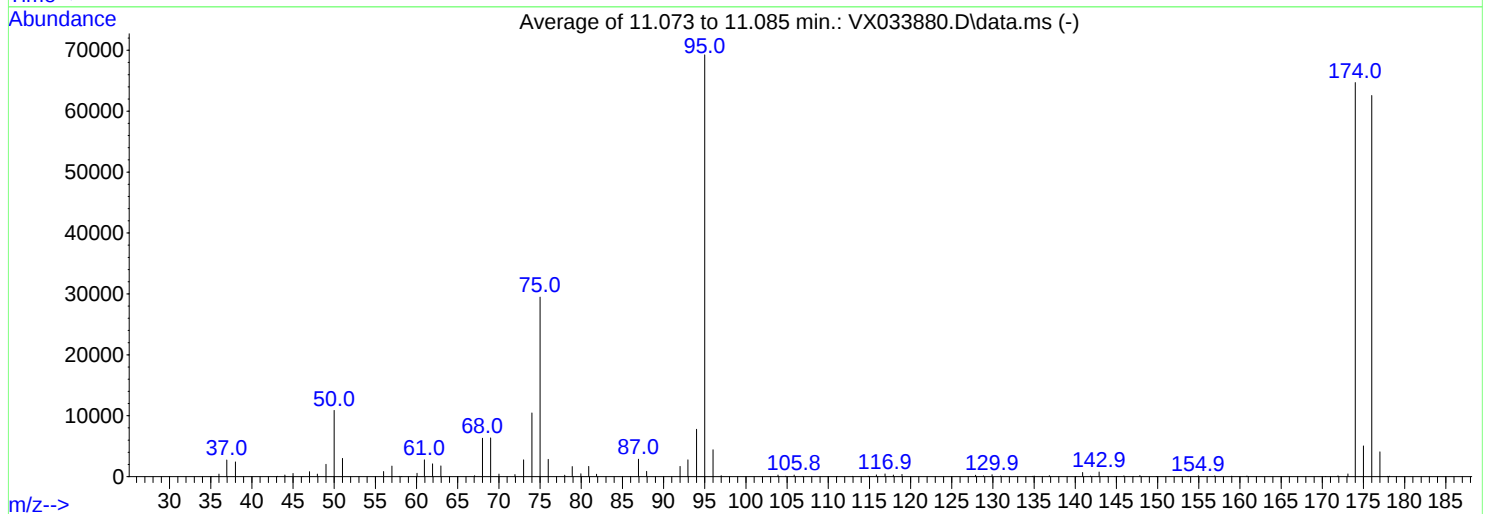


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012523\
Data File : VX033880.D
Acq On : 25 Jan 2023 10:41
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDCCC050

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Title : SW846 8260
Last Update : Wed Jan 11 14:48:42 2023

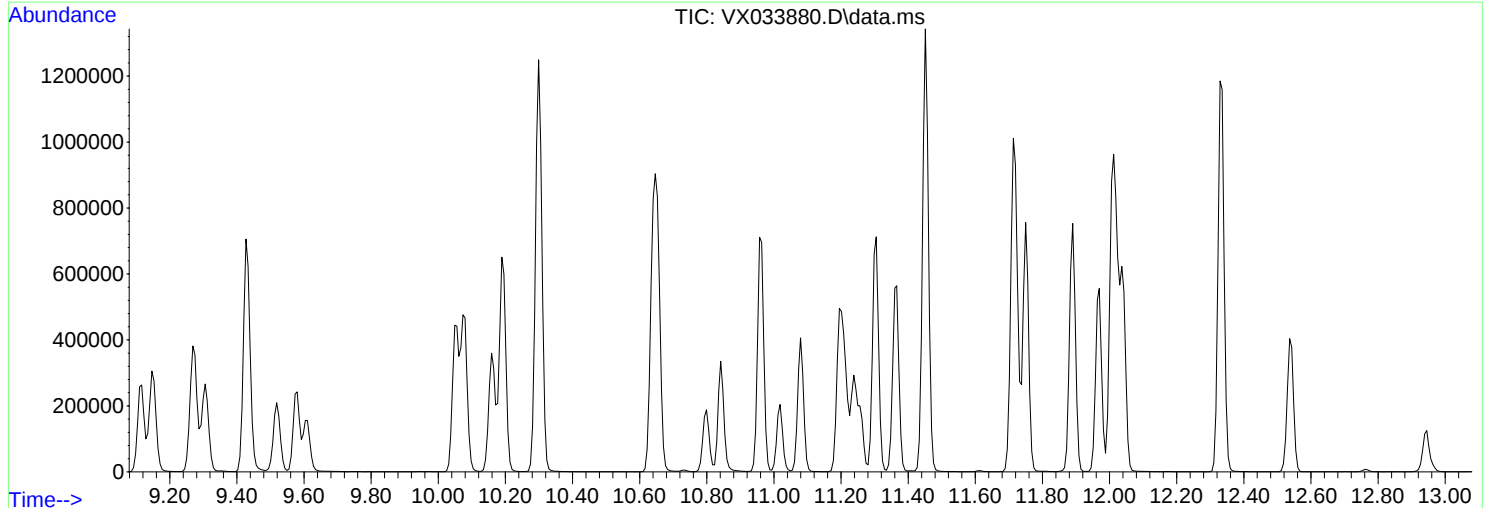

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	10869	PASS
75	95	30	60	42.6	29473	PASS
95	95	100	100	100.0	69251	PASS
96	95	5	9	6.4	4422	PASS
173	174	0.00	2	0.7	462	PASS
174	95	50	100	93.4	64688	PASS
175	174	5	9	7.8	5046	PASS
176	174	95	101	96.7	62573	PASS
177	176	5	9	6.5	4082	PASS