

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012524\
 Data File : VX039958.D
 Acq On : 25 Jan 2024 16:50
 Operator : JC/MD
 Sample : P1218-07DL 5X
 Misc : 5.07g/10mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 26 01:36:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 03:51:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	82618	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	151769	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	140080	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	78244	50.000	ug/l	0.00


System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	65188	47.102	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.200%
35) Dibromofluoromethane	5.385	113	46769	45.752	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.500%
50) Toluene-d8	8.647	98	186004	48.245	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.500%
62) 4-Bromofluorobenzene	11.079	95	78409	52.008	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	104.020%

Target Compounds			Qvalue			
5) Bromomethane	1.605	94	301	0.458	ug/l #	69
11) Tert butyl alcohol	2.947	59	1176	3.264	ug/l #	78
16) Acetone	2.386	43	2193	2.818	ug/l #	85
20) Methylene Chloride	2.782	84	250	0.212	ug/l #	62
31) Cyclohexane	5.501	56	4395	2.406	ug/l #	52
36) 1,1-Dichloropropene	5.550	75	7934	4.986	ug/l #	50
38) Carbon Tetrachloride	5.550	117	9271	6.362	ug/l #	15
39) Methylcyclohexane	7.373	83	3209	1.680	ug/l #	88
43) Isopropyl Acetate	6.196	43	2335	0.750	ug/l #	62
48) Methyl methacrylate	7.653	41	897	0.586	ug/l #	67
51) 4-Methyl-2-Pentanone	8.641	43	974	0.454	ug/l #	1
52) Toluene	8.720	92	322541	119.853	ug/l	95
53) t-1,3-Dichloropropene	8.714	75	4012	2.445	ug/l #	1
55) 1,1,2-Trichloroethane	9.104	97	537	0.469	ug/l #	17
59) 2-Hexanone	9.391	43	394	0.232	ug/l #	26
67) Ethyl Benzene	10.195	91	5929	1.095	ug/l	96
68) m/p-Xylenes	10.299	106	7894	3.963	ug/l	89
69) o-Xylene	10.640	106	3645	1.848	ug/l	94
73) Isopropylbenzene	10.964	105	1869	0.300	ug/l	92
76) 1,2,3-Trichloropropane	11.079	75	44376	21.876	ug/l #	39
78) n-propylbenzene	11.305	91	7480	0.992	ug/l	93
79) 2-Chlorotoluene	11.378	91	3501	0.751	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	6227	1.177	ug/l	93
81) trans-1,4-Dichloro-2-b...	11.079	75	44376	63.525	ug/l #	5
82) 4-Chlorotoluene	11.457	91	1332	0.252	ug/l #	55
83) tert-Butylbenzene	11.969	119	1918	0.380	ug/l	73
84) 1,2,4-Trimethylbenzene	11.750	105	23739	4.497	ug/l	99
85) sec-Butylbenzene	11.890	105	2099	0.320	ug/l	86
86) p-Isopropyltoluene	11.969	119	1989	0.380	ug/l	80
89) n-Butylbenzene	12.335	91	5191	1.026	ug/l #	64
90) Hexachloroethane	12.536	117	486	0.550	ug/l #	17
95) Naphthalene	13.780	128	1920	0.325	ug/l #	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jan 26 01:36:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 03:51:26 2024
Response via : Initial Calibration






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50




Instrument :

MSVOA_X

ClientSampleId :







Tgt Ion:168 Resp: 82618
Ion Ratio Lower Upper
168 100
99 68.0 56.6 85.0



#5
Bromomethane
Concen: 0.458 ug/l
RT: 1.605 min Scan# 85
Delta R.T. 0.006 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Tgt Ion: 94 Resp: 301
Ion Ratio Lower Upper
94 100
96 63.1 74.6 111.8#



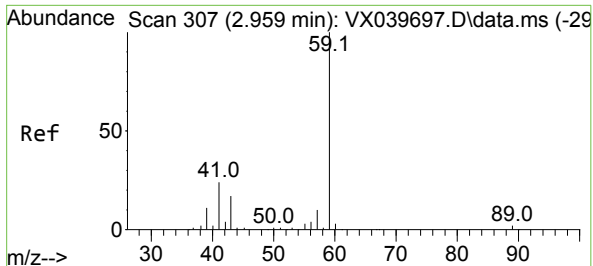

#11

Tert butyl alcohol

Concen: 3.264 ug/l

RT: 2.947 min Scan# 307

Delta R.T. -0.012 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 59 Resp: 1176

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

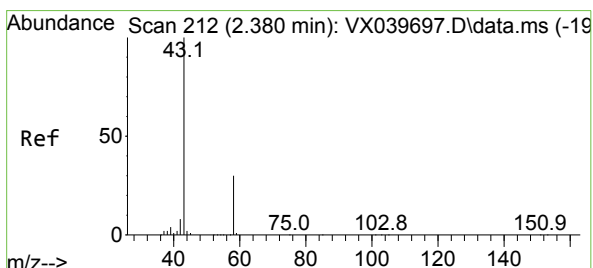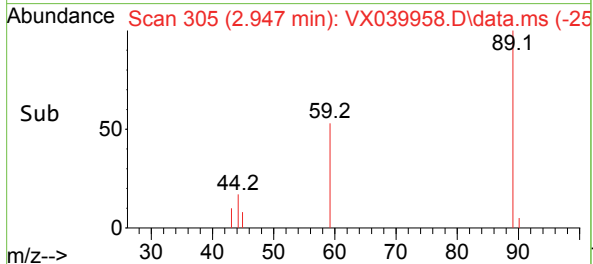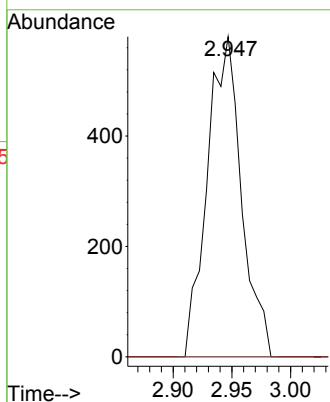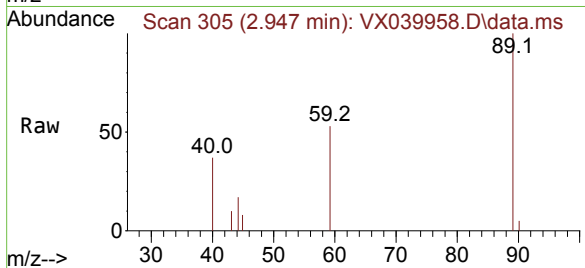

#16

Acetone

Concen: 2.818 ug/l

RT: 2.386 min Scan# 213

Delta R.T. 0.006 min

Lab File: VX039958.D




Acq: 25 Jan 2024 16:50


Tgt Ion: 43 Resp: 2193

Ion Ratio Lower Upper

43 100


58 19.6 21.9 32.9#

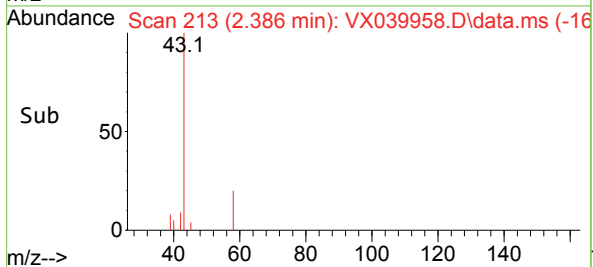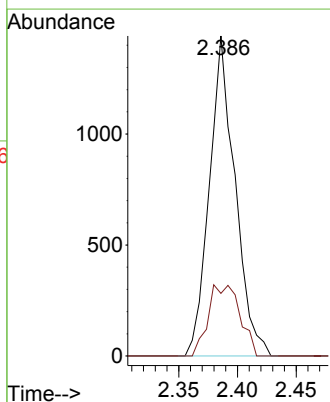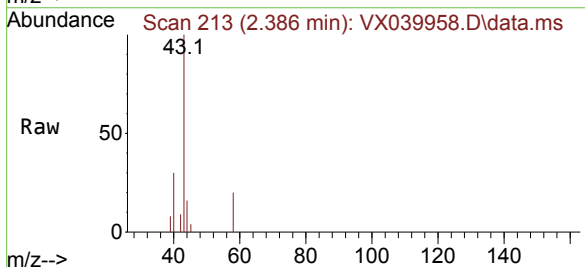





#20
Methylene Chloride
Concen: 0.212 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 84	Resp: 250
Ion Ratio	Lower Upper
84	100
49	90.3 103.6 155.4#
51	0.0 33.8 50.6#
86	42.0 49.4 74.0#



#31
Cyclohexane
Concen: 2.406 ug/l
RT: 5.501 min Scan# 724
Delta R.T. 0.031 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Tgt Ion: 56	Resp: 4395
Ion Ratio	Lower Upper
56	100
69	14.0 23.4 35.2#
84	33.5 65.9 98.9#





#33

1,2-Dichloroethane-d4

Concen: 47.102 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 65188

Ion Ratio Lower Upper

65 100

67 52.1 0.0 100.2

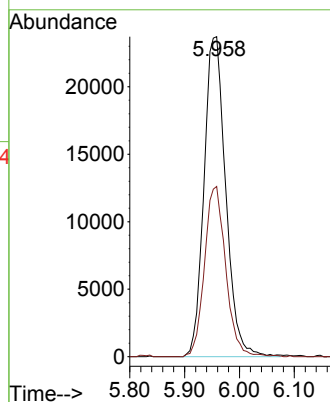

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50




Tgt Ion: 114 Resp: 151769


Ion Ratio Lower Upper

114 100

63 21.2 0.0 45.0


88 16.7 0.0 36.6

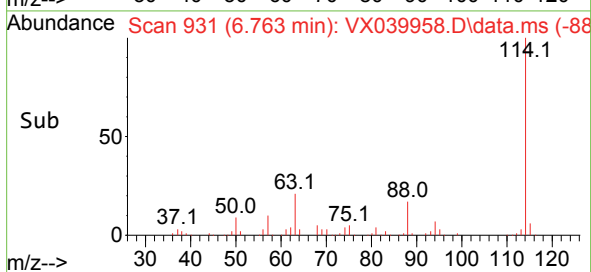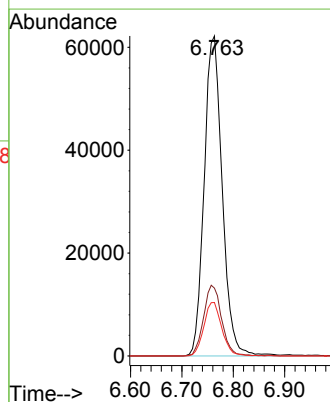



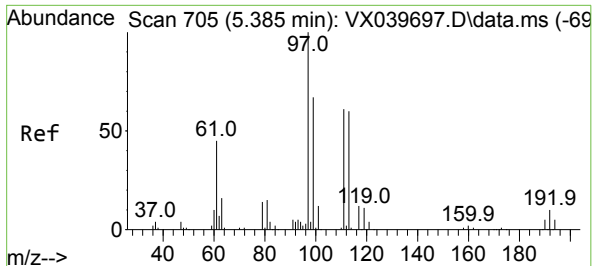


#35
Dibromofluoromethane
Concen: 45.752 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Instrument :
MSVOA_X
ClientSampleId :



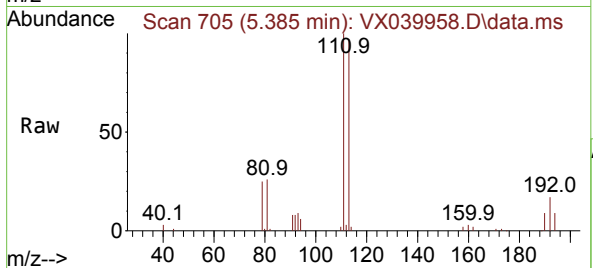



Tgt Ion:113 Resp: 46769
Ion Ratio Lower Upper
113 100
111 103.6 82.9 124.3
192 16.5 13.3 19.9

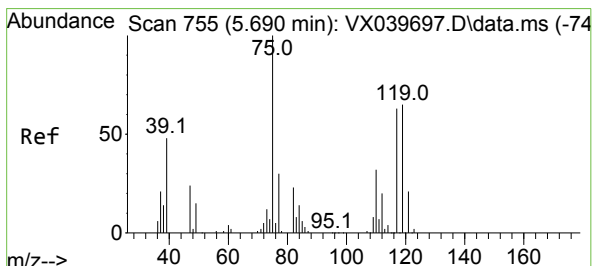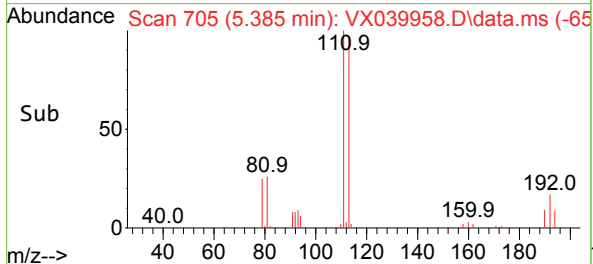

#36
1,1-Dichloropropene
Concen: 4.986 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50


Tgt Ion: 75 Resp: 7934
Ion Ratio Lower Upper
75 100
110 8.2 17.0 50.9#
77 0.0 24.7 37.1#

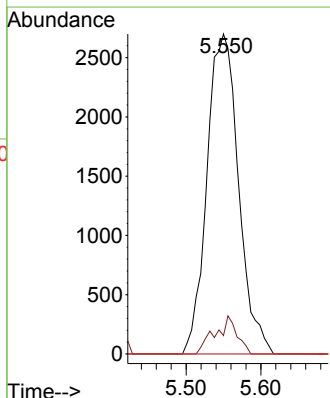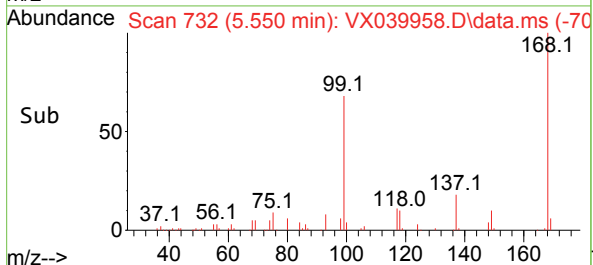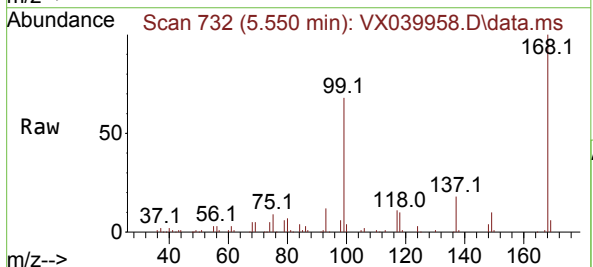






#38
Carbon Tetrachloride
Concen: 6.362 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 9271
Ion Ratio Lower Upper
117 100
119 4.9 78.2 117.2#
121 0.0 24.4 36.6#

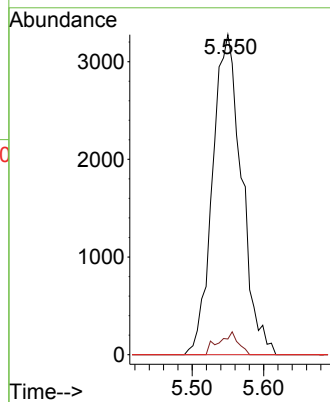

#39
Methylcyclohexane
Concen: 1.680 ug/l
RT: 7.373 min Scan# 1031
Delta R.T. -0.006 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50


Tgt Ion: 83 Resp: 3209
Ion Ratio Lower Upper
83 100
55 73.8 64.6 97.0
98 32.4 36.7 55.1#

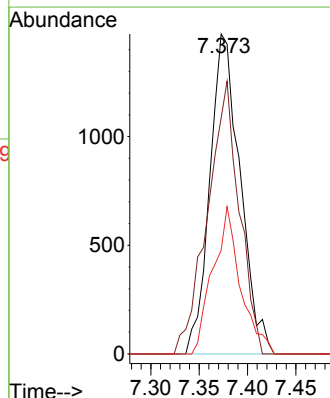






#43
Isopropyl Acetate
Concen: 0.750 ug/l
RT: 6.196 min Scan# 81
Delta R.T. -0.140 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 43 Resp: 2335
Ion Ratio Lower Upper
43 100
61 0.0 15.2 22.8#
87 0.0 9.8 14.6#

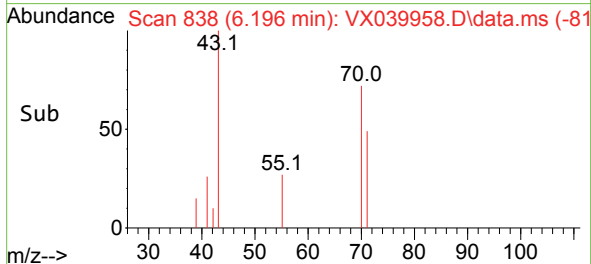

#48
Methyl methacrylate
Concen: 0.586 ug/l
RT: 7.653 min Scan# 1077
Delta R.T. -0.036 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Tgt Ion: 41 Resp: 897
Ion Ratio Lower Upper
41 100
69 124.9 59.2 88.8#
39 59.4 47.7 71.5









#50
Toluene-d8
Concen: 48.245 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 186004
Ion Ratio Lower Upper
98 100
100 64.1 53.1 79.7

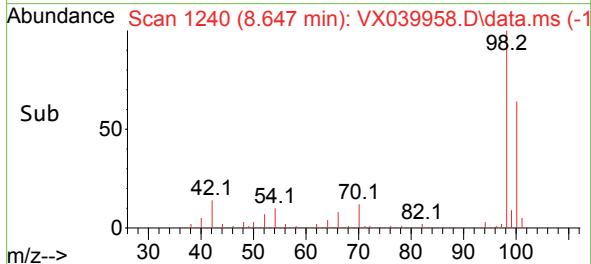

#51
4-Methyl-2-Pentanone
Concen: 0.454 ug/l
RT: 8.641 min Scan# 1239
Delta R.T. 0.067 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Tgt Ion: 43 Resp: 974
Ion Ratio Lower Upper
43 100
58 172.3 30.4 45.6#





#52

Toluene

Concen: 119.853 ug/l

RT: 8.720 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 92 Resp: 322541

Ion Ratio Lower Upper

92 100

91 175.0 134.2 201.2

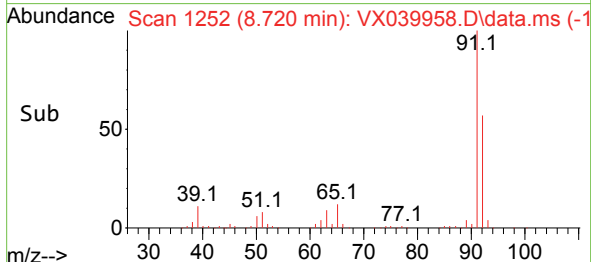

#53

t-1,3-Dichloropropene

Concen: 2.445 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. -0.262 min

Lab File: VX039958.D




Acq: 25 Jan 2024 16:50


Tgt Ion: 75 Resp: 4012

Ion Ratio Lower Upper

75 100

77 160.3 25.7 38.5#

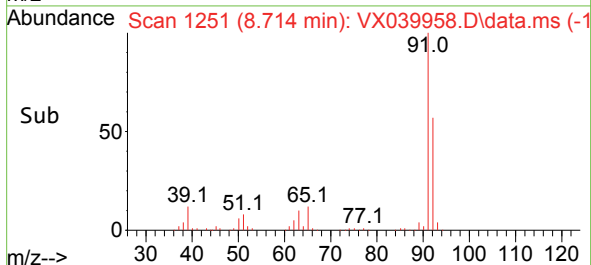



#55

1,1,2-Trichloroethane

Concen: 0.469 ug/l

RT: 9.104 min Scan# 11

Delta R.T. -0.049 min


Lab File: VX039958.D

Acq: 25 Jan 2024 16:50

Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion: 97 Resp: 537




Ion Ratio Lower Upper

97 100

83 0.0 65.8 98.8#

85 0.0 41.6 62.4#

99 0.0 47.8 71.8#



#59

2-Hexanone

Concen: 0.232 ug/l

RT: 9.391 min Scan# 1362

Delta R.T. -0.036 min

Lab File: VX039958.D




Acq: 25 Jan 2024 16:50


Tgt Ion: 43 Resp: 394

Ion Ratio Lower Upper

43 100

58 0.0 26.2 78.5#









#62
4-Bromofluorobenzene
Concen: 52.008 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 78409
Ion Ratio Lower Upper
95 100
174 69.3 0.0 135.6
176 66.5 0.0 131.0

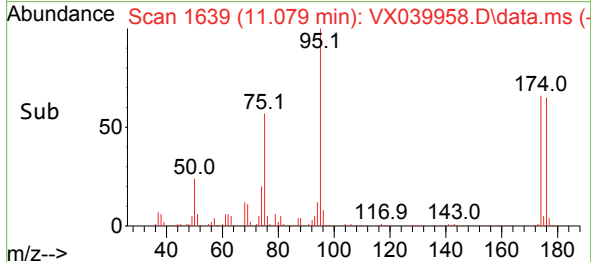

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Tgt Ion: 117 Resp: 140080
Ion Ratio Lower Upper
117 100
82 58.4 46.2 69.4
119 31.9 25.5 38.3


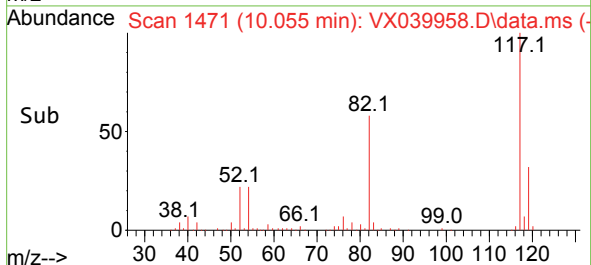






#67
Ethyl Benzene
Concen: 1.095 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 5929
Ion Ratio Lower Upper
91 100
106 33.4 24.9 37.3

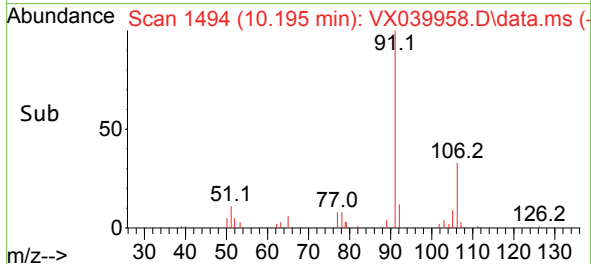

#68
m/p-Xylenes
Concen: 3.963 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Tgt Ion: 106 Resp: 7894
Ion Ratio Lower Upper
106 100
91 224.5 165.5 248.3









#69
o-Xylene
Concen: 1.848 ug/l
RT: 10.640 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 3645
Ion Ratio Lower Upper
106 100
91 226.7 108.9 326.8

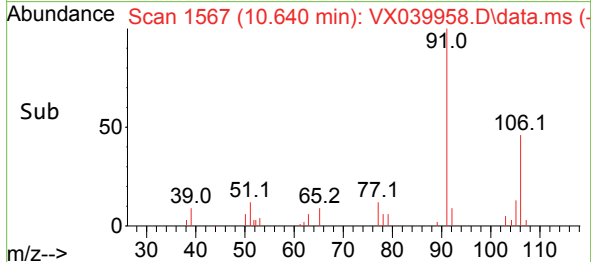

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Tgt Ion:152 Resp: 78244
Ion Ratio Lower Upper
152 100
115 64.7 43.3 129.9
150 157.2 0.0 345.0





#73

Isopropylbenzene

Concen: 0.300 ug/l

RT: 10.964 min Scan# 1620

Delta R.T. 0.000 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 1869

Ion Ratio Lower Upper

105 100

120 21.9 12.9 38.6

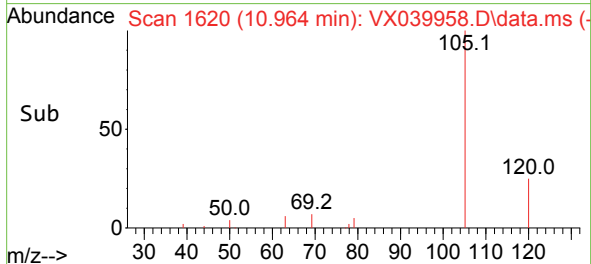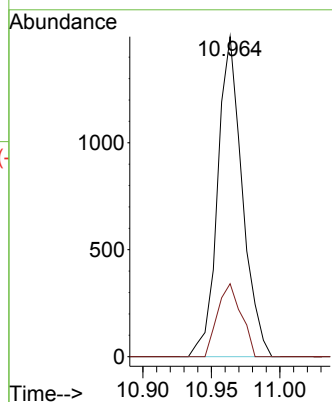

#76

1,2,3-Trichloropropane

Concen: 21.876 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX039958.D




Acq: 25 Jan 2024 16:50


Tgt Ion: 75 Resp: 44376

Ion Ratio Lower Upper

75 100

77 1.3 19.1 57.5#




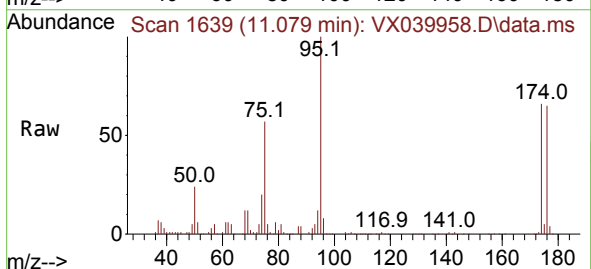




#78
n-propylbenzene
Concen: 0.992 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 7480
Ion Ratio Lower Upper
91 100
120 19.7 11.5 34.4

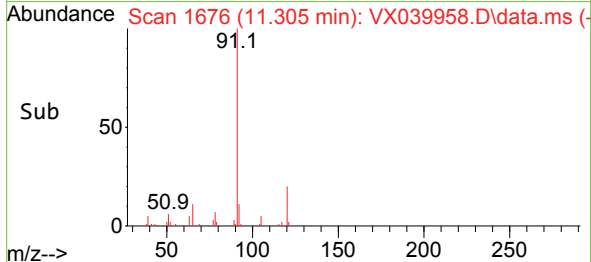

#79
2-Chlorotoluene
Concen: 0.751 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Tgt Ion: 91 Resp: 3501
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

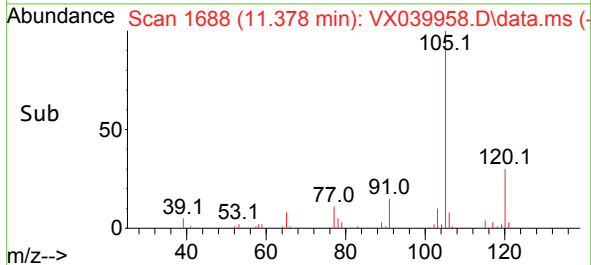



#80

1,3,5-Trimethylbenzene

Concen: 1.177 ug/l

RT: 11.451 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 6227

Ion Ratio Lower Upper

105 100

120 43.2 24.1 72.3

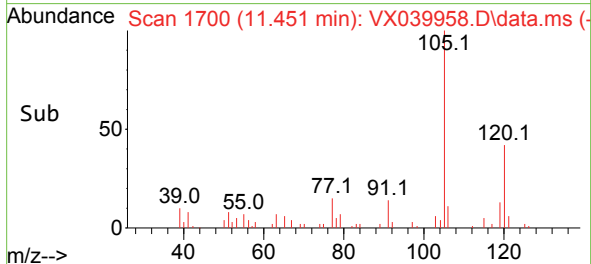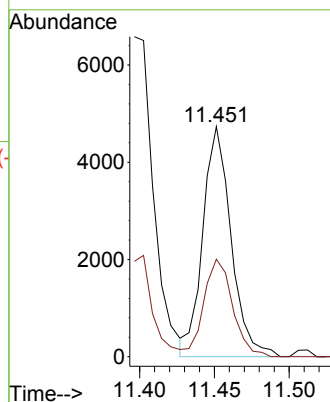

#81

trans-1,4-Dichloro-2-butene

Concen: 63.525 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50




Tgt Ion: 75 Resp: 44376


Ion Ratio Lower Upper

75 100

53 0.2 90.5 135.7#

89 0.0 36.9 55.3#

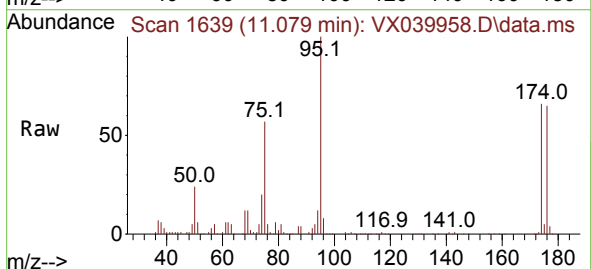



#82

4-Chlorotoluene

Concen: 0.252 ug/l

RT: 11.457 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 1332

Ion Ratio Lower Upper

91 100

126 4.8 14.2 42.6#

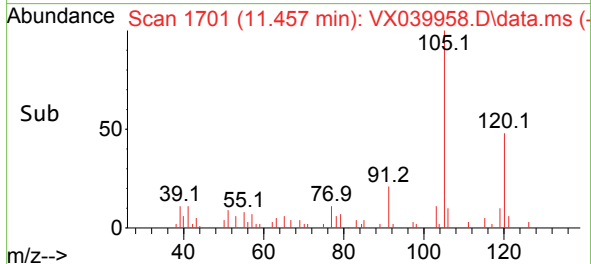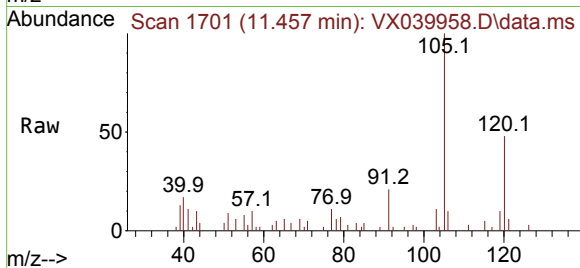

#83

tert-Butylbenzene

Concen: 0.380 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. 0.256 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50




Tgt Ion: 119 Resp: 1918


Ion Ratio Lower Upper

119 100

91 40.1 31.2 93.6

134 34.3 11.7 35.0

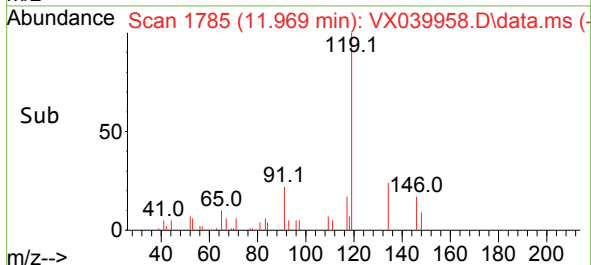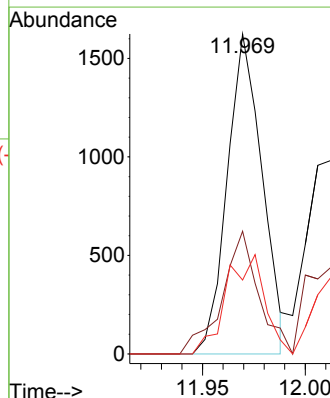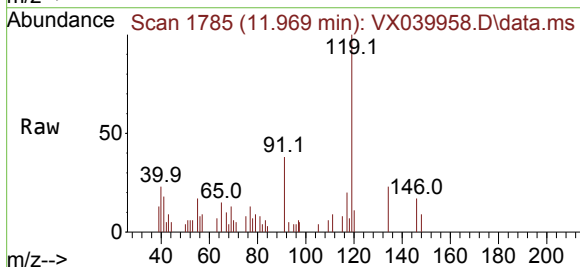



#84

1,2,4-Trimethylbenzene

Concen: 4.497 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 23739

Ion Ratio Lower Upper

105 100

120 41.9 21.2 63.6

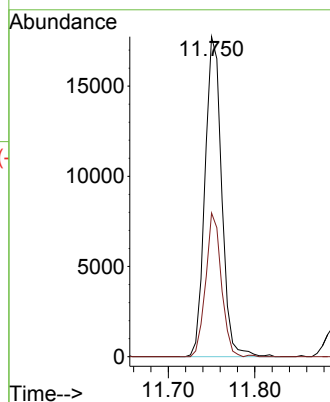

#85

sec-Butylbenzene

Concen: 0.320 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. 0.000 min

Lab File: VX039958.D




Acq: 25 Jan 2024 16:50


Tgt Ion:105 Resp: 2099

Ion Ratio Lower Upper

105 100

134 26.0 9.8 29.4



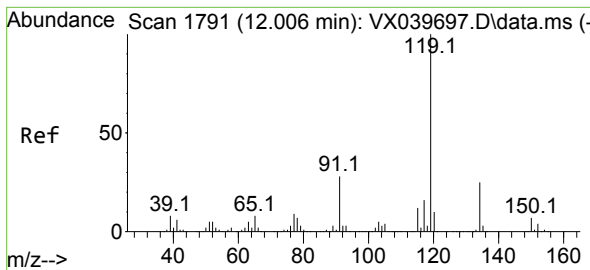

#86

p-Isopropyltoluene

Concen: 0.380 ug/l

RT: 11.969 min Scan# 11

Delta R.T. -0.036 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:119 Resp: 1989

Ion Ratio Lower Upper

119 100

134 33.1 12.8 38.3

91 38.7 13.1 39.3

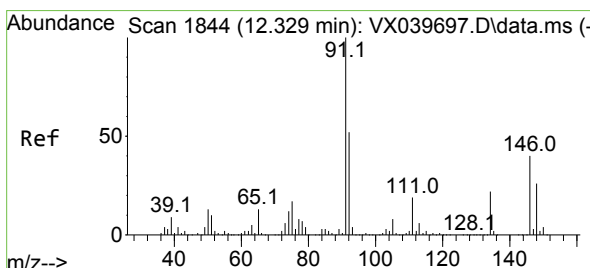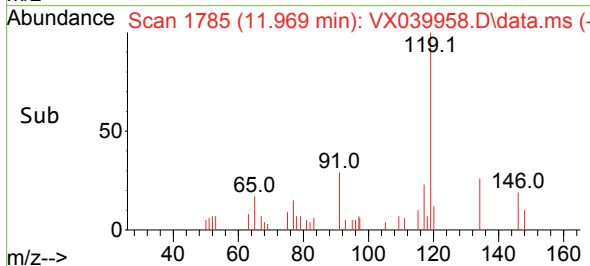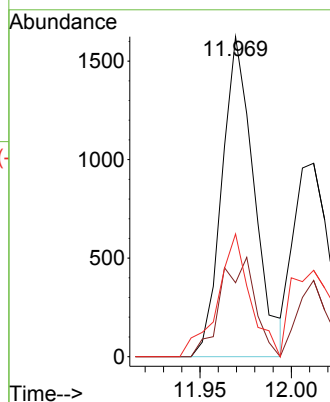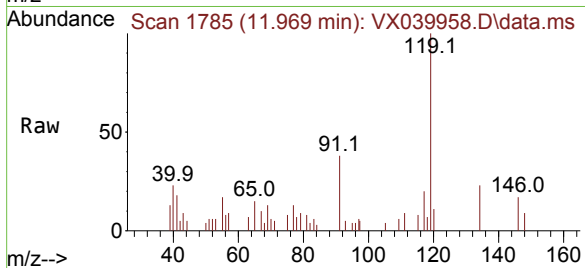

#89

n-Butylbenzene

Concen: 1.026 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.006 min

Lab File: VX039958.D

Acq: 25 Jan 2024 16:50




Tgt Ion: 91 Resp: 5191


Ion Ratio Lower Upper

91 100

92 38.5 27.4 82.0

134 59.0 12.6 37.8#


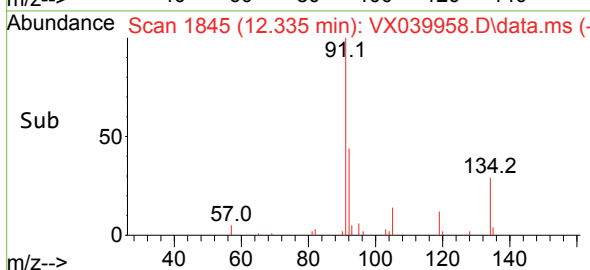

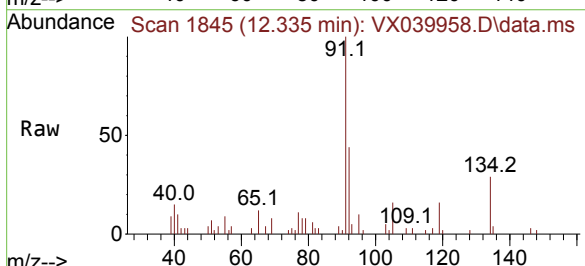




#90
Hexachloroethane
Concen: 0.550 ug/l
RT: 12.536 min Scan# 117
Delta R.T. 0.000 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:117 Resp: 486
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

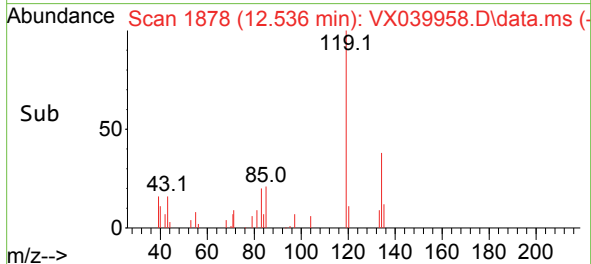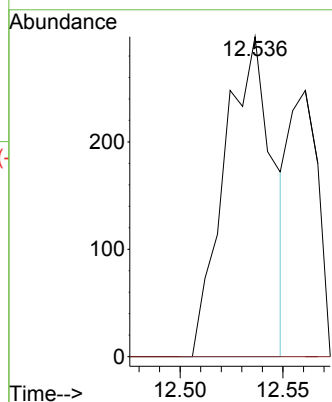

#95
Naphthalene
Concen: 0.325 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX039958.D
Acq: 25 Jan 2024 16:50

Tgt Ion:128 Resp: 1920
Ion Ratio Lower Upper
128 100
127 10.3 10.3 15.5#
129 12.4 8.8 13.2

