

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX012619\
 Data File : VX007254.D
 Acq On : 26 Jan 2019 02:27
 Operator : JC/SP
 Sample : K1238-50
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 28 00:22:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 08 14:06:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	533130	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	831121	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	799361	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	385700	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	288022	51.69	ug/l	0.00
Spiked Amount			Recovery	=	103.38%	
35) Dibromofluoromethane	5.51	113	256280	48.15	ug/l	0.00
Spiked Amount			Recovery	=	96.30%	
50) Toluene-d8	8.71	98	1012429	51.97	ug/l	0.00
Spiked Amount			Recovery	=	103.94%	
62) 4-Bromofluorobenzene	11.13	95	361205	53.18	ug/l	0.00
Spiked Amount			Recovery	=	106.36%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.33	50	2287	0.449	ug/l #	85
8) Diethyl Ether	2.19	74	866	0.246	ug/l	88
11) Tert butyl alcohol	3.06	59	3624	2.757	ug/l #	72
13) Acrolein	2.30	56	376	3.739	ug/l #	13
14) Allyl chloride	2.86	41	32590	3.881	ug/l #	26
16) Acetone	2.45	43	69839	25.355	ug/l	98
18) Methyl Acetate	2.78	43	13670	1.714	ug/l #	89
20) Methylene Chloride	2.86	84	945963	182.057	ug/l	94
25) 2-Butanone	4.70	43	15392	3.905	ug/l	94
29) Tetrahydrofuran	5.16	42	16340	6.380	ug/l	97
36) 1,1-Dichloropropene	5.66	75	33654	4.657	ug/l #	49
38) Carbon Tetrachloride	5.66	117	48149	6.623	ug/l #	14
43) Isopropyl Acetate	6.46	43	24008	1.965	ug/l	94
48) Methyl methacrylate	7.68	41	12112	1.930	ug/l #	12
49) 1,4-Dioxane	7.77	88	167	Below Cal	#	27
51) 4-Methyl-2-Pentanone	8.62	43	131276	16.717	ug/l #	50
54) cis-1,3-Dichloropropene	8.62	75	64576	7.953	ug/l #	63
57) 1,3-Dichloropropane	9.54	76	15578	1.676	ug/l #	45
59) 2-Hexanone	9.54	43	214040	35.766	ug/l #	50
74) N-amyl acetate	10.69	43	19744	1.803	ug/l #	54
76) 1,2,3-Trichloropropane	11.13	75	171488	21.941	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.51	105	6523	0.287	ug/l	97
81) trans-1,4-Dichloro-2-buten	11.13	75	171488	64.987	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.81	105	8283	0.362	ug/l	95
90) Hexachloroethane	12.58	117	286	2.978	ug/l #	6
95) Naphthalene	13.83	128	44030	1.584	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012619\
Data File : VX007254.D
Acq On : 26 Jan 2019 02:27
Operator : JC/SP
Sample : K1238-50
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jan 28 00:22:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 08 14:06:59 2019
Response via : Initial Calibration

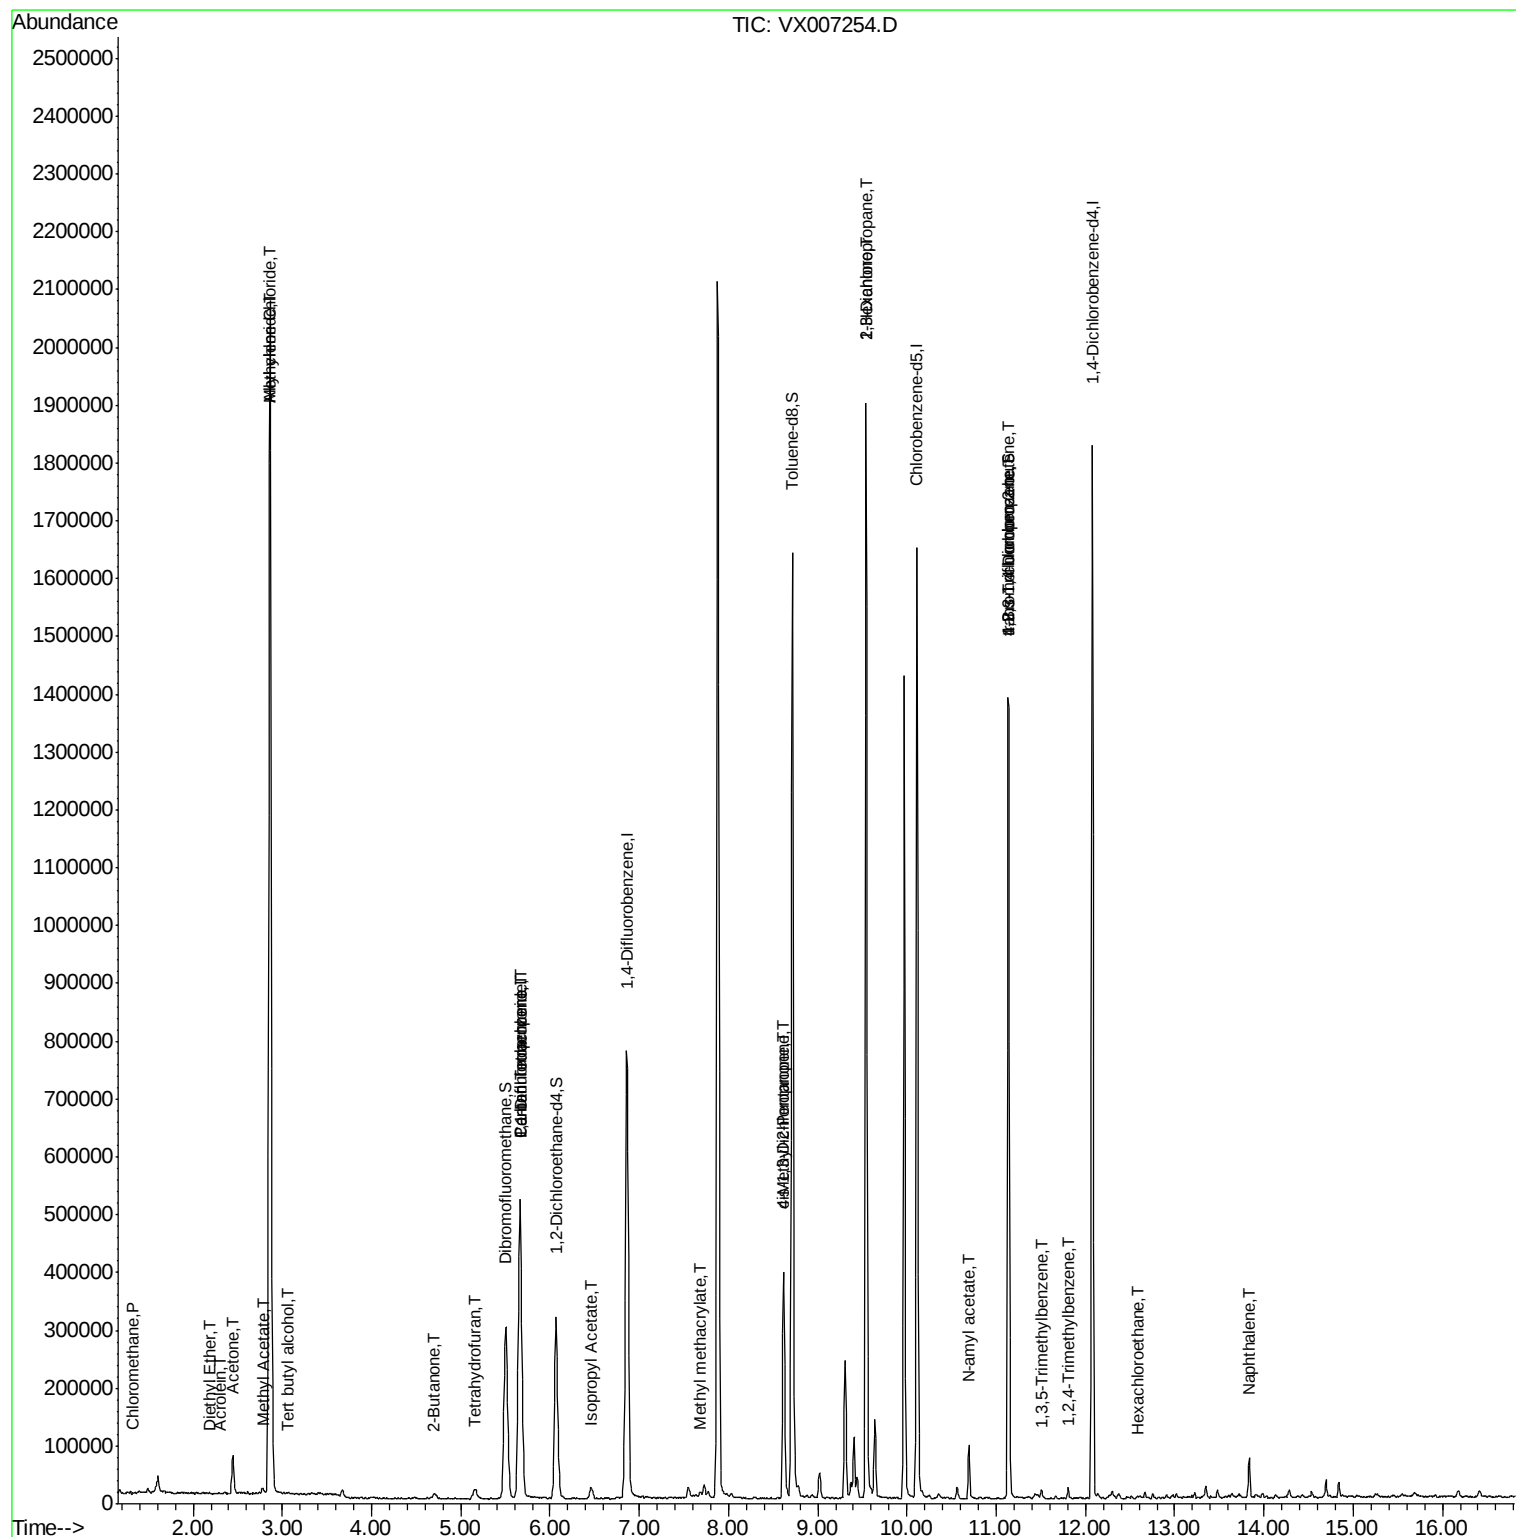

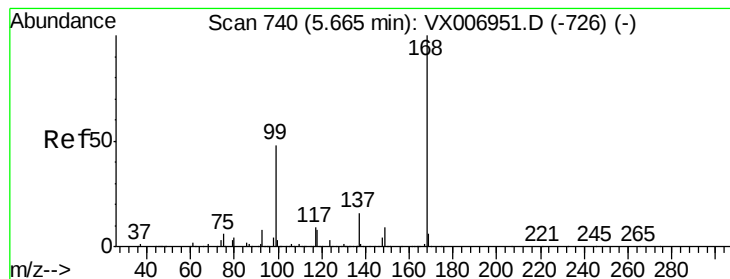

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:168 Resp: 533130

Ion Ratio Lower Upper

168 100

99 49.5 41.8 62.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

200000

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

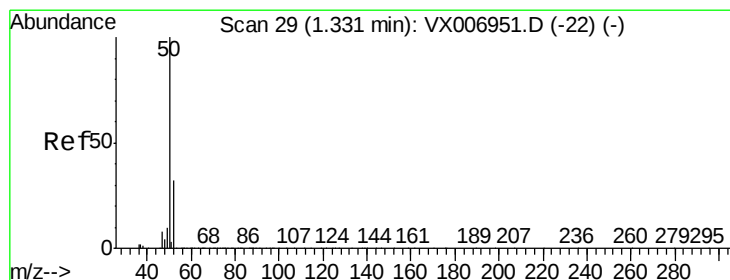

#3

Chloromethane

Concen: 0.449 ug/l

RT: 1.33 min Scan# 29

Delta R.T. -0.00 min

Lab File: VX007254.D


Acq: 26 Jan 2019 02:27

Tgt Ion: 50 Resp: 2287

Ion Ratio Lower Upper

50 100

52 40.4 25.4 38.2#

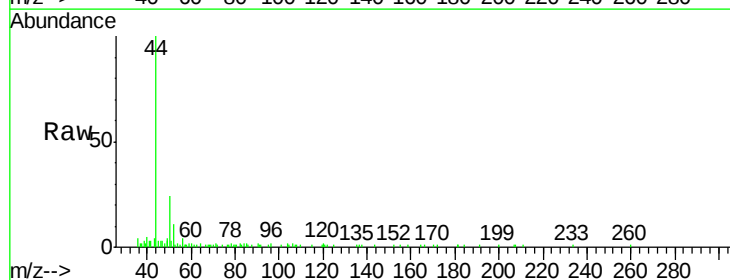

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.33

2000

1500


1000


500

0

Time-->

1.30 1.35

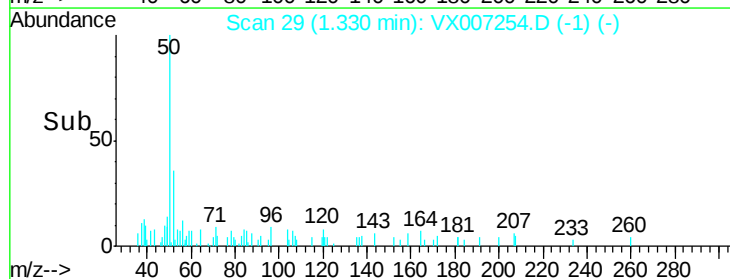

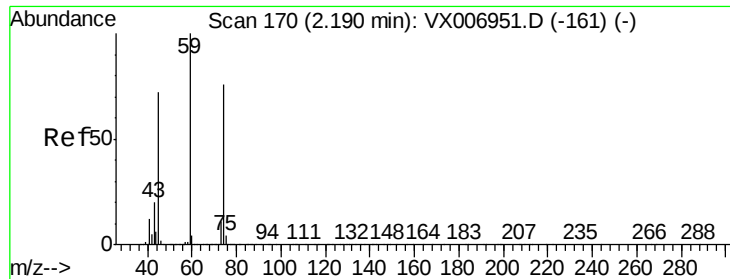

#8

Diethyl Ether

Concen: 0.246 ug/l

RT: 2.19 min Scan# 170

Delta R.T. -0.00 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 74 Resp: 866

Ion Ratio Lower Upper




74 100

45 104.3 46.3 138.9



Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

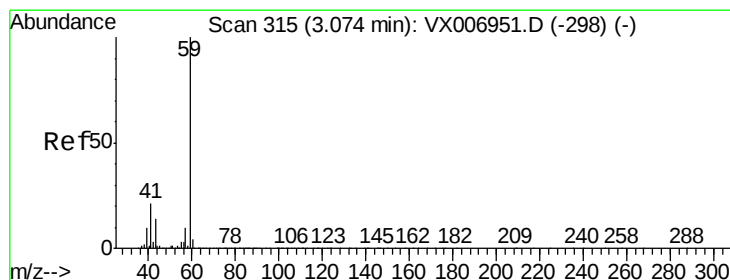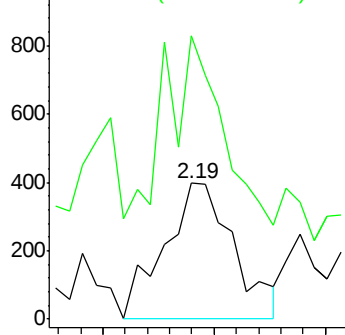

#11

Tert butyl alcohol

Concen: 2.757 ug/l

RT: 3.06 min Scan# 312

Delta R.T. -0.02 min

Lab File: VX007254.D


Acq: 26 Jan 2019 02:27

Tgt Ion: 59 Resp: 3624

Ion Ratio Lower Upper



59 100


57 0.0 8.5 12.7#

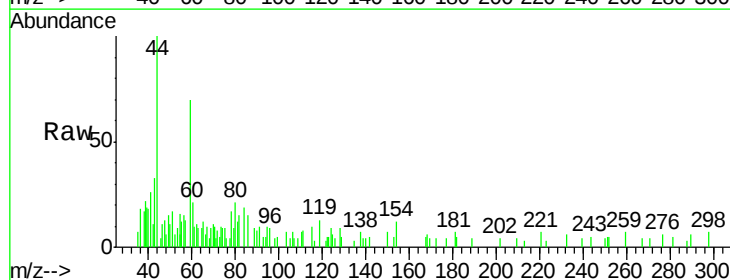

Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

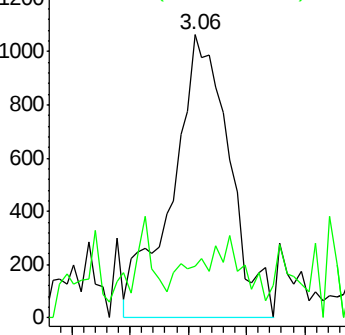

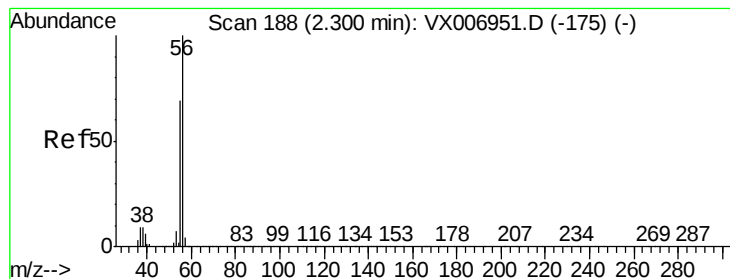

#13

Acrolein

Concen: 3.739 ug/l

RT: 2.30 min Scan# 188

Delta R.T. -0.00 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X


ClientSampled :

Tot Ion: 56 Resp: 376

Ion Ratio Lower Upper




56 100

55 0.0 58.2 87.4#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

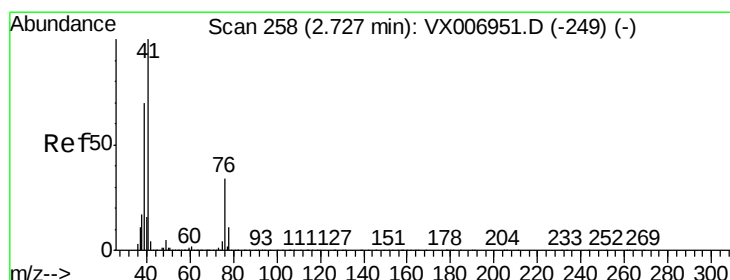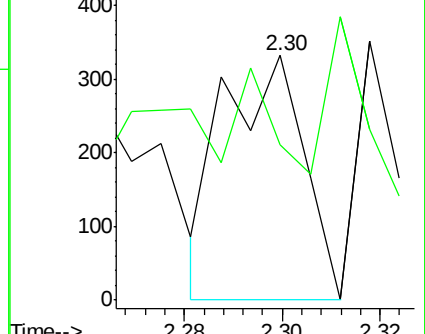

#14

Allyl chloride

Concen: 3.881 ug/l

RT: 2.86 min Scan# 280

Delta R.T. 0.13 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27


Tgt Ion: 41 Resp: 32590

Ion Ratio Lower Upper

41 100

39 2.0 53.6 80.4#



76 0.3 27.4 41.2#




Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

Ion 75.90 (75.60 to 76.60): VX0

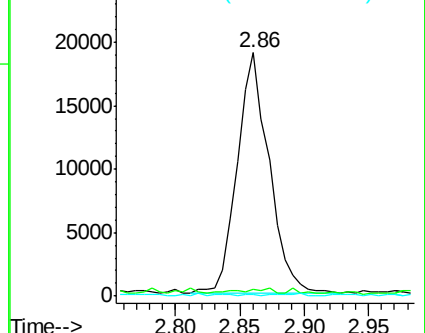

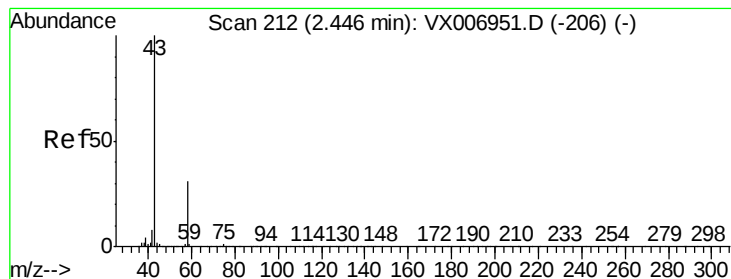

#16

Acetone

Concen: 25.355 ug/l

RT: 2.45 min Scan# 212

Delta R.T. -0.00 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27





Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 43 Resp: 69839

Ion Ratio Lower Upper

43 100

58 32.4 25.0 37.6

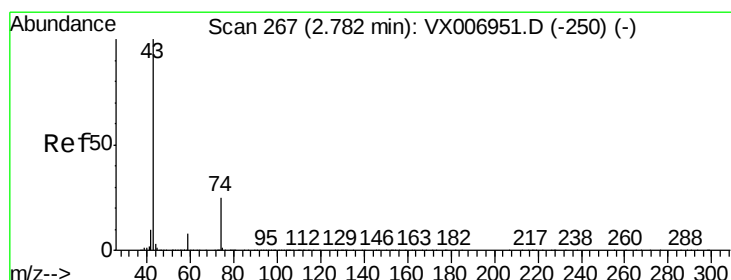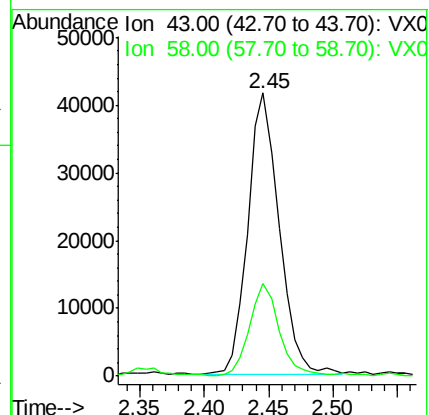

#18

Methyl Acetate

Concen: 1.714 ug/l

RT: 2.78 min Scan# 267

Delta R.T. -0.00 min

Lab File: VX007254.D




Acq: 26 Jan 2019 02:27


Tgt Ion: 43 Resp: 13670

Ion Ratio Lower Upper

43 100

74 28.5 18.6 28.0#



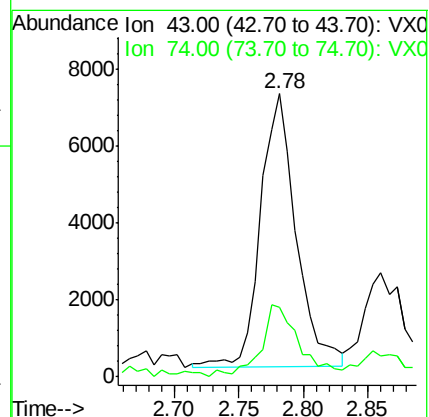
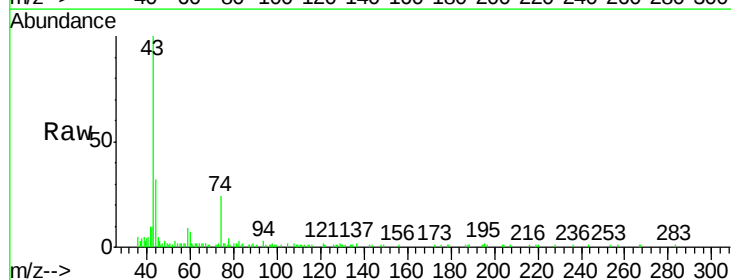




#20
Methvlene Chloride
Concen: 182.057 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.00 min
Lab File: VX007254.D
Acq: 26 Jan 2019 02:27




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion:	84	Resp:	945963
Ion	Ratio	Lower	Upper
84	100		
49	124.2	91.8	137.6
51	37.5	28.5	42.7
86	65.6	50.2	75.2

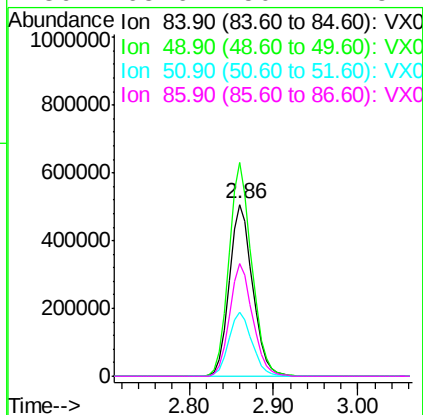

#25
2-Butanone
Concen: 3.905 ug/l
RT: 4.70 min Scan# 582
Delta R.T. -0.00 min
Lab File: VX007254.D
Acq: 26 Jan 2019 02:27

Tgt Ion:	43	Resp:	15392
Ion	Ratio	Lower	Upper
43	100		
72	25.1	22.4	33.6

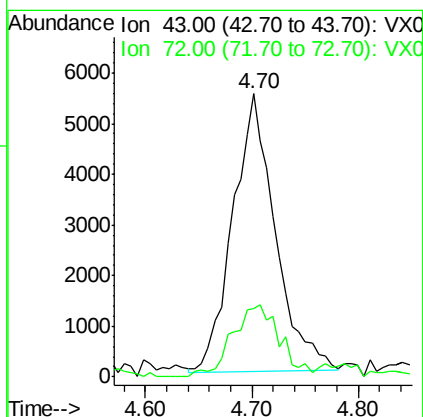

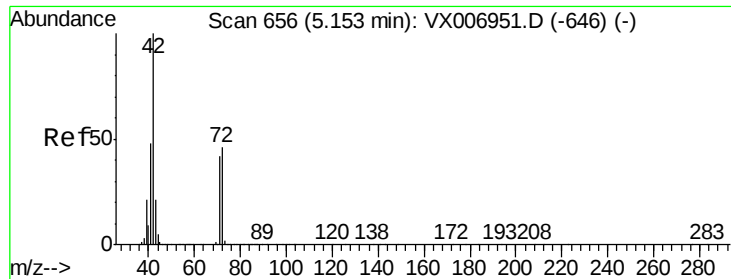

#29

Tetrahydrofuran

Concen: 6.380 ug/l

RT: 5.16 min Scan# 657

Delta R.T. 0.01 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 42 Resp: 16340

Ion Ratio Lower Upper

42 100

72 45.0 38.9 58.3




71 45.1 36.2 54.4

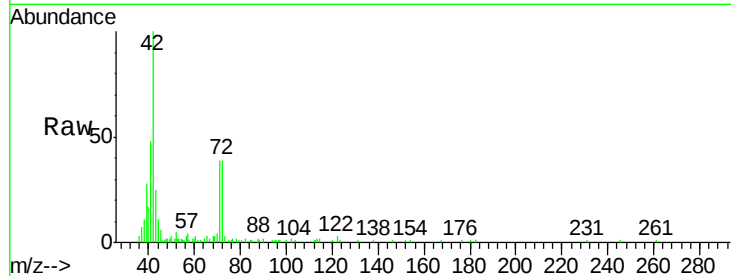

Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

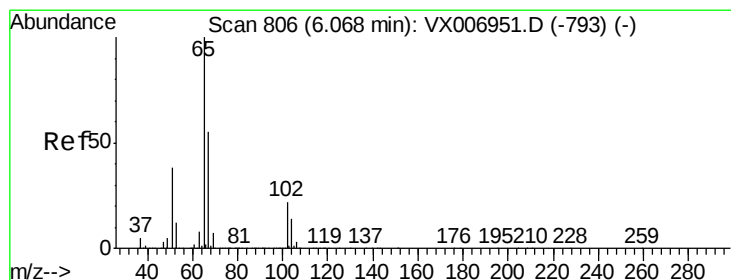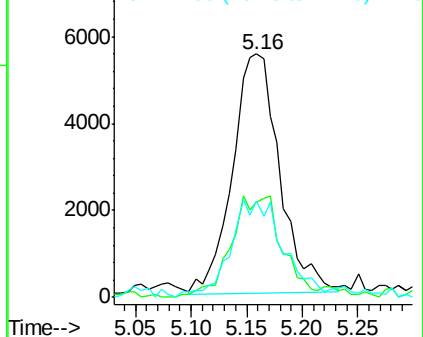

#33

1,2-Dichloroethane-d4

Concen: 51.694 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX007254.D


Acq: 26 Jan 2019 02:27

Tgt Ion: 65 Resp: 288022

Ion Ratio Lower Upper



65 100


67 53.6 0.0 105.0



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

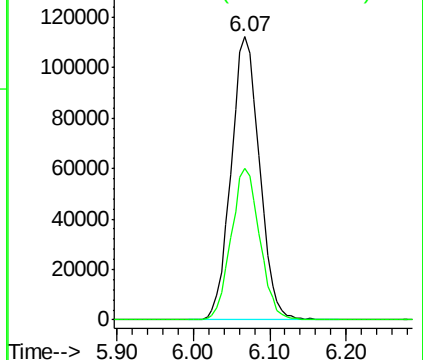

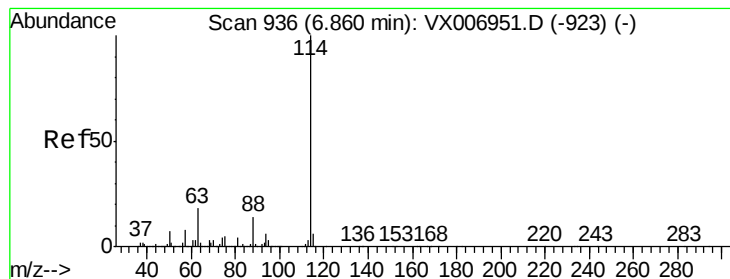

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:114 Resp: 831121

Ion Ratio Lower Upper

114 100

63 18.4 0.0 34.8




88 14.3 0.0 28.8



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

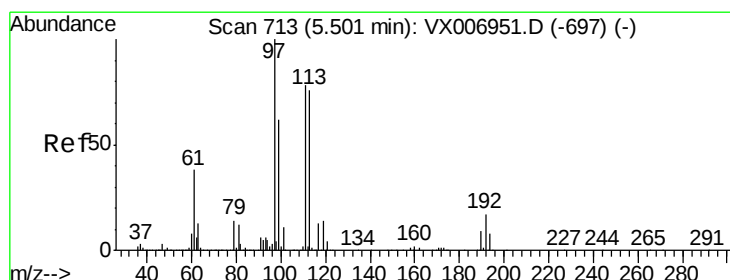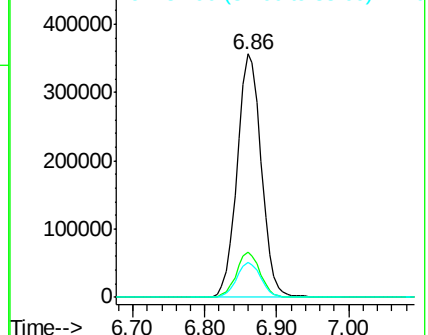

#35

Dibromofluoromethane

Concen: 48.151 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27


Tgt Ion:113 Resp: 256280

Ion Ratio Lower Upper

113 100

111 101.1 81.6 122.4



192 22.2 16.7 25.1

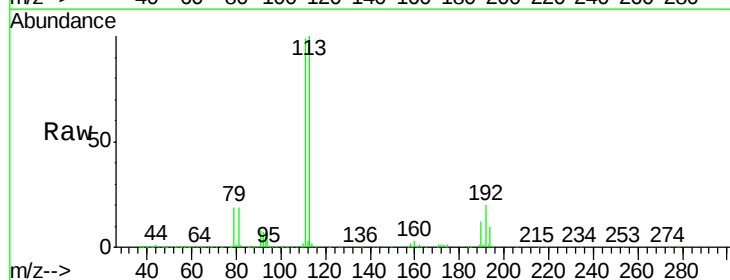


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

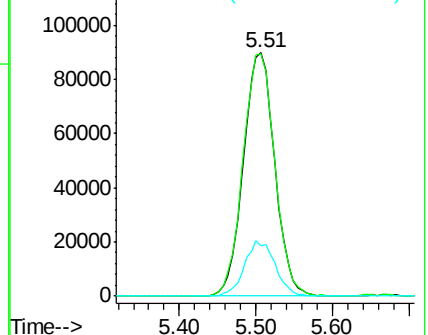



#36

1,1-Dichloropropene

Concen: 4.657 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :
MSVOA_X
ClientSampleId :





Tot Ion: 75 Resp: 33654

Ion Ratio Lower Upper

75 100

110 10.8 20.2 60.5#

77 0.7 24.8 37.2#

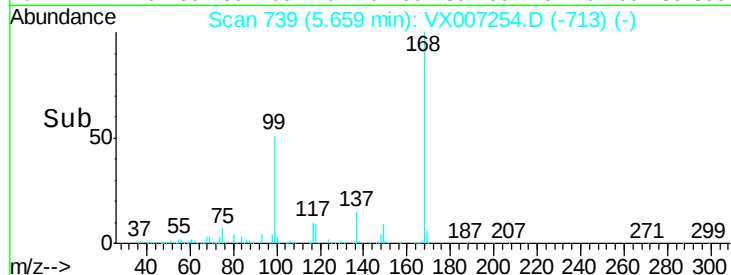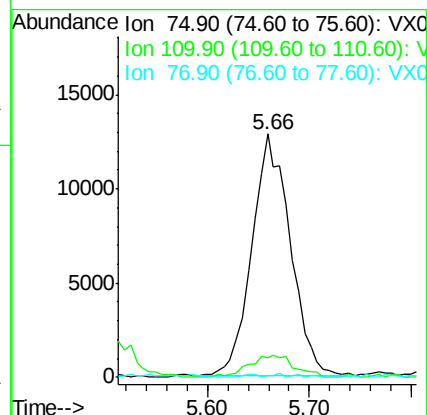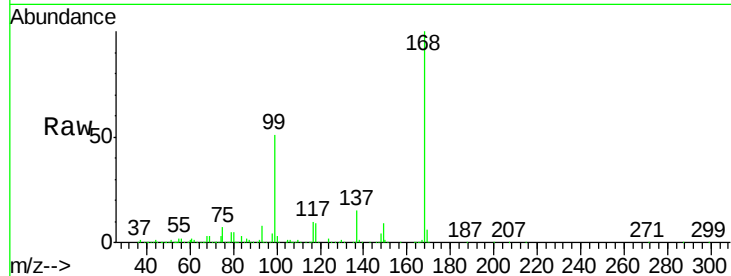

#38

Carbon Tetrachloride

Concen: 6.623 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.12 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27




Tgt Ion: 117 Resp: 48149


Ion Ratio Lower Upper

117 100

119 4.7 79.4 119.2#

121 0.0 24.0 36.0#

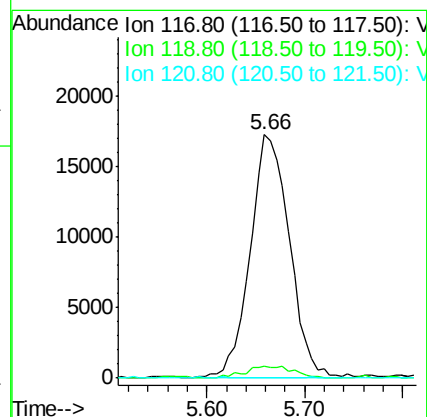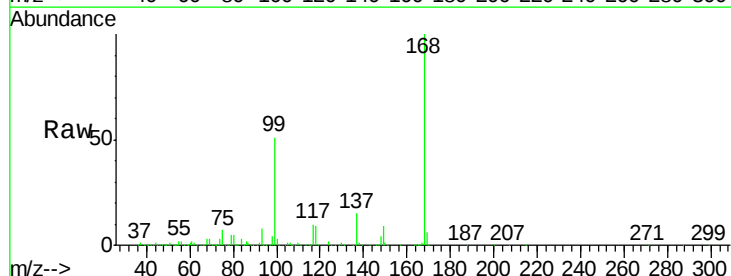



#43

Isopropyl Acetate

Concen: 1.965 ug/l

RT: 6.46 min Scan# 870

Delta R.T. -0.00 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X

ClientSampled :


Tot Ion: 43 Resp: 24008

Ion Ratio Lower Upper

43 100

61 23.9 16.8 25.2




87 18.2 12.4 18.6

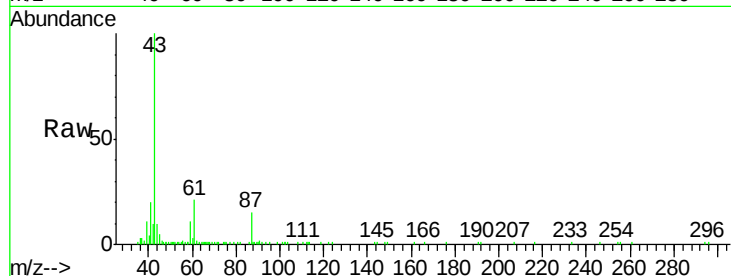

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

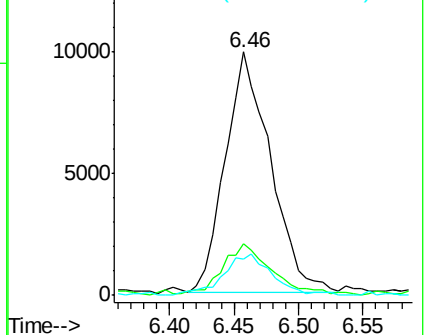

#48

Methyl methacrylate

Concen: 1.930 ug/l

RT: 7.68 min Scan# 1071

Delta R.T. -0.09 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27


Tgt Ion: 41 Resp: 12112

Ion Ratio Lower Upper

41 100

69 1.4 72.4 108.6#



39 0.0 45.8 68.8#




Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

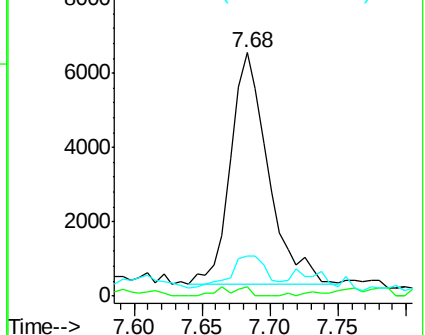

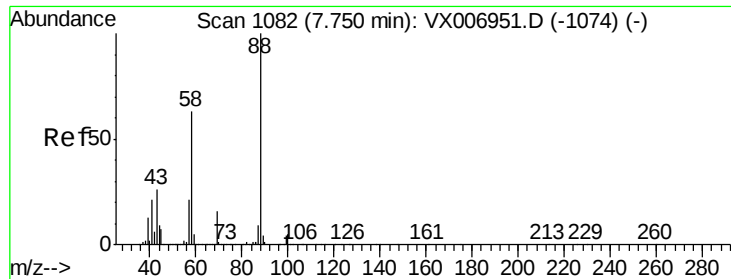

#49

1,4-Dioxane

Concen: Below Cal

RT: 7.77 min Scan# 1086

Delta R.T. 0.02 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X

ClientSampleId :





Tot Ion: 88 Resp: 167

Ion Ratio Lower Upper

88 100

43 0.0 22.2 33.4#

58 0.0 51.0 76.4#

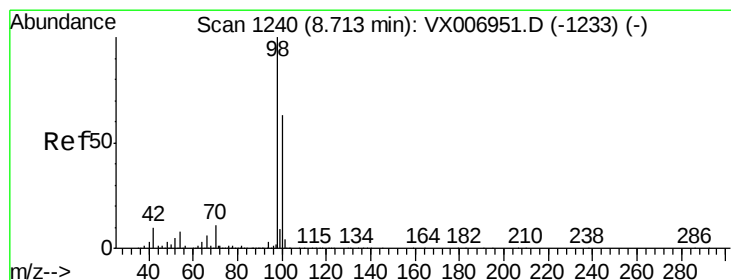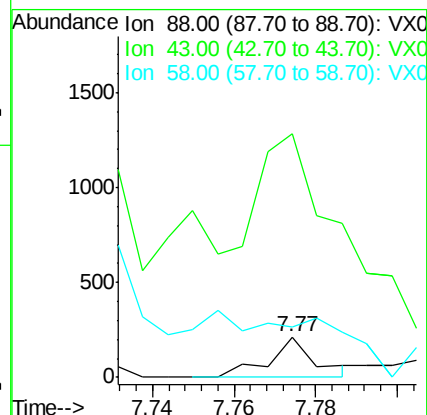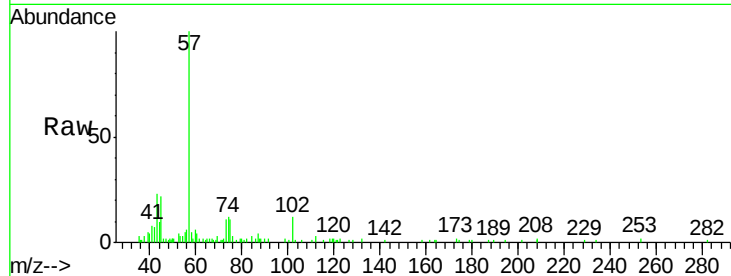

#50

Toluene-d8

Concen: 51.968 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX007254.D




Acq: 26 Jan 2019 02:27


Tgt Ion: 98 Resp: 1012429

Ion Ratio Lower Upper

98 100

100 64.4 52.0 78.0

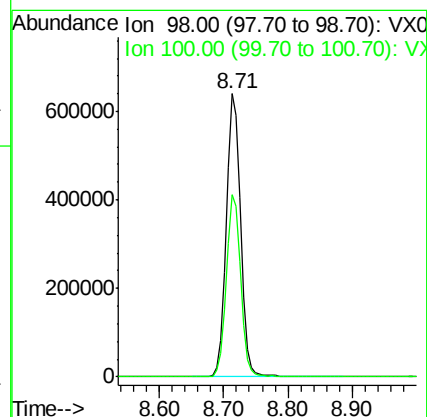

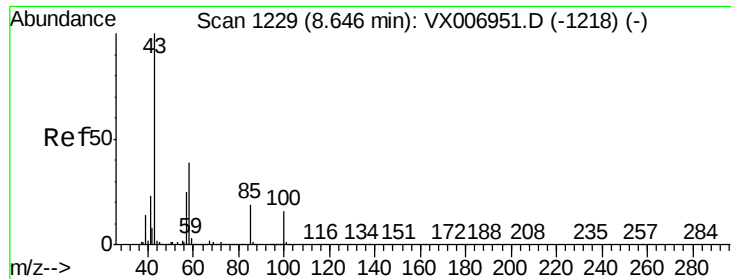

#51

4-Methyl-2-Pentanone

Concen: 16.717 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. -0.03 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 43 Resp: 131276

Ion Ratio Lower Upper

43 100

58 9.0 31.8 47.6#

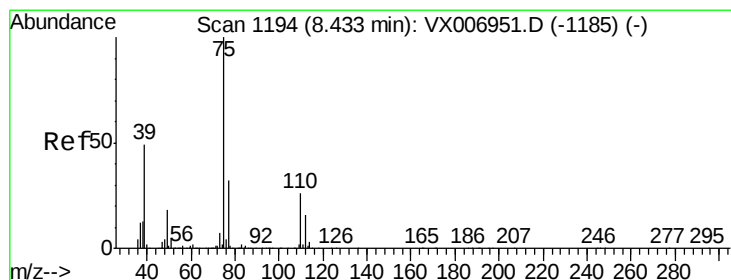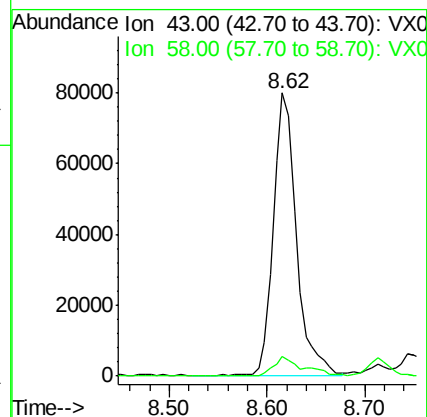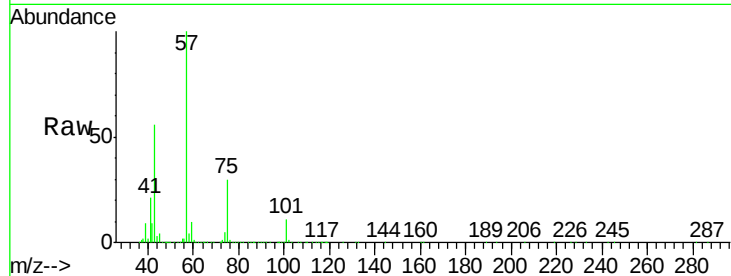

#54

cis-1,3-Dichloropropene

Concen: 7.953 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. 0.18 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27




Tgt Ion: 75 Resp: 64576


Ion Ratio Lower Upper

75 100

77 0.5 26.2 39.2#

39 30.9 36.7 55.1#

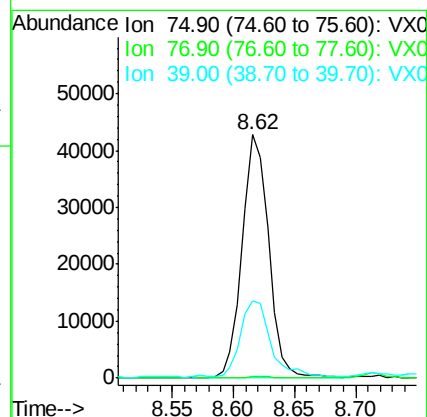



#57

1,3-Dichloropropane

Concen: 1.676 ug/l

RT: 9.54 min Scan# 1376

Delta R.T. 0.17 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 76 Resp: 15578

Ion Ratio Lower Upper

76 100

78 1.4 26.0 39.0#

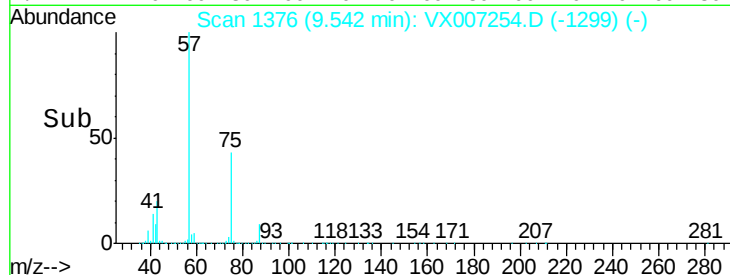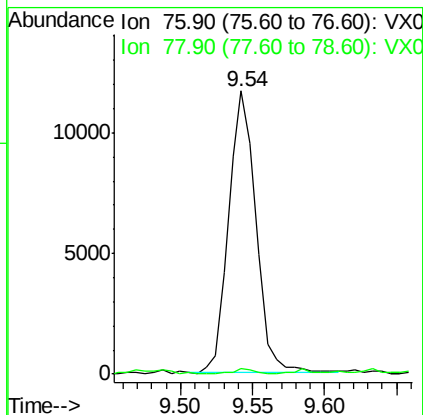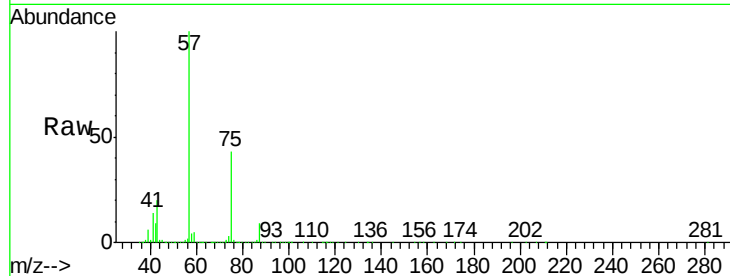

#59

2-Hexanone

Concen: 35.766 ug/l

RT: 9.54 min Scan# 1376

Delta R.T. 0.05 min

Lab File: VX007254.D




Acq: 26 Jan 2019 02:27


Tgt Ion: 43 Resp: 214040

Ion Ratio Lower Upper

43 100

58 19.3 27.7 83.1#

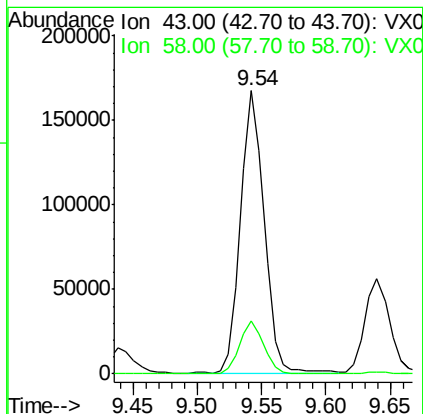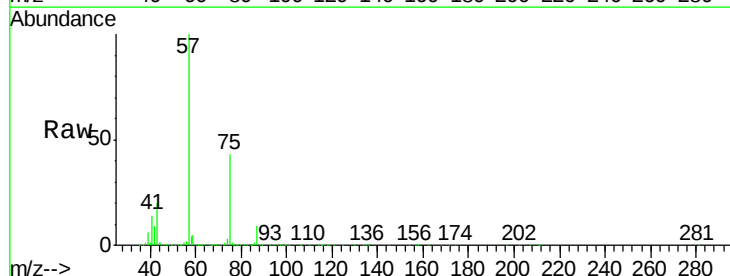

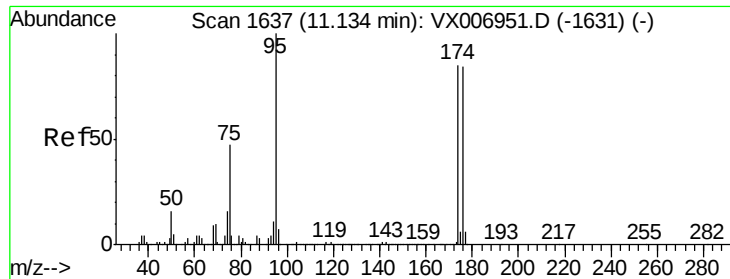

#62

4-Bromofluorobenzene

Concen: 53.182 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 95 Resp: 361205

Ion Ratio Lower Upper

95 100

174 92.6 0.0 182.2




176 91.3 0.0 178.8

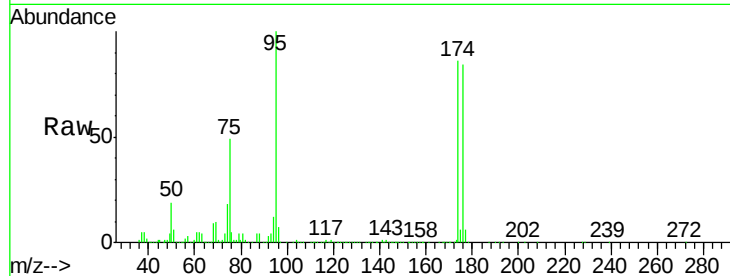

Abundance Ion 94.90 (94.60 to 95.60): VX006951.D (-1631) (-)

Ion 173.80 (173.50 to 174.50): VX006951.D (-1631) (-)

Ion 175.80 (175.50 to 176.50): VX006951.D (-1631) (-)

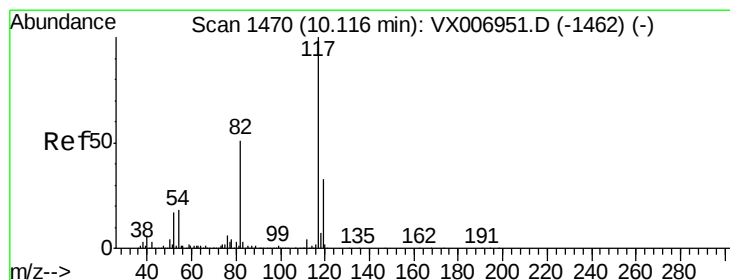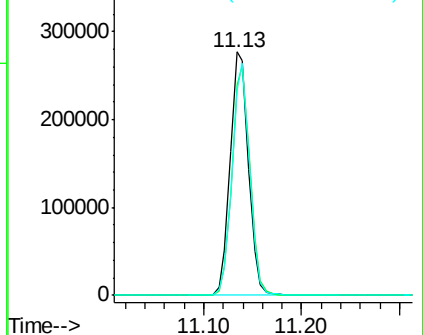

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1470

Delta R.T. -0.00 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27


Tgt Ion: 117 Resp: 799361

Ion Ratio Lower Upper

117 100

82 50.4 41.0 61.6



119 32.0 25.4 38.0




Abundance Ion 116.90 (116.60 to 117.60): VX006951.D (-1462) (-)

Ion 82.00 (81.70 to 82.70): VX006951.D (-1462) (-)

Ion 118.90 (118.60 to 119.60): VX006951.D (-1462) (-)

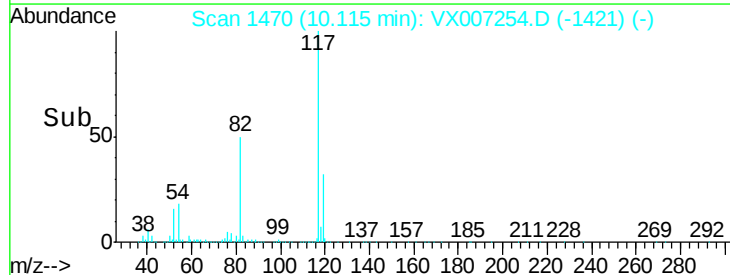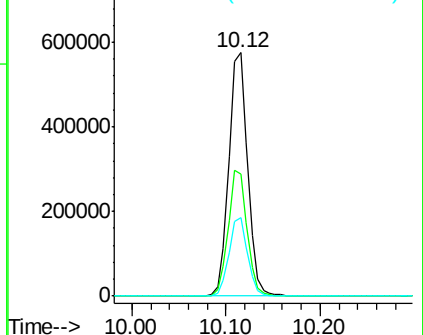



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:152 Resp: 385700

Ion Ratio Lower Upper

152 100

115 55.4 39.1 117.2




150 158.1 0.0 344.8



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

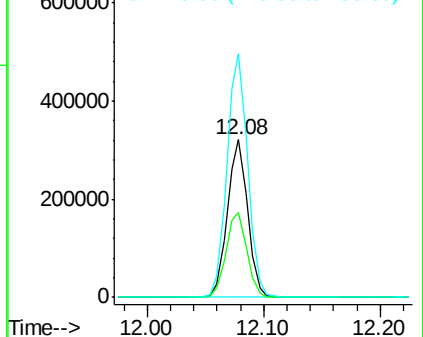

#74

N-ethyl acetate

Concen: 1.803 ug/l

RT: 10.69 min Scan# 1565

Delta R.T. -0.20 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Tgt Ion: 43 Resp: 19744


Ion Ratio Lower Upper

43 100

70 4.1 35.8 53.8#

55 5.4 19.4 29.0#

61 12.3 20.1 30.1#






Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0




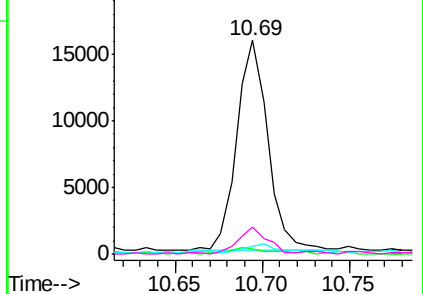




#76
 1,2,3-Trichloropropane
 Concen: 21.941 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. -0.16 min
 Lab File: VX007254.D
 Acq: 26 Jan 2019 02:27




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion: 75 Resp: 171488
 Ion Ratio Lower Upper
 75 100
 77 1.4 18.5 55.5#

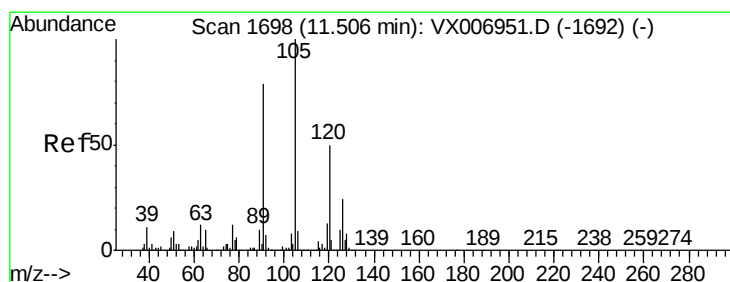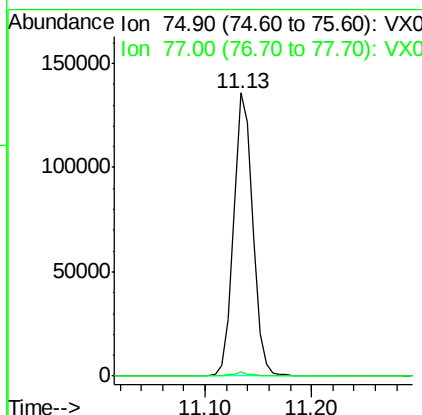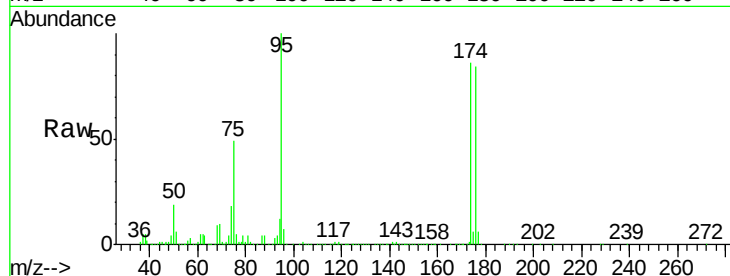

#80
 1,3,5-Trimethylbenzene
 Concen: 0.287 ug/l
 RT: 11.51 min Scan# 1698
 Delta R.T. -0.00 min
 Lab File: VX007254.D
 Acq: 26 Jan 2019 02:27

Tgt Ion: 105 Resp: 6523
 Ion Ratio Lower Upper
 105 100
 120 52.2 25.1 75.3

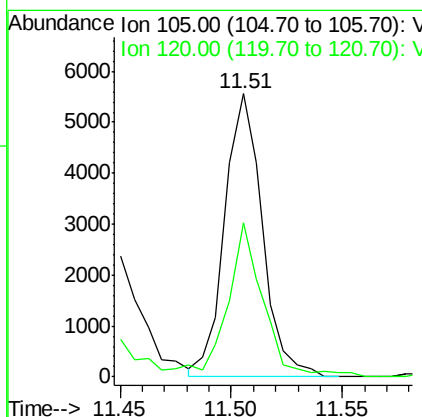



#81

trans-1,4-Dichloro-2-butene

Concen: 64.987 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 75 Resp: 171488

Ion Ratio Lower Upper

75 100

53 0.1 79.7 119.5#




89 0.1 38.0 57.0#

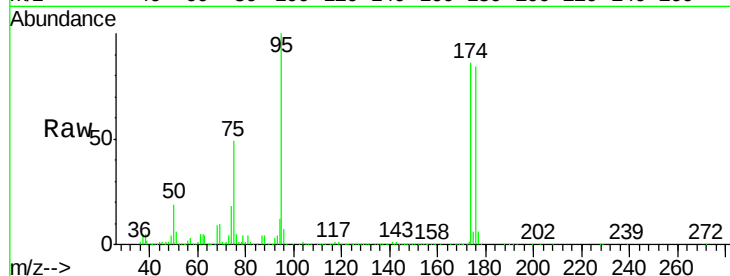

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

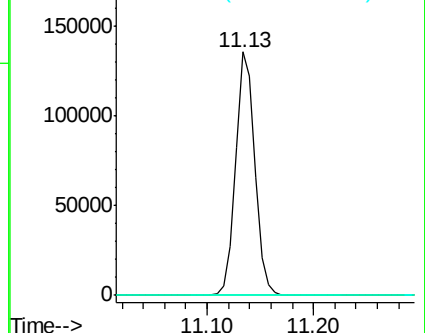

#84

1,2,4-Trimethylbenzene

Concen: 0.362 ug/l

RT: 11.81 min Scan# 1748

Delta R.T. 0.01 min

Lab File: VX007254.D


Acq: 26 Jan 2019 02:27

Tgt Ion: 105 Resp: 8283

Ion Ratio Lower Upper



105 100


120 49.9 23.2 69.6



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

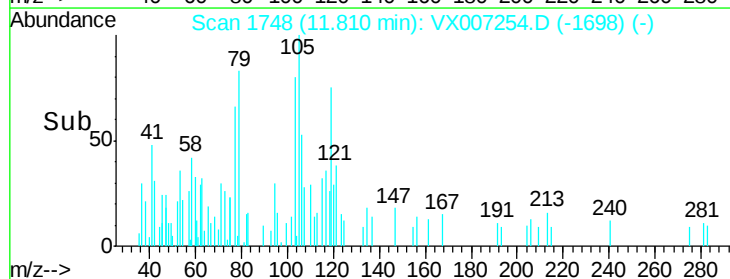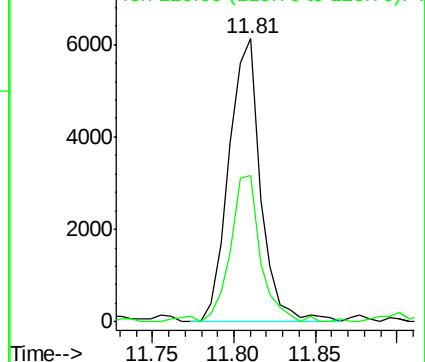



#90

Hexachloroethane

Concen: 2.978 ug/l

RT: 12.58 min Scan# 1874

Delta R.T. -0.02 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:117 Resp: 286

Ion Ratio Lower Upper

117 100

201 0.0 42.9 128.7#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

12.58

250

200



150

100

50

0

Time-->



#95

Naphthalene

Concen: 1.584 ug/l

RT: 13.83 min Scan# 2080

Delta R.T. -0.00 min

Lab File: VX007254.D

Acq: 26 Jan 2019 02:27


Tgt Ion:128 Resp: 44030

Ion Ratio Lower Upper

128 100

127 14.5 10.1 15.1

129 11.0 8.6 13.0



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

13.83

50000

40000

30000

20000

10000

0

Time-->

